

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091522\
 Data File : PL077790.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2022 19:22
 Operator : AR\AJ
 Sample : N4630-21 10X
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 WC-17-4-5

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/16/2022
 Supervised By : Ankita Jodhani 09/16/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 03:54:27 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091222.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 13 13:26:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.412	2.623	2099749	4085443	1.310m	1.376m
28) SA Decachlor...	8.904	7.723	1639633	2763745	1.269m	1.101

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091522\
Data File : PL077790.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2022 19:22
Operator : AR\AJ
Sample : N4630-21 10X
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
WC-17-4-5


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 09/16/2022
Supervised By : Ankita Jodhani 09/16/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 03:54:27 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091222.M
Quant Title : GC Extractables
QLast Update : Tue Sep 13 13:26:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

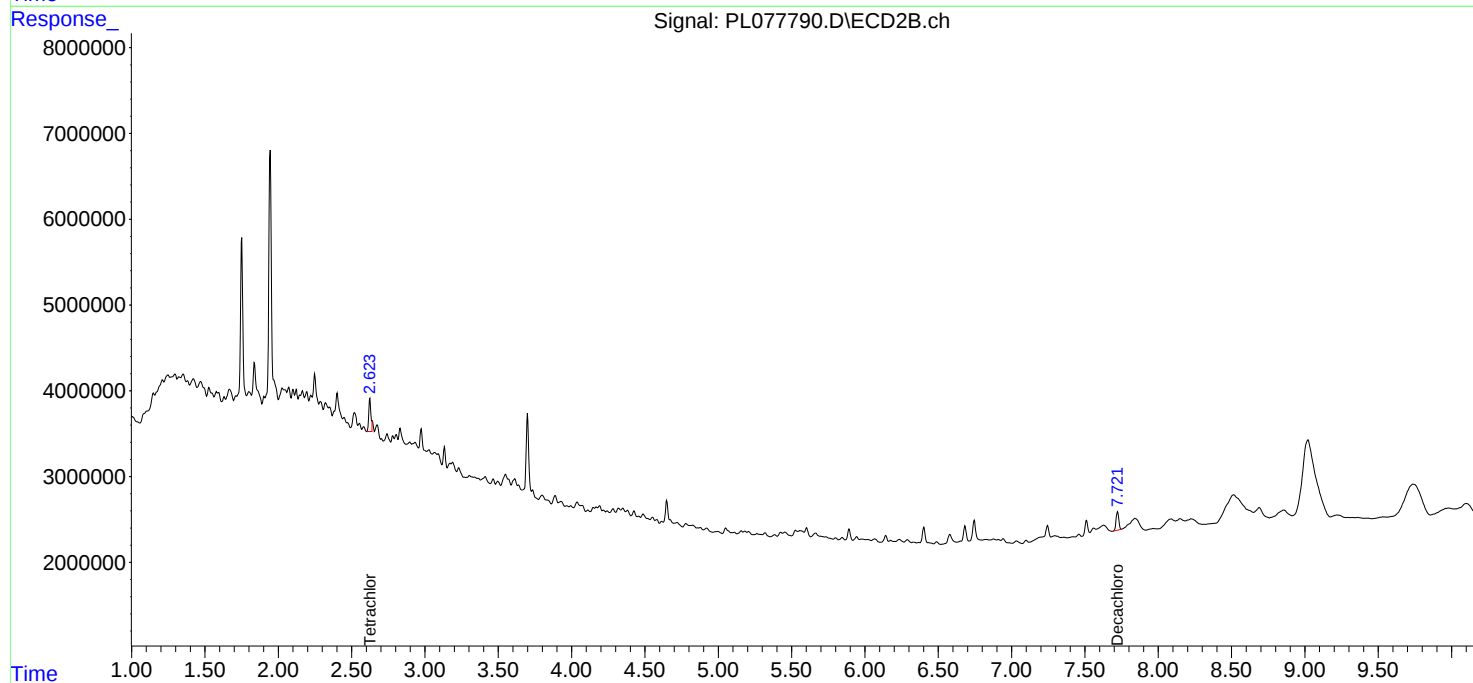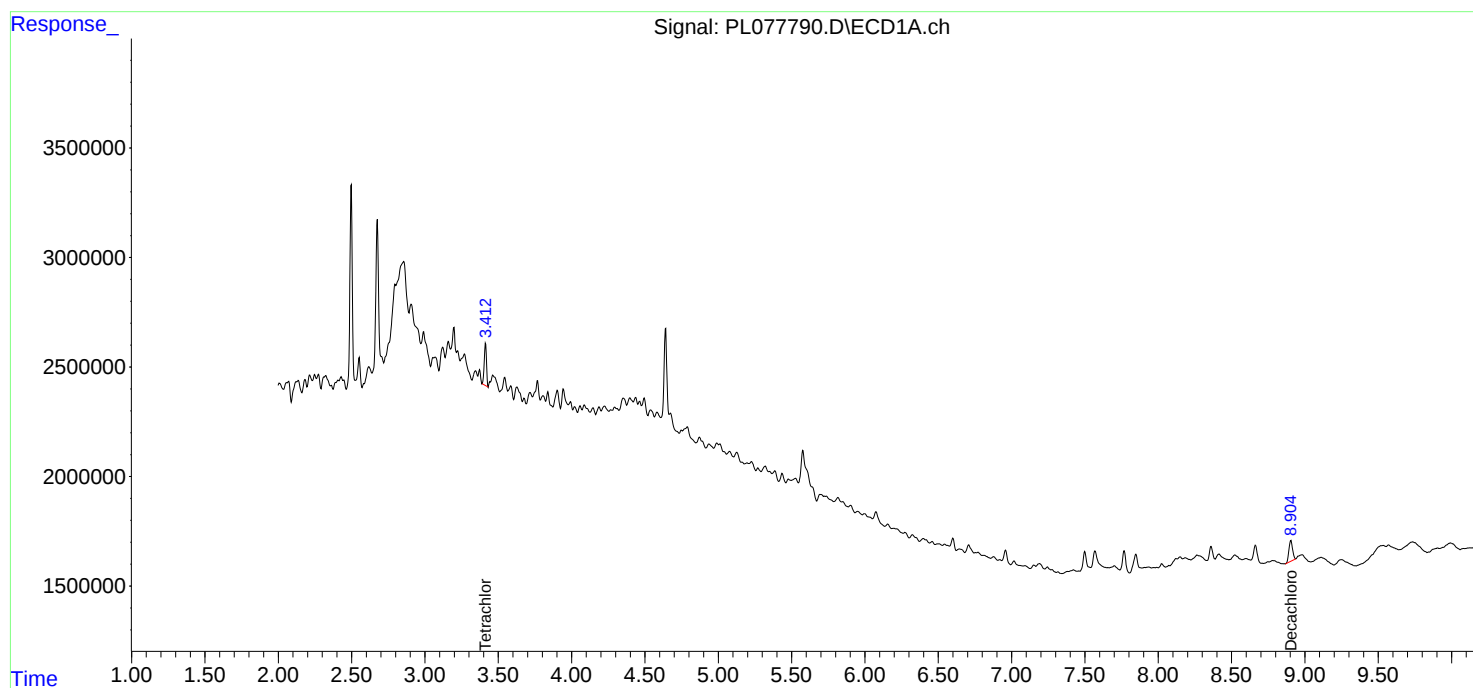

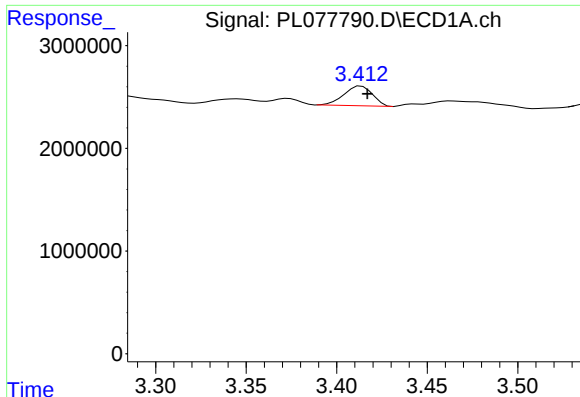


#1 Tetrachloro-m-xylene

R.T.: 3.412 min
Delta R.T.: -0.005 min
Response: 2099749
Conc: 1.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
WC-17-4-5


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/16/2022
Supervised By :Ankita Jodhani 09/16/2022

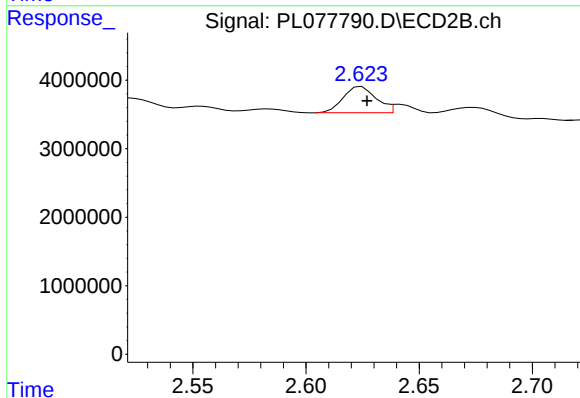


#1 Tetrachloro-m-xylene

R.T.: 2.623 min
Delta R.T.: -0.004 min
Response: 4085443
Conc: 1.38 ng/ml m

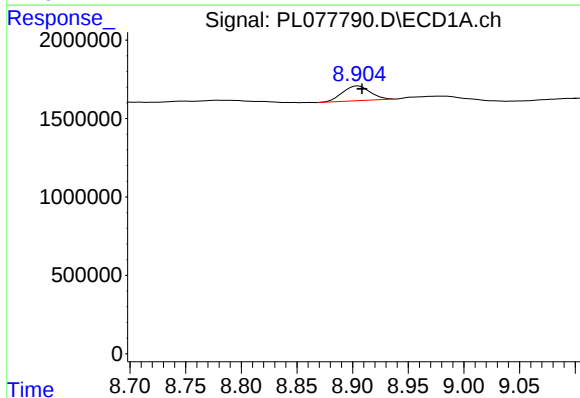

#28 Decachlorobiphenyl

R.T.: 8.904 min
Delta R.T.: -0.005 min
Response: 1639633
Conc: 1.27 ng/ml m

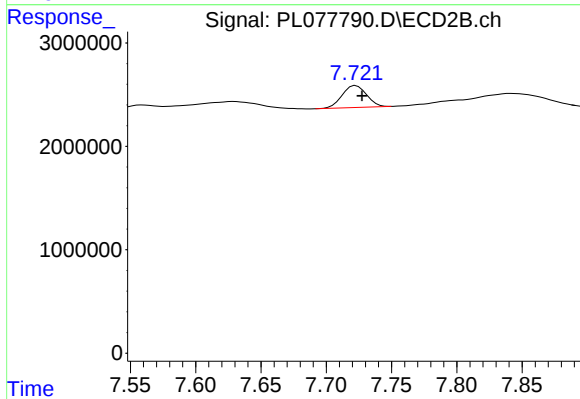

#28 Decachlorobiphenyl

R.T.: 7.723 min
Delta R.T.: -0.005 min
Response: 2763745
Conc: 1.10 ng/ml