

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091523\
 Data File : PL085341.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Sep 2023 17:46
 Operator : AR\AJ
 Sample : 04423-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HD-01-09132023

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 09/15/2023
 Supervised By :Ankita Jodhani 09/15/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 14 22:21:04 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090523.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 05 15:22:36 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.474	2.682	25731564	13261584	10.520m	11.672
28) SA Decachlor...	9.022	7.859	22487896	14972555	13.984	11.248

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091523\
Data File : PL085341.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Sep 2023 17:46
Operator : AR\AJ
Sample : 04423-01
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
HD-01-09132023


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 09/15/2023
Supervised By : Ankita Jodhani 09/15/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 14 22:21:04 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090523.M
Quant Title : GC Extractables
QLast Update : Tue Sep 05 15:22:36 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

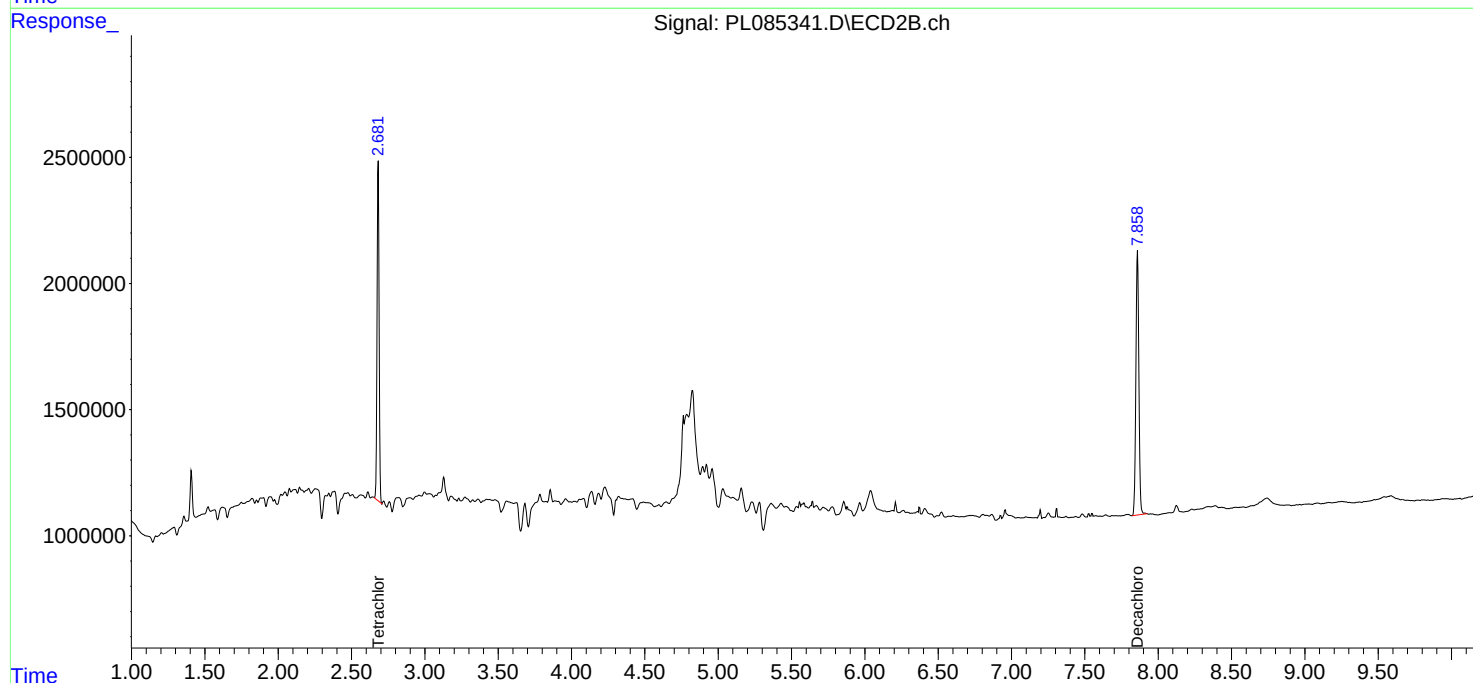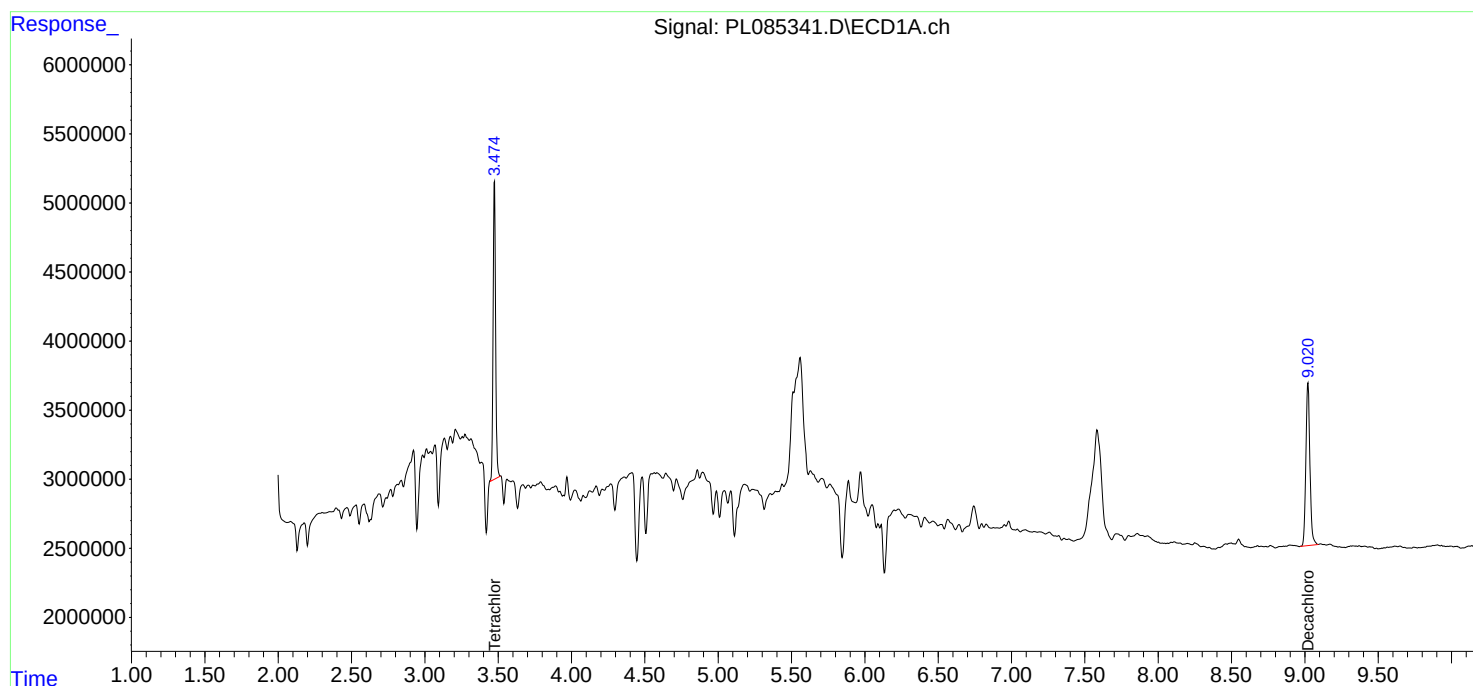

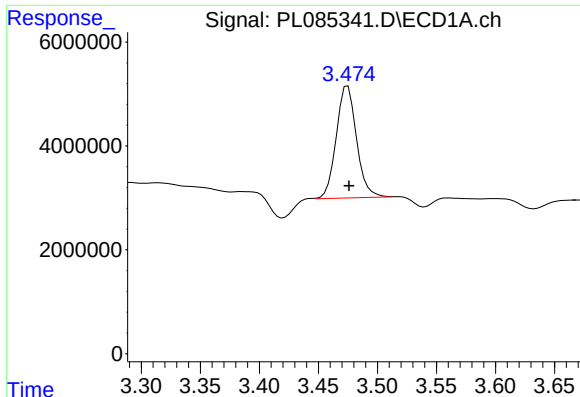


#1 Tetrachloro-m-xylene

R.T.: 3.474 min
Delta R.T.: -0.002 min
Response: 25731564
Conc: 10.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
HD-01-09132023


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/15/2023
Supervised By :Ankita Jodhani 09/15/2023

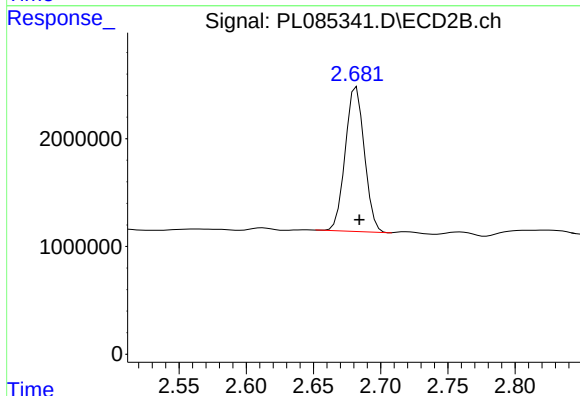


#1 Tetrachloro-m-xylene

R.T.: 2.682 min
Delta R.T.: -0.002 min
Response: 13261584
Conc: 11.67 ng/ml

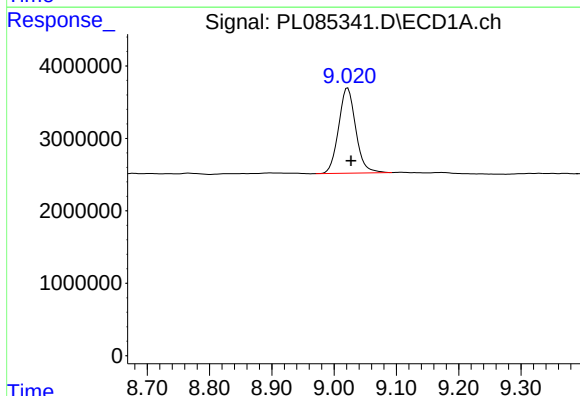

#28 Decachlorobiphenyl

R.T.: 9.022 min
Delta R.T.: -0.005 min
Response: 22487896
Conc: 13.98 ng/ml

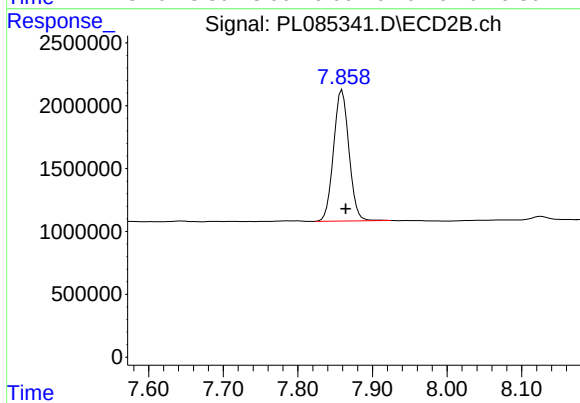

#28 Decachlorobiphenyl

R.T.: 7.859 min
Delta R.T.: -0.005 min
Response: 14972555
Conc: 11.25 ng/ml