

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091523\
 Data File : PL085351.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Sep 2023 20:08
 Operator : AR\AJ
 Sample : 04436-04
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 B103-05

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 14 22:24:04 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090523.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 05 15:22:36 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.475	2.683	34061671	16022878	13.926	14.102
28)	SA Decachlor...	9.021	7.860	18622206	13677275	11.580	10.275
Target Compounds							
11)	B alpha-Chl...	5.972	4.960	2971760	478772	1.155	0.320 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091523\
Data File : PL085351.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Sep 2023 20:08
Operator : AR\AJ
Sample : 04436-04
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
B103-05

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 14 22:24:04 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090523.M
Quant Title : GC Extractables
QLast Update : Tue Sep 05 15:22:36 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

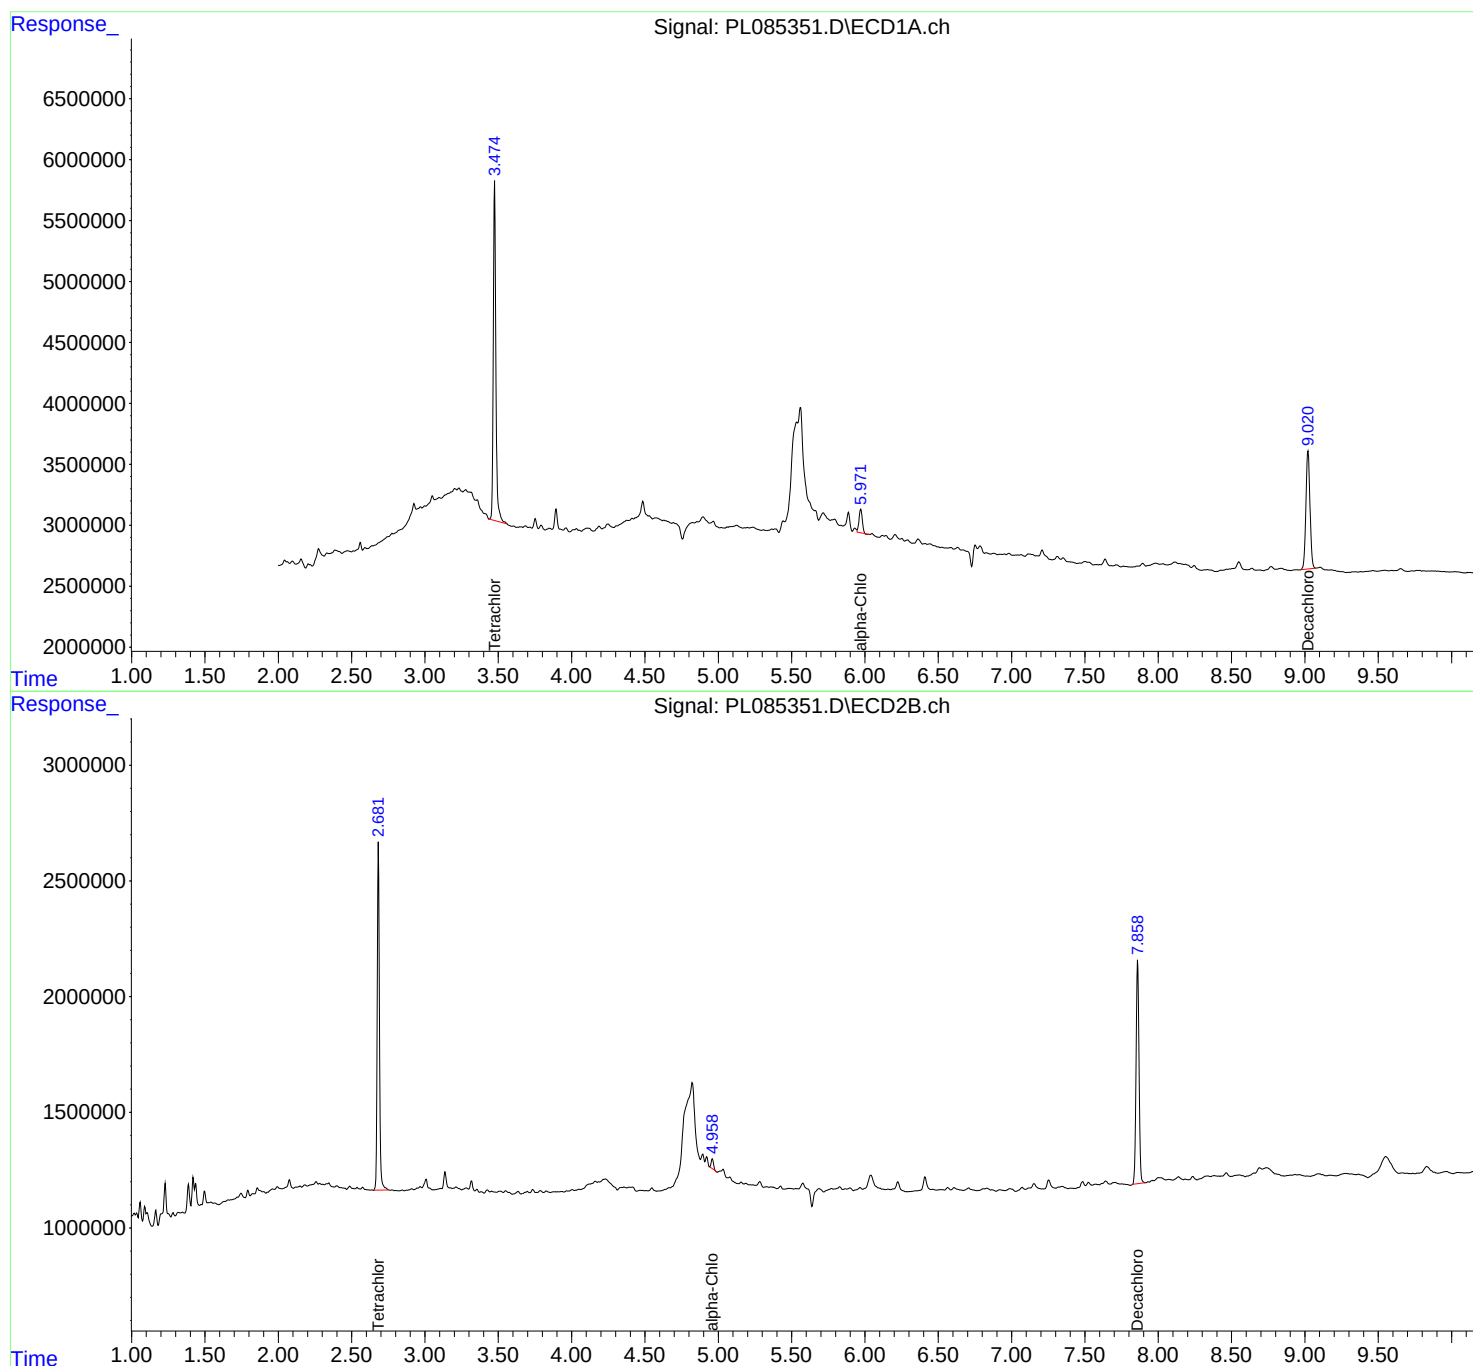


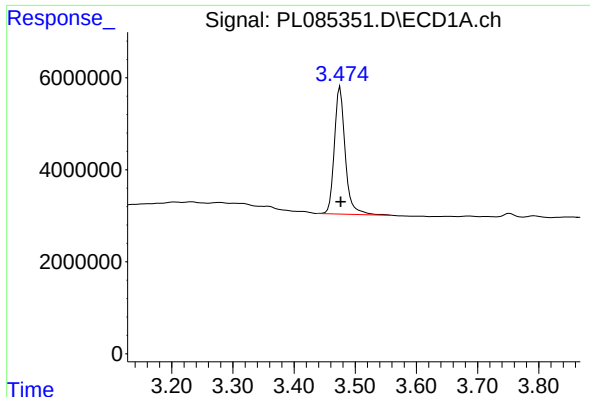

#1 Tetrachloro-m-xylene


R.T.: 3.475 min
Delta R.T.: 0.000 min
Response: 34061671
Conc: 13.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
B103-05

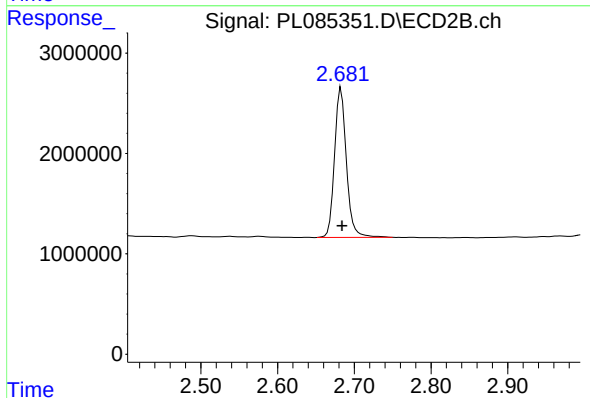


#1 Tetrachloro-m-xylene

R.T.: 2.683 min
Delta R.T.: -0.001 min
Response: 16022878
Conc: 14.10 ng/ml

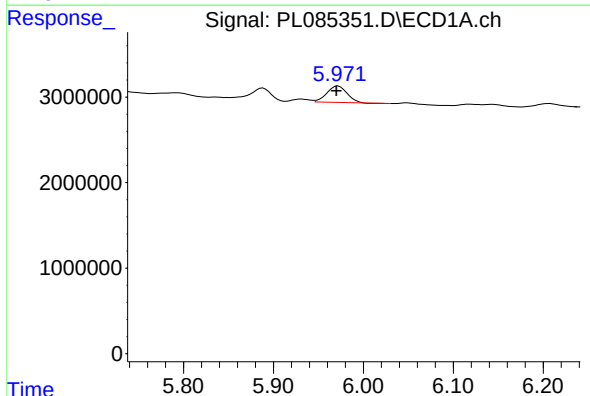


#11 alpha-Chlordane

R.T.: 5.972 min
Delta R.T.: 0.002 min
Response: 2971760
Conc: 1.15 ng/ml

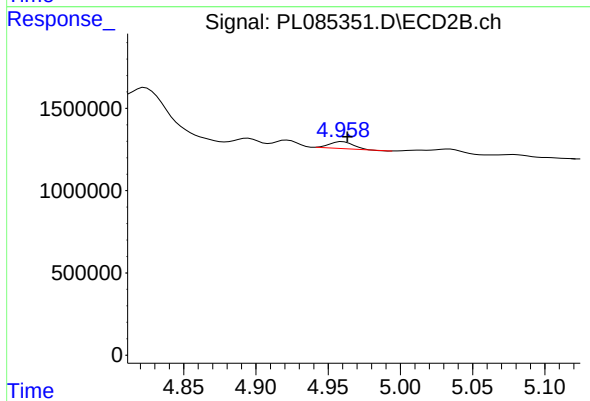

#11 alpha-Chlordane


R.T.: 4.960 min
Delta R.T.: -0.003 min
Response: 478772
Conc: 0.32 ng/ml

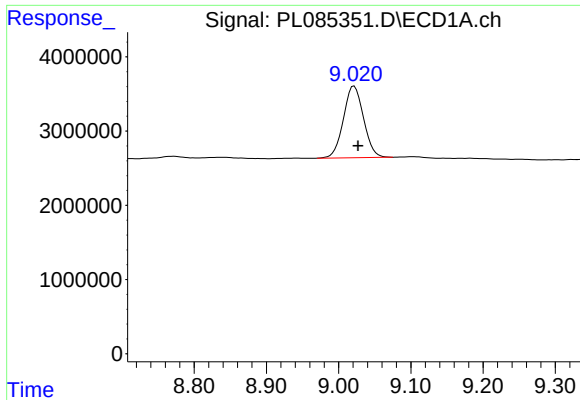

#28 Decachlorobiphenyl

R.T.: 9.021 min
Delta R.T.: -0.006 min
Response: 18622206
Conc: 11.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
B103-05

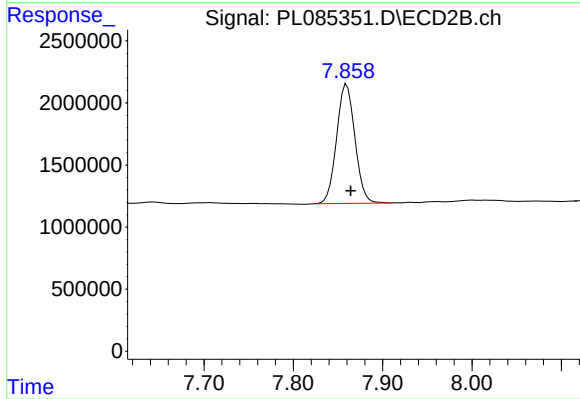

#28 Decachlorobiphenyl

R.T.: 7.860 min
Delta R.T.: -0.005 min
Response: 13677275
Conc: 10.28 ng/ml