

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091523\
 Data File : PL085353.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Sep 2023 20:36
 Operator : AR\AJ
 Sample : 04436-08
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CPT103-02

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 14 22:24:39 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090523.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 05 15:22:36 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.475	2.683	34145953	16260796	13.960	14.312
28)	SA Decachlor...	9.022	7.860	13857869	10231241	8.618	7.686
Target Compounds							
12)	B 4,4'-DDE	6.146	5.158	3829753	2063745	1.842	1.659
17)	MA 4,4'-DDT	6.982	5.967	2780087	1682377	1.650	1.443



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091523\
Data File : PL085353.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Sep 2023 20:36
Operator : AR\AJ
Sample : 04436-08
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
CPT103-02

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 14 22:24:39 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090523.M
Quant Title : GC Extractables
QLast Update : Tue Sep 05 15:22:36 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

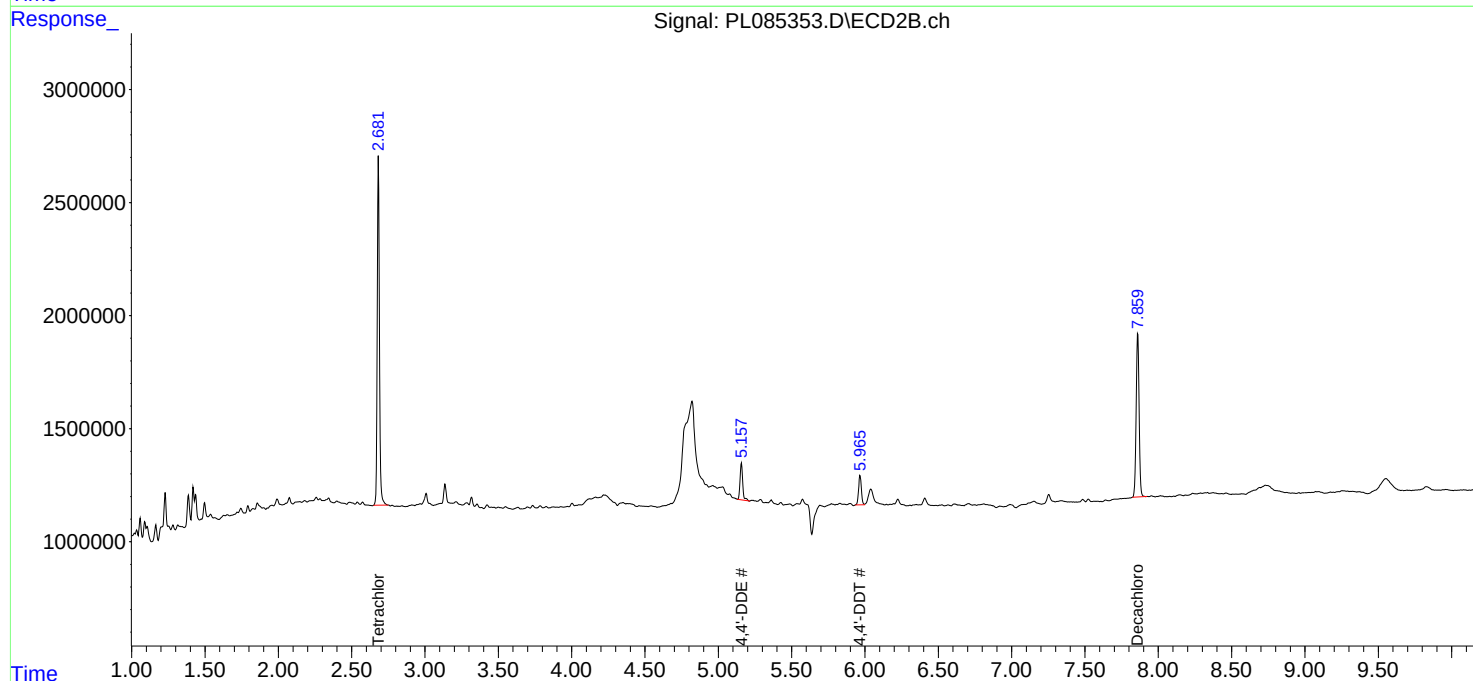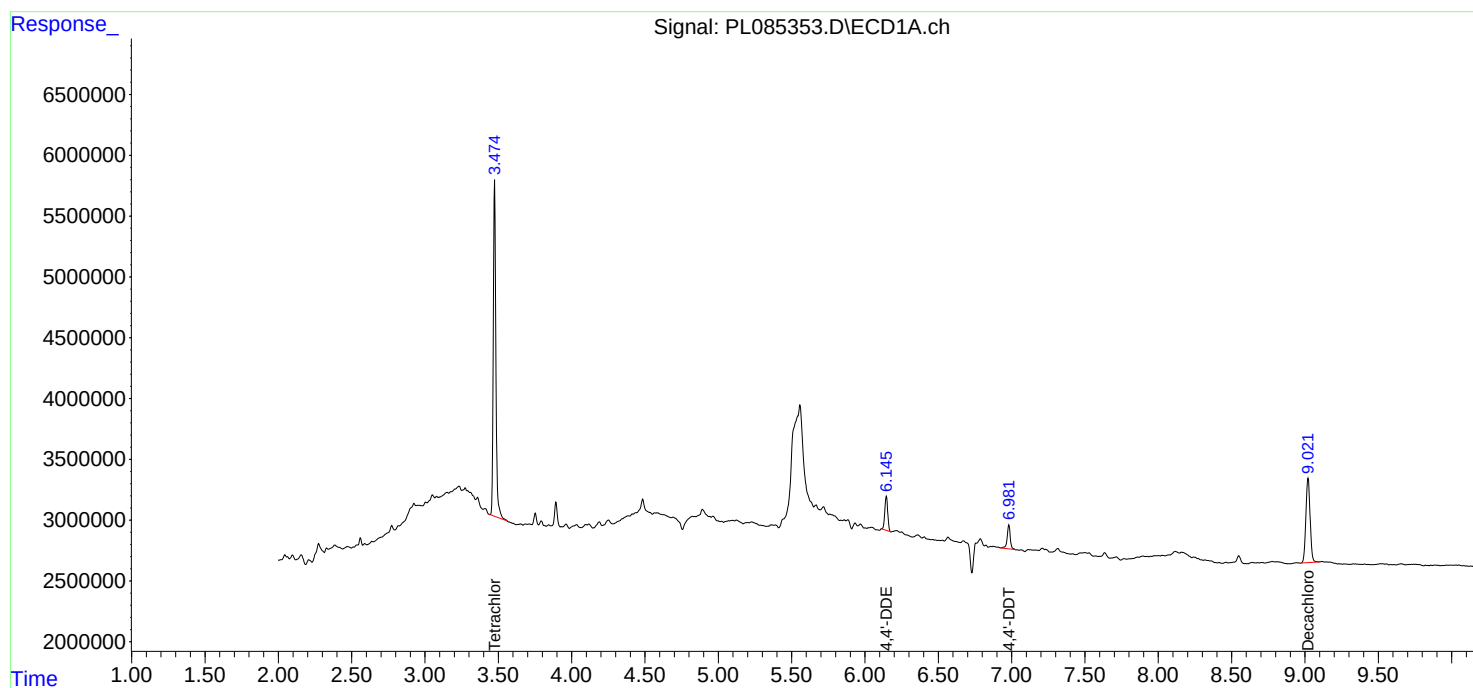


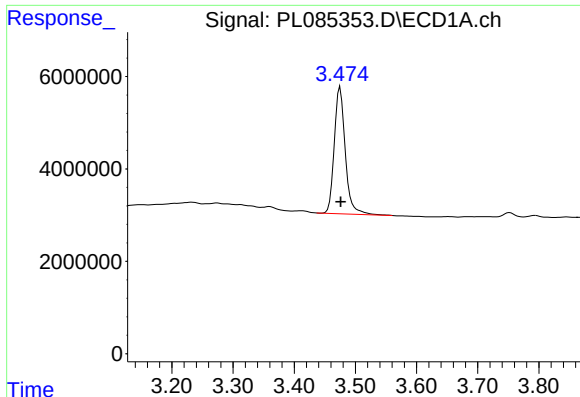

#1 Tetrachloro-m-xylene


R.T.: 3.475 min
Delta R.T.: 0.000 min
Response: 34145953
Conc: 13.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
CPT103-02

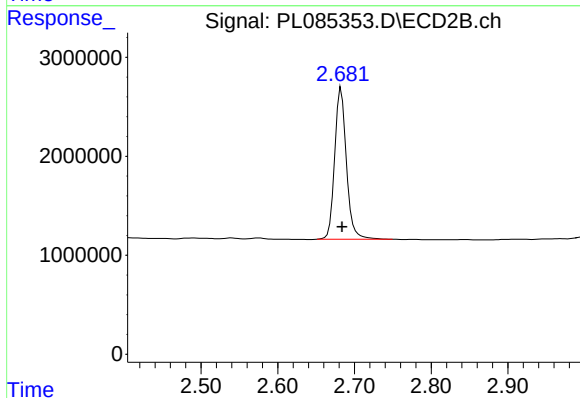


#1 Tetrachloro-m-xylene

R.T.: 2.683 min
Delta R.T.: -0.002 min
Response: 16260796
Conc: 14.31 ng/ml

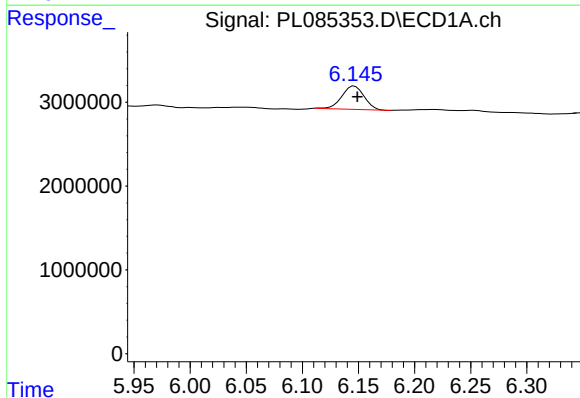


#12 4,4'-DDE

R.T.: 6.146 min
Delta R.T.: -0.003 min
Response: 3829753
Conc: 1.84 ng/ml

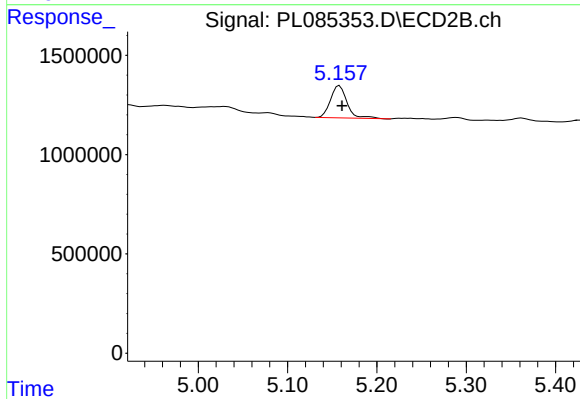

#12 4,4'-DDE


R.T.: 5.158 min
Delta R.T.: -0.003 min
Response: 2063745
Conc: 1.66 ng/ml

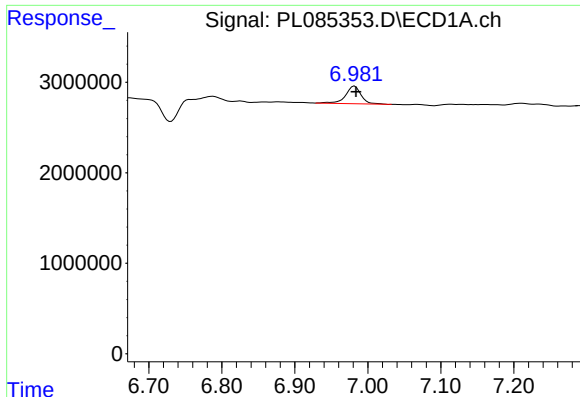

#17 4,4'-DDT


R.T.: 6.982 min
Delta R.T.: -0.002 min
Response: 2780087
Conc: 1.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
CPT103-02

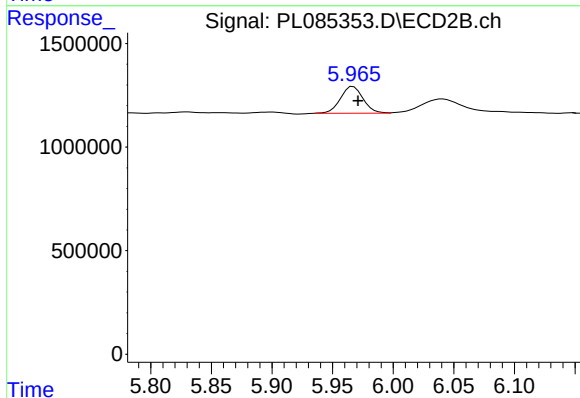


#17 4,4'-DDT

R.T.: 5.967 min
Delta R.T.: -0.004 min
Response: 1682377
Conc: 1.44 ng/ml

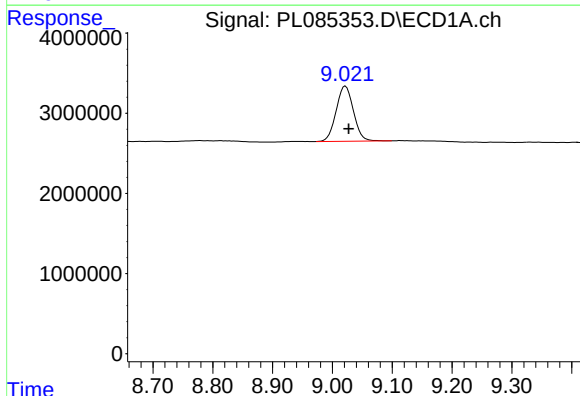

#28 Decachlorobiphenyl

R.T.: 9.022 min
Delta R.T.: -0.005 min
Response: 13857869
Conc: 8.62 ng/ml

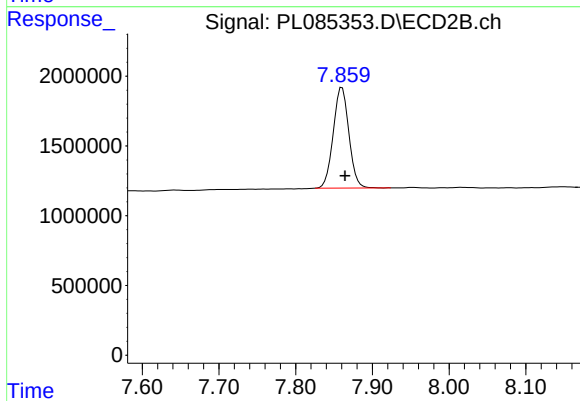

#28 Decachlorobiphenyl

R.T.: 7.860 min
Delta R.T.: -0.004 min
Response: 10231241
Conc: 7.69 ng/ml