

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091523\
 Data File : PL085356.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Sep 2023 21:18
 Operator : AR\AJ
 Sample : 04436-14
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CPT102-23

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/15/2023
 Supervised By : Ankita Jodhani 09/15/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 14 22:25:31 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090523.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 05 15:22:36 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.475	2.682	32622847	15265773	13.338	13.436
28)	SA Decachlor...	9.022	7.859	13451448	9885485	8.365	7.427
Target Compounds							
17)	MA 4,4'-DDT	6.975	5.972	709996	494268	0.421m	0.424

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091523\
Data File : PL085356.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Sep 2023 21:18
Operator : AR\AJ
Sample : 04436-14
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
CPT102-23


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 09/15/2023
Supervised By : Ankita Jodhani 09/15/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 14 22:25:31 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090523.M
Quant Title : GC Extractables
QLast Update : Tue Sep 05 15:22:36 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

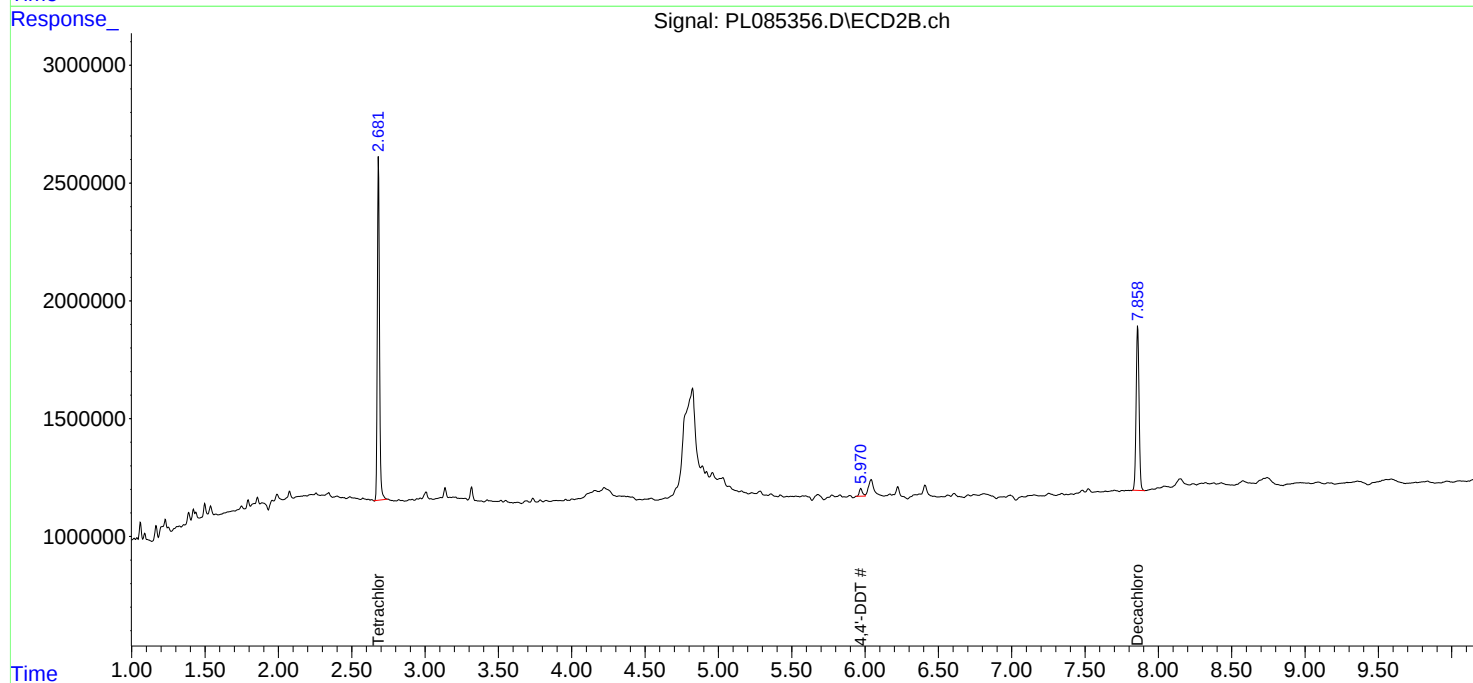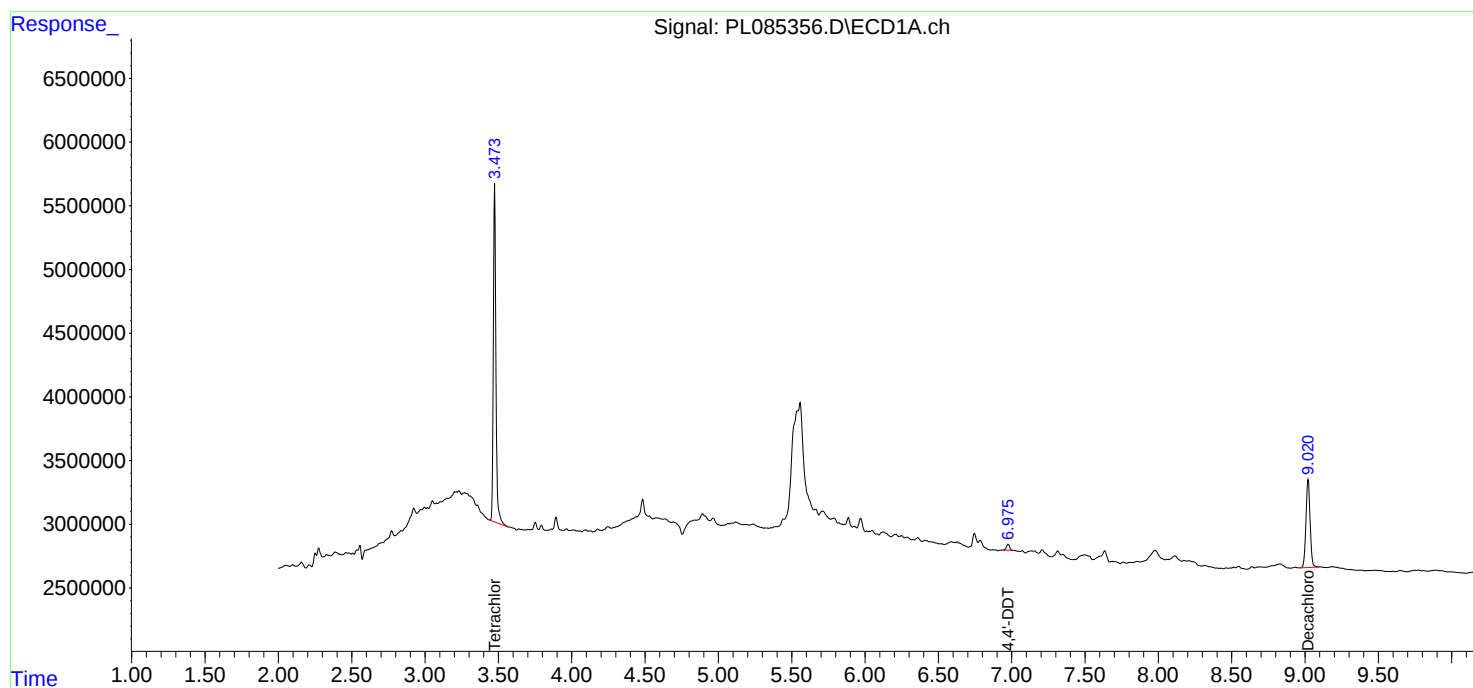

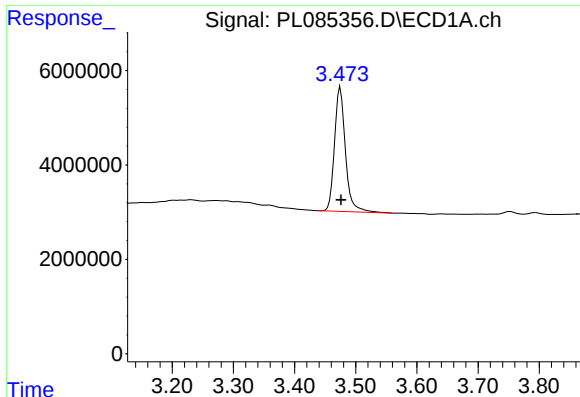


#1 Tetrachloro-m-xylene

R.T.: 3.475 min
Delta R.T.: -0.001 min
Response: 32622847
Conc: 13.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
CPT102-23


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/15/2023
Supervised By :Ankita Jodhani 09/15/2023

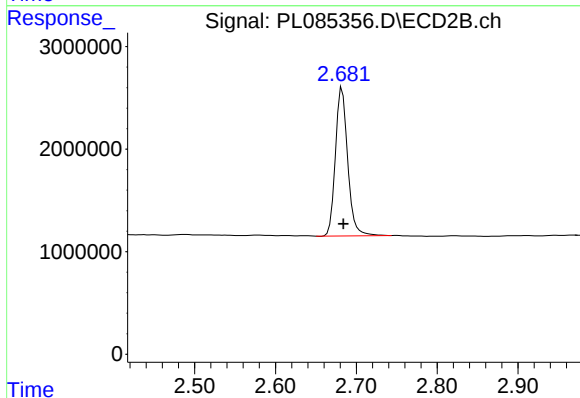


#1 Tetrachloro-m-xylene

R.T.: 2.682 min
Delta R.T.: -0.002 min
Response: 15265773
Conc: 13.44 ng/ml

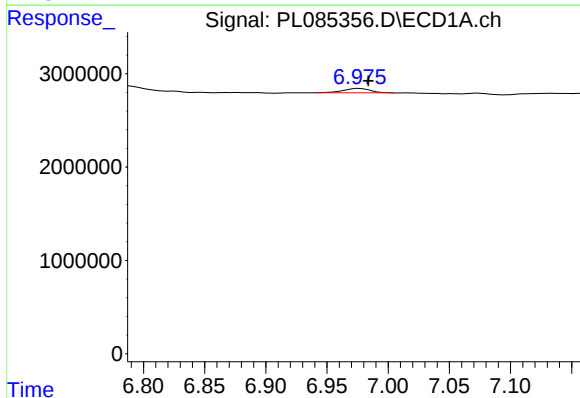


#17 4,4'-DDT

R.T.: 6.975 min
Delta R.T.: -0.009 min
Response: 709996
Conc: 0.42 ng/ml m

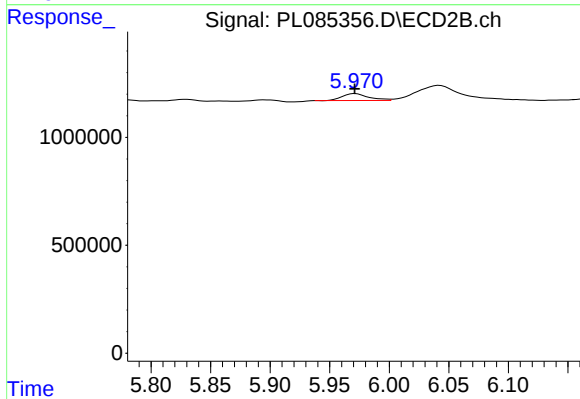

#17 4,4'-DDT

R.T.: 5.972 min
Delta R.T.: 0.000 min
Response: 494268
Conc: 0.42 ng/ml

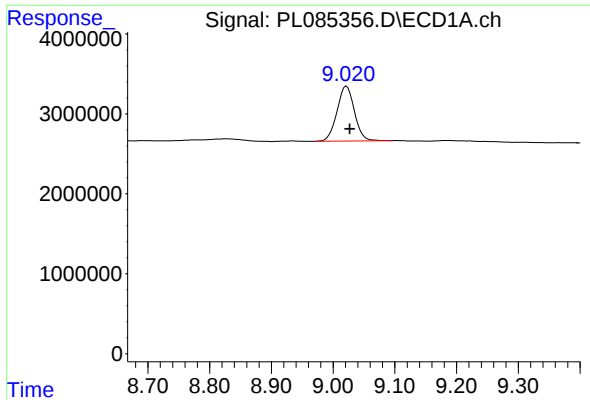


#28 Decachlorobiphenyl

R.T.: 9.022 min
Delta R.T.: -0.005 min
Response: 13451448
Conc: 8.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
CPT102-23

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/15/2023
Supervised By :Ankita Jodhani 09/15/2023

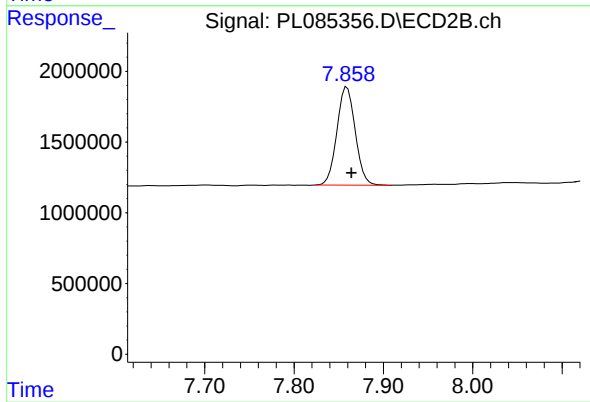

#28 Decachlorobiphenyl

R.T.: 7.859 min
Delta R.T.: -0.005 min
Response: 9885485
Conc: 7.43 ng/ml