

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091620\
 Data File : PL061517.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Sep 2020 15:10
 Operator : DD\AJ
 Sample : L4021-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 B14-1-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 17 01:02:14 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 09 01:27:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.459	4.008	27205579	50086796	15.774	16.283
28)	SA Decachlor...	8.209	9.093	25438150	38428964	15.248	16.252
Target Compounds							
11)	B alpha-Chl...	0.000	6.196	0	2317789	N.D.	0.666 #
12)	B 4,4'-DDE	5.620	6.350	2602502	5771799	1.531	1.801
17)	MA 4,4'-DDT	6.373	0.000	3232500	0	2.354	N.D. #
26)	Chlordane-4	0.000	6.196	0	2317789	N.D.	4.428 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091620\
Data File : PL061517.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Sep 2020 15:10
Operator : DD\AJ
Sample : L4021-01
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
B14-1-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 01:02:14 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
Quant Title : GC Extractables
QLast Update : Wed Sep 09 01:27:38 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

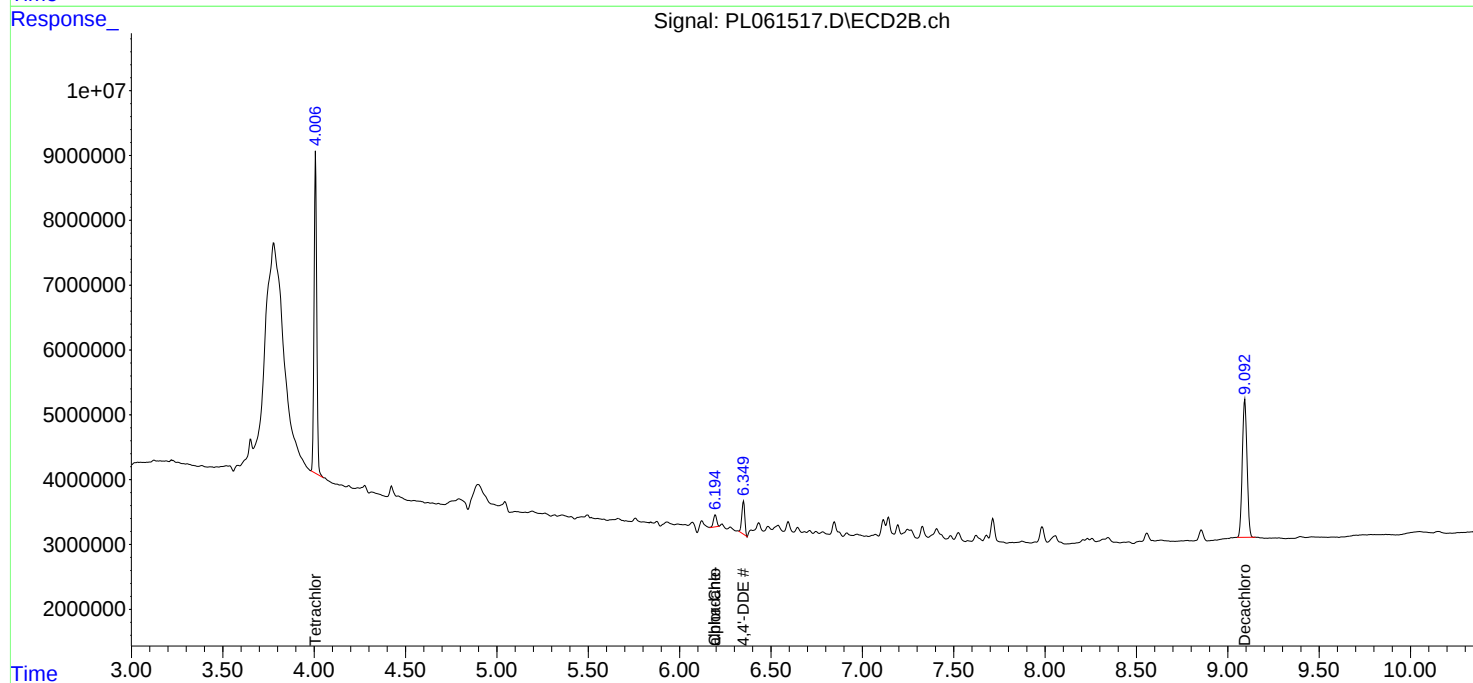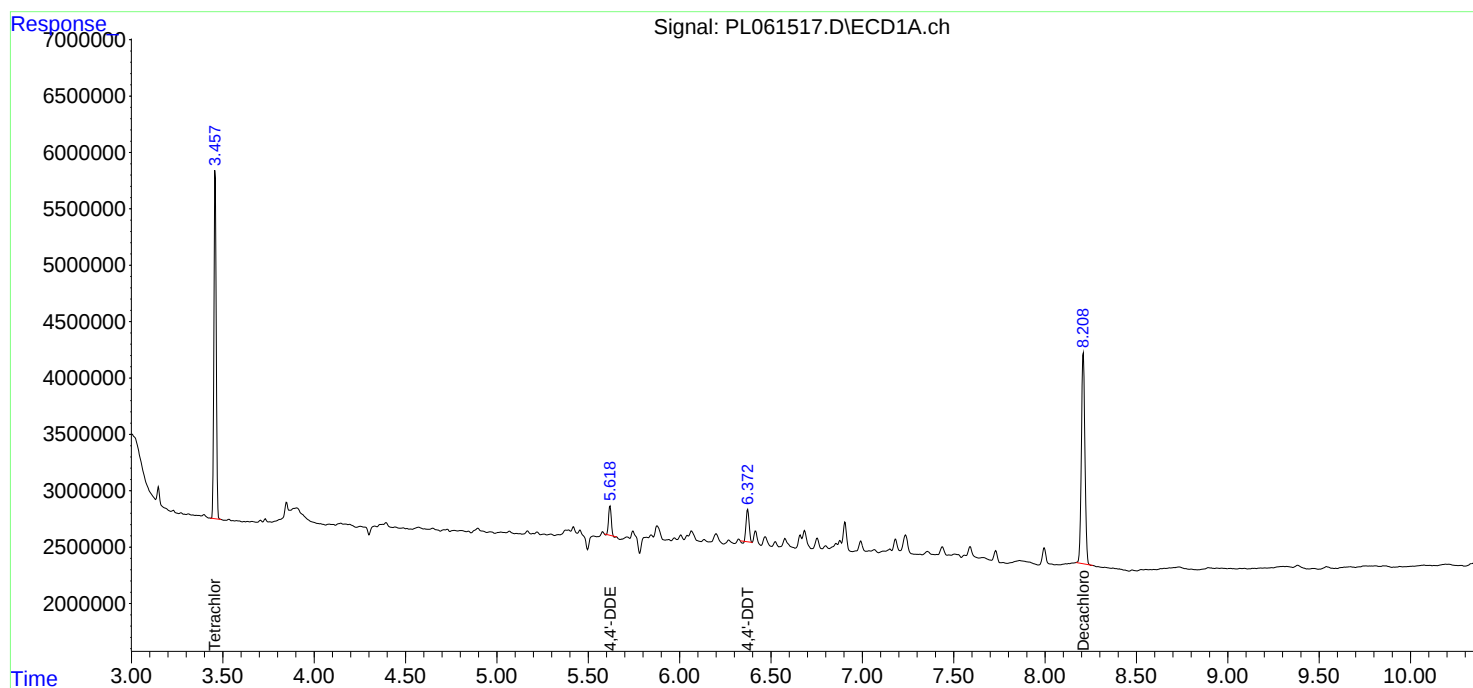


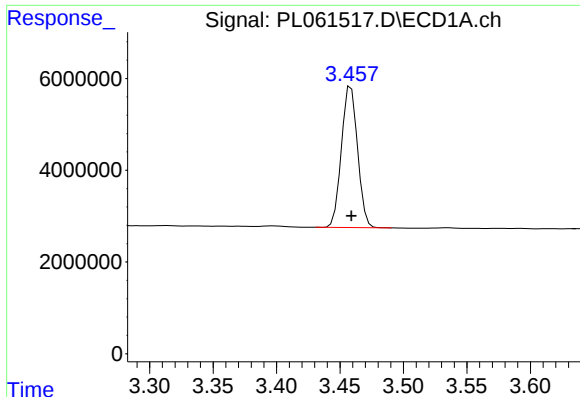

#1 Tetrachloro-m-xylene


R.T.: 3.459 min
Delta R.T.: 0.000 min
Response: 27205579
Conc: 15.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
B14-1-3

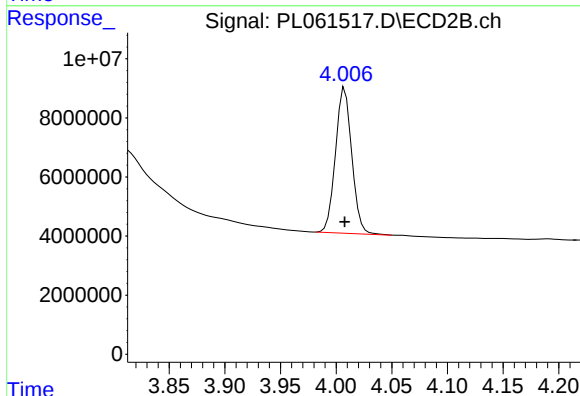


#1 Tetrachloro-m-xylene

R.T.: 4.008 min
Delta R.T.: 0.000 min
Response: 50086796
Conc: 16.28 ng/ml

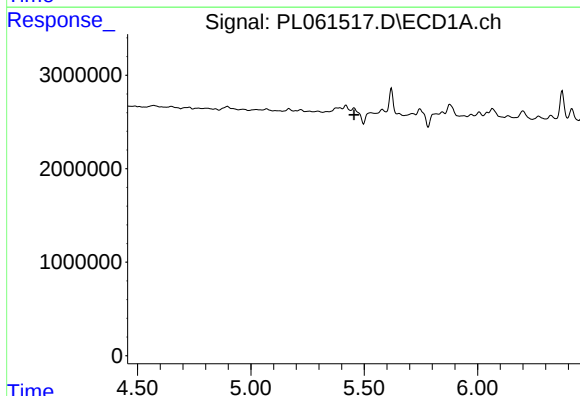


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.456 min
Response: 0
Conc: N.D.

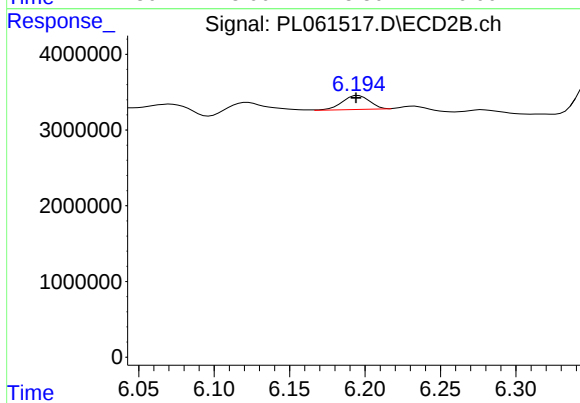

#11 alpha-Chlordane


R.T.: 6.196 min
Delta R.T.: 0.002 min
Response: 2317789
Conc: 0.67 ng/ml

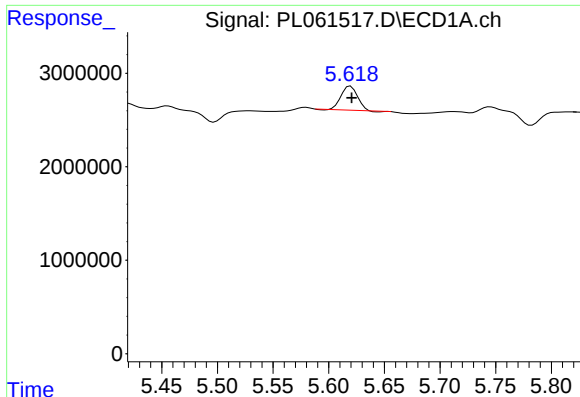

#12 4,4'-DDE


R.T.: 5.620 min
Delta R.T.: -0.001 min
Response: 2602502
Conc: 1.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
B14-1-3

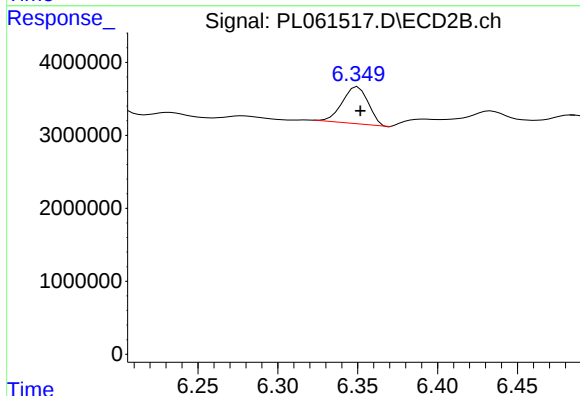


#12 4,4'-DDE

R.T.: 6.350 min
Delta R.T.: -0.002 min
Response: 5771799
Conc: 1.80 ng/ml

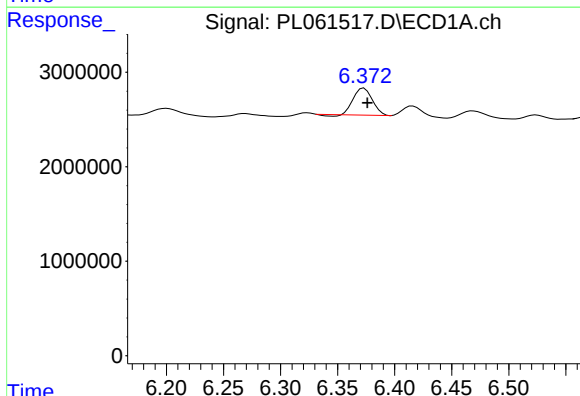


#17 4,4'-DDT

R.T.: 6.373 min
Delta R.T.: -0.003 min
Response: 3232500
Conc: 2.35 ng/ml

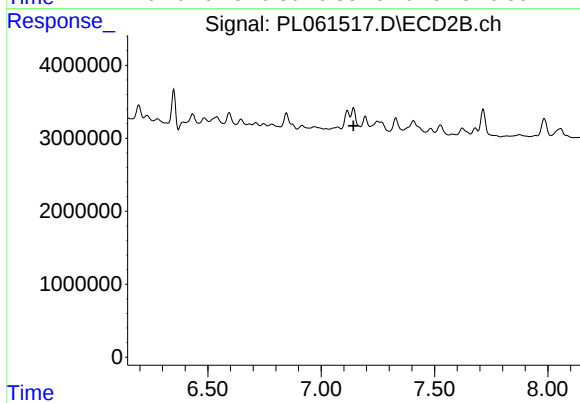

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 7.143 min
Response: 0
Conc: N.D.

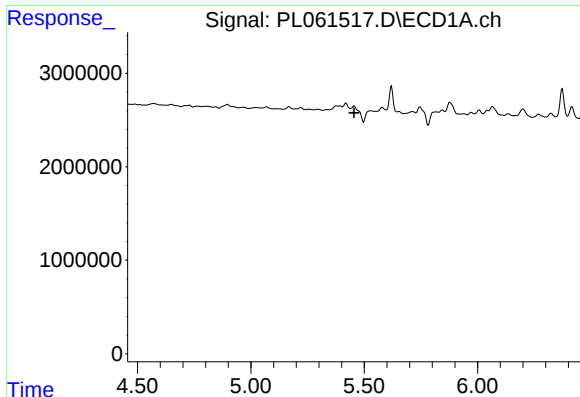

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.456 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
B14-1-3

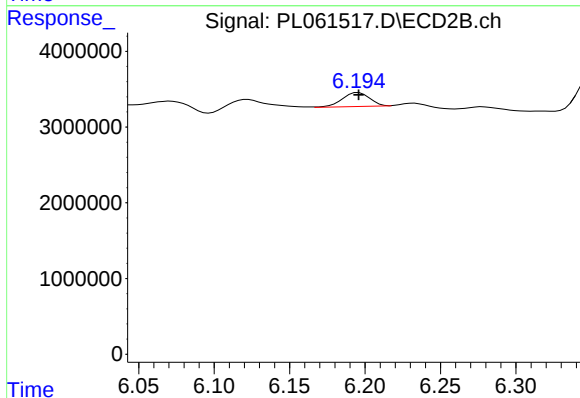


#26 Chlordane-4

R.T.: 6.196 min
Delta R.T.: 0.000 min
Response: 2317789
Conc: 4.43 ng/ml

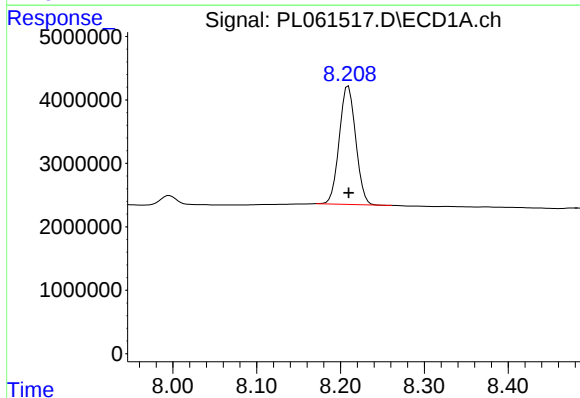

#28 Decachlorobiphenyl

R.T.: 8.209 min
Delta R.T.: 0.000 min
Response: 25438150
Conc: 15.25 ng/ml

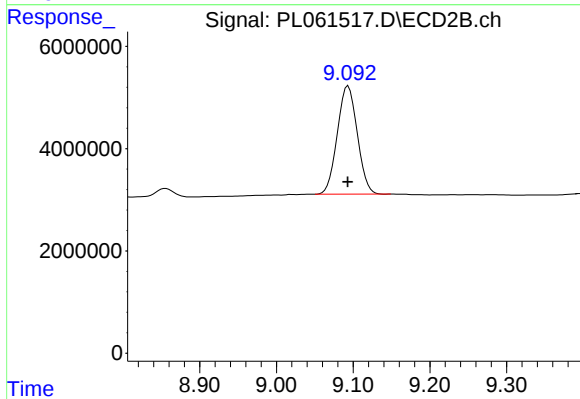

#28 Decachlorobiphenyl

R.T.: 9.093 min
Delta R.T.: 0.000 min
Response: 38428964
Conc: 16.25 ng/ml