

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091620\
 Data File : PL061519.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Sep 2020 15:39
 Operator : DD\AJ
 Sample : L4021-03
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 B15-1-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 17 01:02:32 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 09 01:27:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.459	4.008	38772703	69186810	22.481	22.493
28)	SA Decachlor...	8.209	9.095	26589006	38271296	15.938	16.185
Target Compounds							
2)	A alpha-BHC	0.000	4.423f	0	3730988	N.D.	0.808 #
10)	B gamma-Chl...	0.000	6.128	0	4293470	N.D.	1.245 #
15)	B Endosulfa...	0.000	6.945f	0	7428854	N.D.	2.515 #
21)	B Endrin ke...	0.000	7.748	0	3035647	N.D.	1.118 #
23)	Chlordane-1	4.329	0.000	1224919	0	23.351	N.D. #
25)	Chlordane-3	0.000	6.128	0	4293470	N.D.	9.939 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091620\
Data File : PL061519.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Sep 2020 15:39
Operator : DD\AJ
Sample : L4021-03
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
B15-1-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 01:02:32 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
Quant Title : GC Extractables
QLast Update : Wed Sep 09 01:27:38 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

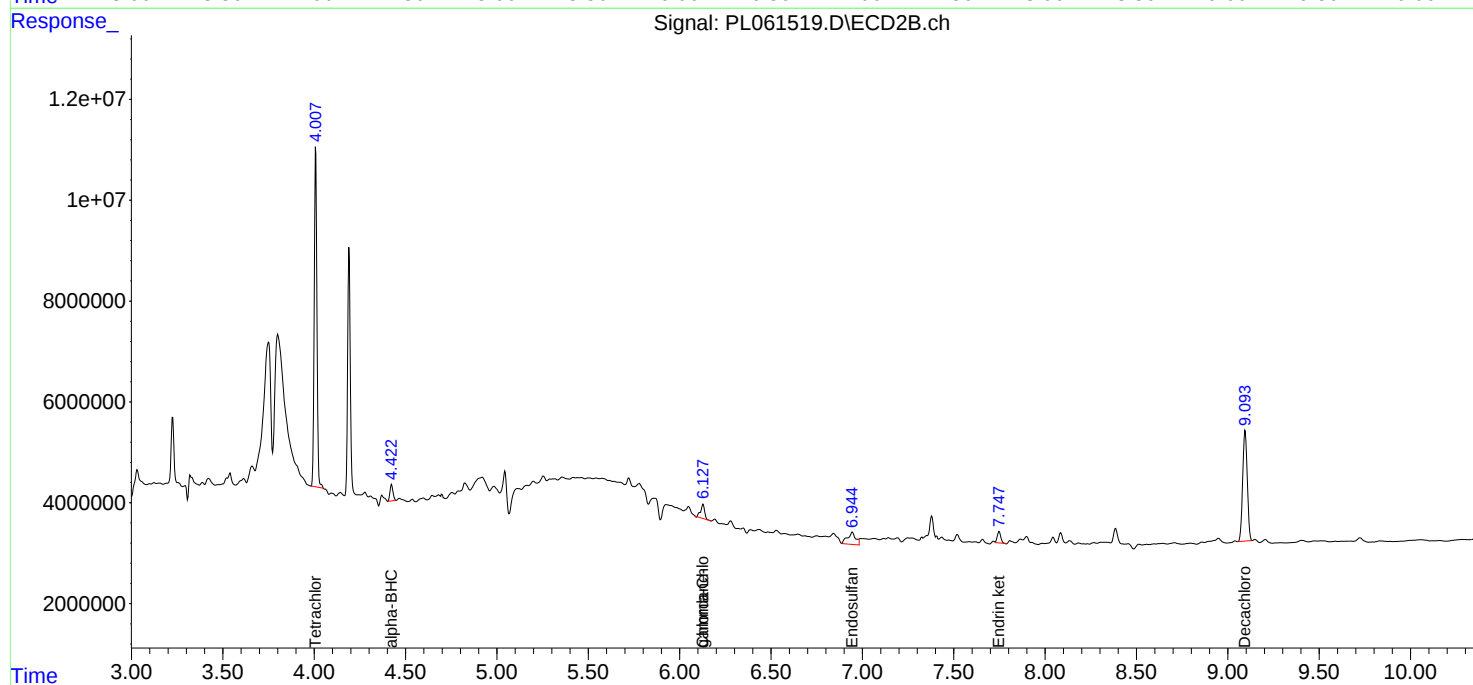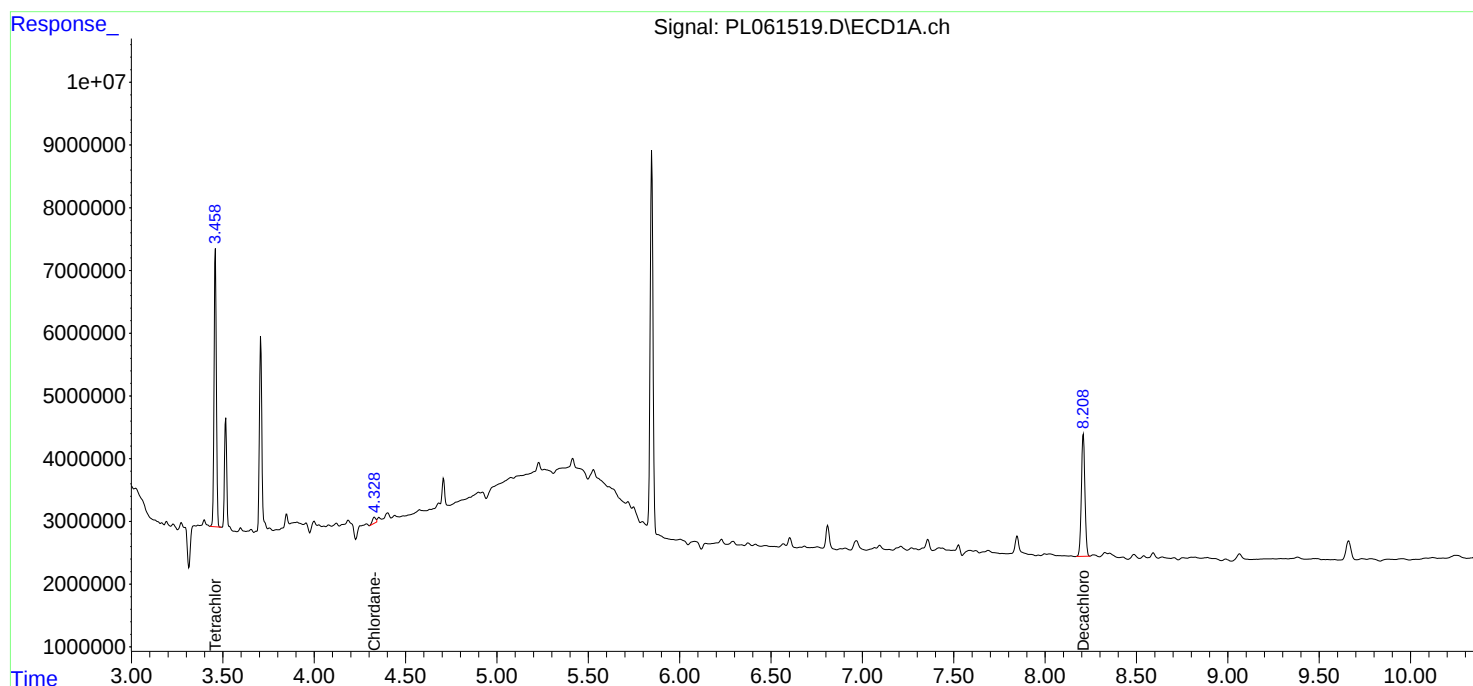


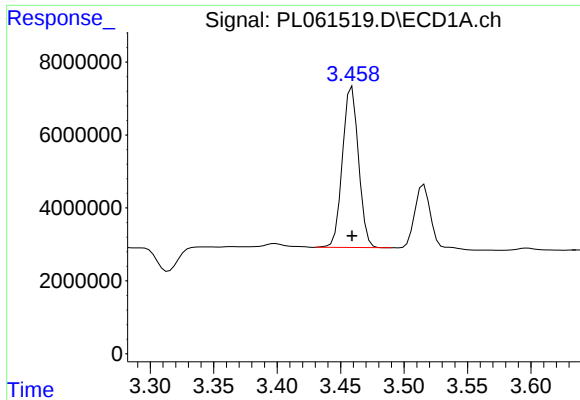

#1 Tetrachloro-m-xylene


R.T.: 3.459 min
Delta R.T.: 0.000 min
Response: 38772703
Conc: 22.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
B15-1-3

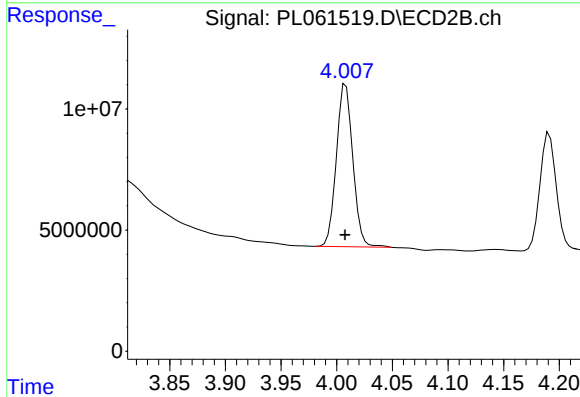


#1 Tetrachloro-m-xylene

R.T.: 4.008 min
Delta R.T.: 0.000 min
Response: 69186810
Conc: 22.49 ng/ml

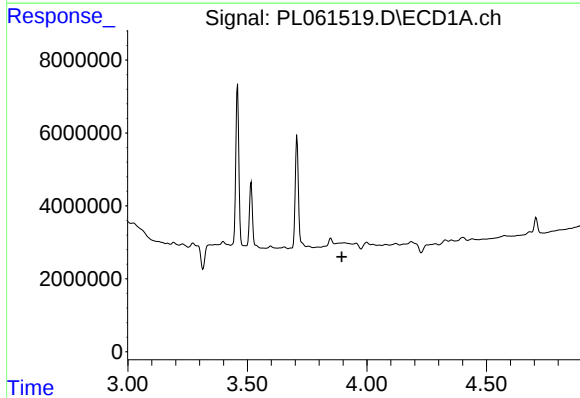


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.895 min
Response: 0
Conc: N.D.

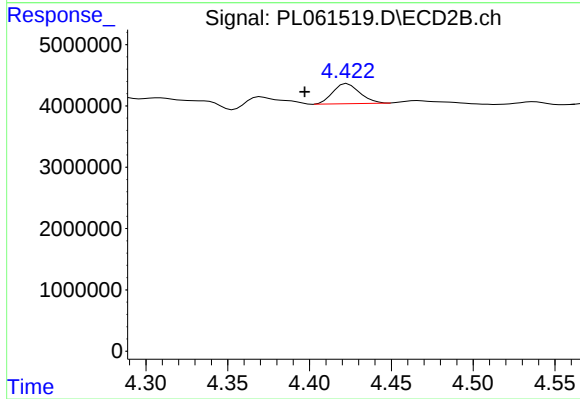

#2 alpha-BHC


R.T.: 4.423 min
Delta R.T.: 0.026 min
Response: 3730988
Conc: 0.81 ng/ml

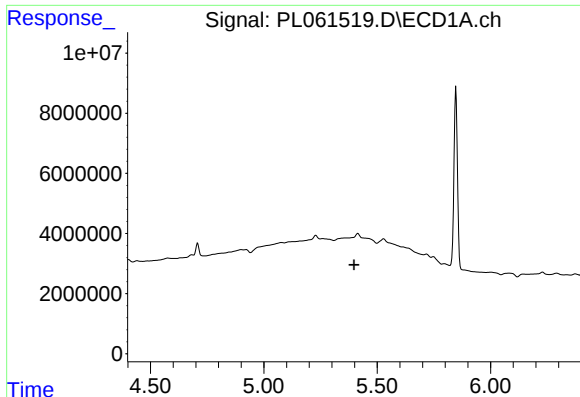

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.398 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
B15-1-3

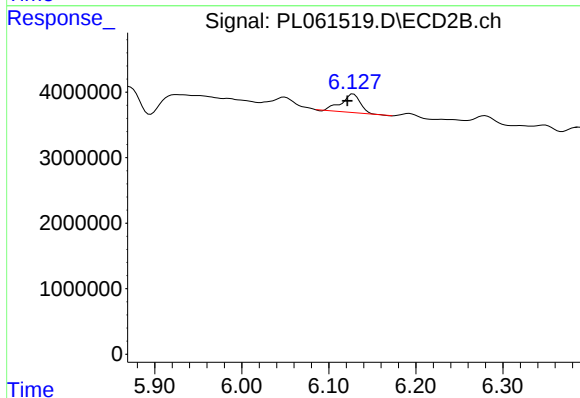


#10 gamma-Chlordane

R.T.: 6.128 min
Delta R.T.: 0.007 min
Response: 4293470
Conc: 1.25 ng/ml

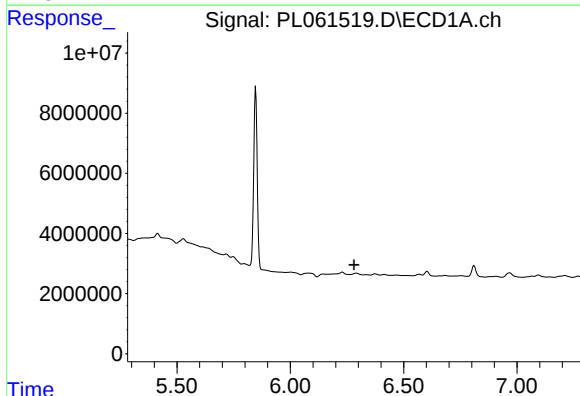


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.281 min
Response: 0
Conc: N.D.

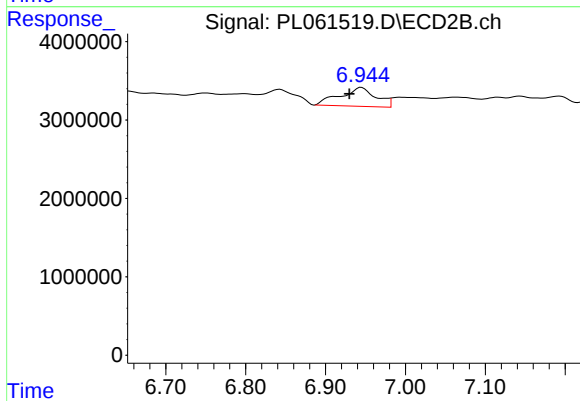

#15 Endosulfan II


R.T.: 6.945 min
Delta R.T.: 0.015 min
Response: 7428854
Conc: 2.52 ng/ml

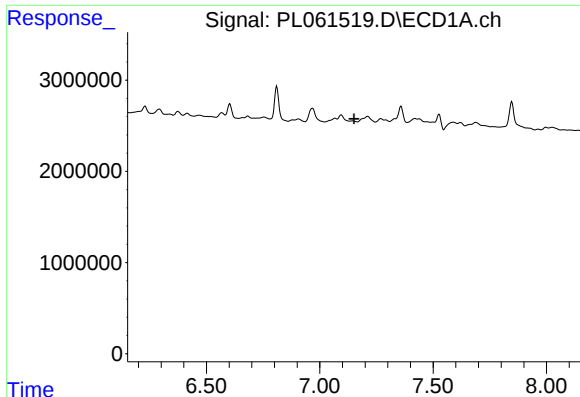

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.151 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
B15-1-3

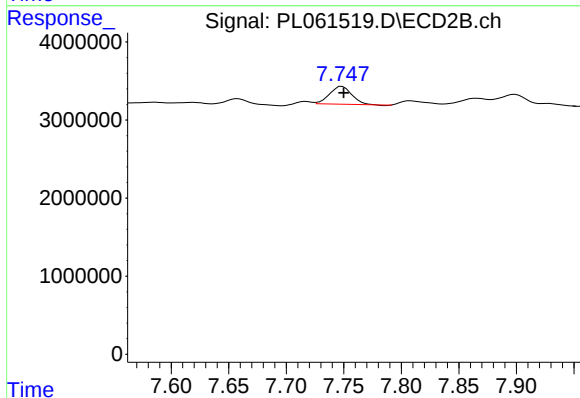


#21 Endrin ketone

R.T.: 7.748 min
Delta R.T.: -0.002 min
Response: 3035647
Conc: 1.12 ng/ml

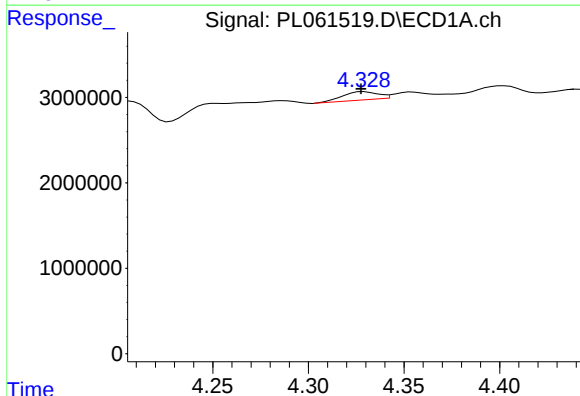


#23 Chlordane-1

R.T.: 4.329 min
Delta R.T.: 0.001 min
Response: 1224919
Conc: 23.35 ng/ml

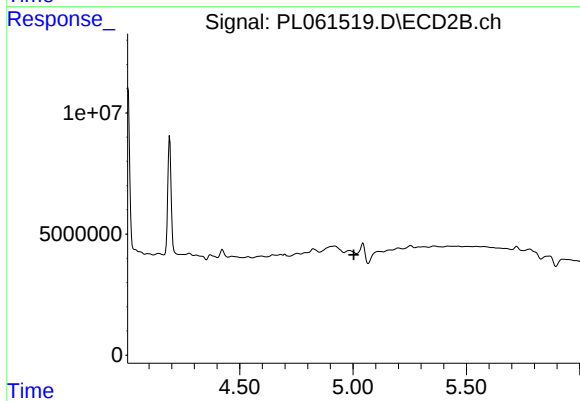

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.004 min
Response: 0
Conc: N.D.

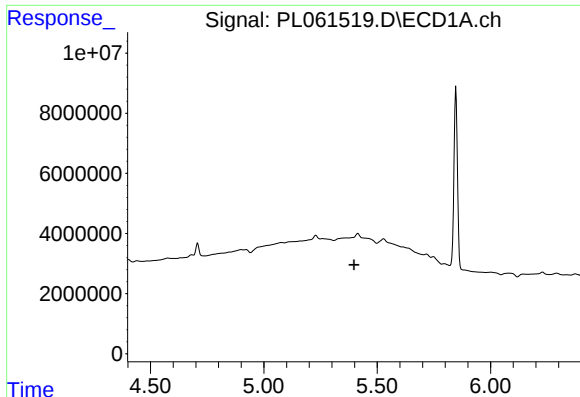

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.398 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
B15-1-3

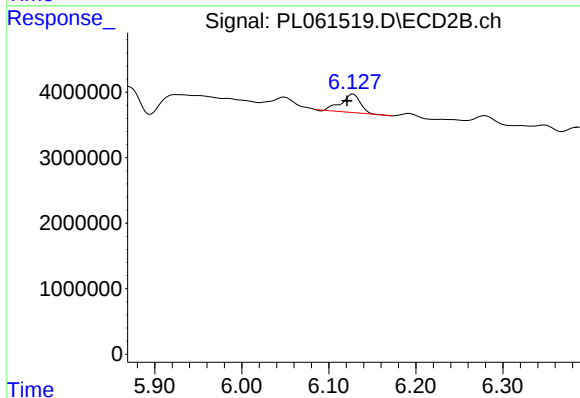


#25 Chlordane-3

R.T.: 6.128 min
Delta R.T.: 0.007 min
Response: 4293470
Conc: 9.94 ng/ml

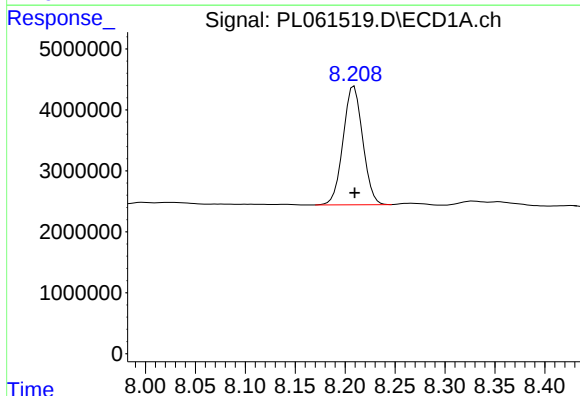

#28 Decachlorobiphenyl

R.T.: 8.209 min
Delta R.T.: 0.000 min
Response: 26589006
Conc: 15.94 ng/ml

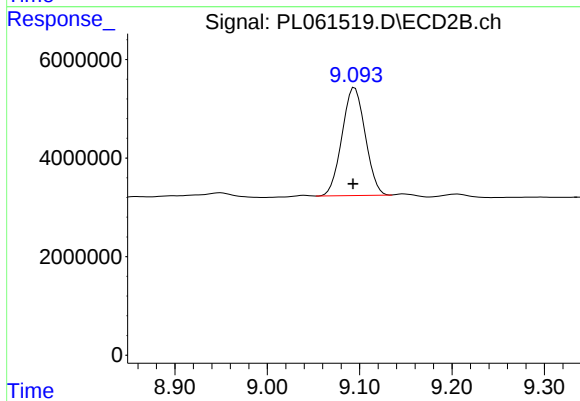

#28 Decachlorobiphenyl

R.T.: 9.095 min
Delta R.T.: 0.002 min
Response: 38271296
Conc: 16.19 ng/ml