

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091620\
 Data File : PL061521.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Sep 2020 16:07
 Operator : DD\AJ
 Sample : L4021-05
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 B15A-5-7

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 17 01:02:51 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 09 01:27:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.459	4.007	40106438	73169032	23.254	23.787
28) SA Decachlor...	8.210	9.094	32263363	47787212	19.339	20.210
Target Compounds						
15) B Endosulfa...	0.000	6.945f	0	3819548	N.D.	1.293 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091620\
Data File : PL061521.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Sep 2020 16:07
Operator : DD\AJ
Sample : L4021-05
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
B15A-5-7

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 01:02:51 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
Quant Title : GC Extractables
QLast Update : Wed Sep 09 01:27:38 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

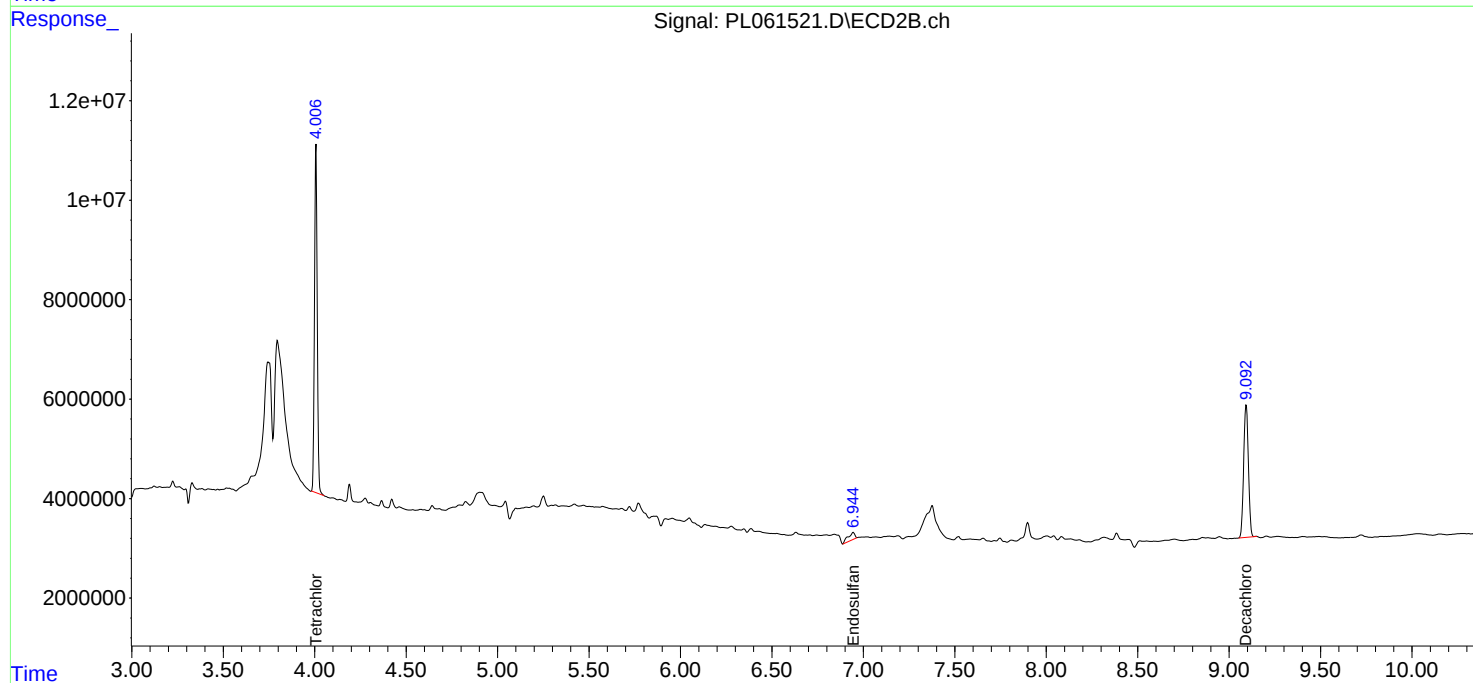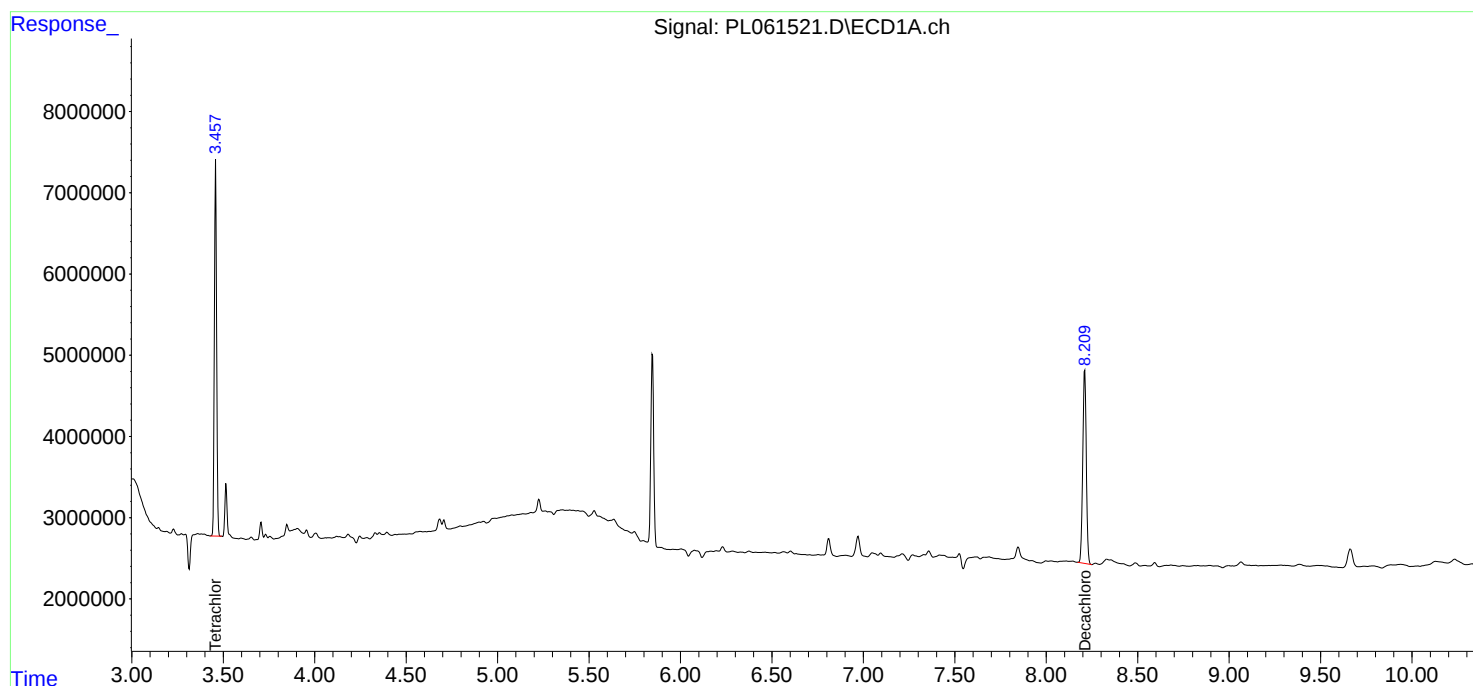


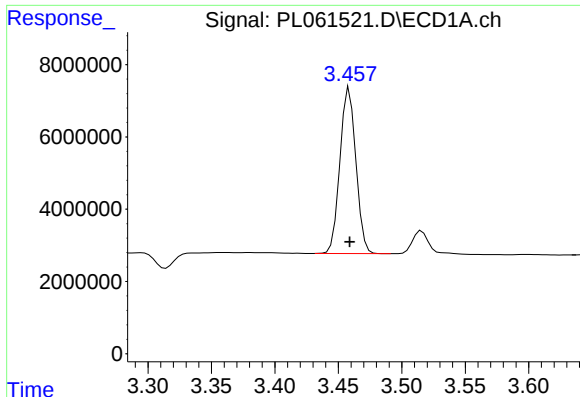

#1 Tetrachloro-m-xylene


R.T.: 3.459 min
Delta R.T.: 0.000 min
Response: 40106438
Conc: 23.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
B15A-5-7

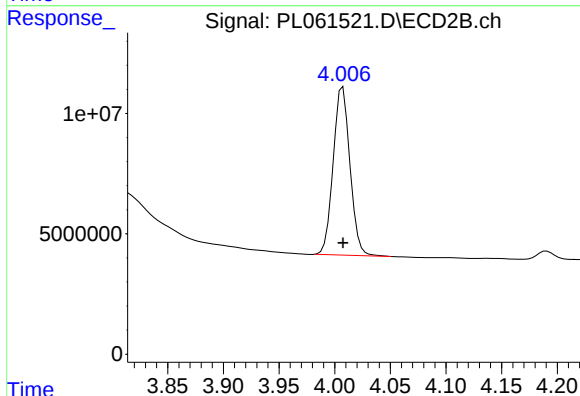


#1 Tetrachloro-m-xylene

R.T.: 4.007 min
Delta R.T.: 0.000 min
Response: 73169032
Conc: 23.79 ng/ml

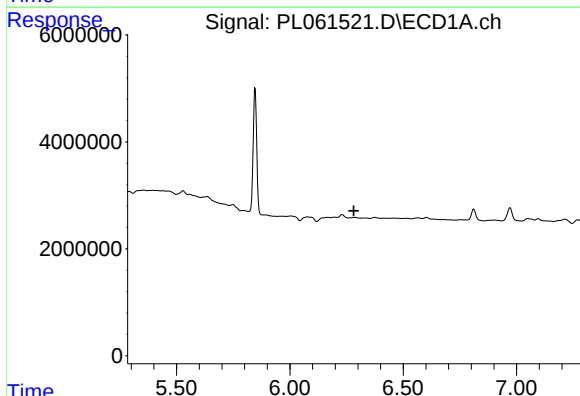


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.281 min
Response: 0
Conc: N.D.

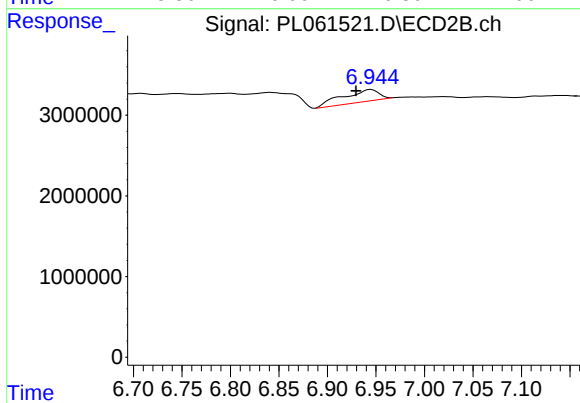

#15 Endosulfan II


R.T.: 6.945 min
Delta R.T.: 0.015 min
Response: 3819548
Conc: 1.29 ng/ml

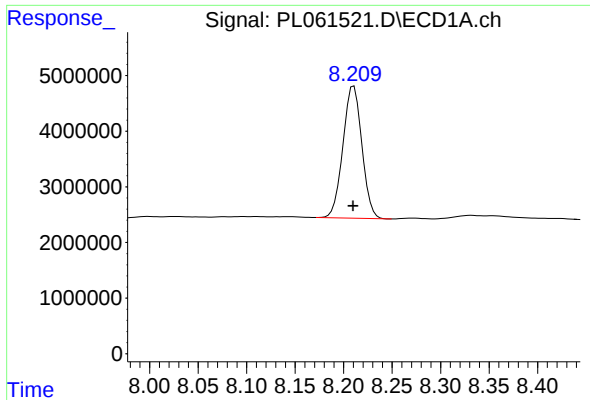

#28 Decachlorobiphenyl

R.T.: 8.210 min
Delta R.T.: 0.000 min
Response: 32263363
Conc: 19.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
B15A-5-7

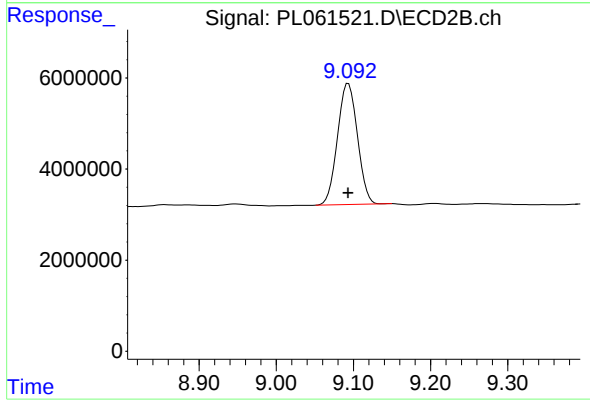

#28 Decachlorobiphenyl

R.T.: 9.094 min
Delta R.T.: 0.000 min
Response: 47787212
Conc: 20.21 ng/ml