

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091620\
 Data File : PL061516.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Sep 2020 14:56
 Operator : DD\AJ
 Sample : L4020-03
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ETGI-370

Manual Integrations
 APPROVED

Ankita
 9/17/2020 2:03:18 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 17 01:02:03 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 09 01:27:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.459	4.008	25958609	46175742	15.051	15.012
28)	SA Decachlor...	8.209	9.094	25301836	36661268	15.166	15.504
Target Compounds							
10)	B gamma-Chl...	5.396	6.121	1942524	3932069	1.049m	1.141m
11)	B alpha-Chl...	5.453	6.194	2763346	9080362	1.492m	2.609m#
17)	MA 4,4'-DDT	6.373	7.142	2776108	2635473	2.022m	1.053m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091620\
Data File : PL061516.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Sep 2020 14:56
Operator : DD\AJ
Sample : L4020-03
Misc :
ALS Vial : 22 Sample Multiplier: 1


Instrument :
ECD_L
ClientSampleId :
ETGI-370


Manual Integrations
APPROVED

Ankita
9/17/2020 2:03:18 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 01:02:03 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
Quant Title : GC Extractables
QLast Update : Wed Sep 09 01:27:38 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

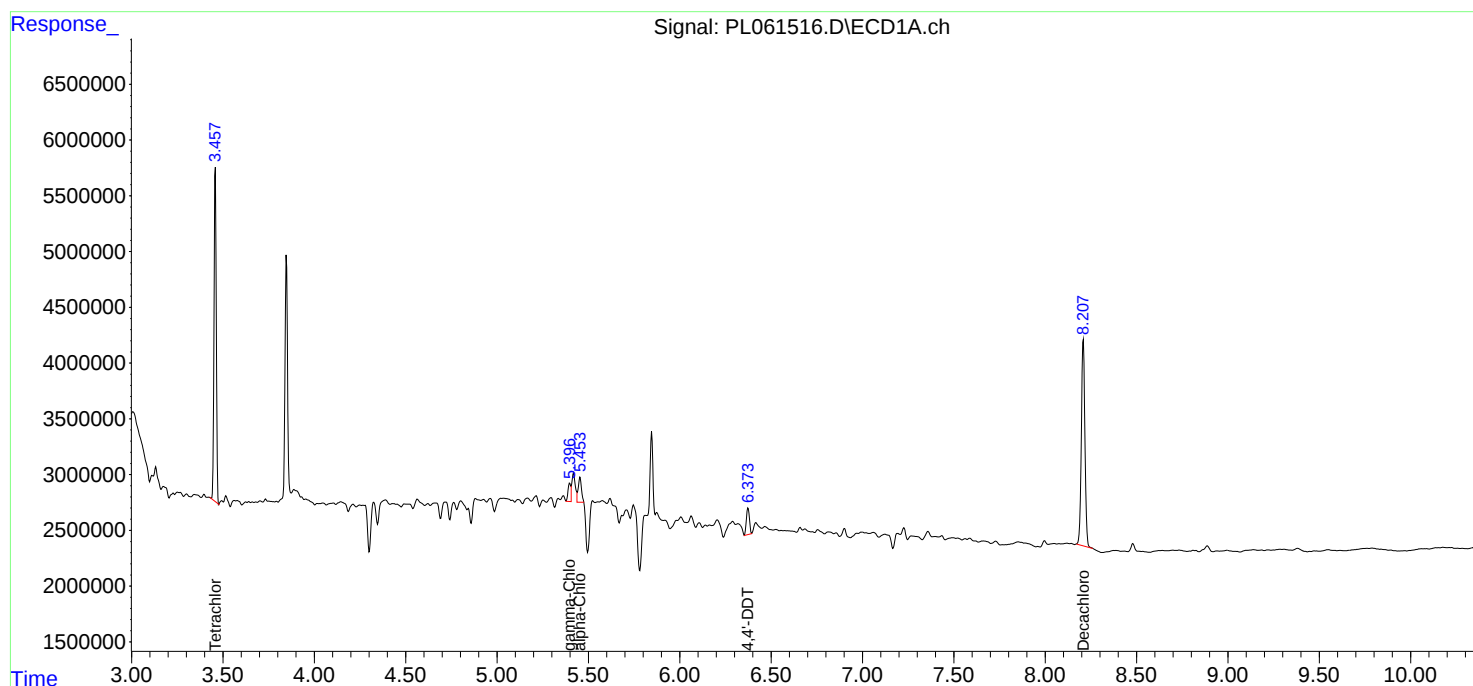

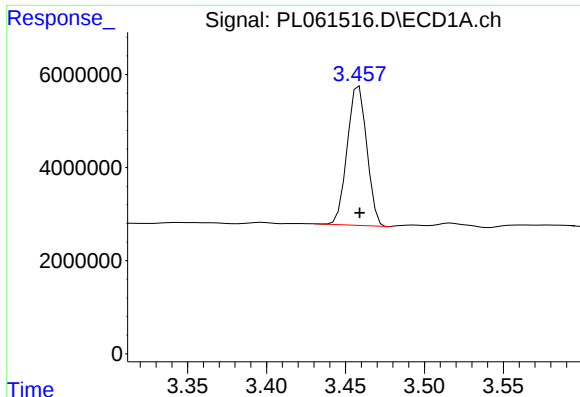


#1 Tetrachloro-m-xylene

R.T.: 3.459 min
Delta R.T.: 0.000 min
Response: 25958609
Conc: 15.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
ETGI-370


Manual Integrations
APPROVED

Ankita
9/17/2020 2:03:18 PM

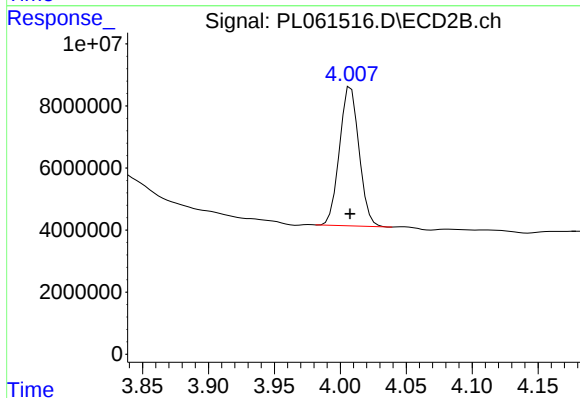


#1 Tetrachloro-m-xylene

R.T.: 4.008 min
Delta R.T.: 0.000 min
Response: 46175742
Conc: 15.01 ng/ml

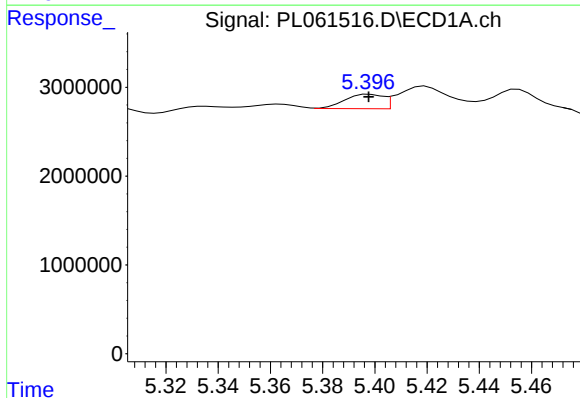


#10 gamma-Chlordane

R.T.: 5.396 min
Delta R.T.: -0.001 min
Response: 1942524
Conc: 1.05 ng/ml m

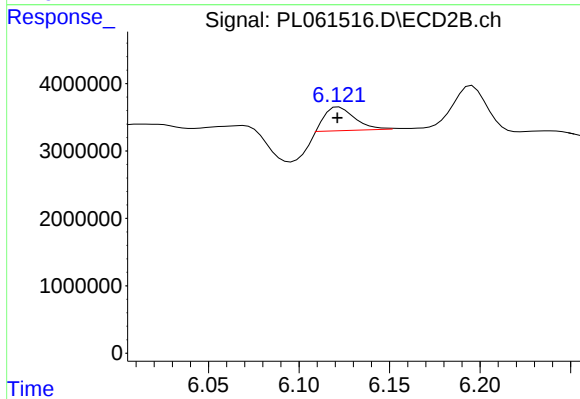

#10 gamma-Chlordane

R.T.: 6.121 min
Delta R.T.: 0.000 min
Response: 3932069
Conc: 1.14 ng/ml m

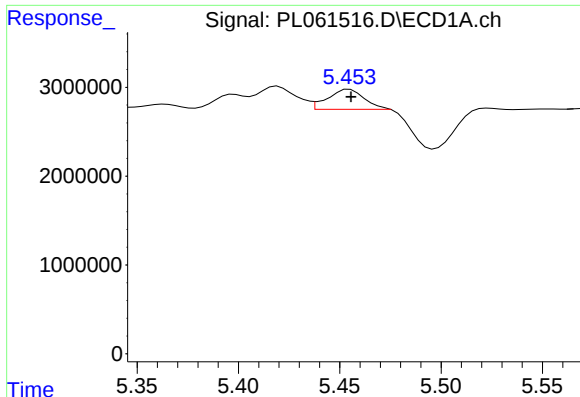


#11 alpha-Chlordane

R.T.: 5.453 min
Delta R.T.: -0.002 min
Response: 2763346
Conc: 1.49 ng/ml m

Instrument :
ECD_L
ClientSampleId :
ETGI-370


Manual Integrations
APPROVED

Ankita
9/17/2020 2:03:18 PM

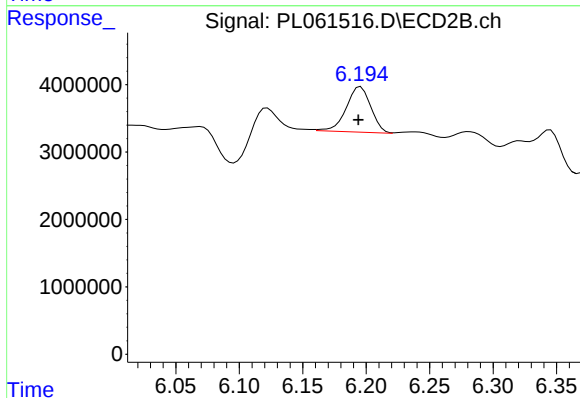


#11 alpha-Chlordane

R.T.: 6.194 min
Delta R.T.: 0.000 min
Response: 9080362
Conc: 2.61 ng/ml m

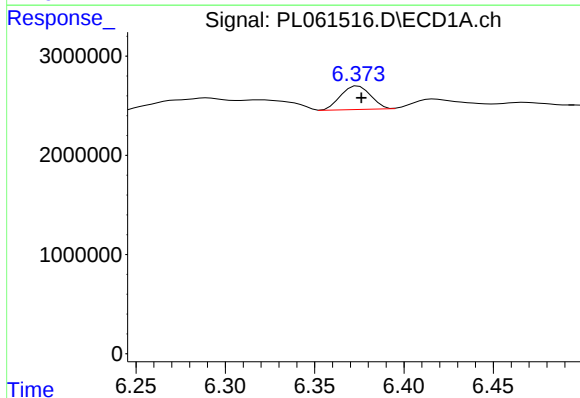


#17 4,4'-DDT

R.T.: 6.373 min
Delta R.T.: -0.003 min
Response: 2776108
Conc: 2.02 ng/ml m

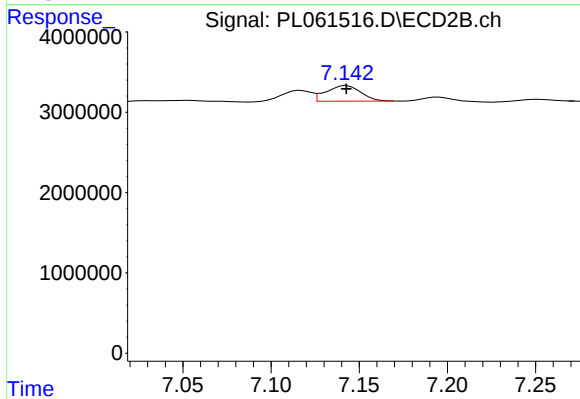

#17 4,4'-DDT

R.T.: 7.142 min
Delta R.T.: -0.001 min
Response: 2635473
Conc: 1.05 ng/ml m

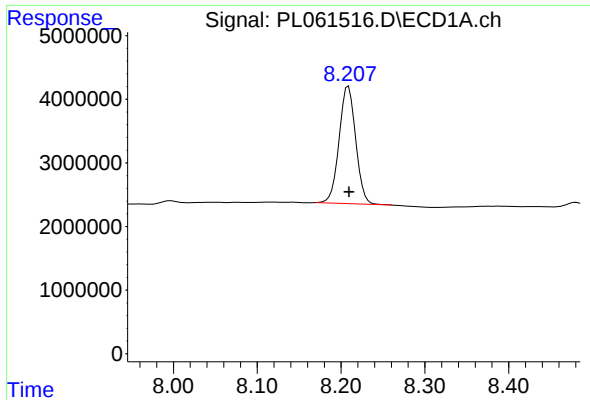


#28 Decachlorobiphenyl

R.T.: 8.209 min
Delta R.T.: 0.000 min
Response: 25301836
Conc: 15.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
ETGI-370

Manual Integrations
APPROVED

Ankita
9/17/2020 2:03:18 PM

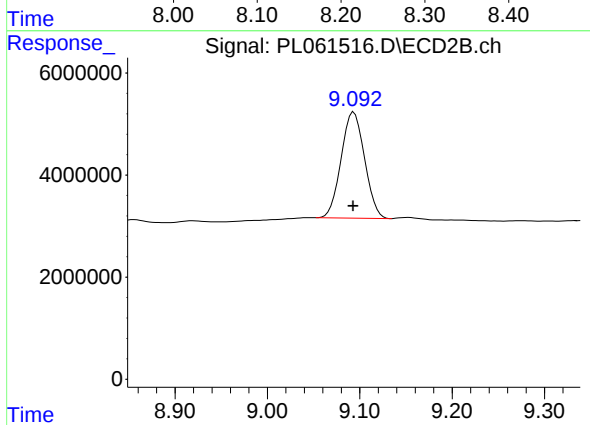

#28 Decachlorobiphenyl

R.T.: 9.094 min
Delta R.T.: 0.000 min
Response: 36661268
Conc: 15.50 ng/ml