

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091622\
 Data File : PL077801.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Sep 2022 13:23
 Operator : AR\AJ
 Sample : PB147676BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 18:35:56 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091222.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 13 13:26:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.416	2.626	34506880	62711765	21.527	21.124
28)	SA Decachlor...	8.909	7.726	30541990	52822523	23.632	21.043
Target Compounds							
8)	B Heptachlo...	5.571	0.000	19297728	0	11.070	N.D. #
9)	A Endosulfan I	0.000	4.937f	0	309134	N.D.	0.098 #
10)	B gamma-Chl...	5.805f	0.000	10241875	0	5.850	N.D. #
13)	MA Dieldrin	0.000	5.172	0	8296377	N.D.	2.502 #
14)	MA Endrin	0.000	5.472f	0	22378943	N.D.	7.848 #
15)	B Endosulfa...	6.711f	5.754	860602	-1532262	0.623	N.D. #
21)	B Endrin ke...	7.572f	0.000	600396	0	0.435	N.D. #
25)	Chlordane-3	5.805	0.000	10241875	0	41.589	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091622\
Data File : PL077801.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Sep 2022 13:23
Operator : AR\AJ
Sample : PB147676BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 18:35:56 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091222.M
Quant Title : GC Extractables
QLast Update : Tue Sep 13 13:26:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

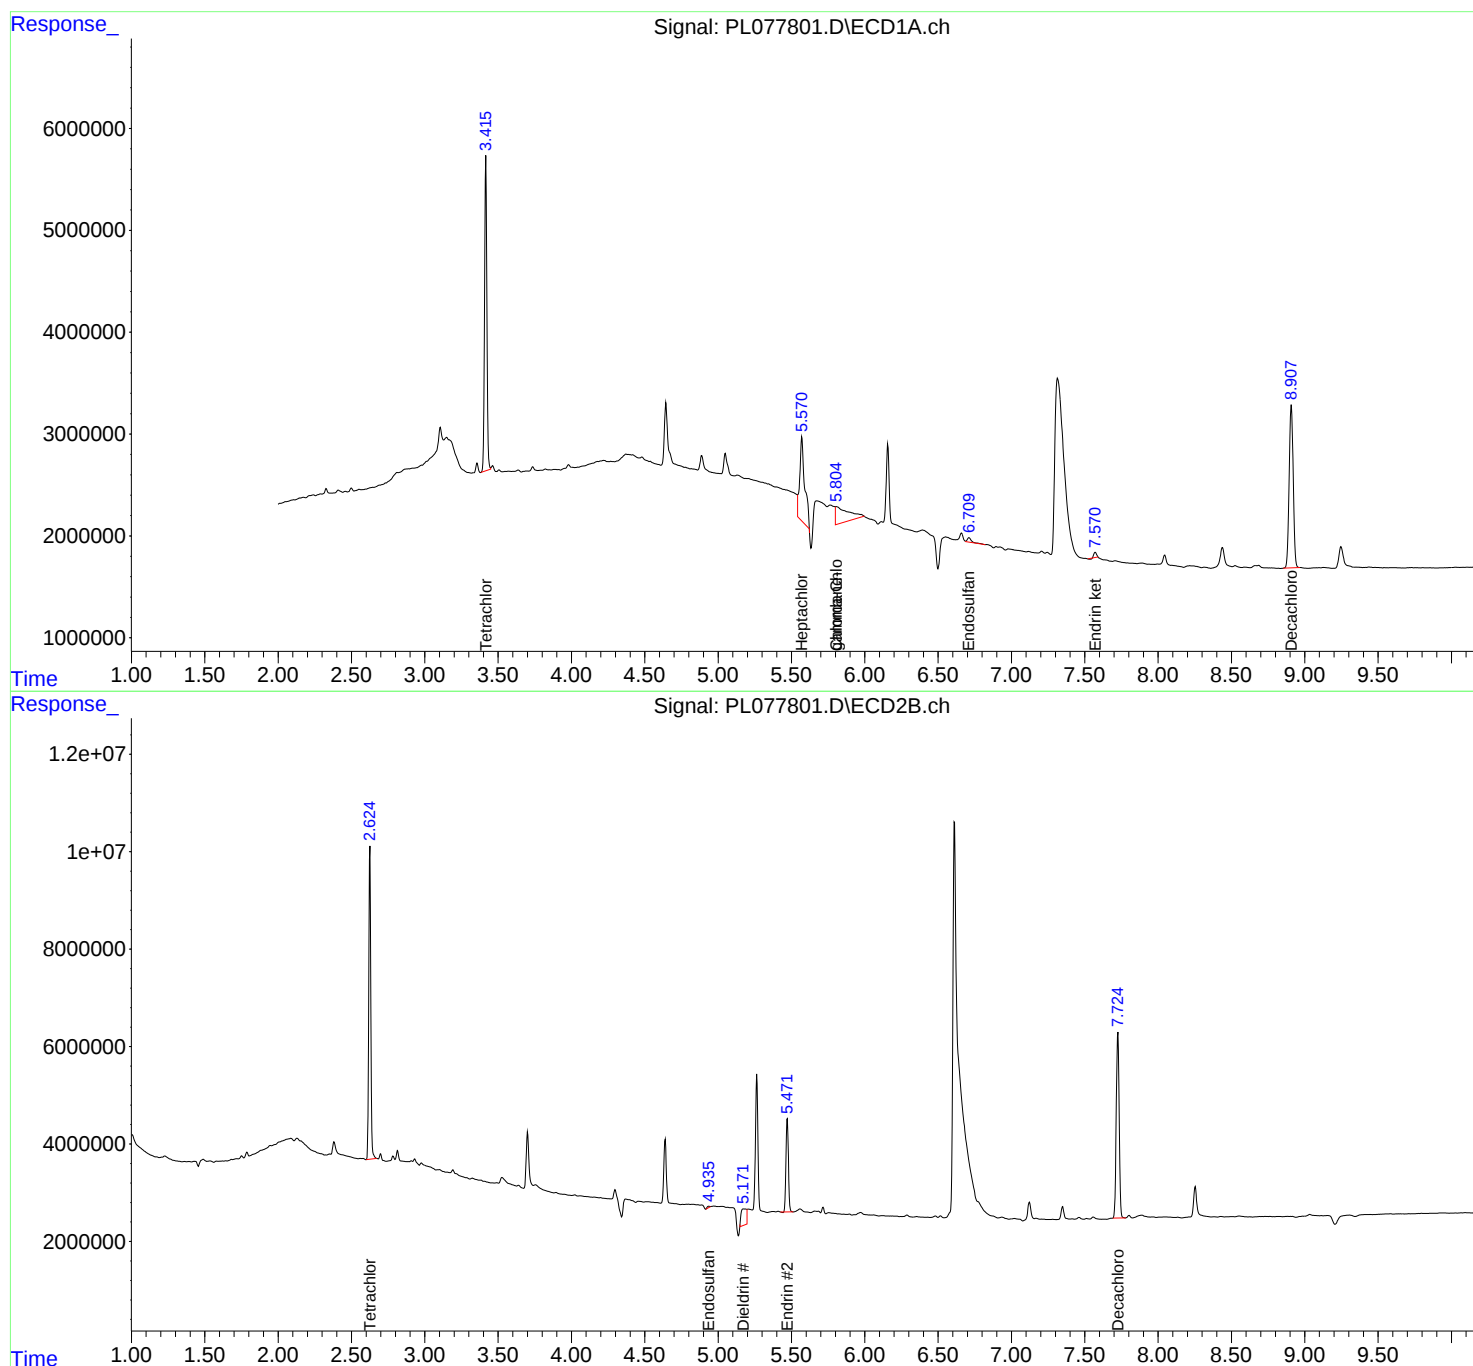


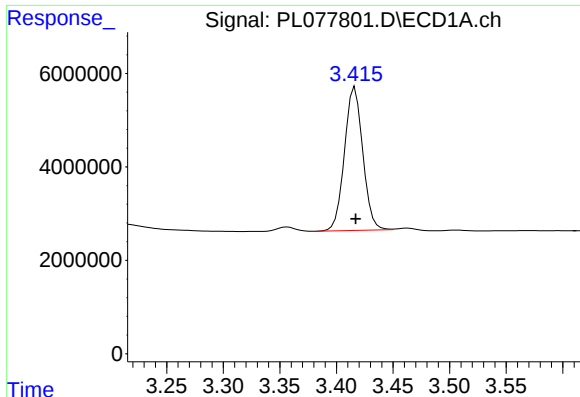

#1 Tetrachloro-m-xylene


R.T.: 3.416 min
Delta R.T.: 0.000 min
Response: 34506880
Conc: 21.53 ng/ml

Instrument :
ECD_L
ClientSampleId :

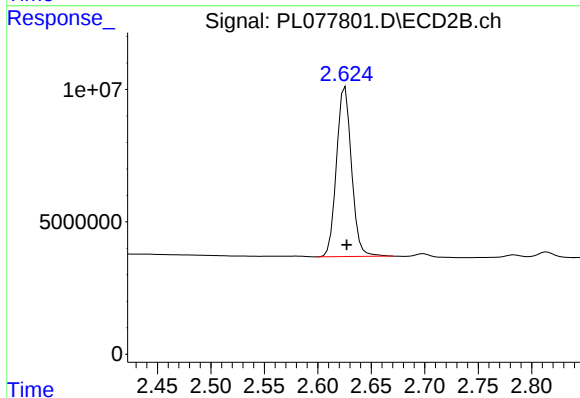


#1 Tetrachloro-m-xylene

R.T.: 2.626 min
Delta R.T.: -0.001 min
Response: 62711765
Conc: 21.12 ng/ml

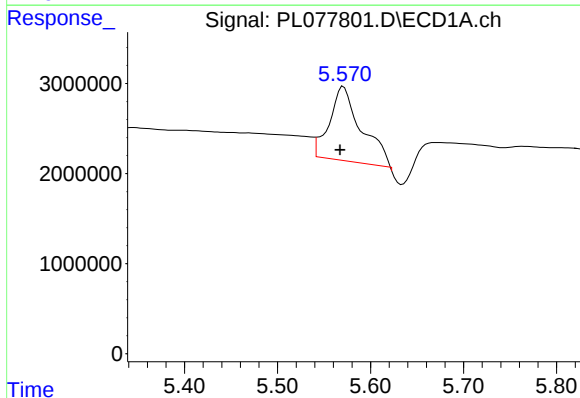


#8 Heptachlor epoxide

R.T.: 5.571 min
Delta R.T.: 0.004 min
Response: 19297728
Conc: 11.07 ng/ml

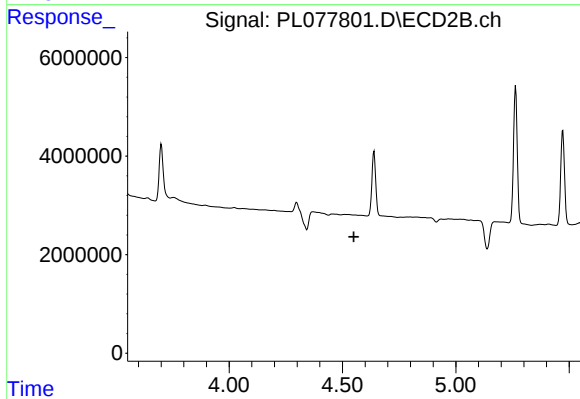

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.549 min
Response: 0
Conc: N.D.

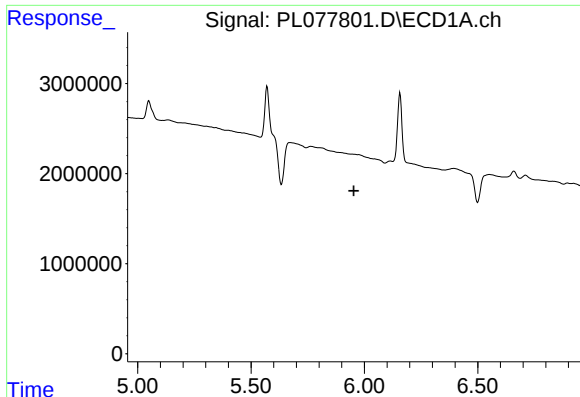

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.954 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

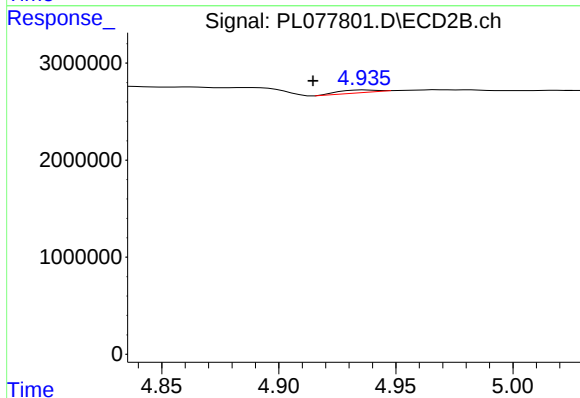


#9 Endosulfan I

R.T.: 4.937 min
Delta R.T.: 0.022 min
Response: 309134
Conc: 0.10 ng/ml

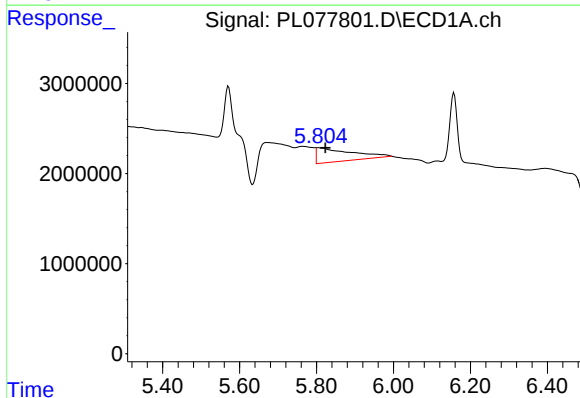


#10 gamma-Chlordane

R.T.: 5.805 min
Delta R.T.: -0.017 min
Response: 10241875
Conc: 5.85 ng/ml

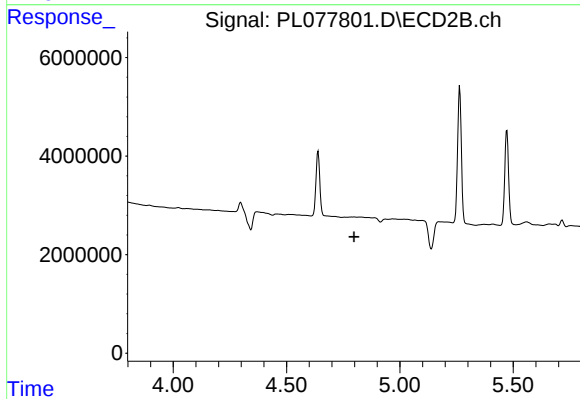

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 4.799 min
Response: 0
Conc: N.D.

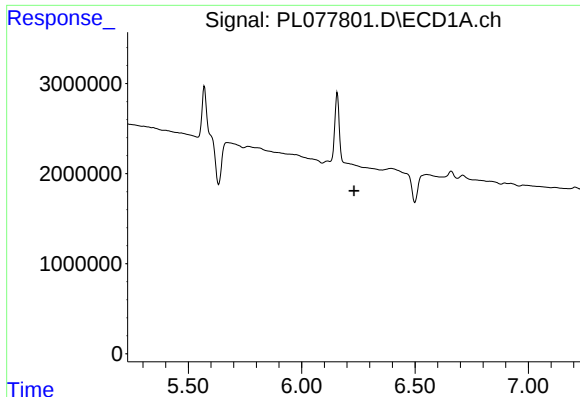

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.232 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

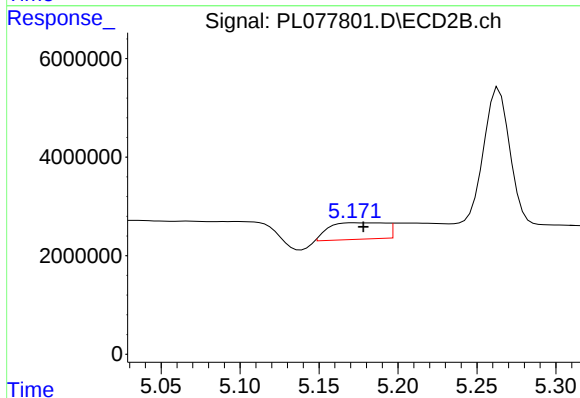


#13 Dieldrin

R.T.: 5.172 min
Delta R.T.: -0.006 min
Response: 8296377
Conc: 2.50 ng/ml

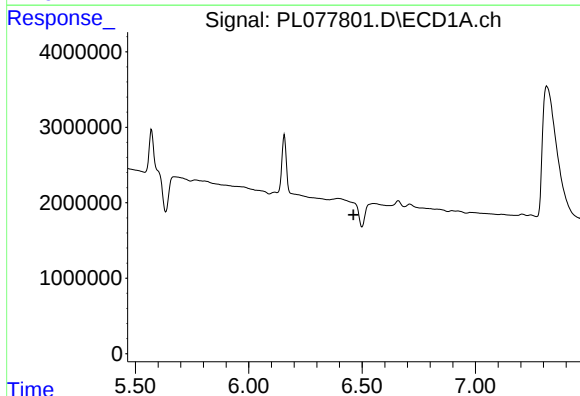


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.463 min
Response: 0
Conc: N.D.

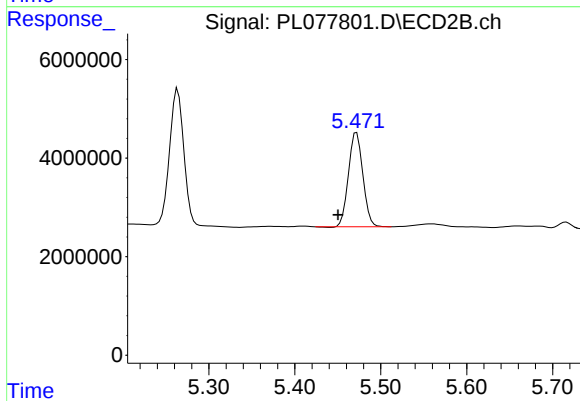

#14 Endrin


R.T.: 5.472 min
Delta R.T.: 0.021 min
Response: 22378943
Conc: 7.85 ng/ml

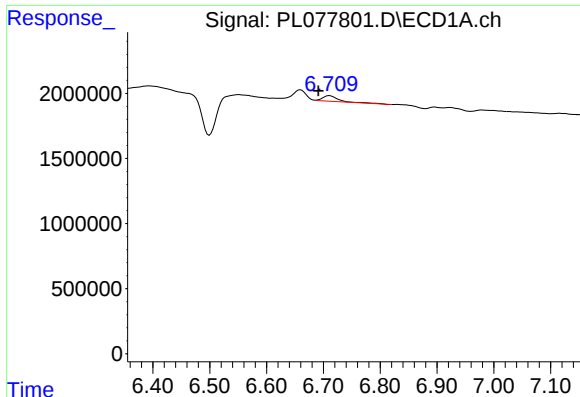

#15 Endosulfan II


R.T.: 6.711 min
Delta R.T.: 0.020 min
Response: 860602
Conc: 0.62 ng/ml

Instrument :
ECD_L
ClientSampleId :

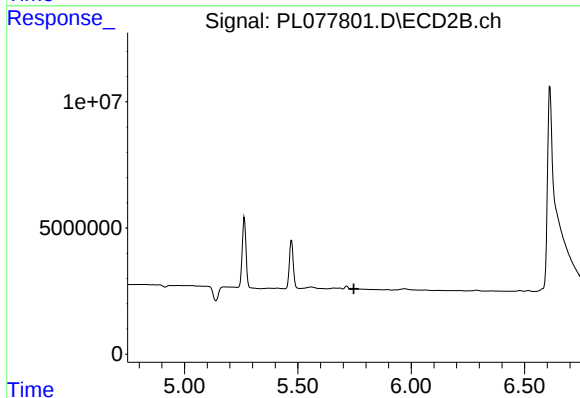


#15 Endosulfan II

R.T.: 5.754 min
Delta R.T.: 0.007 min
Response: -1532262
Conc: N.D.

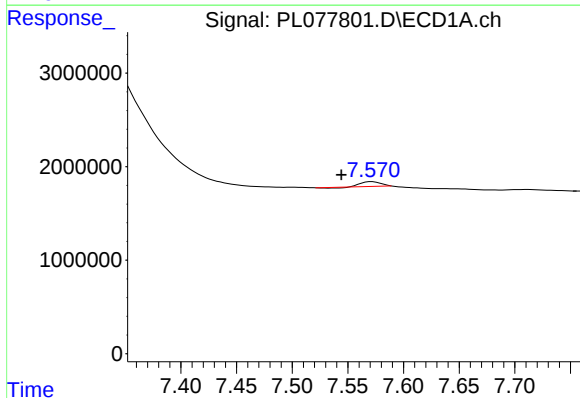


#21 Endrin ketone

R.T.: 7.572 min
Delta R.T.: 0.027 min
Response: 600396
Conc: 0.43 ng/ml

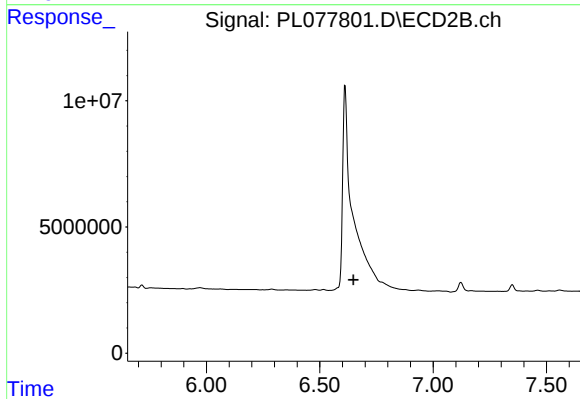

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 6.649 min
Response: 0
Conc: N.D.

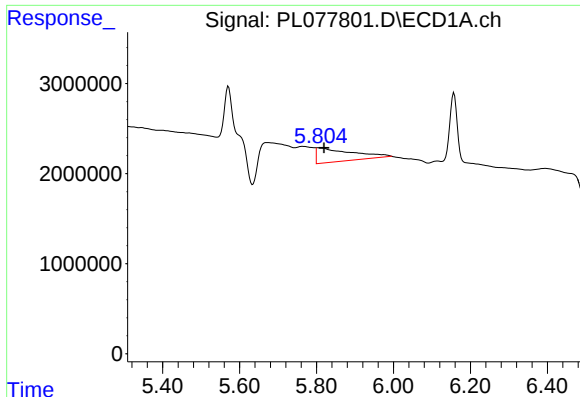

#25 Chlordane-3


R.T.: 5.805 min
Delta R.T.: -0.015 min
Response: 10241875
Conc: 41.59 ng/ml

Instrument :
ECD_L
ClientSampleId :

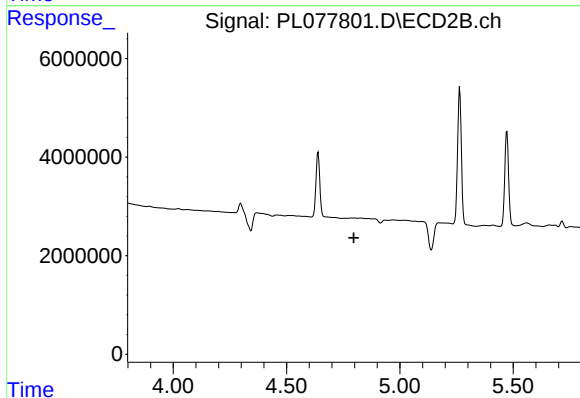


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 4.796 min
Response: 0
Conc: N.D.

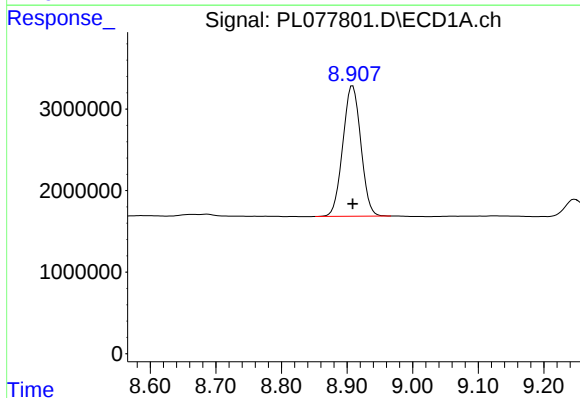

#28 Decachlorobiphenyl

R.T.: 8.909 min
Delta R.T.: 0.000 min
Response: 30541990
Conc: 23.63 ng/ml

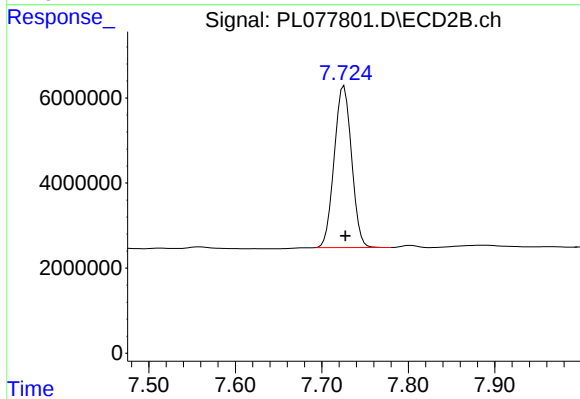

#28 Decachlorobiphenyl

R.T.: 7.726 min
Delta R.T.: -0.002 min
Response: 52822523
Conc: 21.04 ng/ml