

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091622\
 Data File : PL077816.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Sep 2022 23:46
 Operator : AR\AJ
 Sample : PB147675BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 17 02:43:03 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091222.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 13 13:26:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.416	2.626	33191029	58677904	20.706	19.765
28)	SA Decachlor...	8.905	7.723	58843647	100.9E6	45.530	40.206
Target Compounds							
3)	MA gamma-BHC...	4.235f	0.000	8538	0	0.004	N.D. #
7)	B delta-BHC	4.674	0.000	391803	0	0.191	N.D. #
8)	B Heptachlo...	5.595f	0.000	811401	0	0.465	N.D. #
10)	B gamma-Chl...	0.000	4.795	0	247841	N.D.	0.073 #
12)	B 4,4'-DDE	0.000	5.042	0	312990	N.D.	0.096 #
14)	MA Endrin	0.000	5.470f	0	207475	N.D.	0.073 #
15)	B Endosulfa...	6.709f	5.766f	455869	-61864	0.330	N.D. #
21)	B Endrin ke...	7.570f	0.000	645521	0	0.467	N.D. #
25)	Chlordane-3	0.000	4.795	0	247841	N.D.	0.720 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091622\
Data File : PL077816.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Sep 2022 23:46
Operator : AR\AJ
Sample : PB147675BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 02:43:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091222.M
Quant Title : GC Extractables
QLast Update : Tue Sep 13 13:26:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

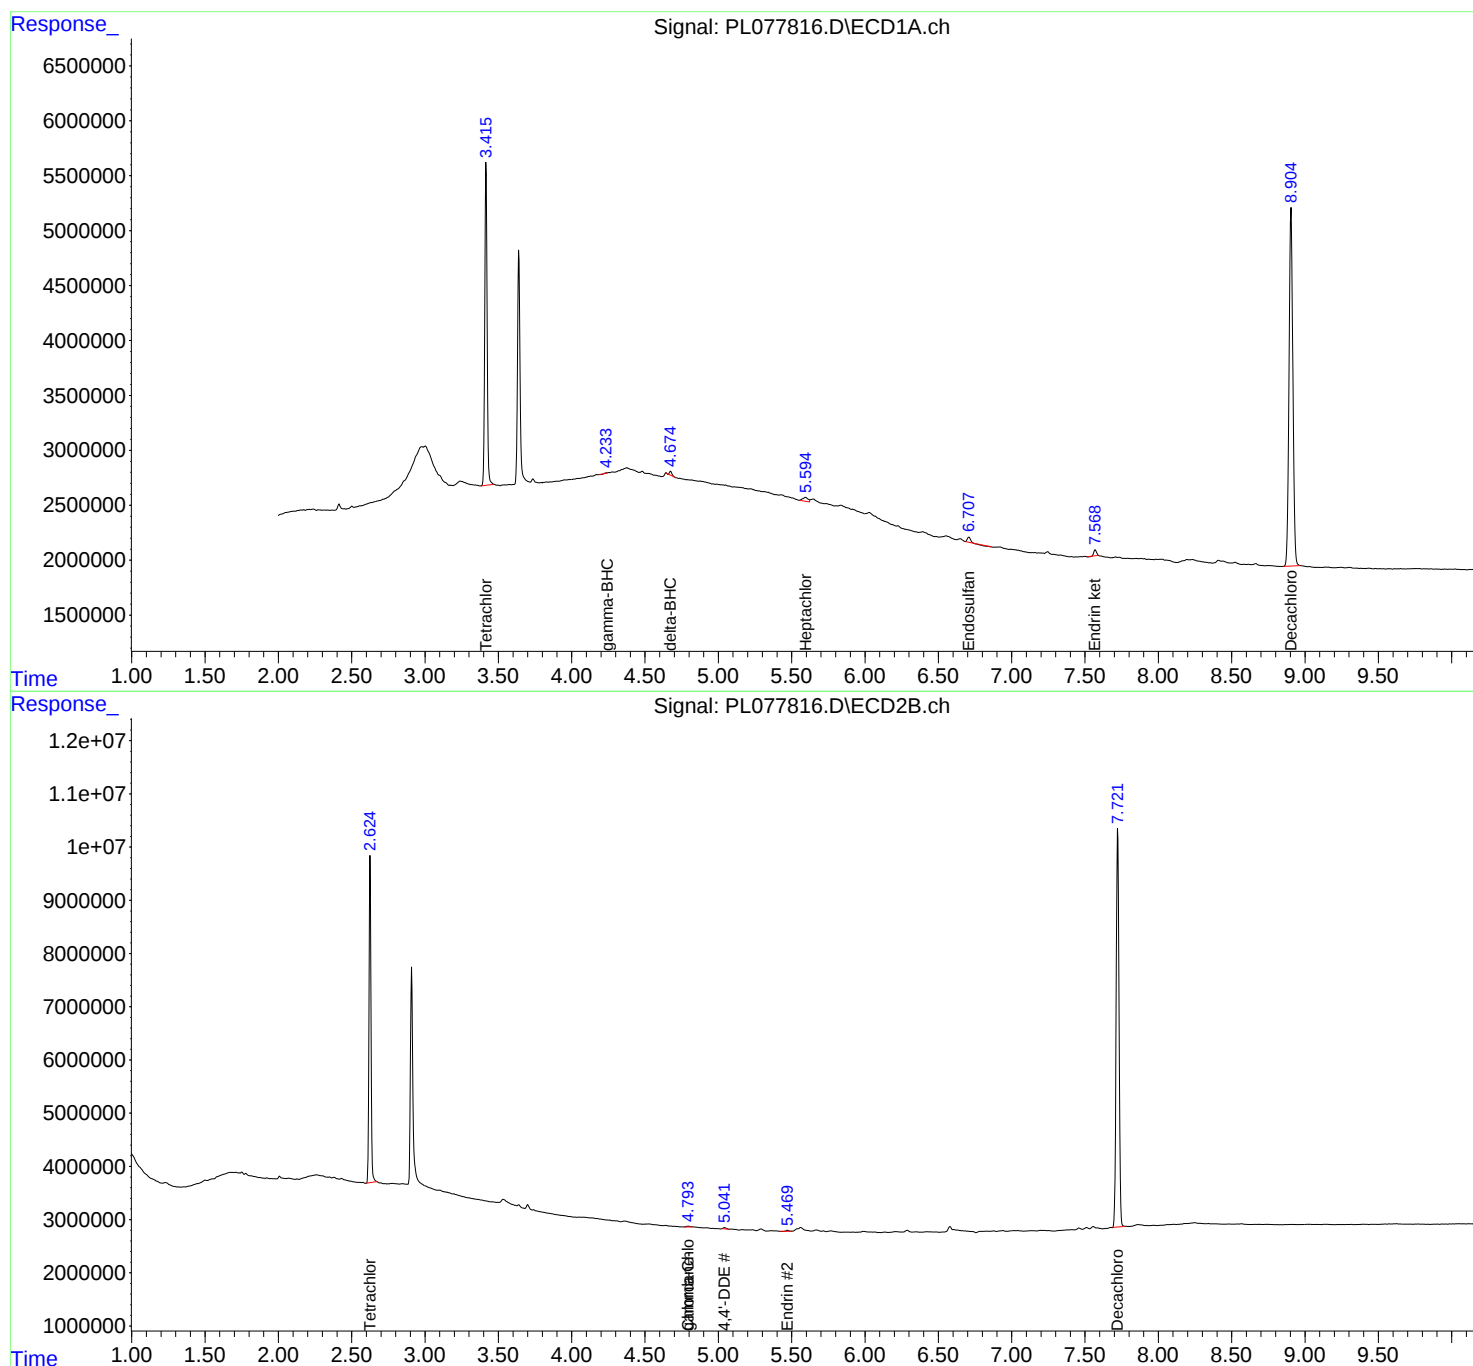


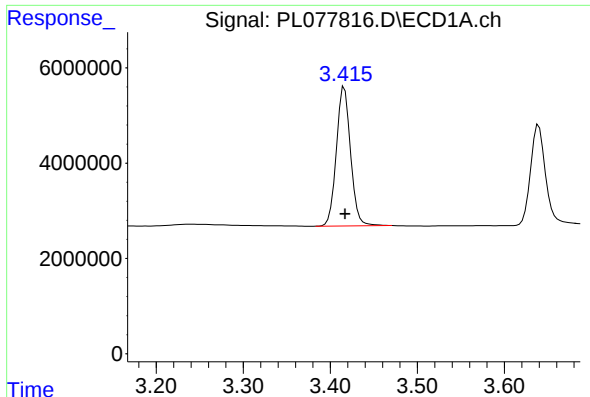

#1 Tetrachloro-m-xylene


R.T.: 3.416 min
Delta R.T.: 0.000 min
Response: 33191029
Conc: 20.71 ng/ml

Instrument :
ECD_L
ClientSampleId :

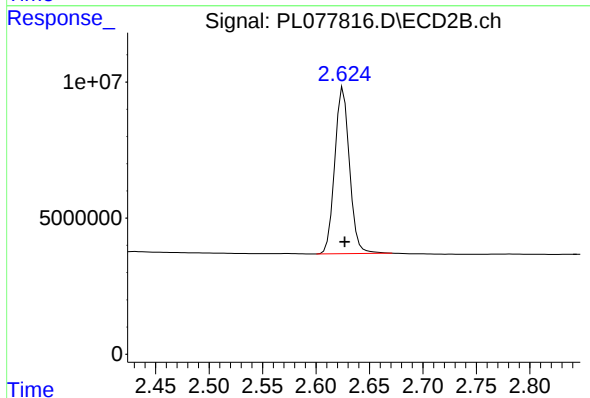


#1 Tetrachloro-m-xylene

R.T.: 2.626 min
Delta R.T.: -0.001 min
Response: 58677904
Conc: 19.77 ng/ml

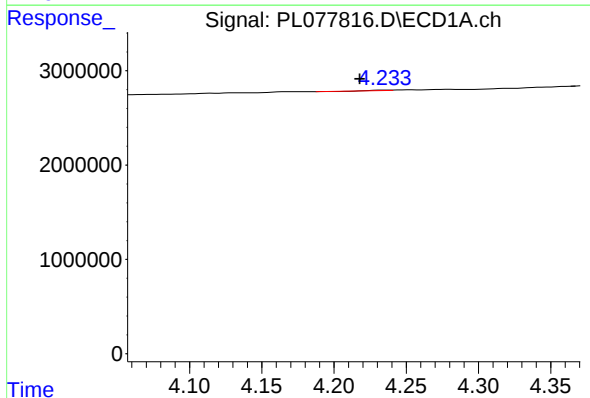


#3 gamma-BHC (Lindane)

R.T.: 4.235 min
Delta R.T.: 0.017 min
Response: 8538
Conc: 0.00 ng/ml

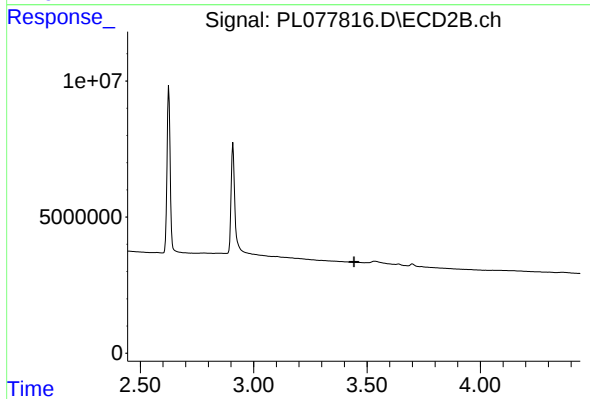

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 3.443 min
Response: 0
Conc: N.D.

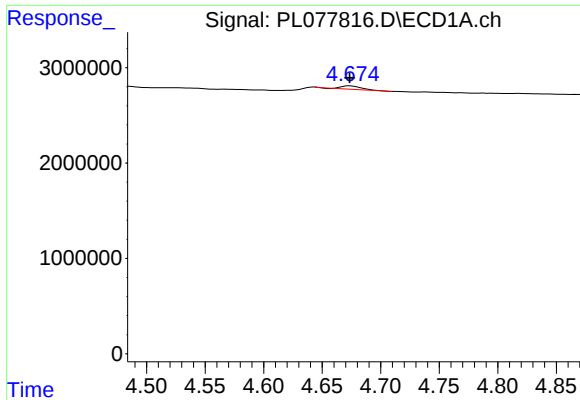

#7 delta-BHC


R.T.: 4.674 min
Delta R.T.: 0.000 min
Response: 391803
Conc: 0.19 ng/ml

Instrument :
ECD_L
ClientSampleId :

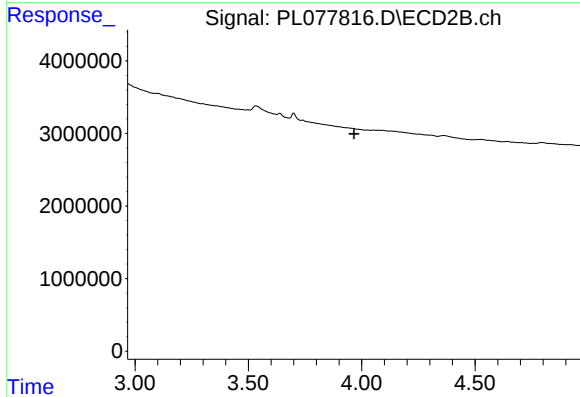


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 3.967 min
Response: 0
Conc: N.D.

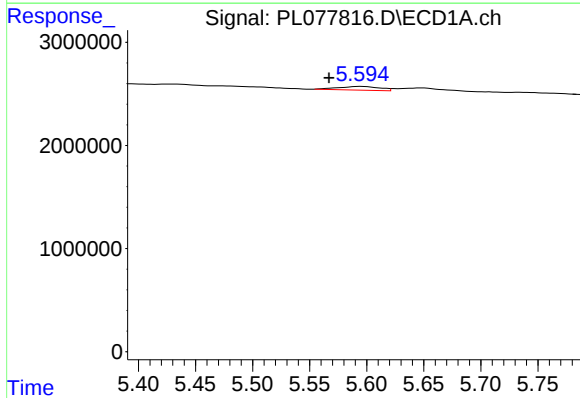


#8 Heptachlor epoxide

R.T.: 5.595 min
Delta R.T.: 0.028 min
Response: 811401
Conc: 0.47 ng/ml

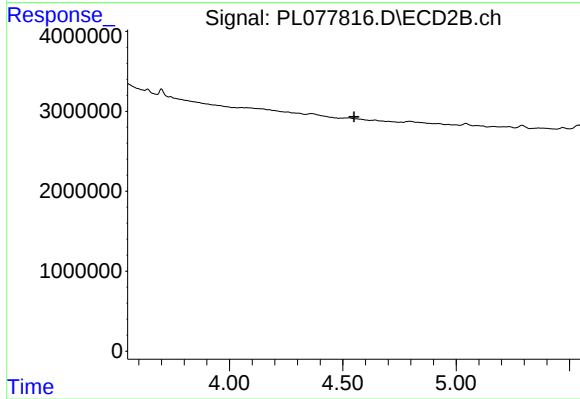

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.549 min
Response: 0
Conc: N.D.

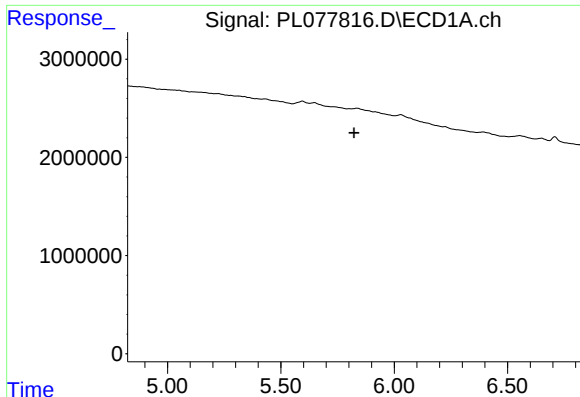

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.823 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

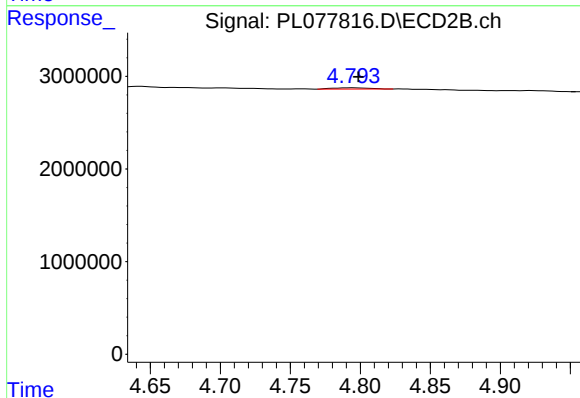


#10 gamma-Chlordane

R.T.: 4.795 min
Delta R.T.: -0.004 min
Response: 247841
Conc: 0.07 ng/ml

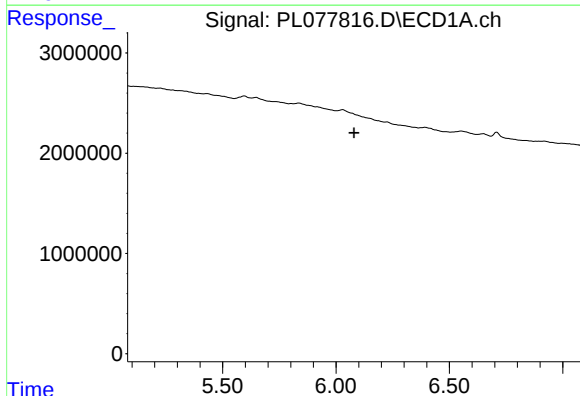


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 6.080 min
Response: 0
Conc: N.D.

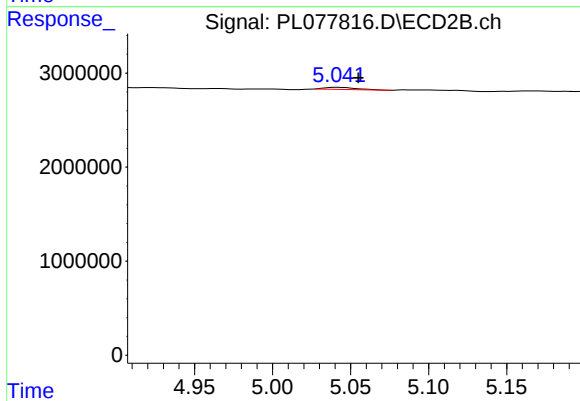

#12 4,4'-DDE


R.T.: 5.042 min
Delta R.T.: -0.013 min
Response: 312990
Conc: 0.10 ng/ml

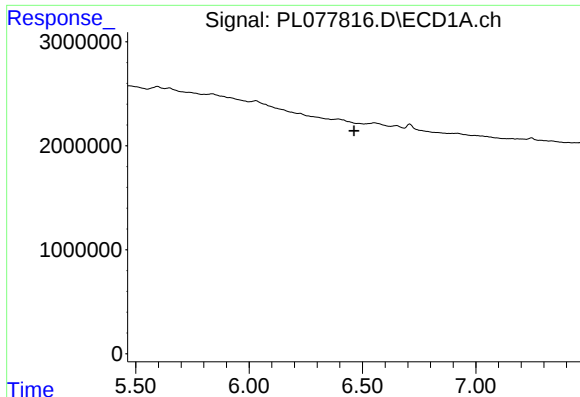

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.463 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

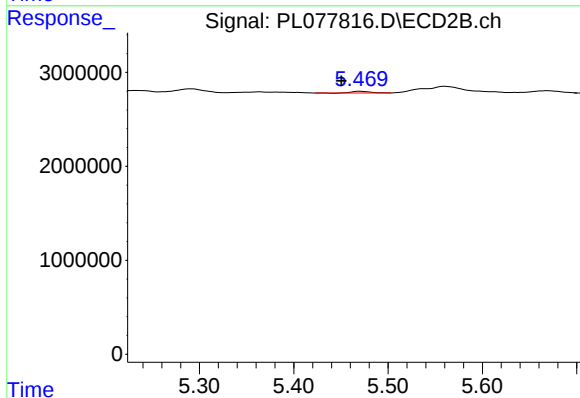


#14 Endrin

R.T.: 5.470 min
Delta R.T.: 0.020 min
Response: 207475
Conc: 0.07 ng/ml

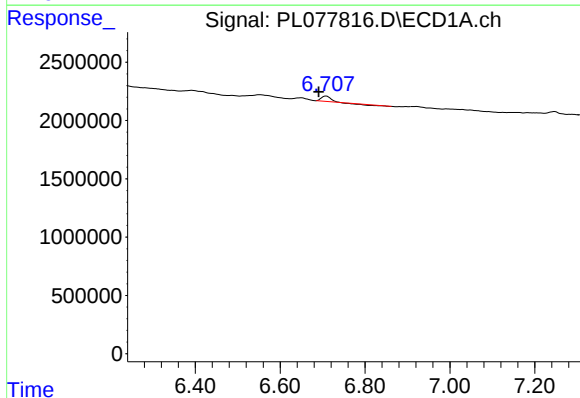


#15 Endosulfan II

R.T.: 6.709 min
Delta R.T.: 0.017 min
Response: 455869
Conc: 0.33 ng/ml

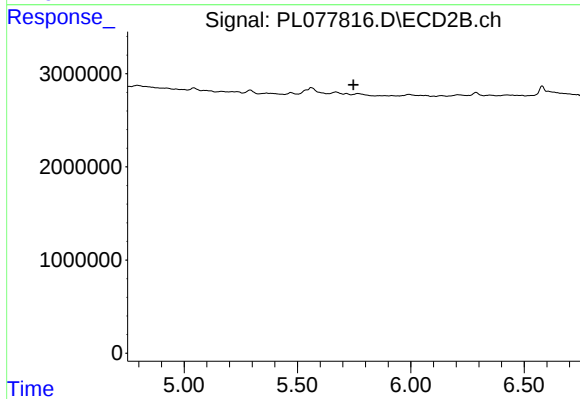

#15 Endosulfan II


R.T.: 5.766 min
Delta R.T.: 0.019 min
Response: -61864
Conc: N.D.

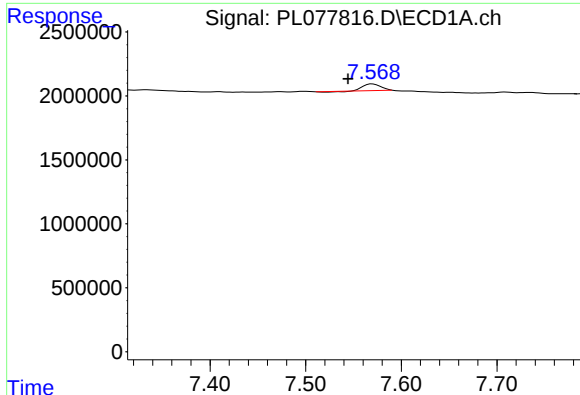

#21 Endrin ketone


R.T.: 7.570 min
Delta R.T.: 0.025 min
Response: 645521
Conc: 0.47 ng/ml

Instrument :
ECD_L
ClientSampleId :

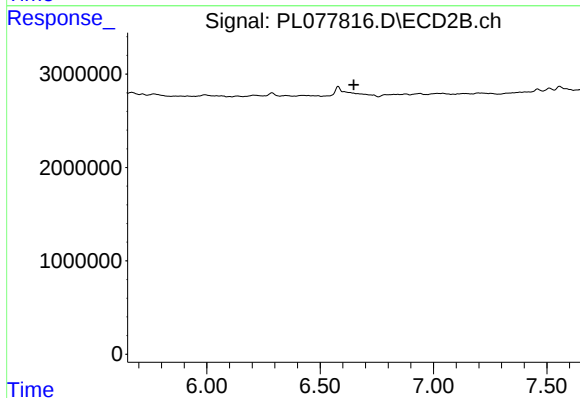


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 6.649 min
Response: 0
Conc: N.D.

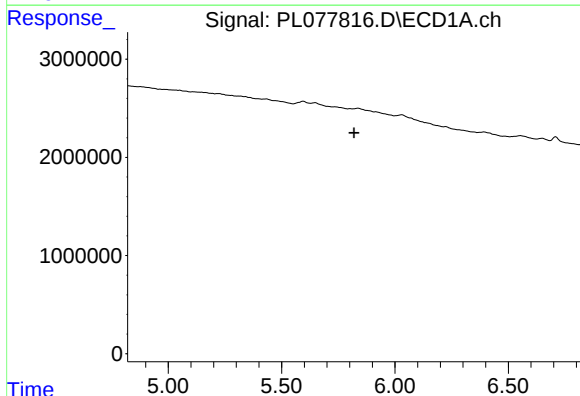


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.820 min
Response: 0
Conc: N.D.

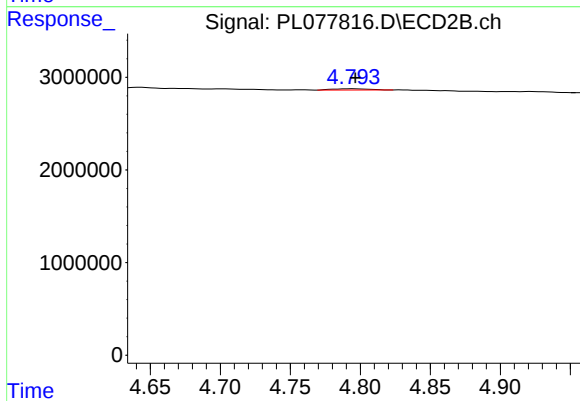

#25 Chlordane-3


R.T.: 4.795 min
Delta R.T.: -0.002 min
Response: 247841
Conc: 0.72 ng/ml

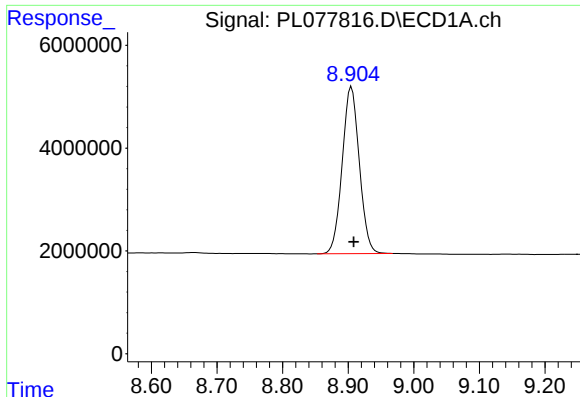

#28 Decachlorobiphenyl

R.T.: 8.905 min
Delta R.T.: -0.003 min
Response: 58843647
Conc: 45.53 ng/ml

Instrument :
ECD_L
ClientSampleId :

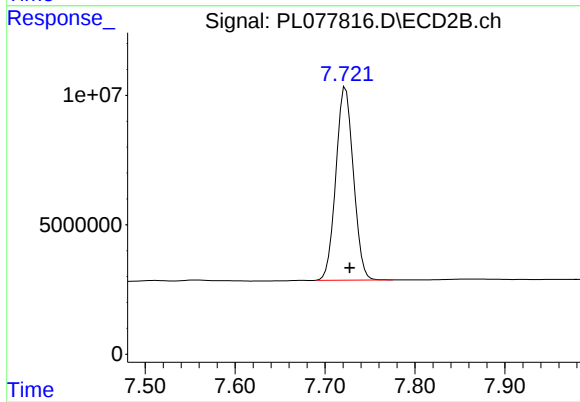

#28 Decachlorobiphenyl

R.T.: 7.723 min
Delta R.T.: -0.005 min
Response: 100927318
Conc: 40.21 ng/ml