

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091622\
 Data File : PL077804.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Sep 2022 14:04
 Operator : AR\AJ
 Sample : N4630-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 WC-17-4-1

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/19/2022
 Supervised By : Ankita Jodhani 09/19/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 18:36:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091222.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 13 13:26:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.415	2.625	26069032	51708299	16.263	17.418
2) SA Decachlor...	8.900	7.724	24159198	40921282	18.693m	16.302

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091622\
Data File : PL077804.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Sep 2022 14:04
Operator : AR\AJ
Sample : N4630-02
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
WC-17-4-1


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 09/19/2022
Supervised By : Ankita Jodhani 09/19/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 18:36:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091222.M
Quant Title : GC Extractables
QLast Update : Tue Sep 13 13:26:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

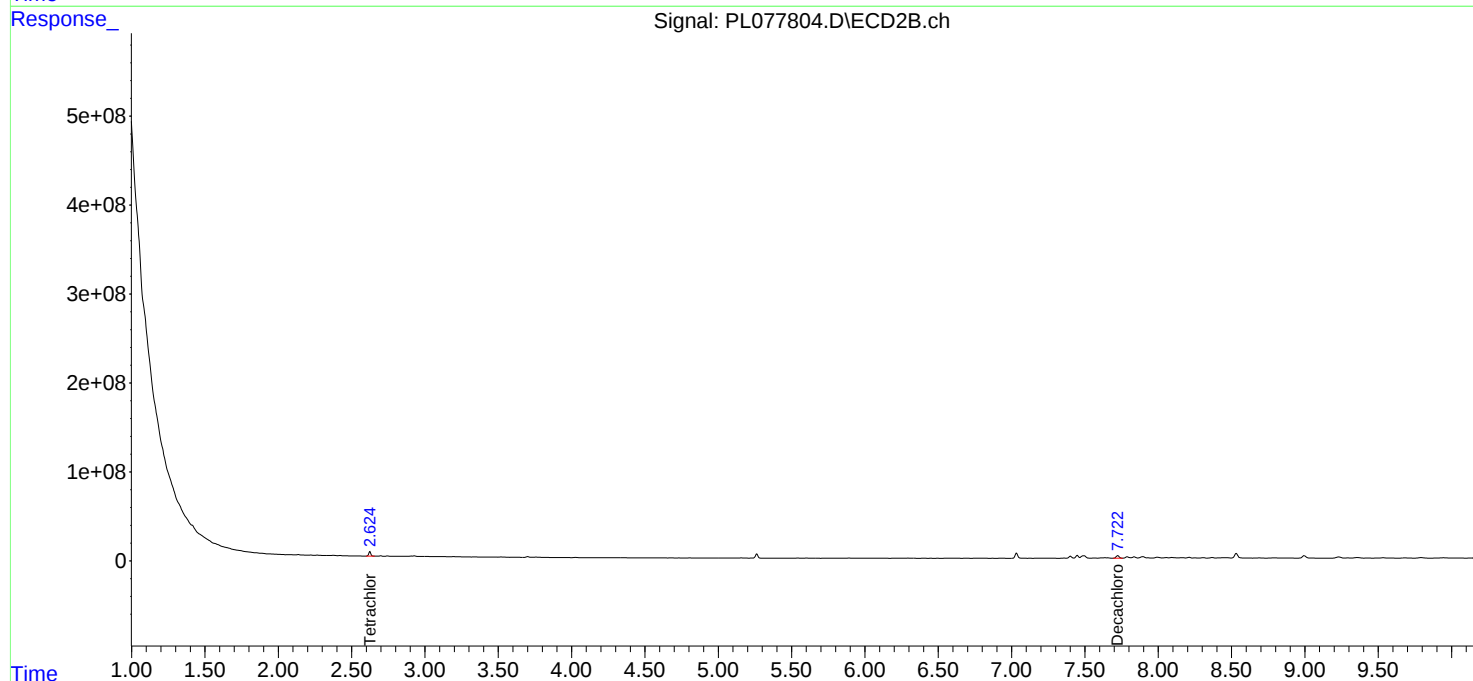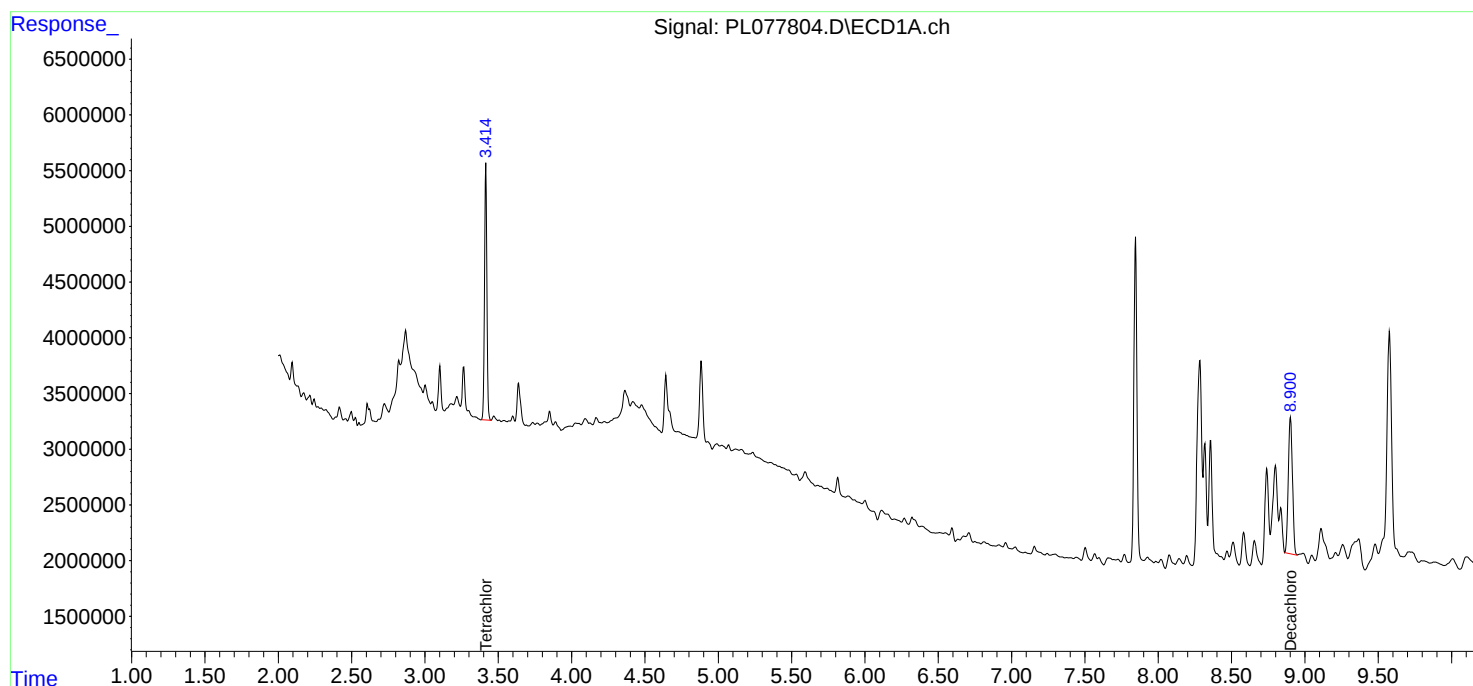

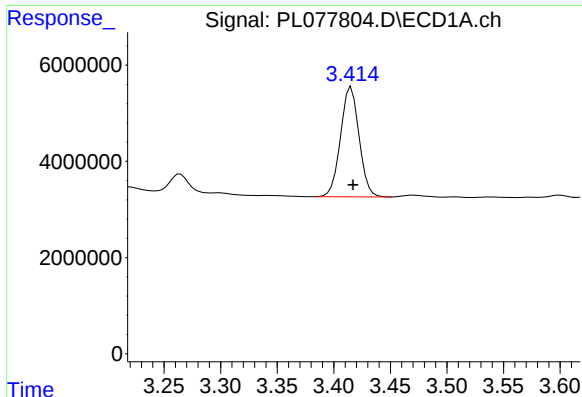


#1 Tetrachloro-m-xylene

R.T.: 3.415 min
Delta R.T.: -0.002 min
Response: 26069032
Conc: 16.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
WC-17-4-1


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/19/2022
Supervised By :Ankita Jodhani 09/19/2022

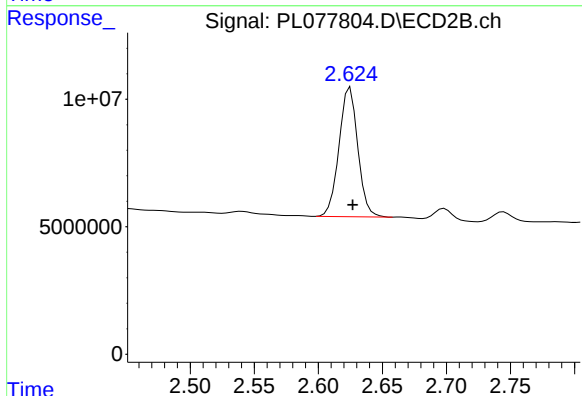


#1 Tetrachloro-m-xylene

R.T.: 2.625 min
Delta R.T.: -0.002 min
Response: 51708299
Conc: 17.42 ng/ml

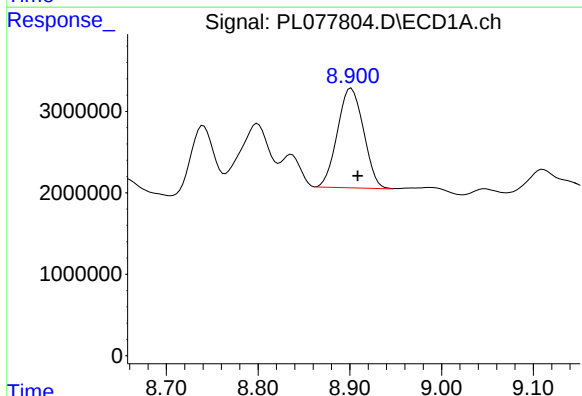

#28 Decachlorobiphenyl

R.T.: 8.900 min
Delta R.T.: -0.008 min
Response: 24159198
Conc: 18.69 ng/ml m

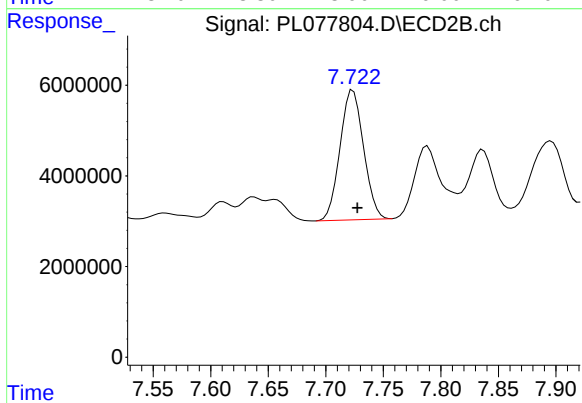

#28 Decachlorobiphenyl

R.T.: 7.724 min
Delta R.T.: -0.004 min
Response: 40921282
Conc: 16.30 ng/ml