

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091622\
 Data File : PL077808.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Sep 2022 16:55
 Operator : AR\AJ
 Sample : N4636-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BI-WEEKLY-DECANT

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 09/19/2022
 Supervised By :Ankita Jodhani 09/19/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 18:36:48 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091222.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 13 13:26:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.415	2.624	32063405	50146628	20.002	16.892m
28) SA Decachlor...	8.907	7.720	17454638	48922590	13.505	19.489m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091622\
Data File : PL077808.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Sep 2022 16:55
Operator : AR\AJ
Sample : N4636-01
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
BI-WEEKLY-DECANT


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 09/19/2022
Supervised By : Ankita Jodhani 09/19/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 18:36:48 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091222.M
Quant Title : GC Extractables
QLast Update : Tue Sep 13 13:26:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

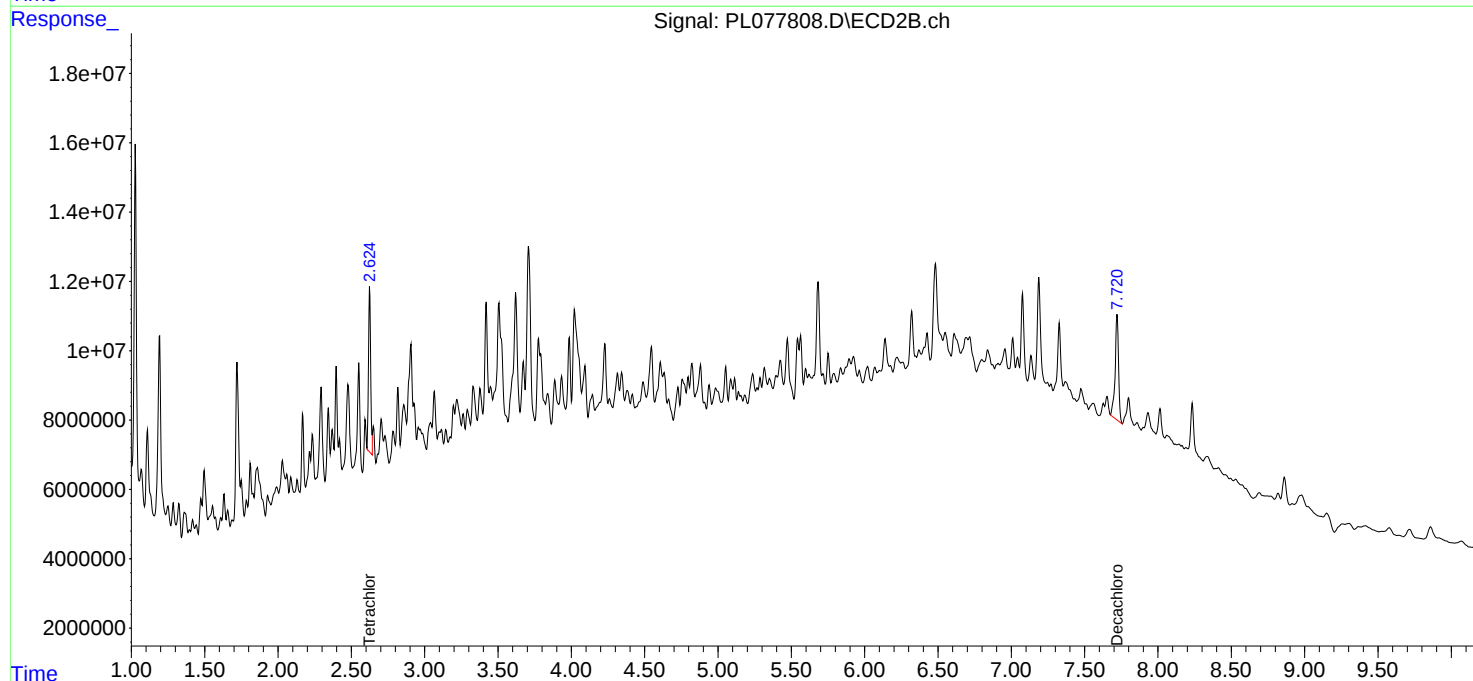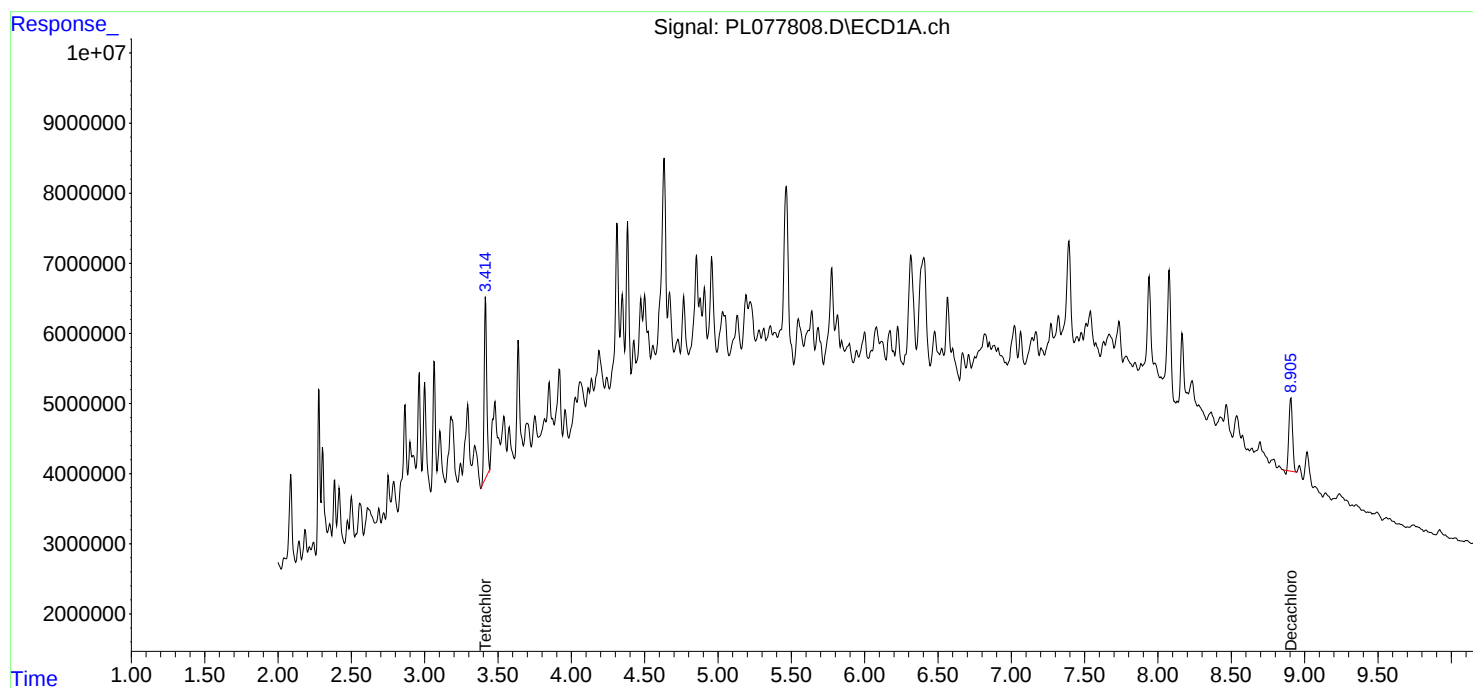

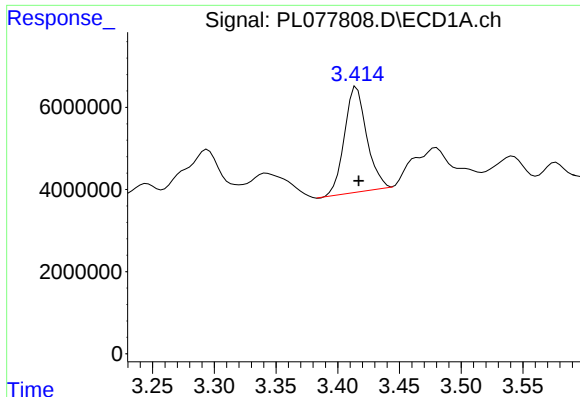


#1 Tetrachloro-m-xylene

R.T.: 3.415 min
Delta R.T.: -0.002 min
Response: 32063405
Conc: 20.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
BI-WEEKLY-DECANT


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/19/2022
Supervised By :Ankita Jodhani 09/19/2022

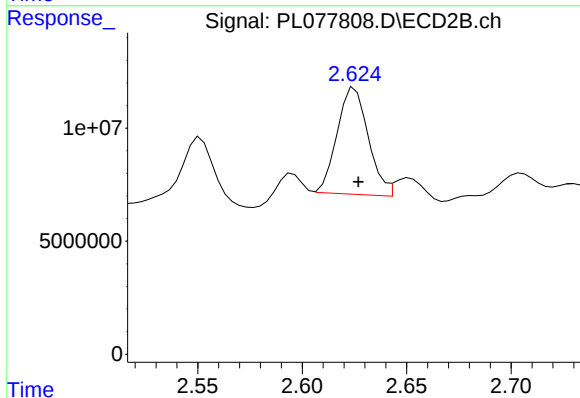


#1 Tetrachloro-m-xylene

R.T.: 2.624 min
Delta R.T.: -0.003 min
Response: 50146628
Conc: 16.89 ng/ml m

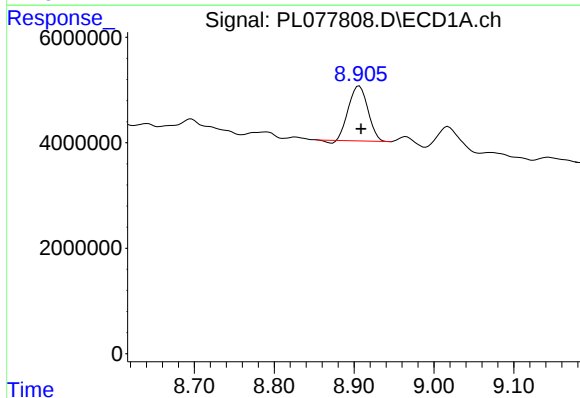

#28 Decachlorobiphenyl

R.T.: 8.907 min
Delta R.T.: -0.002 min
Response: 17454638
Conc: 13.51 ng/ml

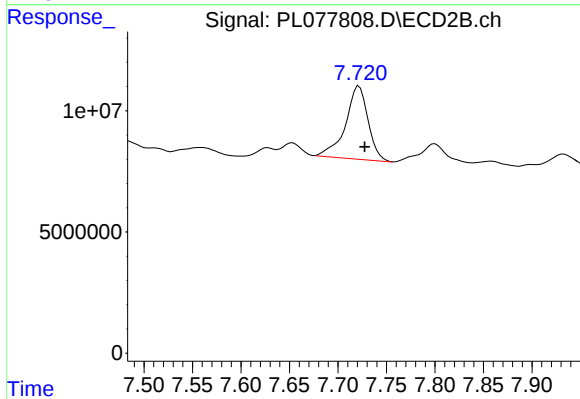

#28 Decachlorobiphenyl

R.T.: 7.720 min
Delta R.T.: -0.007 min
Response: 48922590
Conc: 19.49 ng/ml m