

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091623\
 Data File : PL085382.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2023 21:07
 Operator : AR\AJ
 Sample : 04453-08
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CPT102-14

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 15 22:41:04 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090523.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 05 15:22:36 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.474	2.682	49579851	23261697	20.270	20.473
28)	SA Decachlor...	9.022	7.860	28000033	20228578	17.412	15.197
Target Compounds							
12)	B 4,4'-DDE	6.146	5.158	1013850	456122	0.488	0.367
17)	MA 4,4'-DDT	6.980	5.967	683135	546515	0.406	0.469


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091623\
Data File : PL085382.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2023 21:07
Operator : AR\AJ
Sample : 04453-08
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
CPT102-14

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 15 22:41:04 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090523.M
Quant Title : GC Extractables
QLast Update : Tue Sep 05 15:22:36 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

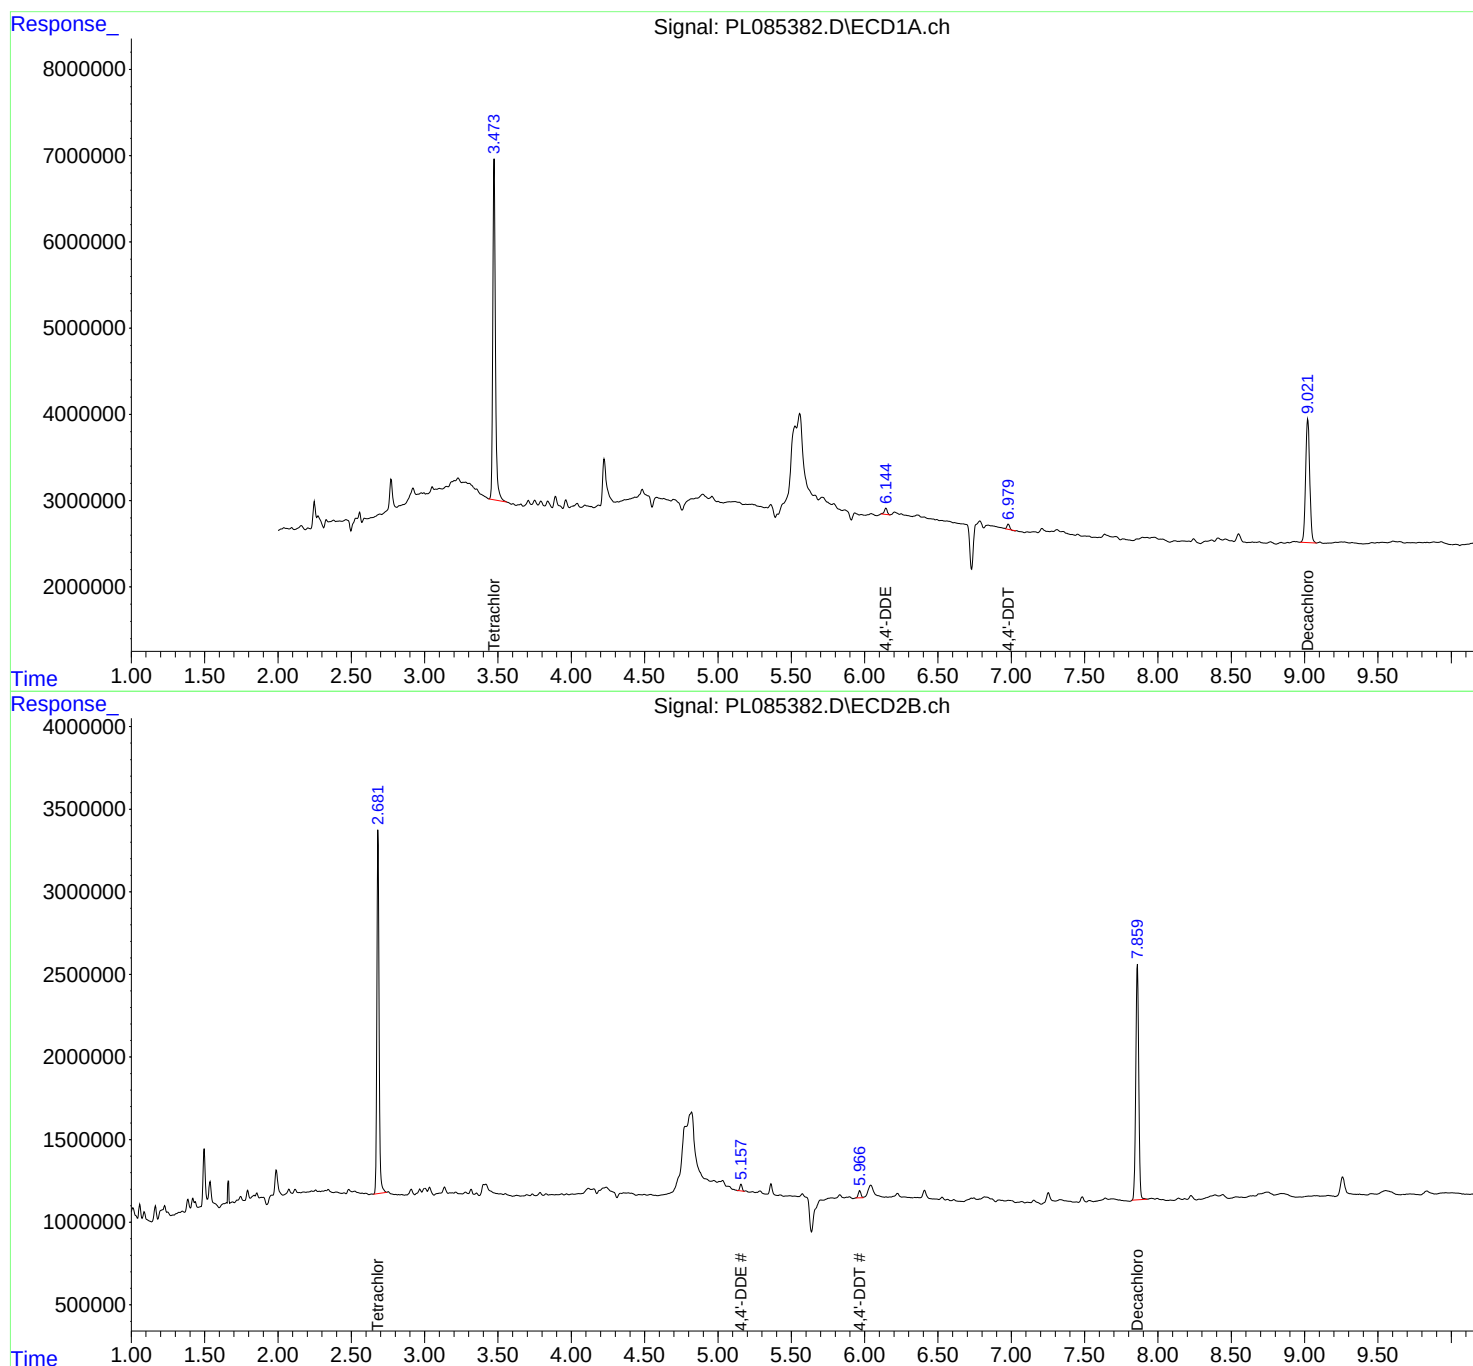


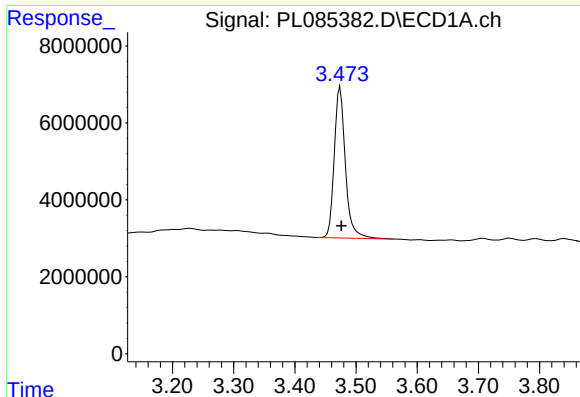

#1 Tetrachloro-m-xylene


R.T.: 3.474 min
Delta R.T.: -0.002 min
Response: 49579851
Conc: 20.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
CPT102-14

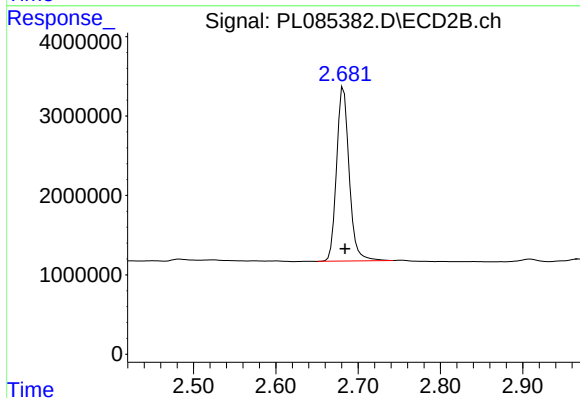


#1 Tetrachloro-m-xylene

R.T.: 2.682 min
Delta R.T.: -0.002 min
Response: 23261697
Conc: 20.47 ng/ml

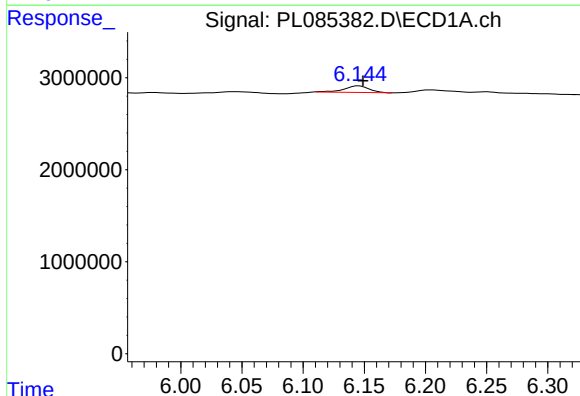


#12 4,4'-DDE

R.T.: 6.146 min
Delta R.T.: -0.003 min
Response: 1013850
Conc: 0.49 ng/ml

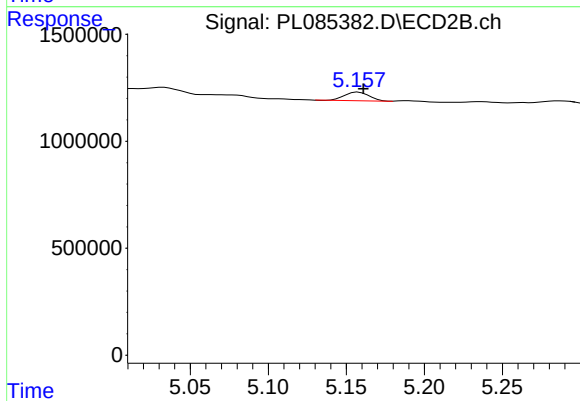

#12 4,4'-DDE


R.T.: 5.158 min
Delta R.T.: -0.003 min
Response: 456122
Conc: 0.37 ng/ml

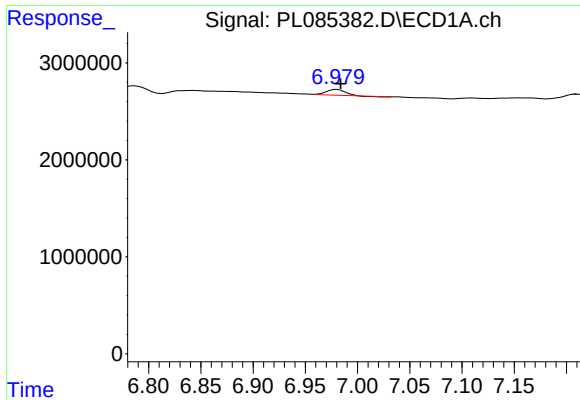

#17 4,4'-DDT


R.T.: 6.980 min
Delta R.T.: -0.004 min
Response: 683135
Conc: 0.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
CPT102-14

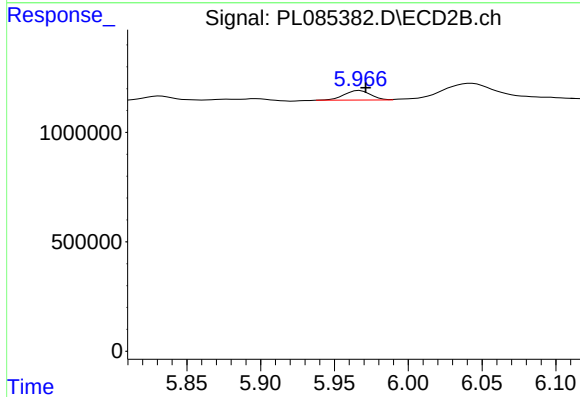


#17 4,4'-DDT

R.T.: 5.967 min
Delta R.T.: -0.004 min
Response: 546515
Conc: 0.47 ng/ml

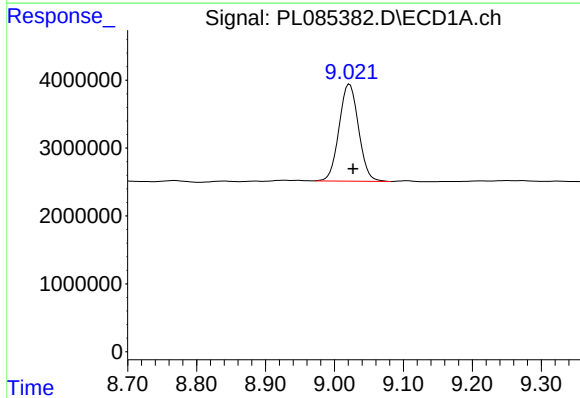

#28 Decachlorobiphenyl

R.T.: 9.022 min
Delta R.T.: -0.005 min
Response: 28000033
Conc: 17.41 ng/ml

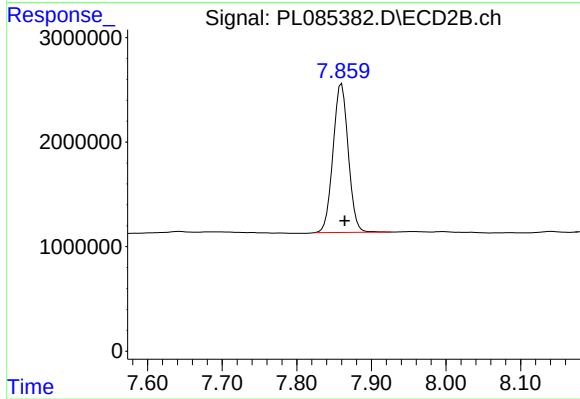

#28 Decachlorobiphenyl

R.T.: 7.860 min
Delta R.T.: -0.004 min
Response: 20228578
Conc: 15.20 ng/ml