

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091624\
 Data File : PL091772.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Sep 2024 12:53
 Operator : AR\AJ
 Sample : PSTDCCC050
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PSTDCCC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 17 01:25:28 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090924.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 09 19:26:36 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.542	2.781	84666071	104.0E6	54.322	55.602
2)	SA Decachlor...	9.057	7.921	54962559	88678834	45.225	48.024
Target Compounds							
2)	A alpha-BHC	3.997	3.285	115.5E6	148.9E6	53.456	55.969
3)	MA gamma-BHC...	4.330	3.615	109.6E6	138.8E6	53.328	56.432
4)	MA Heptachlor	4.919	3.954	100.6E6	134.4E6	53.688	55.791
5)	MB Aldrin	5.260	4.234	94316308	129.6E6	50.637	56.785
6)	B beta-BHC	4.527	3.914	49376625	59984624	54.259	54.908
7)	B delta-BHC	4.774	4.143	103.4E6	133.3E6	53.841	57.938
8)	B Heptachlo...	5.686	4.737	86720621	113.0E6	51.968	53.631
9)	A Endosulfan I	6.072	5.106	80700446	103.2E6	51.794	53.501
10)	B gamma-Chl...	5.943	4.987	87233102	117.9E6	52.211	53.469
11)	B alpha-Chl...	6.022	5.051	86920119	115.3E6	53.926	55.718
12)	B 4,4'-DDE	6.194	5.240	78052750	110.9E6	53.510	58.482
13)	MA Dieldrin	6.347	5.371	84831547	112.1E6	51.988	54.523
14)	MA Endrin	6.576	5.646	62529858	90941362	47.026	48.189
15)	B Endosulfa...	6.796	5.941	76408901	97762246	49.296	55.267
16)	A 4,4'-DDD	6.712	5.794	68340970	90077037	53.916	53.753
17)	MA 4,4'-DDT	7.025	6.044	63845610	82901465	48.672	51.595
18)	B Endrin al...	6.926	6.120	61040601	75681556	51.375	55.362
19)	B Endosulfa...	7.160	6.342	68861600	92360678	49.314	53.820
20)	A Methoxychlor	7.501	6.619	32441738	44477886	47.958	50.214
21)	B Endrin ke...	7.645	6.848	78173855	107.2E6	50.555	53.319
22)	Mirex	8.118	7.029	57722017	84907475	48.205	47.883
24)	Chlordane-2	5.260f	4.372	94316308	5921874	1226.764	79.009 #
25)	Chlordane-3	5.943	4.987	87233102	117.9E6	339.562	505.852 #
26)	Chlordane-4	6.022	5.051	86920119	115.3E6	293.494	552.819 #
27)	Chlordane-5	0.000	5.941	0	97762246	N.D.	1364.240 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091624\
Data File : PL091772.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Sep 2024 12:53
Operator : AR\AJ
Sample : PSTDCCC050
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 01:25:28 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090924.M
Quant Title : GC Extractables
QLast Update : Mon Sep 09 19:26:36 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

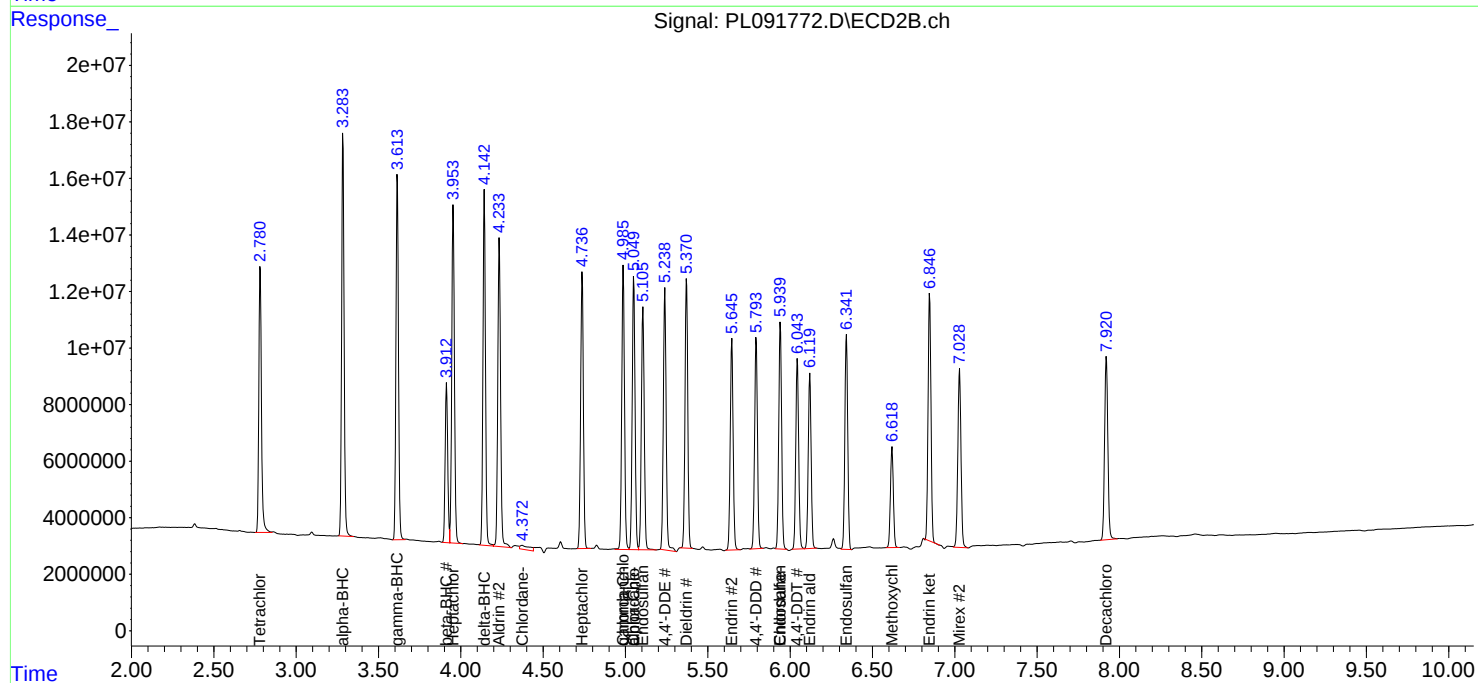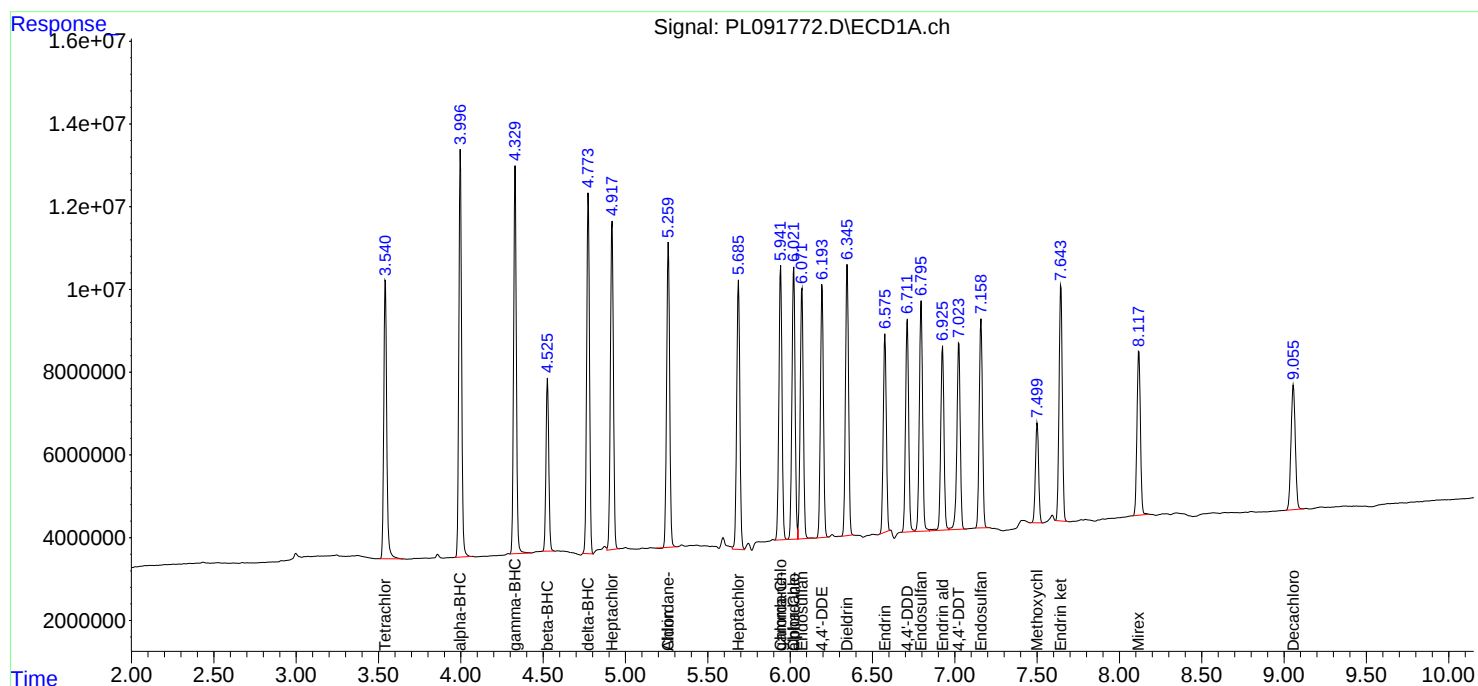


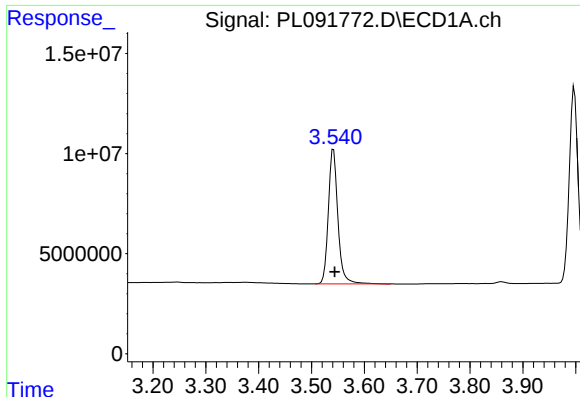

#1 Tetrachloro-m-xylene


R.T.: 3.542 min
Delta R.T.: -0.002 min
Response: 84666071
Conc: 54.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

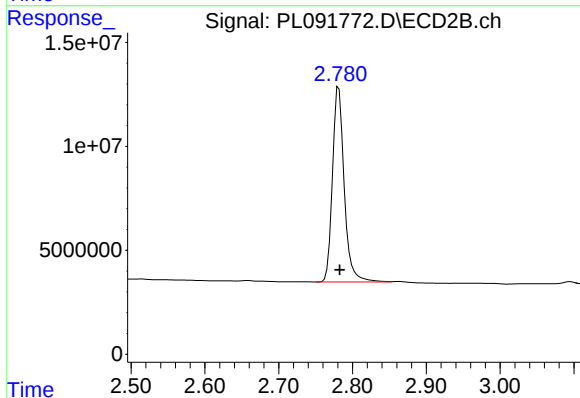


#1 Tetrachloro-m-xylene

R.T.: 2.781 min
Delta R.T.: -0.001 min
Response: 103992357
Conc: 55.60 ng/ml

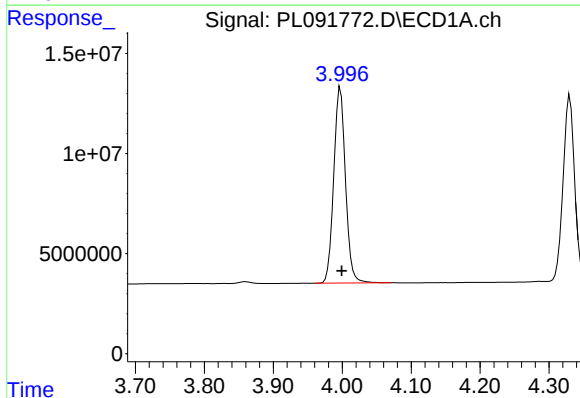


#2 alpha-BHC

R.T.: 3.997 min
Delta R.T.: -0.002 min
Response: 115460505
Conc: 53.46 ng/ml

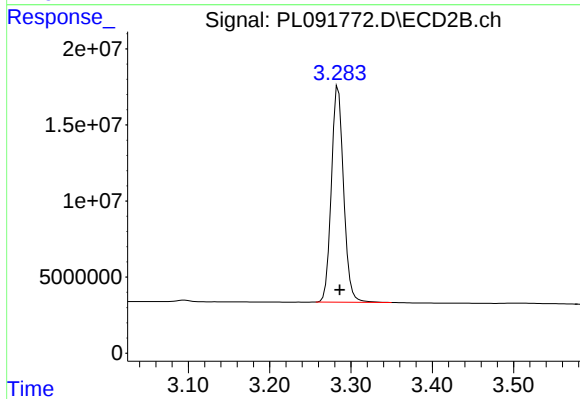

#2 alpha-BHC


R.T.: 3.285 min
Delta R.T.: -0.002 min
Response: 148854174
Conc: 55.97 ng/ml

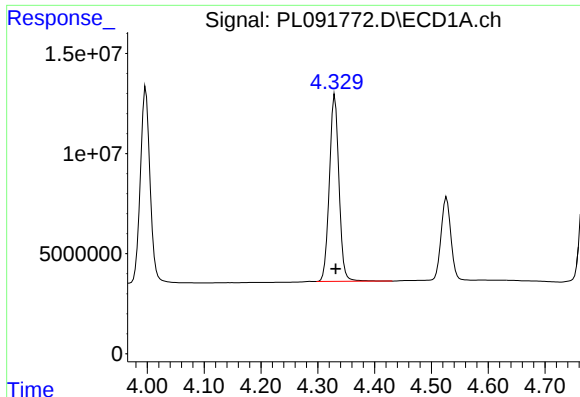

#3 gamma-BHC (Lindane)


R.T.: 4.330 min
Delta R.T.: -0.002 min
Response: 109625494
Conc: 53.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

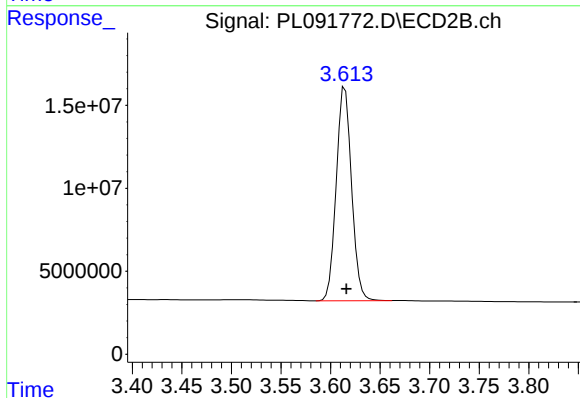


#3 gamma-BHC (Lindane)

R.T.: 3.615 min
Delta R.T.: -0.002 min
Response: 138792654
Conc: 56.43 ng/ml

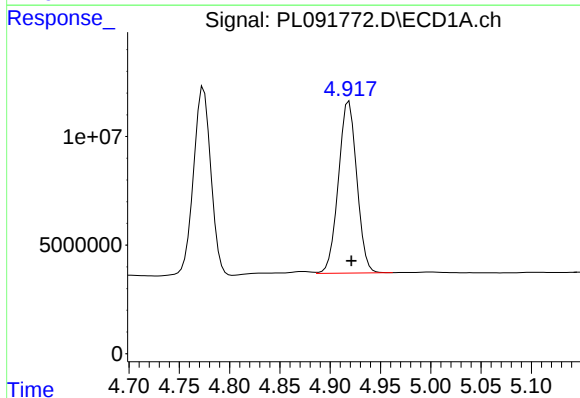


#4 Heptachlor

R.T.: 4.919 min
Delta R.T.: -0.002 min
Response: 100559741
Conc: 53.69 ng/ml

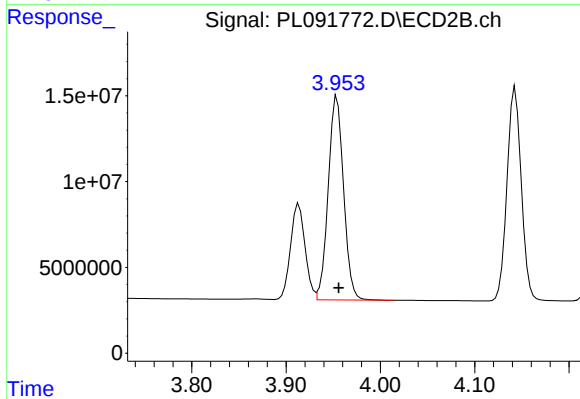

#4 Heptachlor


R.T.: 3.954 min
Delta R.T.: -0.002 min
Response: 134361484
Conc: 55.79 ng/ml

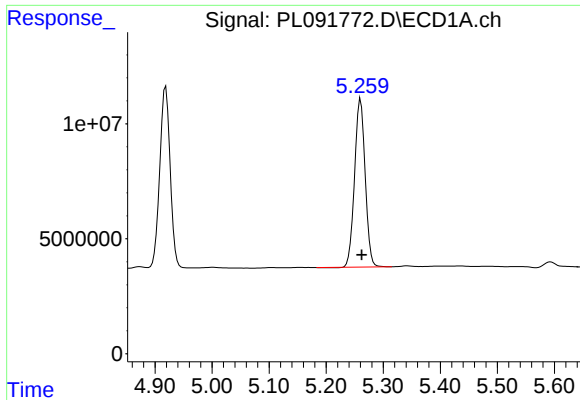

#5 Aldrin


R.T.: 5.260 min
Delta R.T.: -0.002 min
Response: 94316308
Conc: 50.64 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

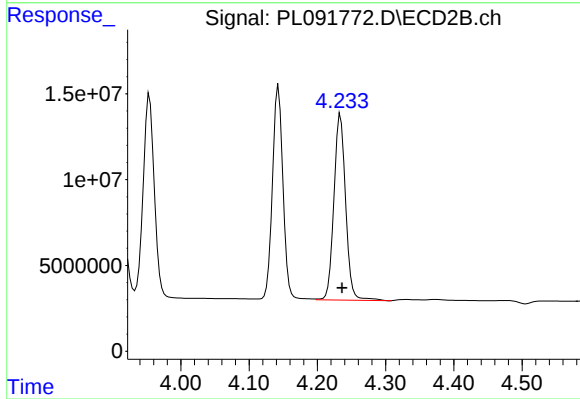


#5 Aldrin

R.T.: 4.234 min
Delta R.T.: -0.002 min
Response: 129555610
Conc: 56.79 ng/ml

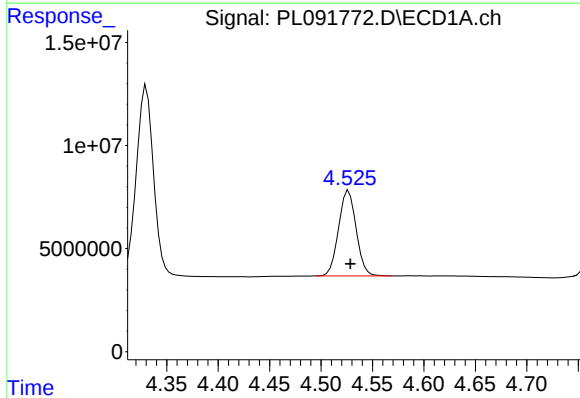


#6 beta-BHC

R.T.: 4.527 min
Delta R.T.: -0.002 min
Response: 49376625
Conc: 54.26 ng/ml

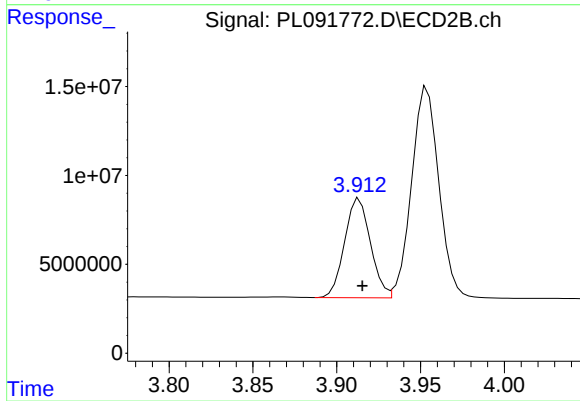

#6 beta-BHC


R.T.: 3.914 min
Delta R.T.: -0.002 min
Response: 59984624
Conc: 54.91 ng/ml

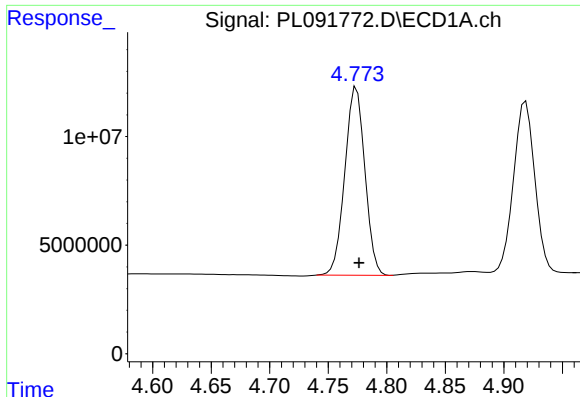

#7 delta-BHC


R.T.: 4.774 min
Delta R.T.: -0.002 min
Response: 103437363
Conc: 53.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

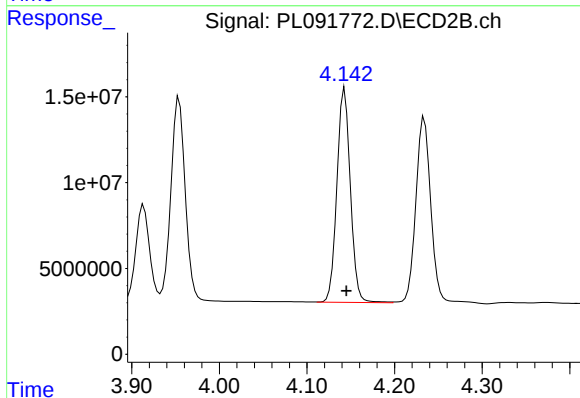


#7 delta-BHC

R.T.: 4.143 min
Delta R.T.: -0.002 min
Response: 133299266
Conc: 57.94 ng/ml

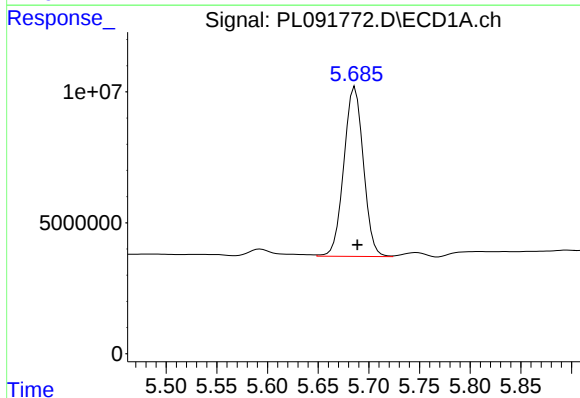


#8 Heptachlor epoxide

R.T.: 5.686 min
Delta R.T.: -0.002 min
Response: 86720621
Conc: 51.97 ng/ml

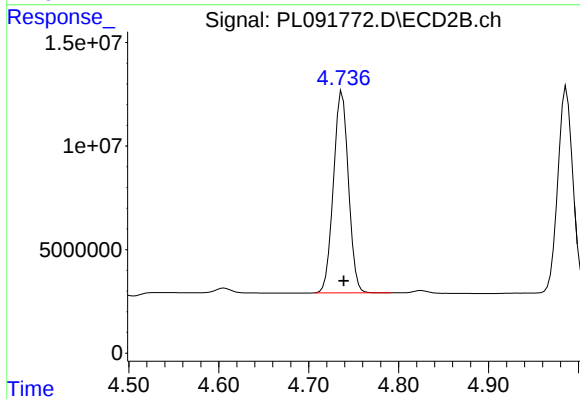

#8 Heptachlor epoxide


R.T.: 4.737 min
Delta R.T.: -0.002 min
Response: 113039021
Conc: 53.63 ng/ml

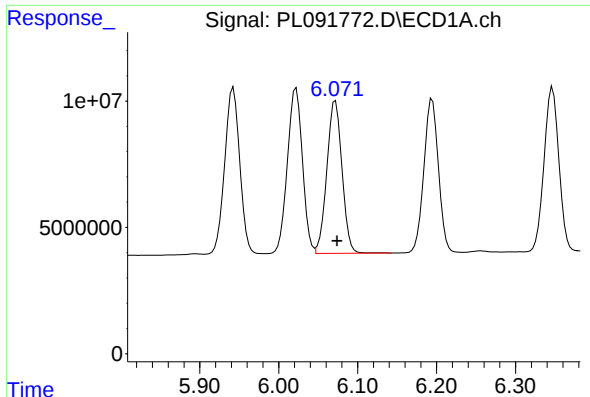

#9 Endosulfan I


R.T.: 6.072 min
Delta R.T.: -0.002 min
Response: 80700446
Conc: 51.79 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

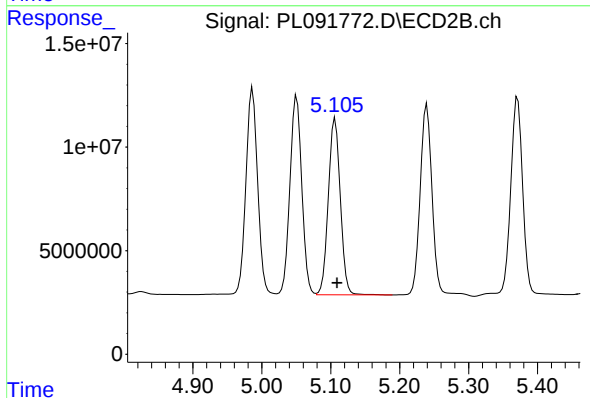


#9 Endosulfan I

R.T.: 5.106 min
Delta R.T.: -0.003 min
Response: 103222219
Conc: 53.50 ng/ml

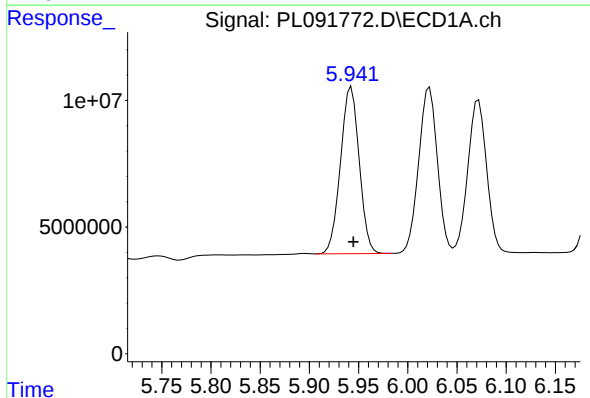


#10 gamma-Chlordane

R.T.: 5.943 min
Delta R.T.: -0.002 min
Response: 87233102
Conc: 52.21 ng/ml

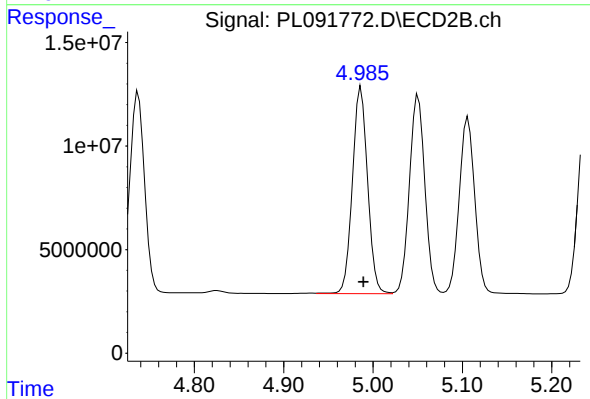

#10 gamma-Chlordane


R.T.: 4.987 min
Delta R.T.: -0.003 min
Response: 117934939
Conc: 53.47 ng/ml

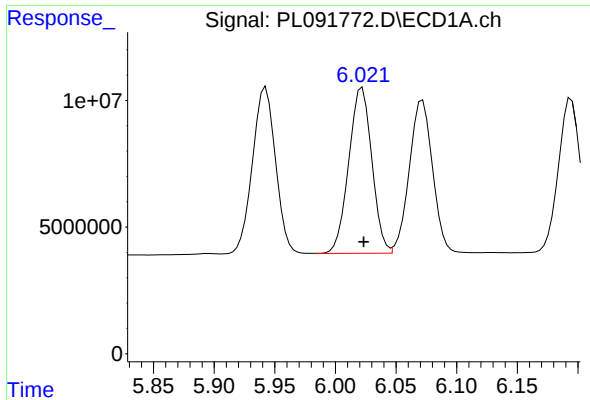

#11 alpha-Chlordane


R.T.: 6.022 min
Delta R.T.: -0.001 min
Response: 86920119
Conc: 53.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

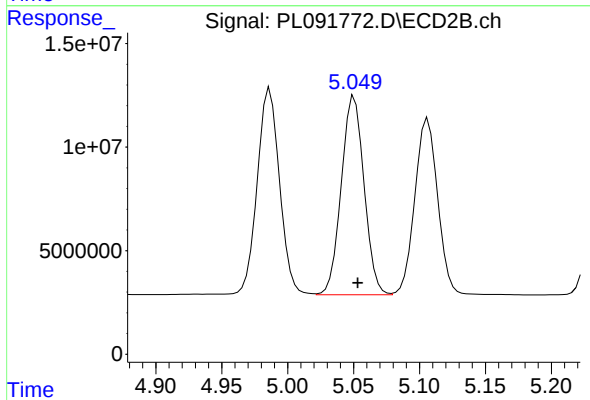


#11 alpha-Chlordane

R.T.: 5.051 min
Delta R.T.: -0.003 min
Response: 115280915
Conc: 55.72 ng/ml

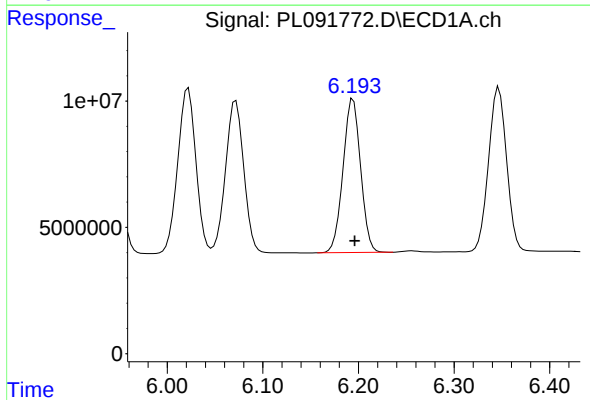


#12 4,4'-DDE

R.T.: 6.194 min
Delta R.T.: -0.002 min
Response: 78052750
Conc: 53.51 ng/ml

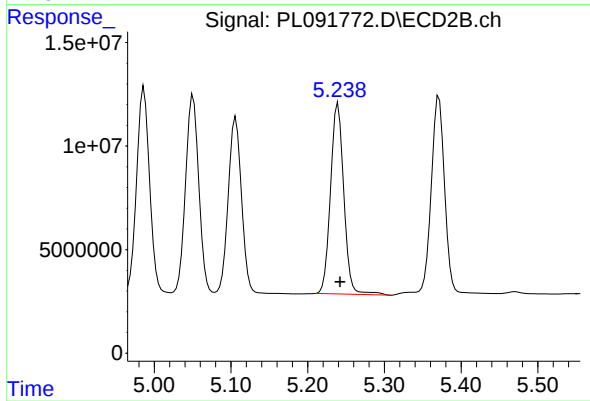

#12 4,4'-DDE


R.T.: 5.240 min
Delta R.T.: -0.002 min
Response: 110923600
Conc: 58.48 ng/ml

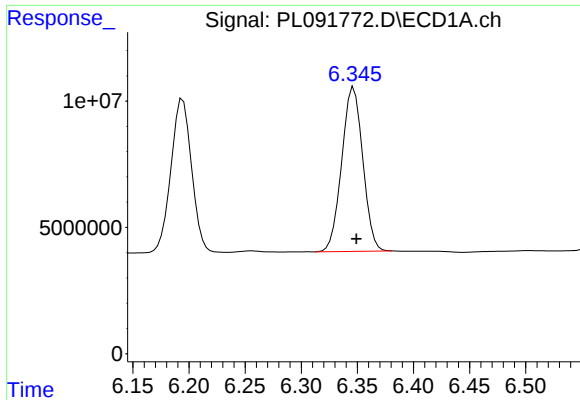

#13 Dieldrin


R.T.: 6.347 min
Delta R.T.: -0.002 min
Response: 84831547
Conc: 51.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

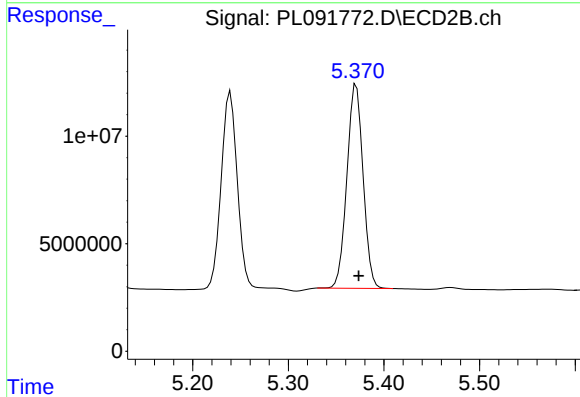


#13 Dieldrin

R.T.: 5.371 min
Delta R.T.: -0.002 min
Response: 112068258
Conc: 54.52 ng/ml

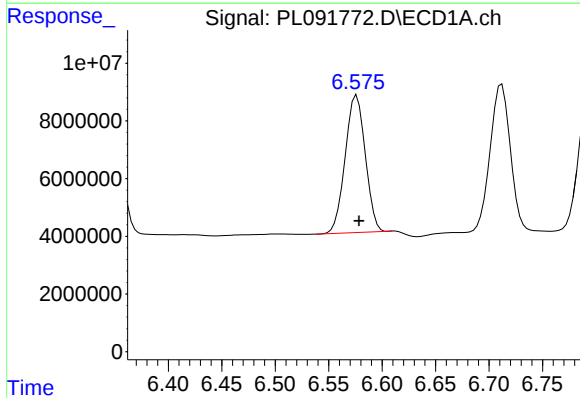


#14 Endrin

R.T.: 6.576 min
Delta R.T.: -0.002 min
Response: 62529858
Conc: 47.03 ng/ml

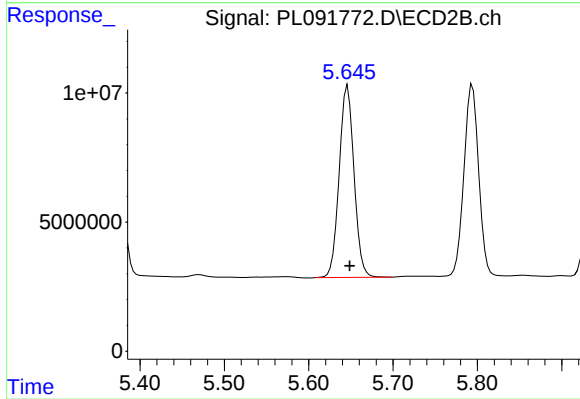

#14 Endrin


R.T.: 5.646 min
Delta R.T.: -0.003 min
Response: 90941362
Conc: 48.19 ng/ml

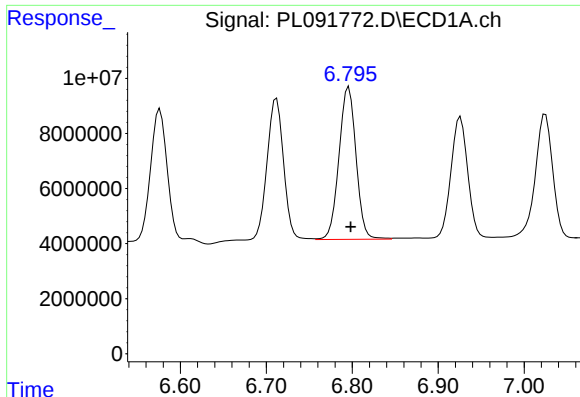

#15 Endosulfan II


R.T.: 6.796 min
Delta R.T.: -0.002 min
Response: 76408901
Conc: 49.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

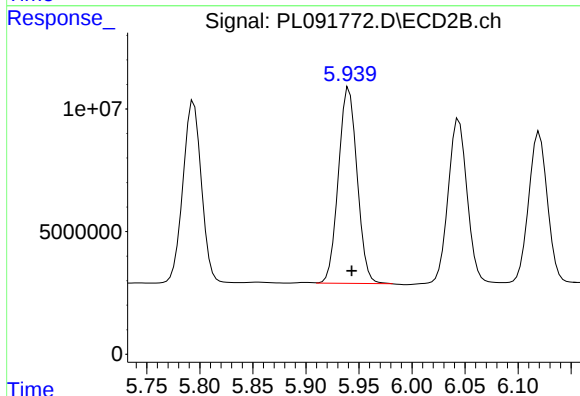


#15 Endosulfan II

R.T.: 5.941 min
Delta R.T.: -0.003 min
Response: 97762246
Conc: 55.27 ng/ml

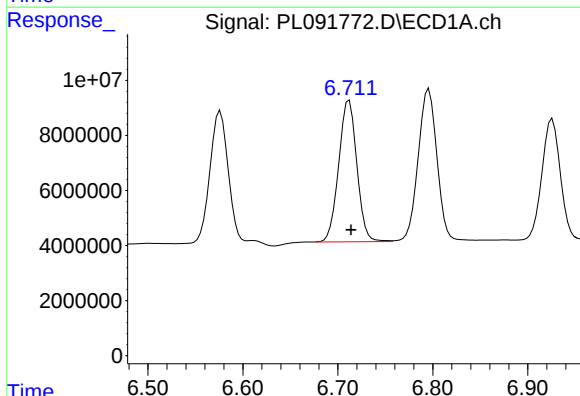


#16 4,4'-DDD

R.T.: 6.712 min
Delta R.T.: -0.002 min
Response: 68340970
Conc: 53.92 ng/ml

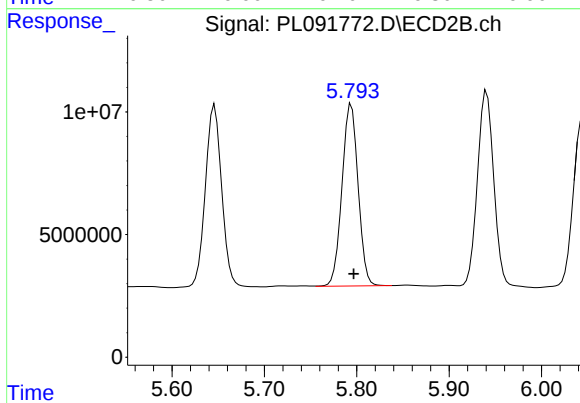

#16 4,4'-DDD


R.T.: 5.794 min
Delta R.T.: -0.003 min
Response: 90077037
Conc: 53.75 ng/ml

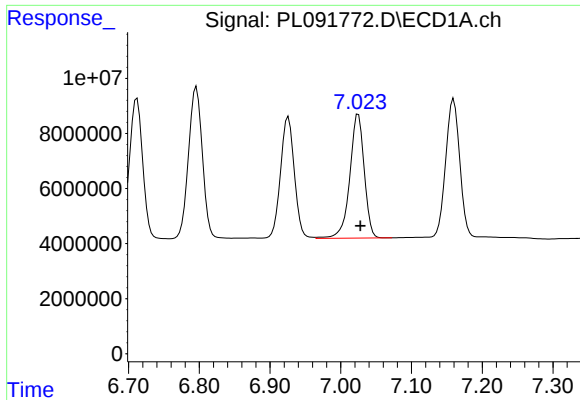

#17 4,4'-DDT


R.T.: 7.025 min
Delta R.T.: -0.003 min
Response: 63845610
Conc: 48.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

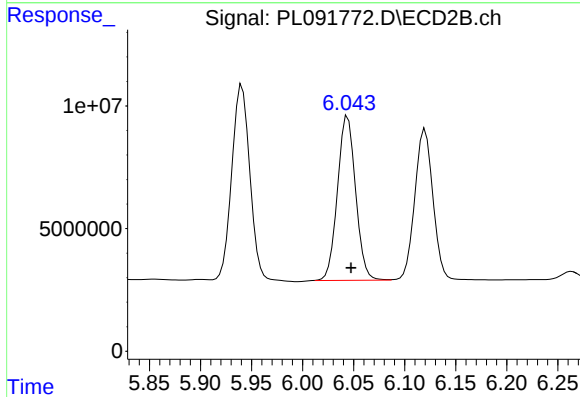


#17 4,4'-DDT

R.T.: 6.044 min
Delta R.T.: -0.003 min
Response: 82901465
Conc: 51.59 ng/ml

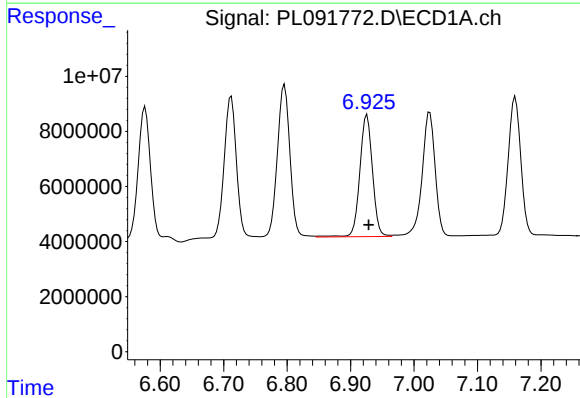


#18 Endrin aldehyde

R.T.: 6.926 min
Delta R.T.: -0.003 min
Response: 61040601
Conc: 51.38 ng/ml

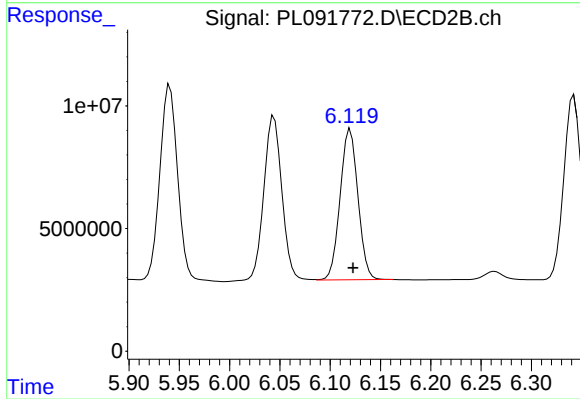

#18 Endrin aldehyde


R.T.: 6.120 min
Delta R.T.: -0.003 min
Response: 75681556
Conc: 55.36 ng/ml

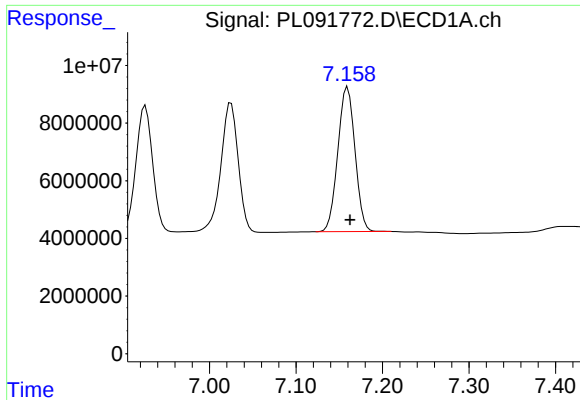

#19 Endosulfan Sulfate


R.T.: 7.160 min
Delta R.T.: -0.003 min
Response: 68861600
Conc: 49.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

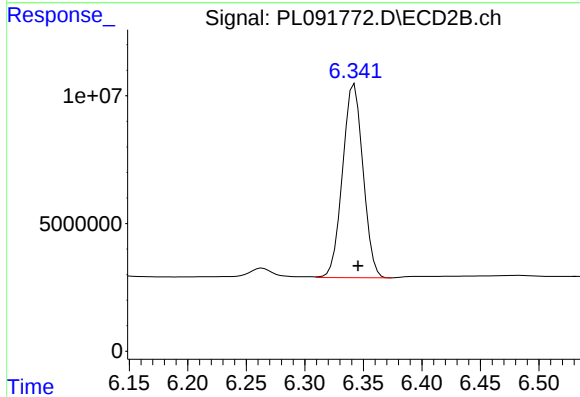


#19 Endosulfan Sulfate

R.T.: 6.342 min
Delta R.T.: -0.003 min
Response: 92360678
Conc: 53.82 ng/ml

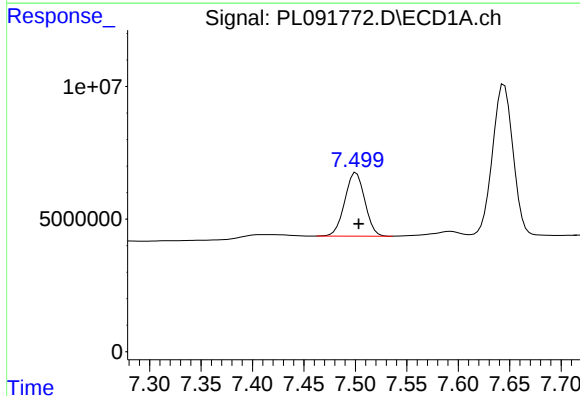


#20 Methoxychlor

R.T.: 7.501 min
Delta R.T.: -0.003 min
Response: 32441738
Conc: 47.96 ng/ml

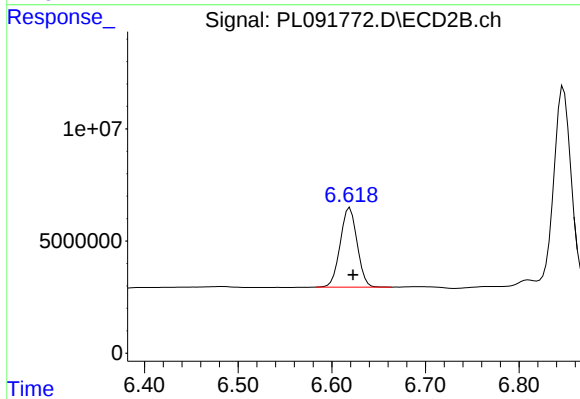

#20 Methoxychlor


R.T.: 6.619 min
Delta R.T.: -0.003 min
Response: 44477886
Conc: 50.21 ng/ml

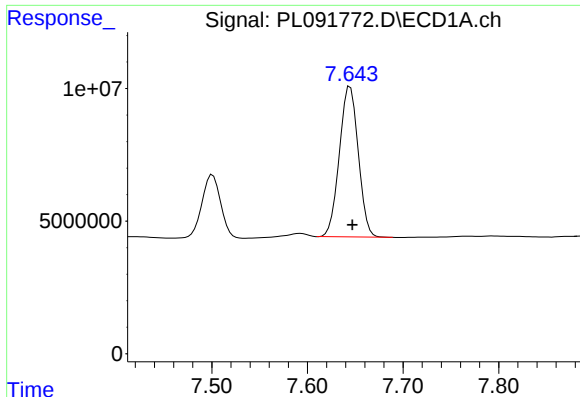

#21 Endrin ketone


R.T.: 7.645 min
Delta R.T.: -0.002 min
Response: 78173855
Conc: 50.55 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

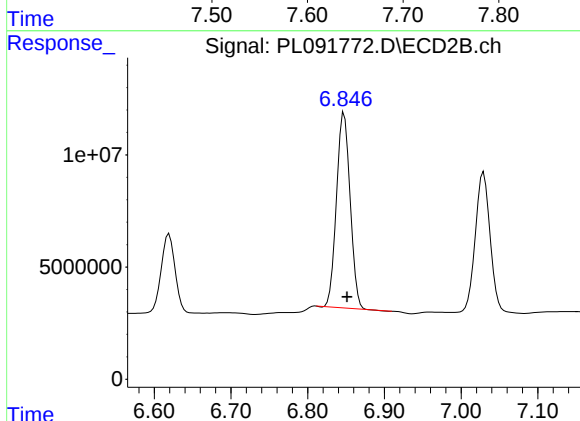


#21 Endrin ketone

R.T.: 6.848 min
Delta R.T.: -0.004 min
Response: 107245440
Conc: 53.32 ng/ml

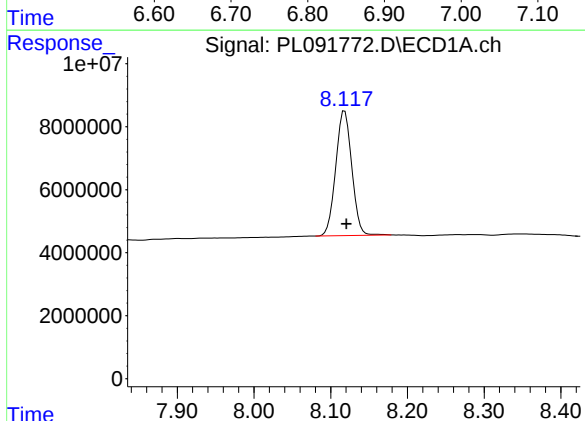


#22 Mirex

R.T.: 8.118 min
Delta R.T.: -0.003 min
Response: 57722017
Conc: 48.20 ng/ml

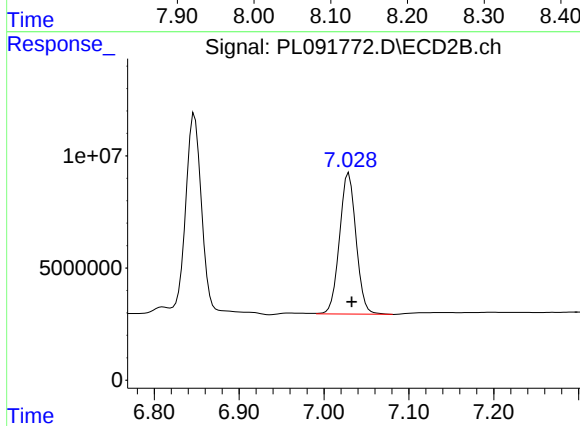

#22 Mirex


R.T.: 7.029 min
Delta R.T.: -0.003 min
Response: 84907475
Conc: 47.88 ng/ml

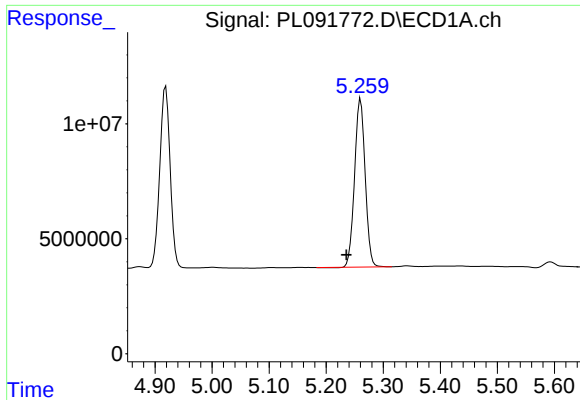

#24 Chlordane-2


R.T.: 5.260 min
Delta R.T.: 0.025 min
Response: 94316308
Conc: 1226.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

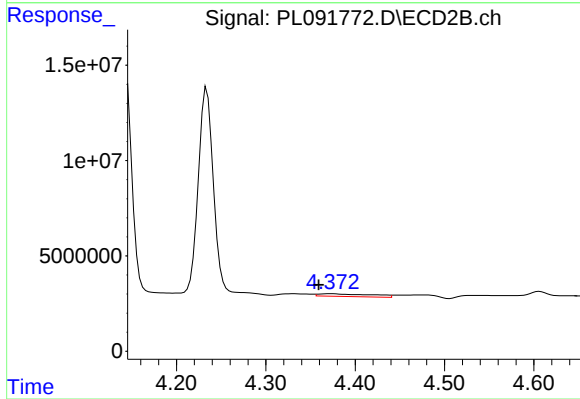


#24 Chlordane-2

R.T.: 4.372 min
Delta R.T.: 0.013 min
Response: 5921874
Conc: 79.01 ng/ml

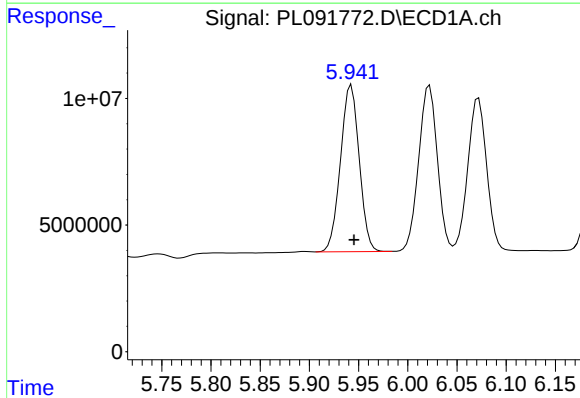


#25 Chlordane-3

R.T.: 5.943 min
Delta R.T.: -0.003 min
Response: 87233102
Conc: 339.56 ng/ml

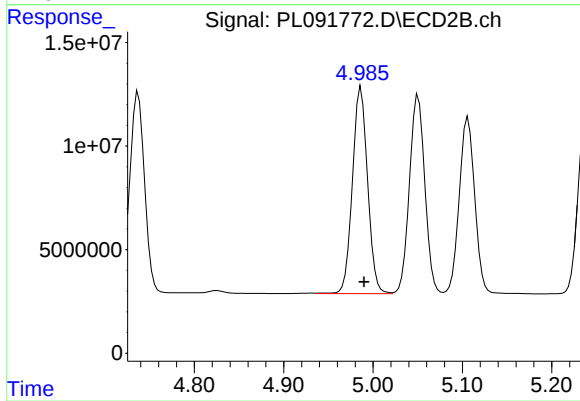

#25 Chlordane-3


R.T.: 4.987 min
Delta R.T.: -0.003 min
Response: 117934939
Conc: 505.85 ng/ml

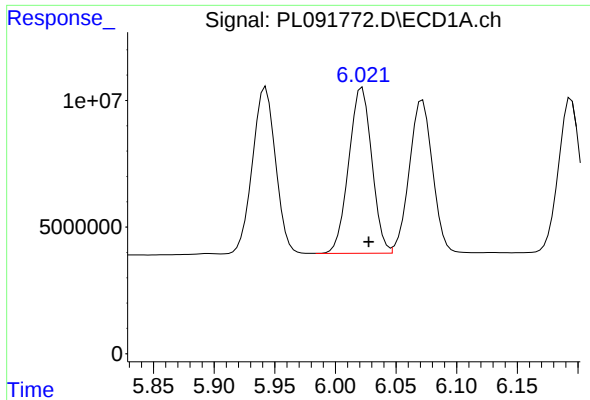

#26 Chlordane-4


R.T.: 6.022 min
Delta R.T.: -0.005 min
Response: 86920119
Conc: 293.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

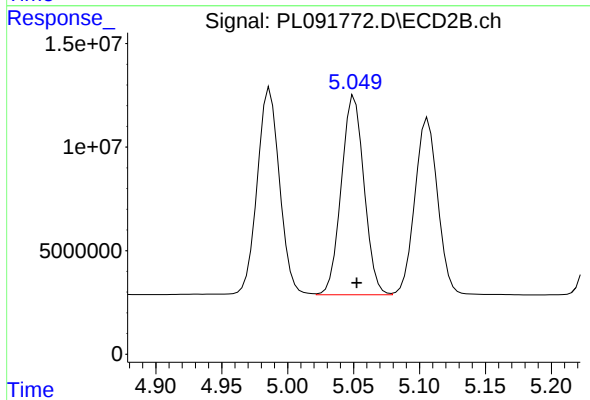


#26 Chlordane-4

R.T.: 5.051 min
Delta R.T.: -0.002 min
Response: 115280915
Conc: 552.82 ng/ml

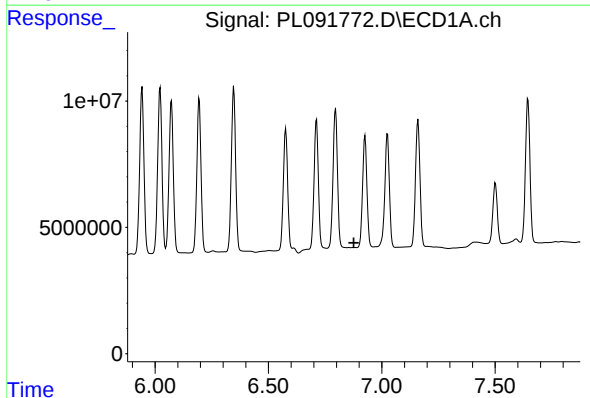


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.876 min
Response: 0
Conc: N.D.

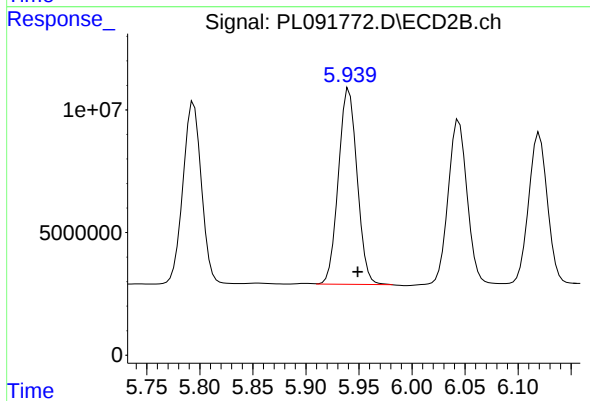

#27 Chlordane-5


R.T.: 5.941 min
Delta R.T.: -0.008 min
Response: 97762246
Conc: 1364.24 ng/ml

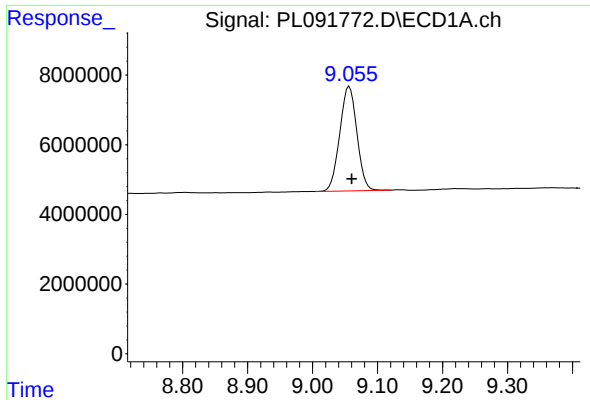

#28 Decachlorobiphenyl

R.T.: 9.057 min
Delta R.T.: -0.004 min
Response: 54962559
Conc: 45.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

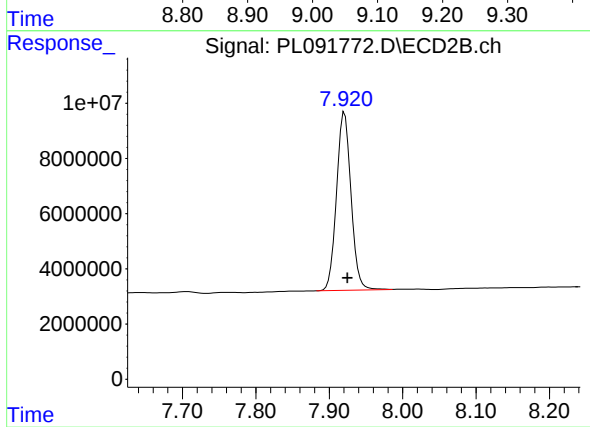

#28 Decachlorobiphenyl

R.T.: 7.921 min
Delta R.T.: -0.004 min
Response: 88678834
Conc: 48.02 ng/ml