

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091625\
 Data File : PL097214.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Sep 2025 10:44
 Operator : AR\AJ
 Sample : INDA101
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 INDA1312

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 17 04:42:24 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091625CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 17 04:40:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.527	2.823	17253517	24748910	5.086	5.130
27)	SA Decachlor...	8.997	7.982	27605234	47401727	10.778	10.907
Target Compounds							
2)	A alpha-BHC	3.974	3.328	25669867	33779551	4.841	4.714
3)	MA gamma-BHC...	4.302	3.660	25531935	32667448	5.064	4.874
4)	MA Heptachlor	4.893	4.008	26246804	34264961	5.087	5.076
9)	A Endosulfan I	6.032	5.162	20912868	27586635	5.302	5.174
13)	MA Dieldrin	6.304	5.427	40958127	58970114	9.805	9.860
14)	MA Endrin	6.530	5.701	33328283	54215068	9.839	10.164
16)	A 4,4'-DDD	6.663	5.848	26929441	46130675	9.795	9.768
17)	MA 4,4'-DDT	6.977	6.100	27838310	44316362	9.762	9.352
20)	A Methoxychlor	7.450	6.672	79422804	138.0E6	51.803	53.846


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091625\
Data File : PL097214.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Sep 2025 10:44
Operator : AR\AJ
Sample : INDA101
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 04:42:24 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091625CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 17 04:40:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

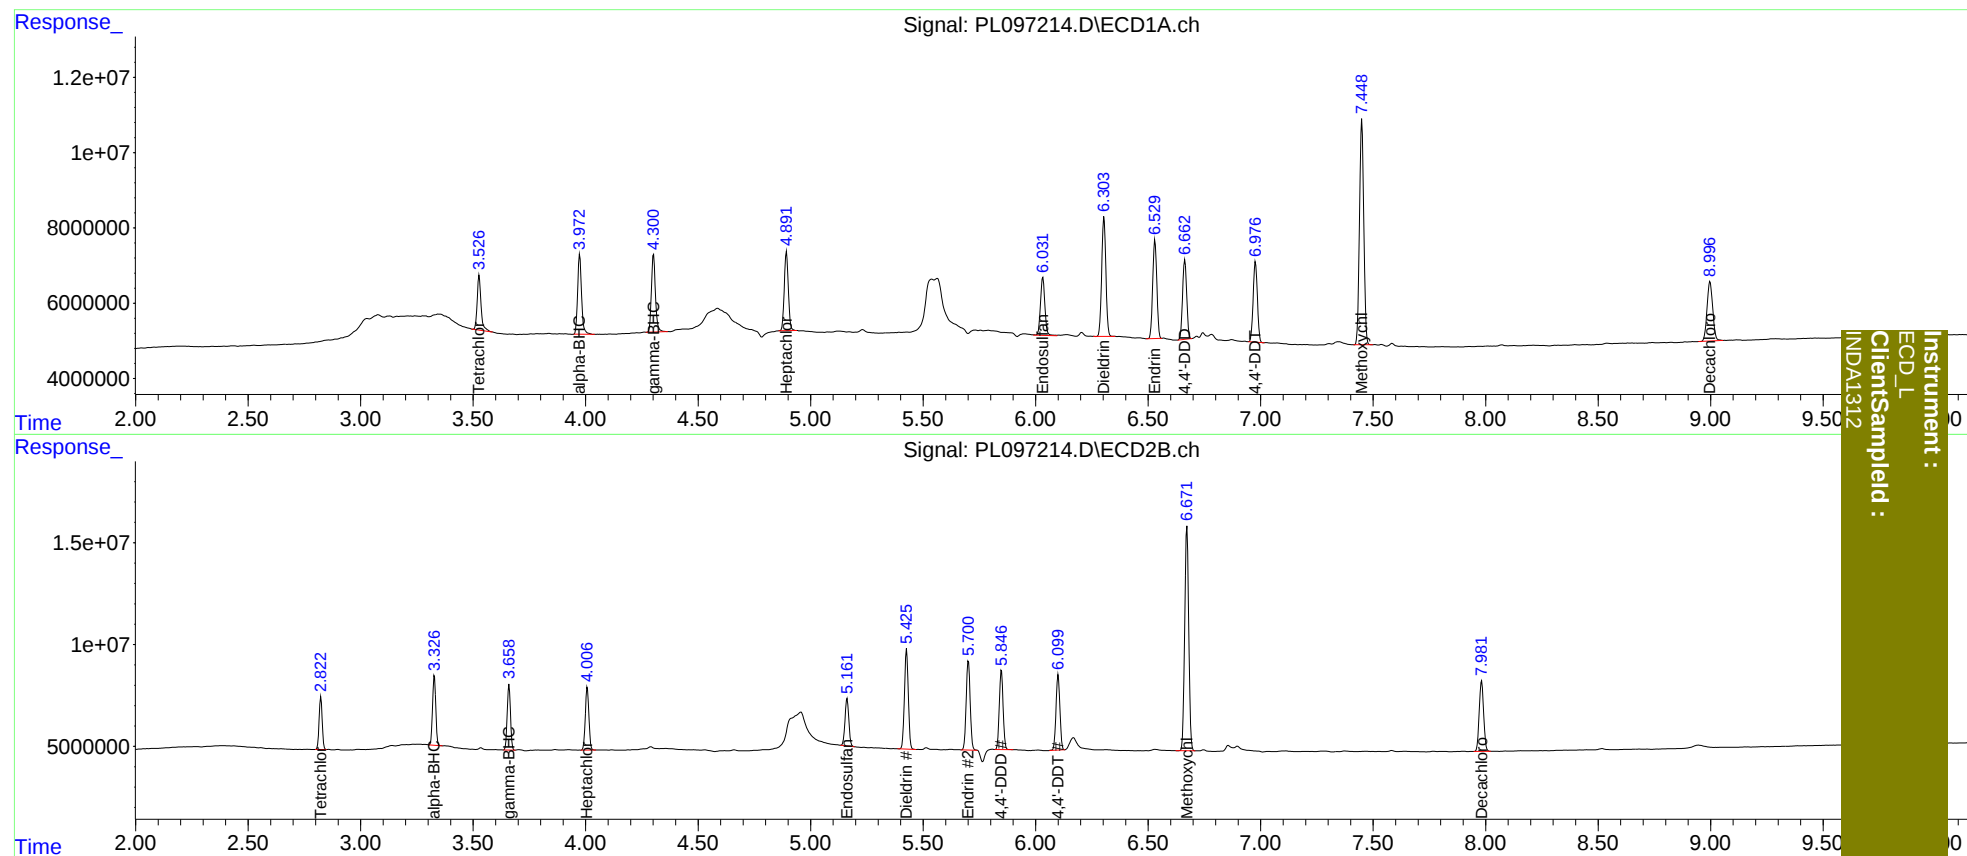


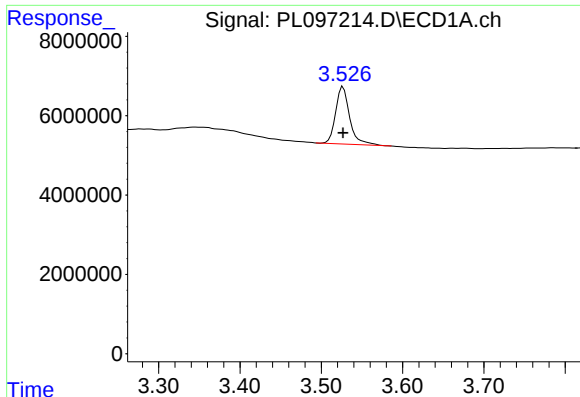

#1 Tetrachloro-m-xylene


R.T.: 3.527 min
Delta R.T.: 0.000 min
Response: 17253517
Conc: 5.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA1312

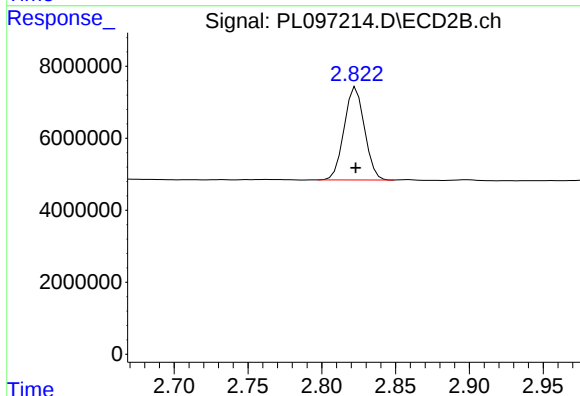


#1 Tetrachloro-m-xylene

R.T.: 2.823 min
Delta R.T.: 0.000 min
Response: 24748910
Conc: 5.13 ng/ml

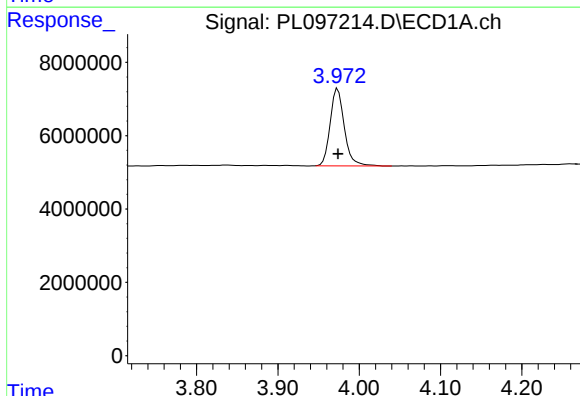


#2 alpha-BHC

R.T.: 3.974 min
Delta R.T.: 0.000 min
Response: 25669867
Conc: 4.84 ng/ml

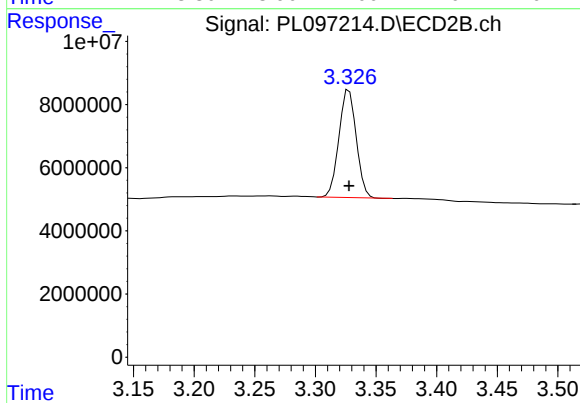

#2 alpha-BHC


R.T.: 3.328 min
Delta R.T.: 0.000 min
Response: 33779551
Conc: 4.71 ng/ml

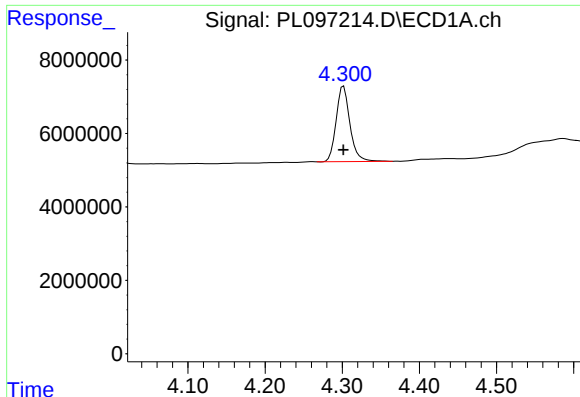

#3 gamma-BHC (Lindane)


R.T.: 4.302 min
Delta R.T.: 0.000 min
Response: 25531935
Conc: 5.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA1312

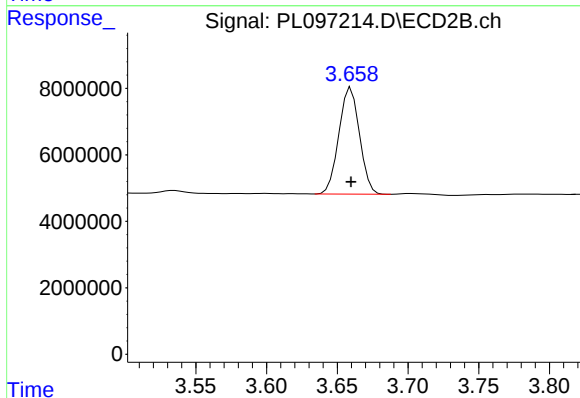


#3 gamma-BHC (Lindane)

R.T.: 3.660 min
Delta R.T.: 0.000 min
Response: 32667448
Conc: 4.87 ng/ml

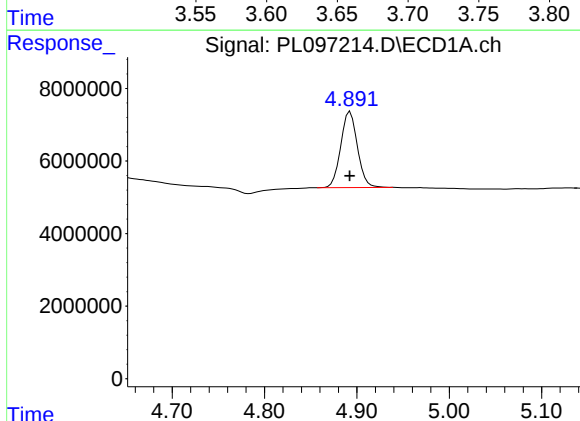


#4 Heptachlor

R.T.: 4.893 min
Delta R.T.: 0.000 min
Response: 26246804
Conc: 5.09 ng/ml

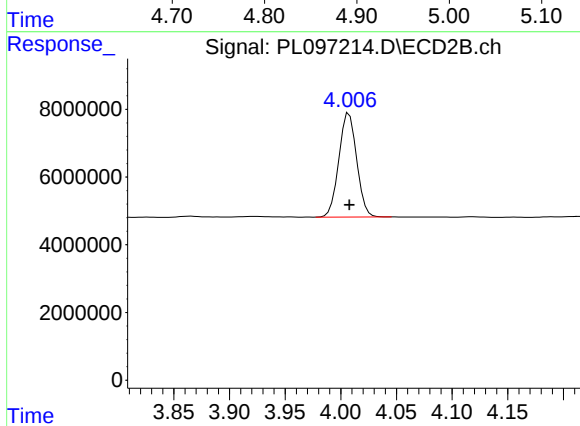

#4 Heptachlor


R.T.: 4.008 min
Delta R.T.: 0.000 min
Response: 34264961
Conc: 5.08 ng/ml

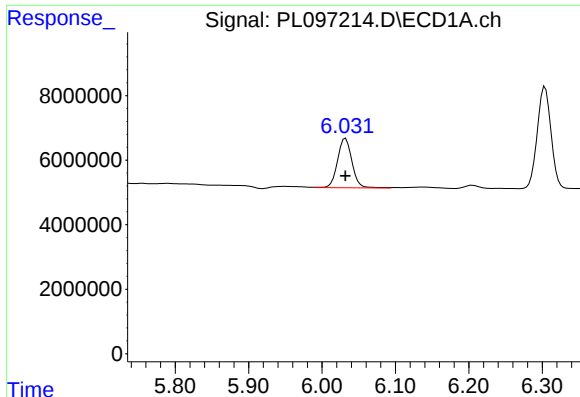

#9 Endosulfan I


R.T.: 6.032 min
Delta R.T.: 0.000 min
Response: 20912868
Conc: 5.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA1312

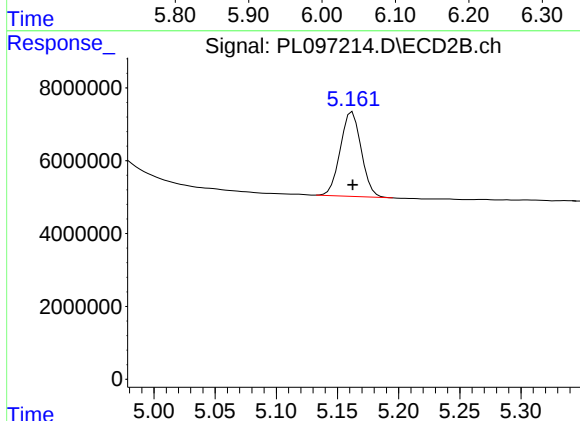


#9 Endosulfan I

R.T.: 5.162 min
Delta R.T.: 0.000 min
Response: 27586635
Conc: 5.17 ng/ml

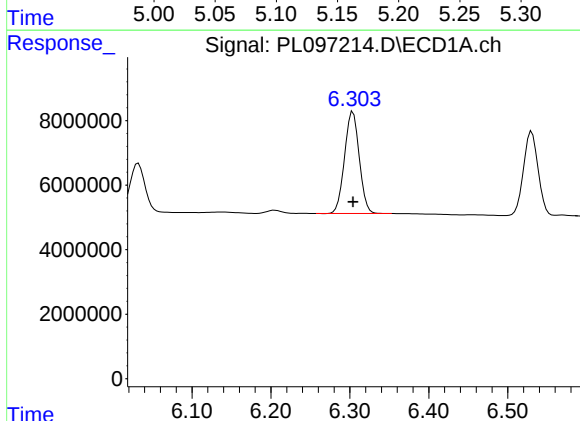


#13 Dieldrin

R.T.: 6.304 min
Delta R.T.: 0.000 min
Response: 40958127
Conc: 9.80 ng/ml

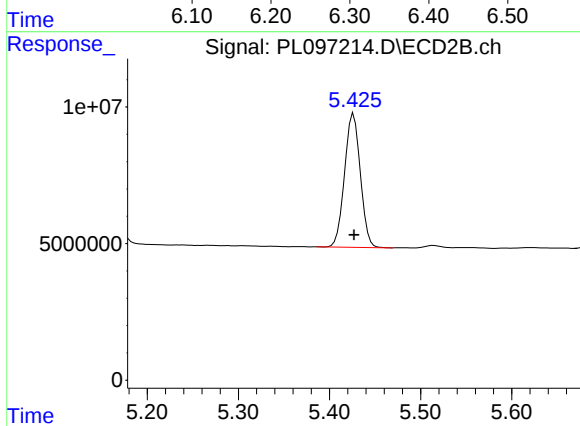

#13 Dieldrin


R.T.: 5.427 min
Delta R.T.: 0.000 min
Response: 58970114
Conc: 9.86 ng/ml

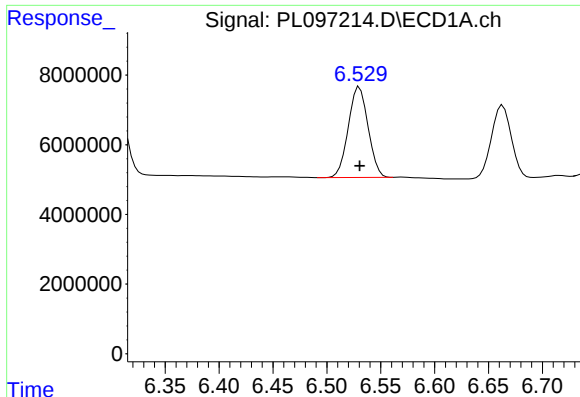

#14 Endrin


R.T.: 6.530 min
Delta R.T.: 0.000 min
Response: 33328283
Conc: 9.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA1312

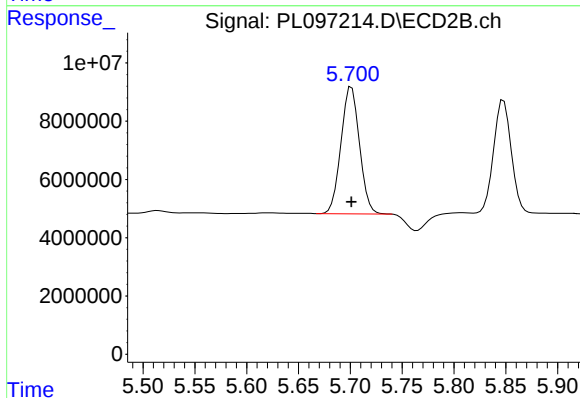


#14 Endrin

R.T.: 5.701 min
Delta R.T.: 0.000 min
Response: 54215068
Conc: 10.16 ng/ml

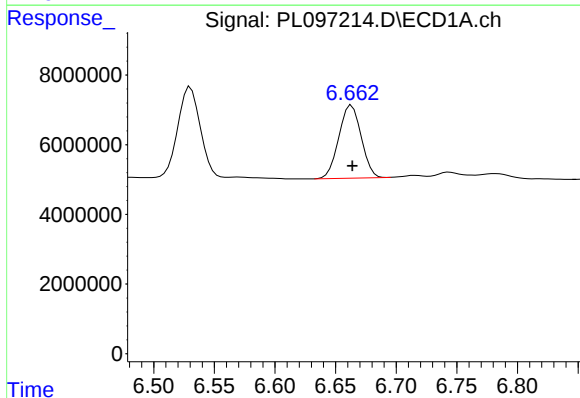


#16 4,4'-DDD

R.T.: 6.663 min
Delta R.T.: 0.000 min
Response: 26929441
Conc: 9.80 ng/ml

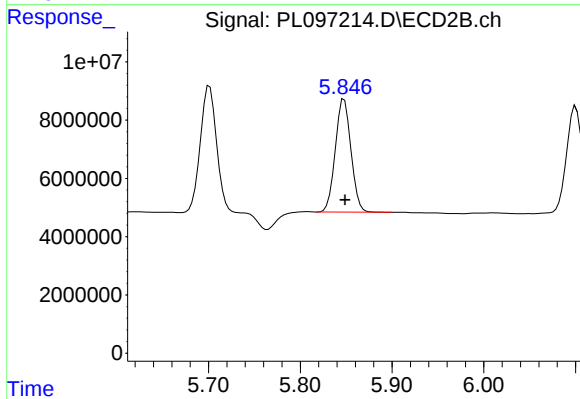

#16 4,4'-DDD


R.T.: 5.848 min
Delta R.T.: 0.000 min
Response: 46130675
Conc: 9.77 ng/ml

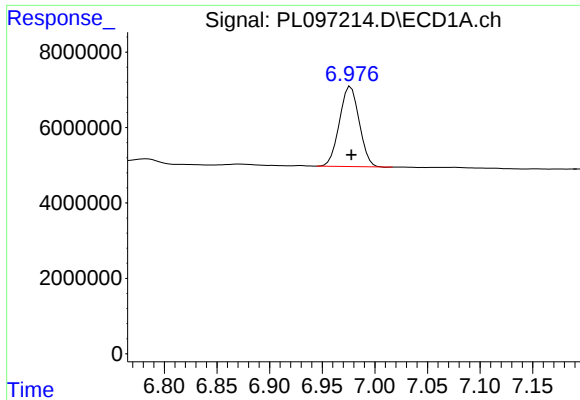

#17 4,4'-DDT


R.T.: 6.977 min
Delta R.T.: 0.000 min
Response: 27838310
Conc: 9.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA1312

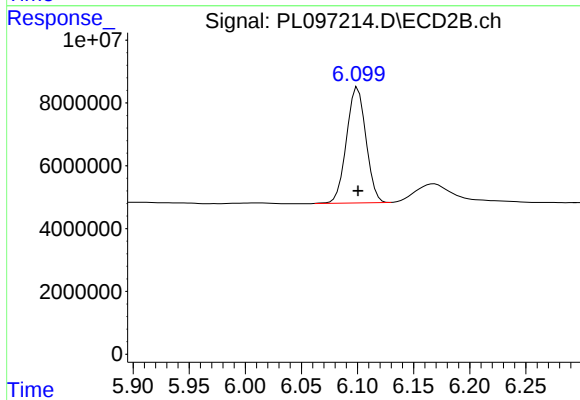


#17 4,4'-DDT

R.T.: 6.100 min
Delta R.T.: 0.000 min
Response: 44316362
Conc: 9.35 ng/ml

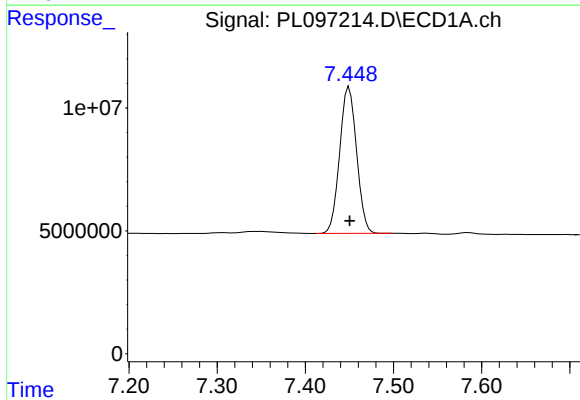


#20 Methoxychlor

R.T.: 7.450 min
Delta R.T.: 0.000 min
Response: 79422804
Conc: 51.80 ng/ml

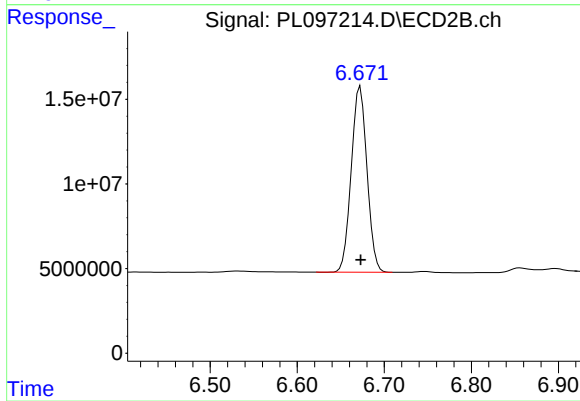

#20 Methoxychlor


R.T.: 6.672 min
Delta R.T.: 0.000 min
Response: 137977650
Conc: 53.85 ng/ml

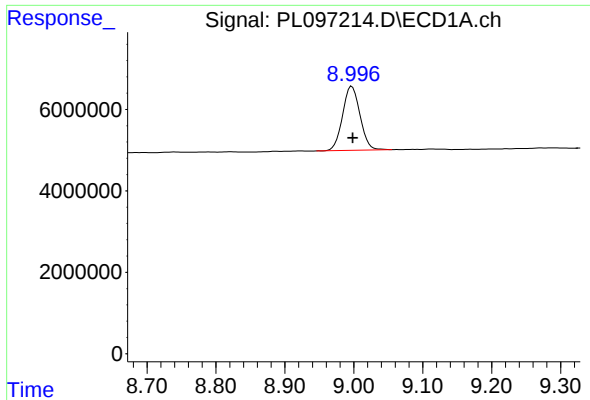

#27 Decachlorobiphenyl

R.T.: 8.997 min
Delta R.T.: -0.001 min
Response: 27605234
Conc: 10.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA1312

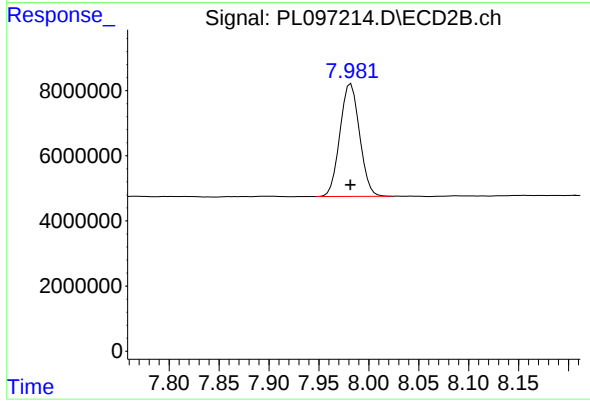

#27 Decachlorobiphenyl

R.T.: 7.982 min
Delta R.T.: 0.000 min
Response: 47401727
Conc: 10.91 ng/ml