

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091625\
 Data File : PL097216.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Sep 2025 11:11
 Operator : AR\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 INDA2314

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 17 04:42:41 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091625CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 17 04:40:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.526	2.823	34258219	48750598	10.098	10.106
27)	SA Decachlor...	8.997	7.982	53774603	90981106	20.996	20.934
Target Compounds							
2)	A alpha-BHC	3.973	3.328	51906184	69341808	9.789	9.677
3)	MA gamma-BHC...	4.301	3.659	50386128	65824854	9.994	9.822
4)	MA Heptachlor	4.892	4.007	52282545	68090359	10.133	10.088
9)	A Endosulfan I	6.032	5.162	43447926	53933190	11.015	10.115
13)	MA Dieldrin	6.305	5.426	83072356	118.2E6	19.886	19.759
14)	MA Endrin	6.531	5.701	67511228	107.2E6	19.931	20.091
16)	A 4,4'-DDD	6.664	5.848	54731638	93169309	19.908	19.728
17)	MA 4,4'-DDT	6.977	6.100	56522626	92175063	19.821	19.451
20)	A Methoxychlor	7.450	6.672	158.4E6	268.4E6	103.319	104.748


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091625\
Data File : PL097216.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Sep 2025 11:11
Operator : AR\AJ
Sample : INDA201
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 04:42:41 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091625CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 17 04:40:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

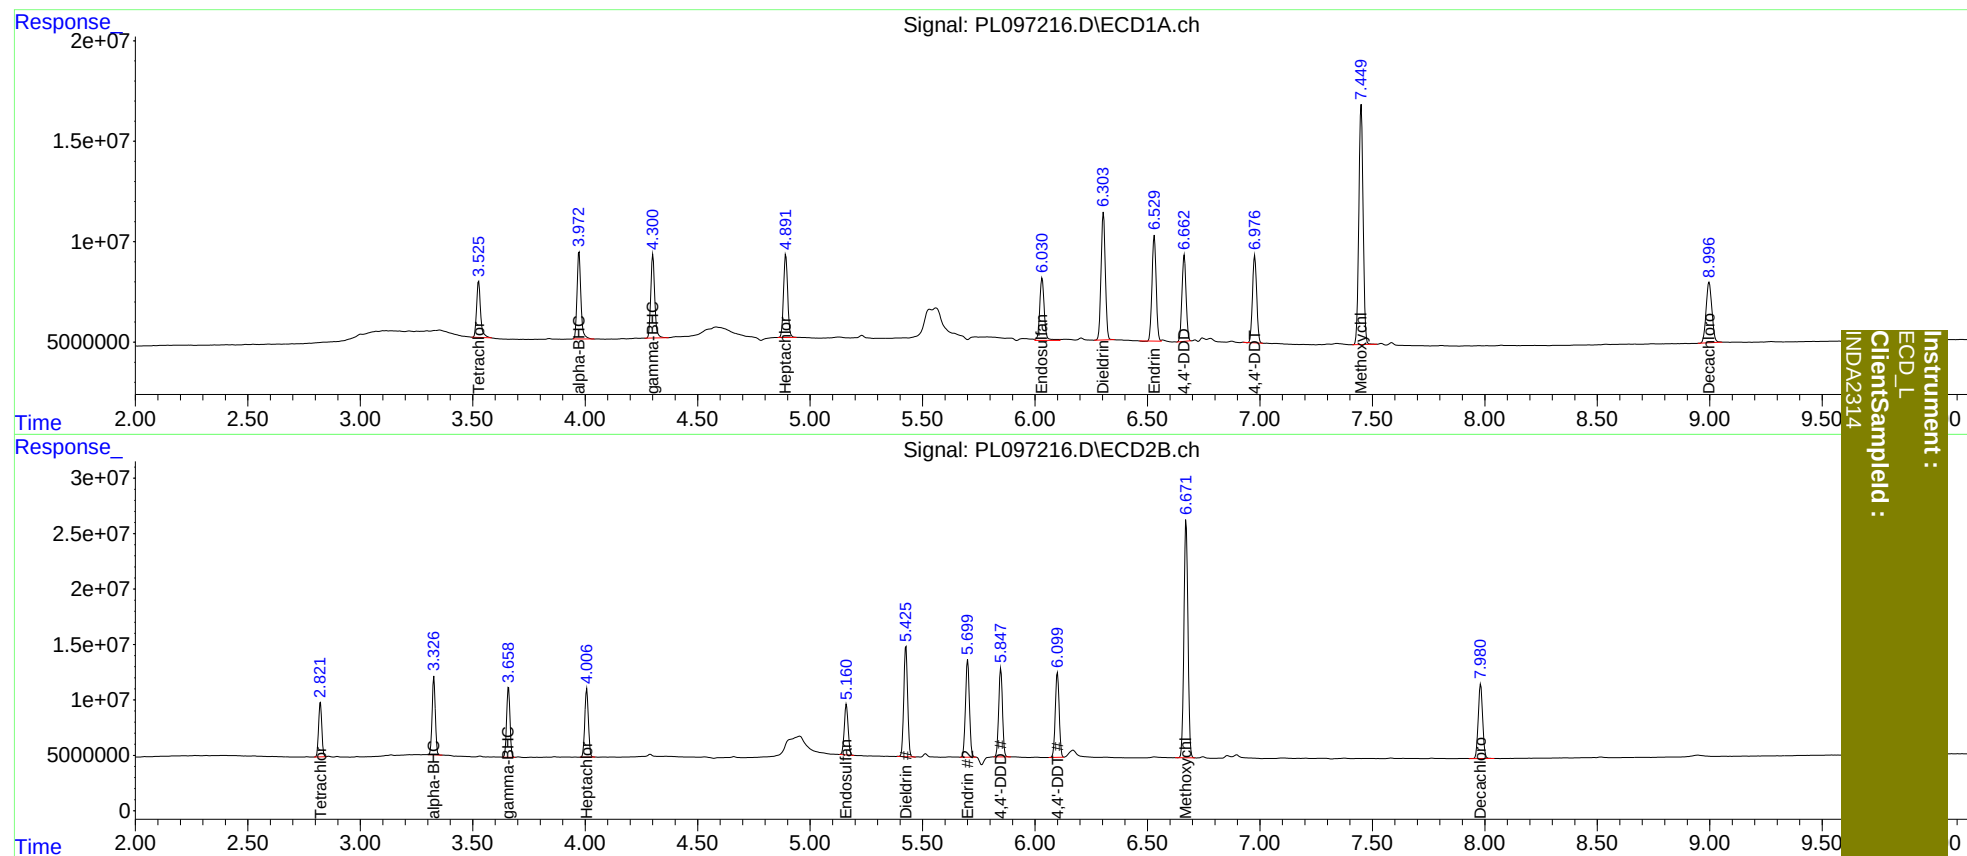


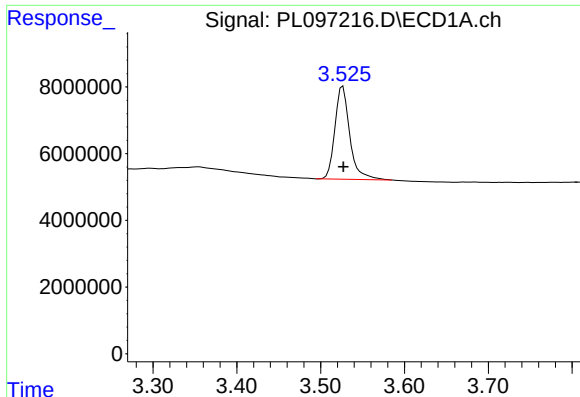

#1 Tetrachloro-m-xylene


R.T.: 3.526 min
Delta R.T.: 0.000 min
Response: 34258219
Conc: 10.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA2314

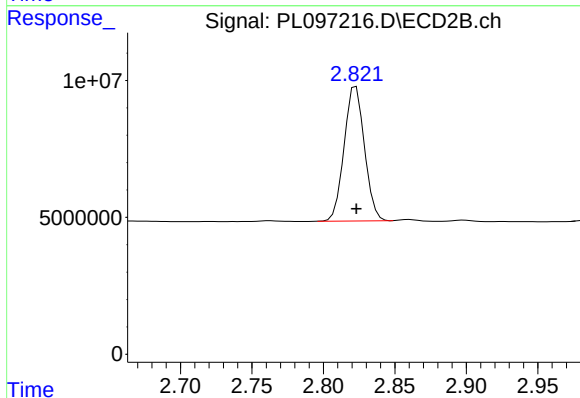


#1 Tetrachloro-m-xylene

R.T.: 2.823 min
Delta R.T.: 0.000 min
Response: 48750598
Conc: 10.11 ng/ml

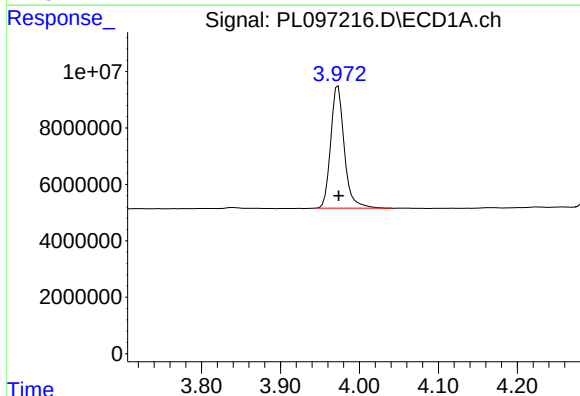


#2 alpha-BHC

R.T.: 3.973 min
Delta R.T.: 0.000 min
Response: 51906184
Conc: 9.79 ng/ml

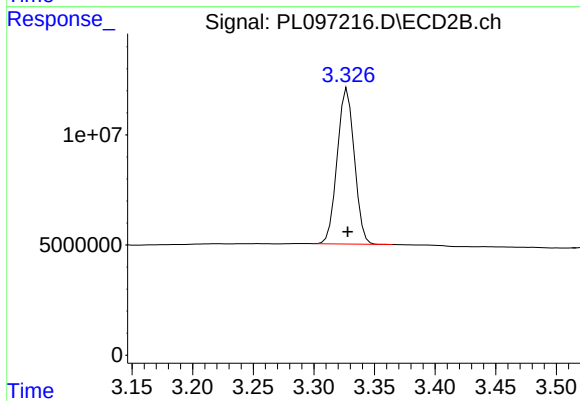

#2 alpha-BHC


R.T.: 3.328 min
Delta R.T.: 0.000 min
Response: 69341808
Conc: 9.68 ng/ml

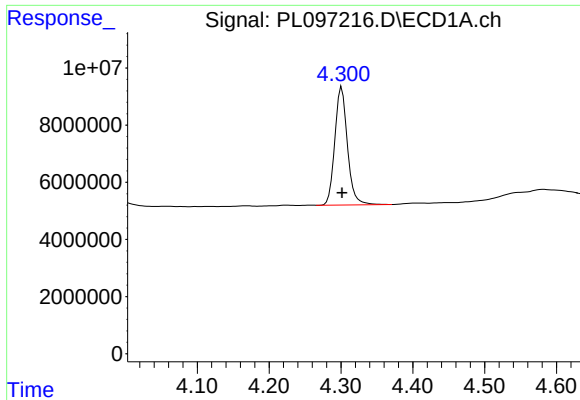

#3 gamma-BHC (Lindane)


R.T.: 4.301 min
Delta R.T.: 0.000 min
Response: 50386128
Conc: 9.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA2314

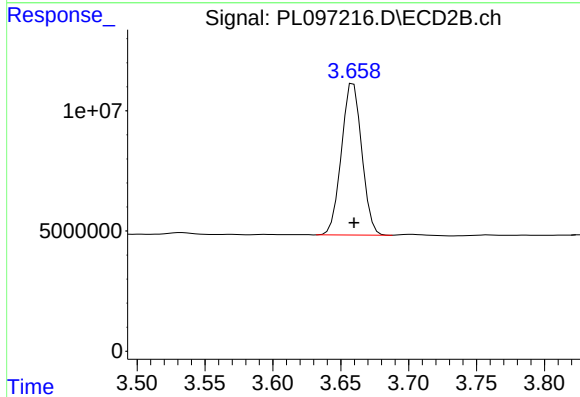


#3 gamma-BHC (Lindane)

R.T.: 3.659 min
Delta R.T.: 0.000 min
Response: 65824854
Conc: 9.82 ng/ml

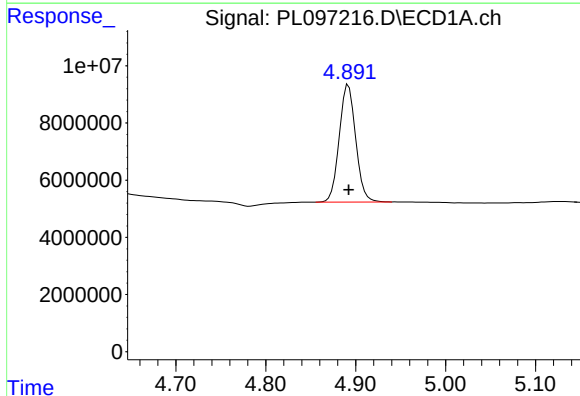


#4 Heptachlor

R.T.: 4.892 min
Delta R.T.: 0.000 min
Response: 52282545
Conc: 10.13 ng/ml

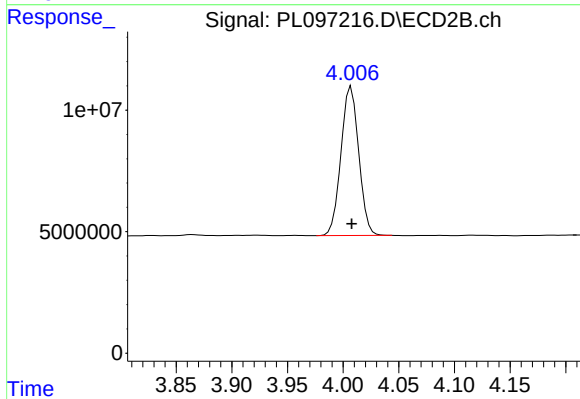

#4 Heptachlor


R.T.: 4.007 min
Delta R.T.: 0.000 min
Response: 68090359
Conc: 10.09 ng/ml

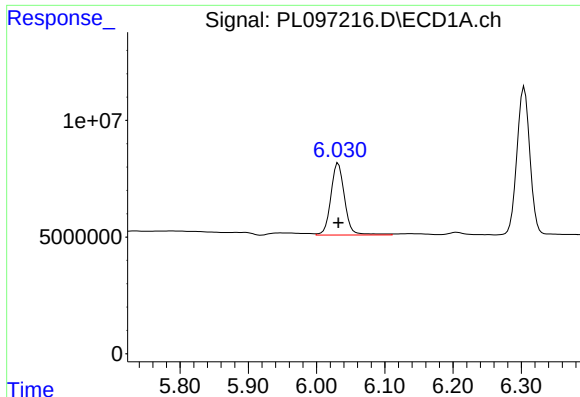

#9 Endosulfan I


R.T.: 6.032 min
Delta R.T.: 0.000 min
Response: 43447926
Conc: 11.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA2314

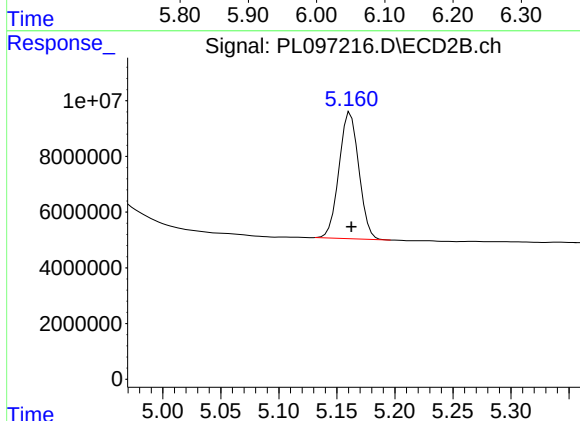


#9 Endosulfan I

R.T.: 5.162 min
Delta R.T.: 0.000 min
Response: 53933190
Conc: 10.12 ng/ml

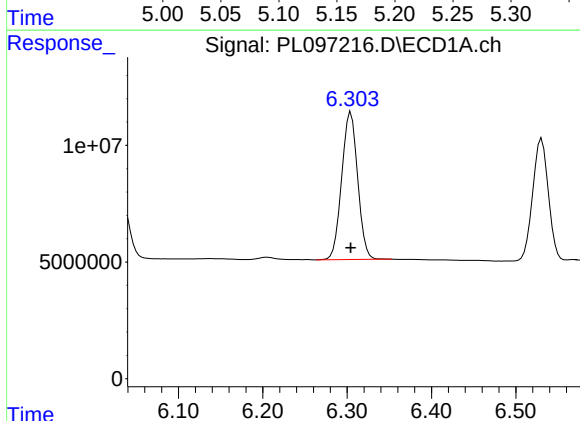


#13 Dieldrin

R.T.: 6.305 min
Delta R.T.: 0.000 min
Response: 83072356
Conc: 19.89 ng/ml

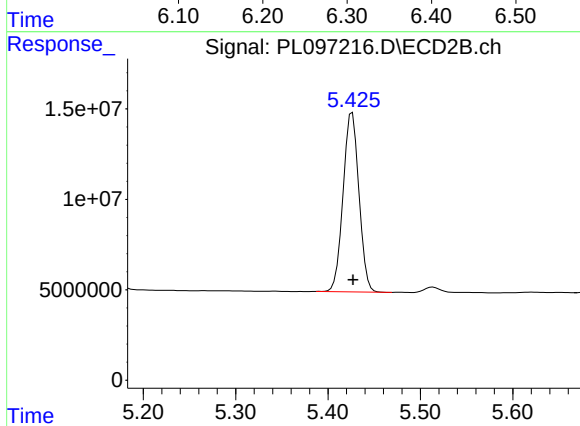

#13 Dieldrin


R.T.: 5.426 min
Delta R.T.: 0.000 min
Response: 118178340
Conc: 19.76 ng/ml

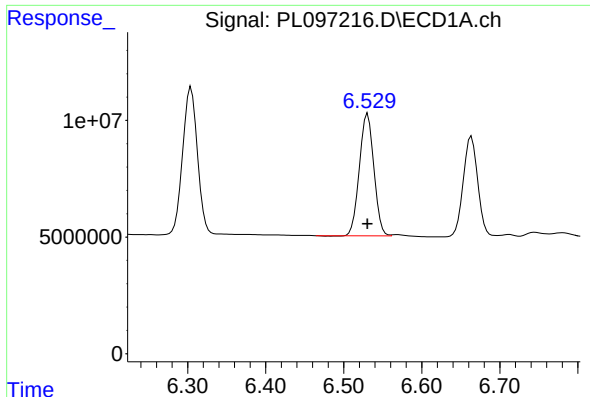

#14 Endrin


R.T.: 6.531 min
Delta R.T.: 0.000 min
Response: 67511228
Conc: 19.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA2314

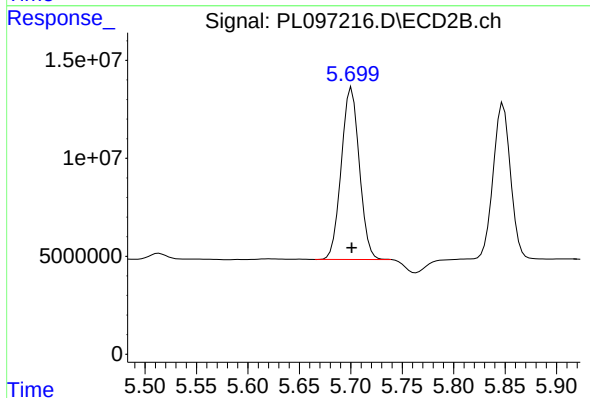


#14 Endrin

R.T.: 5.701 min
Delta R.T.: 0.000 min
Response: 107161410
Conc: 20.09 ng/ml

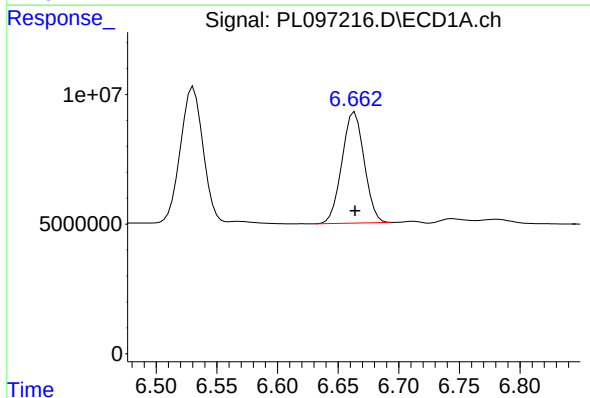


#16 4,4'-DDD

R.T.: 6.664 min
Delta R.T.: 0.000 min
Response: 54731638
Conc: 19.91 ng/ml

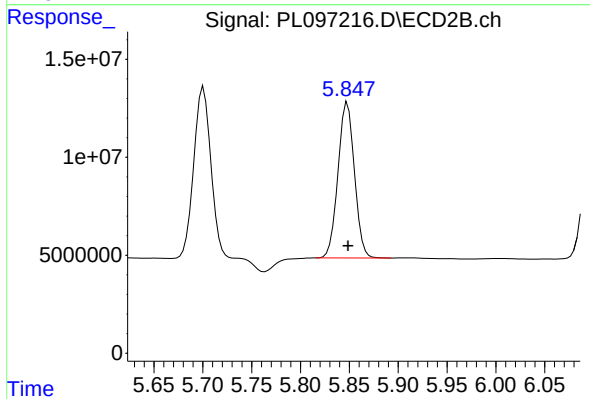

#16 4,4'-DDD


R.T.: 5.848 min
Delta R.T.: 0.000 min
Response: 93169309
Conc: 19.73 ng/ml

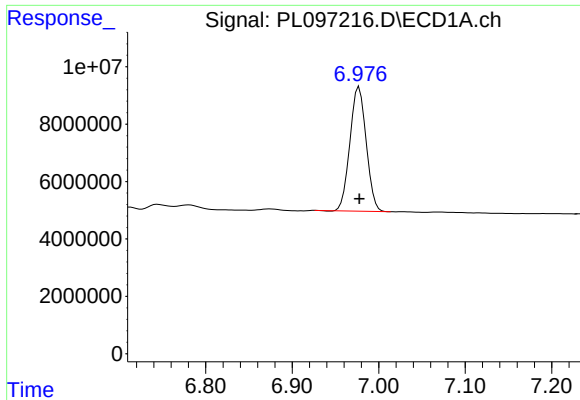

#17 4,4'-DDT


R.T.: 6.977 min
Delta R.T.: 0.000 min
Response: 56522626
Conc: 19.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA2314

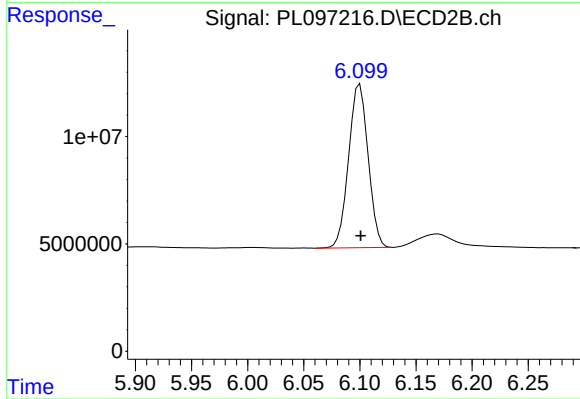


#17 4,4'-DDT

R.T.: 6.100 min
Delta R.T.: 0.000 min
Response: 92175063
Conc: 19.45 ng/ml

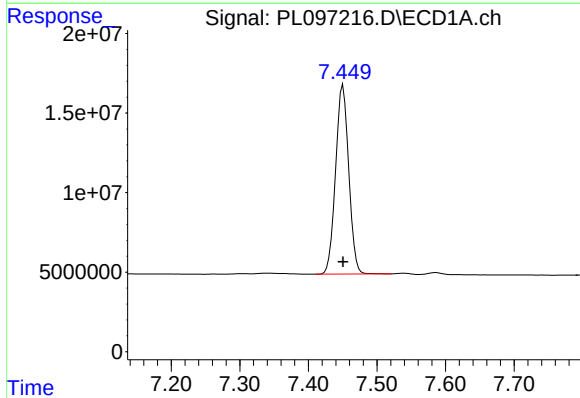


#20 Methoxychlor

R.T.: 7.450 min
Delta R.T.: 0.000 min
Response: 158405086
Conc: 103.32 ng/ml

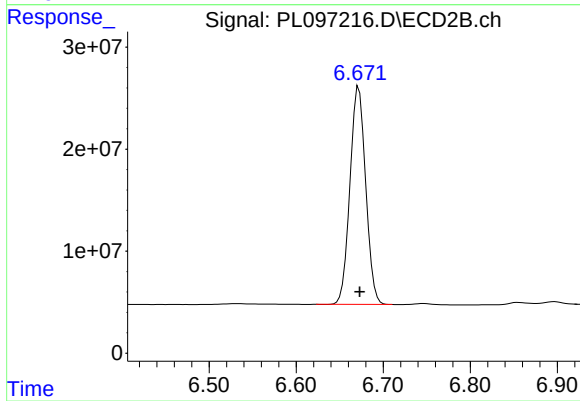

#20 Methoxychlor


R.T.: 6.672 min
Delta R.T.: 0.000 min
Response: 268412053
Conc: 104.75 ng/ml

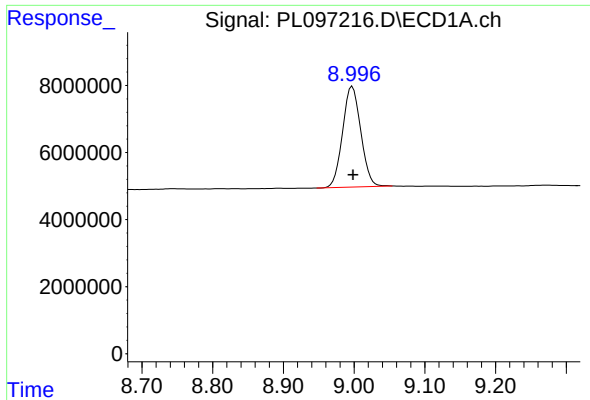

#27 Decachlorobiphenyl

R.T.: 8.997 min
Delta R.T.: 0.000 min
Response: 53774603
Conc: 21.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA2314

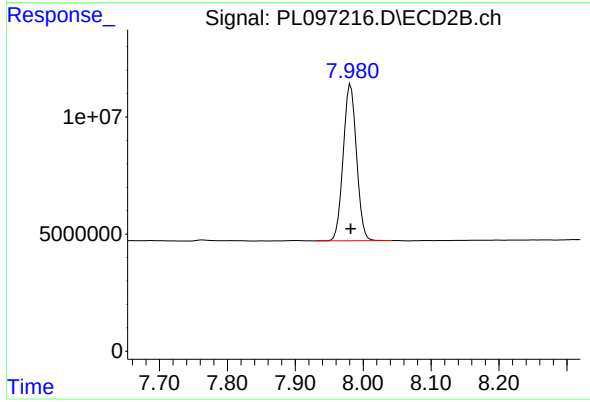

#27 Decachlorobiphenyl

R.T.: 7.982 min
Delta R.T.: 0.000 min
Response: 90981106
Conc: 20.93 ng/ml