

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091625\
 Data File : PL097222.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Sep 2025 12:32
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 INDA5320

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 17 04:44:17 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091625CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 17 04:40:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.527	2.823	280.4E6	397.1E6	82.645	82.329
27)	SA Decachlor...	8.998	7.982	405.7E6	680.1E6	158.393	156.485
Target Compounds							
2)	A alpha-BHC	3.974	3.328	478.7E6	641.3E6	90.275	89.491
3)	MA gamma-BHC...	4.301	3.660	446.1E6	589.3E6	88.478	87.934
4)	MA Heptachlor	4.892	4.008	441.1E6	572.8E6	85.482	84.867
9)	A Endosulfan I	6.032	5.162	336.0E6	445.2E6	85.194	83.503
13)	MA Dieldrin	6.305	5.427	735.5E6	1019.5E6	176.075	170.455
14)	MA Endrin	6.531	5.701	596.1E6	896.5E6	175.967	168.070
16)	A 4,4'-DDD	6.664	5.848	490.2E6	813.6E6	178.317	172.281
17)	MA 4,4'-DDT	6.978	6.100	514.3E6	845.0E6	180.337	178.320
20)	A Methoxychlor	7.450	6.673	1278.0E6	1862.5E6	833.548	726.858


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091625\
Data File : PL097222.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Sep 2025 12:32
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 04:44:17 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091625CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 17 04:40:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

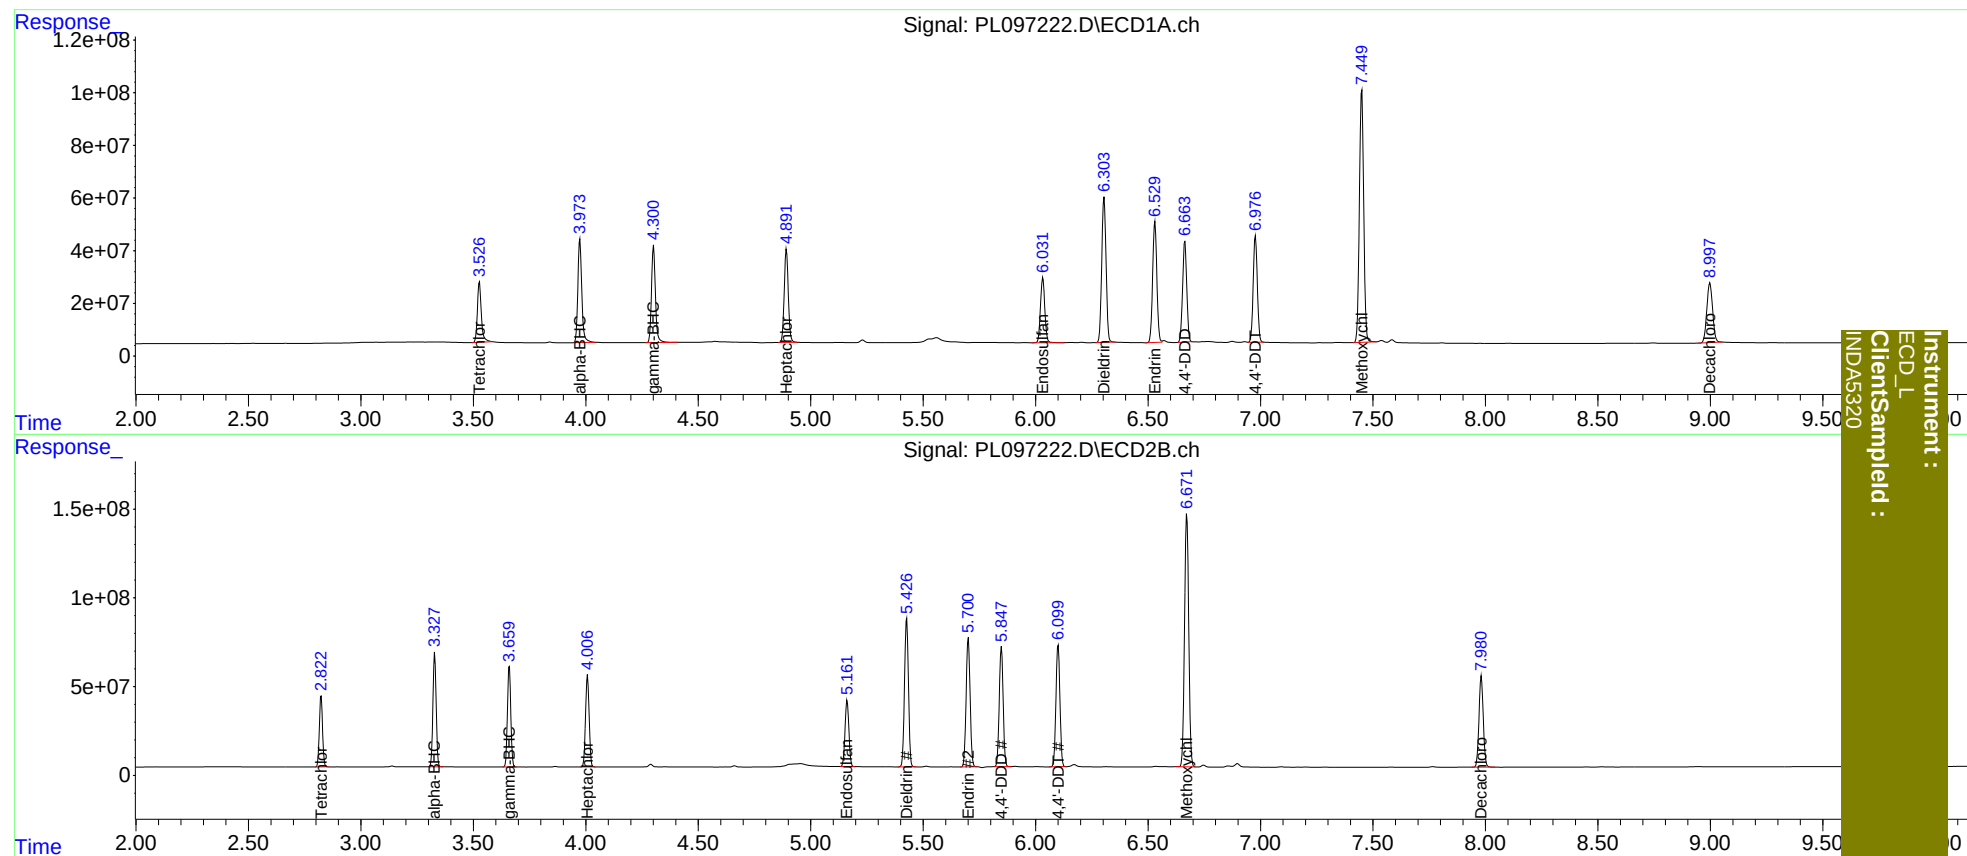


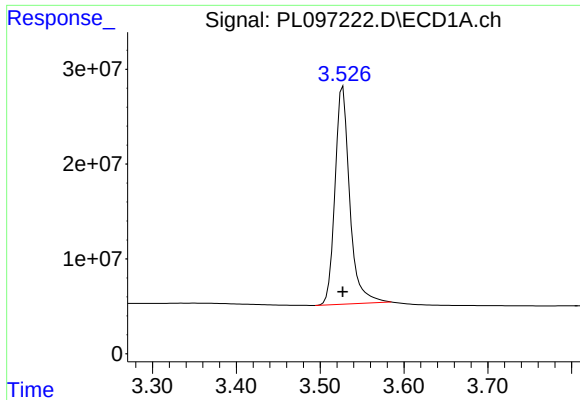

#1 Tetrachloro-m-xylene


R.T.: 3.527 min
Delta R.T.: 0.000 min
Response: 280368366
Conc: 82.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA5320

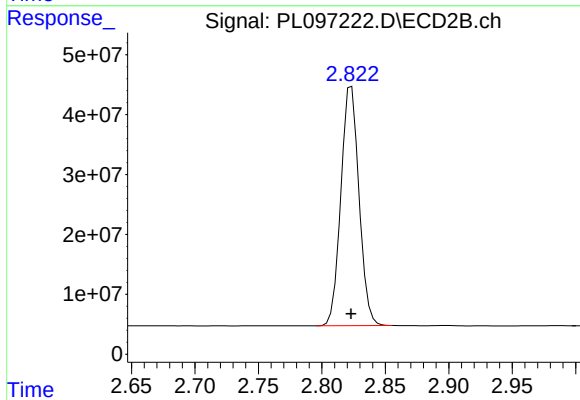


#1 Tetrachloro-m-xylene

R.T.: 2.823 min
Delta R.T.: 0.000 min
Response: 397149862
Conc: 82.33 ng/ml

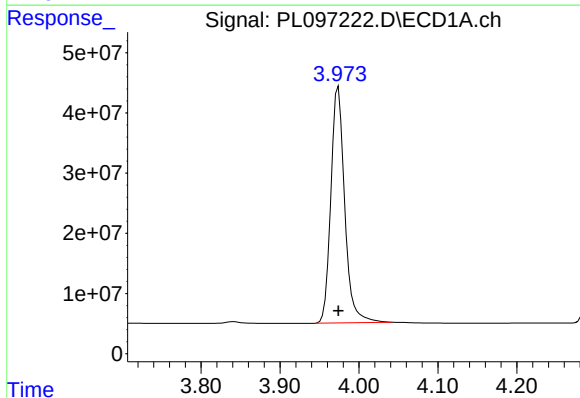


#2 alpha-BHC

R.T.: 3.974 min
Delta R.T.: 0.000 min
Response: 478696076
Conc: 90.27 ng/ml

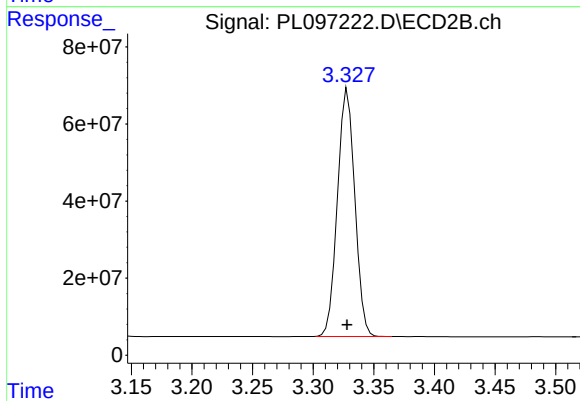

#2 alpha-BHC


R.T.: 3.328 min
Delta R.T.: 0.000 min
Response: 641263644
Conc: 89.49 ng/ml

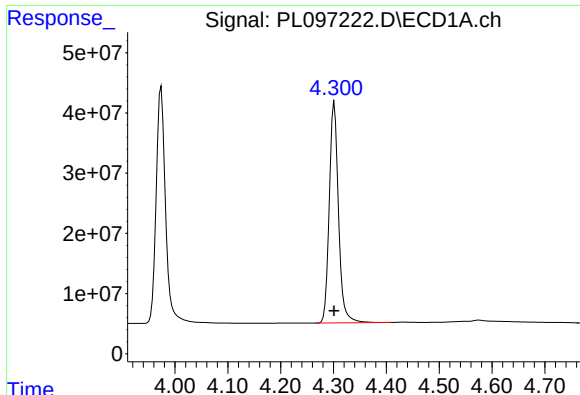

#3 gamma-BHC (Lindane)


R.T.: 4.301 min
Delta R.T.: 0.000 min
Response: 446069513
Conc: 88.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA5320

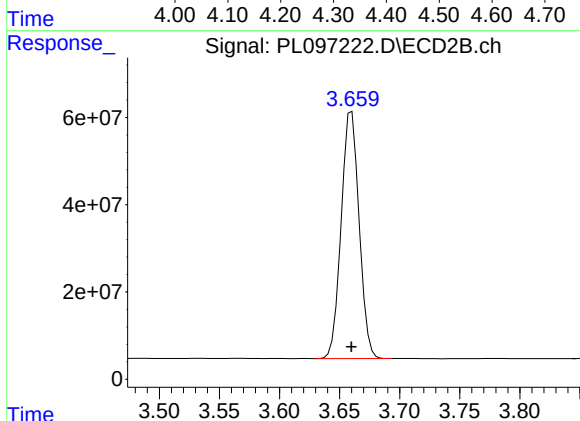


#3 gamma-BHC (Lindane)

R.T.: 3.660 min
Delta R.T.: 0.000 min
Response: 589317515
Conc: 87.93 ng/ml

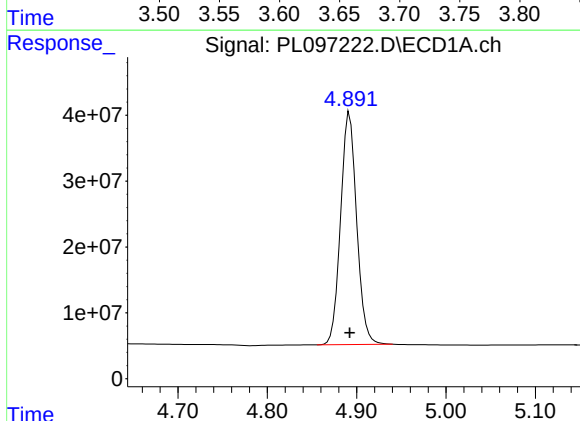


#4 Heptachlor

R.T.: 4.892 min
Delta R.T.: 0.000 min
Response: 441060845
Conc: 85.48 ng/ml

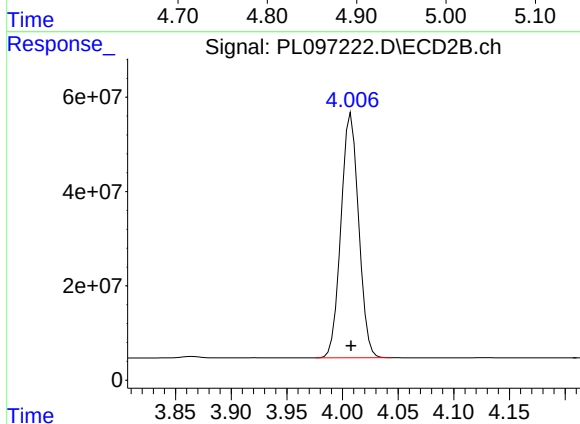

#4 Heptachlor


R.T.: 4.008 min
Delta R.T.: 0.000 min
Response: 572827935
Conc: 84.87 ng/ml

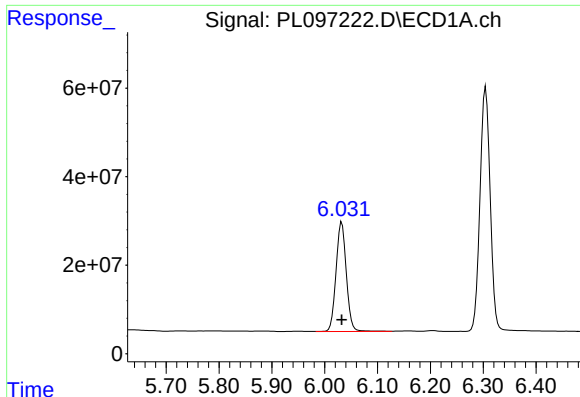

#9 Endosulfan I


R.T.: 6.032 min
Delta R.T.: 0.000 min
Response: 336049542
Conc: 85.19 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA5320

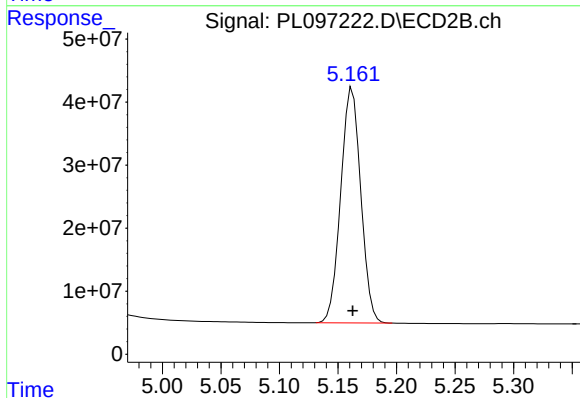


#9 Endosulfan I

R.T.: 5.162 min
Delta R.T.: 0.000 min
Response: 445234569
Conc: 83.50 ng/ml

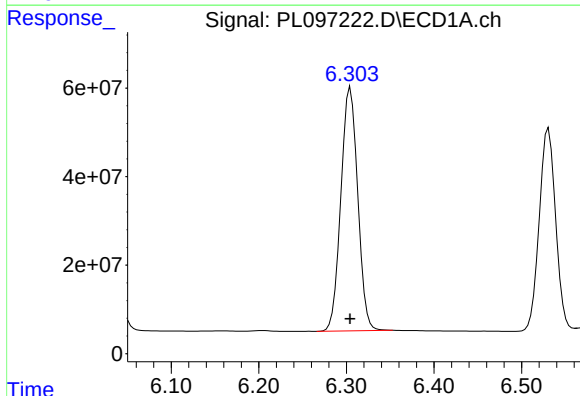


#13 Dieldrin

R.T.: 6.305 min
Delta R.T.: 0.000 min
Response: 735531392
Conc: 176.08 ng/ml

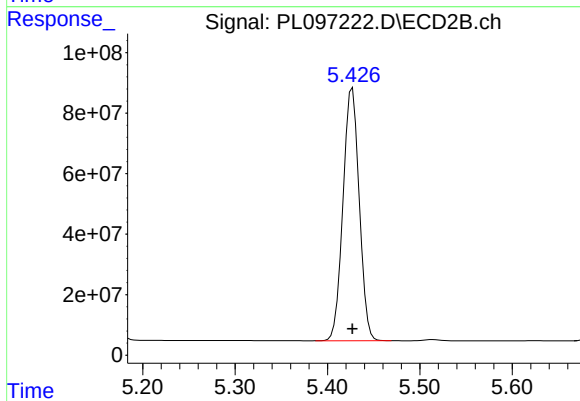

#13 Dieldrin


R.T.: 5.427 min
Delta R.T.: 0.000 min
Response: 1019466241
Conc: 170.46 ng/ml

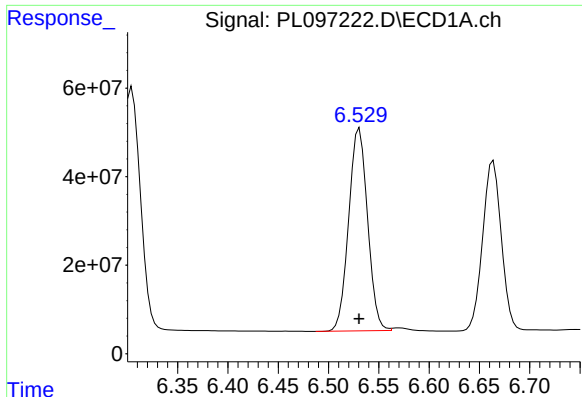

#14 Endrin


R.T.: 6.531 min
Delta R.T.: 0.000 min
Response: 596053579
Conc: 175.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA5320

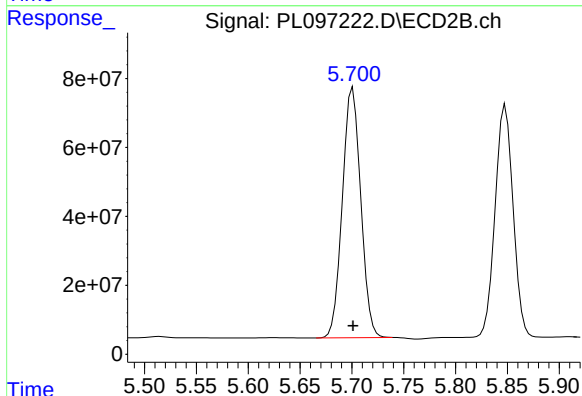


#14 Endrin

R.T.: 5.701 min
Delta R.T.: 0.000 min
Response: 896452473
Conc: 168.07 ng/ml

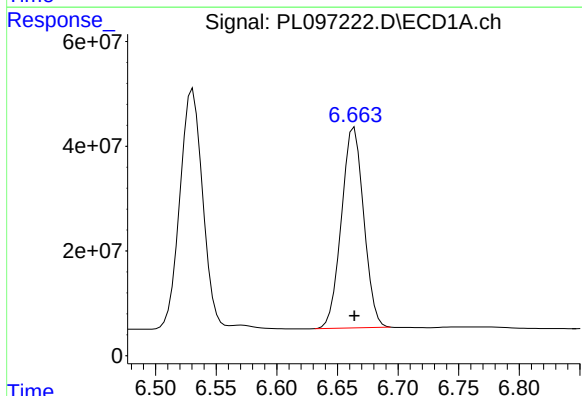


#16 4,4'-DDD

R.T.: 6.664 min
Delta R.T.: 0.000 min
Response: 490236318
Conc: 178.32 ng/ml

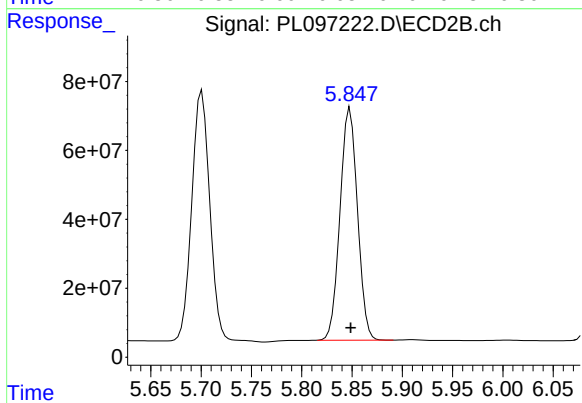

#16 4,4'-DDD


R.T.: 5.848 min
Delta R.T.: 0.000 min
Response: 813647680
Conc: 172.28 ng/ml

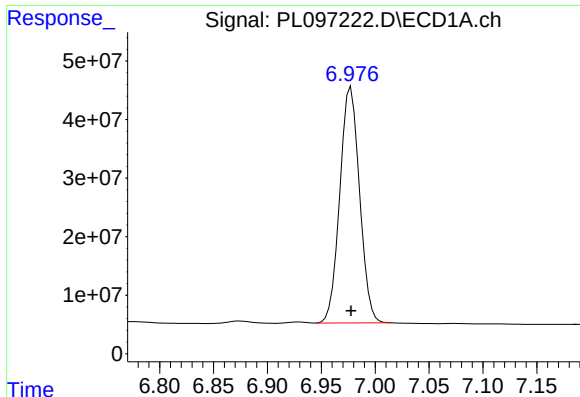

#17 4,4'-DDT


R.T.: 6.978 min
Delta R.T.: 0.000 min
Response: 514261248
Conc: 180.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA5320

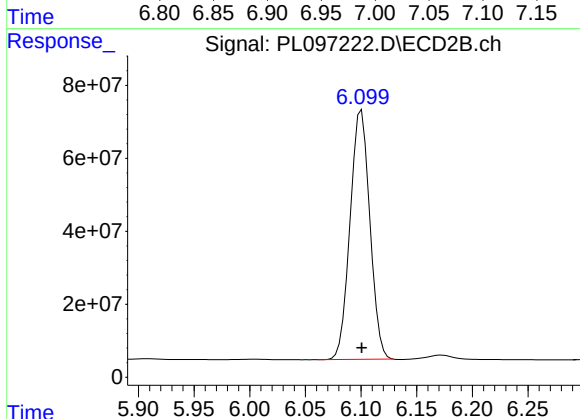


#17 4,4'-DDT

R.T.: 6.100 min
Delta R.T.: 0.000 min
Response: 845044631
Conc: 178.32 ng/ml

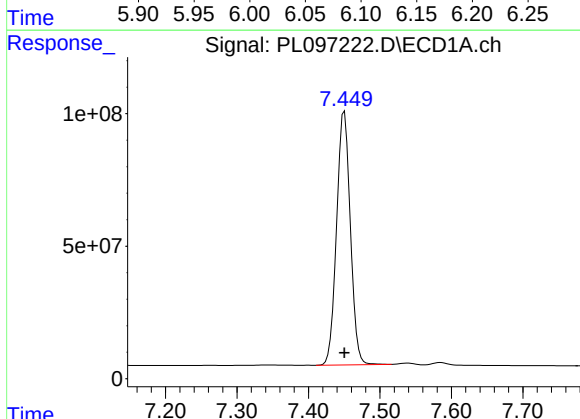


#20 Methoxychlor

R.T.: 7.450 min
Delta R.T.: 0.000 min
Response: 1277965604
Conc: 833.55 ng/ml

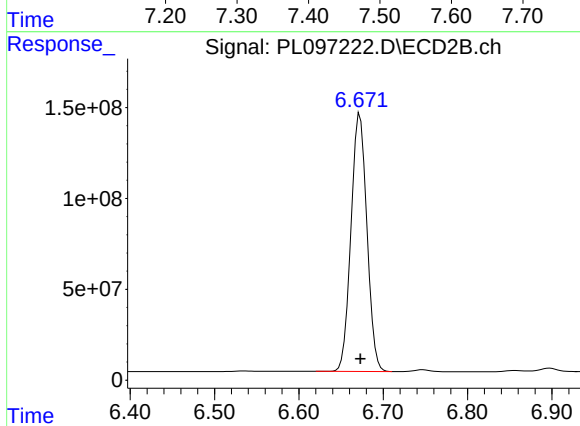

#20 Methoxychlor


R.T.: 6.673 min
Delta R.T.: 0.000 min
Response: 1862543218
Conc: 726.86 ng/ml

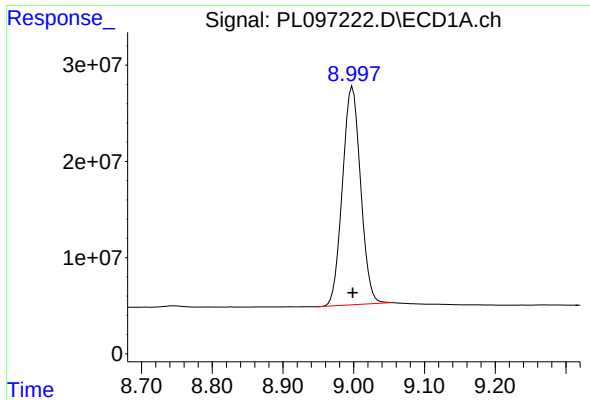

#27 Decachlorobiphenyl

R.T.: 8.998 min
Delta R.T.: 0.000 min
Response: 405677498
Conc: 158.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA5320

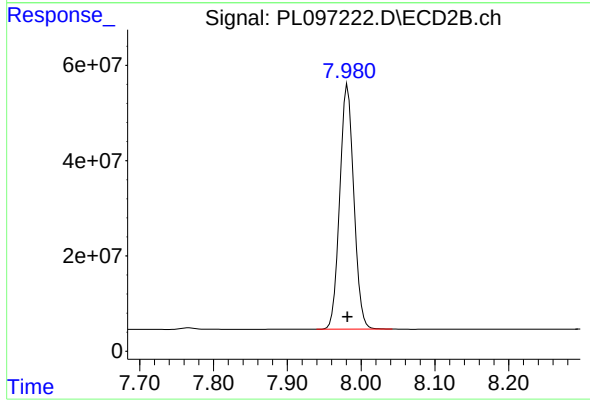

#27 Decachlorobiphenyl

R.T.: 7.982 min
Delta R.T.: 0.000 min
Response: 680101857
Conc: 156.48 ng/ml