

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091718\
 Data File : PL039981.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Sep 2018 10:41
 Operator : AJ\SJ
 Sample : J4773-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 18 01:09:36 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 14 23:10:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.301	3.903	110.3E6	40209284	14.222	12.602
28)	SA Decachlor...	7.953	8.888	98626094	41077536	11.836	15.124 #
Target Compounds							
9)	A Endosulfan I	0.000	6.052f	0	9083770	N.D.	2.558 #
10)	B gamma-Chl...	0.000	5.972	0	9570086	N.D.	2.529 #
11)	B alpha-Chl...	0.000	6.052	0	9083770	N.D.	2.293 #
23)	Chlordane-1	0.000	4.883	0	3456034	N.D.	22.319 #
25)	Chlordane-3	0.000	5.972	0	9570086	N.D.	18.694 #
26)	Chlordane-4	0.000	6.052	0	9083770	N.D.	14.676 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091718\
Data File : PL039981.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Sep 2018 10:41
Operator : AJ\SJ
Sample : J4773-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 18 01:09:36 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
Quant Title : GC Extractables
QLast Update : Fri Sep 14 23:10:39 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

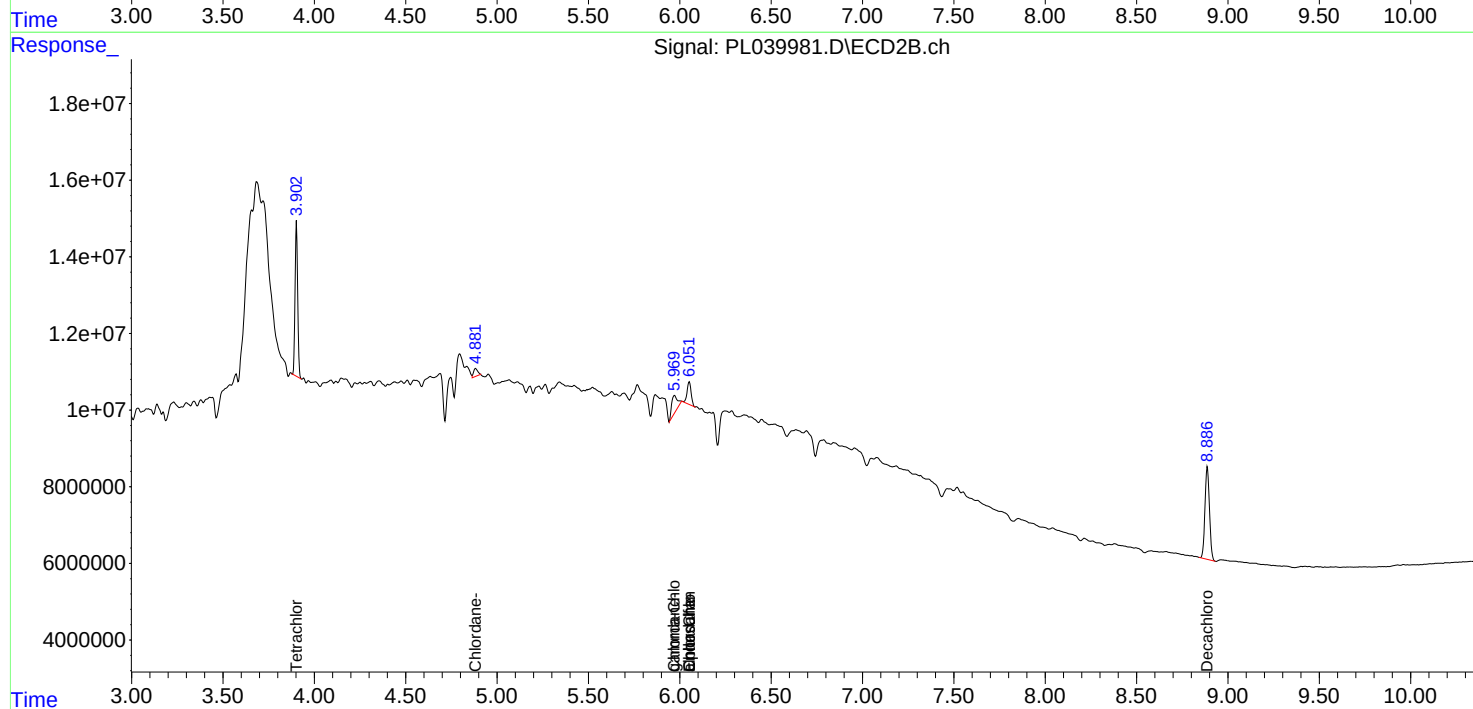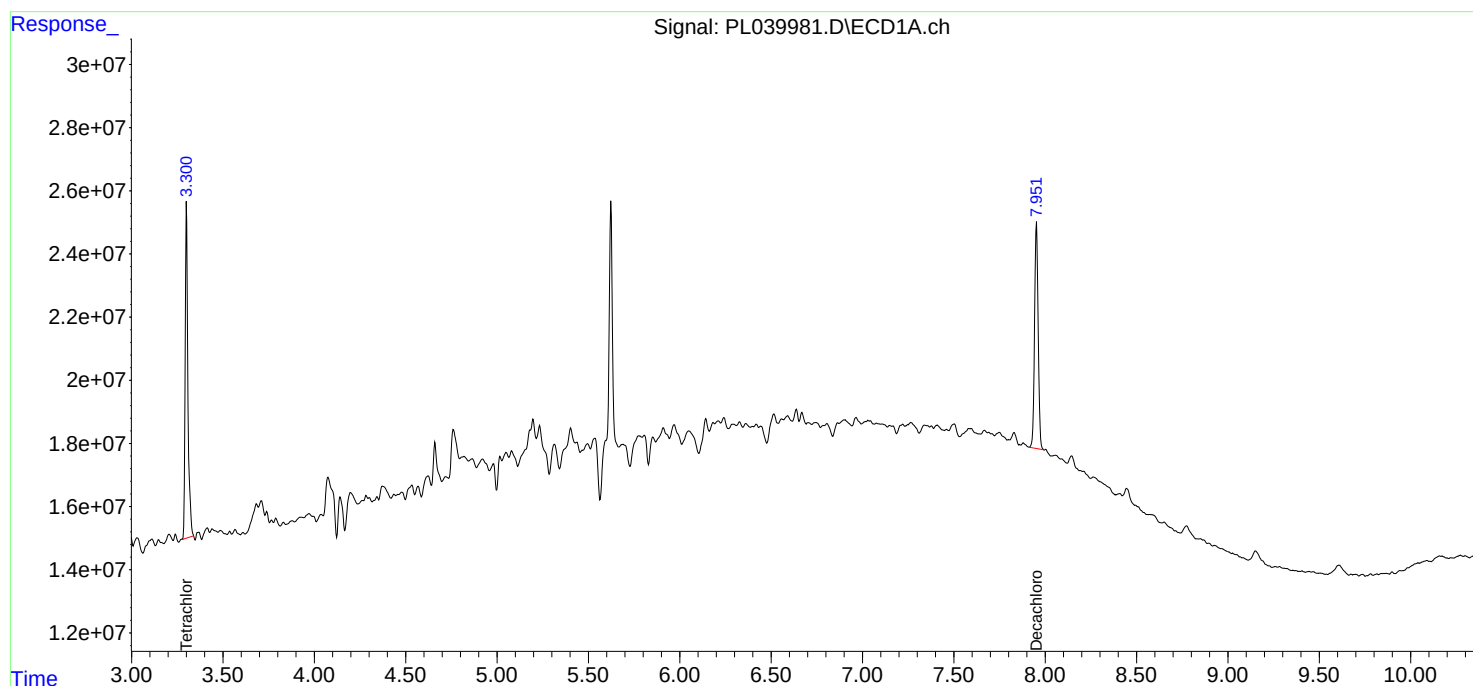


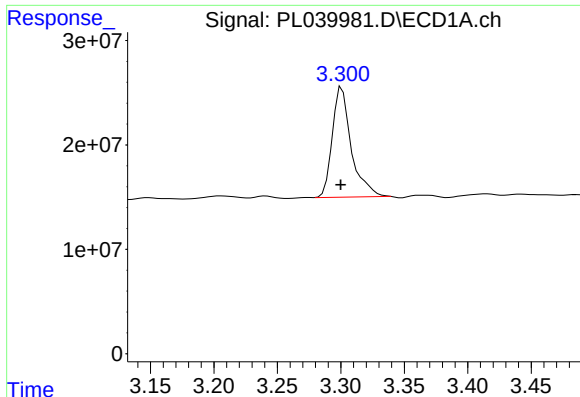

#1 Tetrachloro-m-xylene


R.T.: 3.301 min
Delta R.T.: 0.000 min
Response: 110291542
Conc: 14.22 ng/ml

Instrument :
ECD_L
ClientSampleId :

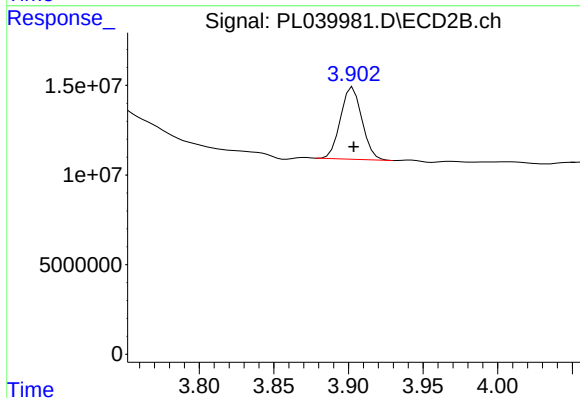


#1 Tetrachloro-m-xylene

R.T.: 3.903 min
Delta R.T.: 0.000 min
Response: 40209284
Conc: 12.60 ng/ml

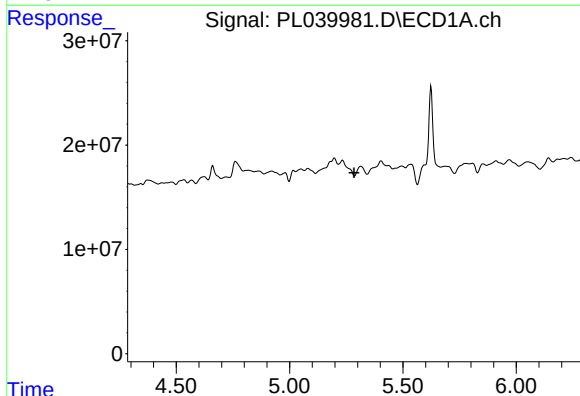


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.285 min
Response: 0
Conc: N.D.

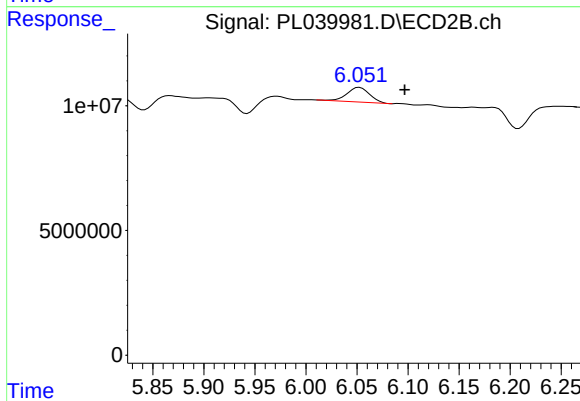

#9 Endosulfan I


R.T.: 6.052 min
Delta R.T.: -0.044 min
Response: 9083770
Conc: 2.56 ng/ml

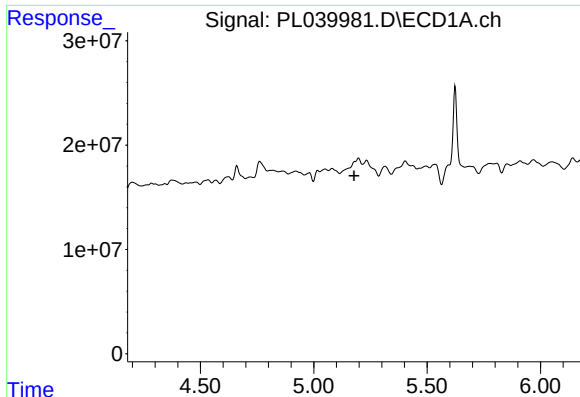

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.178 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

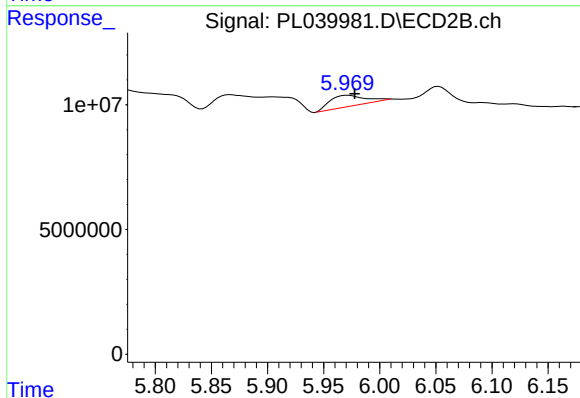


#10 gamma-Chlordane

R.T.: 5.972 min
Delta R.T.: -0.006 min
Response: 9570086
Conc: 2.53 ng/ml

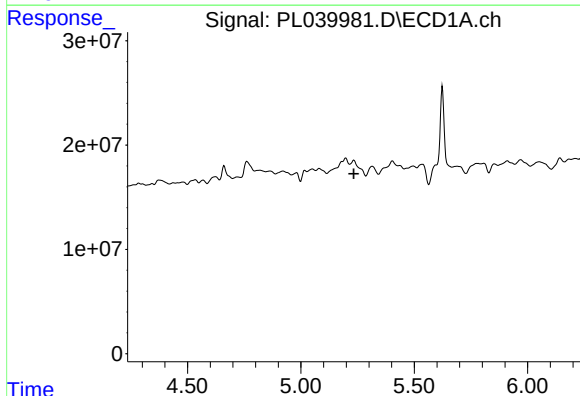


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.233 min
Response: 0
Conc: N.D.

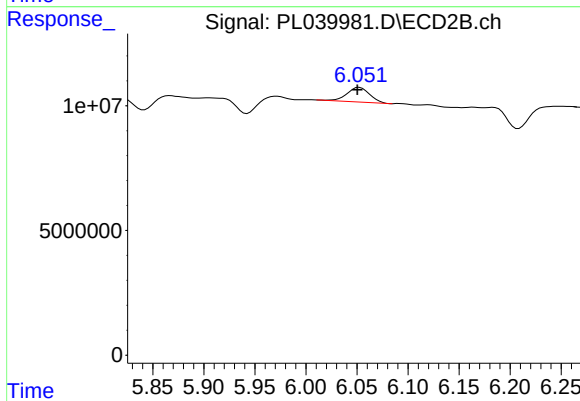

#11 alpha-Chlordane


R.T.: 6.052 min
Delta R.T.: 0.002 min
Response: 9083770
Conc: 2.29 ng/ml

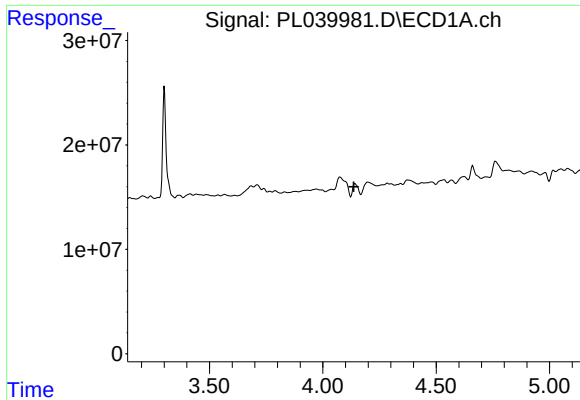

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.136 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

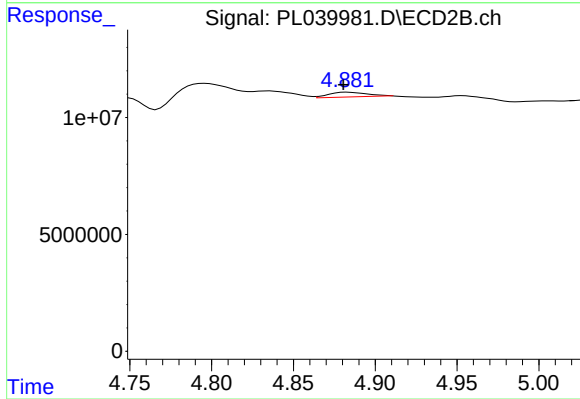


#23 Chlordane-1

R.T.: 4.883 min
Delta R.T.: 0.002 min
Response: 3456034
Conc: 22.32 ng/ml

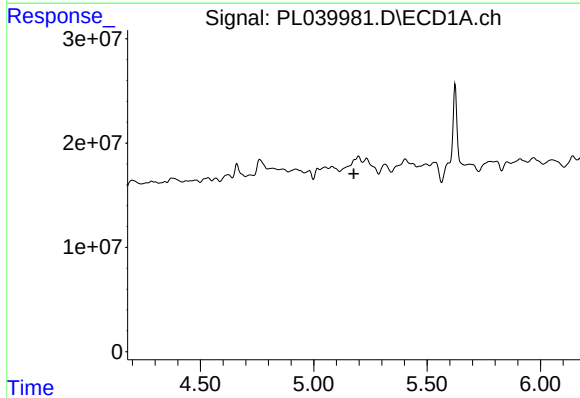


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.176 min
Response: 0
Conc: N.D.

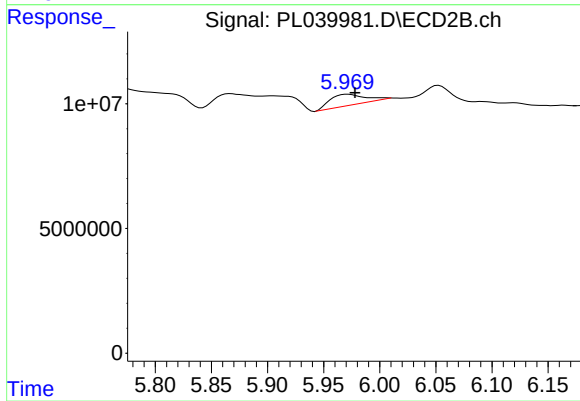

#25 Chlordane-3


R.T.: 5.972 min
Delta R.T.: -0.006 min
Response: 9570086
Conc: 18.69 ng/ml

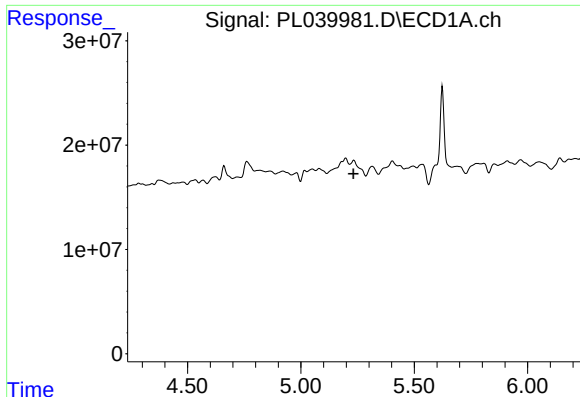

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.232 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

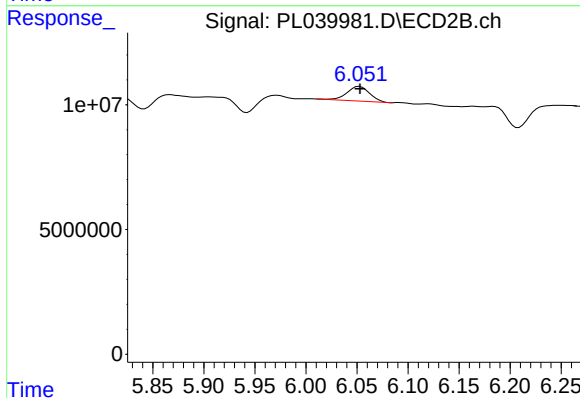


#26 Chlordane-4

R.T.: 6.052 min
Delta R.T.: 0.000 min
Response: 9083770
Conc: 14.68 ng/ml

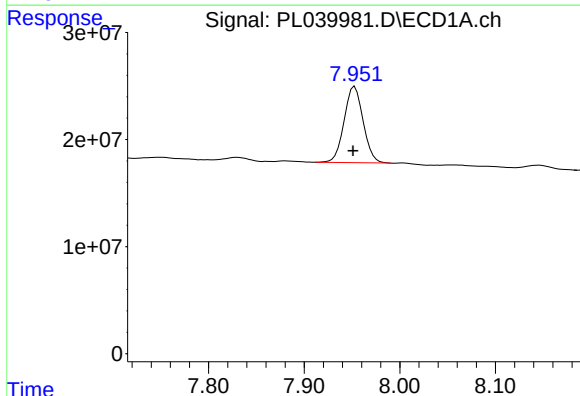

#28 Decachlorobiphenyl

R.T.: 7.953 min
Delta R.T.: 0.002 min
Response: 98626094
Conc: 11.84 ng/ml

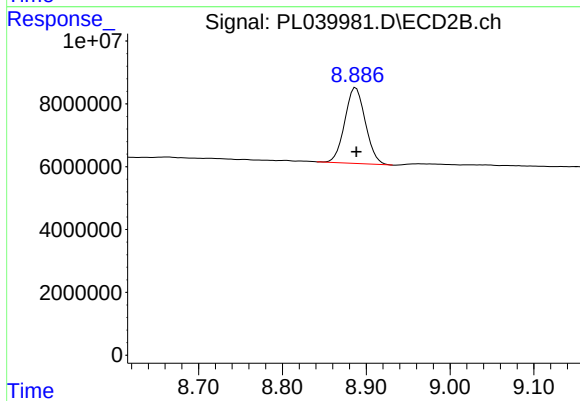

#28 Decachlorobiphenyl

R.T.: 8.888 min
Delta R.T.: 0.000 min
Response: 41077536
Conc: 15.12 ng/ml