

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091718\
 Data File : PL039982.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Sep 2018 10:55
 Operator : AJ\SJ
 Sample : J4773-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 18 01:09:46 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 14 23:10:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.300	3.903	130.3E6	37497631	16.807	11.752 #
28)	SA Decachlor...	7.952	8.888	72597348	30064356	8.712	11.069 #
Target Compounds							
4)	MA Heptachlor	4.283	0.000	26512347	0	2.298	N.D. #
7)	B delta-BHC	0.000	4.885f	0	4504678	N.D.	1.132 #
8)	B Heptachlo...	0.000	5.770	0	1747424	N.D.	0.442 #
9)	A Endosulfan I	0.000	6.053f	0	9978391	N.D.	2.810 #
11)	B alpha-Chl...	0.000	6.053	0	9978391	N.D.	2.519 #
23)	Chlordane-1	4.142	4.885	26888083	4504678	74.186	29.091 #
24)	Chlordane-2	4.660	0.000	36623440	0	97.243	N.D. #
26)	Chlordane-4	0.000	6.053	0	9978391	N.D.	16.121 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091718\
Data File : PL039982.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Sep 2018 10:55
Operator : AJ\SJ
Sample : J4773-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 18 01:09:46 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
Quant Title : GC Extractables
QLast Update : Fri Sep 14 23:10:39 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

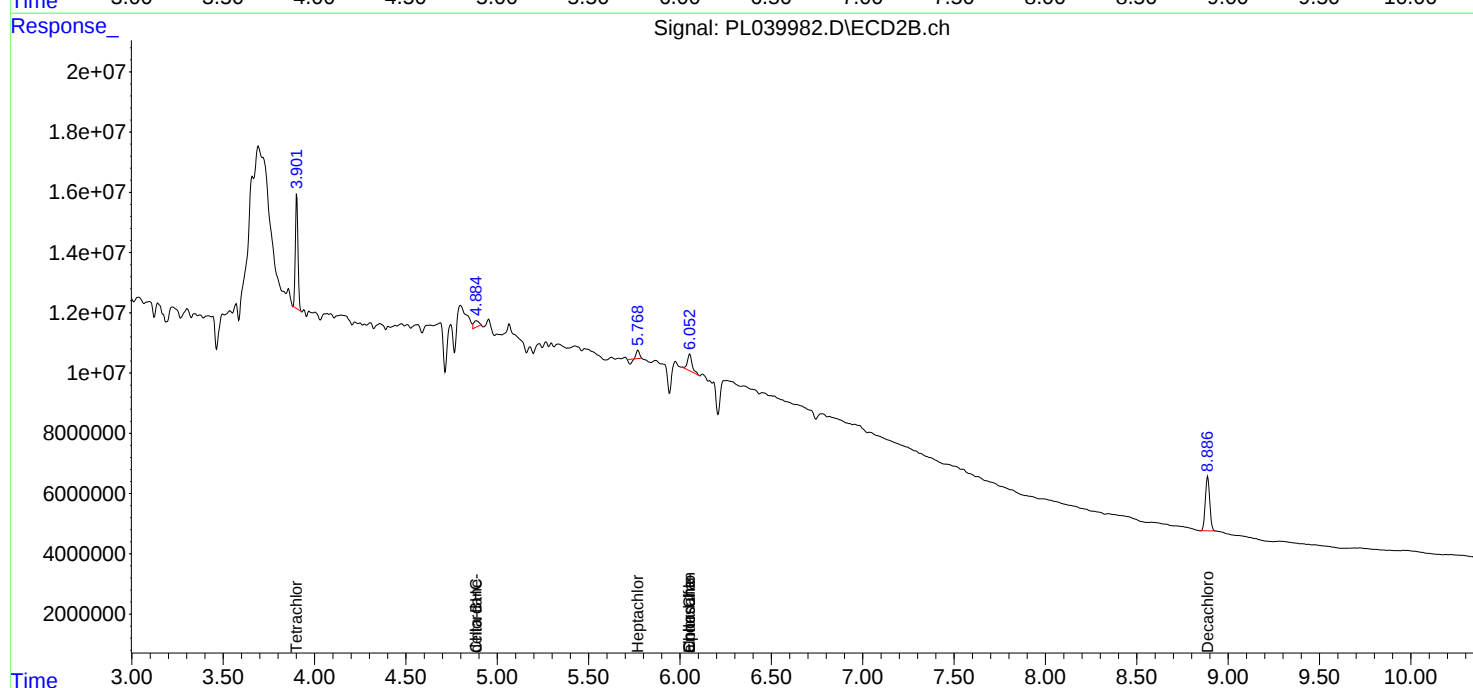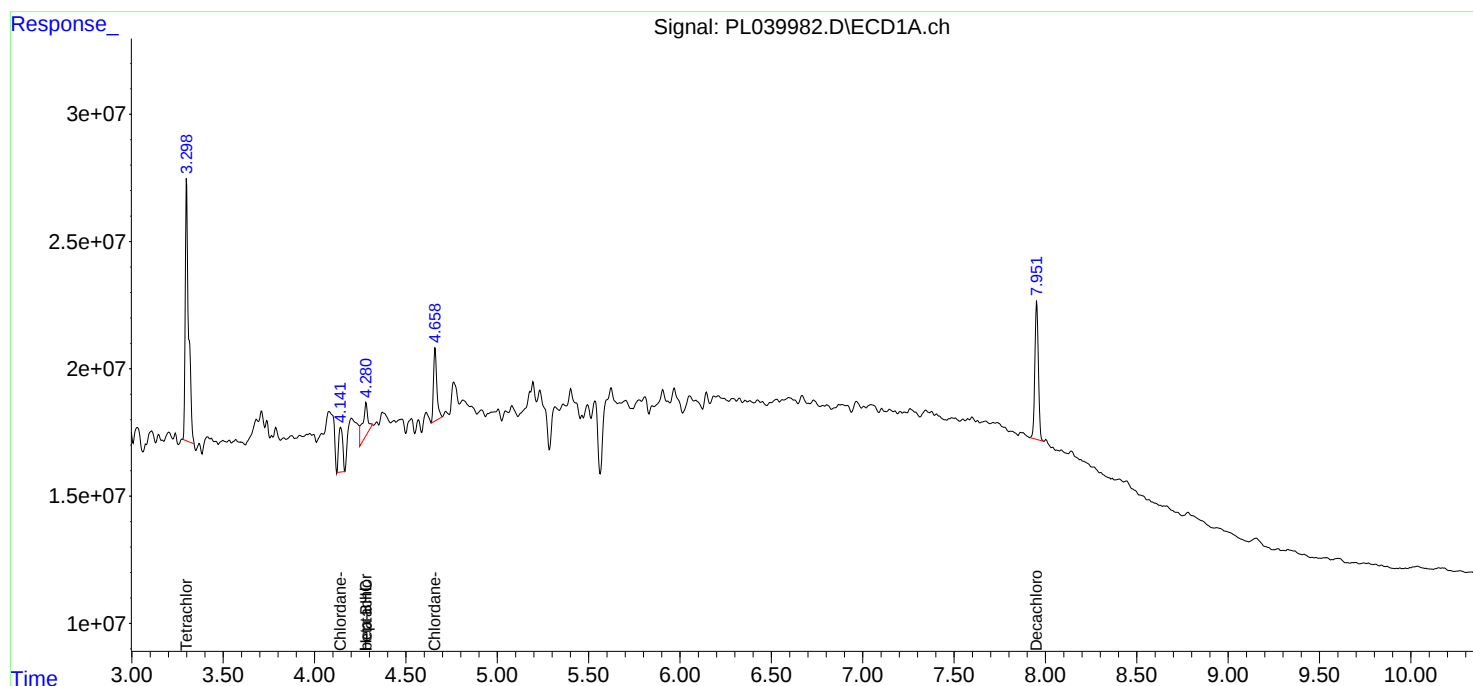


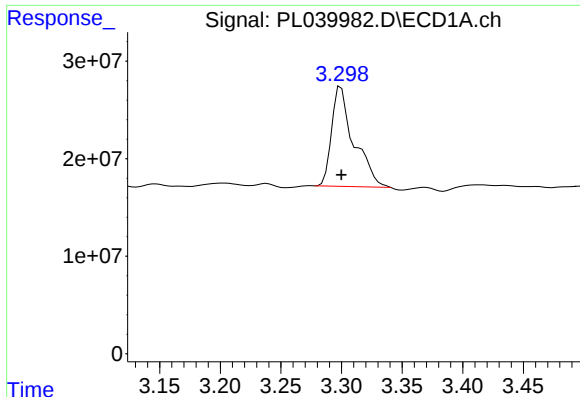

#1 Tetrachloro-m-xylene


R.T.: 3.300 min
Delta R.T.: 0.000 min
Response: 130337414
Conc: 16.81 ng/ml

Instrument :
ECD_L
ClientSampleId :

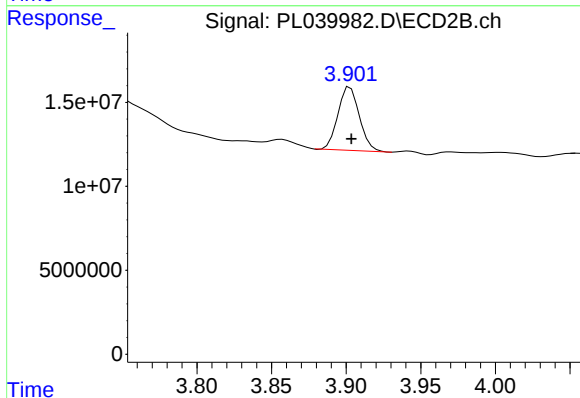


#1 Tetrachloro-m-xylene

R.T.: 3.903 min
Delta R.T.: 0.000 min
Response: 37497631
Conc: 11.75 ng/ml

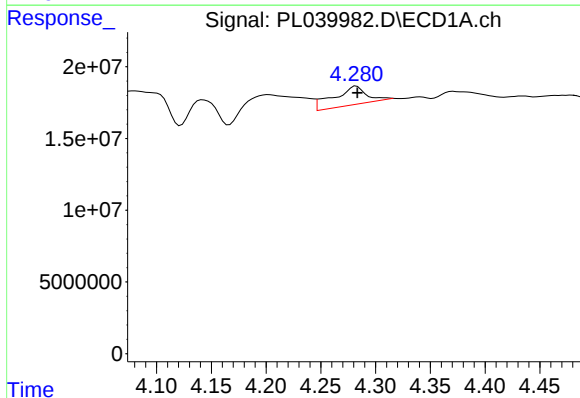


#4 Heptachlor

R.T.: 4.283 min
Delta R.T.: 0.000 min
Response: 26512347
Conc: 2.30 ng/ml

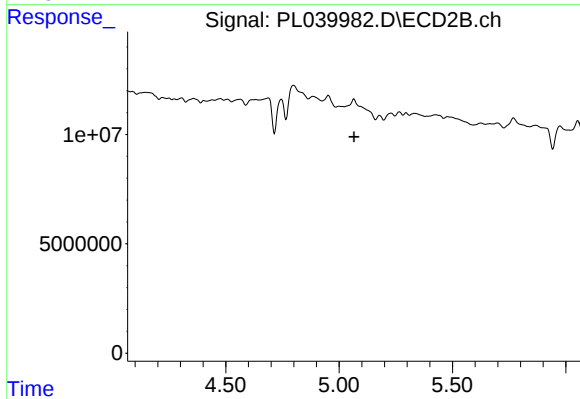

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 5.066 min
Response: 0
Conc: N.D.

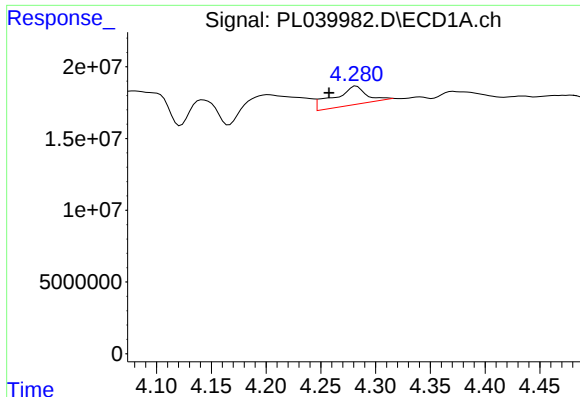

#6 beta-BHC


R.T.: 4.283 min
Delta R.T.: 0.025 min
Response: 26512347
Conc: 5.39 ng/ml

Instrument :
ECD_L
ClientSampleId :

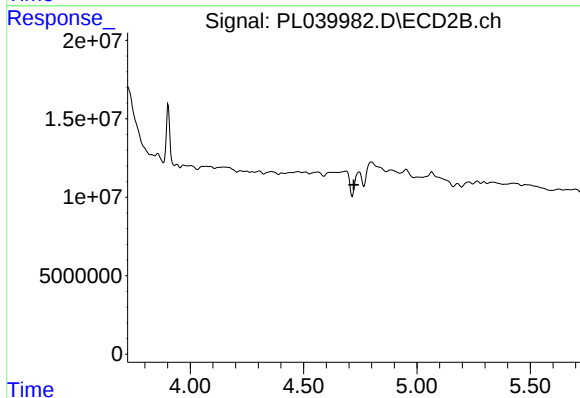


#6 beta-BHC

R.T.: 4.746 min
Delta R.T.: 0.024 min
Response: -11151610
Conc: N.D.

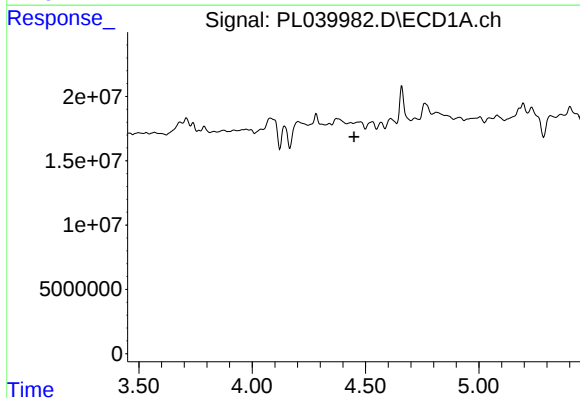


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.449 min
Response: 0
Conc: N.D.

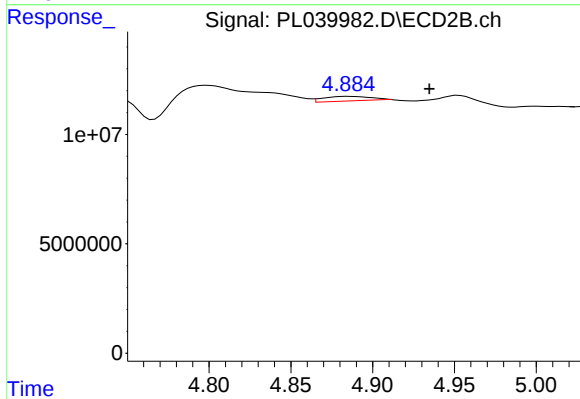

#7 delta-BHC


R.T.: 4.885 min
Delta R.T.: -0.050 min
Response: 4504678
Conc: 1.13 ng/ml

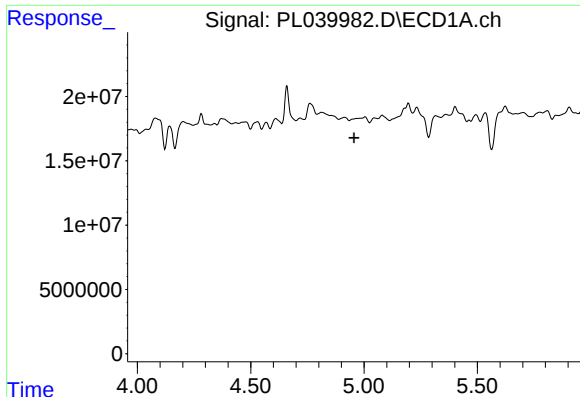

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.956 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

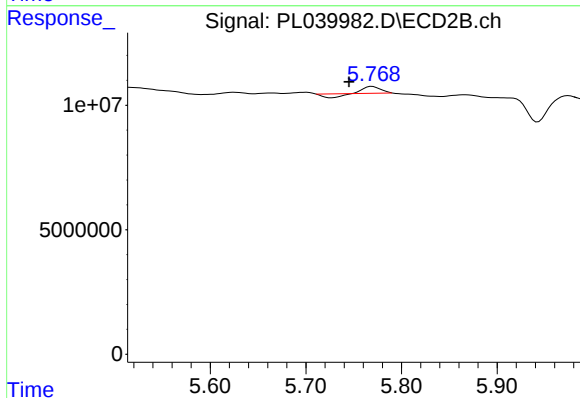


#8 Heptachlor epoxide

R.T.: 5.770 min
Delta R.T.: 0.024 min
Response: 1747424
Conc: 0.44 ng/ml

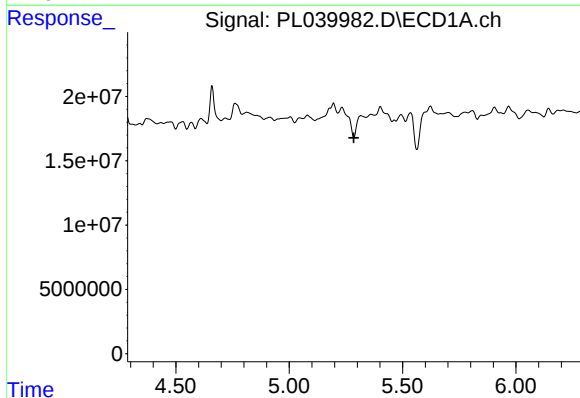


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.285 min
Response: 0
Conc: N.D.

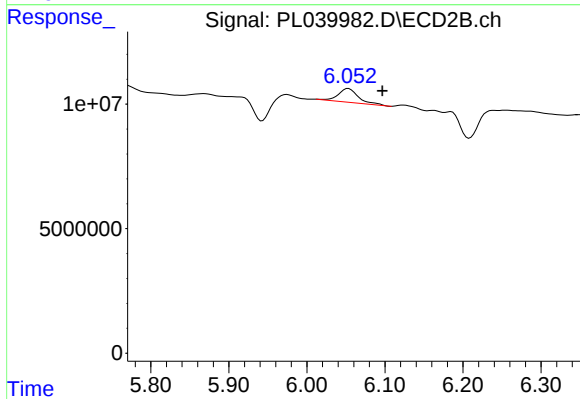

#9 Endosulfan I


R.T.: 6.053 min
Delta R.T.: -0.044 min
Response: 9978391
Conc: 2.81 ng/ml

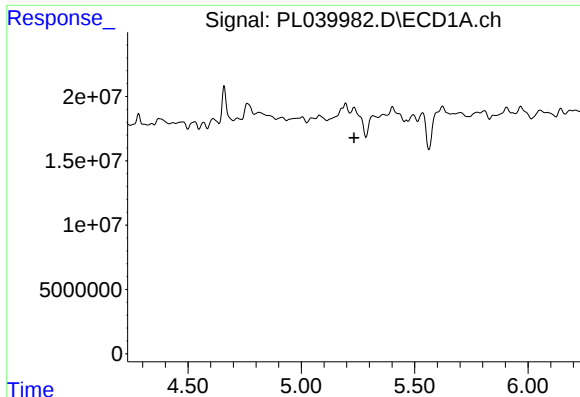

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.233 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

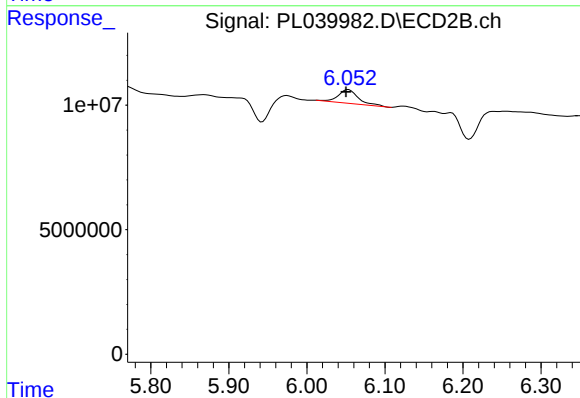


#11 alpha-Chlordane

R.T.: 6.053 min
Delta R.T.: 0.003 min
Response: 9978391
Conc: 2.52 ng/ml

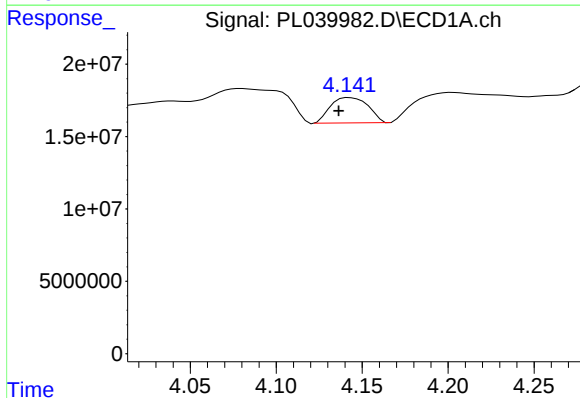


#23 Chlordane-1

R.T.: 4.142 min
Delta R.T.: 0.006 min
Response: 26888083
Conc: 74.19 ng/ml

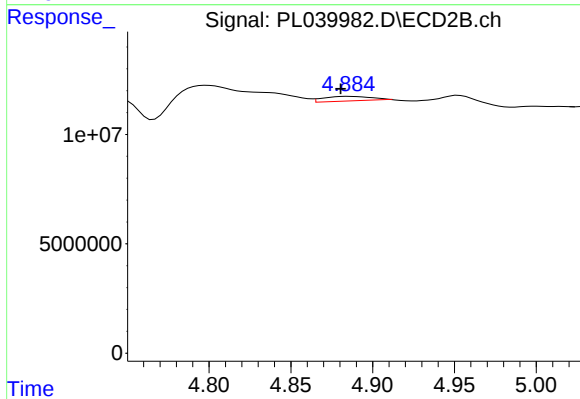

#23 Chlordane-1


R.T.: 4.885 min
Delta R.T.: 0.004 min
Response: 4504678
Conc: 29.09 ng/ml

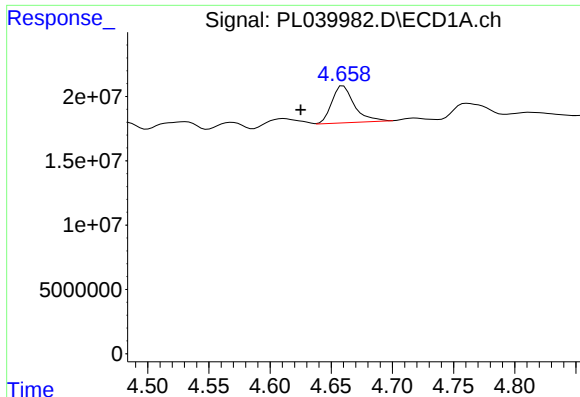

#24 Chlordane-2


R.T.: 4.660 min
Delta R.T.: 0.035 min
Response: 36623440
Conc: 97.24 ng/ml

Instrument :
ECD_L
ClientSampleId :

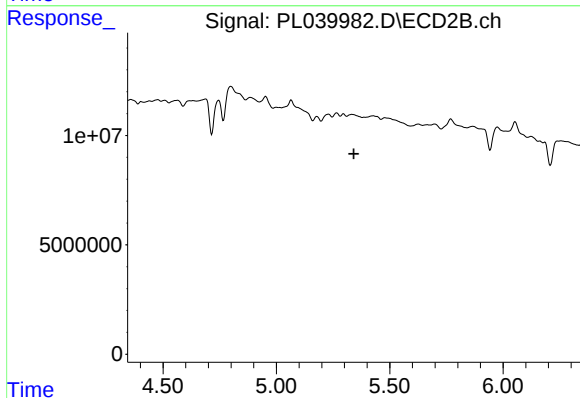


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.341 min
Response: 0
Conc: N.D.

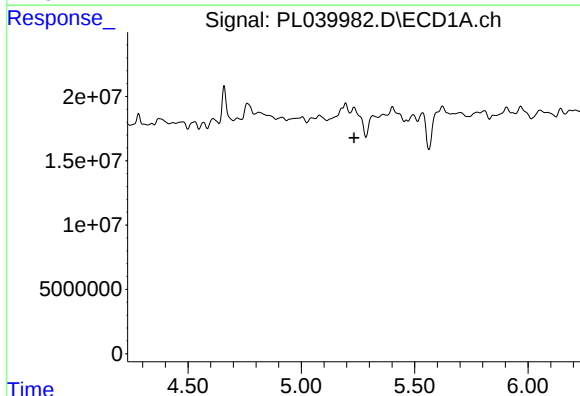


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.232 min
Response: 0
Conc: N.D.

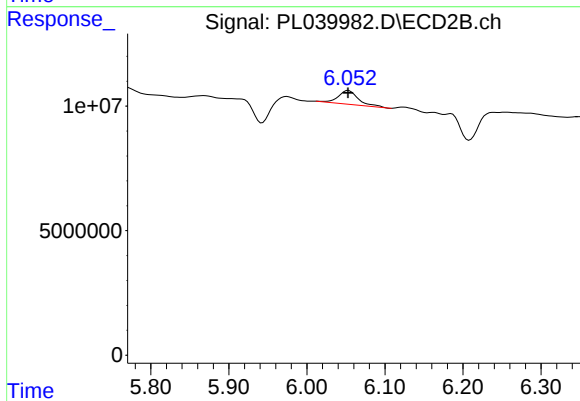

#26 Chlordane-4


R.T.: 6.053 min
Delta R.T.: 0.000 min
Response: 9978391
Conc: 16.12 ng/ml

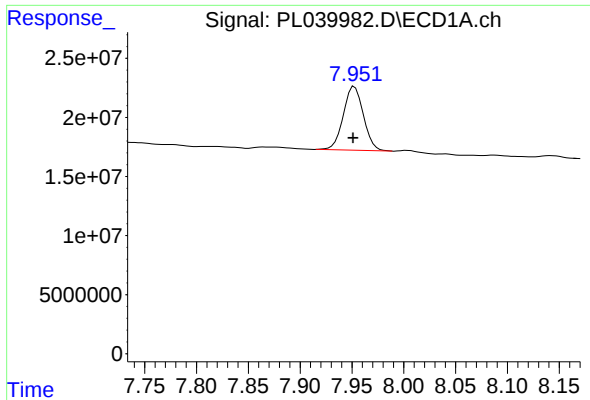

#28 Decachlorobiphenyl

R.T.: 7.952 min
Delta R.T.: 0.001 min
Response: 72597348
Conc: 8.71 ng/ml

Instrument :
ECD_L
ClientSampleId :

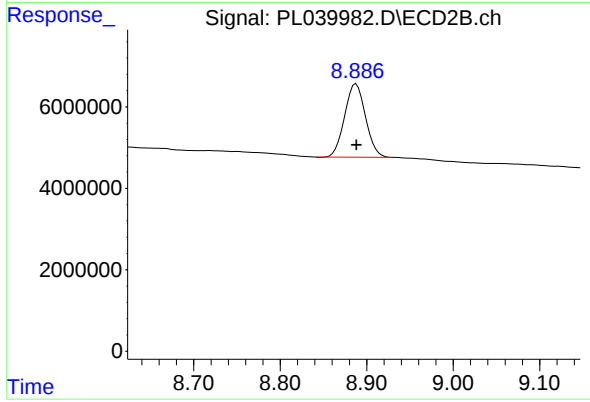

#28 Decachlorobiphenyl

R.T.: 8.888 min
Delta R.T.: 0.000 min
Response: 30064356
Conc: 11.07 ng/ml