

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091718\
 Data File : PL039983.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Sep 2018 11:09
 Operator : AJ\SJ
 Sample : J4773-05
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 18 01:09:57 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 14 23:10:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.300	3.903	108.7E6	35849155	14.016	11.235
28)	SA Decachlor...	7.951	8.887	84211815	36576883	10.106	13.467 #
Target Compounds							
8)	B Heptachlo...	0.000	5.770	0	2541411	N.D.	0.643 #
9)	A Endosulfan I	0.000	6.053f	0	14004993	N.D.	3.944 #
10)	B gamma-Chl...	5.196	5.976	14493356	1531896	1.301	0.405 #
11)	B alpha-Chl...	5.196f	6.053	14493356	14004993	1.357	3.535 #
23)	Chlordane-1	4.203	4.884	29020803	2817335	80.070	18.194 #
24)	Chlordane-2	4.660	0.000	33969291	0	90.196	N.D. #
25)	Chlordane-3	5.196	5.976	14493356	1531896	11.811	2.992 #
26)	Chlordane-4	5.196	6.053	14493356	14004993	13.221	22.627 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091718\
Data File : PL039983.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Sep 2018 11:09
Operator : AJ\SJ
Sample : J4773-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 18 01:09:57 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
Quant Title : GC Extractables
QLast Update : Fri Sep 14 23:10:39 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

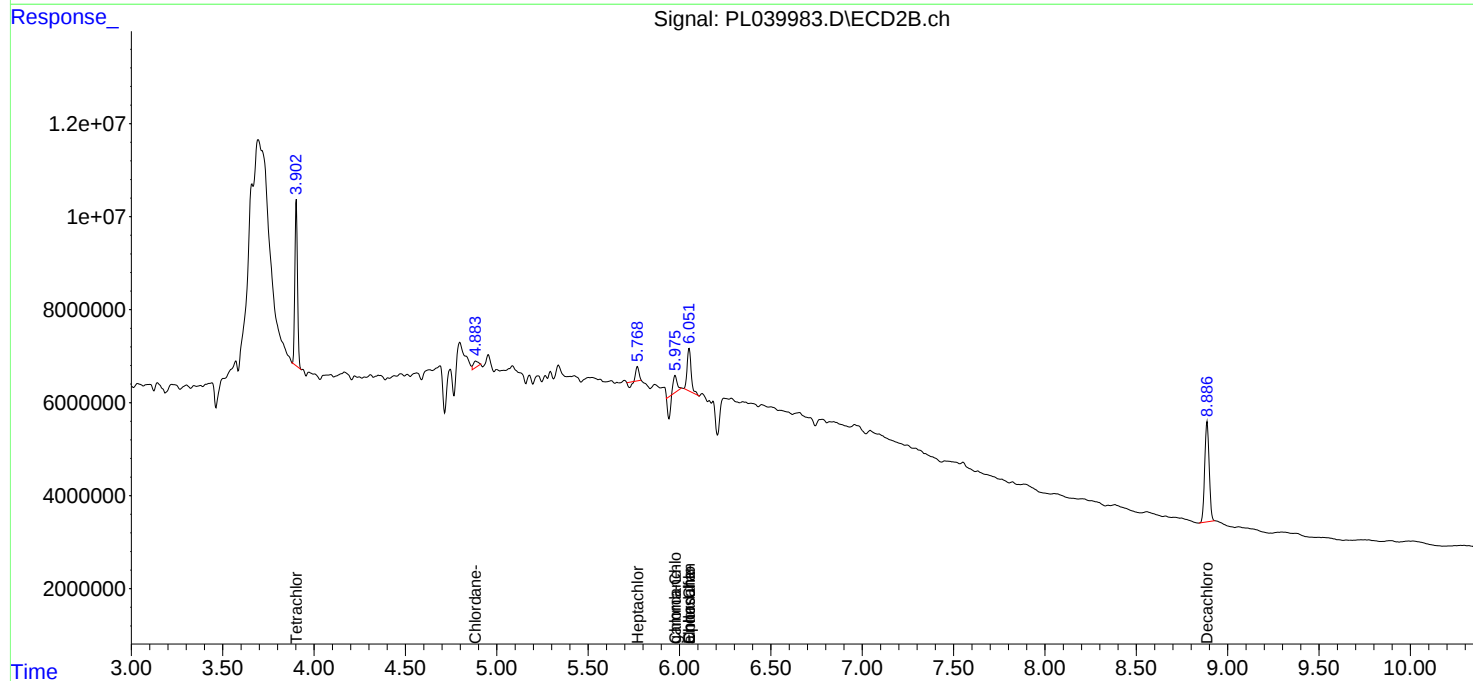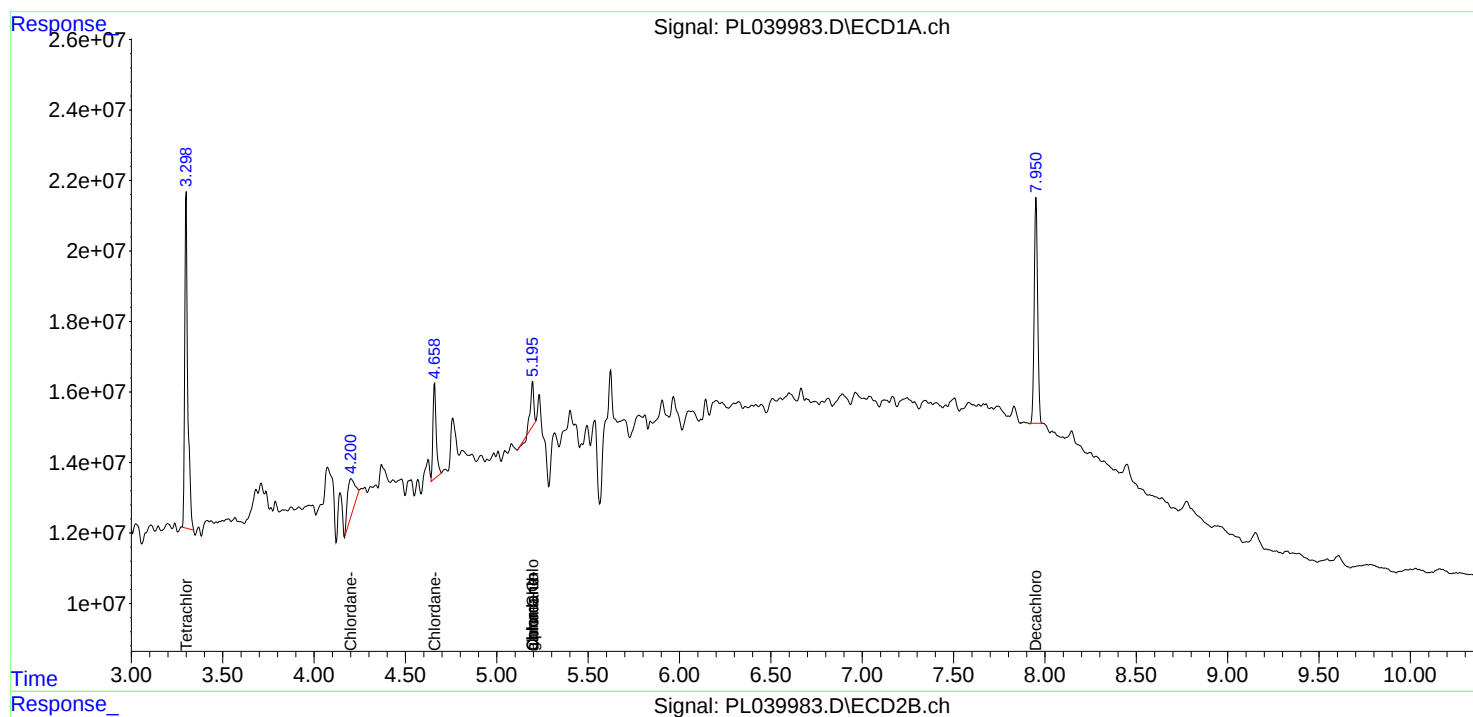


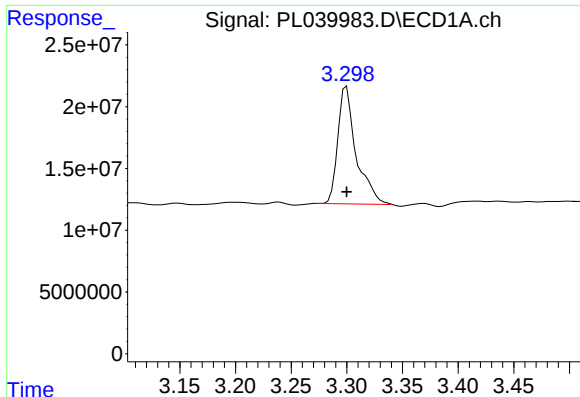

#1 Tetrachloro-m-xylene


R.T.: 3.300 min
Delta R.T.: 0.000 min
Response: 108695104
Conc: 14.02 ng/ml

Instrument :
ECD_L
ClientSampleId :

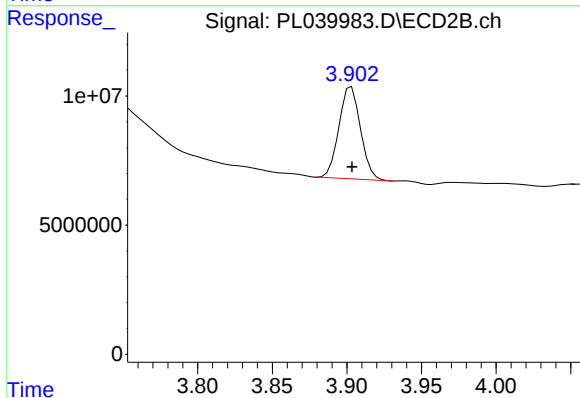


#1 Tetrachloro-m-xylene

R.T.: 3.903 min
Delta R.T.: 0.000 min
Response: 35849155
Conc: 11.24 ng/ml

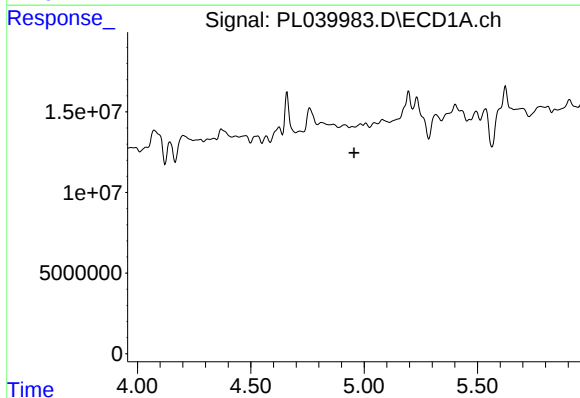


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.956 min
Response: 0
Conc: N.D.

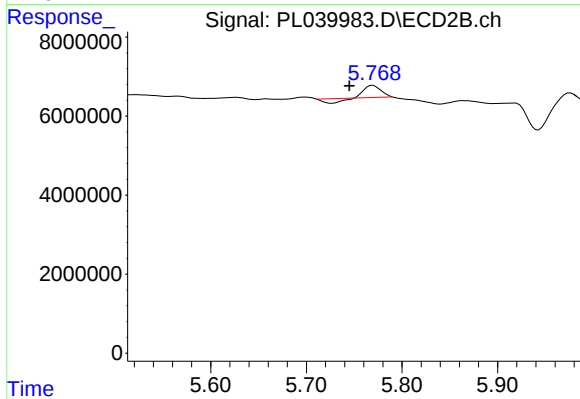

#8 Heptachlor epoxide


R.T.: 5.770 min
Delta R.T.: 0.025 min
Response: 2541411
Conc: 0.64 ng/ml

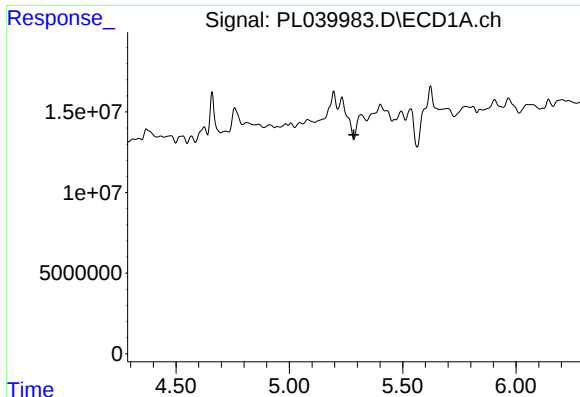

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.285 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

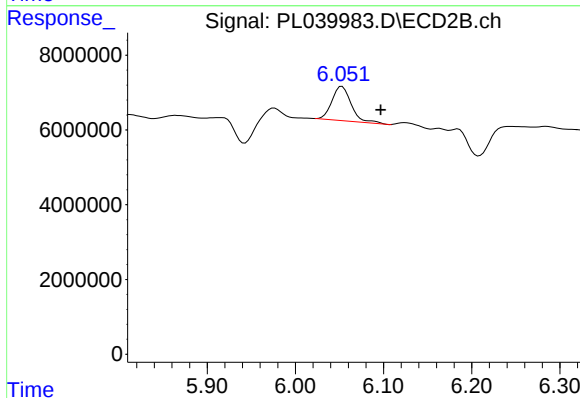


#9 Endosulfan I

R.T.: 6.053 min
Delta R.T.: -0.044 min
Response: 14004993
Conc: 3.94 ng/ml

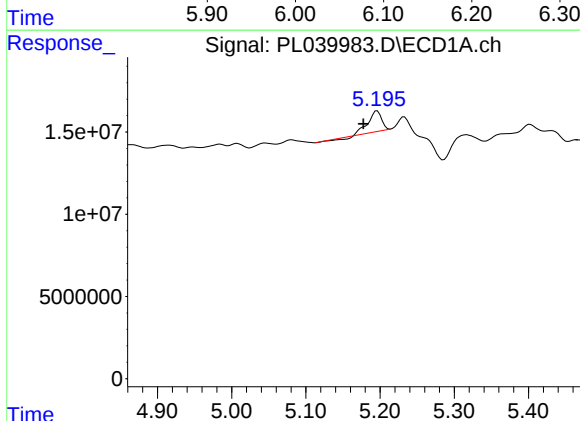


#10 gamma-Chlordane

R.T.: 5.196 min
Delta R.T.: 0.019 min
Response: 14493356
Conc: 1.30 ng/ml

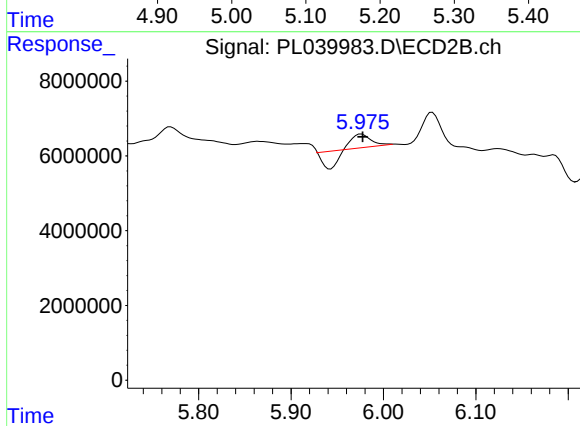

#10 gamma-Chlordane


R.T.: 5.976 min
Delta R.T.: -0.001 min
Response: 1531896
Conc: 0.40 ng/ml

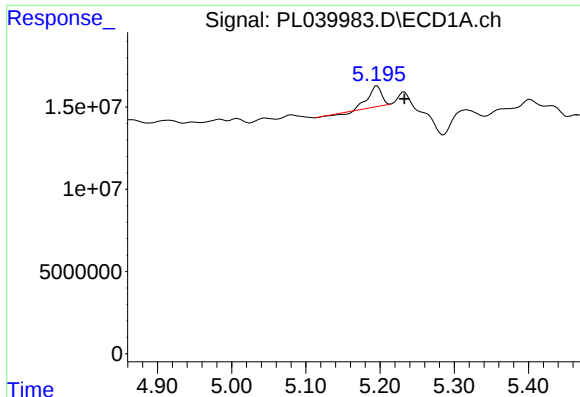

#11 alpha-Chlordane


R.T.: 5.196 min
Delta R.T.: -0.037 min
Response: 14493356
Conc: 1.36 ng/ml

Instrument :
ECD_L
ClientSampleId :

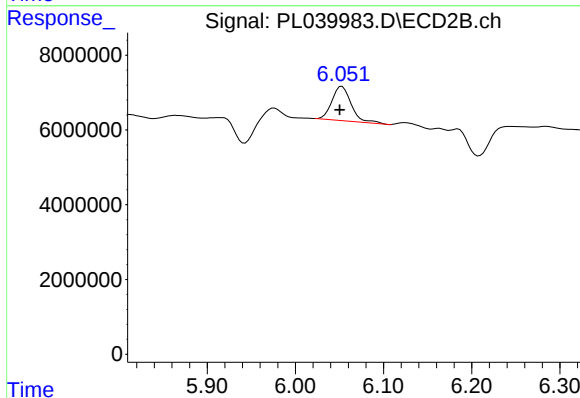


#11 alpha-Chlordane

R.T.: 6.053 min
Delta R.T.: 0.003 min
Response: 14004993
Conc: 3.54 ng/ml

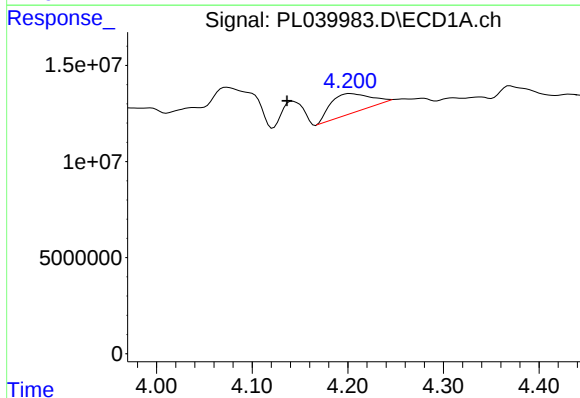


#23 Chlordane-1

R.T.: 4.203 min
Delta R.T.: 0.066 min
Response: 29020803
Conc: 80.07 ng/ml

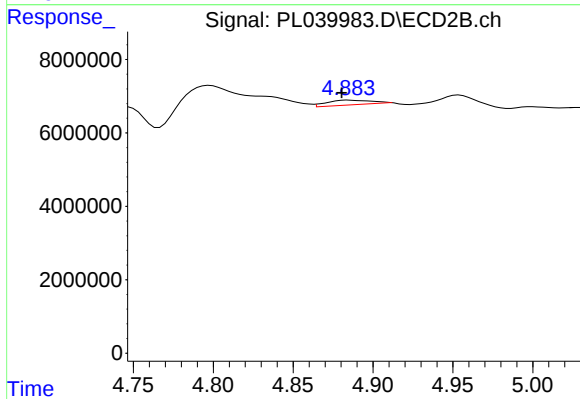

#23 Chlordane-1


R.T.: 4.884 min
Delta R.T.: 0.004 min
Response: 2817335
Conc: 18.19 ng/ml

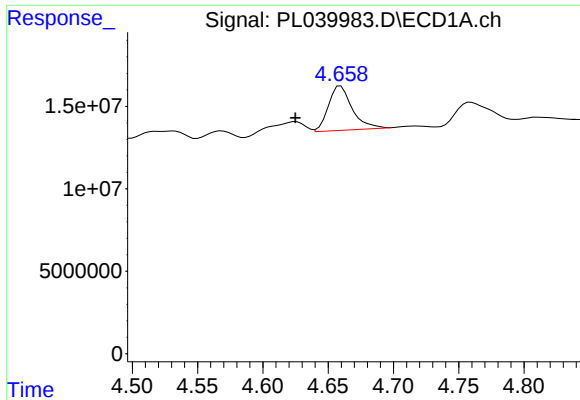

#24 Chlordane-2


R.T.: 4.660 min
Delta R.T.: 0.035 min
Response: 33969291
Conc: 90.20 ng/ml

Instrument :
ECD_L
ClientSampleId :

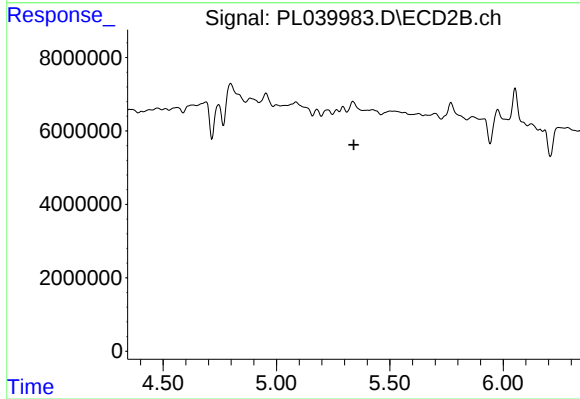


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.341 min
Response: 0
Conc: N.D.

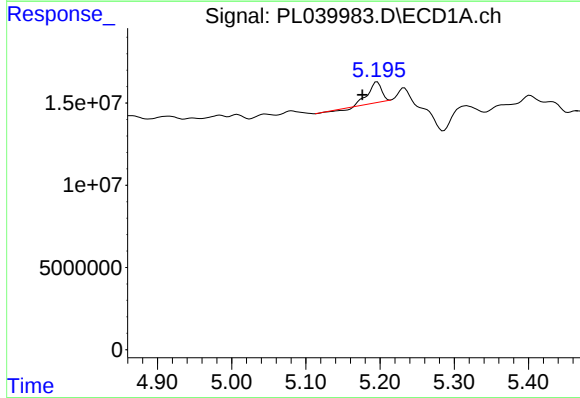


#25 Chlordane-3

R.T.: 5.196 min
Delta R.T.: 0.020 min
Response: 14493356
Conc: 11.81 ng/ml

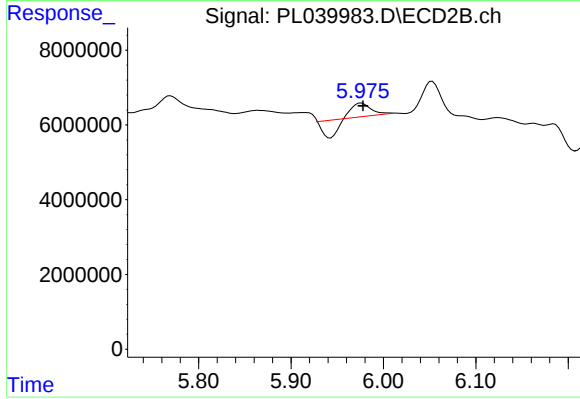

#25 Chlordane-3


R.T.: 5.976 min
Delta R.T.: -0.002 min
Response: 1531896
Conc: 2.99 ng/ml

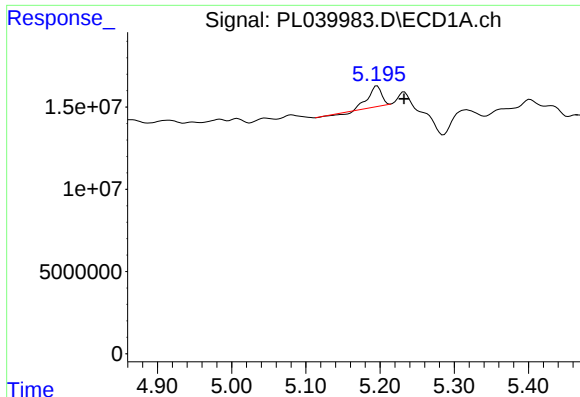

#26 Chlordane-4


R.T.: 5.196 min
Delta R.T.: -0.036 min
Response: 14493356
Conc: 13.22 ng/ml

Instrument :
ECD_L
ClientSampleId :

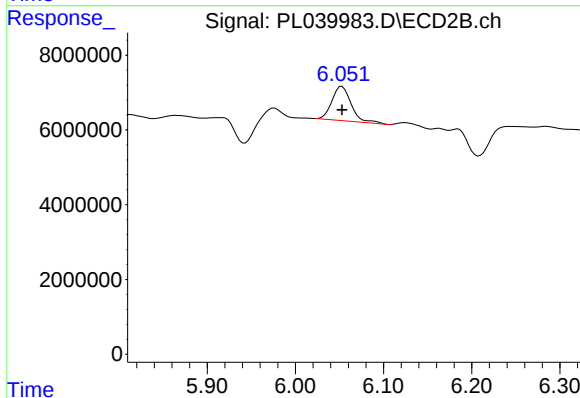


#26 Chlordane-4

R.T.: 6.053 min
Delta R.T.: 0.000 min
Response: 14004993
Conc: 22.63 ng/ml

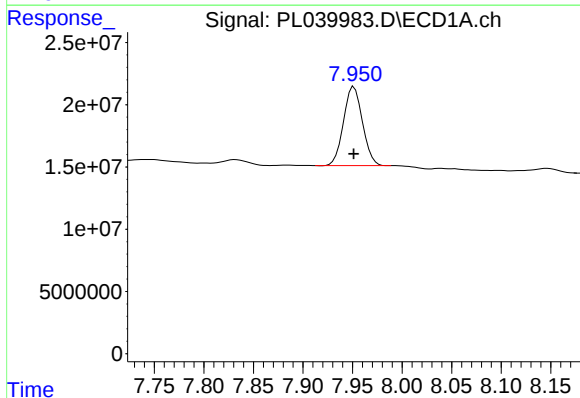

#28 Decachlorobiphenyl

R.T.: 7.951 min
Delta R.T.: 0.000 min
Response: 84211815
Conc: 10.11 ng/ml

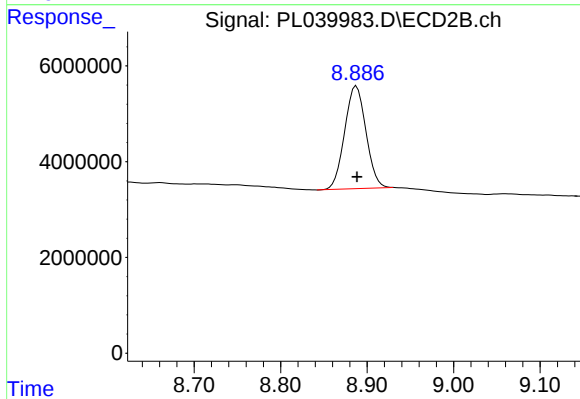

#28 Decachlorobiphenyl

R.T.: 8.887 min
Delta R.T.: 0.000 min
Response: 36576883
Conc: 13.47 ng/ml