

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091718\
 Data File : PL039985.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Sep 2018 11:38
 Operator : AJ\SJ
 Sample : J4773-09
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 18 01:10:19 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 14 23:10:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.300	3.903	100.3E6	37225551	12.932	11.667
28)	SA Decachlor...	7.952	8.888	76937054	34598626	9.233	12.739 #
Target Compounds							
24)	Chlordane-2	4.660	0.000	22487847	0	59.710	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091718\
Data File : PL039985.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Sep 2018 11:38
Operator : AJ\SJ
Sample : J4773-09
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 18 01:10:19 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
Quant Title : GC Extractables
QLast Update : Fri Sep 14 23:10:39 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

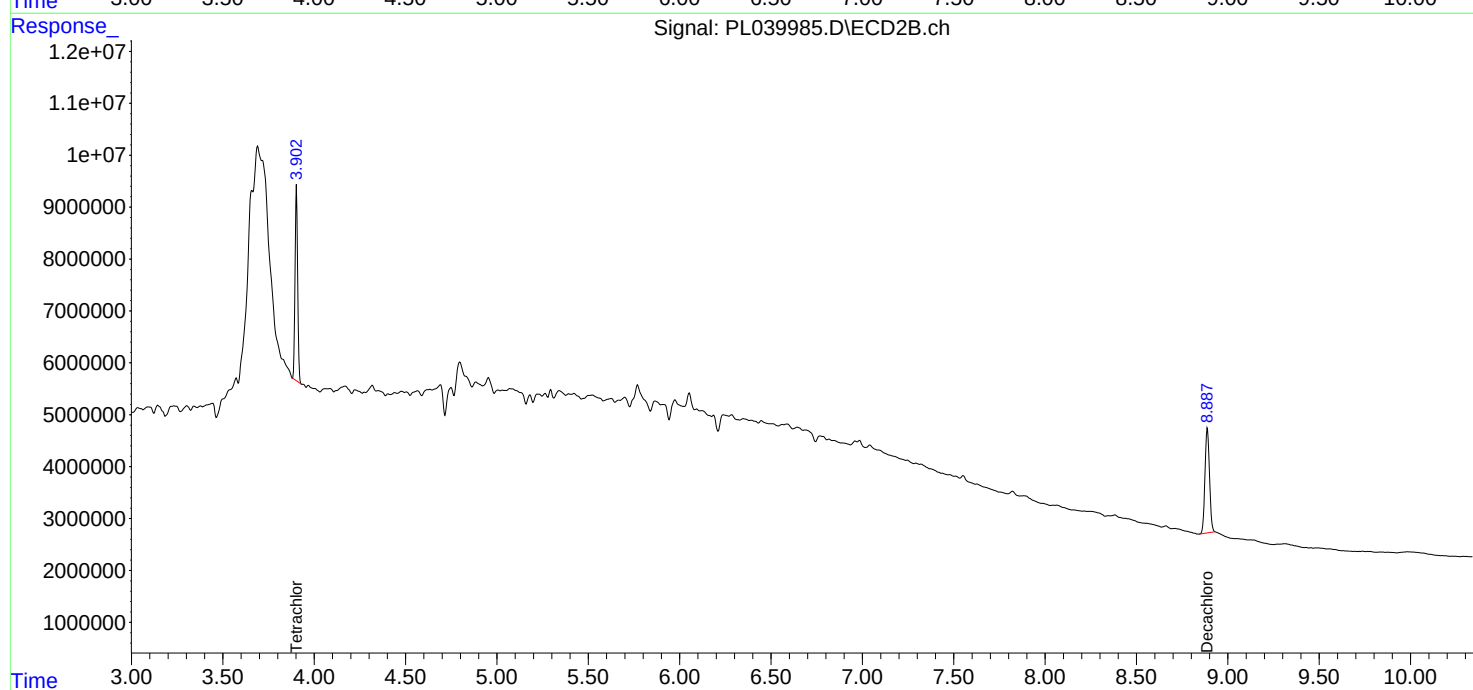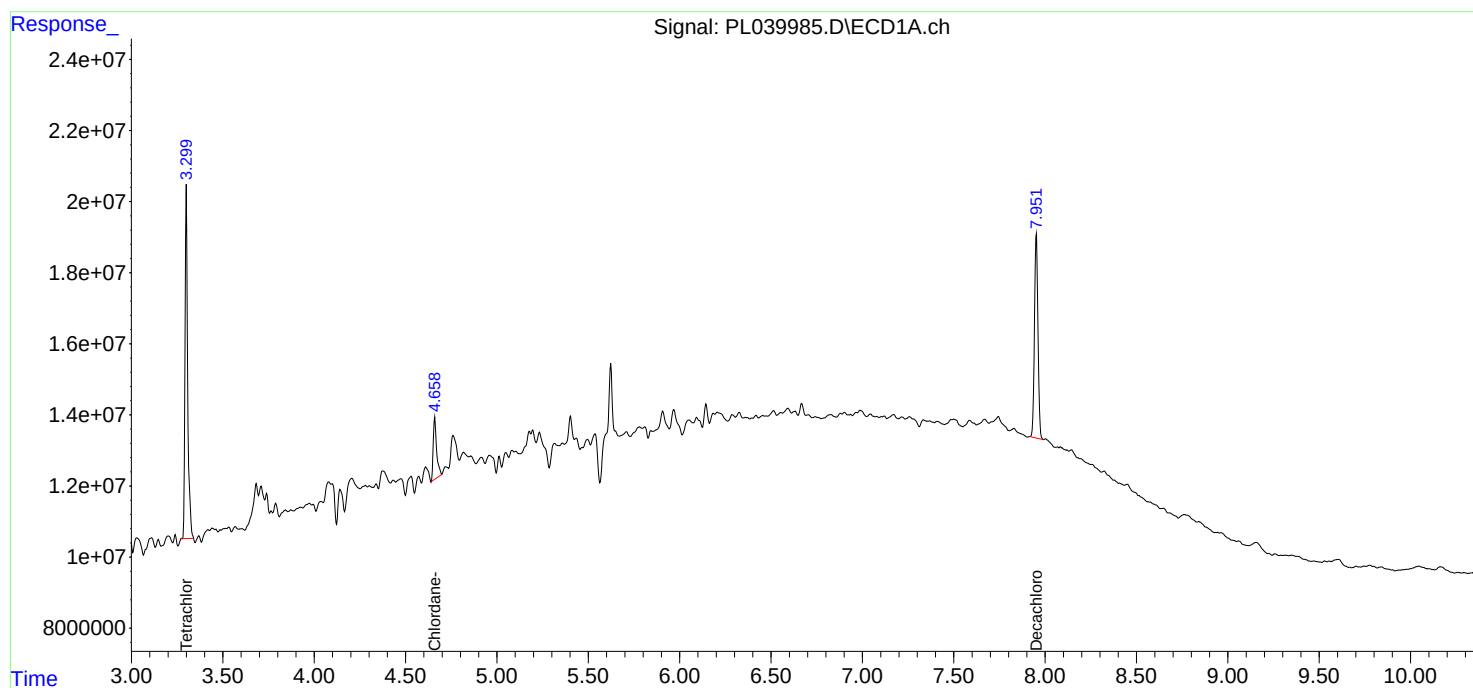


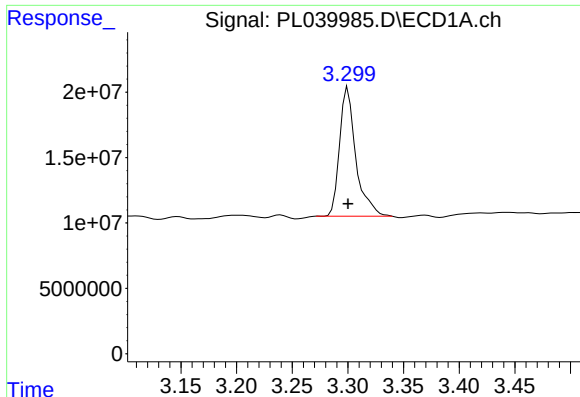

#1 Tetrachloro-m-xylene


R.T.: 3.300 min
Delta R.T.: 0.000 min
Response: 100286955
Conc: 12.93 ng/ml

Instrument :
ECD_L
ClientSampleId :

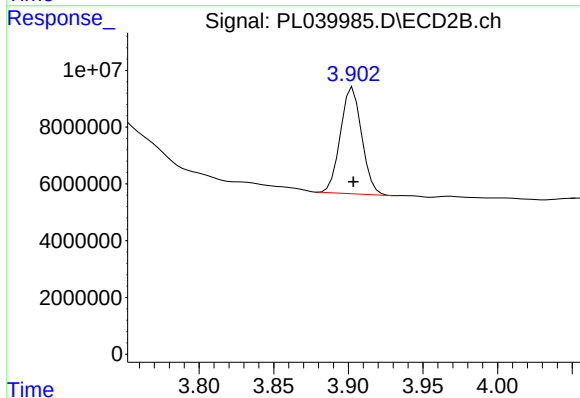


#1 Tetrachloro-m-xylene

R.T.: 3.903 min
Delta R.T.: 0.000 min
Response: 37225551
Conc: 11.67 ng/ml

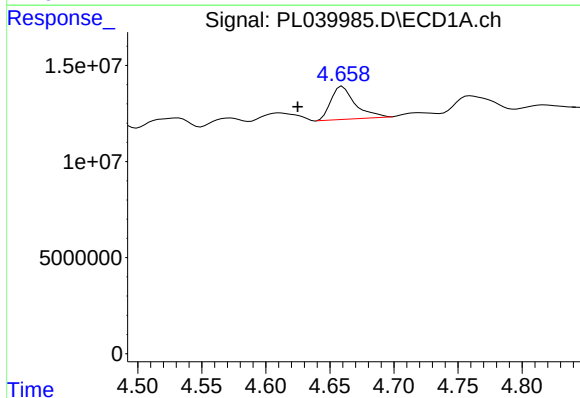


#24 Chlordane-2

R.T.: 4.660 min
Delta R.T.: 0.035 min
Response: 22487847
Conc: 59.71 ng/ml

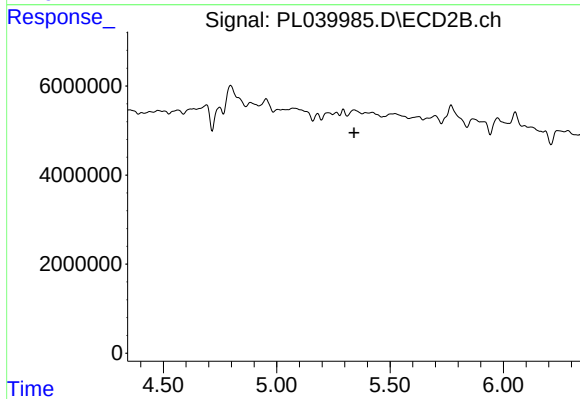

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 5.341 min
Response: 0
Conc: N.D.

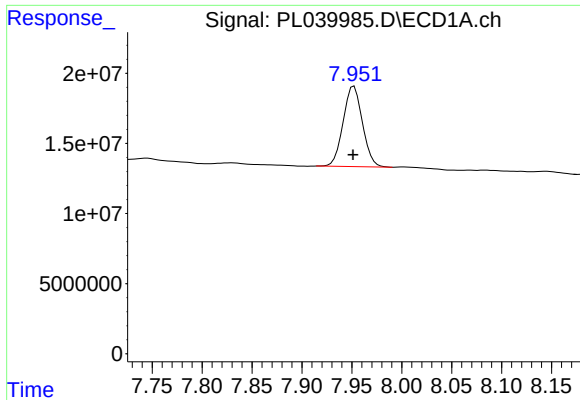

#28 Decachlorobiphenyl

R.T.: 7.952 min
Delta R.T.: 0.000 min
Response: 76937054
Conc: 9.23 ng/ml

Instrument :
ECD_L
ClientSampleId :

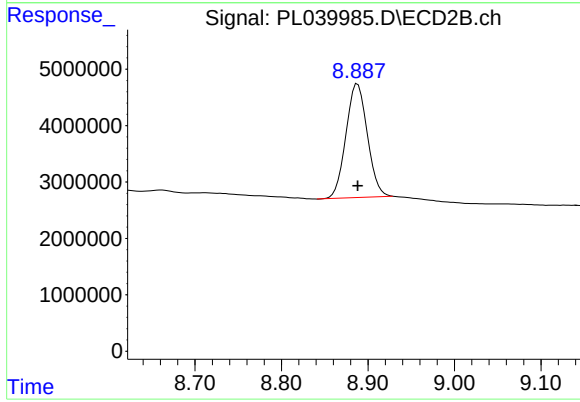

#28 Decachlorobiphenyl

R.T.: 8.888 min
Delta R.T.: 0.000 min
Response: 34598626
Conc: 12.74 ng/ml