

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091718\
 Data File : PL039994.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Sep 2018 13:45
 Operator : AJ\SJ
 Sample : J4929-09
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 18 01:12:02 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 14 23:10:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.300	3.903	154.7E6	65782128	19.943	20.616
28)	SA Decachlor...	7.952	8.888	117.4E6	51857837	14.093	19.093 #
Target Compounds							
3)	MA gamma-BHC...	4.049f	0.000	165.4E6	0	14.454	N.D. #
7)	B delta-BHC	0.000	4.953	0	21684686	N.D.	5.452 #
8)	B Heptachlo...	0.000	5.770	0	11105394	N.D.	2.808 #
10)	B gamma-Chl...	0.000	5.947	0	14830189	N.D.	3.919 #
13)	MA Dieldrin	5.523	6.366	36406014	5144284	3.283	1.352 #
16)	A 4,4'-DDD	5.874f	6.672	469918	8124045	0.054	2.810 #
17)	MA 4,4'-DDT	6.205f	0.000	30854100	0	3.409	N.D. #
18)	B Endrin al...	6.205	0.000	30854100	0	4.025	N.D. #
25)	Chlordane-3	0.000	5.947	0	14830189	N.D.	28.969 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091718\
Data File : PL039994.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Sep 2018 13:45
Operator : AJ\SJ
Sample : J4929-09
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 18 01:12:02 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
Quant Title : GC Extractables
QLast Update : Fri Sep 14 23:10:39 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

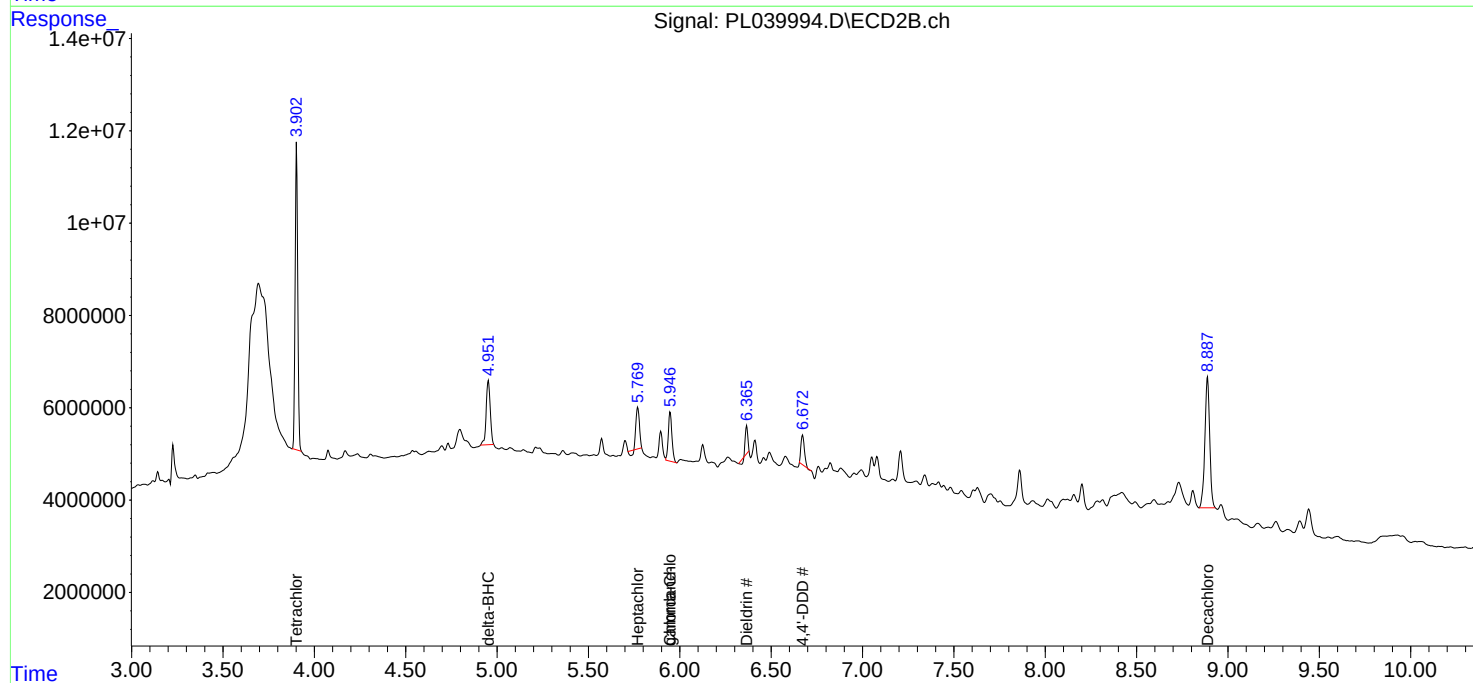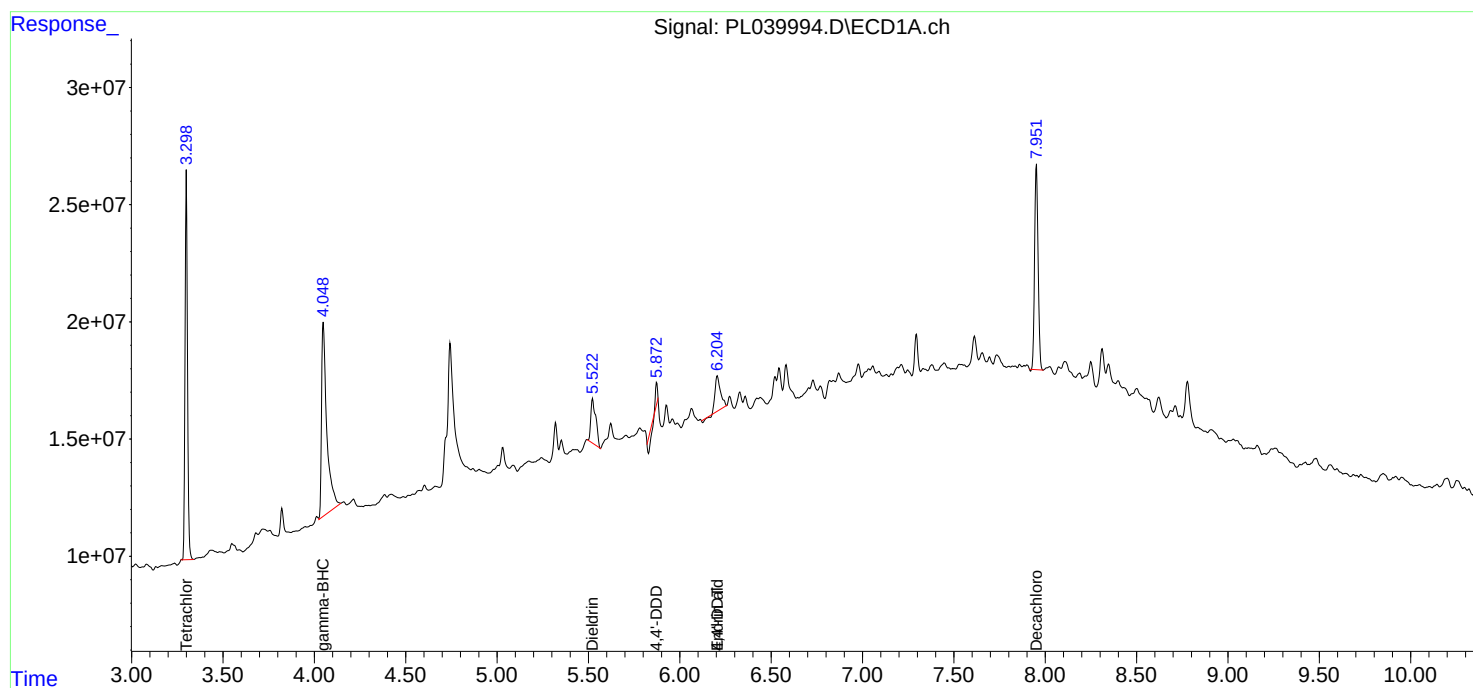


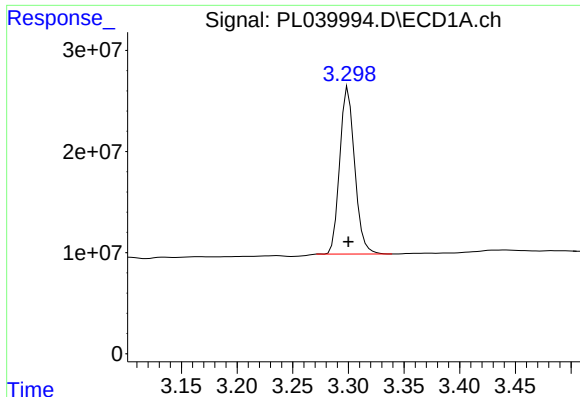

#1 Tetrachloro-m-xylene


R.T.: 3.300 min
Delta R.T.: 0.000 min
Response: 154657054
Conc: 19.94 ng/ml

Instrument :
ECD_L
ClientSampleId :

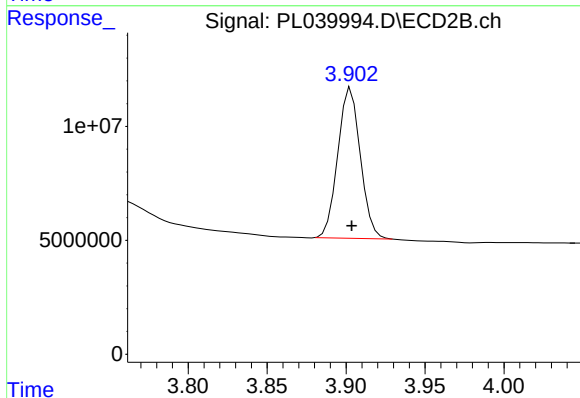


#1 Tetrachloro-m-xylene

R.T.: 3.903 min
Delta R.T.: 0.000 min
Response: 65782128
Conc: 20.62 ng/ml

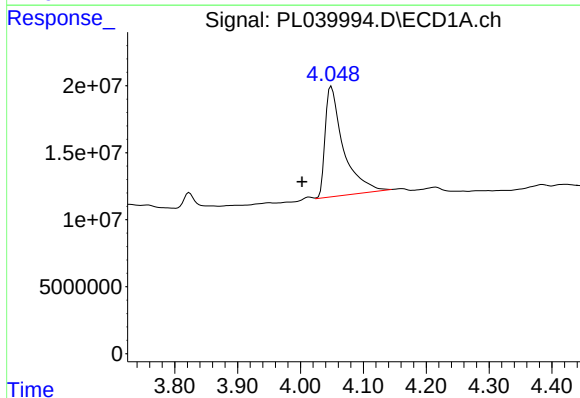


#3 gamma-BHC (Lindane)

R.T.: 4.049 min
Delta R.T.: 0.047 min
Response: 165413661
Conc: 14.45 ng/ml

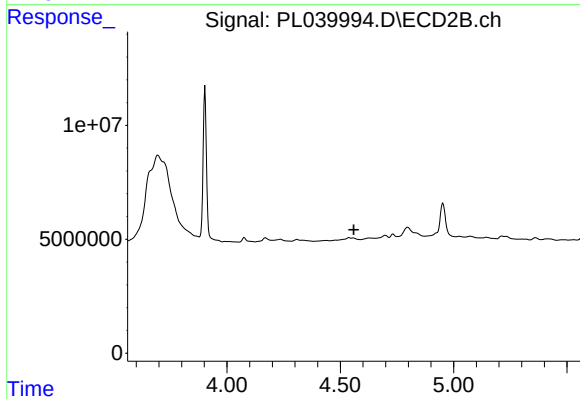

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.559 min
Response: 0
Conc: N.D.

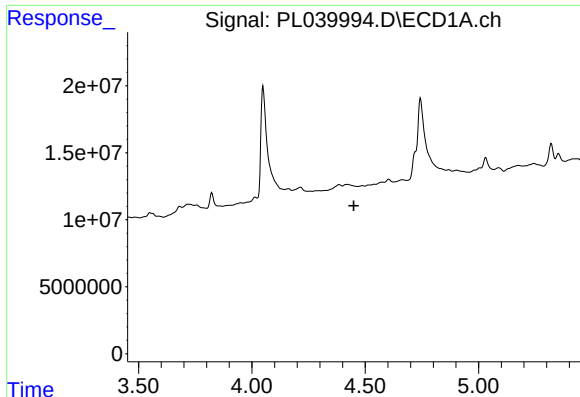

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.449 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

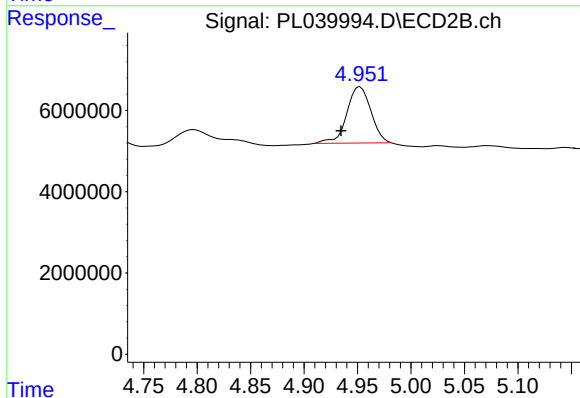


#7 delta-BHC

R.T.: 4.953 min
Delta R.T.: 0.018 min
Response: 21684686
Conc: 5.45 ng/ml

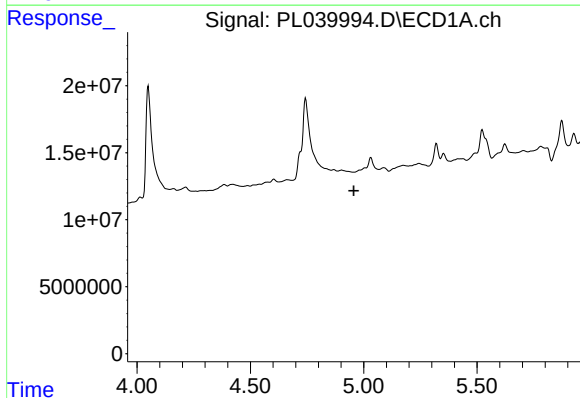


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.956 min
Response: 0
Conc: N.D.

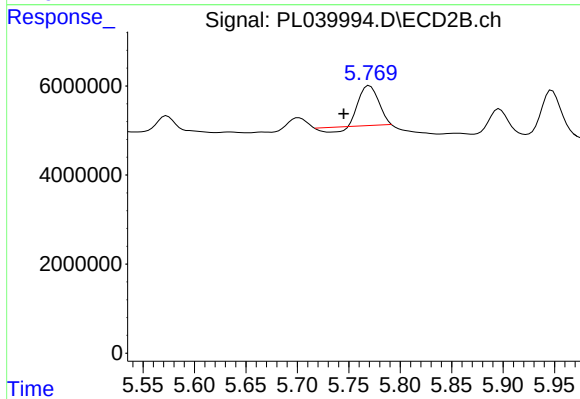

#8 Heptachlor epoxide


R.T.: 5.770 min
Delta R.T.: 0.025 min
Response: 11105394
Conc: 2.81 ng/ml

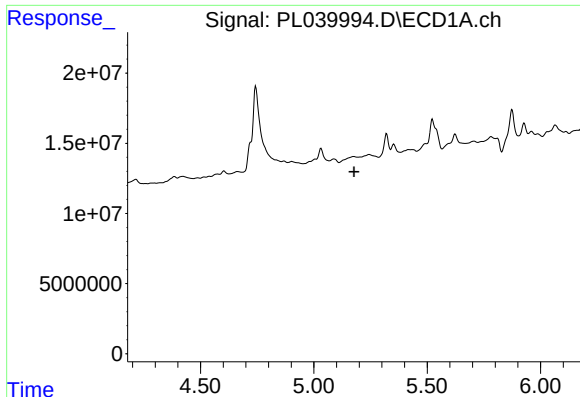

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.178 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

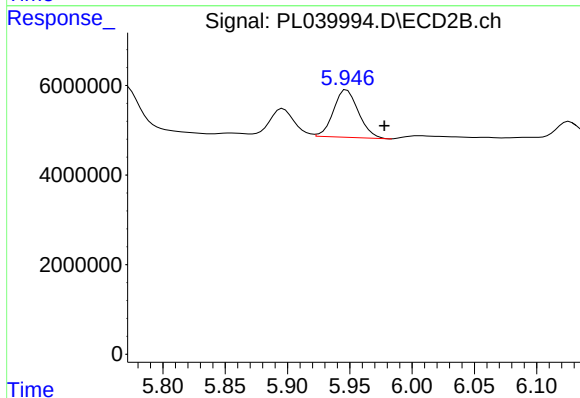


#10 gamma-Chlordane

R.T.: 5.947 min
Delta R.T.: -0.030 min
Response: 14830189
Conc: 3.92 ng/ml

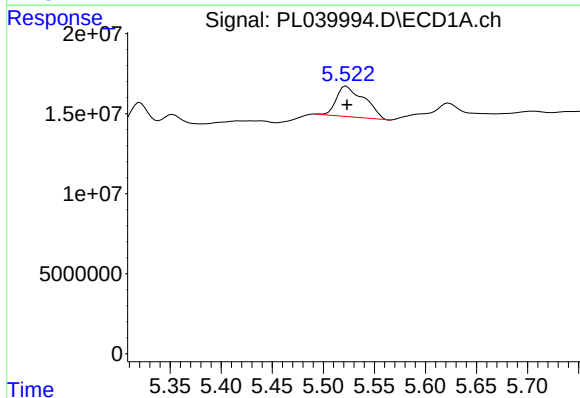


#13 Dieldrin

R.T.: 5.523 min
Delta R.T.: 0.000 min
Response: 36406014
Conc: 3.28 ng/ml

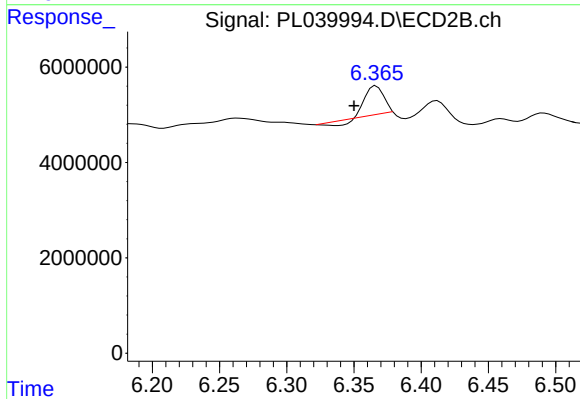

#13 Dieldrin


R.T.: 6.366 min
Delta R.T.: 0.016 min
Response: 5144284
Conc: 1.35 ng/ml

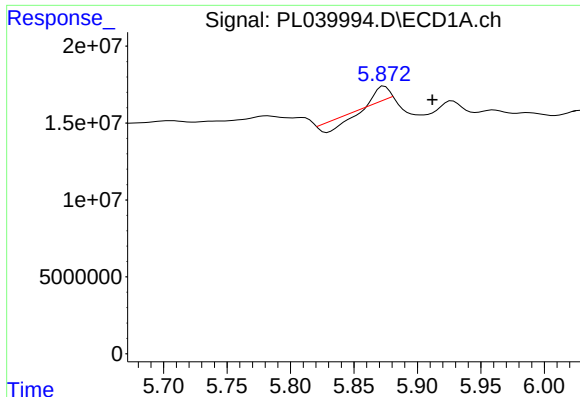

#16 4,4'-DDD


R.T.: 5.874 min
Delta R.T.: -0.038 min
Response: 469918
Conc: 0.05 ng/ml

Instrument :
ECD_L
ClientSampleId :

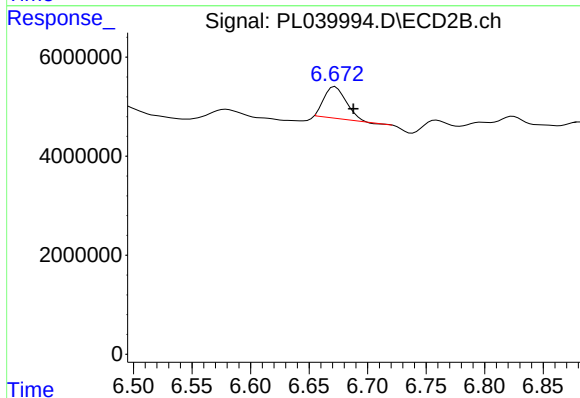


#16 4,4'-DDD

R.T.: 6.672 min
Delta R.T.: -0.016 min
Response: 8124045
Conc: 2.81 ng/ml

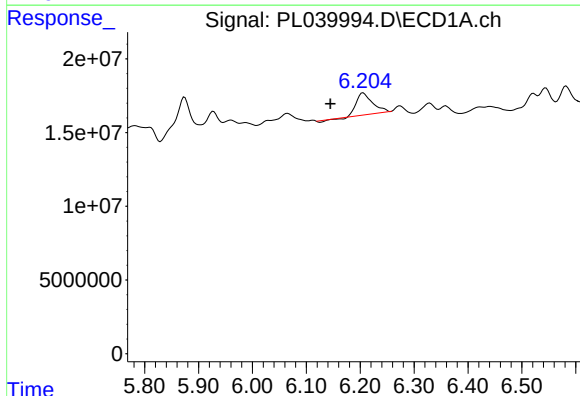


#17 4,4'-DDT

R.T.: 6.205 min
Delta R.T.: 0.061 min
Response: 30854100
Conc: 3.41 ng/ml

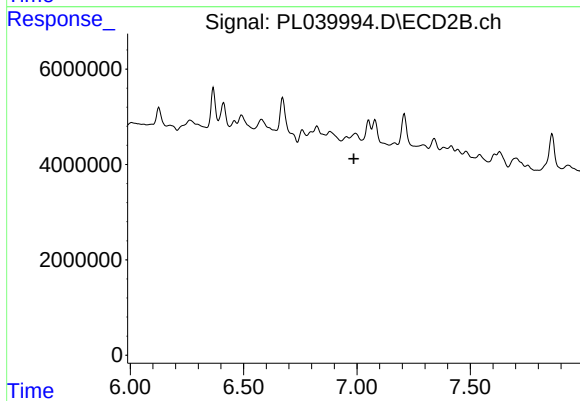

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.986 min
Response: 0
Conc: N.D.

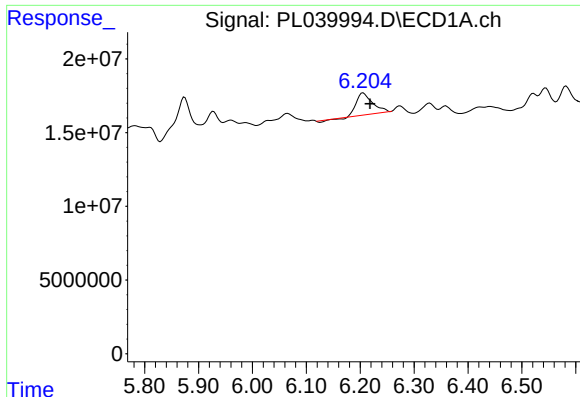

#18 Endrin aldehyde


R.T.: 6.205 min
Delta R.T.: -0.013 min
Response: 30854100
Conc: 4.03 ng/ml

Instrument :
ECD_L
ClientSampleId :

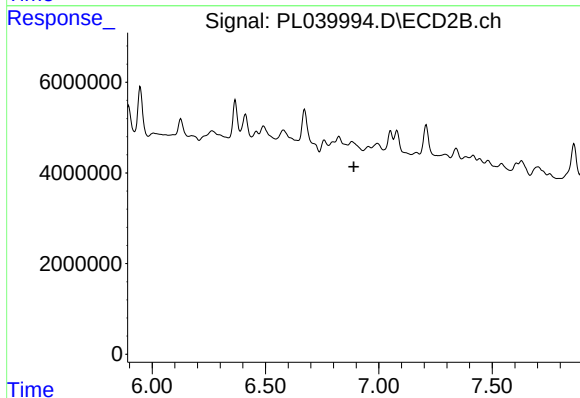


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.890 min
Response: 0
Conc: N.D.

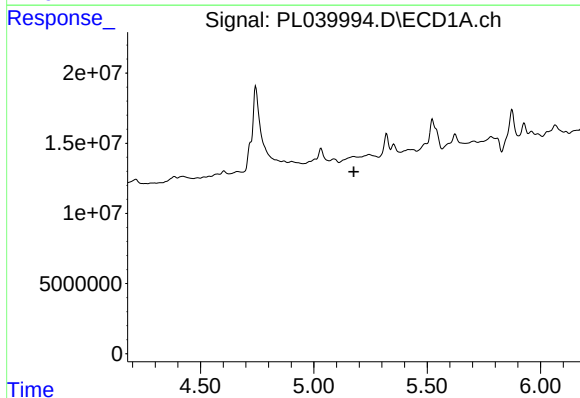


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.176 min
Response: 0
Conc: N.D.

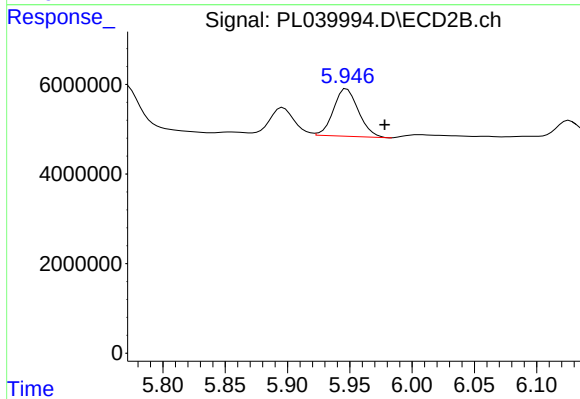

#25 Chlordane-3


R.T.: 5.947 min
Delta R.T.: -0.030 min
Response: 14830189
Conc: 28.97 ng/ml

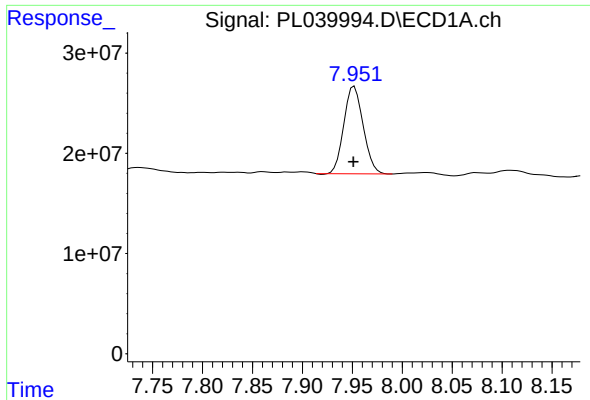

#28 Decachlorobiphenyl

R.T.: 7.952 min
Delta R.T.: 0.000 min
Response: 117429970
Conc: 14.09 ng/ml

Instrument :
ECD_L
ClientSampleId :

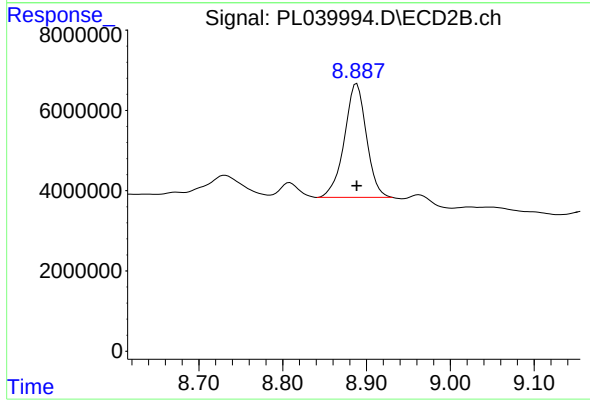

#28 Decachlorobiphenyl

R.T.: 8.888 min
Delta R.T.: 0.000 min
Response: 51857837
Conc: 19.09 ng/ml