

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091718\
 Data File : PL040000.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Sep 2018 16:30
 Operator : AJ\SJ
 Sample : J4773-02
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 18 01:13:12 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 14 23:10:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.302	3.904	132.8E6	56217505	17.125	17.619
28)	SA Decachlor...	7.955	8.891	133.5E6	50302863	16.017	18.521
Target Compounds							
3)	MA gamma-BHC...	4.017	0.000	101.5E6	0	8.868	N.D. #
7)	B delta-BHC	0.000	4.931	0	26415948	N.D.	6.641 #
8)	B Heptachlo...	0.000	5.770	0	23783874	N.D.	6.013 #
10)	B gamma-Chl...	5.209	0.000	65010907	0	5.835	N.D. #
11)	B alpha-Chl...	5.209	0.000	65010907	0	6.085	N.D. #
15)	B Endosulfa...	6.010f	0.000	20270345	0	2.116	N.D. #
20)	A Methoxychlor	6.632f	0.000	41138326	0	8.875	N.D. #
23)	Chlordane-1	0.000	4.931	0	26415948	N.D.	170.595 #
25)	Chlordane-3	5.209	0.000	65010907	0	52.978	N.D. #
26)	Chlordane-4	5.209	0.000	65010907	0	59.303	N.D. #
27)	Chlordane-5	6.010	6.873	20270345	-2055665	54.674	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091718\
Data File : PL040000.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Sep 2018 16:30
Operator : AJ\SJ
Sample : J4773-02
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 18 01:13:12 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
Quant Title : GC Extractables
QLast Update : Fri Sep 14 23:10:39 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

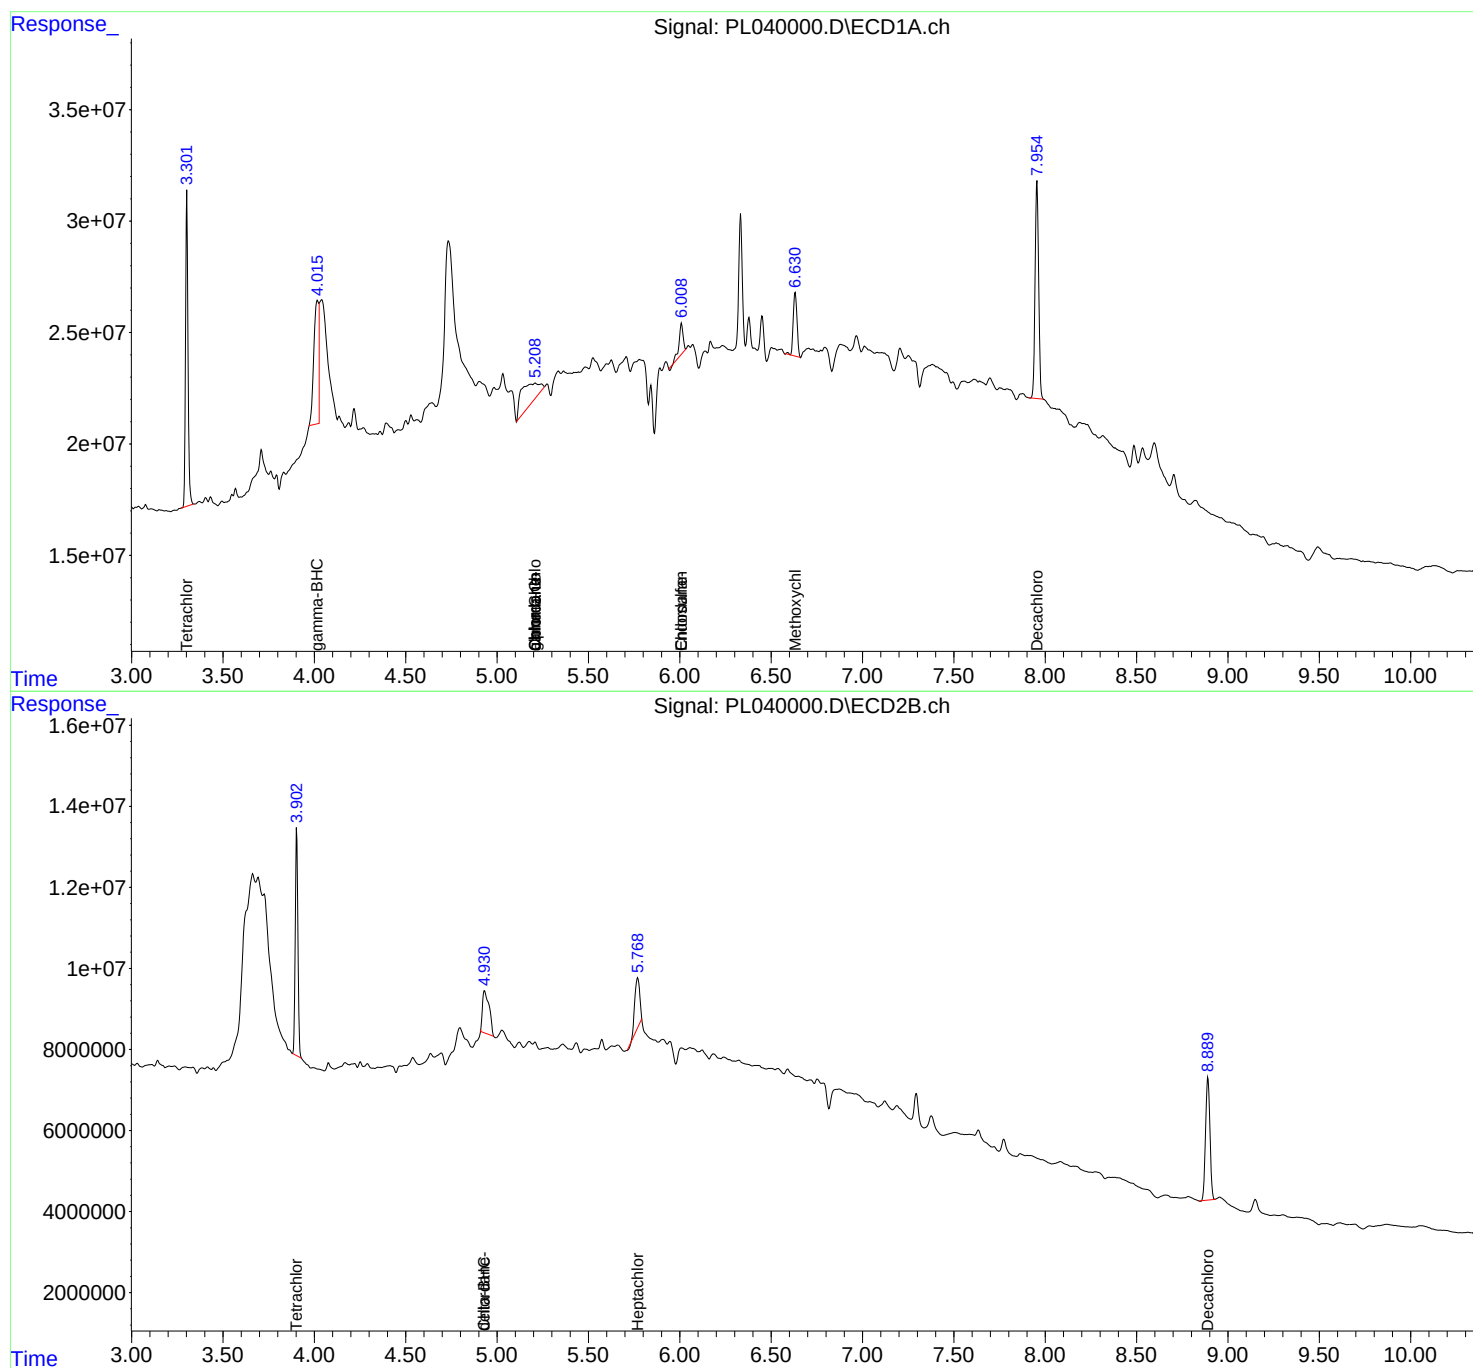


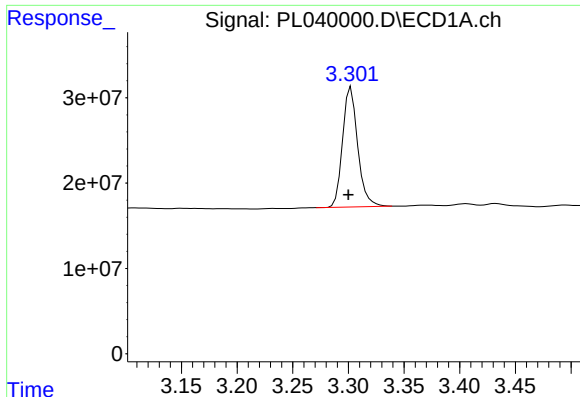

#1 Tetrachloro-m-xylene


R.T.: 3.302 min
Delta R.T.: 0.002 min
Response: 132801963
Conc: 17.12 ng/ml

Instrument :
ECD_L
ClientSampleId :

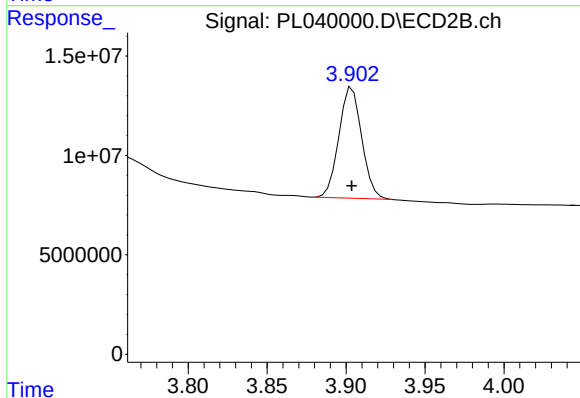


#1 Tetrachloro-m-xylene

R.T.: 3.904 min
Delta R.T.: 0.000 min
Response: 56217505
Conc: 17.62 ng/ml

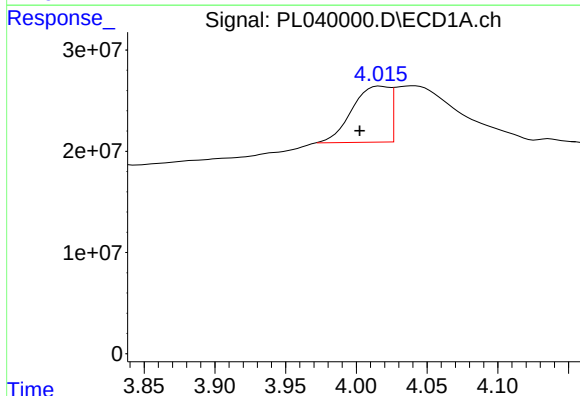


#3 gamma-BHC (Lindane)

R.T.: 4.017 min
Delta R.T.: 0.015 min
Response: 101488811
Conc: 8.87 ng/ml

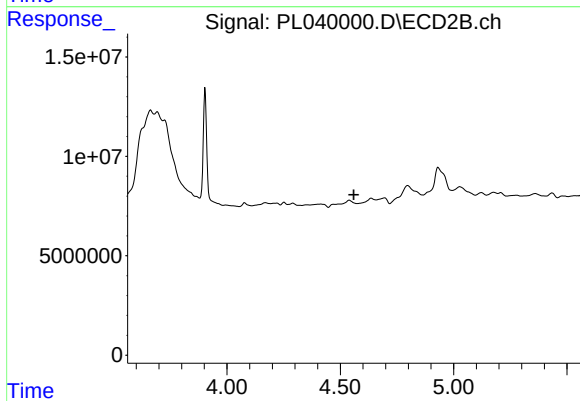

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.559 min
Response: 0
Conc: N.D.

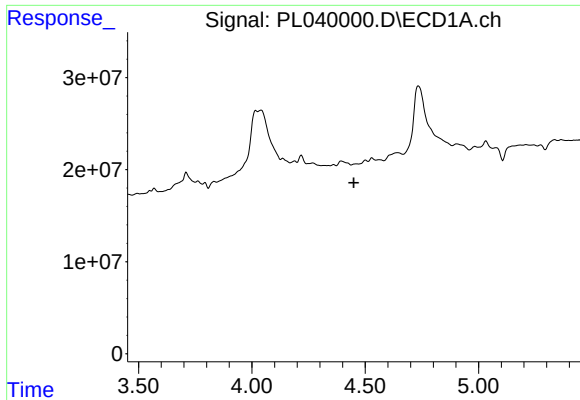

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.449 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

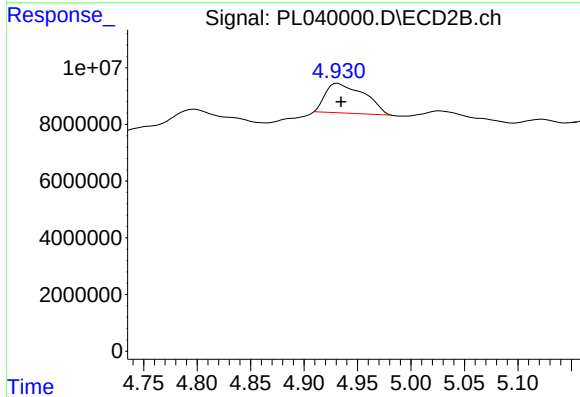


#7 delta-BHC

R.T.: 4.931 min
Delta R.T.: -0.003 min
Response: 26415948
Conc: 6.64 ng/ml

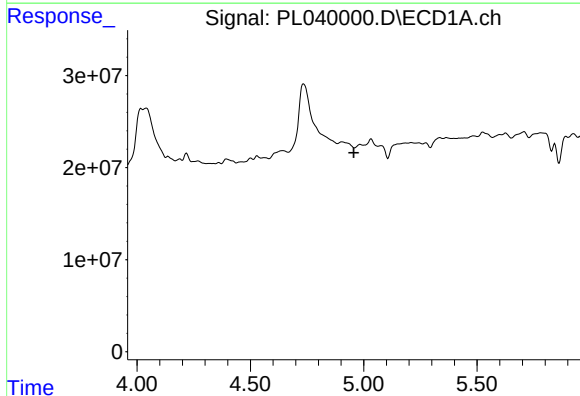


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.956 min
Response: 0
Conc: N.D.

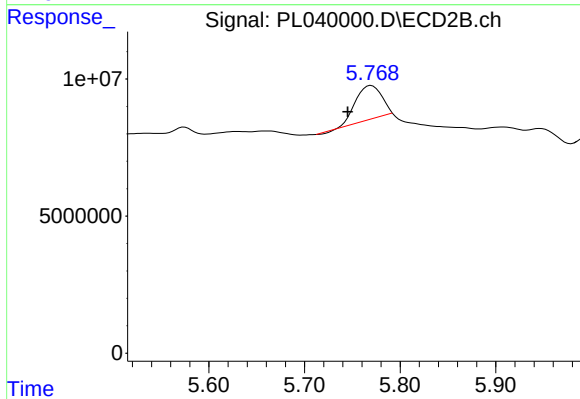

#8 Heptachlor epoxide


R.T.: 5.770 min
Delta R.T.: 0.025 min
Response: 23783874
Conc: 6.01 ng/ml

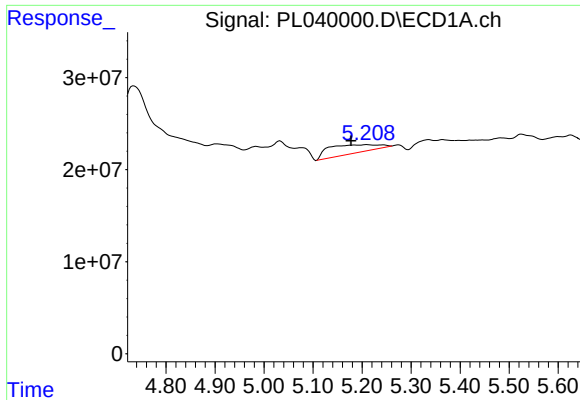

#10 gamma-Chlordane


R.T.: 5.209 min
Delta R.T.: 0.031 min
Response: 65010907
Conc: 5.83 ng/ml

Instrument :
ECD_L
ClientSampleId :

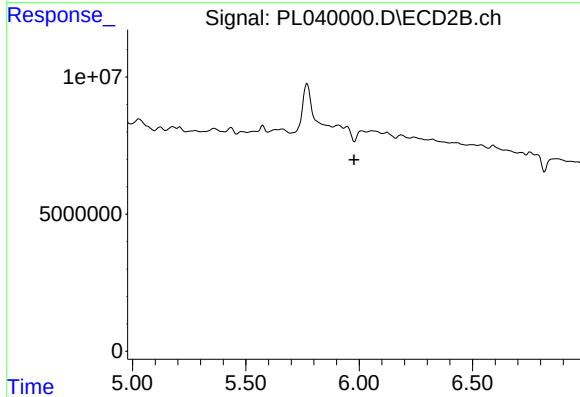


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.978 min
Response: 0
Conc: N.D.

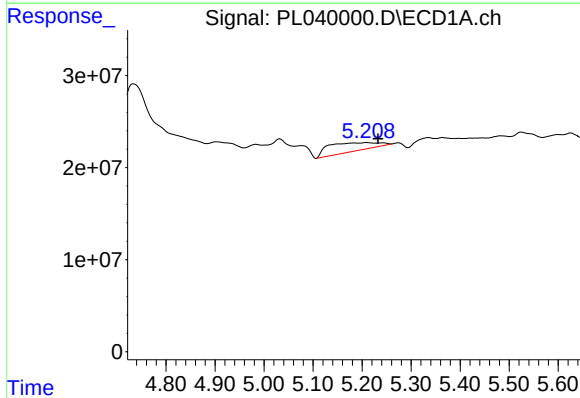


#11 alpha-Chlordane

R.T.: 5.209 min
Delta R.T.: -0.024 min
Response: 65010907
Conc: 6.09 ng/ml

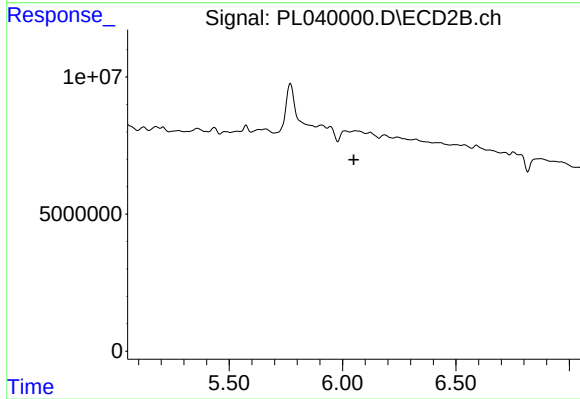

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.050 min
Response: 0
Conc: N.D.

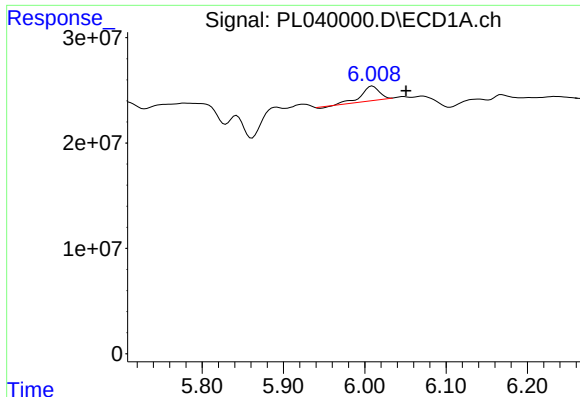

#15 Endosulfan II


R.T.: 6.010 min
Delta R.T.: -0.041 min
Response: 20270345
Conc: 2.12 ng/ml

Instrument :
ECD_L
ClientSampleId :

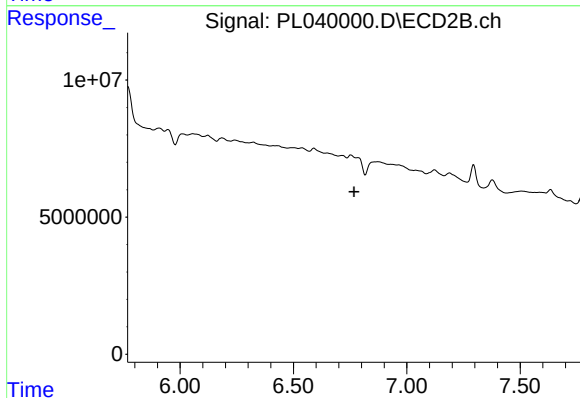


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.767 min
Response: 0
Conc: N.D.

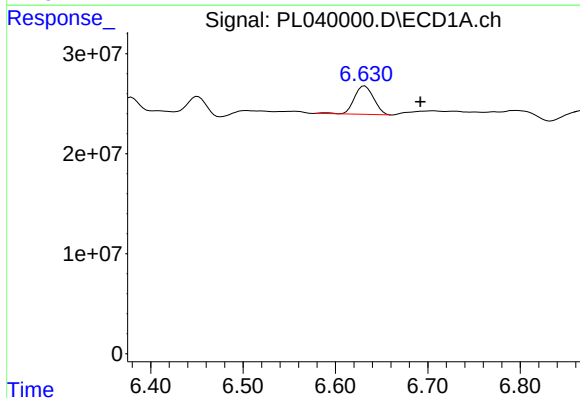


#20 Methoxychlor

R.T.: 6.632 min
Delta R.T.: -0.060 min
Response: 41138326
Conc: 8.88 ng/ml

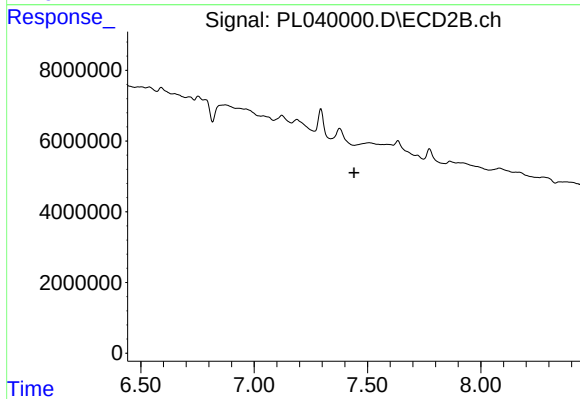

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.441 min
Response: 0
Conc: N.D.

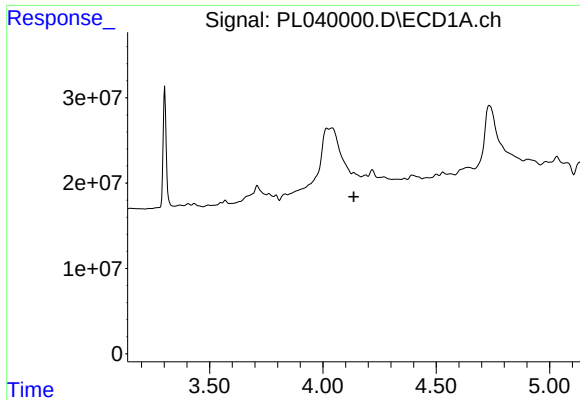

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.136 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

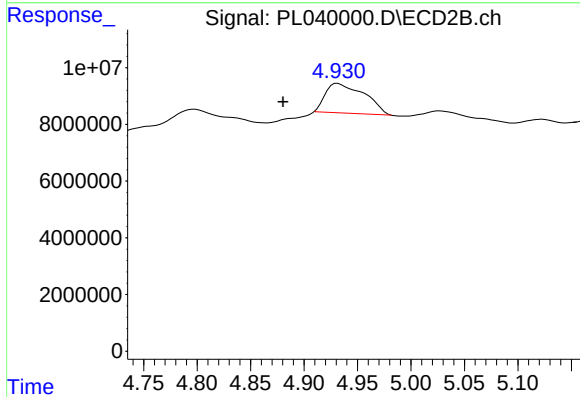


#23 Chlordane-1

R.T.: 4.931 min
Delta R.T.: 0.051 min
Response: 26415948
Conc: 170.59 ng/ml

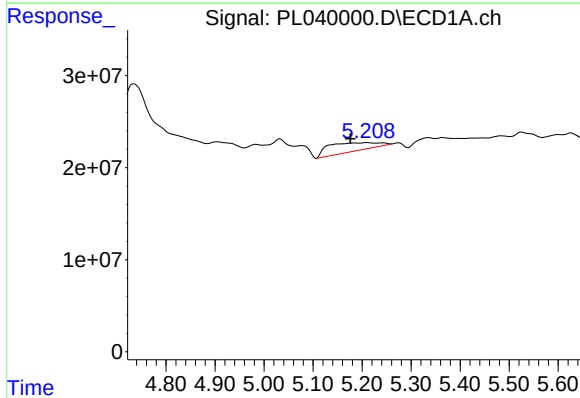


#25 Chlordane-3

R.T.: 5.209 min
Delta R.T.: 0.033 min
Response: 65010907
Conc: 52.98 ng/ml

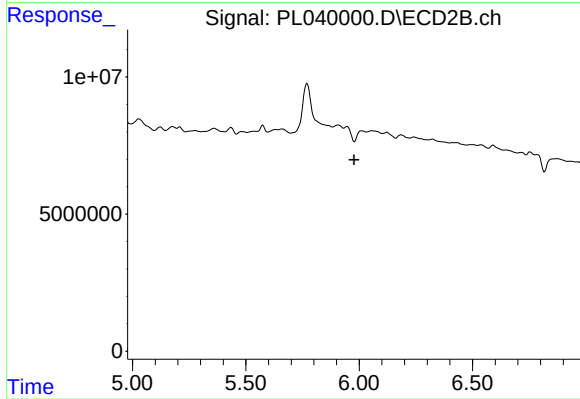

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.978 min
Response: 0
Conc: N.D.

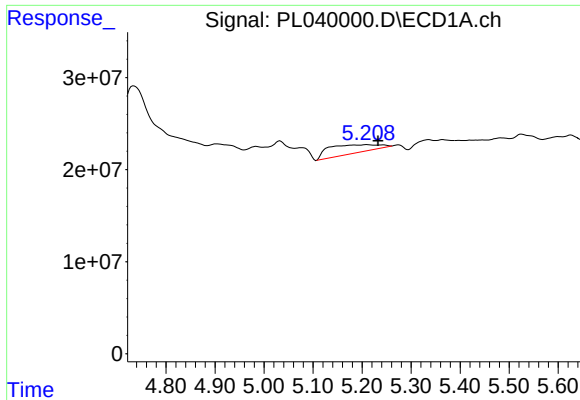

#26 Chlordane-4


R.T.: 5.209 min
Delta R.T.: -0.023 min
Response: 65010907
Conc: 59.30 ng/ml

Instrument :
ECD_L
ClientSampleId :

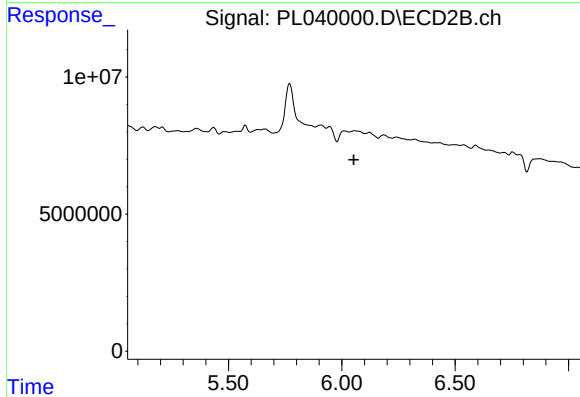


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.053 min
Response: 0
Conc: N.D.

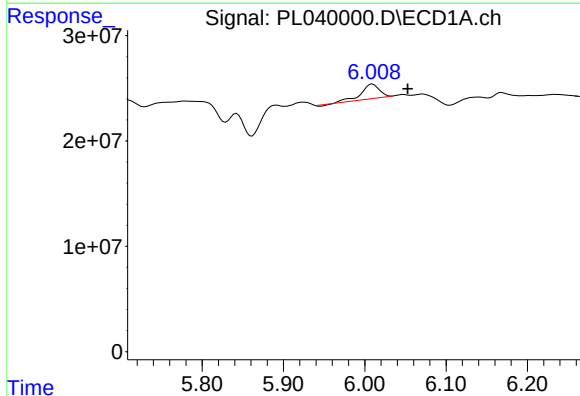


#27 Chlordane-5

R.T.: 6.010 min
Delta R.T.: -0.043 min
Response: 20270345
Conc: 54.67 ng/ml

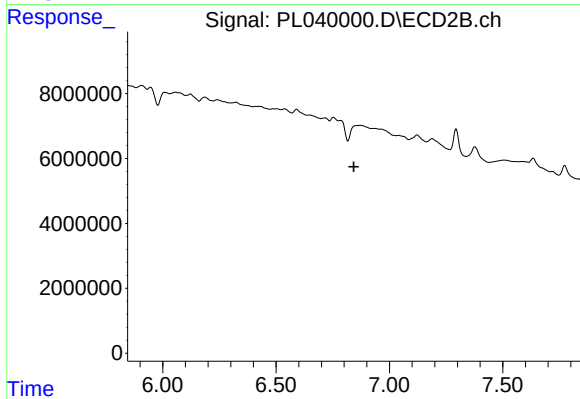

#27 Chlordane-5


R.T.: 6.873 min
Delta R.T.: 0.030 min
Response: -2055665
Conc: N.D.

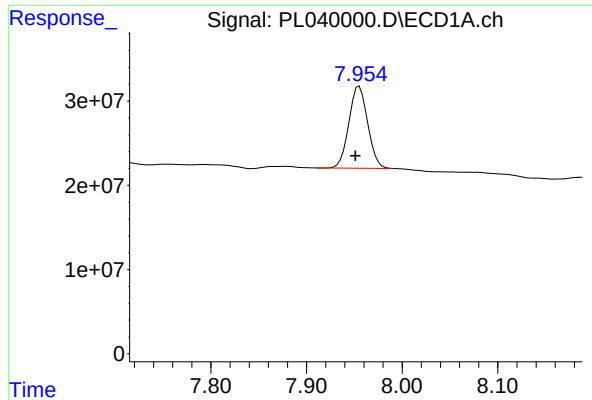

#28 Decachlorobiphenyl

R.T.: 7.955 min
Delta R.T.: 0.004 min
Response: 133463283
Conc: 16.02 ng/ml

Instrument :
ECD_L
ClientSampleId :

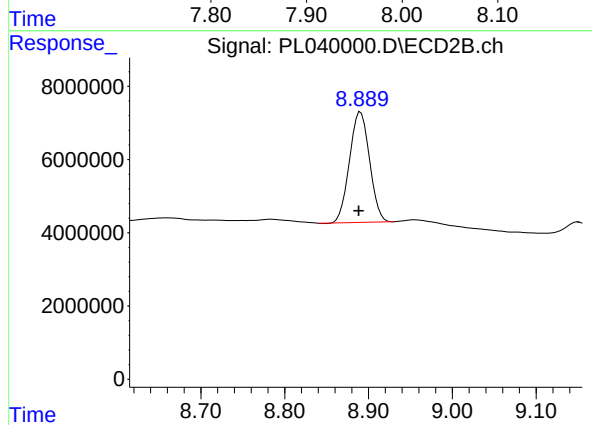

#28 Decachlorobiphenyl

R.T.: 8.891 min
Delta R.T.: 0.002 min
Response: 50302863
Conc: 18.52 ng/ml