

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091718\
 Data File : PL040048.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Sep 2018 03:51
 Operator : AJ\SJ
 Sample : PB112902BL
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 18 04:08:44 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 14 23:10:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.301	3.904	148.0E6	61952724	19.088	19.416
28)	SA Decachlor...	7.954	8.893	164.9E6	62348886	19.793	22.956
Target Compounds							
2)	A alpha-BHC	0.000	4.292	0	5556402	N.D.	1.074 #
3)	MA gamma-BHC...	4.043f	0.000	137.8E6	0	12.039	N.D. #
4)	MA Heptachlor	4.221f	0.000	35833525	0	3.106	N.D. #
6)	B beta-BHC	4.221f	0.000	35833525	0	7.286	N.D. #
7)	B delta-BHC	0.000	4.927	0	4438033	N.D.	1.116 #
8)	B Heptachlo...	0.000	5.772	0	6458769	N.D.	1.633 #
19)	B Endosulfa...	6.450	7.124	81088185	7938537	8.848	2.704 #
20)	A Methoxychlor	6.630f	7.387f	110.8E6	7353721	23.910	5.015 #
23)	Chlordane-1	0.000	4.927	0	4438033	N.D.	28.661 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091718\
Data File : PL040048.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Sep 2018 03:51
Operator : AJ\SJ
Sample : PB112902BL
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 18 04:08:44 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
Quant Title : GC Extractables
QLast Update : Fri Sep 14 23:10:39 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

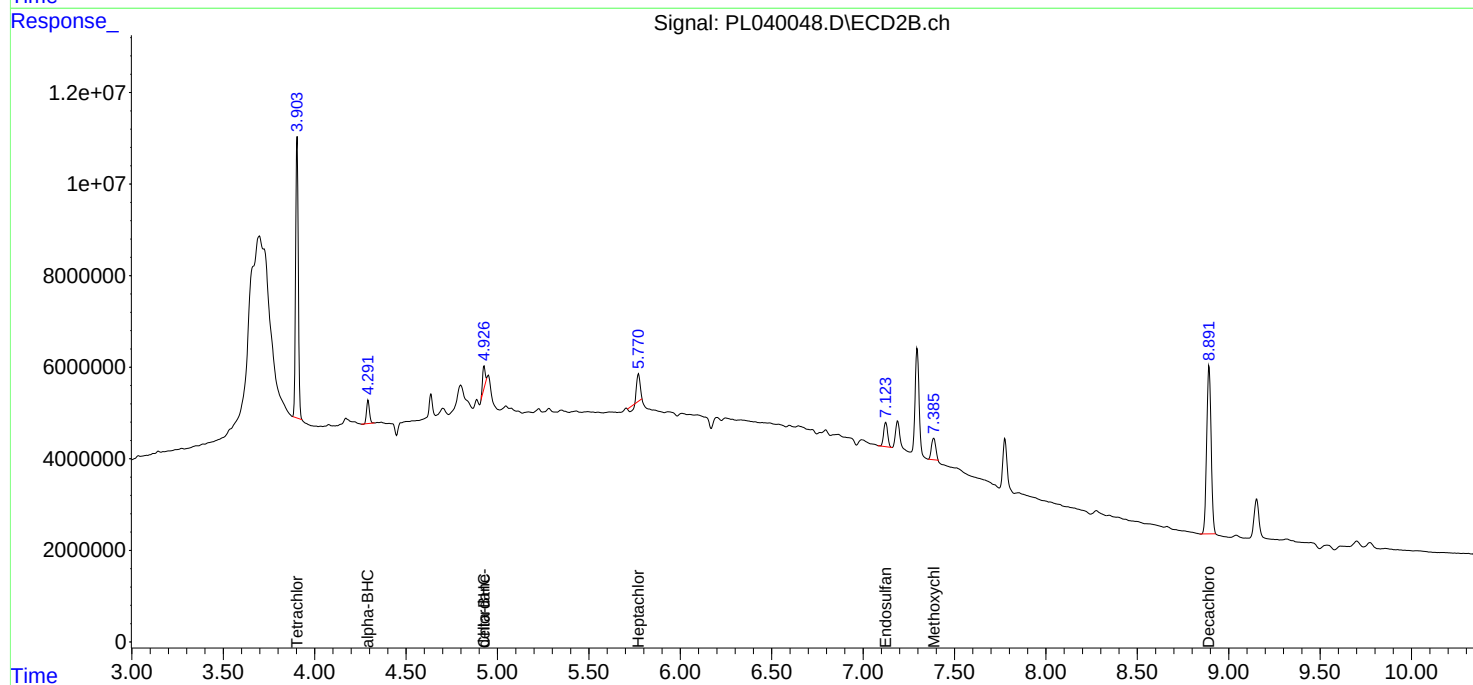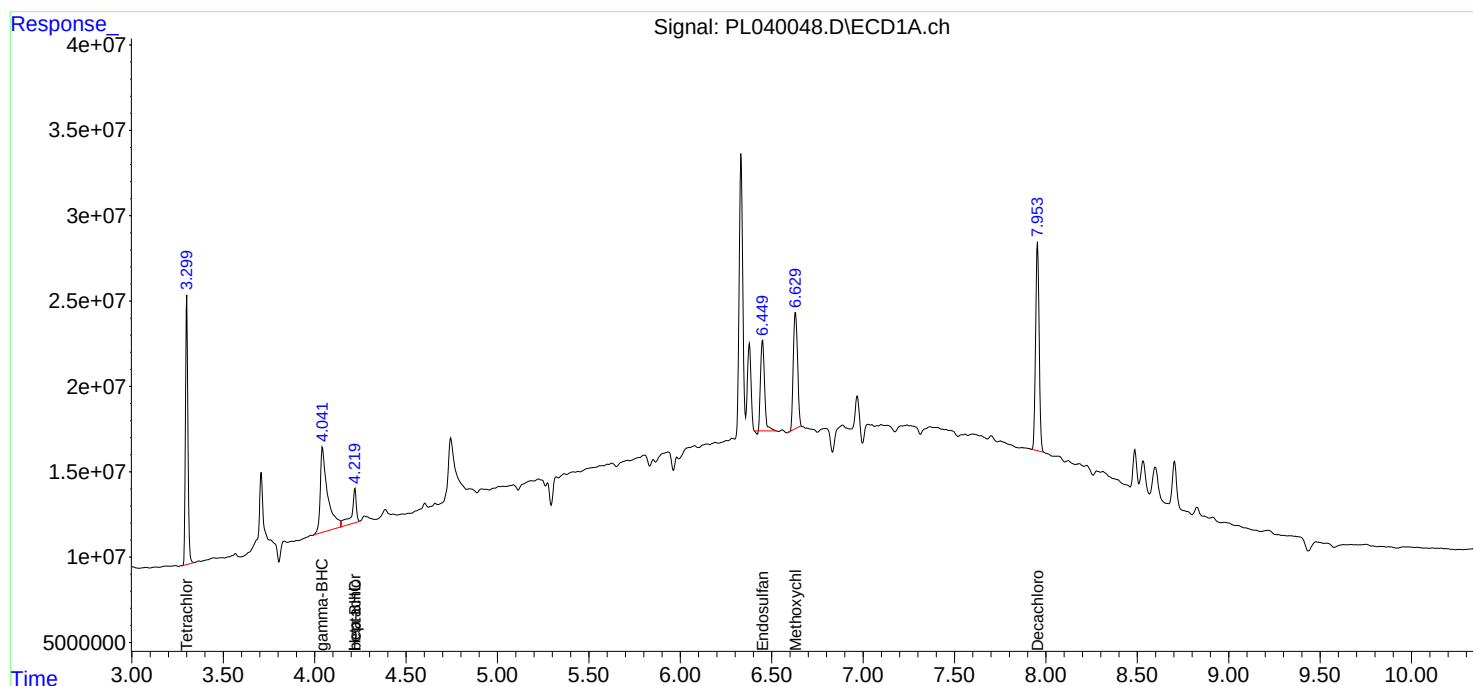


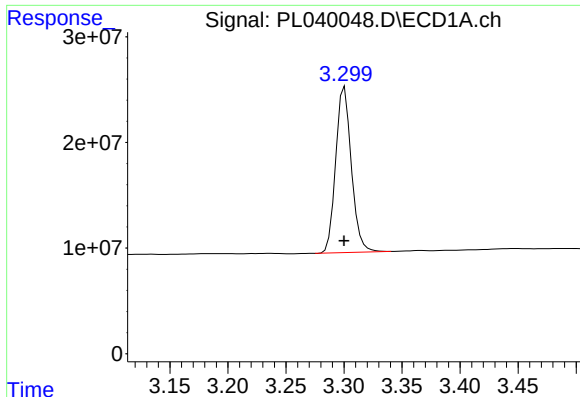

#1 Tetrachloro-m-xylene


R.T.: 3.301 min
Delta R.T.: 0.000 min
Response: 148028476
Conc: 19.09 ng/ml

Instrument :
ECD_L
ClientSampleId :

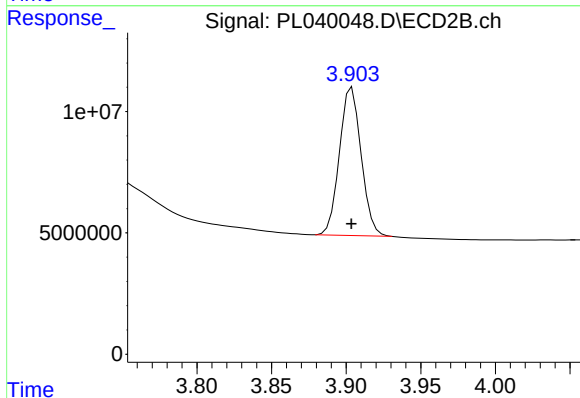


#1 Tetrachloro-m-xylene

R.T.: 3.904 min
Delta R.T.: 0.000 min
Response: 61952724
Conc: 19.42 ng/ml

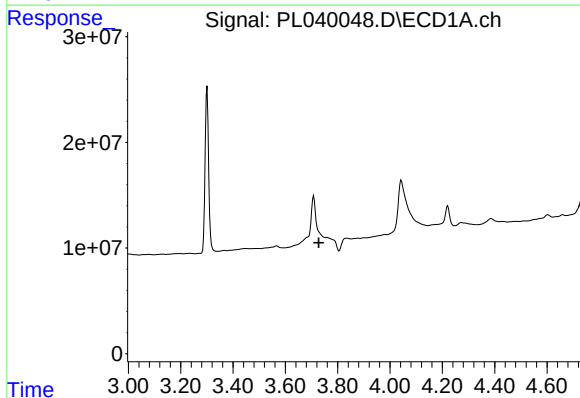


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.727 min
Response: 0
Conc: N.D.

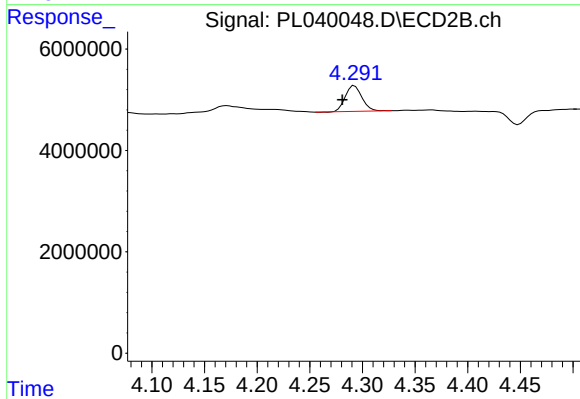

#2 alpha-BHC

R.T.: 4.292 min
Delta R.T.: 0.011 min
Response: 5556402
Conc: 1.07 ng/ml

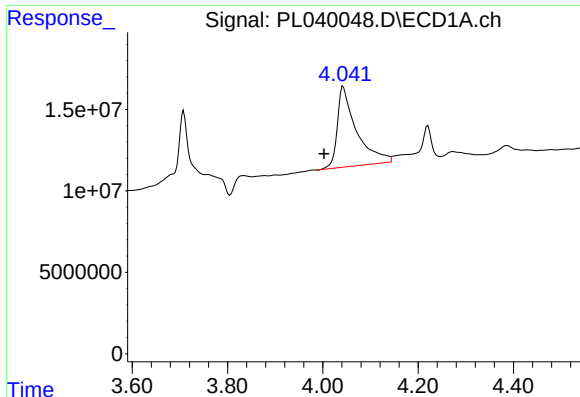

#3 gamma-BHC (Lindane)


R.T.: 4.043 min

Delta R.T.: 0.040 min

Response: 137772711

Conc: 12.04 ng/ml

Instrument :
ECD_L
ClientSampleId :

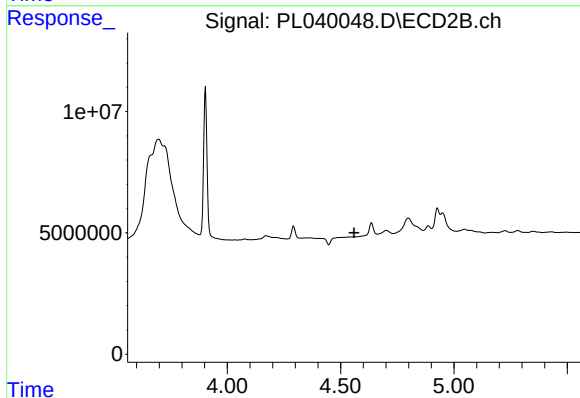


#3 gamma-BHC (Lindane)

R.T.: 0.000 min

Exp R.T. : 4.559 min

Response: 0

Conc: N.D.

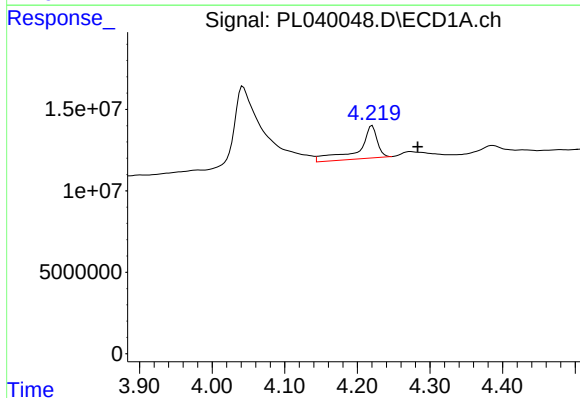


#4 Heptachlor

R.T.: 4.221 min

Delta R.T.: -0.063 min

Response: 35833525

Conc: 3.11 ng/ml

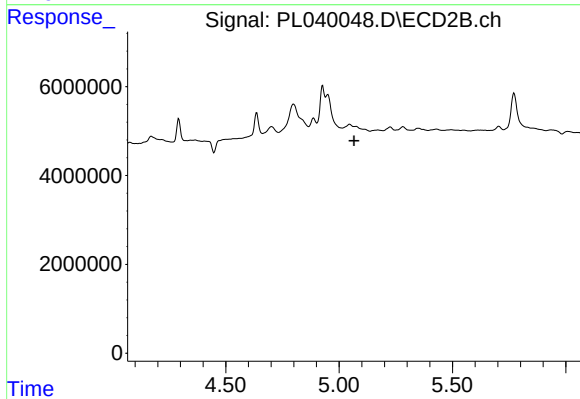


#4 Heptachlor

R.T.: 0.000 min

Exp R.T. : 5.066 min

Response: 0


Conc: N.D.

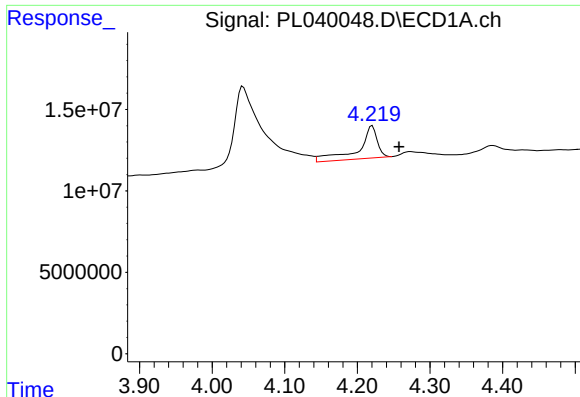

#6 beta-BHC


R.T.: 4.221 min
Delta R.T.: -0.037 min
Response: 35833525
Conc: 7.29 ng/ml

Instrument :
ECD_L
ClientSampleId :

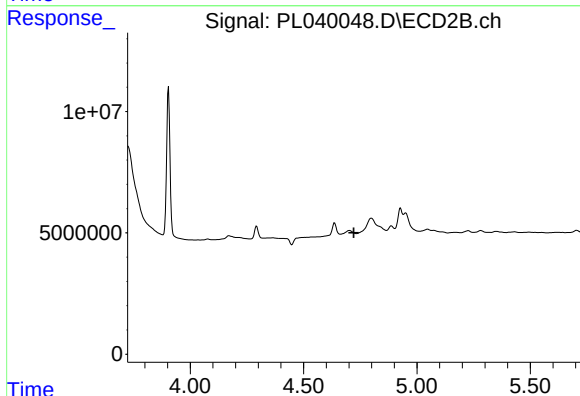


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.722 min
Response: 0
Conc: N.D.

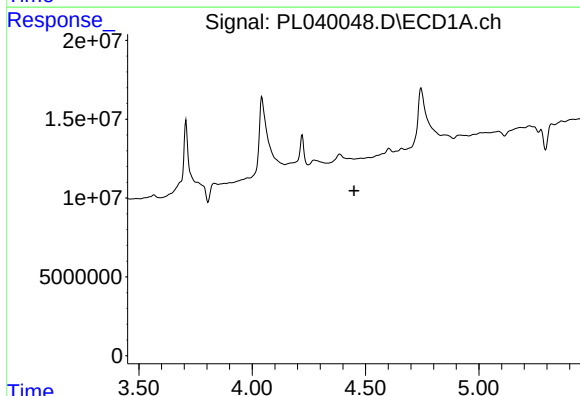


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.449 min
Response: 0
Conc: N.D.

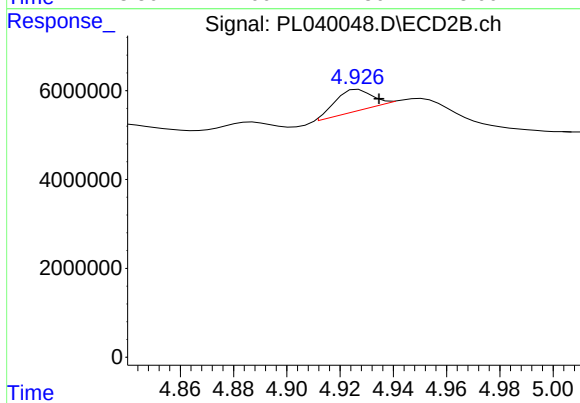

#7 delta-BHC


R.T.: 4.927 min
Delta R.T.: -0.008 min
Response: 4438033
Conc: 1.12 ng/ml

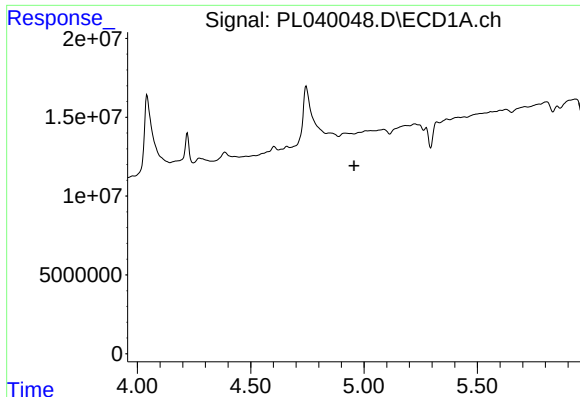

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.956 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

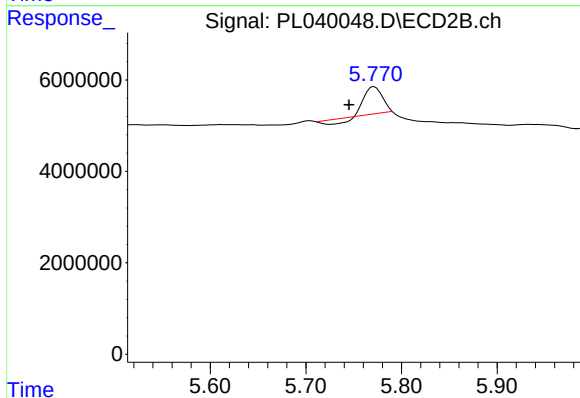


#8 Heptachlor epoxide

R.T.: 5.772 min
Delta R.T.: 0.026 min
Response: 6458769
Conc: 1.63 ng/ml

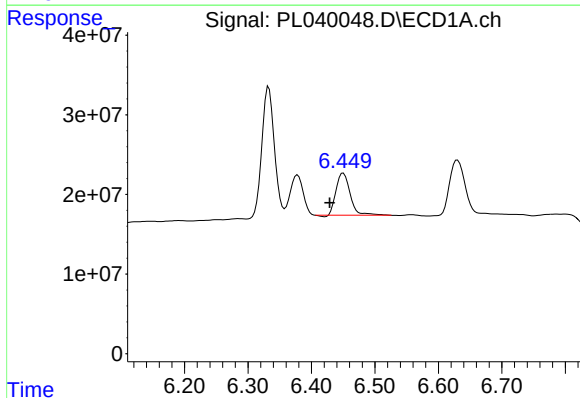


#19 Endosulfan Sulfate

R.T.: 6.450 min
Delta R.T.: 0.021 min
Response: 81088185
Conc: 8.85 ng/ml

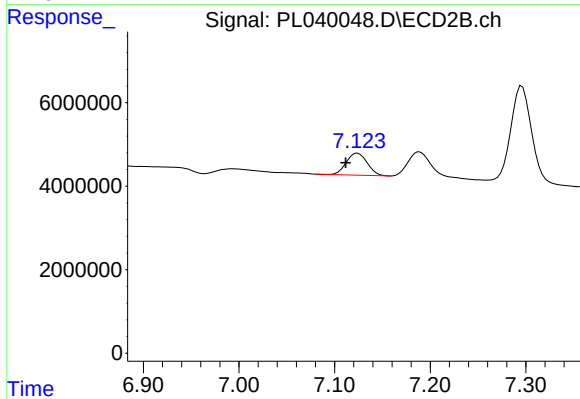

#19 Endosulfan Sulfate


R.T.: 7.124 min
Delta R.T.: 0.012 min
Response: 7938537
Conc: 2.70 ng/ml

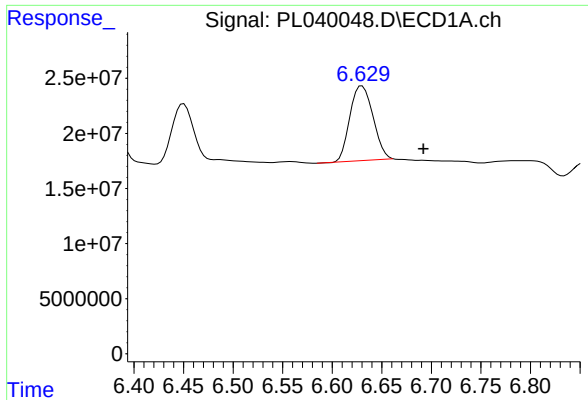

#20 Methoxychlor


R.T.: 6.630 min
Delta R.T.: -0.062 min
Response: 110824060
Conc: 23.91 ng/ml

Instrument :
ECD_L
ClientSampleId :

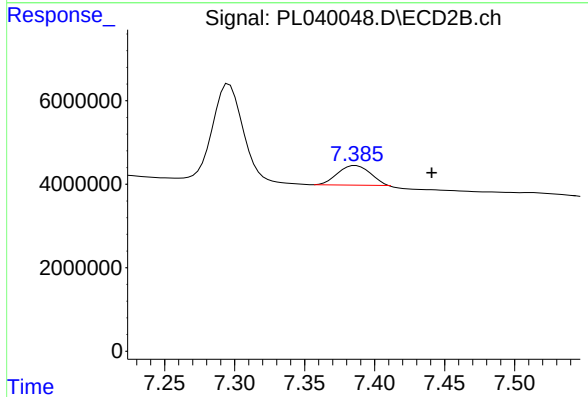


#20 Methoxychlor

R.T.: 7.387 min
Delta R.T.: -0.054 min
Response: 7353721
Conc: 5.02 ng/ml

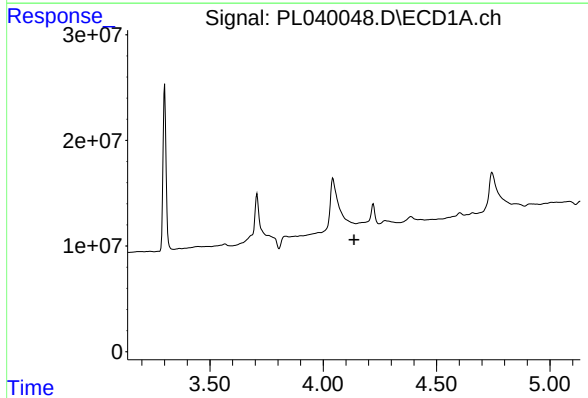


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.136 min
Response: 0
Conc: N.D.

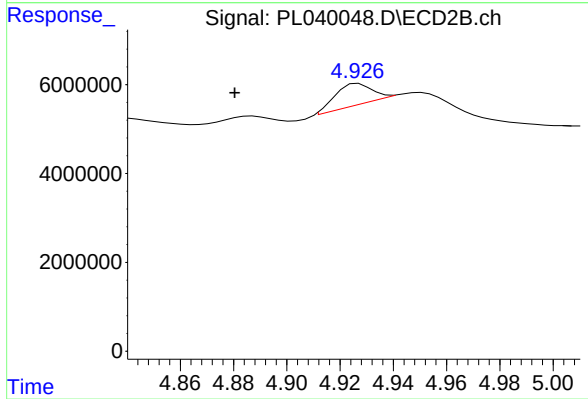

#23 Chlordane-1


R.T.: 4.927 min
Delta R.T.: 0.046 min
Response: 4438033
Conc: 28.66 ng/ml

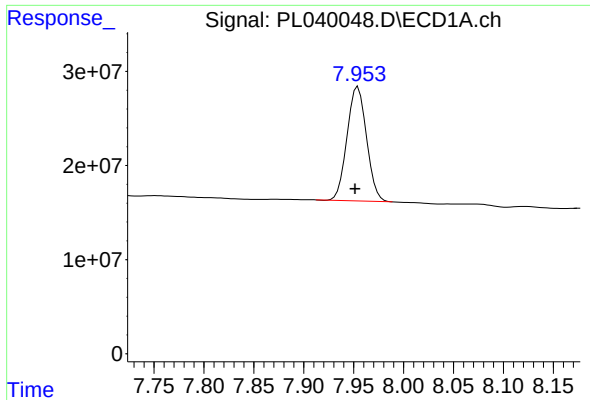

#28 Decachlorobiphenyl

R.T.: 7.954 min
Delta R.T.: 0.003 min
Response: 164931574
Conc: 19.79 ng/ml

Instrument :
ECD_L
ClientSampleId :

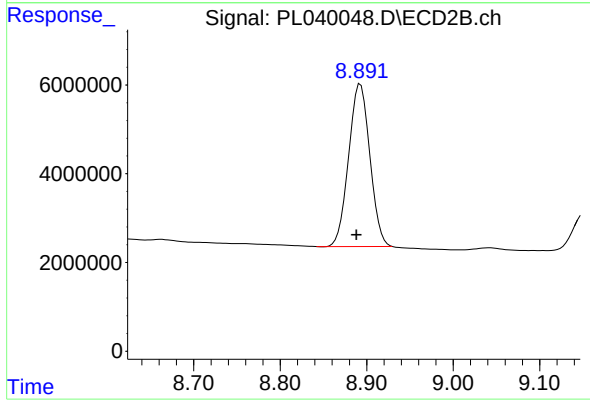

#28 Decachlorobiphenyl

R.T.: 8.893 min
Delta R.T.: 0.005 min
Response: 62348886
Conc: 22.96 ng/ml