

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091718\
 Data File : PL040062.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Sep 2018 07:23
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 18 08:02:38 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 14 23:10:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.300	3.903	144.3E6	61478978	18.604	19.268
28)	SA Decachlor...	7.954	8.890	161.7E6	60410321	19.407	22.242
Target Compounds							
7)	B delta-BHC	0.000	4.950	0	8741990	N.D.	2.198 #
8)	B Heptachlo...	0.000	5.770	0	7324704	N.D.	1.852 #
23)	Chlordane-1	0.000	4.950	0	8741990	N.D.	56.456 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091718\
Data File : PL040062.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Sep 2018 07:23
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 18 08:02:38 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
Quant Title : GC Extractables
QLast Update : Fri Sep 14 23:10:39 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

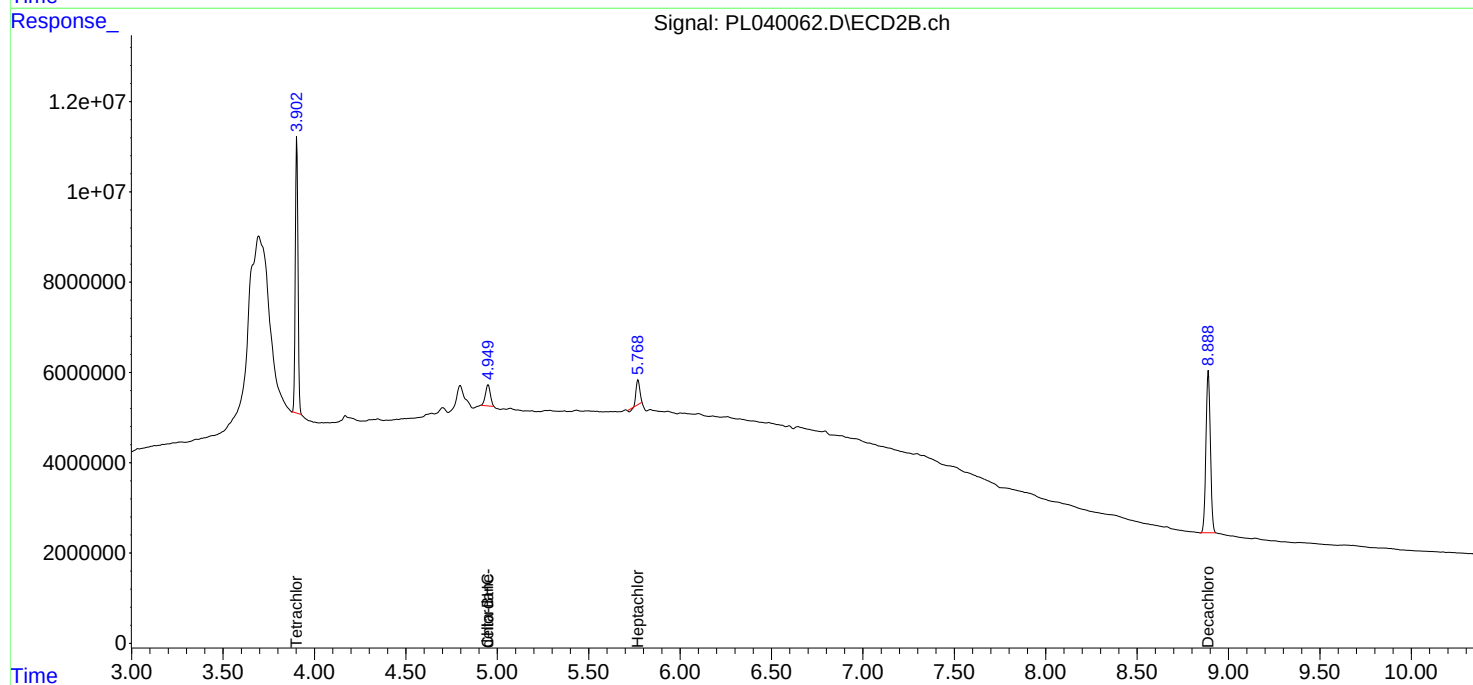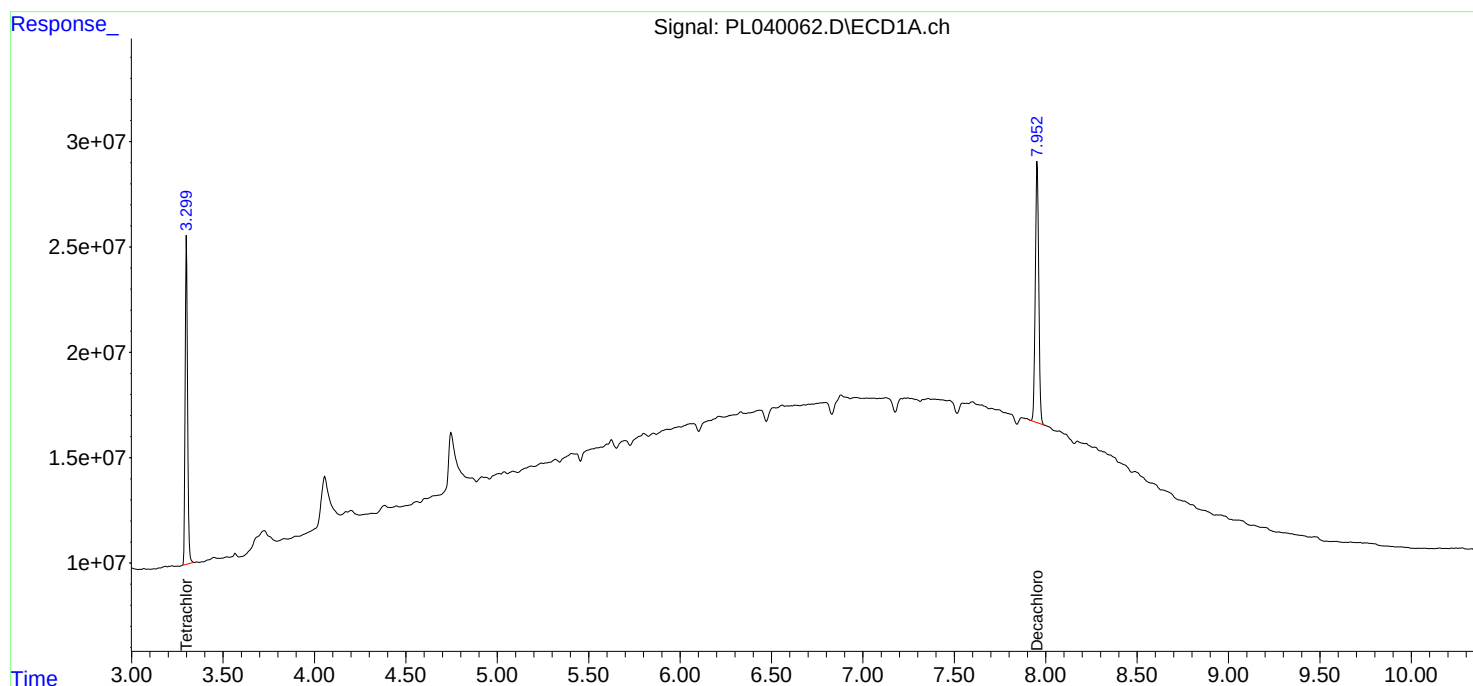


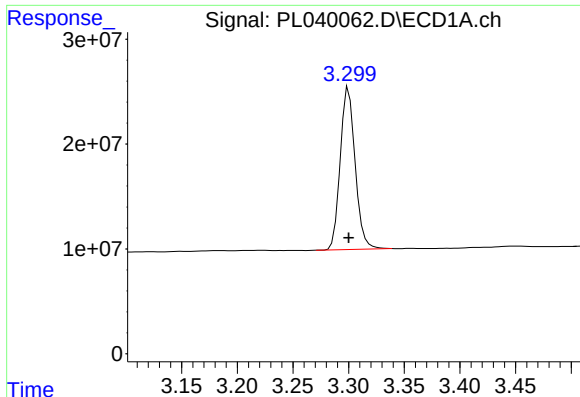

#1 Tetrachloro-m-xylene


R.T.: 3.300 min
Delta R.T.: 0.000 min
Response: 144273894
Conc: 18.60 ng/ml

Instrument :
ECD_L
ClientSampleId :

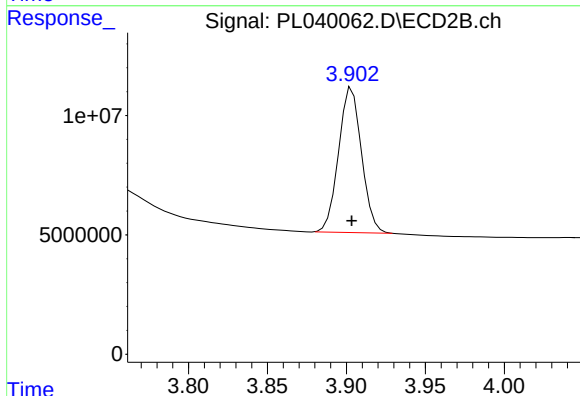


#1 Tetrachloro-m-xylene

R.T.: 3.903 min
Delta R.T.: 0.000 min
Response: 61478978
Conc: 19.27 ng/ml

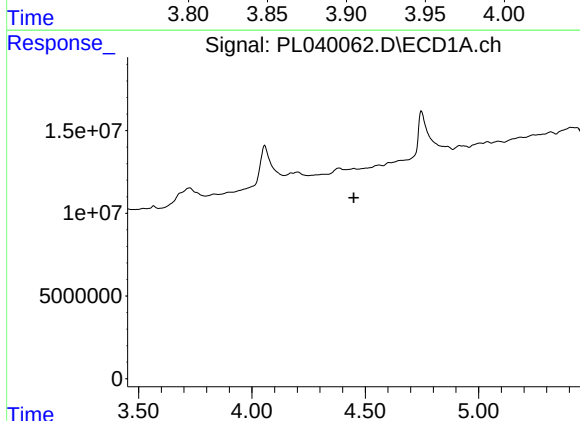


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.449 min
Response: 0
Conc: N.D.

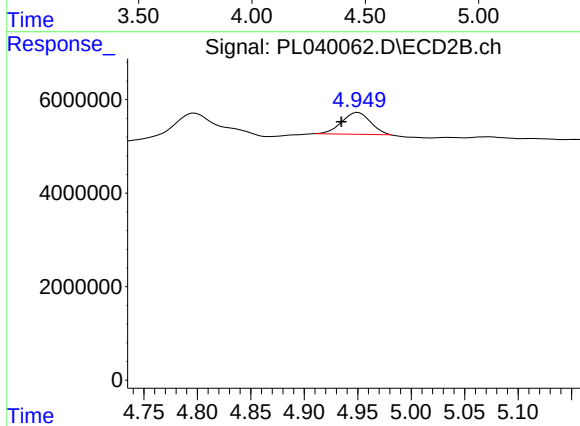

#7 delta-BHC


R.T.: 4.950 min
Delta R.T.: 0.016 min
Response: 8741990
Conc: 2.20 ng/ml

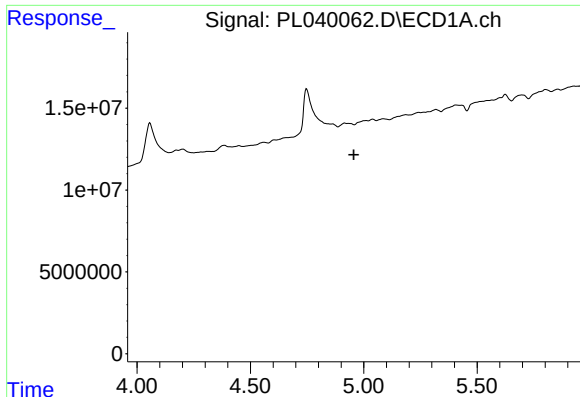

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.956 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

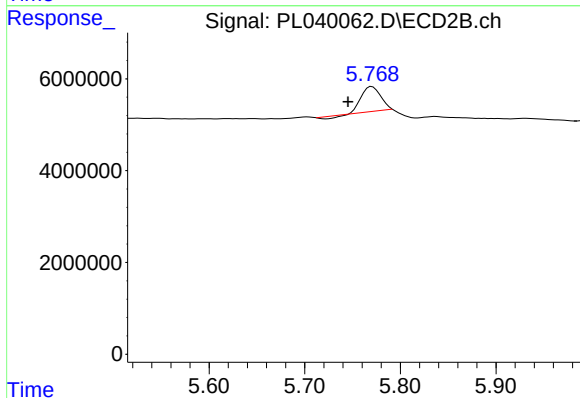


#8 Heptachlor epoxide

R.T.: 5.770 min
Delta R.T.: 0.025 min
Response: 7324704
Conc: 1.85 ng/ml

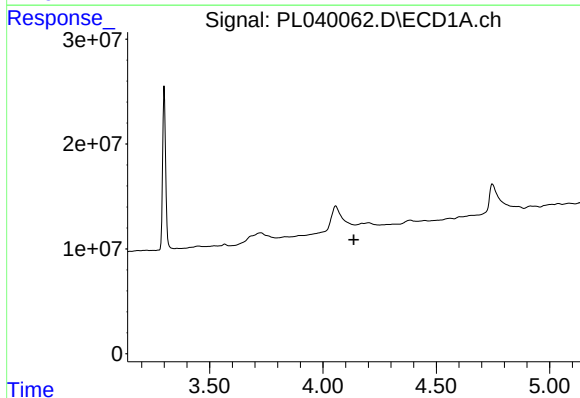


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.136 min
Response: 0
Conc: N.D.

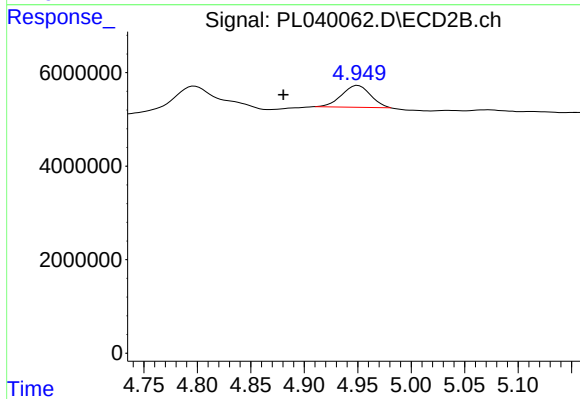

#23 Chlordane-1


R.T.: 4.950 min
Delta R.T.: 0.070 min
Response: 8741990
Conc: 56.46 ng/ml

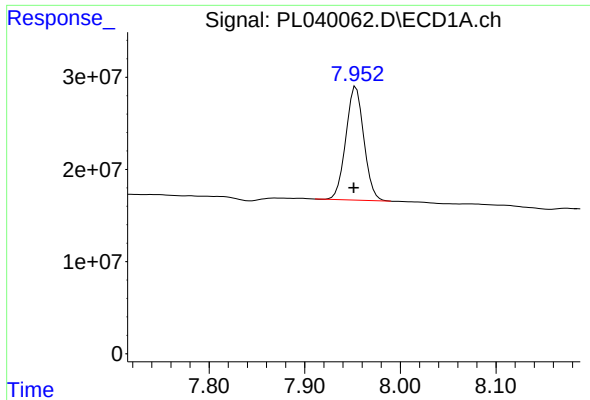

#28 Decachlorobiphenyl

R.T.: 7.954 min
Delta R.T.: 0.002 min
Response: 161708920
Conc: 19.41 ng/ml

Instrument :
ECD_L
ClientSampleId :

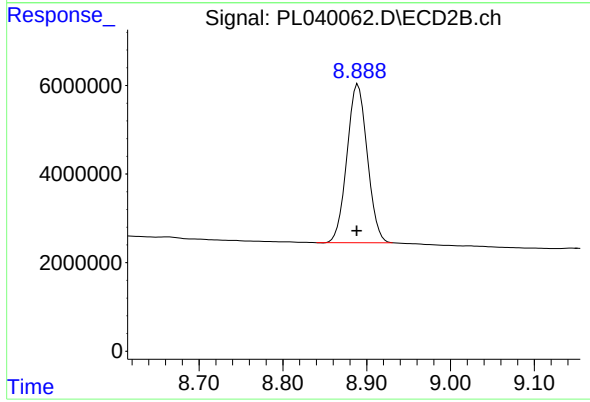

#28 Decachlorobiphenyl

R.T.: 8.890 min
Delta R.T.: 0.002 min
Response: 60410321
Conc: 22.24 ng/ml