

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091719\
 Data File : PL052506.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Sep 2019 17:18
 Operator : SG\AJ
 Sample : K4878-22
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TPA-9

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 18 00:59:48 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091719.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 17 11:25:25 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.553	4.046	153.8E6	44255083	19.729	20.310
28)	SA Decachlor...	8.355	9.120	161.4E6	53271285	18.459	22.246
Target Compounds							
3)	MA gamma-BHC...	0.000	4.701f	0	1487800	N.D.	0.515 #
4)	MA Heptachlor	0.000	5.208f	0	4032456	N.D.	1.374 #
6)	B beta-BHC	4.507f	4.905f	12230510	2228927	2.499	1.671 #
7)	B delta-BHC	0.000	5.085f	0	5507659	N.D.	1.924 #
10)	B gamma-Chl...	0.000	6.141	0	1146391	N.D.	0.451 #
14)	MA Endrin	0.000	6.783f	0	38960	N.D.	0.020 #
23)	Chlordane-1	0.000	5.024f	0	70478	N.D.	0.908 #
25)	Chlordane-3	0.000	6.141f	0	1146391	N.D.	3.747 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091719\
Data File : PL052506.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Sep 2019 17:18
Operator : SG\AJ
Sample : K4878-22
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TPA-9

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 18 00:59:48 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091719.M
Quant Title : GC Extractables
QLast Update : Tue Sep 17 11:25:25 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm




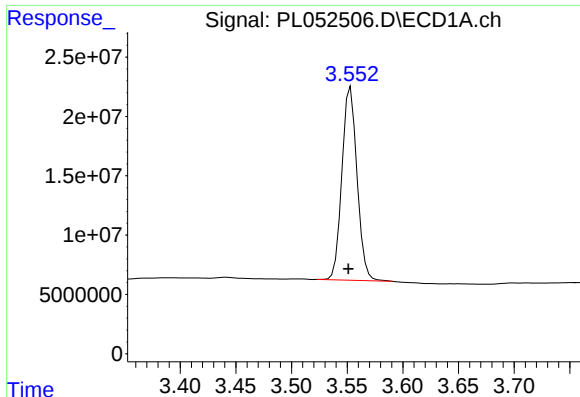

#1 Tetrachloro-m-xylene


R.T.: 3.553 min
Delta R.T.: 0.002 min
Response: 153839041
Conc: 19.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
TPA-9

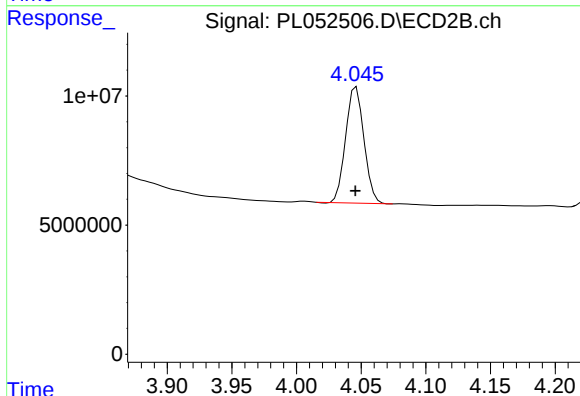


#1 Tetrachloro-m-xylene

R.T.: 4.046 min
Delta R.T.: 0.000 min
Response: 44255083
Conc: 20.31 ng/ml

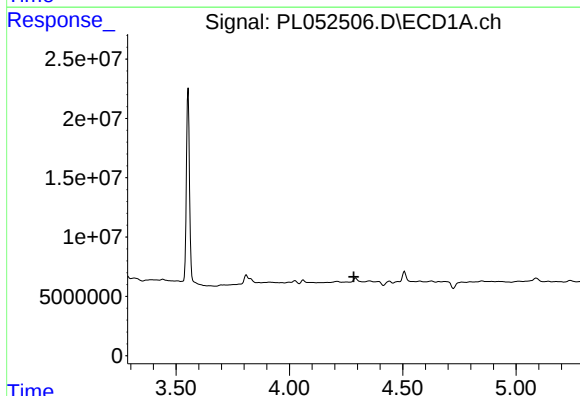


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.284 min
Response: 0
Conc: N.D.

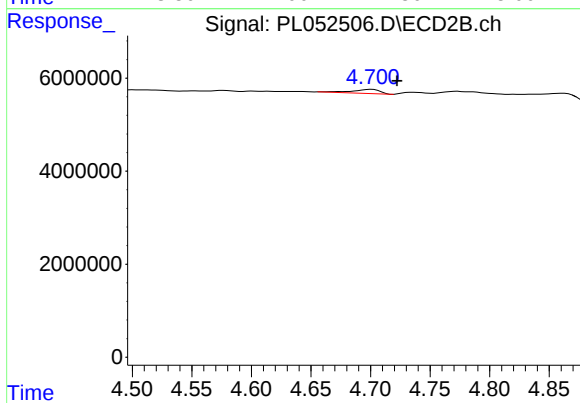

#3 gamma-BHC (Lindane)


R.T.: 4.701 min
Delta R.T.: -0.021 min
Response: 1487800
Conc: 0.52 ng/ml

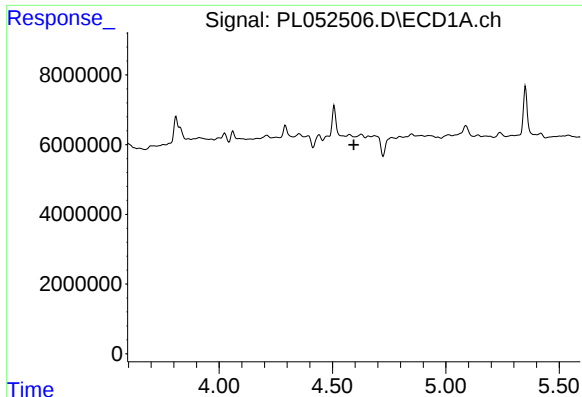

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.594 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TPA-9

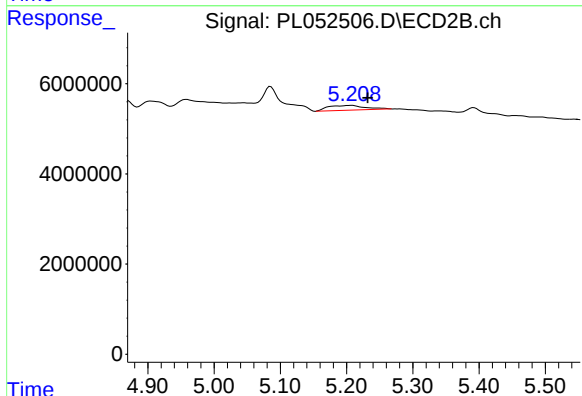


#4 Heptachlor

R.T.: 5.208 min
Delta R.T.: -0.023 min
Response: 4032456
Conc: 1.37 ng/ml

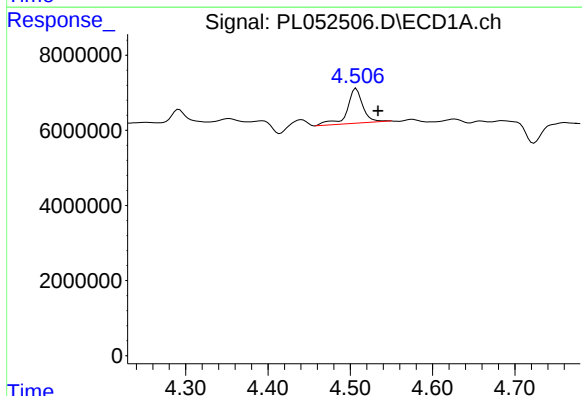


#6 beta-BHC

R.T.: 4.507 min
Delta R.T.: -0.026 min
Response: 12230510
Conc: 2.50 ng/ml

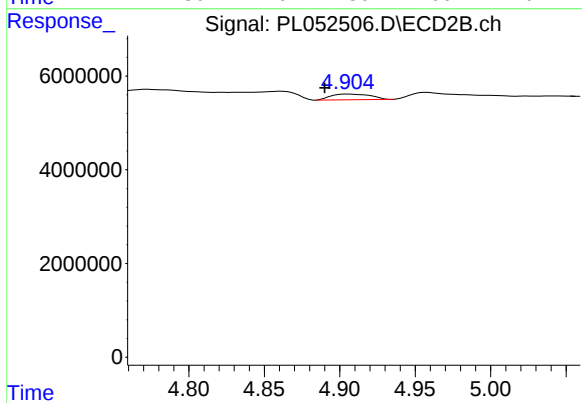

#6 beta-BHC


R.T.: 4.905 min
Delta R.T.: 0.015 min
Response: 2228927
Conc: 1.67 ng/ml

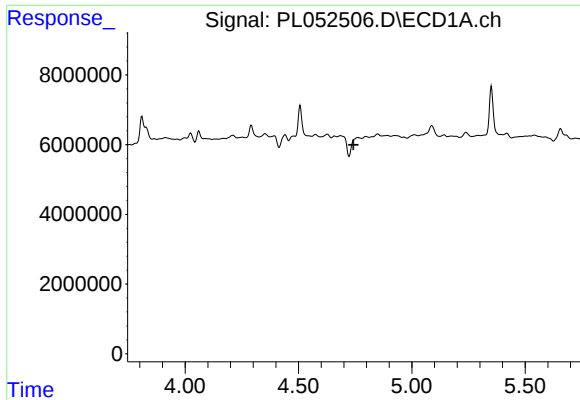

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.743 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TPA-9

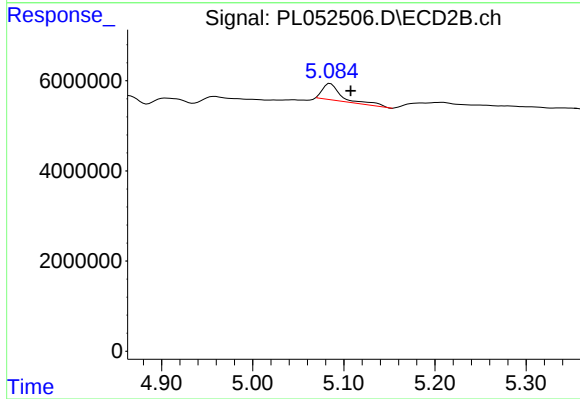


#7 delta-BHC

R.T.: 5.085 min
Delta R.T.: -0.022 min
Response: 5507659
Conc: 1.92 ng/ml

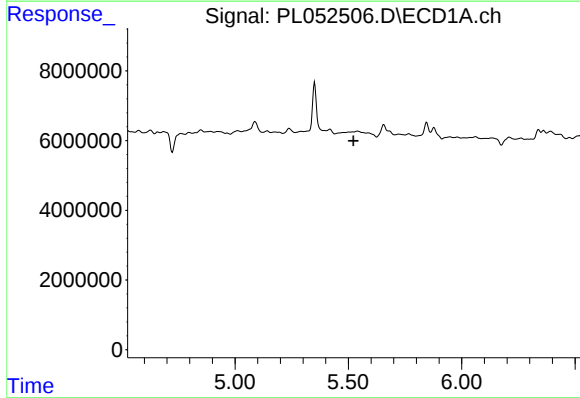


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.523 min
Response: 0
Conc: N.D.

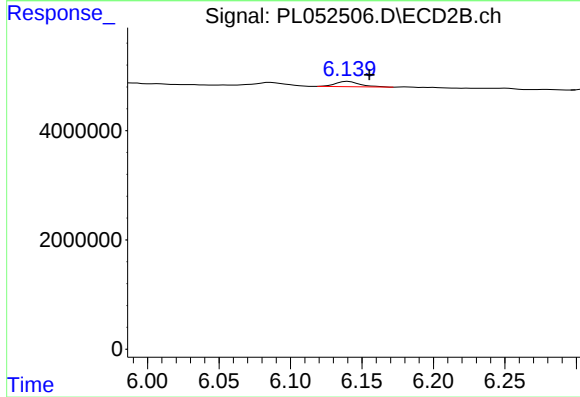

#10 gamma-Chlordane


R.T.: 6.141 min
Delta R.T.: -0.015 min
Response: 1146391
Conc: 0.45 ng/ml

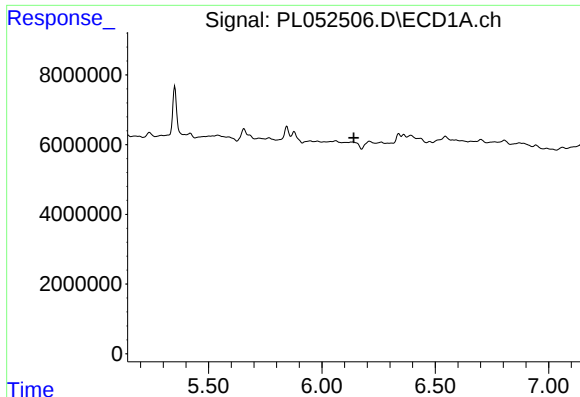

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.140 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TPA-9

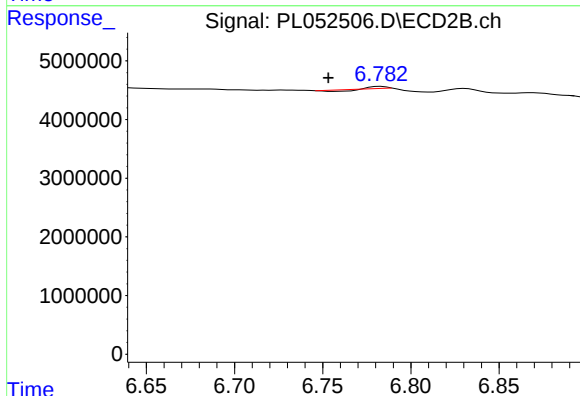


#14 Endrin

R.T.: 6.783 min
Delta R.T.: 0.030 min
Response: 38960
Conc: 0.02 ng/ml

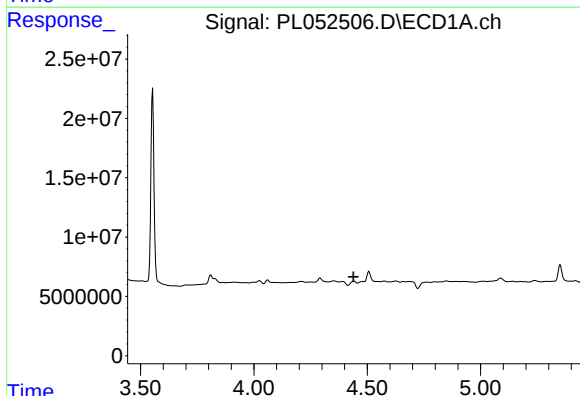


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 4.440 min
Response: 0
Conc: N.D.

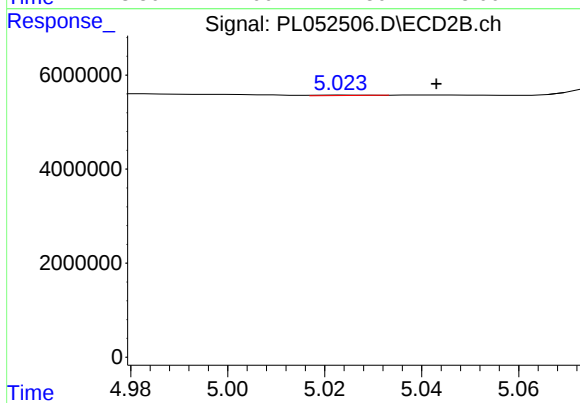

#23 Chlordane-1

R.T.: 5.024 min
Delta R.T.: -0.019 min
Response: 70478
Conc: 0.91 ng/ml

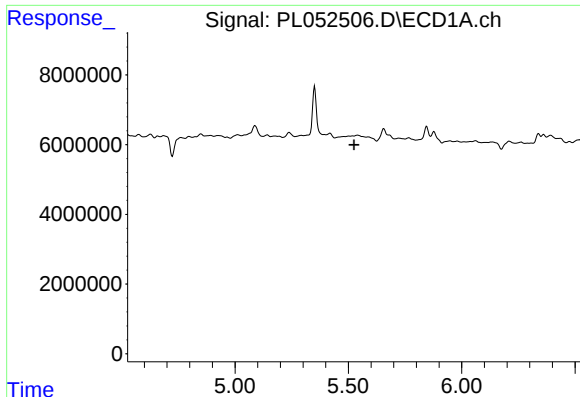

#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.525 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TPA-9

#25 Chlordane-3

R.T.: 6.141 min
Delta R.T.: -0.015 min
Response: 1146391
Conc: 3.75 ng/ml

#28 Decachlorobiphenyl

R.T.: 8.355 min
Delta R.T.: 0.000 min
Response: 161419731
Conc: 18.46 ng/ml

#28 Decachlorobiphenyl

R.T.: 9.120 min
Delta R.T.: 0.001 min
Response: 53271285
Conc: 22.25 ng/ml