

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091719\
 Data File : PL052520.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Sep 2019 20:41
 Operator : SG\AJ
 Sample : K4866-06
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SUMP-PIT

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 18 01:02:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091719.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 17 11:25:25 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.552	4.046	135.5E6	40514510	17.373	18.594
28)	SA Decachlor...	8.354	9.120	147.9E6	48244181	16.910	20.147
Target Compounds							
3)	MA gamma-BHC...	0.000	4.739f	0	654899	N.D.	0.227 #
4)	MA Heptachlor	0.000	5.231	0	28118399	N.D.	9.581 #
5)	MB Aldrin	0.000	5.520f	0	805846	N.D.	0.304 #
7)	B delta-BHC	0.000	5.086f	0	2904516	N.D.	1.015 #
8)	B Heptachlo...	0.000	5.902f	0	4105234	N.D.	1.565 #
14)	MA Endrin	0.000	6.767	0	2241473	N.D.	1.158 #
18)	B Endrin al...	0.000	7.072	0	1568780	N.D.	0.846 #
24)	Chlordane-2	0.000	5.520	0	805846	N.D.	9.826 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091719\
Data File : PL052520.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Sep 2019 20:41
Operator : SG\AJ
Sample : K4866-06
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
SUMP-PIT

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 18 01:02:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091719.M
Quant Title : GC Extractables
QLast Update : Tue Sep 17 11:25:25 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

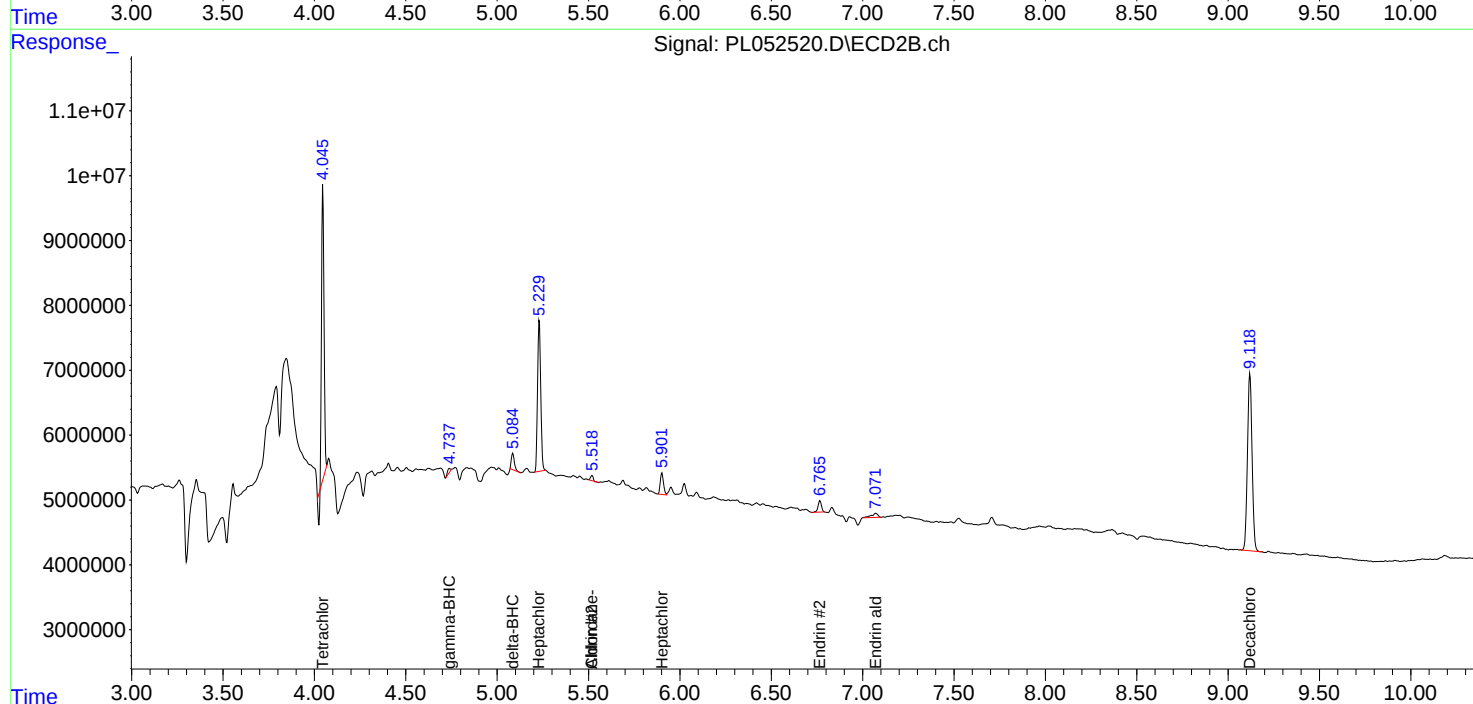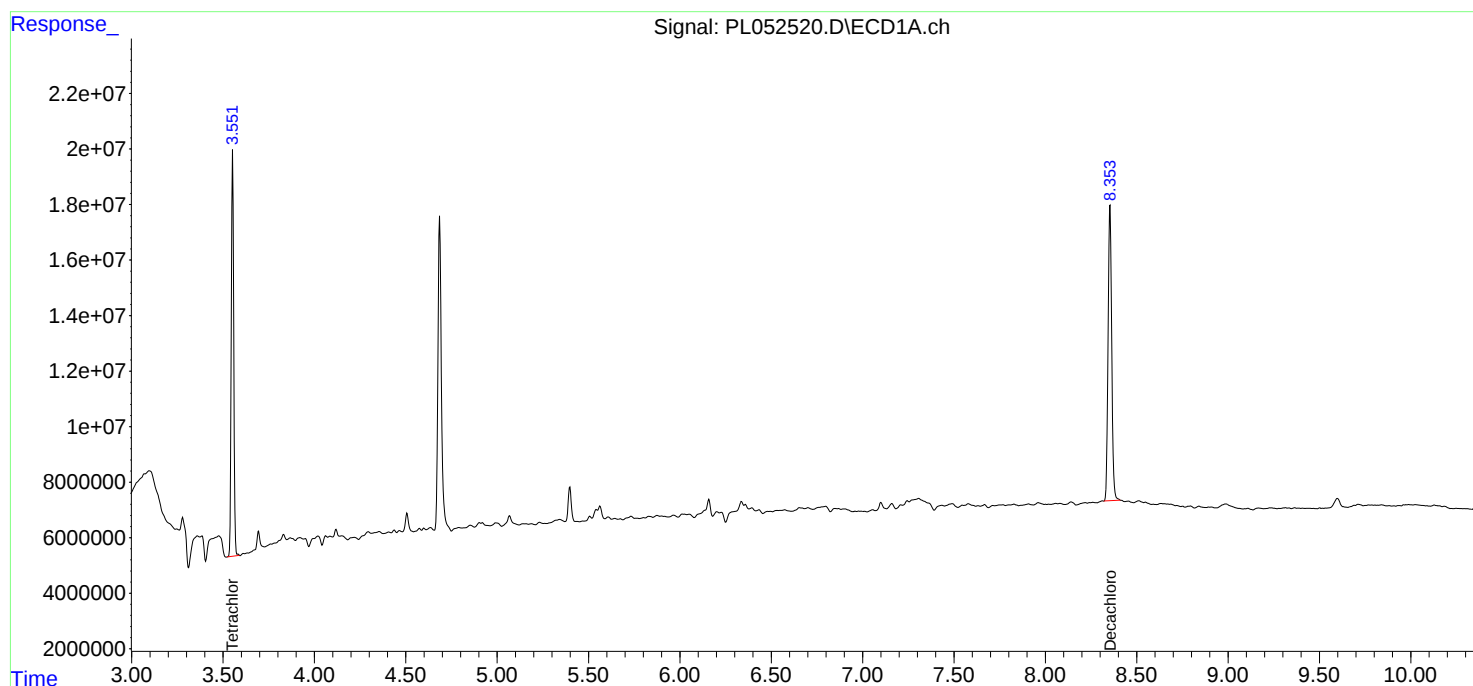


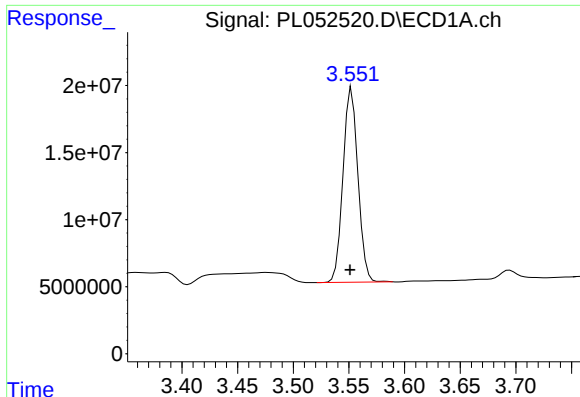

#1 Tetrachloro-m-xylene


R.T.: 3.552 min
Delta R.T.: 0.001 min
Response: 135467241
Conc: 17.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
SUMP-PIT

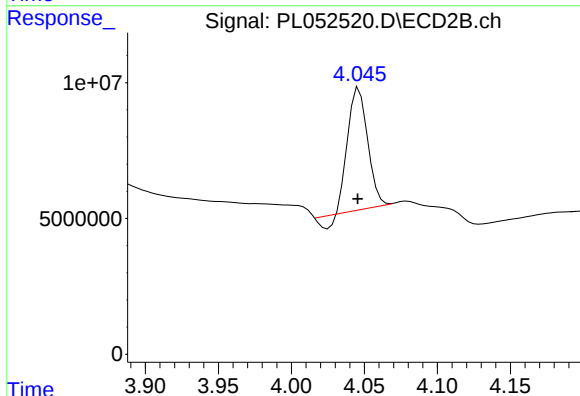


#1 Tetrachloro-m-xylene

R.T.: 4.046 min
Delta R.T.: 0.000 min
Response: 40514510
Conc: 18.59 ng/ml

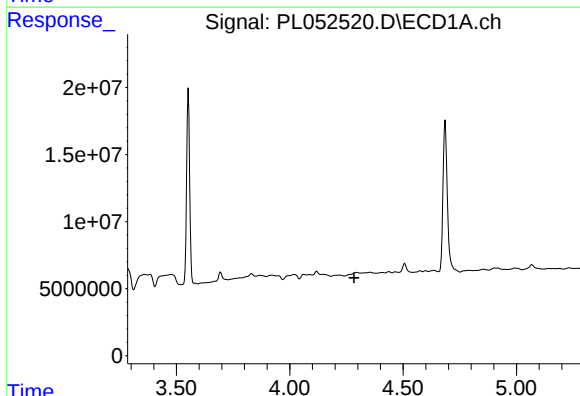


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.284 min
Response: 0
Conc: N.D.

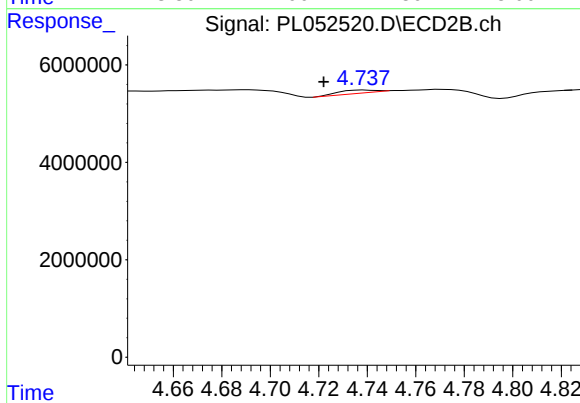

#3 gamma-BHC (Lindane)


R.T.: 4.739 min
Delta R.T.: 0.017 min
Response: 654899
Conc: 0.23 ng/ml

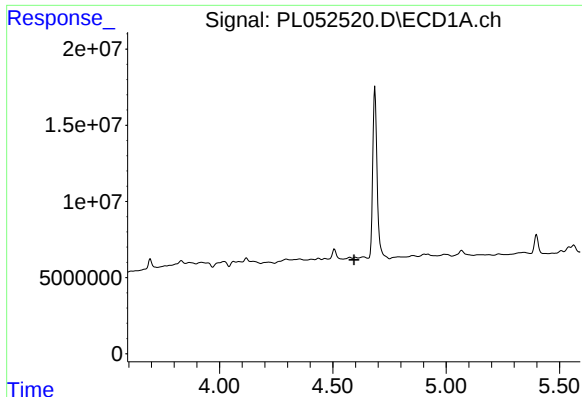

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 4.594 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
SUMP-PIT

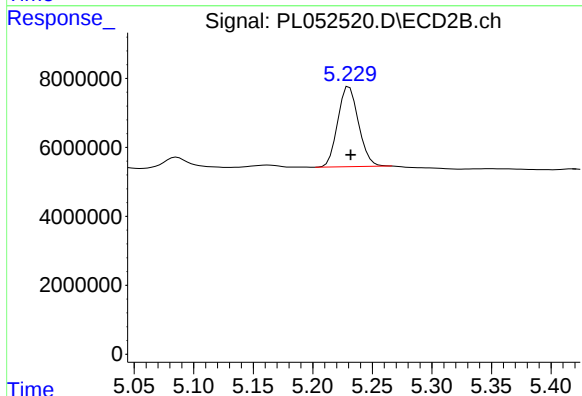


#4 Heptachlor

R.T.: 5.231 min
Delta R.T.: -0.001 min
Response: 28118399
Conc: 9.58 ng/ml

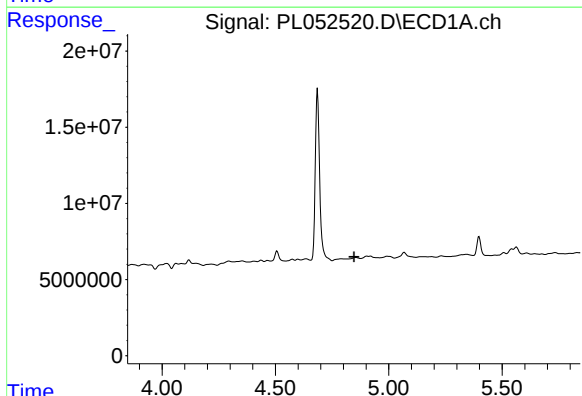


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.847 min
Response: 0
Conc: N.D.

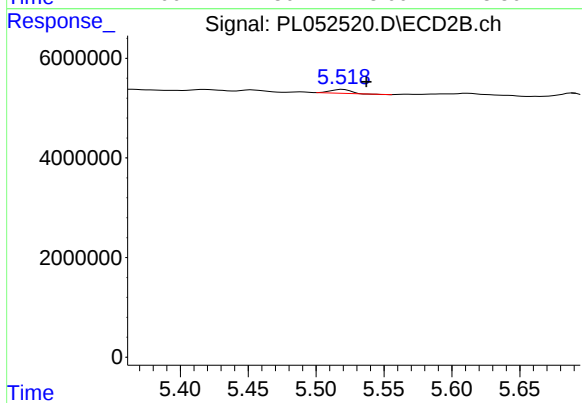

#5 Aldrin


R.T.: 5.520 min
Delta R.T.: -0.017 min
Response: 805846
Conc: 0.30 ng/ml

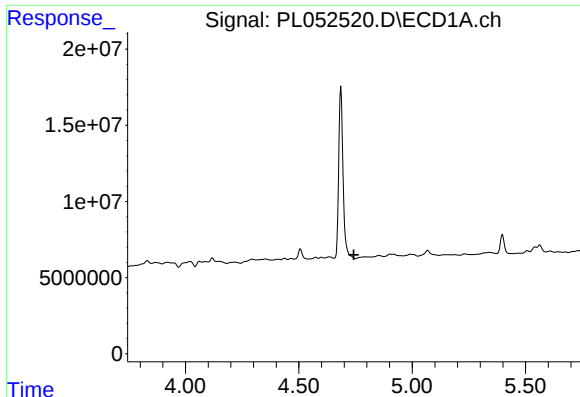

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.743 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
SUMP-PIT

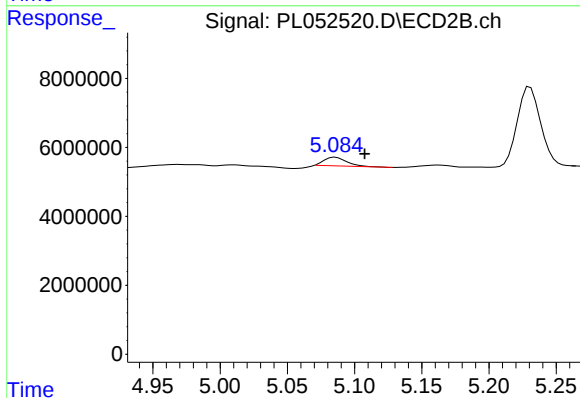


#7 delta-BHC

R.T.: 5.086 min
Delta R.T.: -0.022 min
Response: 2904516
Conc: 1.01 ng/ml

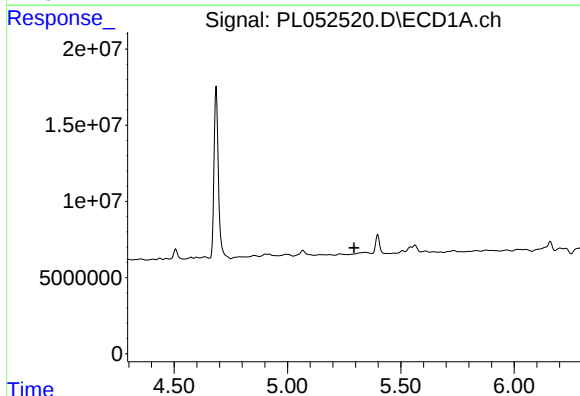


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.293 min
Response: 0
Conc: N.D.

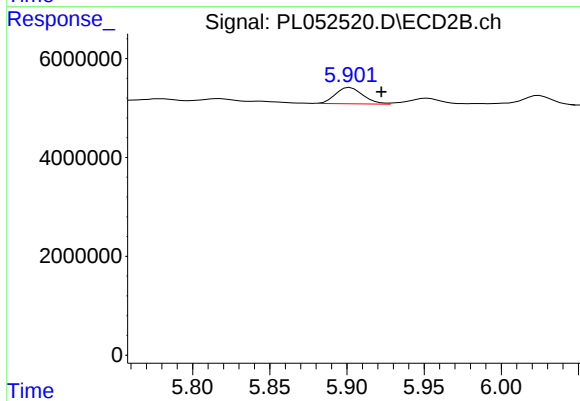

#8 Heptachlor epoxide


R.T.: 5.902 min
Delta R.T.: -0.020 min
Response: 4105234
Conc: 1.57 ng/ml

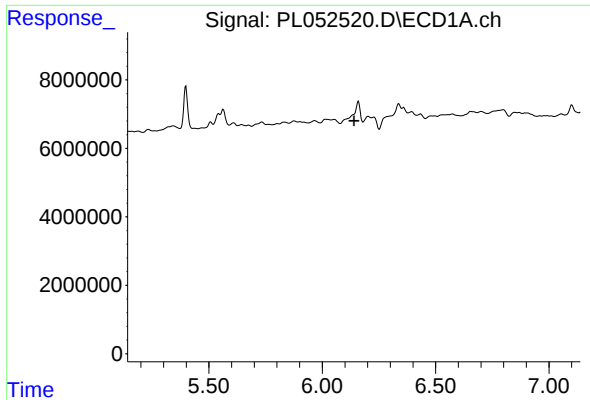

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.140 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
SUMP-PIT

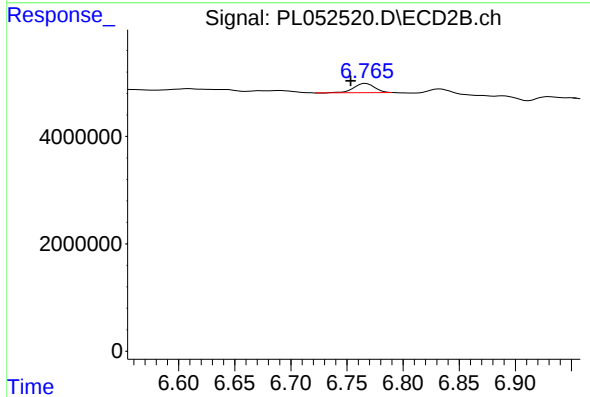


#14 Endrin

R.T.: 6.767 min
Delta R.T.: 0.014 min
Response: 2241473
Conc: 1.16 ng/ml

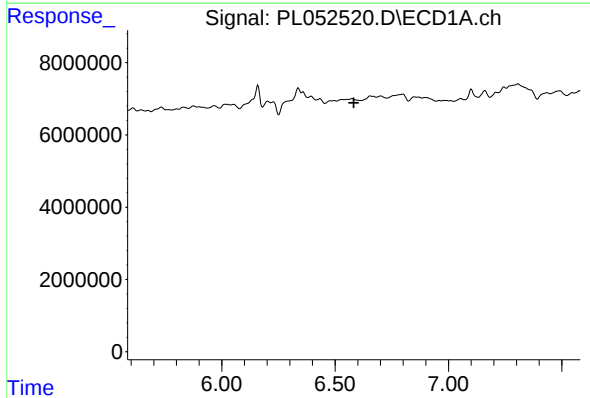


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.583 min
Response: 0
Conc: N.D.

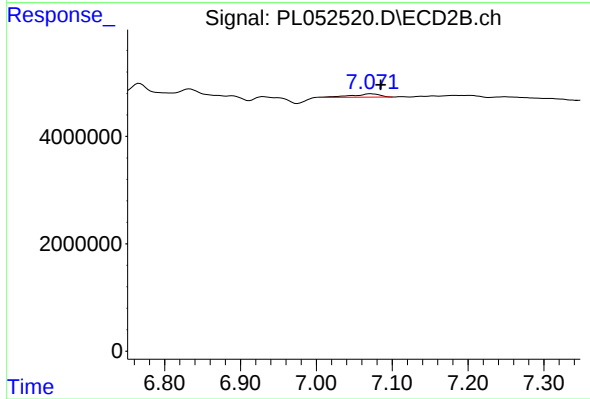

#18 Endrin aldehyde


R.T.: 7.072 min
Delta R.T.: -0.013 min
Response: 1568780
Conc: 0.85 ng/ml

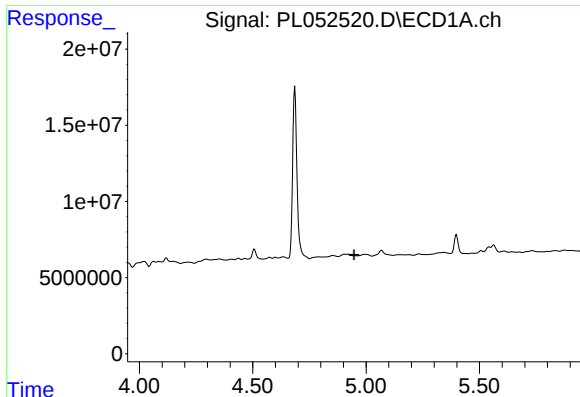

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.948 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
SUMP-PIT

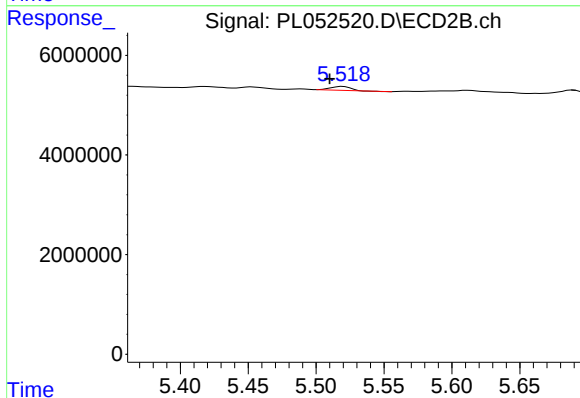


#24 Chlordane-2

R.T.: 5.520 min
Delta R.T.: 0.010 min
Response: 805846
Conc: 9.83 ng/ml

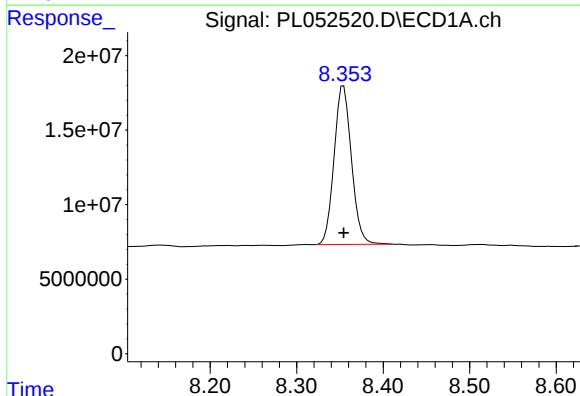

#28 Decachlorobiphenyl

R.T.: 8.354 min
Delta R.T.: 0.000 min
Response: 147868554
Conc: 16.91 ng/ml

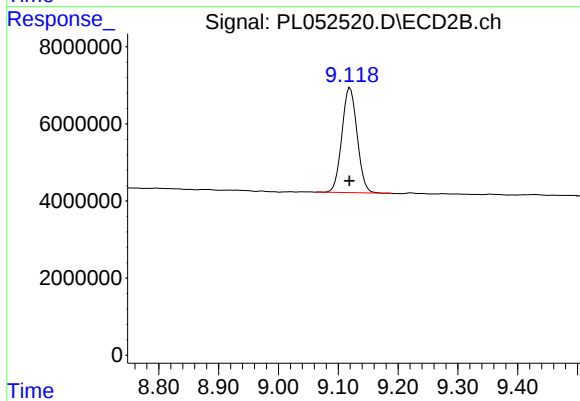

#28 Decachlorobiphenyl

R.T.: 9.120 min
Delta R.T.: 0.001 min
Response: 48244181
Conc: 20.15 ng/ml