

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091719\
 Data File : PL052484.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Sep 2019 10:58
 Operator : SG\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 17 11:22:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091719.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 17 11:22:31 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.552	4.046	472.1E6	105.5E6	50.000	50.000
28)	SA Decachlor...	8.356	9.120	428.5E6	115.3E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.440	5.043	134.5E6	38823097	500.000	500.000
24)	Chlordane-2	4.948	5.510	152.1E6	41005283	500.000	500.000
25)	Chlordane-3	5.525	6.156	483.7E6	153.0E6	500.000	500.000
26)	Chlordane-4	5.583	6.230	393.5E6	192.3E6	500.000	500.000
27)	Chlordane-5	6.426	7.035	154.0E6	32021324	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091719\
Data File : PL052484.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Sep 2019 10:58
Operator : SG\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 11:22:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091719.M
Quant Title : GC Extractables
QLast Update : Tue Sep 17 11:22:31 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

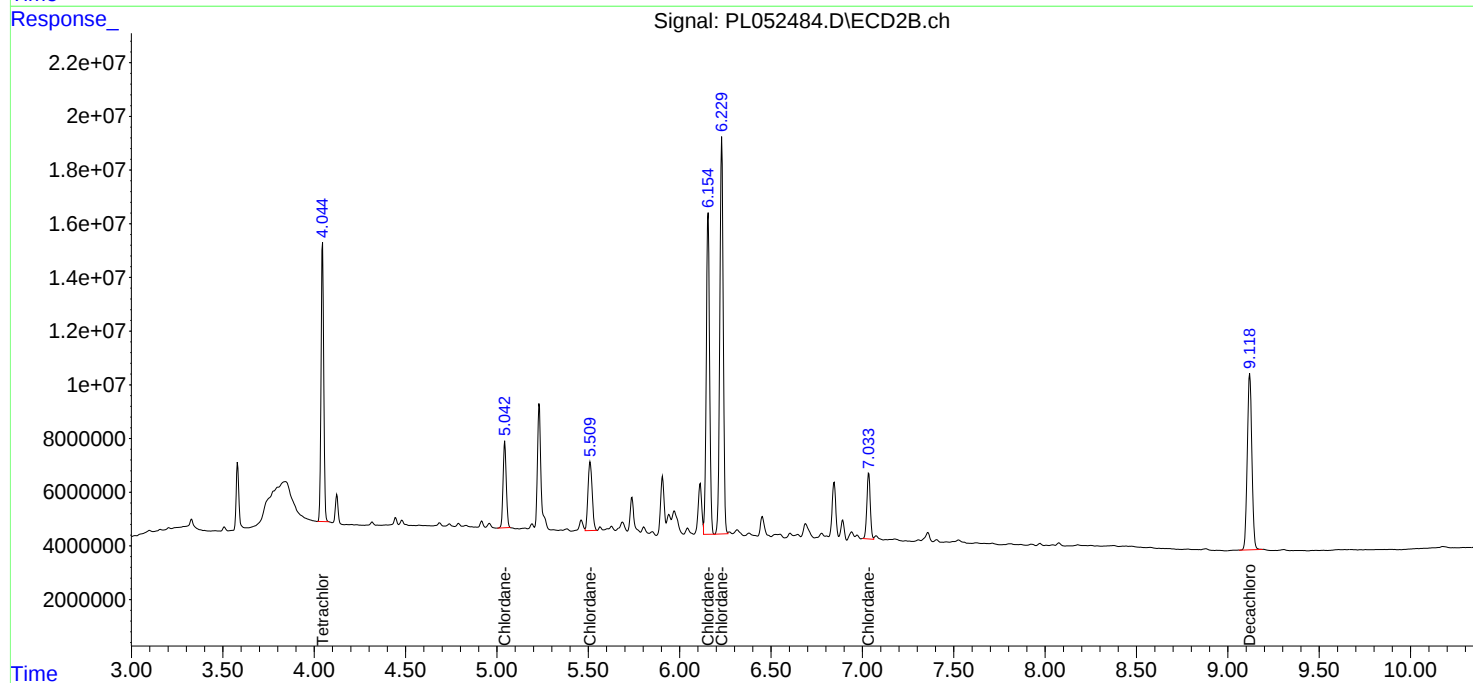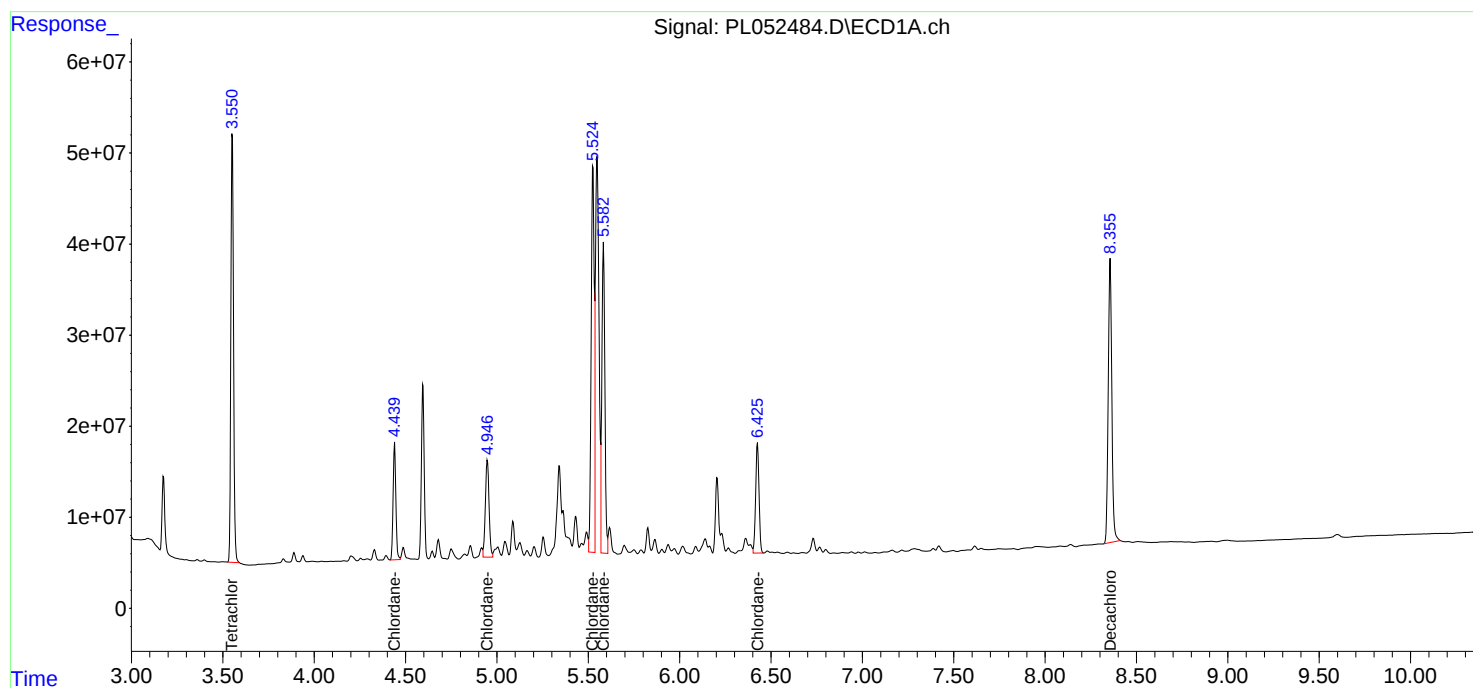


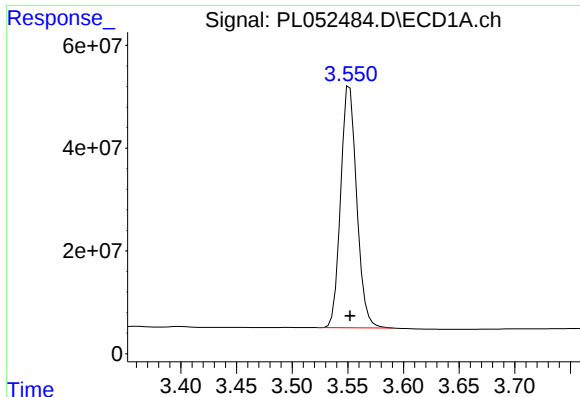

#1 Tetrachloro-m-xylene


R.T.: 3.552 min
Delta R.T.: 0.000 min
Response: 472108971
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

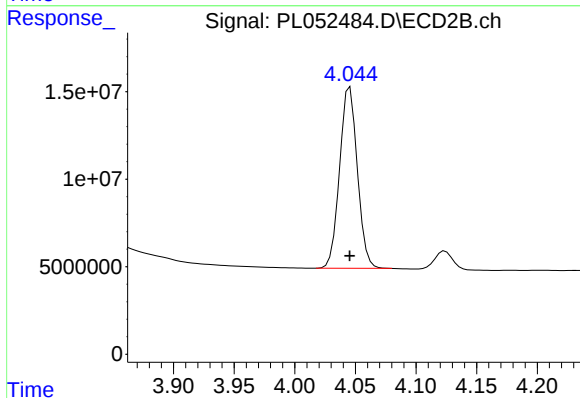


#1 Tetrachloro-m-xylene

R.T.: 4.046 min
Delta R.T.: 0.000 min
Response: 105466989
Conc: 50.00 ng/ml

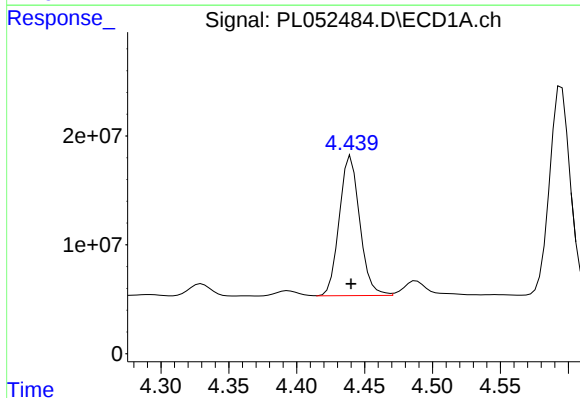


#23 Chlordane-1

R.T.: 4.440 min
Delta R.T.: 0.000 min
Response: 134506578
Conc: 500.00 ng/ml

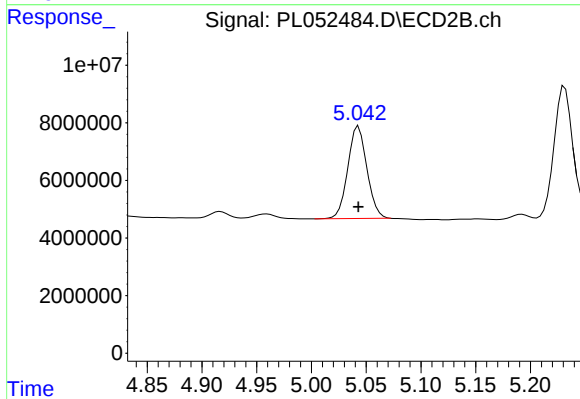

#23 Chlordane-1


R.T.: 5.043 min
Delta R.T.: 0.000 min
Response: 38823097
Conc: 500.00 ng/ml

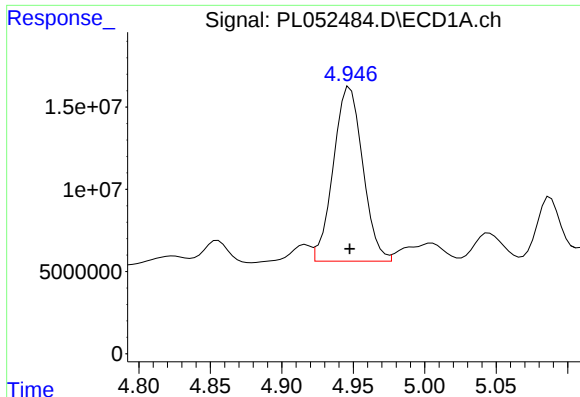

#24 Chlordane-2


R.T.: 4.948 min
Delta R.T.: 0.000 min
Response: 152067644
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

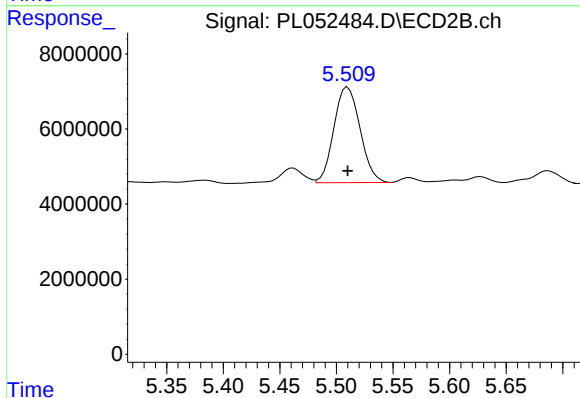


#24 Chlordane-2

R.T.: 5.510 min
Delta R.T.: 0.000 min
Response: 41005283
Conc: 500.00 ng/ml

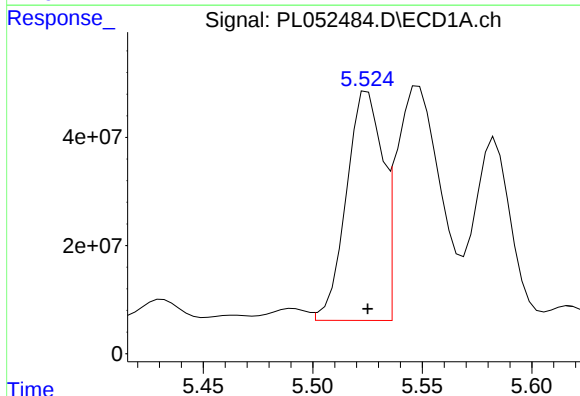


#25 Chlordane-3

R.T.: 5.525 min
Delta R.T.: 0.000 min
Response: 483729241
Conc: 500.00 ng/ml

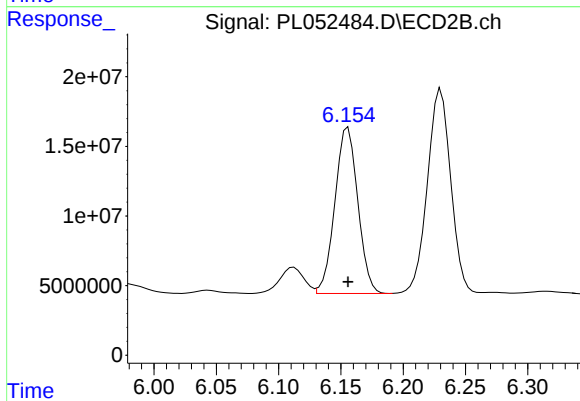

#25 Chlordane-3


R.T.: 6.156 min
Delta R.T.: 0.000 min
Response: 152984530
Conc: 500.00 ng/ml

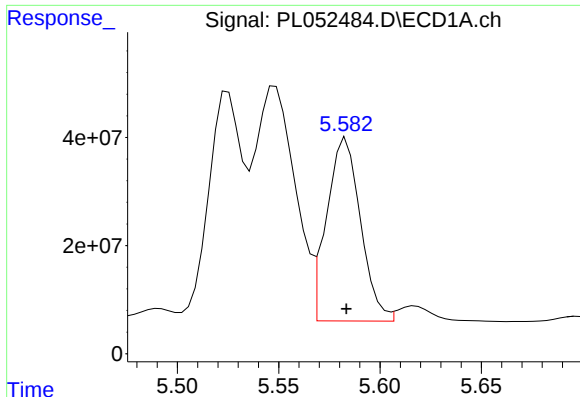

#26 Chlordane-4


R.T.: 5.583 min
Delta R.T.: 0.000 min
Response: 393472323
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

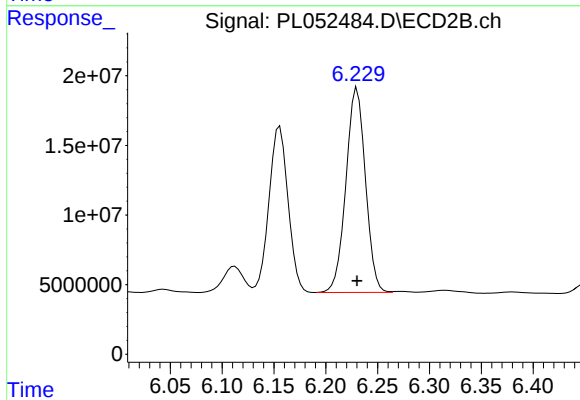


#26 Chlordane-4

R.T.: 6.230 min
Delta R.T.: 0.000 min
Response: 192305660
Conc: 500.00 ng/ml

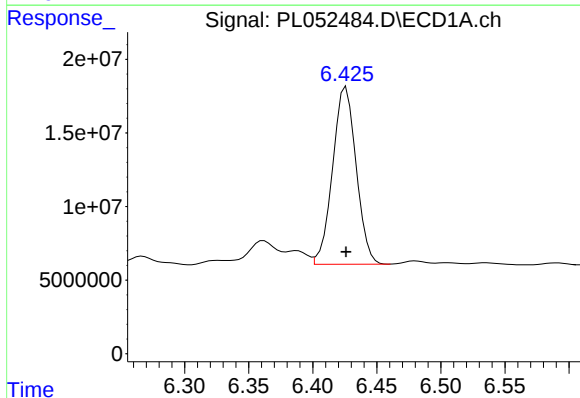


#27 Chlordane-5

R.T.: 6.426 min
Delta R.T.: 0.000 min
Response: 153970349
Conc: 500.00 ng/ml

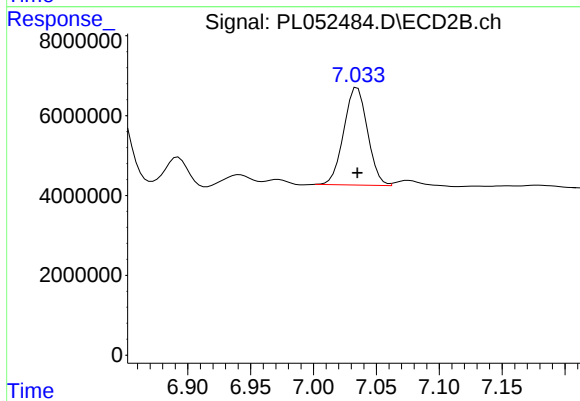

#27 Chlordane-5


R.T.: 7.035 min
Delta R.T.: 0.000 min
Response: 32021324
Conc: 500.00 ng/ml

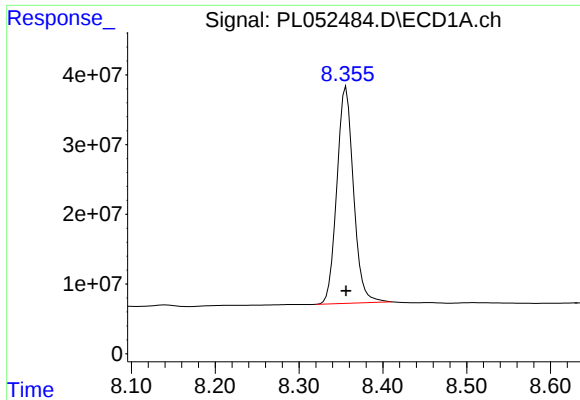

#28 Decachlorobiphenyl

R.T.: 8.356 min
Delta R.T.: 0.000 min
Response: 428517775
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

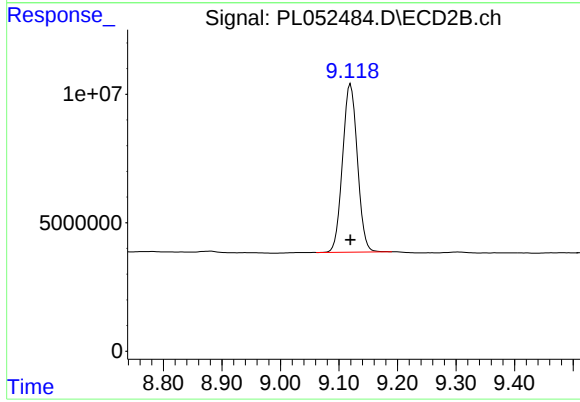

#28 Decachlorobiphenyl

R.T.: 9.120 min
Delta R.T.: 0.000 min
Response: 115297296
Conc: 50.00 ng/ml