

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091720\
 Data File : PL061559.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Sep 2020 15:01
 Operator : DD\AJ
 Sample : L4038-07
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PAV-091620-DP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 18 01:53:29 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 09 01:27:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.458	4.007	27838867	46834848	16.141	15.226
28)	SA Decachlor...	8.210	9.094	24038461	35012584	14.409	14.807
Target Compounds							
3)	MA gamma-BHC...	0.000	4.685	0	5483505	N.D.	1.278 #
5)	MB Aldrin	0.000	5.497	0	12912947	N.D.	3.417 #
6)	B beta-BHC	0.000	4.875f	0	852765	N.D.	0.488 #
9)	A Endosulfan I	5.521	6.273f	24223672	4736036	14.080	1.476 #
10)	B gamma-Chl...	0.000	6.124	0	21766047	N.D.	6.314 #
23)	Chlordane-1	4.324	0.000	7150161	0	136.305	N.D. #
24)	Chlordane-2	0.000	5.497f	0	12912947	N.D.	105.725 #
25)	Chlordane-3	0.000	6.124	0	21766047	N.D.	50.387 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091720\
Data File : PL061559.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Sep 2020 15:01
Operator : DD\AJ
Sample : L4038-07
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PAV-091620-DP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 18 01:53:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
Quant Title : GC Extractables
QLast Update : Wed Sep 09 01:27:38 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

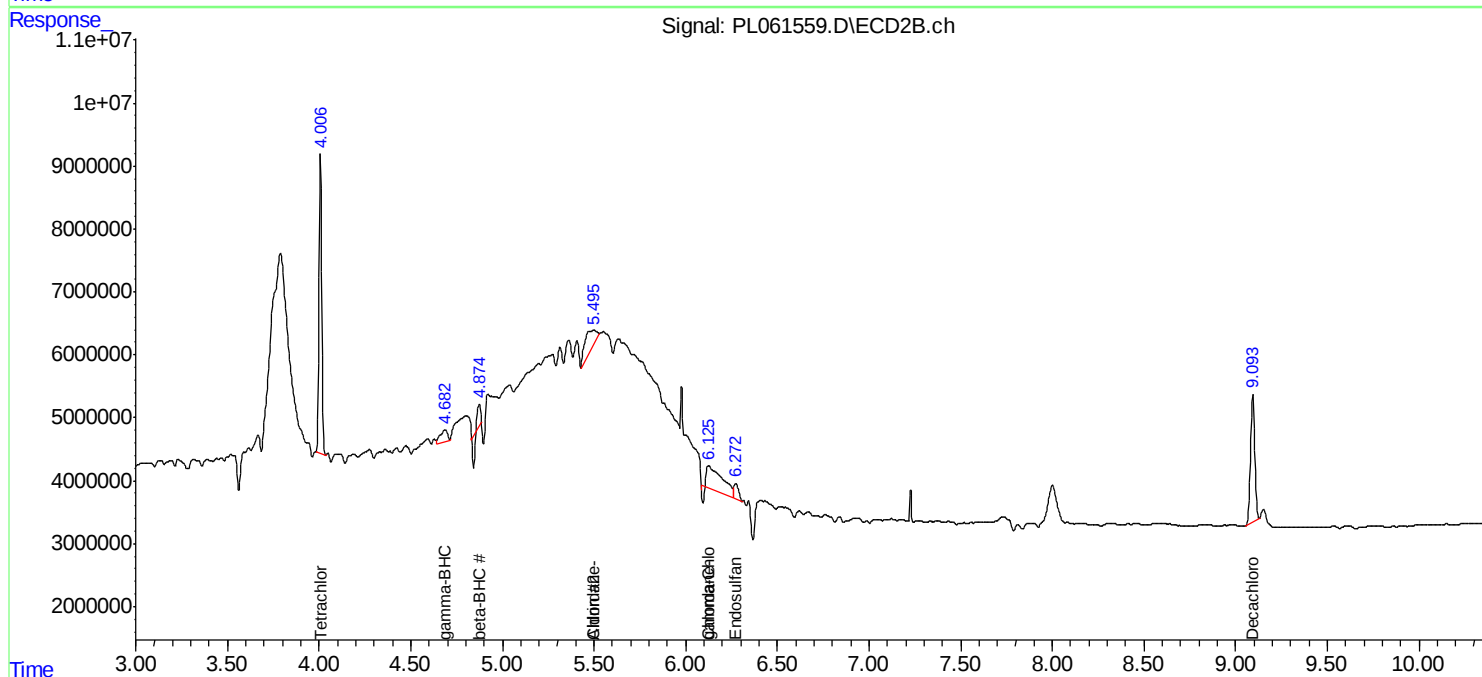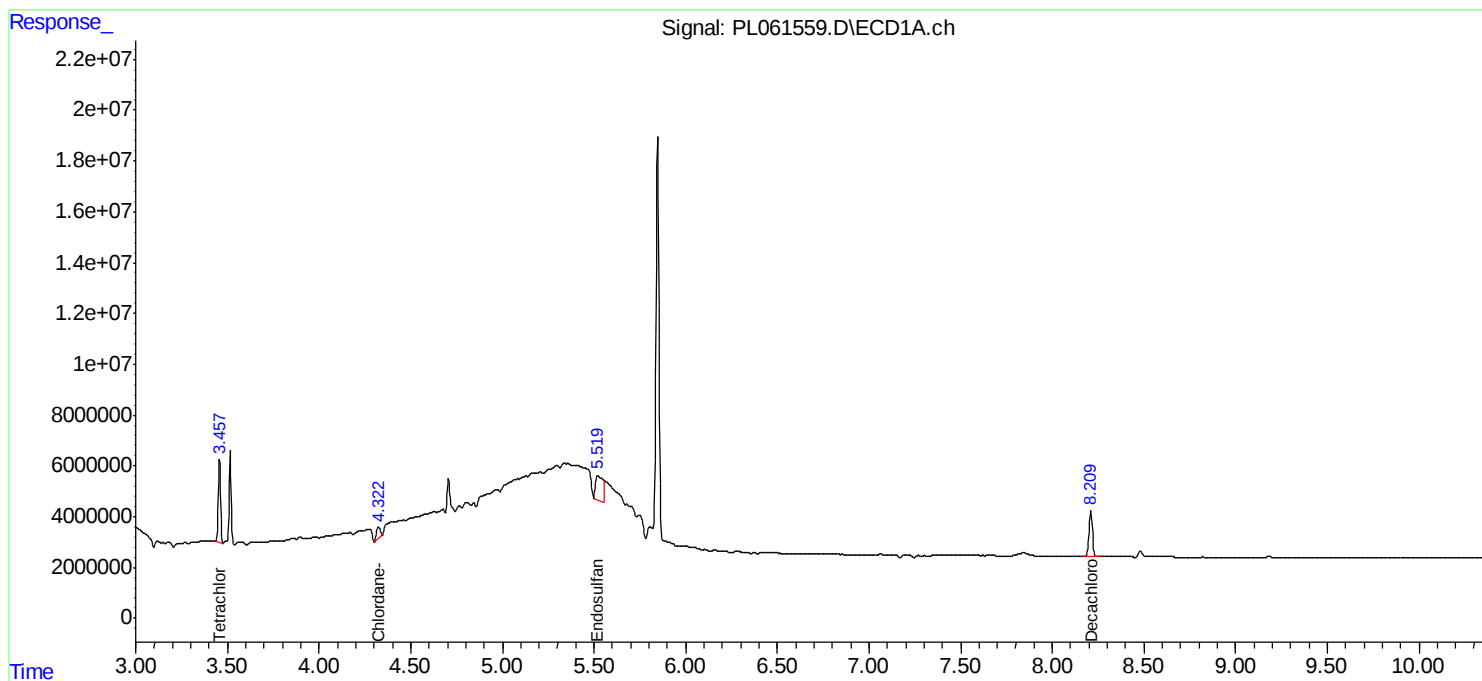


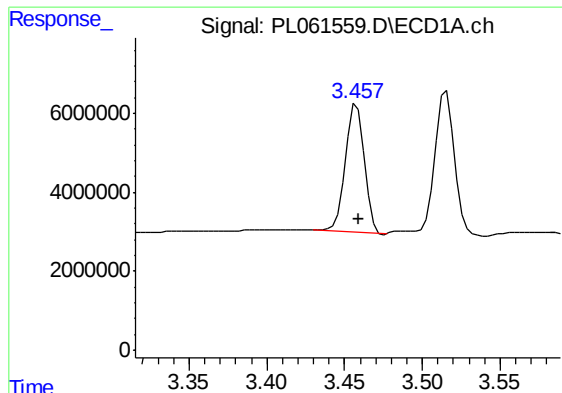

#1 Tetrachloro-m-xylene


R.T.: 3.458 min
Delta R.T.: 0.000 min
Response: 27838867
Conc: 16.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
PAV-091620-DP

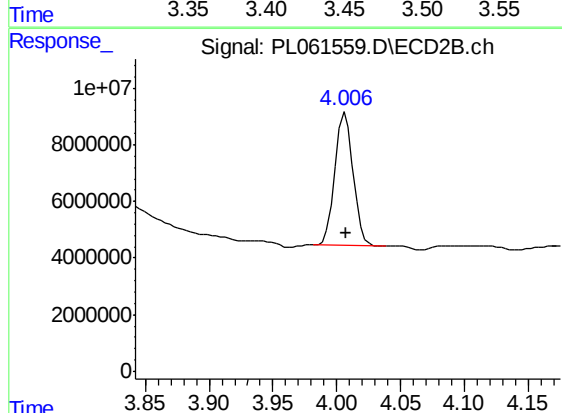


#1 Tetrachloro-m-xylene

R.T.: 4.007 min
Delta R.T.: 0.000 min
Response: 46834848
Conc: 15.23 ng/ml

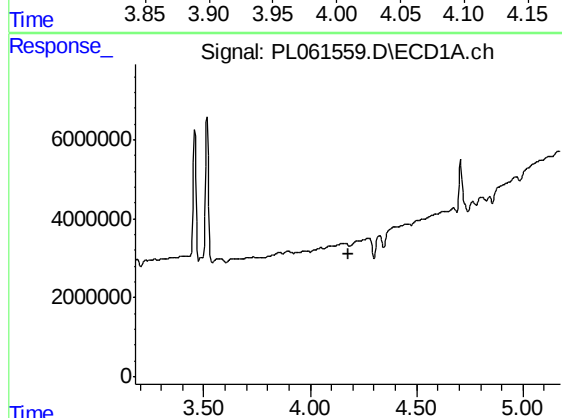


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.178 min
Response: 0
Conc: N.D.

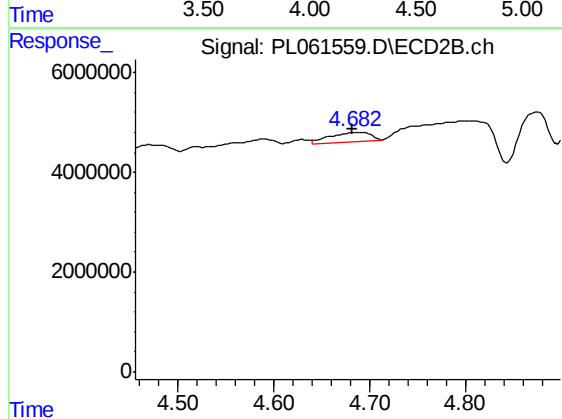

#3 gamma-BHC (Lindane)


R.T.: 4.685 min
Delta R.T.: 0.003 min
Response: 5483505
Conc: 1.28 ng/ml

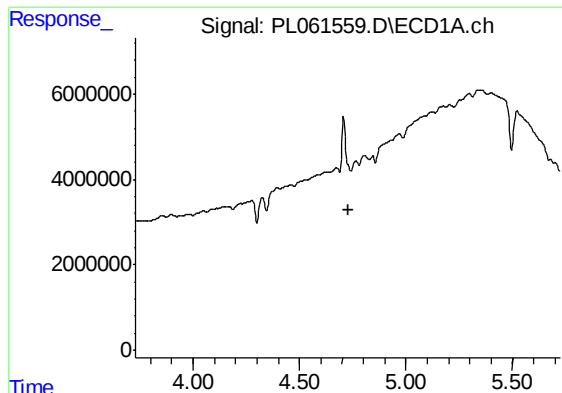

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 4.727 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PAV-091620-DP

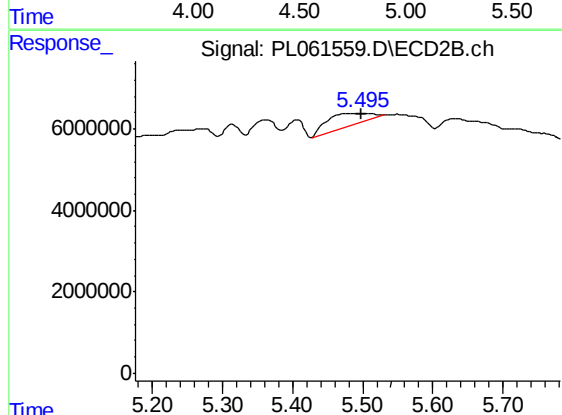


#5 Aldrin

R.T.: 5.497 min
Delta R.T.: -0.002 min
Response: 12912947
Conc: 3.42 ng/ml

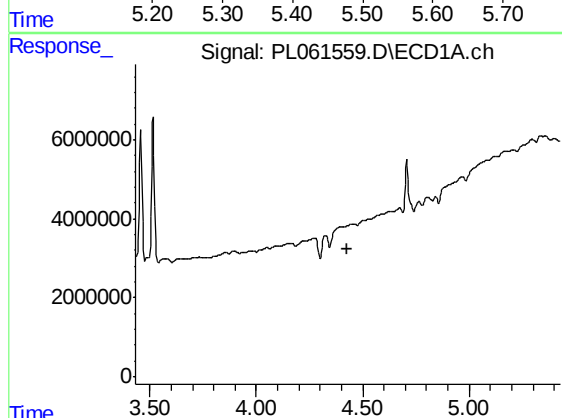


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.429 min
Response: 0
Conc: N.D.

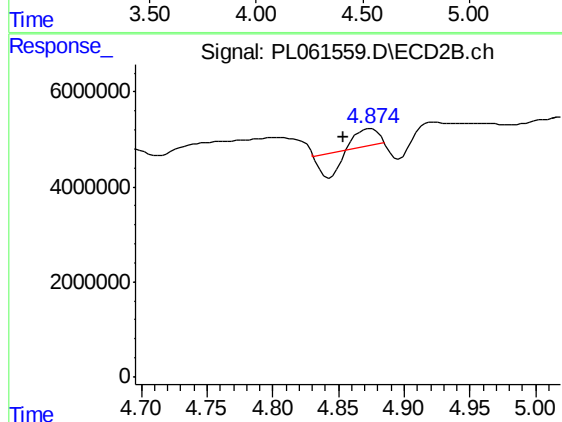

#6 beta-BHC


R.T.: 4.875 min
Delta R.T.: 0.021 min
Response: 852765
Conc: 0.49 ng/ml

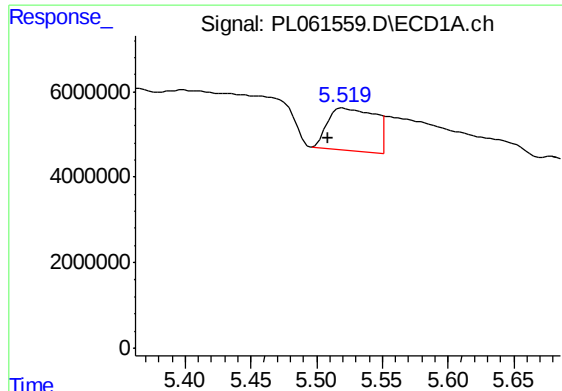

#9 Endosulfan I


R.T.: 5.521 min
Delta R.T.: 0.012 min
Response: 24223672
Conc: 14.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
PAV-091620-DP

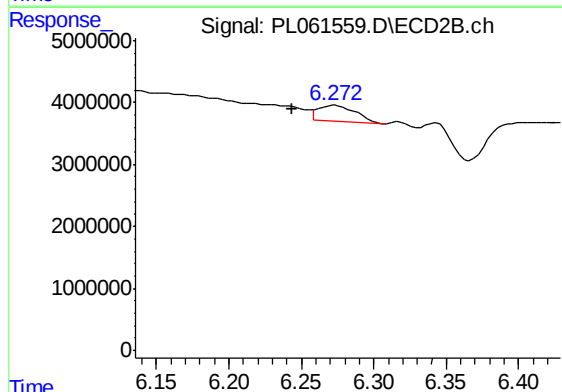


#9 Endosulfan I

R.T.: 6.273 min
Delta R.T.: 0.029 min
Response: 4736036
Conc: 1.48 ng/ml

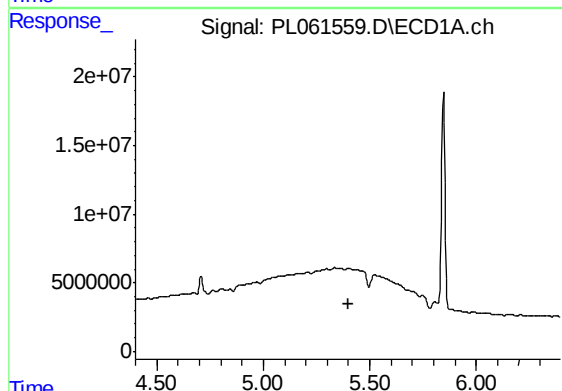


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.398 min
Response: 0
Conc: N.D.

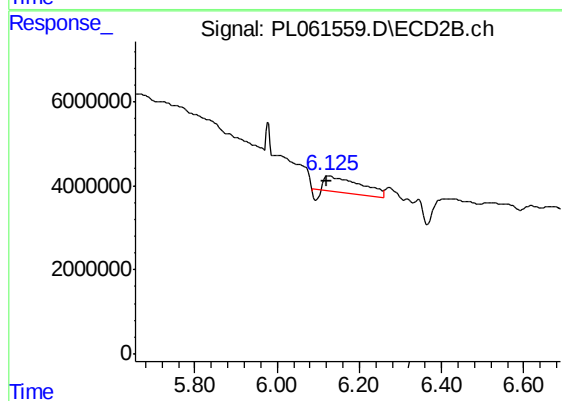

#10 gamma-Chlordane


R.T.: 6.124 min
Delta R.T.: 0.003 min
Response: 21766047
Conc: 6.31 ng/ml

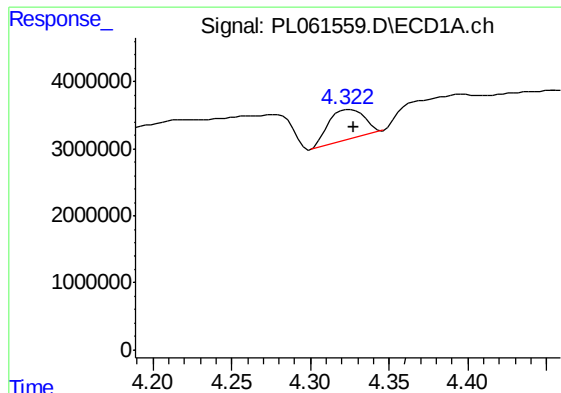

#23 Chlordane-1


R.T.: 4.324 min
Delta R.T.: -0.003 min
Response: 7150161
Conc: 136.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
PAV-091620-DP

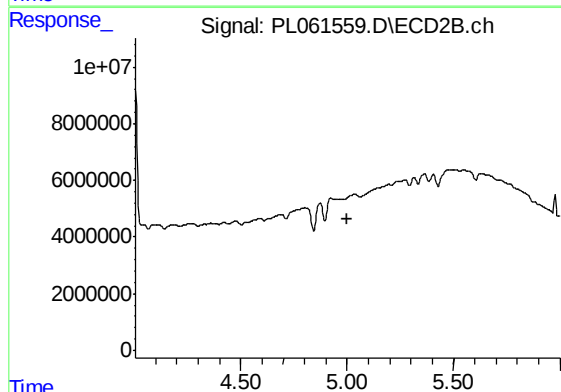


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.004 min
Response: 0
Conc: N.D.

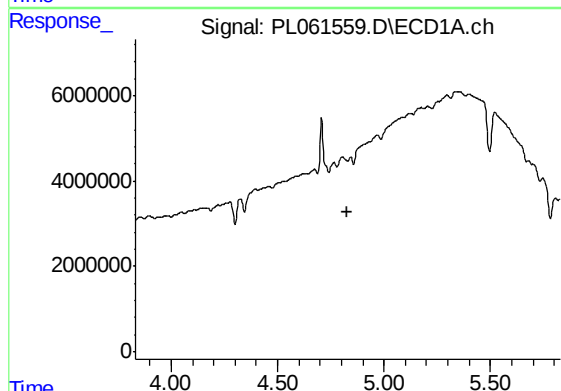


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 4.829 min
Response: 0
Conc: N.D.

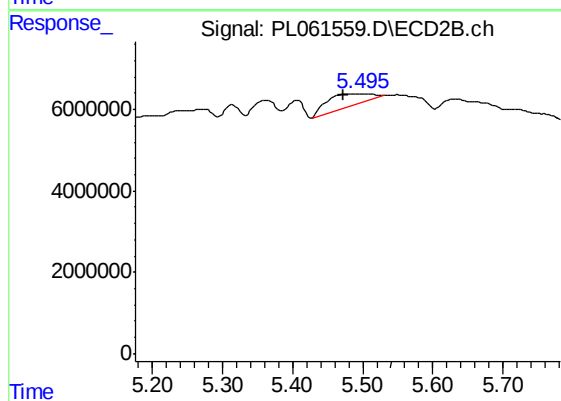

#24 Chlordane-2


R.T.: 5.497 min
Delta R.T.: 0.025 min
Response: 12912947
Conc: 105.72 ng/ml

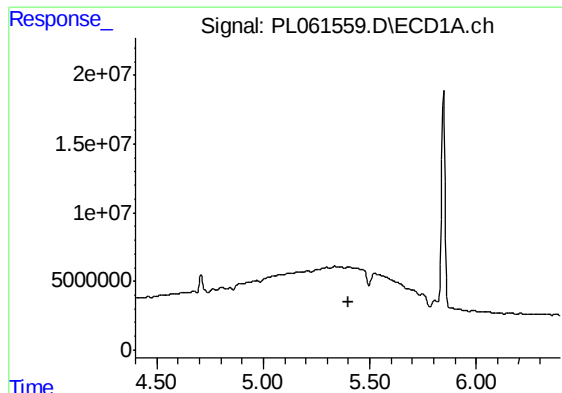

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.398 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PAV-091620-DP

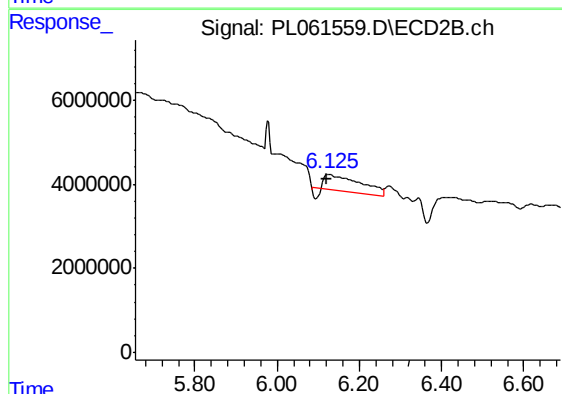


#25 Chlordane-3

R.T.: 6.124 min
Delta R.T.: 0.003 min
Response: 21766047
Conc: 50.39 ng/ml

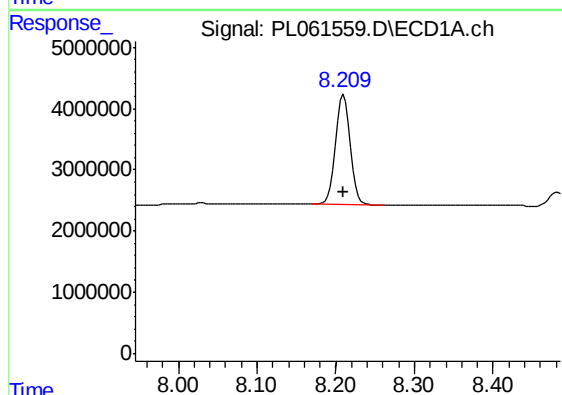

#28 Decachlorobiphenyl

R.T.: 8.210 min
Delta R.T.: 0.000 min
Response: 24038461
Conc: 14.41 ng/ml

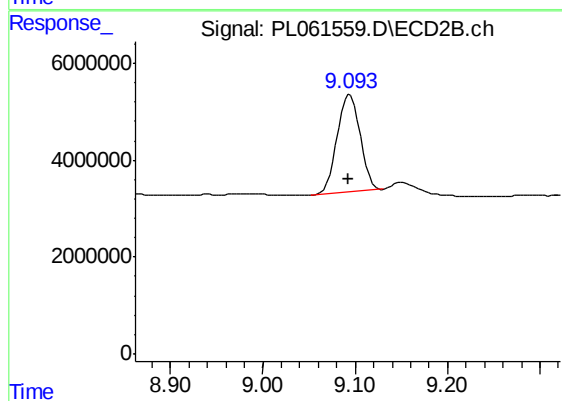

#28 Decachlorobiphenyl

R.T.: 9.094 min
Delta R.T.: 0.001 min
Response: 35012584
Conc: 14.81 ng/ml