

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091721\
 Data File : PL069885.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Sep 2021 09:25
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 18 01:40:38 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091021.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 13 17:55:23 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
8) B	Heptachlo...	0.000	8.037	0	1576817	N.D. 1.229 #
10) B	gamma-Chl...	0.000	8.325f	0	41010	N.D. 0.031 #
11) B	alpha-Chl...	0.000	8.383	0	58405	N.D. 0.043 #
25)	Chlordane-3	0.000	8.325f	0	41010	N.D. 0.216 #
26)	Chlordane-4	0.000	8.383	0	58405	N.D. 0.251 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091721\
Data File : PL069885.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Sep 2021 09:25
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 18 01:40:38 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091021.M
Quant Title : GC Extractables
QLast Update : Mon Sep 13 17:55:23 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

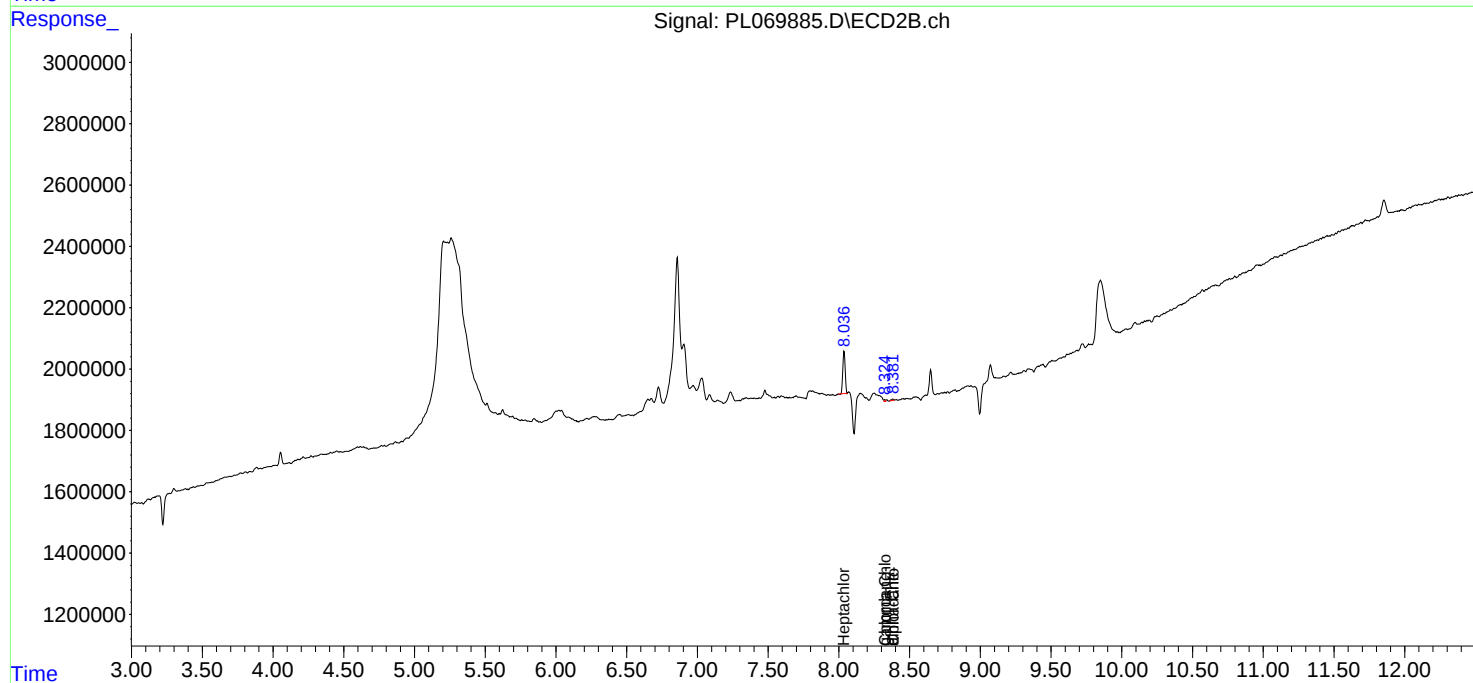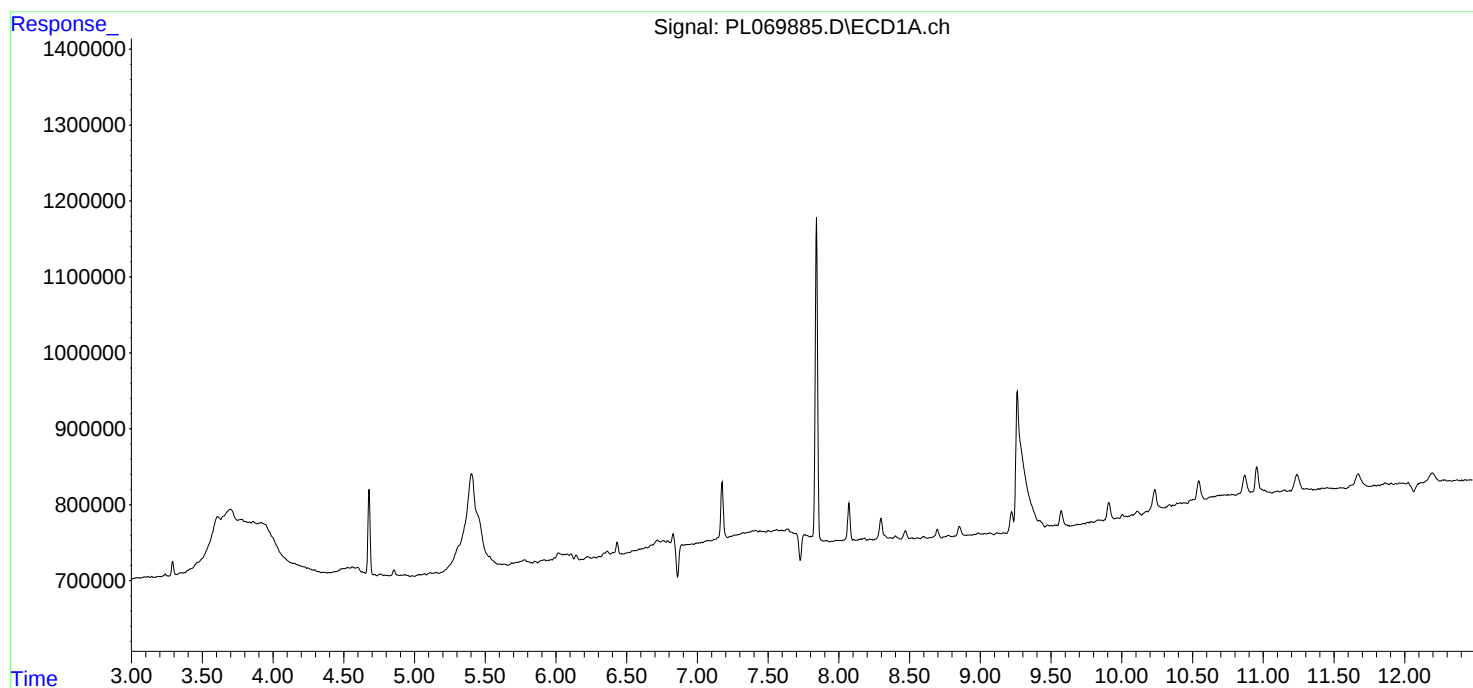


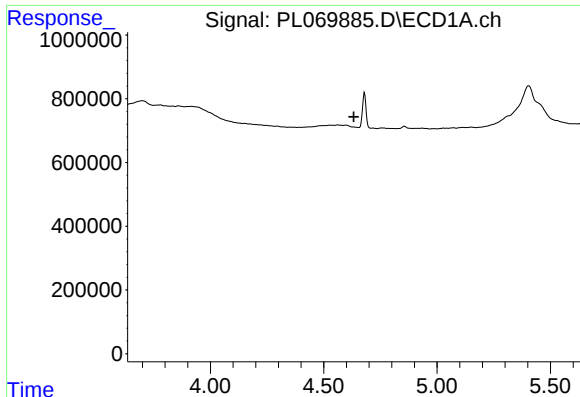

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.633 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

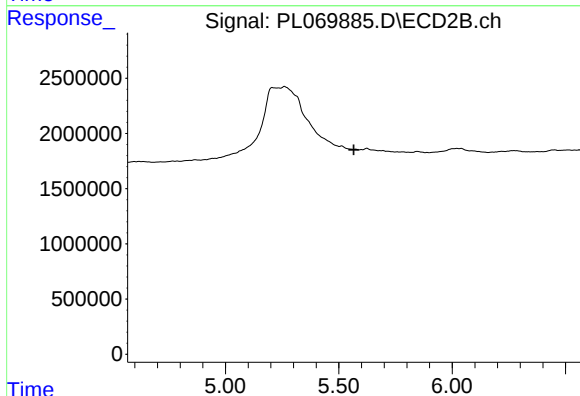


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 5.567 min
Response: 0
Conc: N.D.

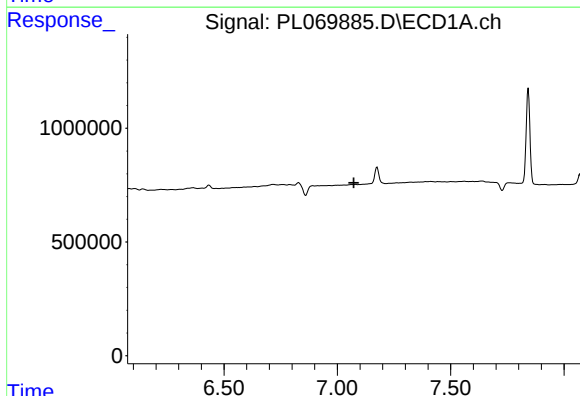


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.073 min
Response: 0
Conc: N.D.

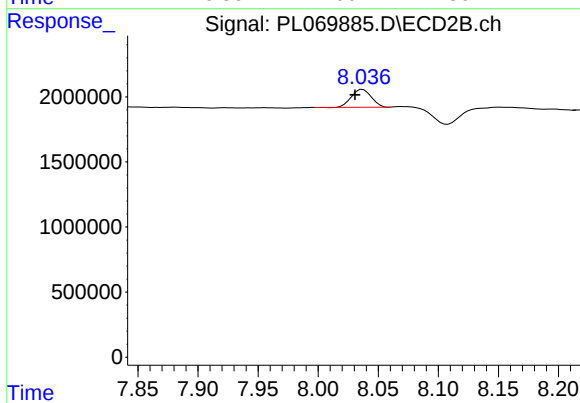

#8 Heptachlor epoxide


R.T.: 8.037 min
Delta R.T.: 0.007 min
Response: 1576817
Conc: 1.23 ng/ml

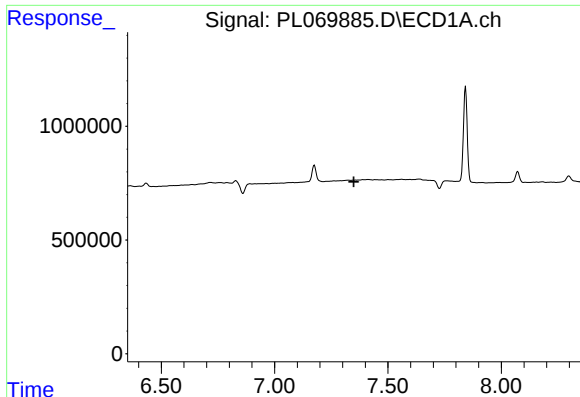

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 7.350 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

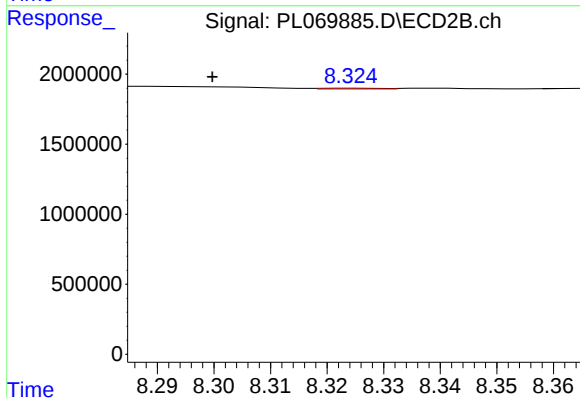


#10 gamma-Chlordane

R.T.: 8.325 min
Delta R.T.: 0.025 min
Response: 41010
Conc: 0.03 ng/ml

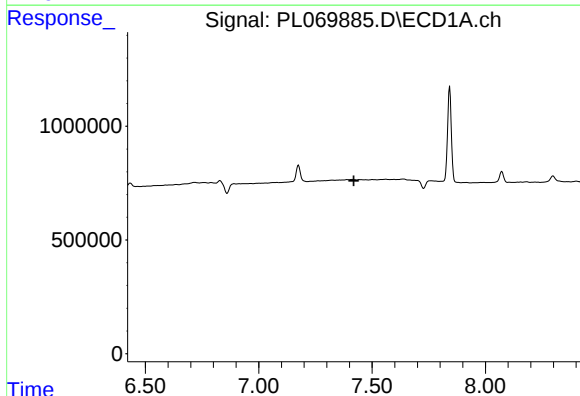


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.420 min
Response: 0
Conc: N.D.

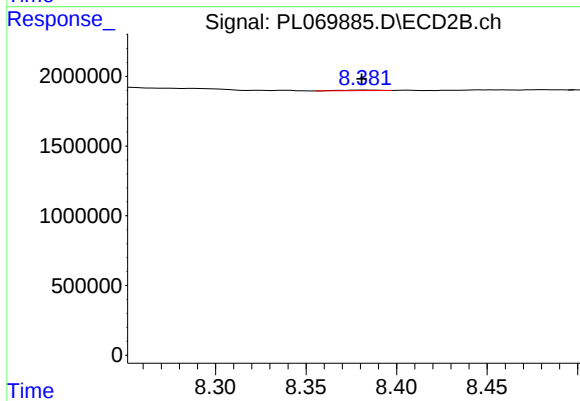

#11 alpha-Chlordane


R.T.: 8.383 min
Delta R.T.: 0.002 min
Response: 58405
Conc: 0.04 ng/ml

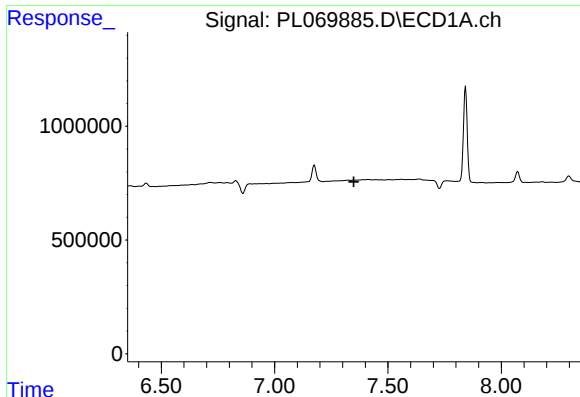

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.350 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

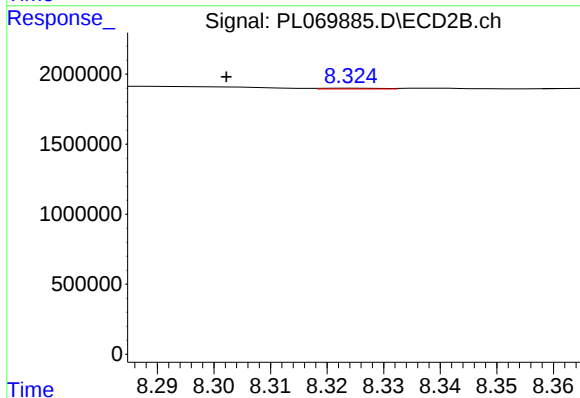


#25 Chlordane-3

R.T.: 8.325 min
Delta R.T.: 0.023 min
Response: 41010
Conc: 0.22 ng/ml

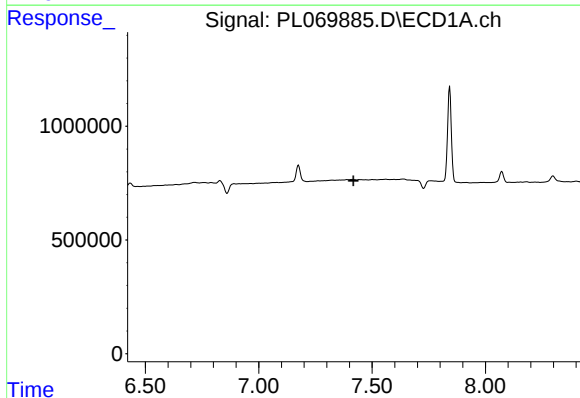


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 7.418 min
Response: 0
Conc: N.D.

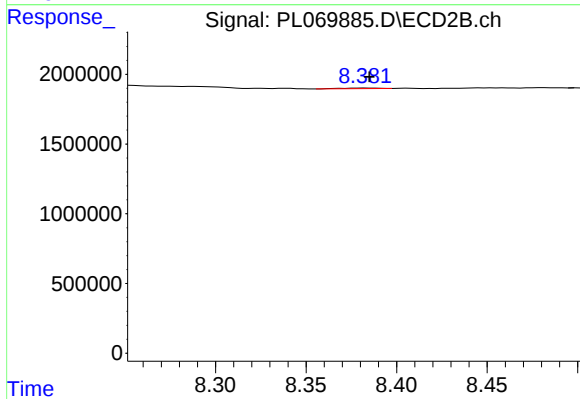

#26 Chlordane-4


R.T.: 8.383 min
Delta R.T.: -0.002 min
Response: 58405
Conc: 0.25 ng/ml

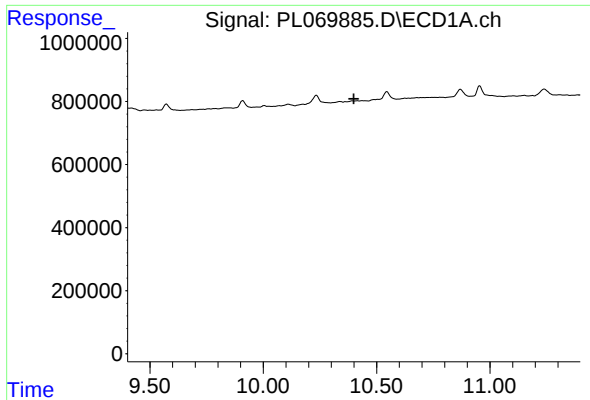

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.399 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

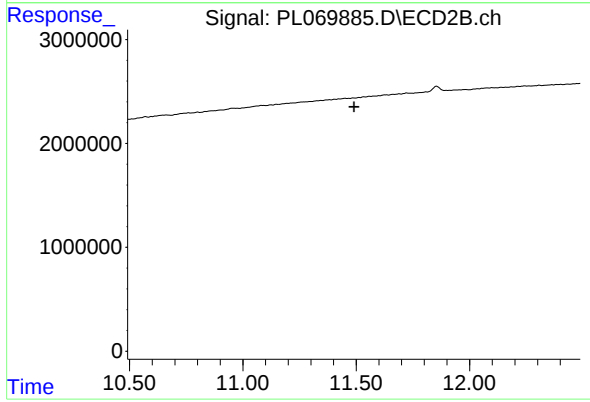

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 11.491 min
Response: 0
Conc: N.D.