

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091724\
 Data File : PL091788.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Sep 2024 16:05
 Operator : AR\AJ
 Sample : P4023-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-9

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 18 01:12:57 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090924.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 09 19:26:36 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.541	2.780	40889376	37605619	26.235	20.107
28)	SA Decachlor...	9.057	7.922	23771685	34911590	19.560	18.906
Target Compounds							
3)	MA gamma-BHC...	0.000	3.630	0	173591	N.D.	0.071 #
4)	MA Heptachlor	0.000	3.950	0	52052	N.D.	0.022 #
5)	MB Aldrin	0.000	4.245	0	577393	N.D.	0.253 #
6)	B beta-BHC	0.000	3.920	0	254318	N.D.	0.233 #
8)	B Heptachlo...	0.000	4.739	0	187875	N.D.	0.089 #
9)	A Endosulfan I	0.000	5.113	0	34060	N.D.	0.018 #
16)	A 4,4'-DDD	0.000	5.803	0	543341	N.D.	0.324 #
17)	MA 4,4'-DDT	0.000	6.044	0	579114	N.D.	0.360 #
19)	B Endosulfa...	0.000	6.346	0	85809	N.D.	0.050 #
20)	A Methoxychlor	0.000	6.623	0	46575	N.D.	0.053 #
22)	Mirex	0.000	7.047	0	192468	N.D.	0.109 #
24)	Chlordane-2	0.000	4.327f	0	287036	N.D.	3.830 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091724\
Data File : PL091788.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Sep 2024 16:05
Operator : AR\AJ
Sample : P4023-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-9

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 18 01:12:57 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090924.M
Quant Title : GC Extractables
QLast Update : Mon Sep 09 19:26:36 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

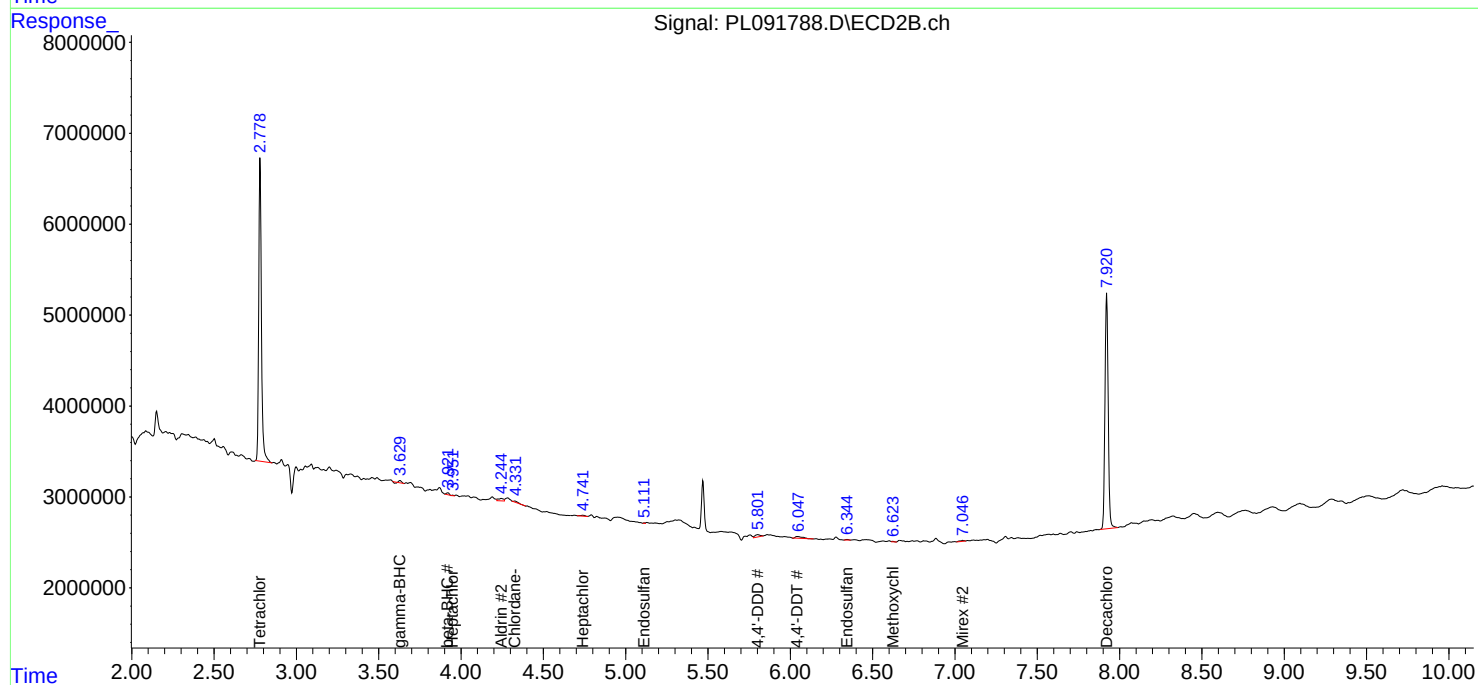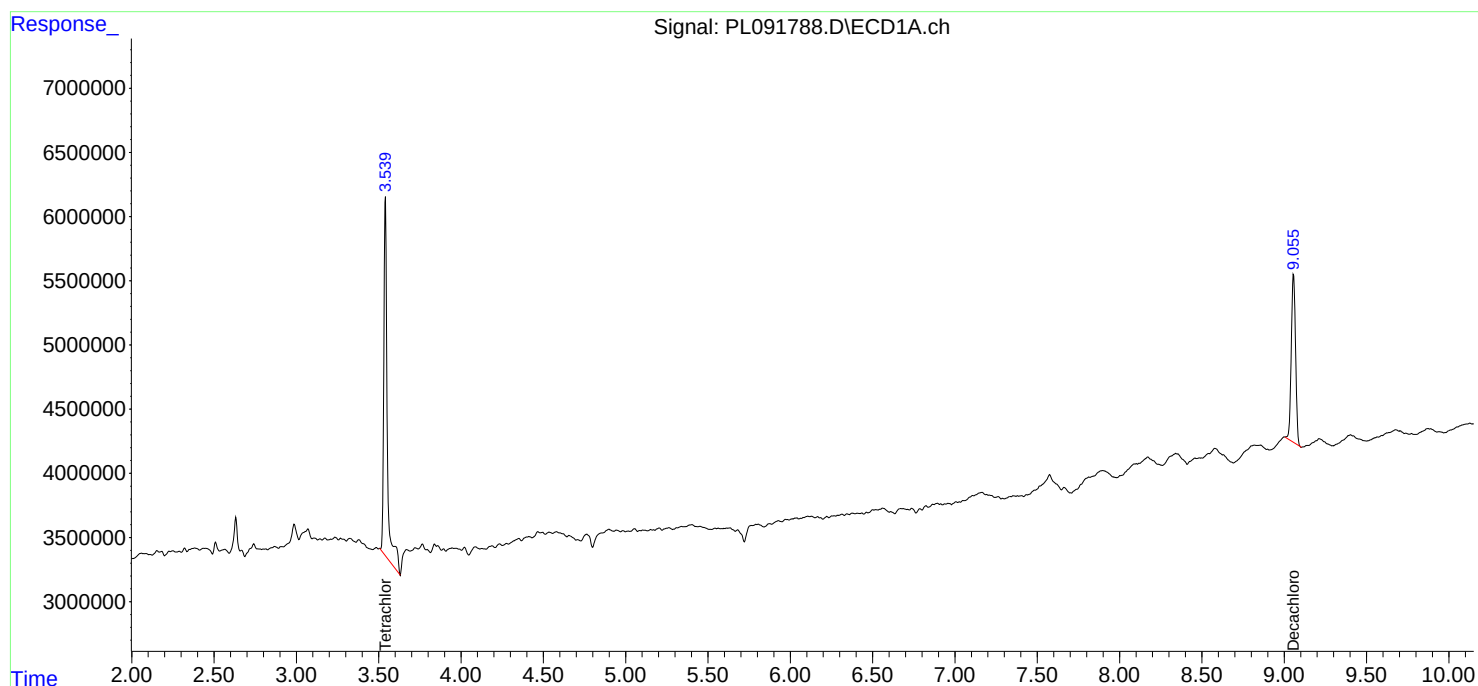


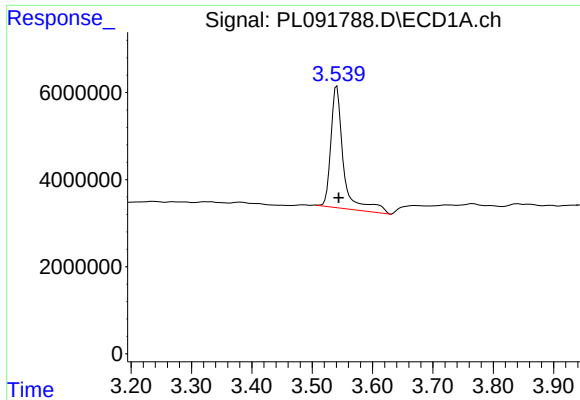

#1 Tetrachloro-m-xylene


R.T.: 3.541 min
Delta R.T.: -0.003 min
Response: 40889376
Conc: 26.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-9

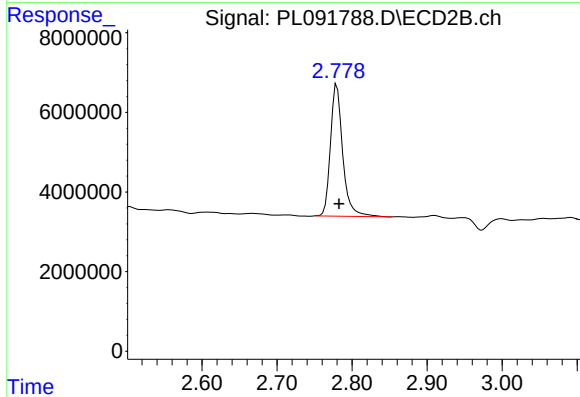


#1 Tetrachloro-m-xylene

R.T.: 2.780 min
Delta R.T.: -0.003 min
Response: 37605619
Conc: 20.11 ng/ml

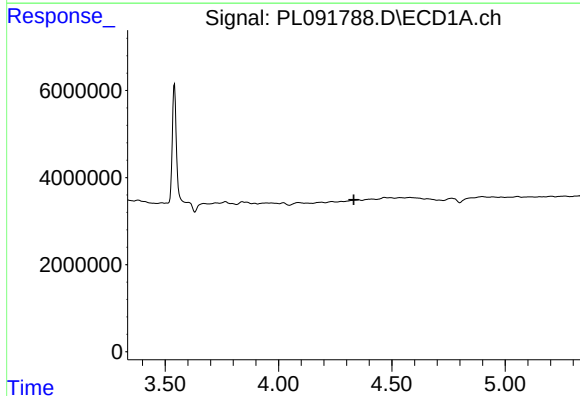


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.332 min
Response: 0
Conc: N.D.

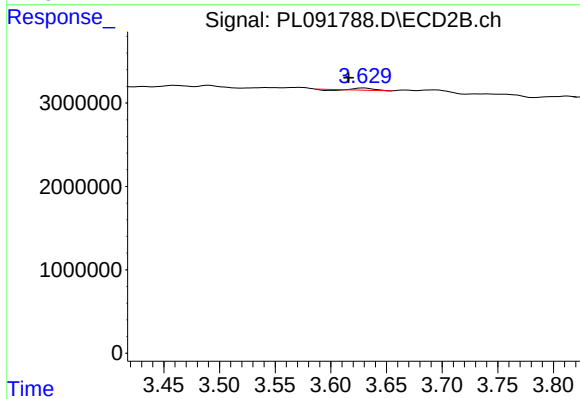

#3 gamma-BHC (Lindane)


R.T.: 3.630 min
Delta R.T.: 0.014 min
Response: 173591
Conc: 0.07 ng/ml

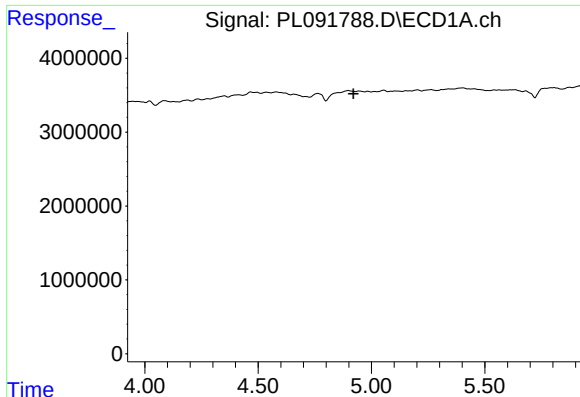

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.921 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-9

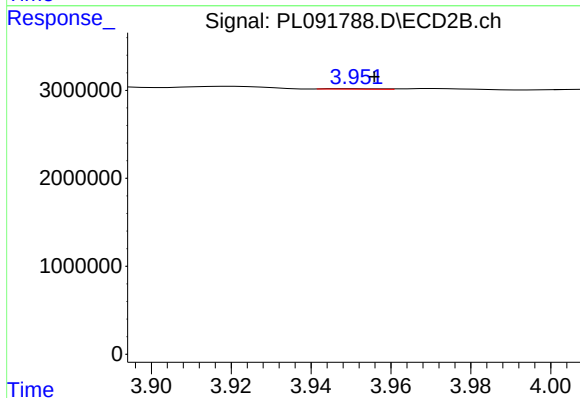


#4 Heptachlor

R.T.: 3.950 min
Delta R.T.: -0.006 min
Response: 52052
Conc: 0.02 ng/ml

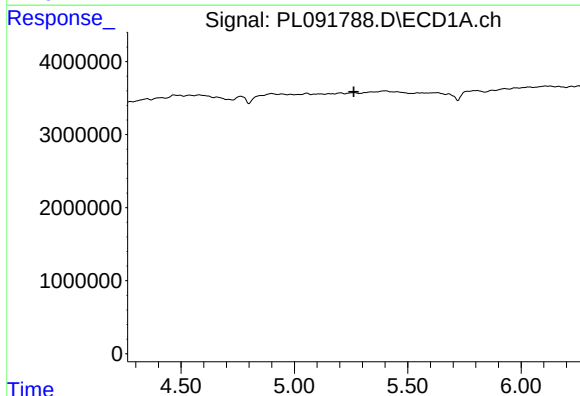


#5 Aldrin

R.T.: 0.000 min
Exp R.T.: 5.262 min
Response: 0
Conc: N.D.

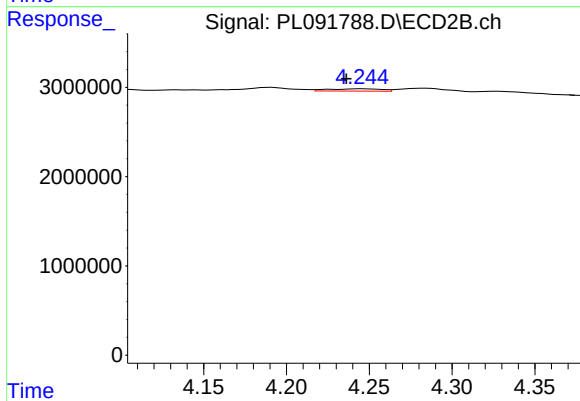

#5 Aldrin


R.T.: 4.245 min
Delta R.T.: 0.009 min
Response: 577393
Conc: 0.25 ng/ml

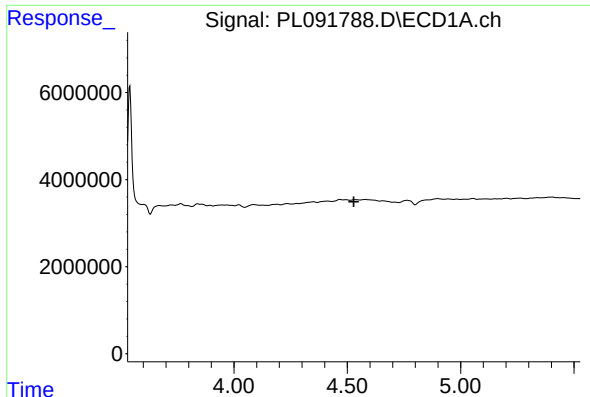

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.528 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-9

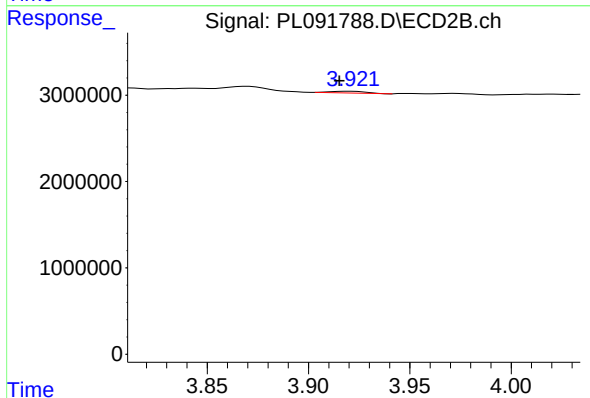


#6 beta-BHC

R.T.: 3.920 min
Delta R.T.: 0.005 min
Response: 254318
Conc: 0.23 ng/ml

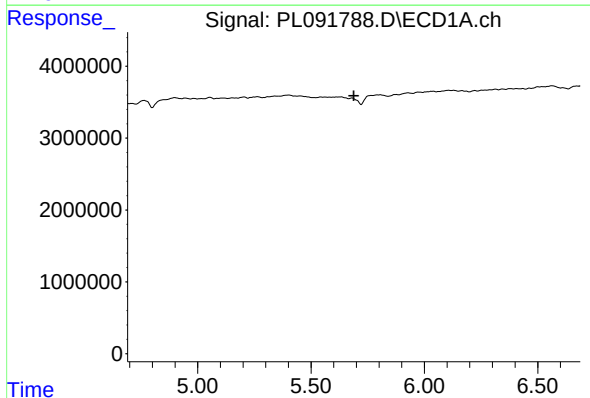


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.689 min
Response: 0
Conc: N.D.

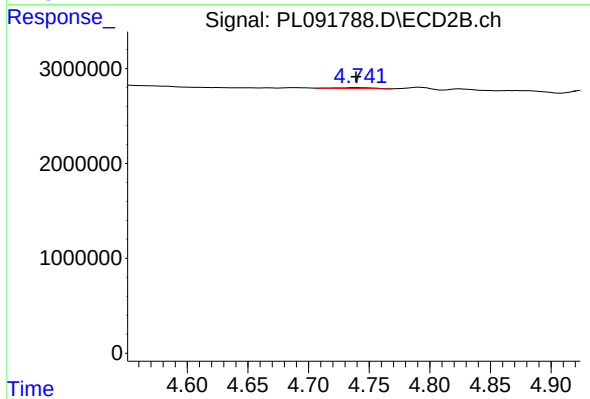

#8 Heptachlor epoxide


R.T.: 4.739 min
Delta R.T.: 0.000 min
Response: 187875
Conc: 0.09 ng/ml

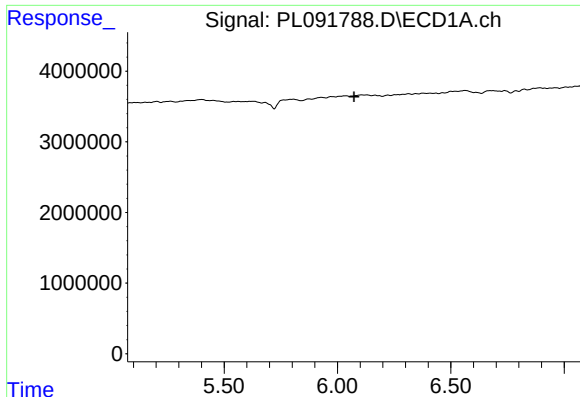

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.074 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-9

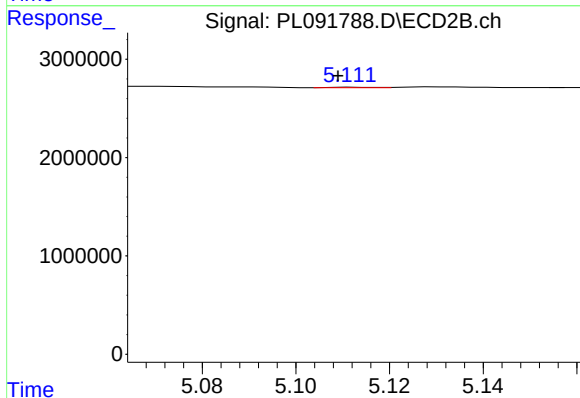


#9 Endosulfan I

R.T.: 5.113 min
Delta R.T.: 0.004 min
Response: 34060
Conc: 0.02 ng/ml

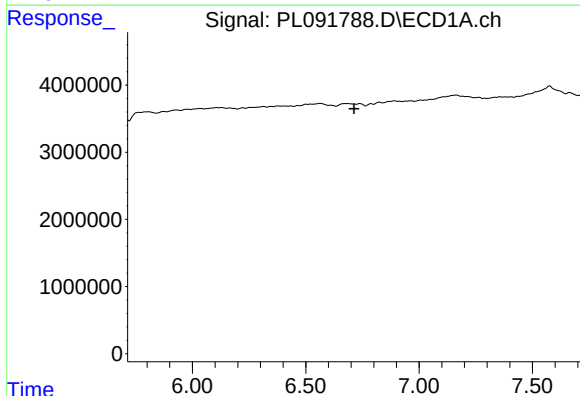


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 6.714 min
Response: 0
Conc: N.D.

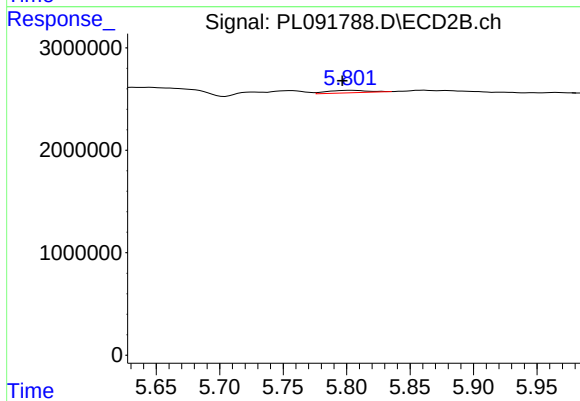

#16 4,4'-DDD


R.T.: 5.803 min
Delta R.T.: 0.006 min
Response: 543341
Conc: 0.32 ng/ml

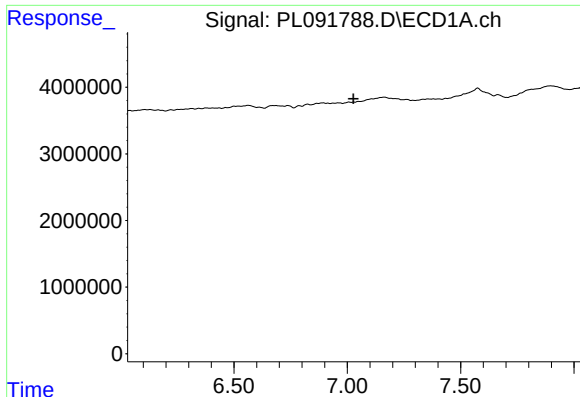

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 7.028 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-9

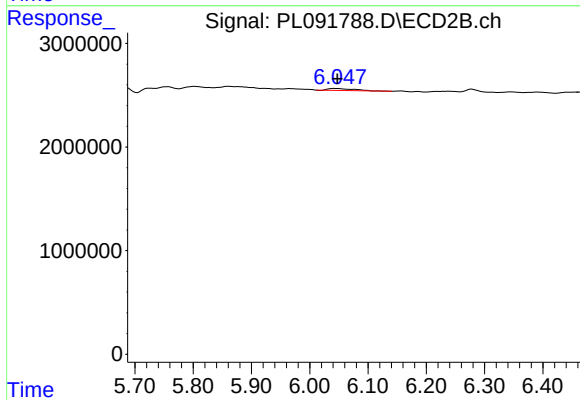


#17 4,4'-DDT

R.T.: 6.044 min
Delta R.T.: -0.003 min
Response: 579114
Conc: 0.36 ng/ml

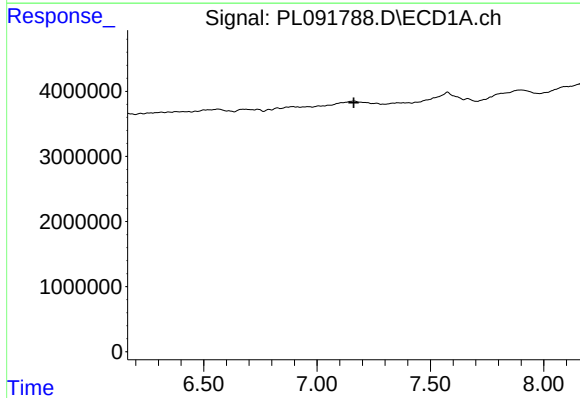


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 7.162 min
Response: 0
Conc: N.D.

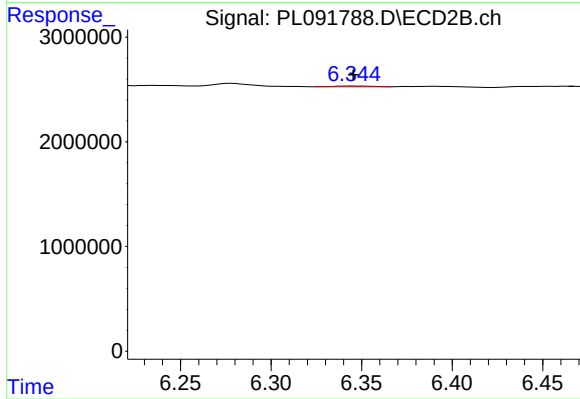

#19 Endosulfan Sulfate


R.T.: 6.346 min
Delta R.T.: 0.000 min
Response: 85809
Conc: 0.05 ng/ml

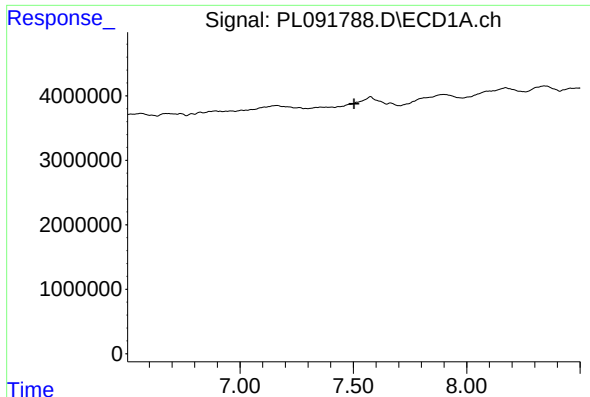

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 7.503 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-9

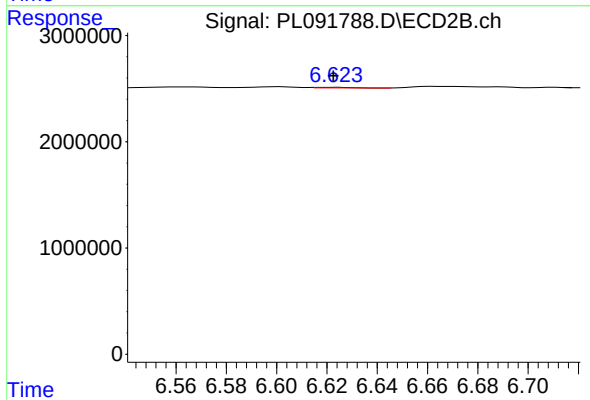


#20 Methoxychlor

R.T.: 6.623 min
Delta R.T.: 0.000 min
Response: 46575
Conc: 0.05 ng/ml

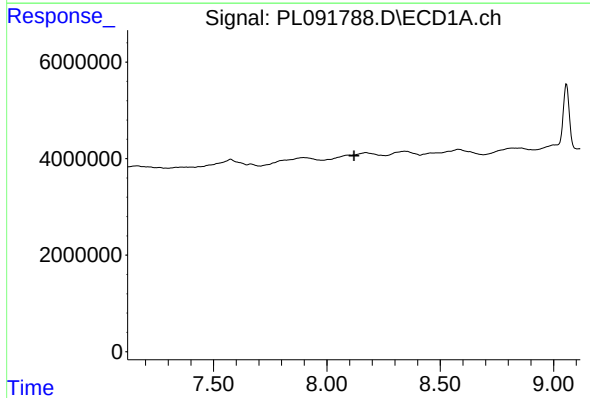


#22 Mirex

R.T.: 0.000 min
Exp R.T.: 8.121 min
Response: 0
Conc: N.D.

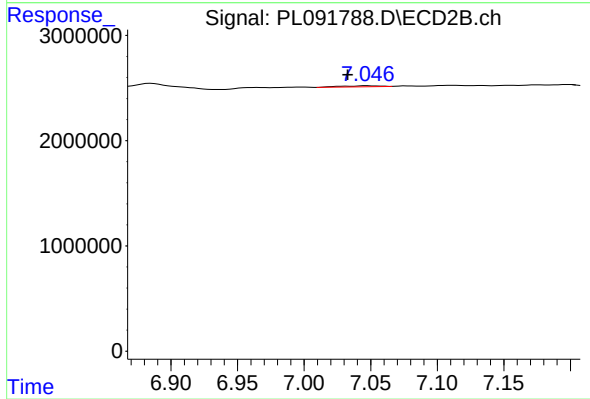

#22 Mirex


R.T.: 7.047 min
Delta R.T.: 0.015 min
Response: 192468
Conc: 0.11 ng/ml

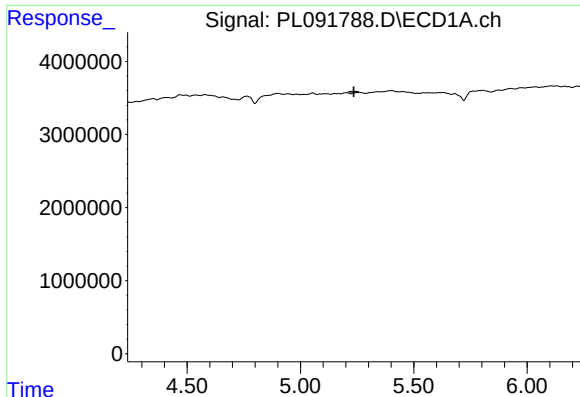

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 5.236 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-9

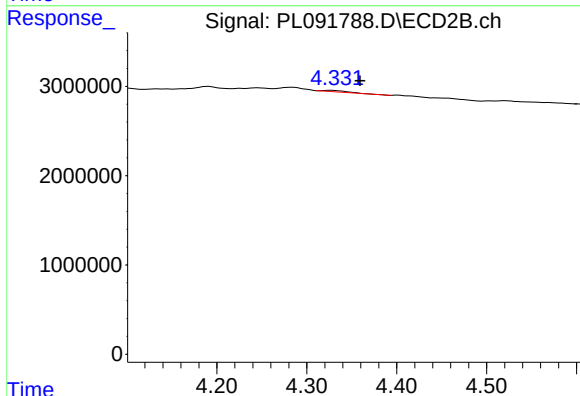


#24 Chlordane-2

R.T.: 4.327 min
Delta R.T.: -0.033 min
Response: 287036
Conc: 3.83 ng/ml

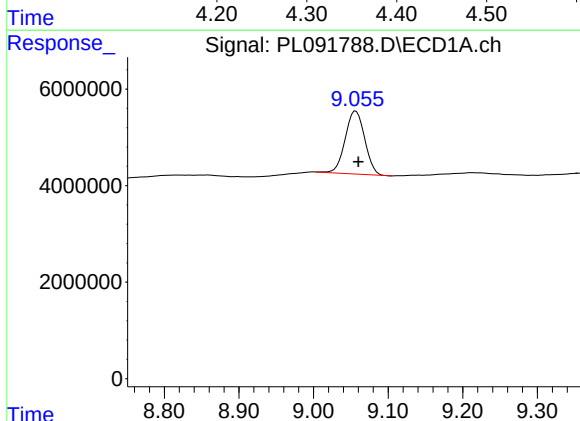

#28 Decachlorobiphenyl

R.T.: 9.057 min
Delta R.T.: -0.004 min
Response: 23771685
Conc: 19.56 ng/ml

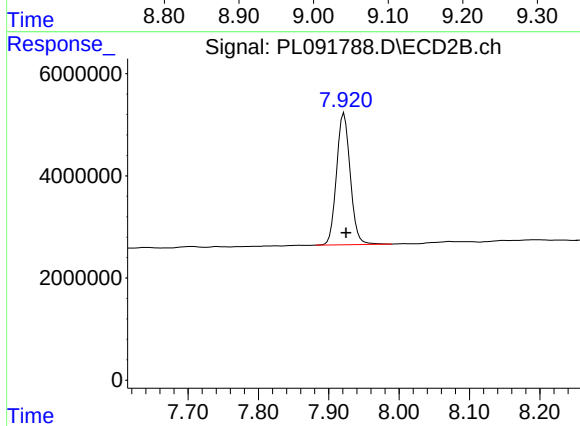

#28 Decachlorobiphenyl

R.T.: 7.922 min
Delta R.T.: -0.003 min
Response: 34911590
Conc: 18.91 ng/ml