

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091818\
 Data File : PL040061.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Sep 2018 07:09
 Operator : AJ\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 18 15:09:55 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 14 23:10:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
7) B	delta-BHC	0.000	4.950	0	8927722	N.D. 2.244 #
8) B	Heptachlo...	0.000	5.741	0	8436910	N.D. 2.133 #
10) B	gamma-Chl...	0.000	5.976	0	2367779	N.D. 0.626 #
21) B	Endrin ke...	6.879	0.000	13813860	0	1.415 N.D. #
23)	Chlordane-1	0.000	4.950	0	8927722	N.D. 57.655 #
25)	Chlordane-3	0.000	5.976	0	2367779	N.D. 4.625 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091818\
Data File : PL040061.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Sep 2018 07:09
Operator : AJ\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 18 15:09:55 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
Quant Title : GC Extractables
QLast Update : Fri Sep 14 23:10:39 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

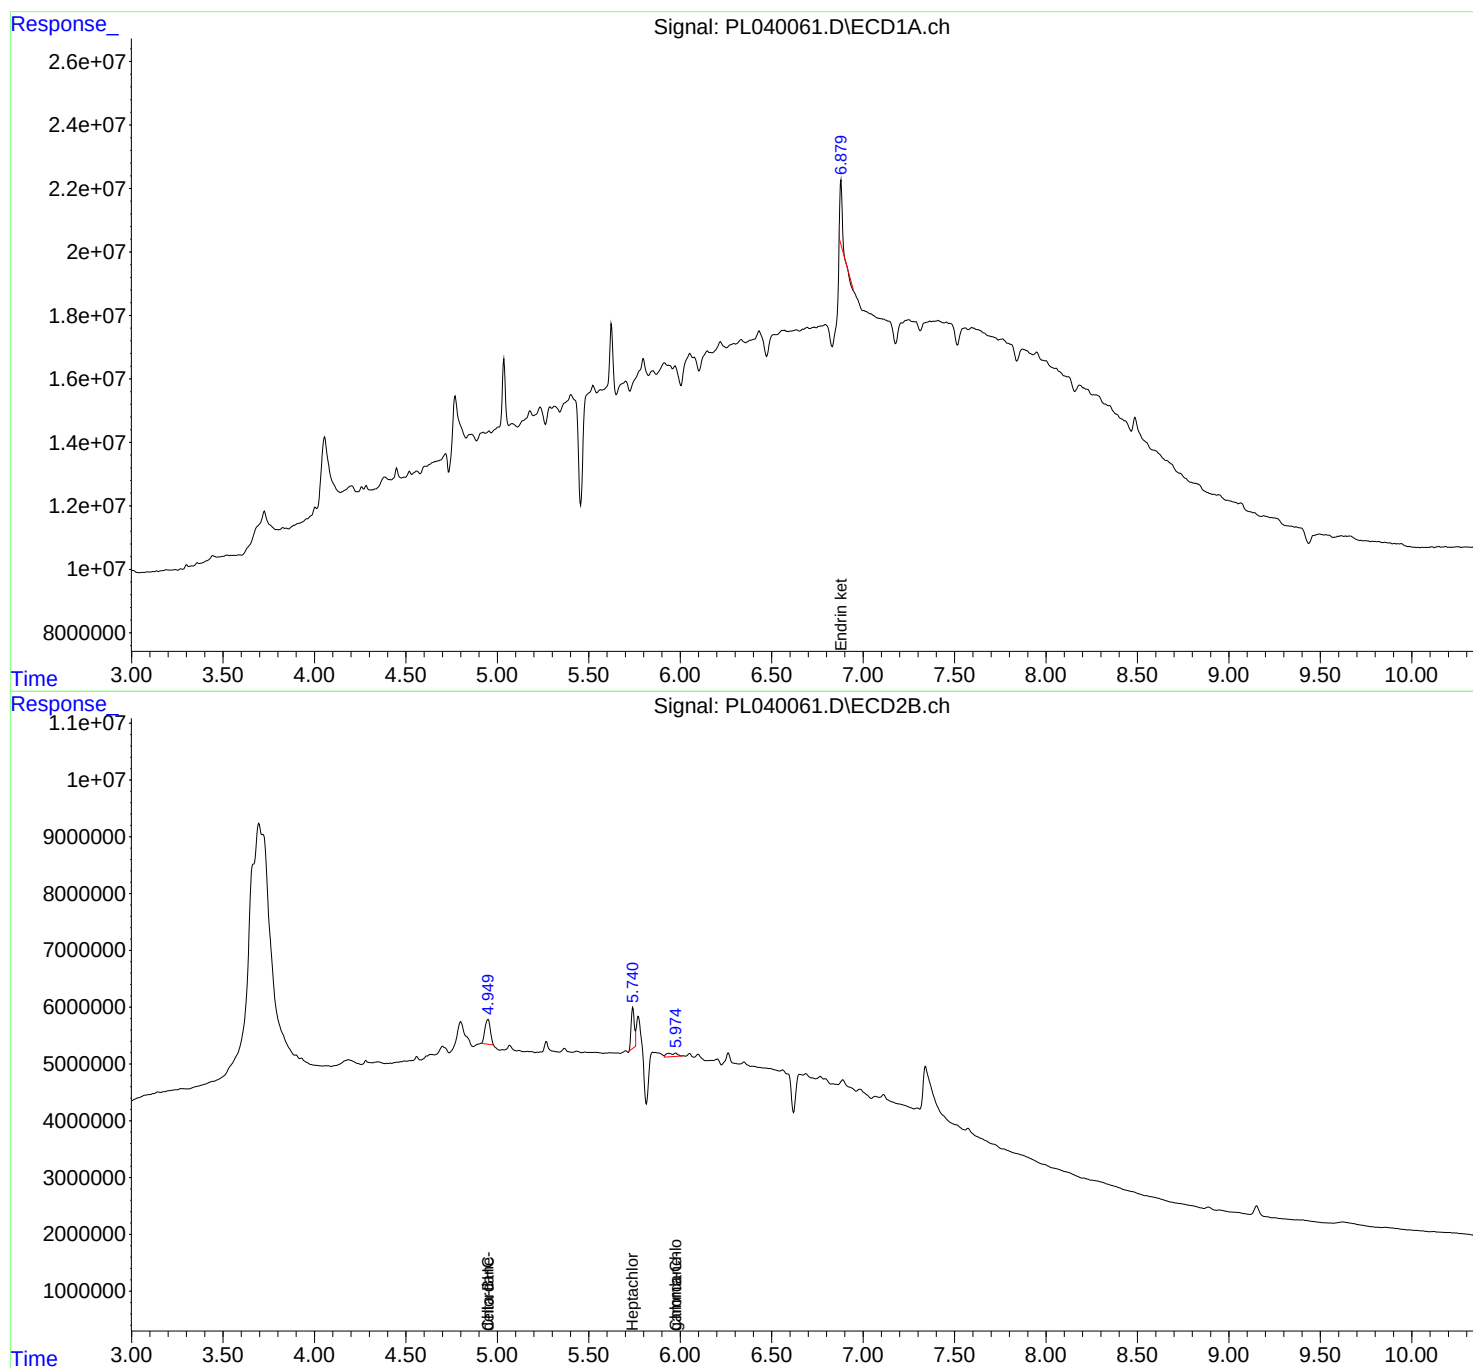


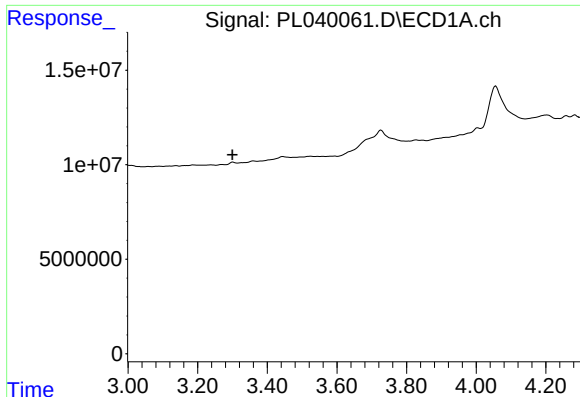

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.300 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

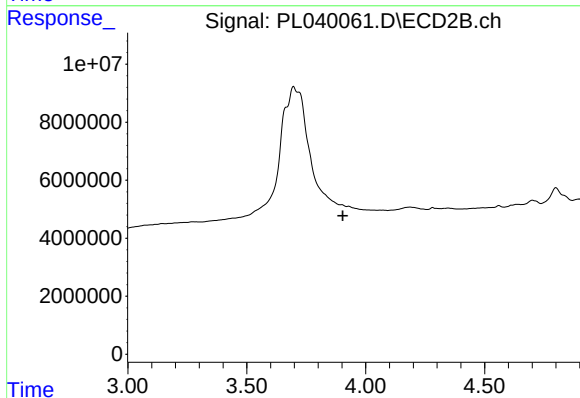


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.903 min
Response: 0
Conc: N.D.

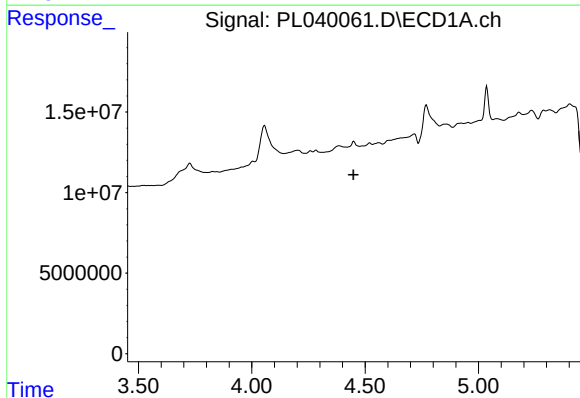


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.449 min
Response: 0
Conc: N.D.

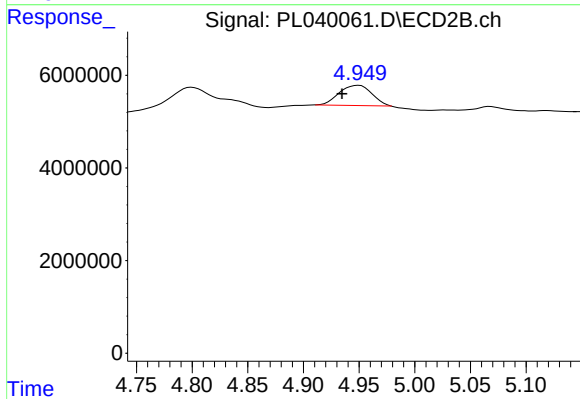

#7 delta-BHC


R.T.: 4.950 min
Delta R.T.: 0.015 min
Response: 8927722
Conc: 2.24 ng/ml

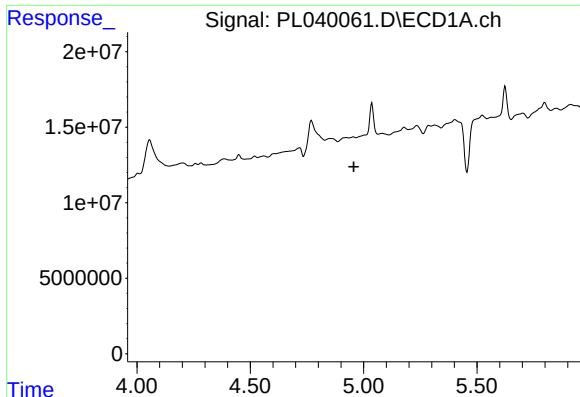

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.956 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

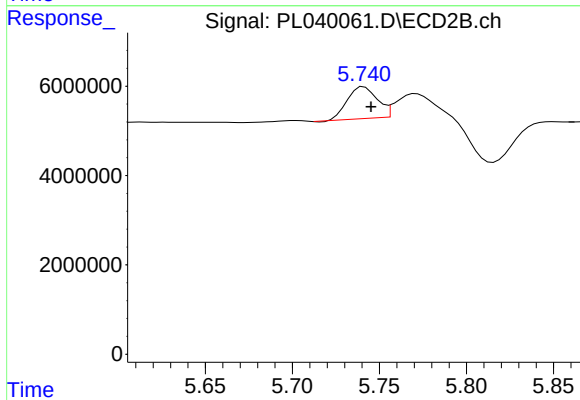


#8 Heptachlor epoxide

R.T.: 5.741 min
Delta R.T.: -0.004 min
Response: 8436910
Conc: 2.13 ng/ml

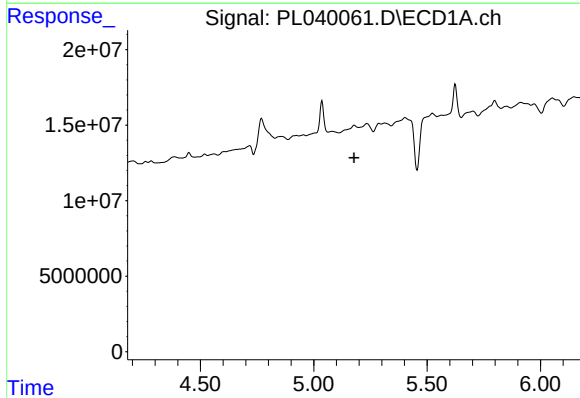


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.178 min
Response: 0
Conc: N.D.

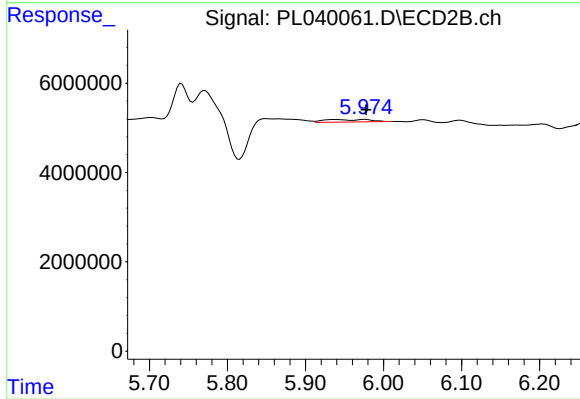

#10 gamma-Chlordane


R.T.: 5.976 min
Delta R.T.: -0.002 min
Response: 2367779
Conc: 0.63 ng/ml

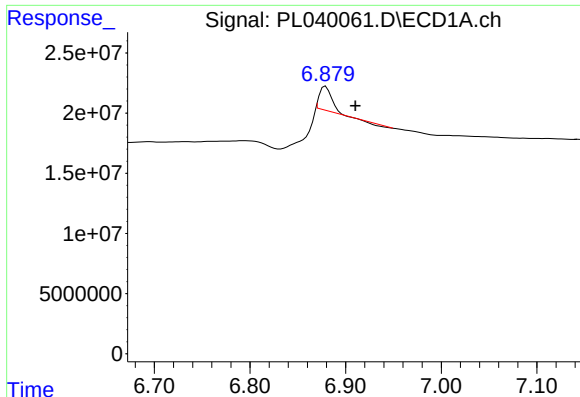

#21 Endrin ketone


R.T.: 6.879 min
Delta R.T.: -0.031 min
Response: 13813860
Conc: 1.41 ng/ml

Instrument :
ECD_L
ClientSampleId :

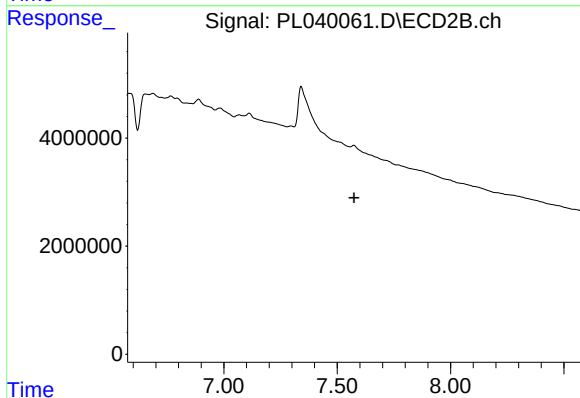


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.574 min
Response: 0
Conc: N.D.

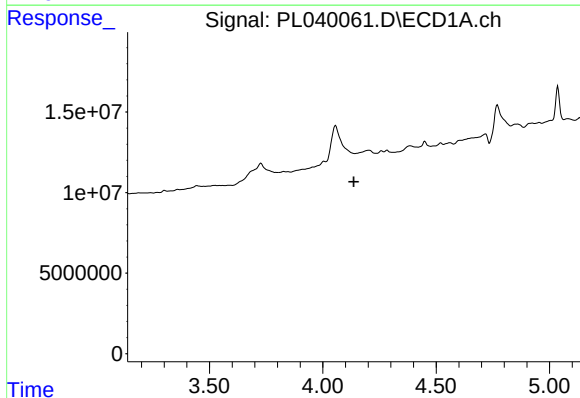


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.136 min
Response: 0
Conc: N.D.

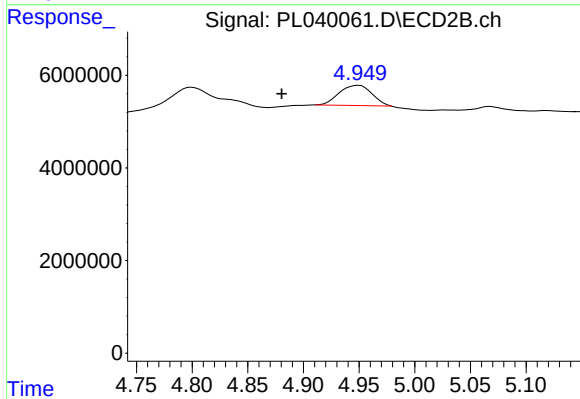

#23 Chlordane-1


R.T.: 4.950 min
Delta R.T.: 0.069 min
Response: 8927722
Conc: 57.66 ng/ml

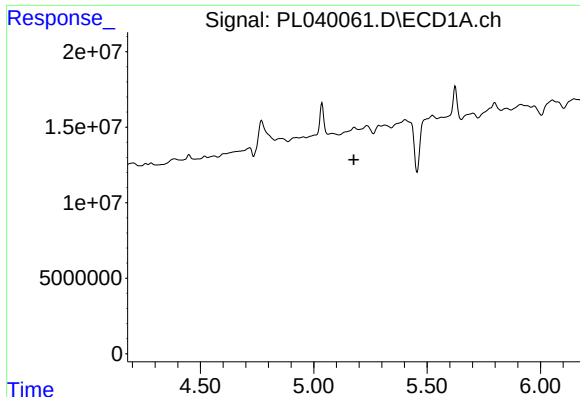

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.176 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

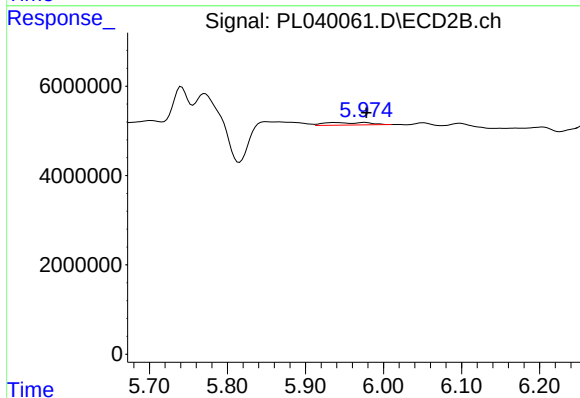


#25 Chlordane-3

R.T.: 5.976 min
Delta R.T.: -0.002 min
Response: 2367779
Conc: 4.63 ng/ml

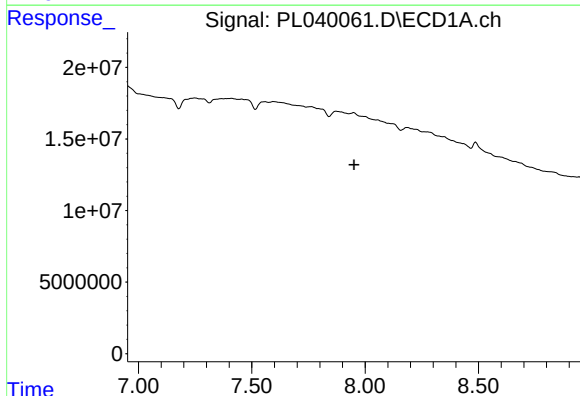

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 7.951 min
Response: 0
Conc: N.D.

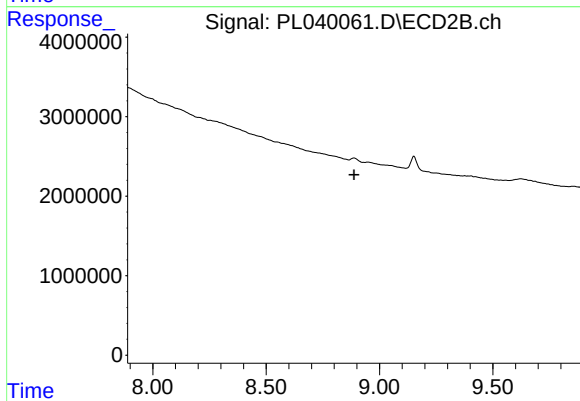

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 8.888 min
Response: 0
Conc: N.D.