

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091818\
 Data File : PL040067.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Sep 2018 08:34
 Operator : AJ\SJ
 Sample : J4947-03
 Misc :
 ALS Vial : 77 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 18 15:10:53 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 14 23:10:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.300	3.904	103.4E6	55569509	13.336	17.416 #
28)	SA Decachlor...	7.953	8.891	137.4E6	52441090	16.495	19.308
Target Compounds							
3)	MA gamma-BHC...	4.048f	0.000	70087465	0	6.124	N.D. #
4)	MA Heptachlor	4.214f	0.000	11223694	0	0.973	N.D. #
6)	B beta-BHC	4.214f	0.000	11223694	0	2.282	N.D. #
10)	B gamma-Chl...	5.200	5.954	235.0E6	9456604	21.095	2.499 #
11)	B alpha-Chl...	5.200	0.000	235.0E6	0	22.001	N.D. #
20)	A Methoxychlor	6.629f	0.000	30235386	0	6.523	N.D. #
25)	Chlordane-3	5.200	5.954	235.0E6	9456604	191.538	18.472 #
26)	Chlordane-4	5.200	0.000	235.0E6	0	214.406	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091818\
Data File : PL040067.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Sep 2018 08:34
Operator : AJ\SJ
Sample : J4947-03
Misc :
ALS Vial : 77 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 18 15:10:53 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
Quant Title : GC Extractables
QLast Update : Fri Sep 14 23:10:39 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

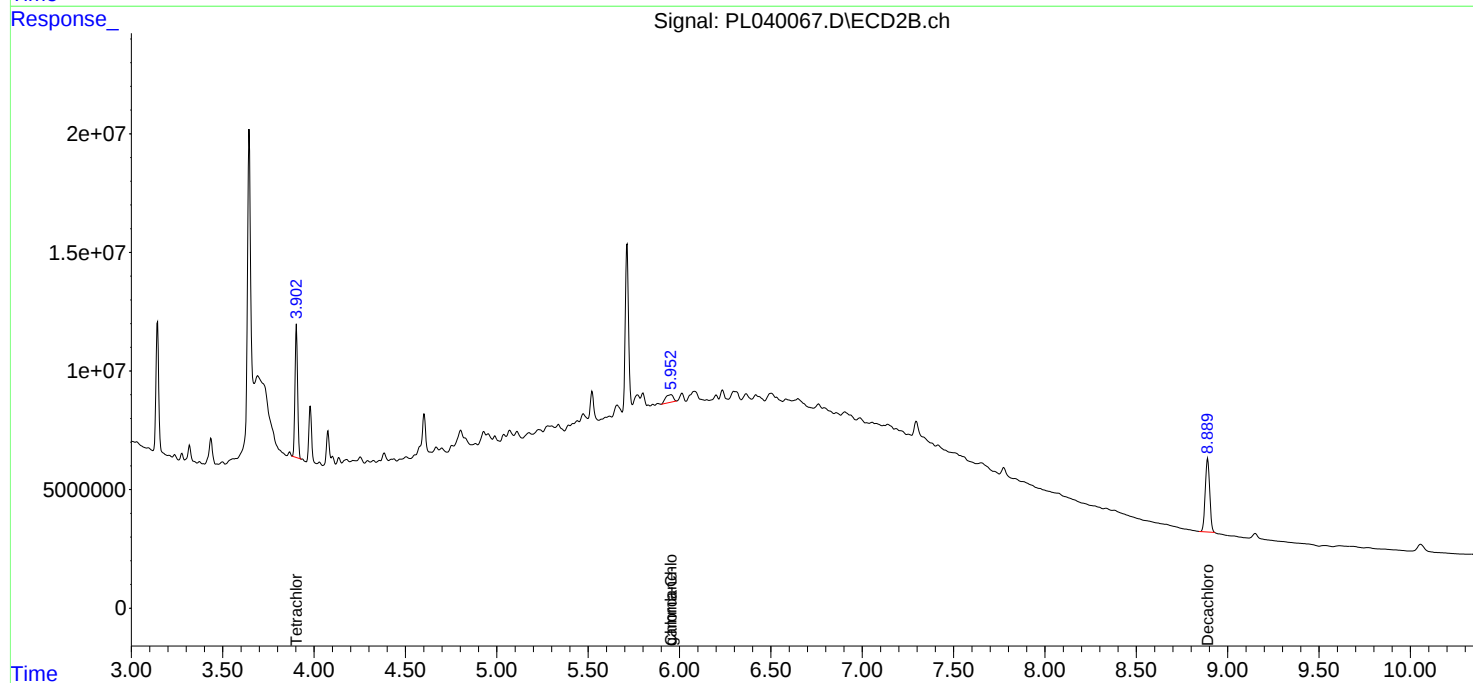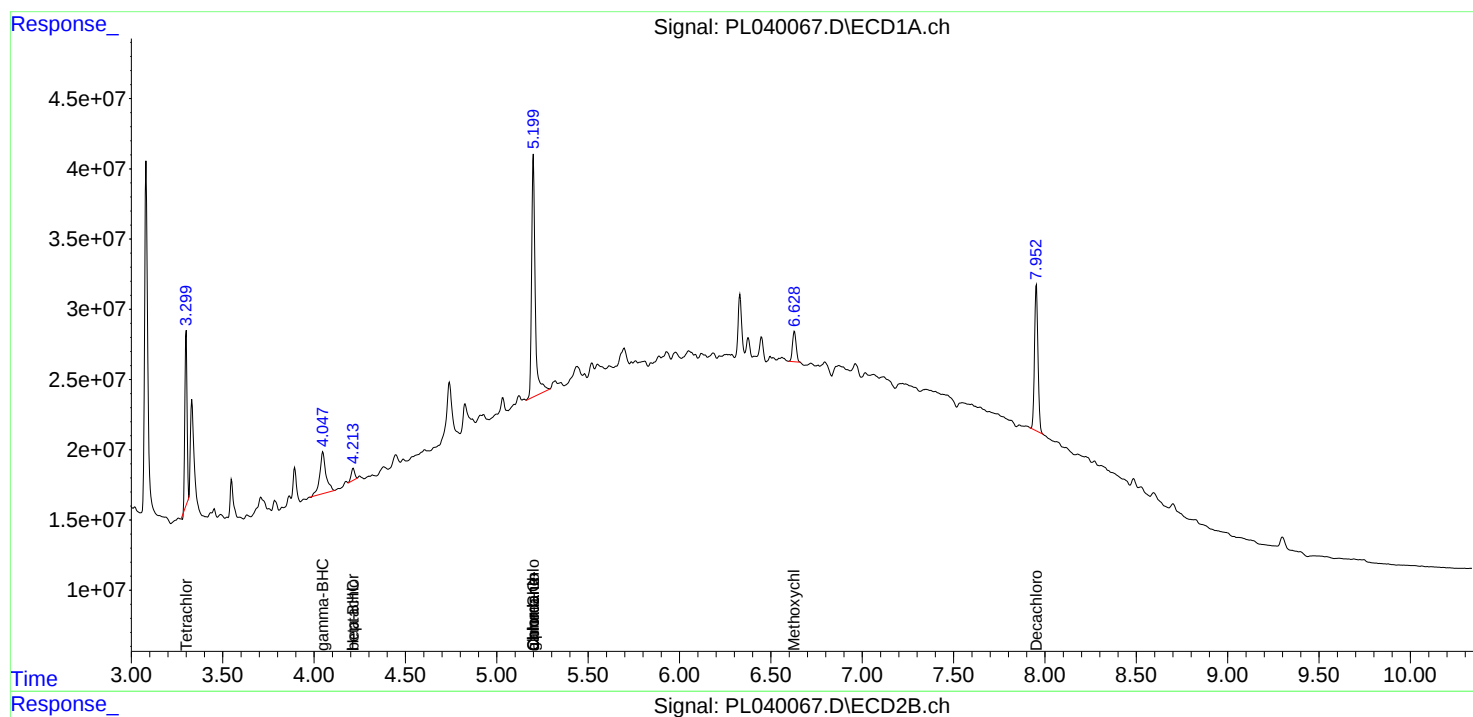


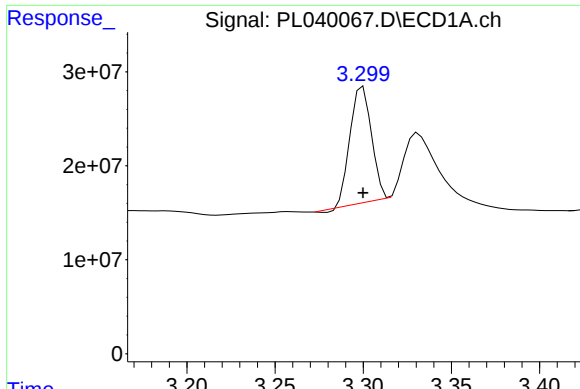

#1 Tetrachloro-m-xylene


R.T.: 3.300 min
Delta R.T.: 0.000 min
Response: 103416200
Conc: 13.34 ng/ml

Instrument :
ECD_L
ClientSampleId :

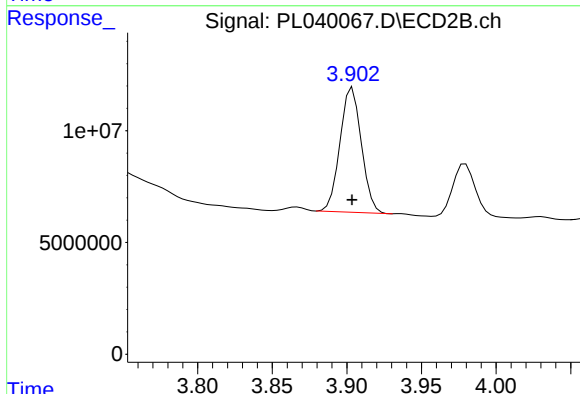


#1 Tetrachloro-m-xylene

R.T.: 3.904 min
Delta R.T.: 0.000 min
Response: 55569509
Conc: 17.42 ng/ml

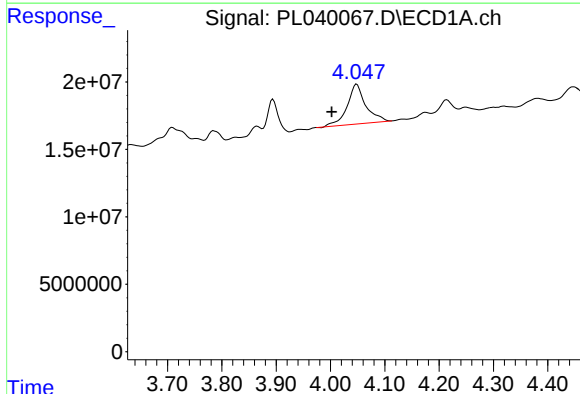


#3 gamma-BHC (Lindane)

R.T.: 4.048 min
Delta R.T.: 0.046 min
Response: 70087465
Conc: 6.12 ng/ml

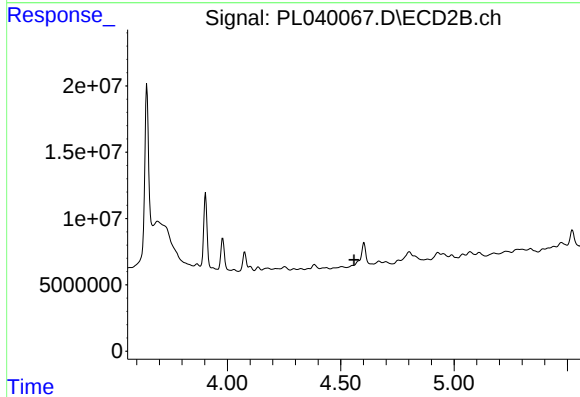

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.559 min
Response: 0
Conc: N.D.

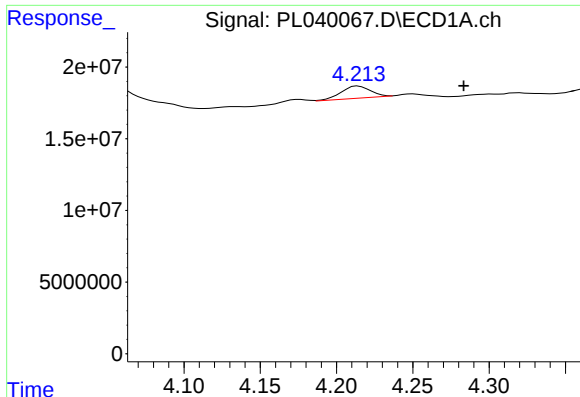

#4 Heptachlor


R.T.: 4.214 min
Delta R.T.: -0.069 min
Response: 11223694
Conc: 0.97 ng/ml

Instrument :
ECD_L
ClientSampleId :

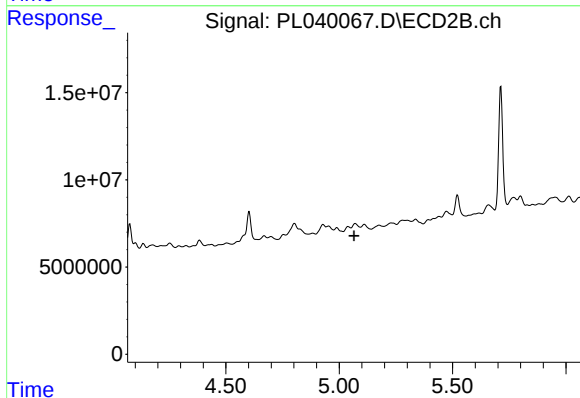


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 5.066 min
Response: 0
Conc: N.D.

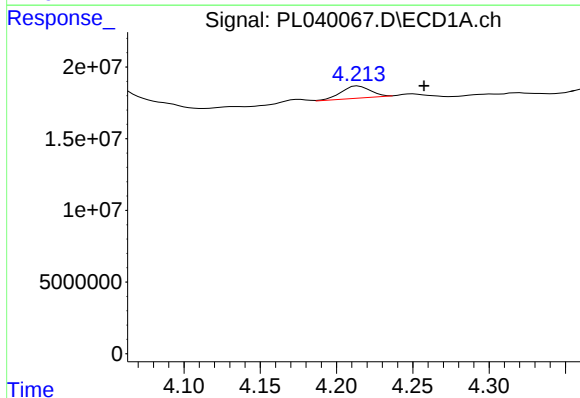


#6 beta-BHC

R.T.: 4.214 min
Delta R.T.: -0.043 min
Response: 11223694
Conc: 2.28 ng/ml

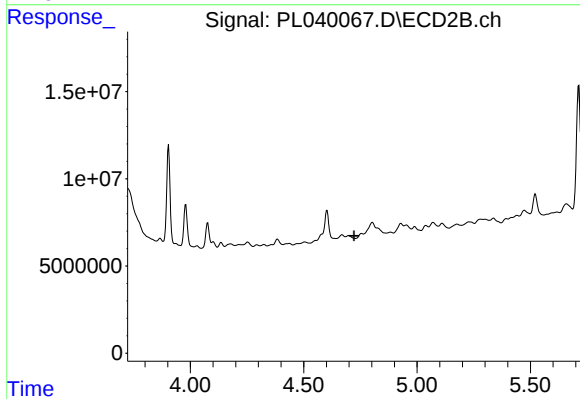

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.722 min
Response: 0
Conc: N.D.

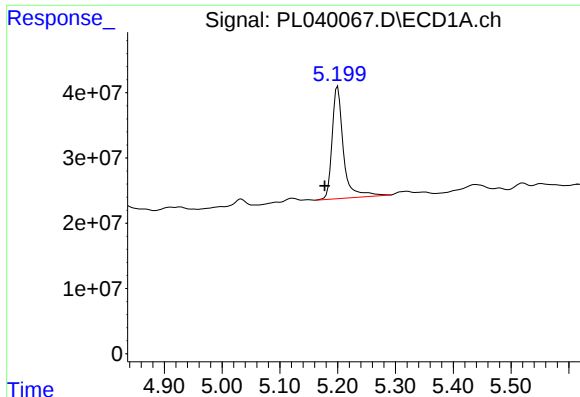

#10 gamma-Chlordane


R.T.: 5.200 min
Delta R.T.: 0.023 min
Response: 235041089
Conc: 21.09 ng/ml

Instrument :
ECD_L
ClientSampleId :

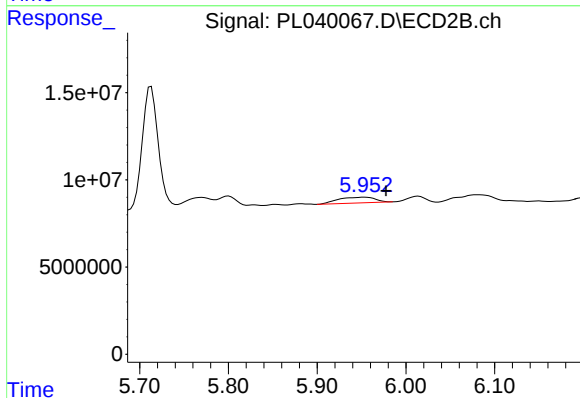


#10 gamma-Chlordane

R.T.: 5.954 min
Delta R.T.: -0.024 min
Response: 9456604
Conc: 2.50 ng/ml

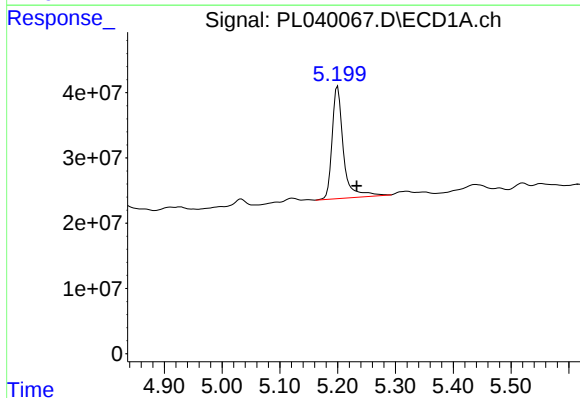


#11 alpha-Chlordane

R.T.: 5.200 min
Delta R.T.: -0.033 min
Response: 235041089
Conc: 22.00 ng/ml

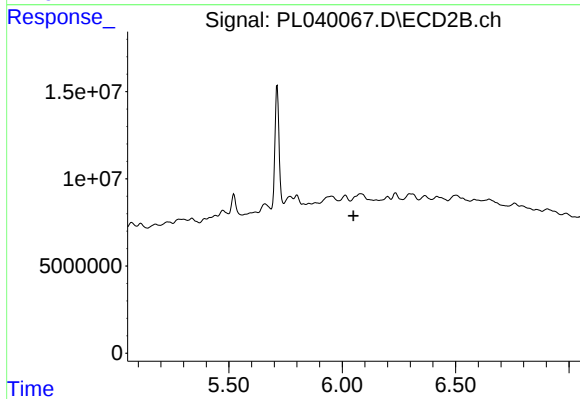

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.050 min
Response: 0
Conc: N.D.

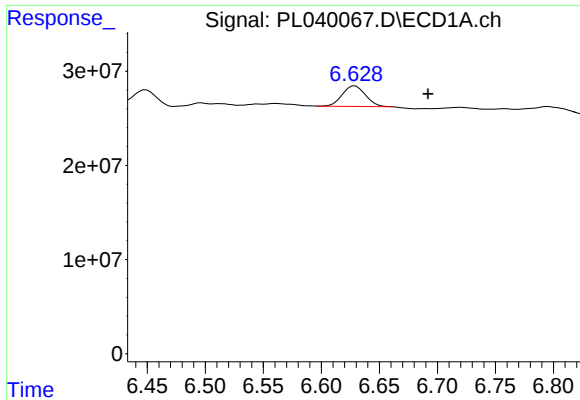

#20 Methoxychlor


R.T.: 6.629 min
Delta R.T.: -0.063 min
Response: 30235386
Conc: 6.52 ng/ml

Instrument :
ECD_L
ClientSampleId :

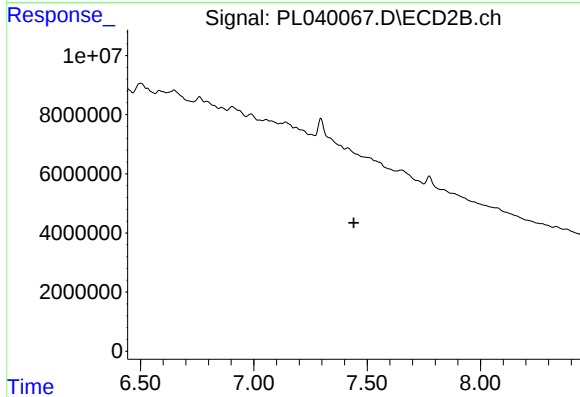


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.441 min
Response: 0
Conc: N.D.

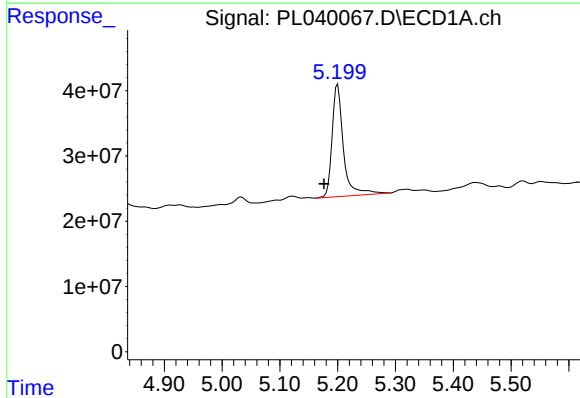


#25 Chlordane-3

R.T.: 5.200 min
Delta R.T.: 0.024 min
Response: 235041089
Conc: 191.54 ng/ml

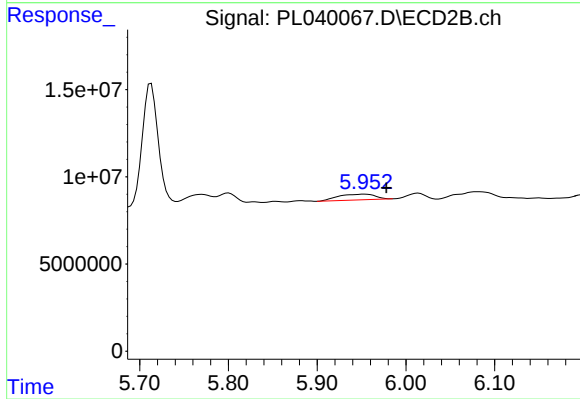

#25 Chlordane-3


R.T.: 5.954 min
Delta R.T.: -0.024 min
Response: 9456604
Conc: 18.47 ng/ml

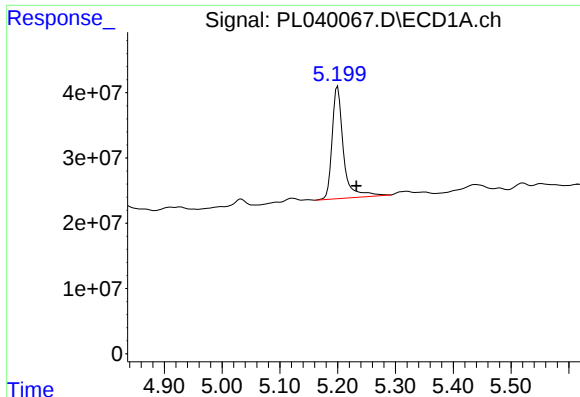

#26 Chlordane-4


R.T.: 5.200 min
Delta R.T.: -0.032 min
Response: 235041089
Conc: 214.41 ng/ml

Instrument :
ECD_L
ClientSampleId :

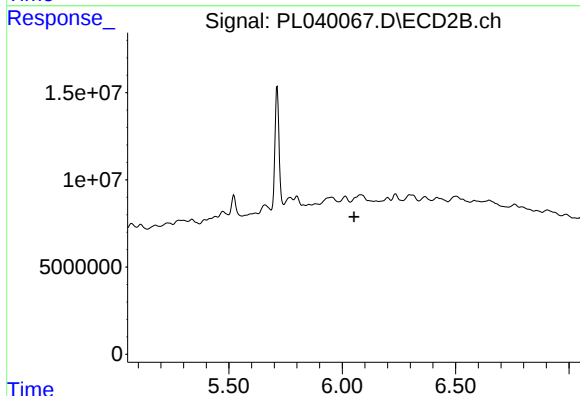


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.053 min
Response: 0
Conc: N.D.

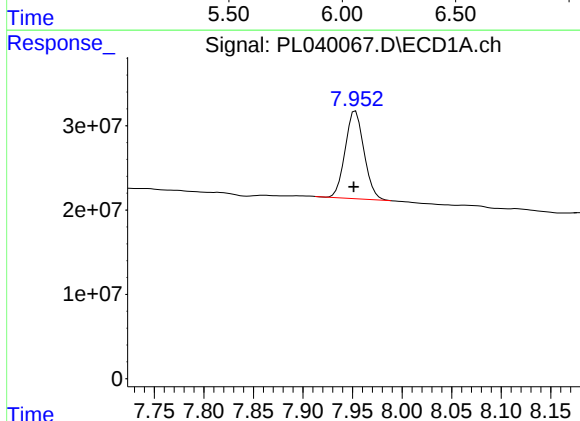

#28 Decachlorobiphenyl

R.T.: 7.953 min
Delta R.T.: 0.002 min
Response: 137442841
Conc: 16.49 ng/ml

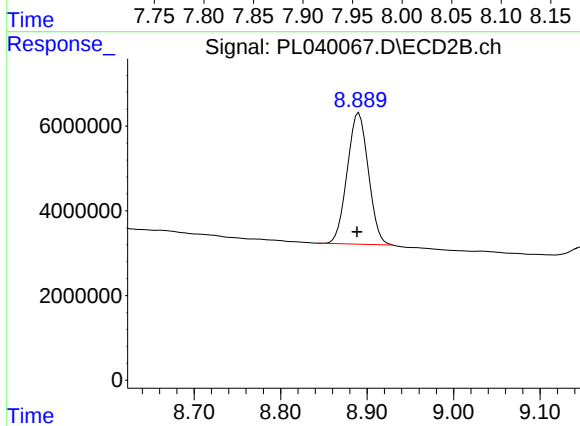

#28 Decachlorobiphenyl

R.T.: 8.891 min
Delta R.T.: 0.002 min
Response: 52441090
Conc: 19.31 ng/ml