

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091818\
 Data File : PL040090.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Sep 2018 14:35
 Operator : AJ\SJ
 Sample : J4949-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 18 15:13:48 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 14 23:10:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.304	3.906	69404928	25398900	8.950	7.960
28)	SA Decachlor...	7.955	8.893	104.8E6	31502102	12.577	11.598
Target Compounds							
7)	B delta-BHC	0.000	4.956	0	9387597	N.D.	2.360 #
8)	B Heptachlo...	0.000	5.773	0	4050578	N.D.	1.024 #
9)	A Endosulfan I	0.000	6.061f	0	4219216	N.D.	1.188 #
10)	B gamma-Chl...	0.000	5.983	0	3446638	N.D.	0.911 #
11)	B alpha-Chl...	0.000	6.061	0	4219216	N.D.	1.065 #
12)	B 4,4'-DDE	5.407	6.212	49359836	17722232	4.657	4.659
17)	MA 4,4'-DDT	6.147	6.990	44051299	8920215	4.867	2.982 #
25)	Chlordane-3	0.000	5.983	0	3446638	N.D.	6.732 #
26)	Chlordane-4	0.000	6.061	0	4219216	N.D.	6.817 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091818\
Data File : PL040090.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Sep 2018 14:35
Operator : AJ\SJ
Sample : J4949-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 18 15:13:48 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
Quant Title : GC Extractables
QLast Update : Fri Sep 14 23:10:39 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

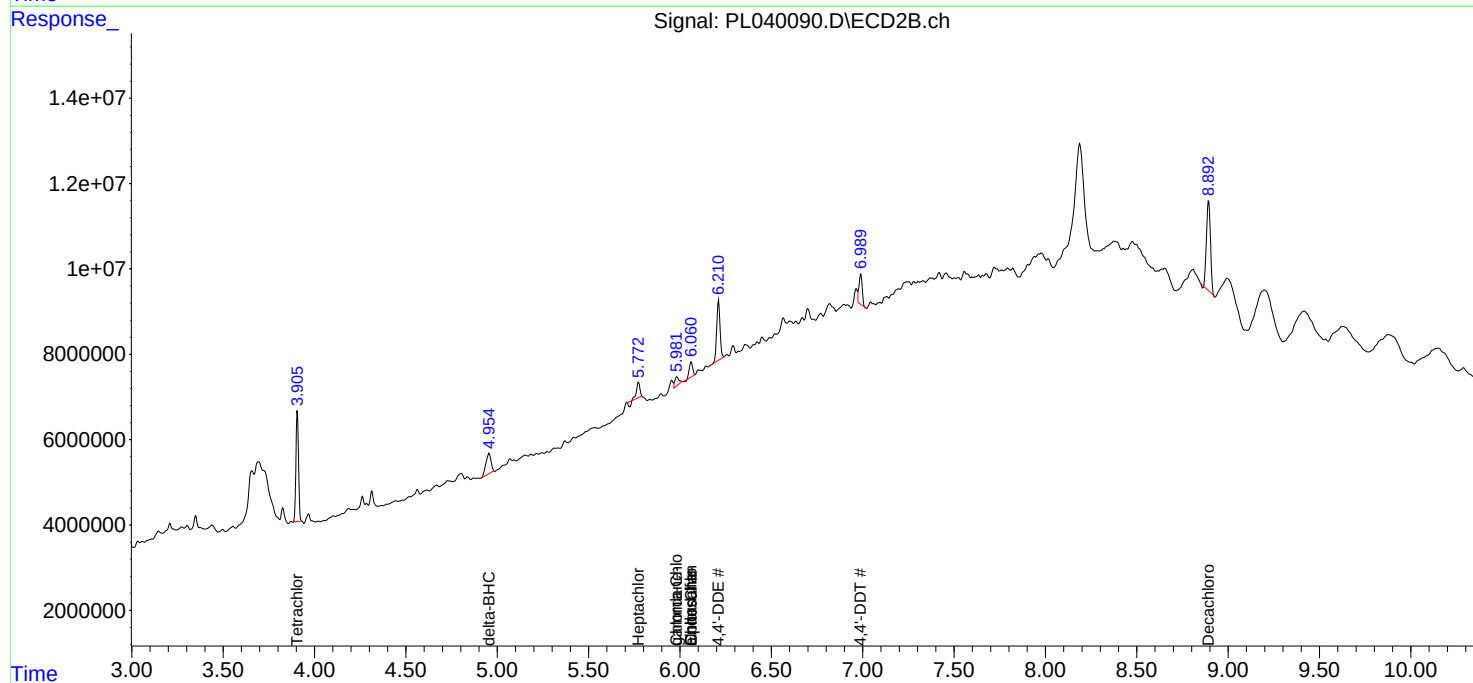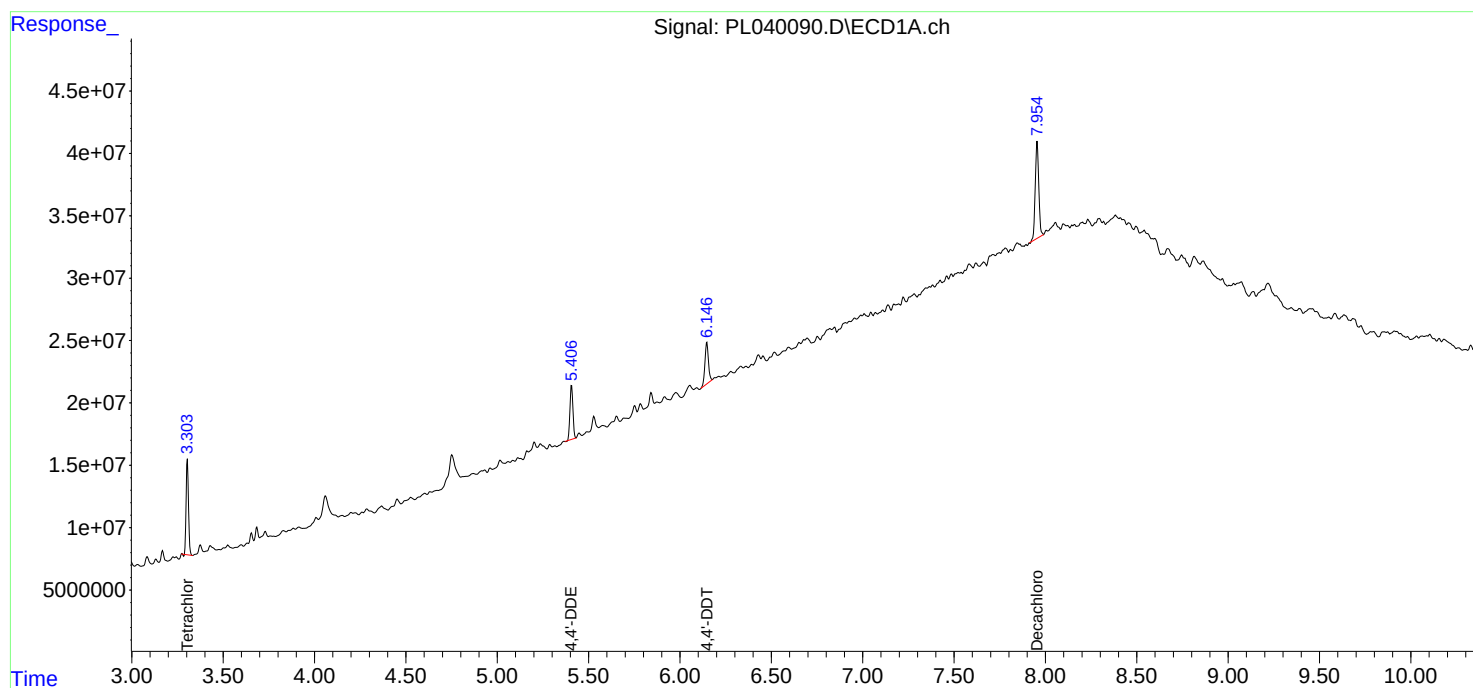


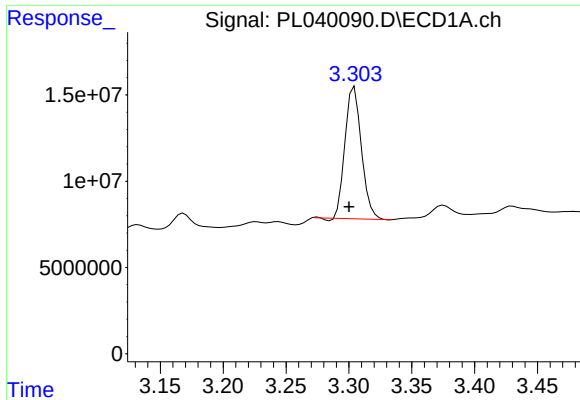

#1 Tetrachloro-m-xylene


R.T.: 3.304 min
Delta R.T.: 0.004 min
Response: 69404928
Conc: 8.95 ng/ml

Instrument :
ECD_L
ClientSampleId :

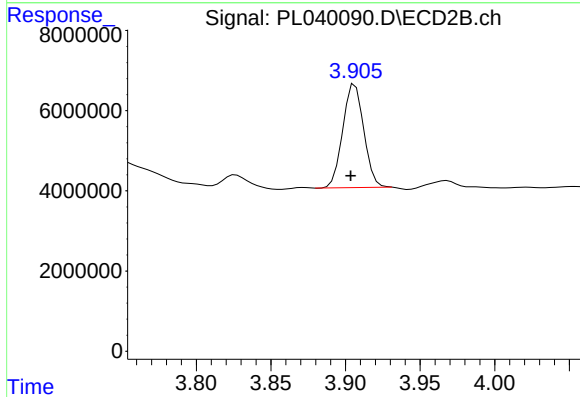


#1 Tetrachloro-m-xylene

R.T.: 3.906 min
Delta R.T.: 0.003 min
Response: 25398900
Conc: 7.96 ng/ml

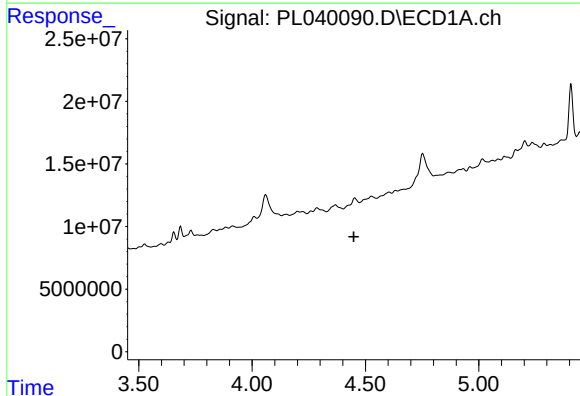


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.449 min
Response: 0
Conc: N.D.

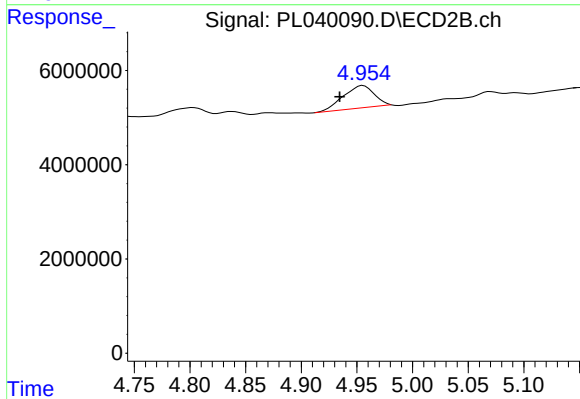

#7 delta-BHC


R.T.: 4.956 min
Delta R.T.: 0.021 min
Response: 9387597
Conc: 2.36 ng/ml

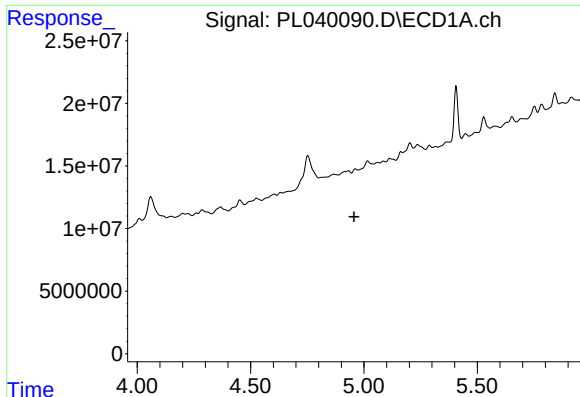

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.956 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

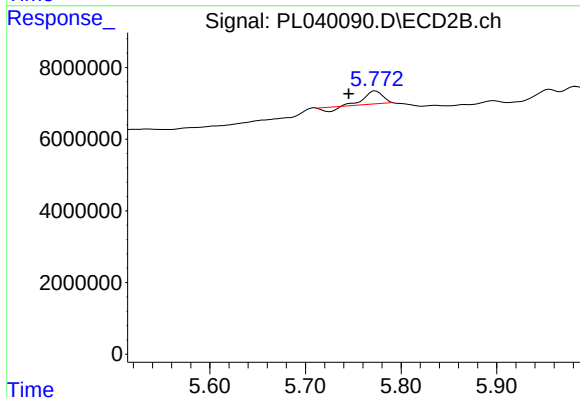


#8 Heptachlor epoxide

R.T.: 5.773 min
Delta R.T.: 0.028 min
Response: 4050578
Conc: 1.02 ng/ml

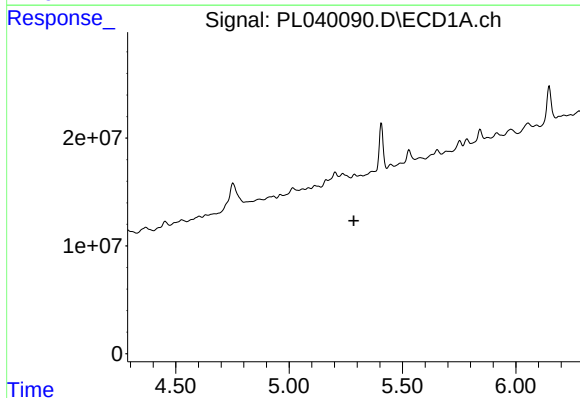


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.285 min
Response: 0
Conc: N.D.

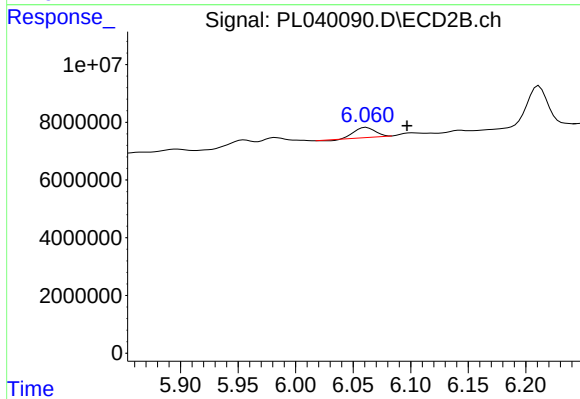

#9 Endosulfan I


R.T.: 6.061 min
Delta R.T.: -0.035 min
Response: 4219216
Conc: 1.19 ng/ml

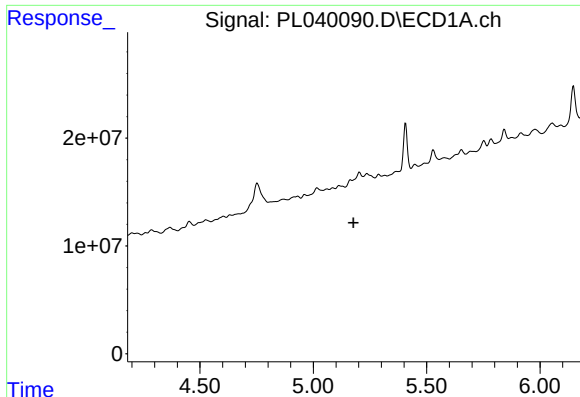

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.178 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

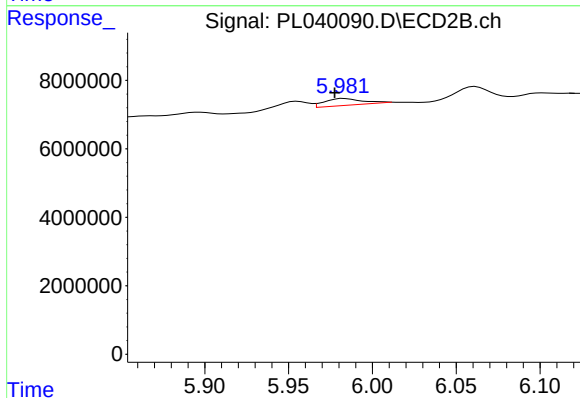


#10 gamma-Chlordane

R.T.: 5.983 min
Delta R.T.: 0.005 min
Response: 3446638
Conc: 0.91 ng/ml

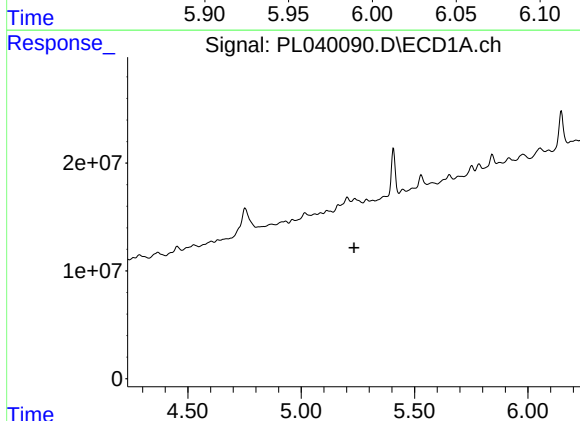


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.233 min
Response: 0
Conc: N.D.

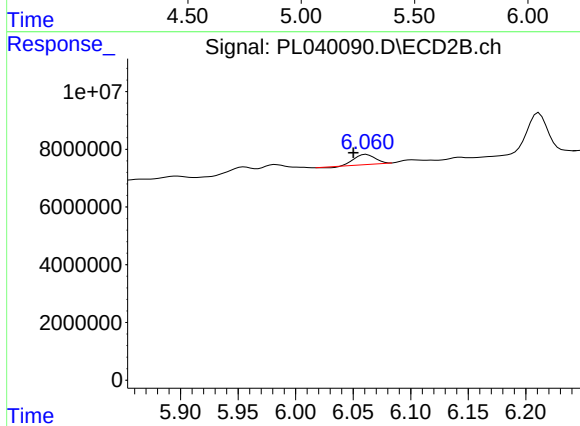

#11 alpha-Chlordane


R.T.: 6.061 min
Delta R.T.: 0.011 min
Response: 4219216
Conc: 1.07 ng/ml

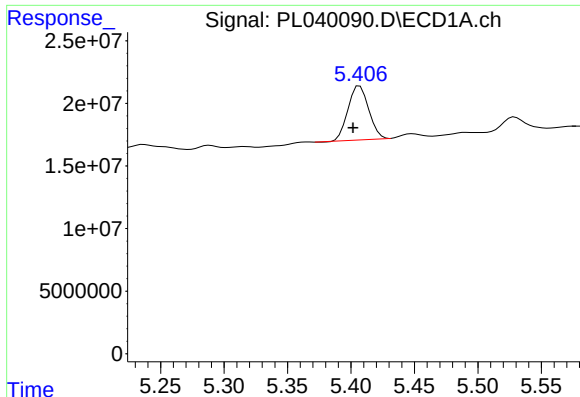

#12 4,4'-DDE


R.T.: 5.407 min
Delta R.T.: 0.005 min
Response: 49359836
Conc: 4.66 ng/ml

Instrument :
ECD_L
ClientSampleId :

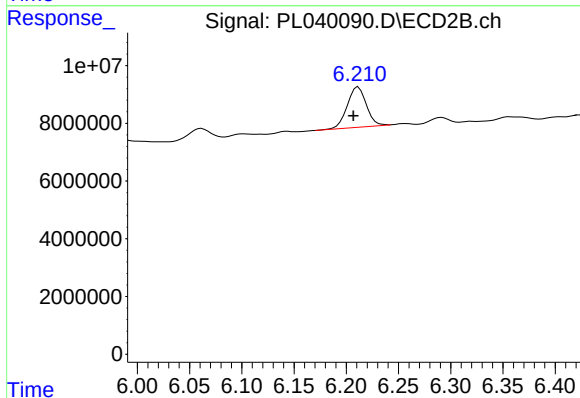


#12 4,4'-DDE

R.T.: 6.212 min
Delta R.T.: 0.005 min
Response: 17722232
Conc: 4.66 ng/ml

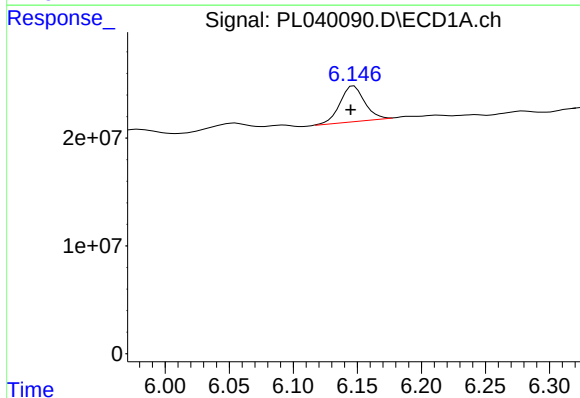


#17 4,4'-DDT

R.T.: 6.147 min
Delta R.T.: 0.003 min
Response: 44051299
Conc: 4.87 ng/ml

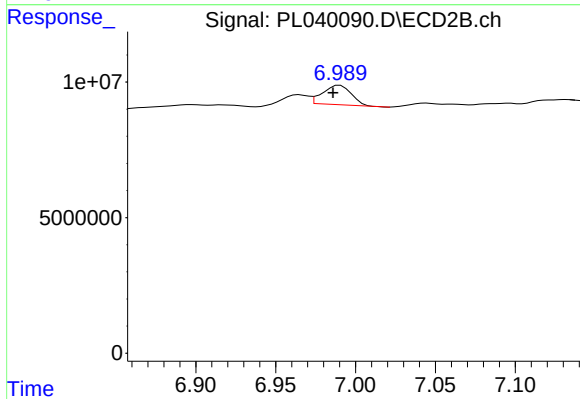

#17 4,4'-DDT


R.T.: 6.990 min
Delta R.T.: 0.004 min
Response: 8920215
Conc: 2.98 ng/ml

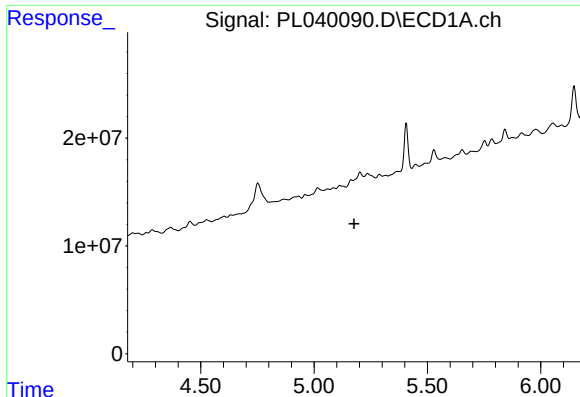

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.176 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

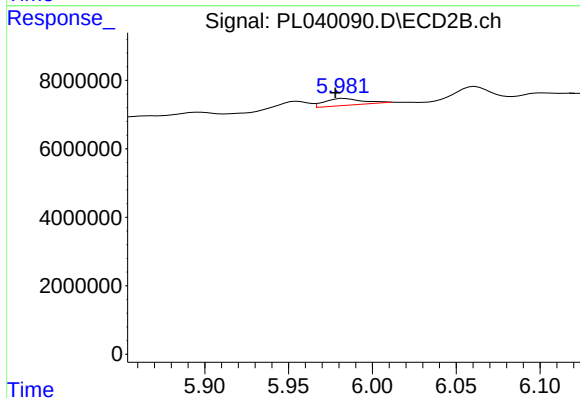


#25 Chlordane-3

R.T.: 5.983 min
Delta R.T.: 0.005 min
Response: 3446638
Conc: 6.73 ng/ml

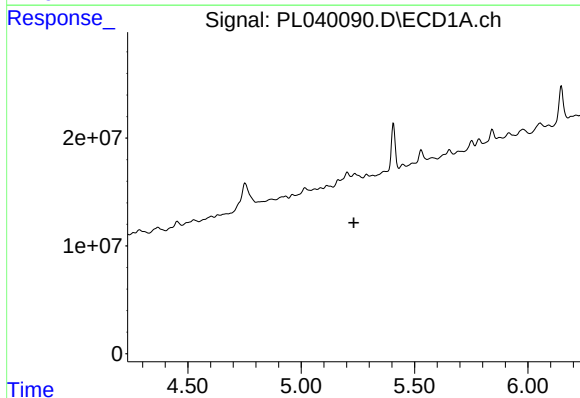


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.232 min
Response: 0
Conc: N.D.

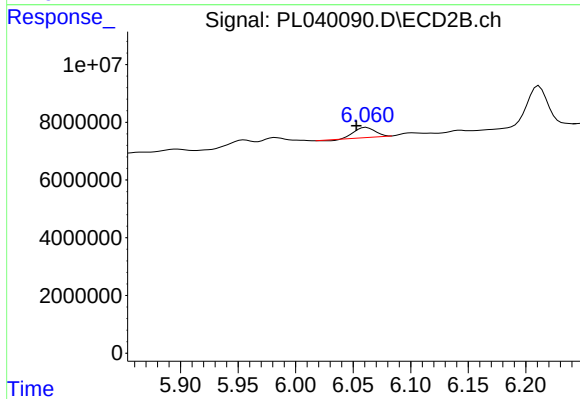

#26 Chlordane-4


R.T.: 6.061 min
Delta R.T.: 0.009 min
Response: 4219216
Conc: 6.82 ng/ml

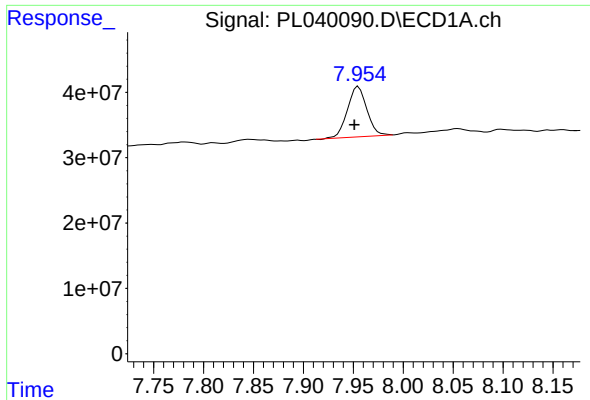

#28 Decachlorobiphenyl

R.T.: 7.955 min
Delta R.T.: 0.004 min
Response: 104800566
Conc: 12.58 ng/ml

Instrument :
ECD_L
ClientSampleId :

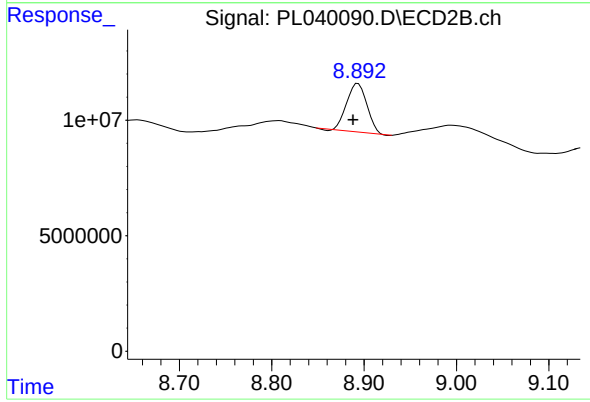

#28 Decachlorobiphenyl

R.T.: 8.893 min
Delta R.T.: 0.005 min
Response: 31502102
Conc: 11.60 ng/ml