

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091818\
 Data File : PL040093.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Sep 2018 15:17
 Operator : AJ\SJ
 Sample : J4952-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 18 16:01:10 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 14 23:10:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.300	3.904	104.7E6	44757132	13.502	14.027
28)	SA Decachlor...	7.954	8.893	109.0E6	39088398	13.083	14.392
Target Compounds							
8)	B Heptachlo...	0.000	5.772	0	5029315	N.D.	1.272 #
9)	A Endosulfan I	5.234f	6.056f	20348964	10580140	2.054	2.979 #
10)	B gamma-Chl...	5.198	0.000	39714863	0	3.564	N.D. #
11)	B alpha-Chl...	5.234	6.056	20348964	10580140	1.905	2.671 #
25)	Chlordane-3	5.198	0.000	39714863	0	32.364	N.D. #
26)	Chlordane-4	5.234	6.056	20348964	10580140	18.562	17.093



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091818\
Data File : PL040093.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Sep 2018 15:17
Operator : AJ\SJ
Sample : J4952-01
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 18 16:01:10 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
Quant Title : GC Extractables
QLast Update : Fri Sep 14 23:10:39 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

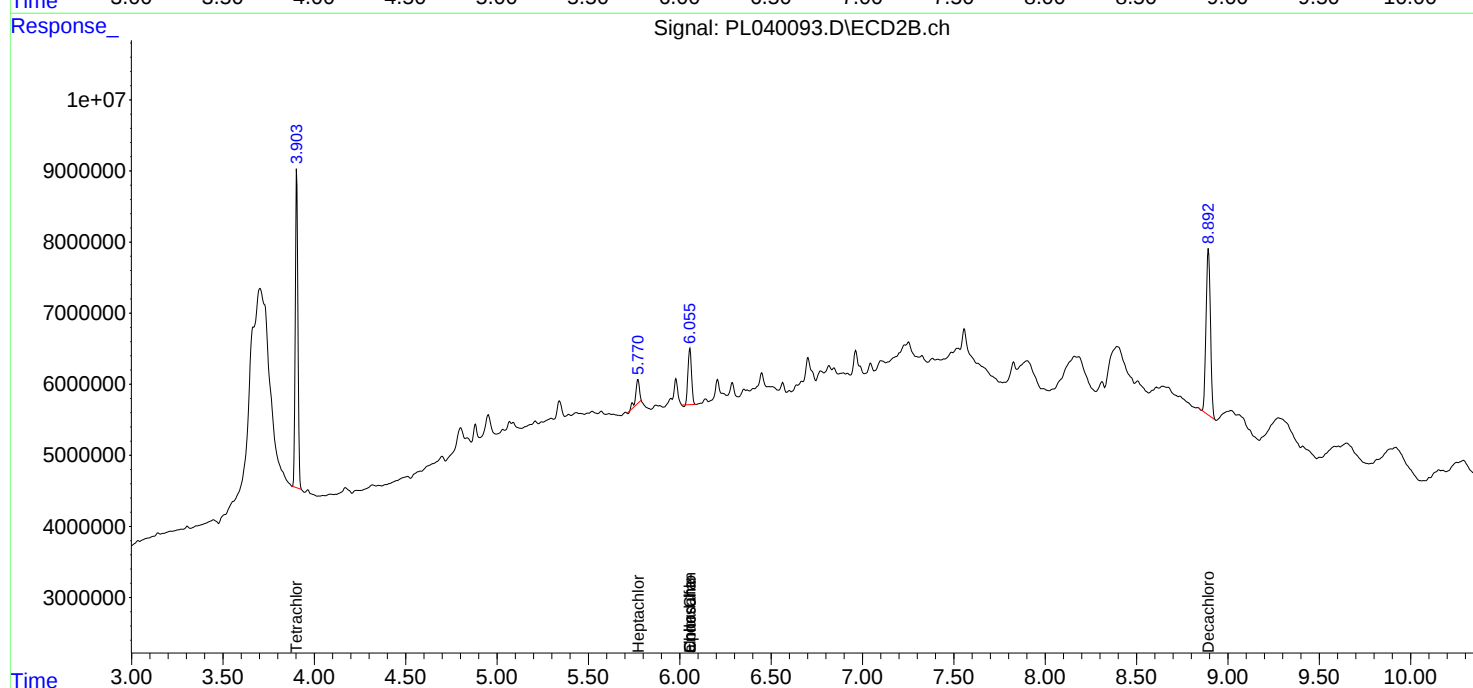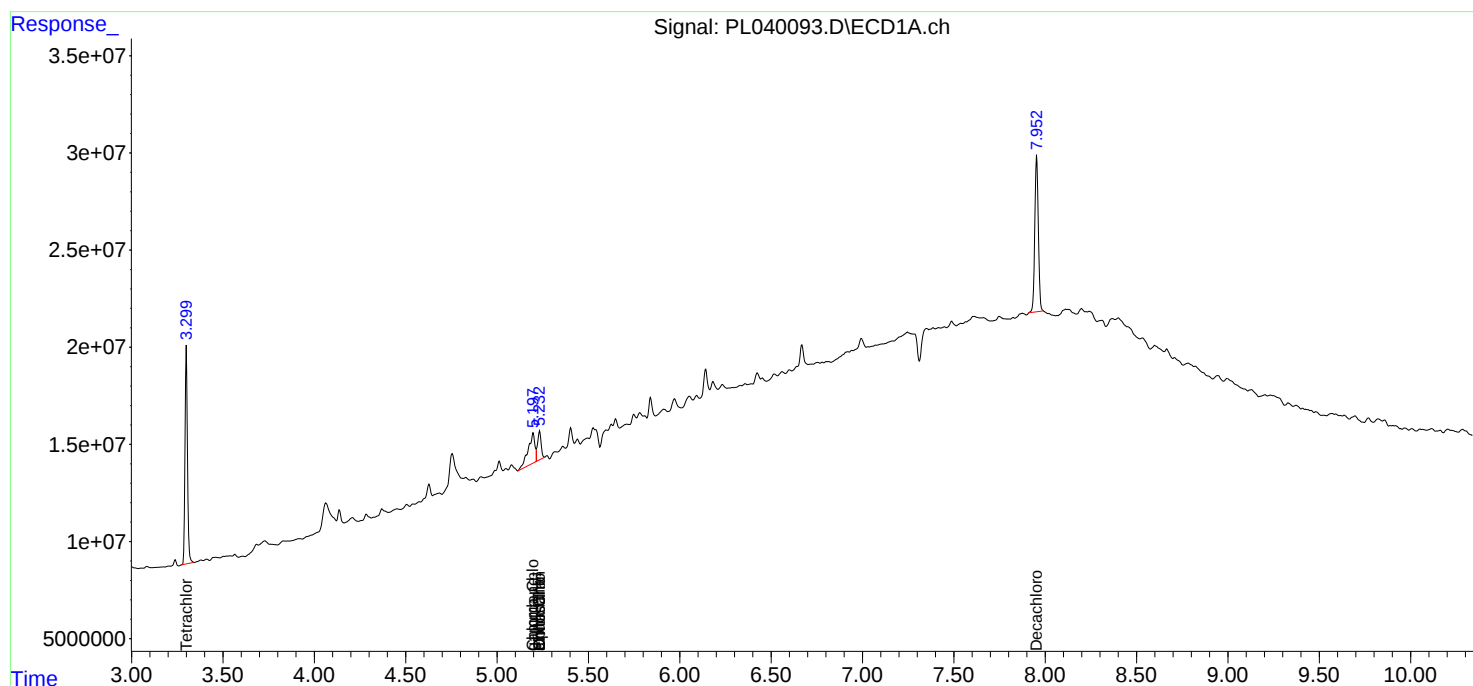


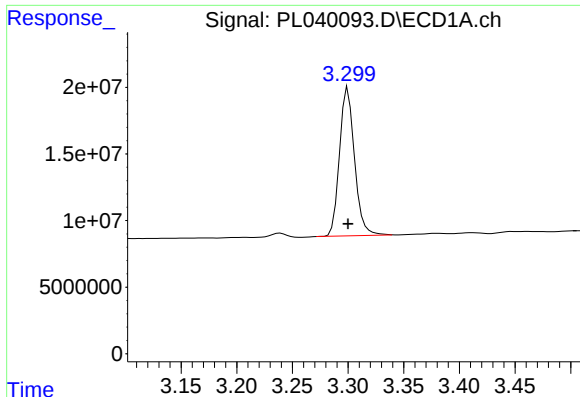

#1 Tetrachloro-m-xylene


R.T.: 3.300 min
Delta R.T.: 0.000 min
Response: 104708734
Conc: 13.50 ng/ml

Instrument :
ECD_L
ClientSampleId :

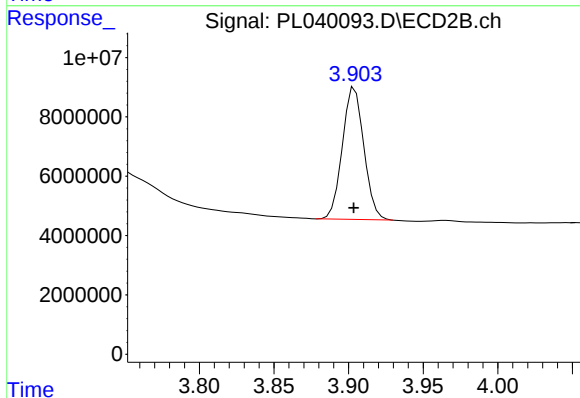


#1 Tetrachloro-m-xylene

R.T.: 3.904 min
Delta R.T.: 0.000 min
Response: 44757132
Conc: 14.03 ng/ml

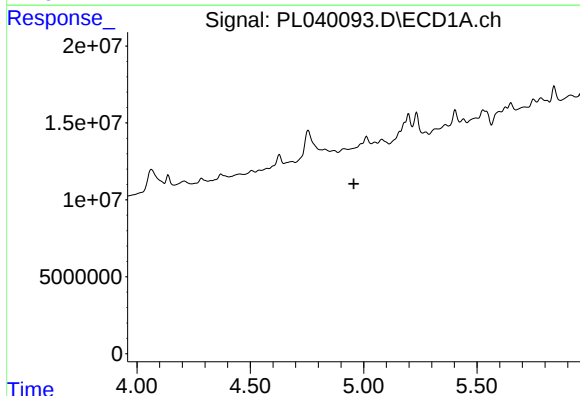


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.956 min
Response: 0
Conc: N.D.

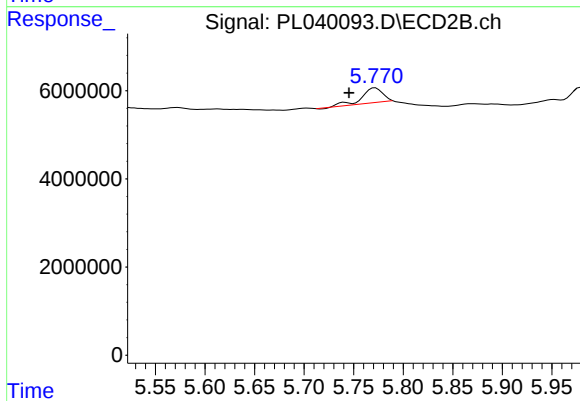

#8 Heptachlor epoxide


R.T.: 5.772 min
Delta R.T.: 0.027 min
Response: 5029315
Conc: 1.27 ng/ml

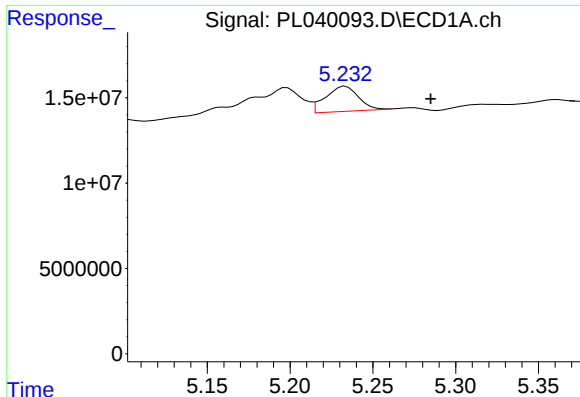

#9 Endosulfan I


R.T.: 5.234 min
Delta R.T.: -0.051 min
Response: 20348964
Conc: 2.05 ng/ml

Instrument :
ECD_L
ClientSampleId :

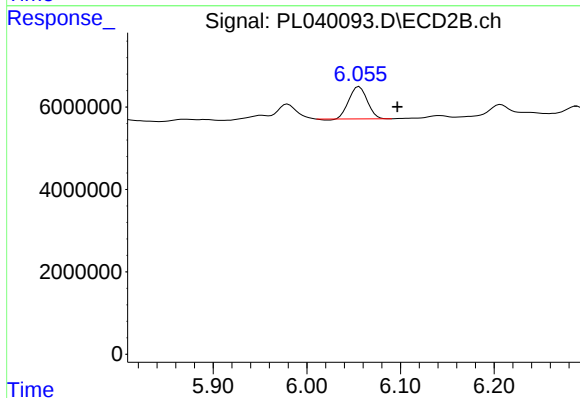


#9 Endosulfan I

R.T.: 6.056 min
Delta R.T.: -0.041 min
Response: 10580140
Conc: 2.98 ng/ml

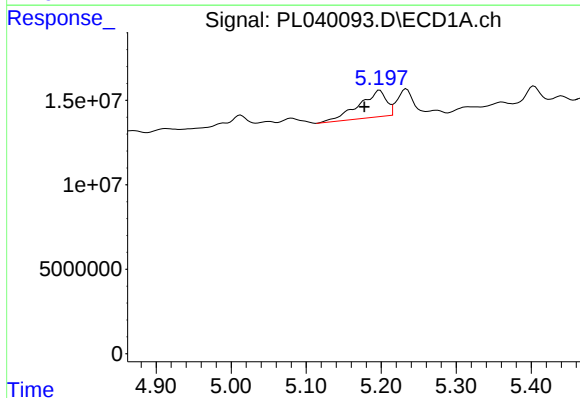


#10 gamma-Chlordane

R.T.: 5.198 min
Delta R.T.: 0.021 min
Response: 39714863
Conc: 3.56 ng/ml

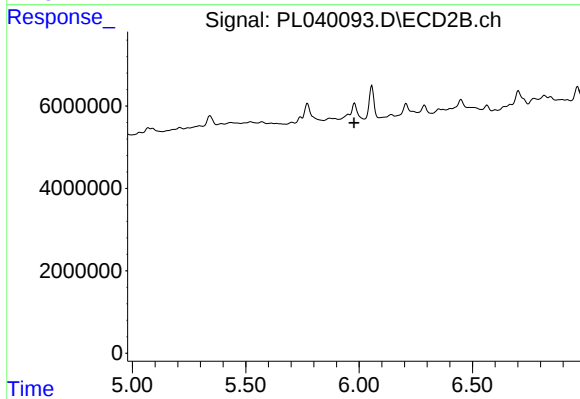

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.978 min
Response: 0
Conc: N.D.

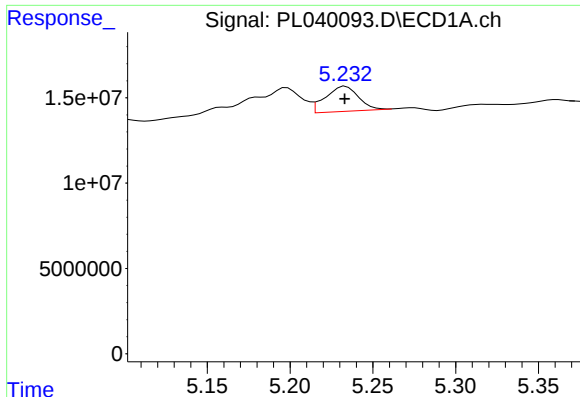

#11 alpha-Chlordane


R.T.: 5.234 min
Delta R.T.: 0.000 min
Response: 20348964
Conc: 1.90 ng/ml

Instrument :
ECD_L
ClientSampleId :

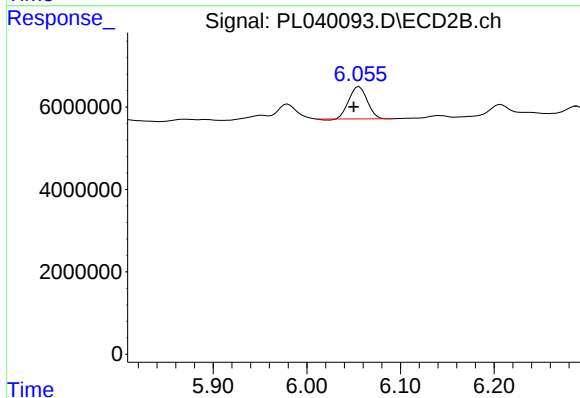


#11 alpha-Chlordane

R.T.: 6.056 min
Delta R.T.: 0.006 min
Response: 10580140
Conc: 2.67 ng/ml

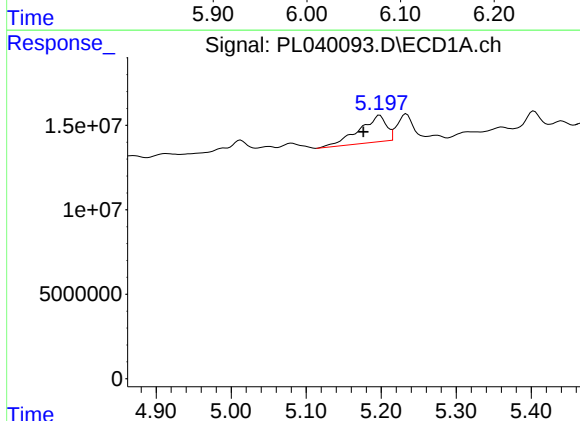


#25 Chlordane-3

R.T.: 5.198 min
Delta R.T.: 0.022 min
Response: 39714863
Conc: 32.36 ng/ml

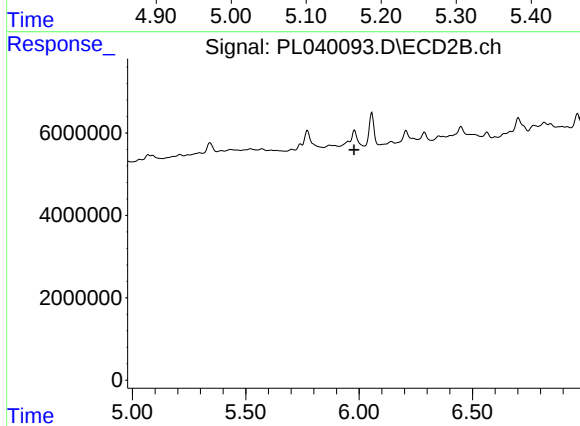

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.978 min
Response: 0
Conc: N.D.

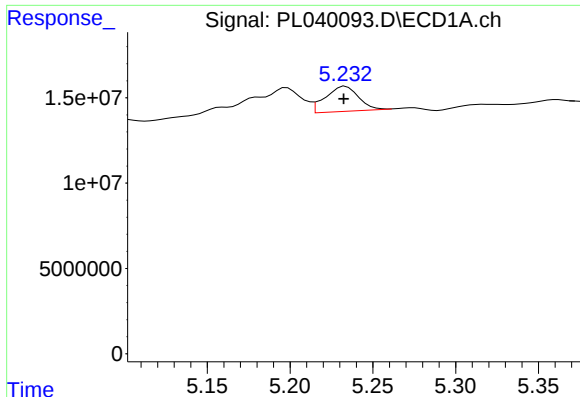

#26 Chlordane-4


R.T.: 5.234 min
Delta R.T.: 0.001 min
Response: 20348964
Conc: 18.56 ng/ml

Instrument :
ECD_L
ClientSampleId :

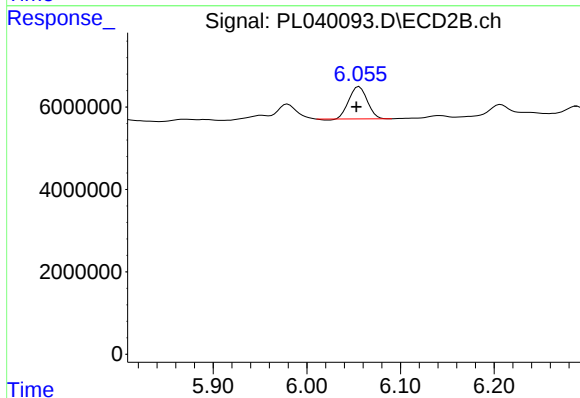


#26 Chlordane-4

R.T.: 6.056 min
Delta R.T.: 0.003 min
Response: 10580140
Conc: 17.09 ng/ml

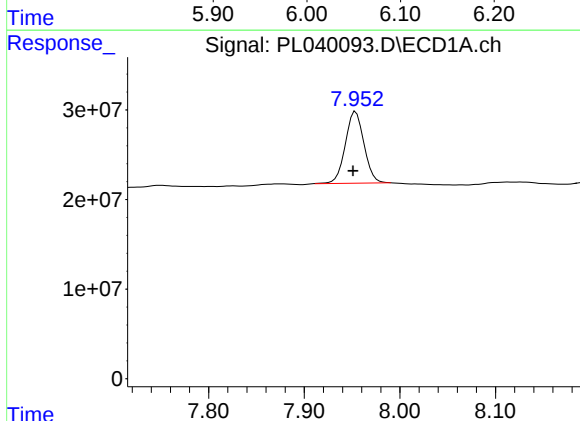

#28 Decachlorobiphenyl

R.T.: 7.954 min
Delta R.T.: 0.003 min
Response: 109017978
Conc: 13.08 ng/ml

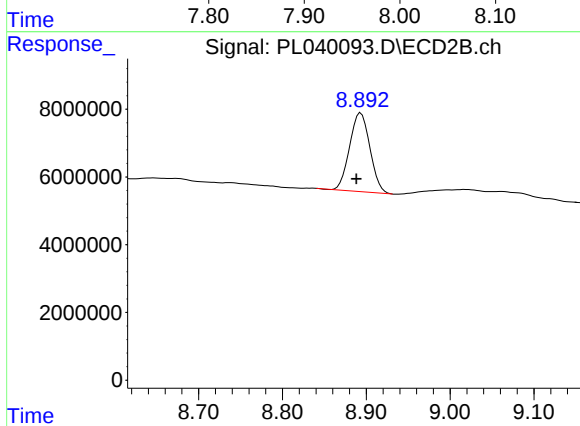

#28 Decachlorobiphenyl

R.T.: 8.893 min
Delta R.T.: 0.005 min
Response: 39088398
Conc: 14.39 ng/ml