

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091818\
 Data File : PL040105.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Sep 2018 18:28
 Operator : AJ\SJ
 Sample : J4702-01
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 19 01:10:54 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 14 23:10:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.300	3.904	110.7E6	36475785	14.269	11.432
28)	SA Decachlor...	7.953	8.893	88204784	36167913	10.585	13.316 #
Target Compounds							
7)	B delta-BHC	0.000	4.953	0	7447672	N.D.	1.872 #
8)	B Heptachlo...	0.000	5.773	0	2004348	N.D.	0.507 #
10)	B gamma-Chl...	0.000	5.976	0	2853375	N.D.	0.754 #
24)	Chlordane-2	4.660	0.000	36733286	0	97.535	N.D. #
25)	Chlordane-3	0.000	5.976	0	2853375	N.D.	5.574 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091818\
Data File : PL040105.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Sep 2018 18:28
Operator : AJ\SJ
Sample : J4702-01
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 19 01:10:54 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
Quant Title : GC Extractables
QLast Update : Fri Sep 14 23:10:39 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

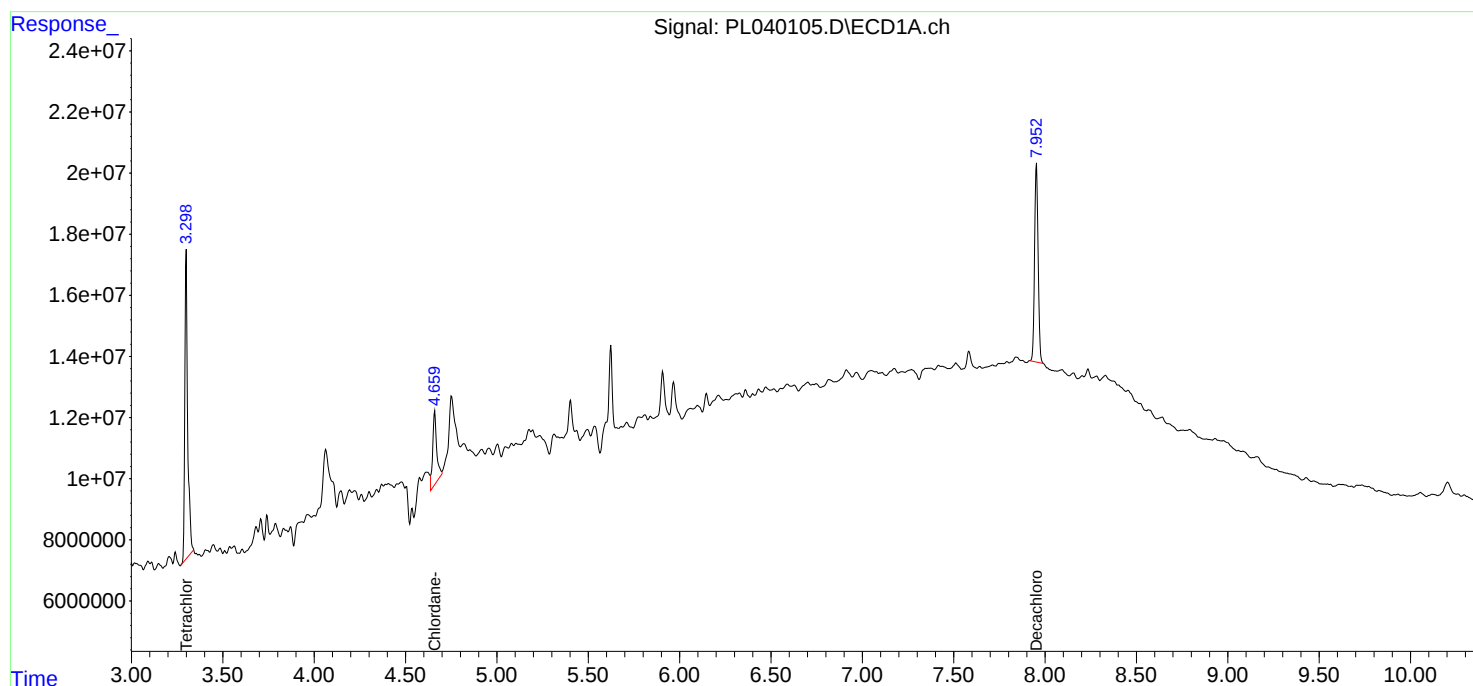


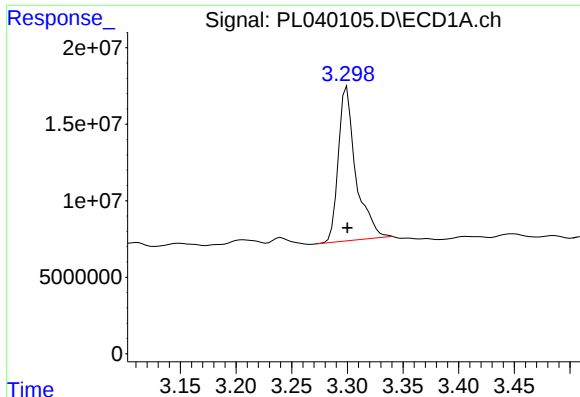

#1 Tetrachloro-m-xylene


R.T.: 3.300 min
Delta R.T.: 0.000 min
Response: 110656304
Conc: 14.27 ng/ml

Instrument :
ECD_L
ClientSampleId :

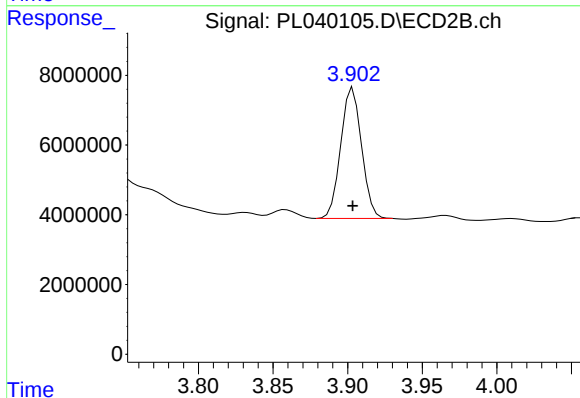


#1 Tetrachloro-m-xylene

R.T.: 3.904 min
Delta R.T.: 0.000 min
Response: 36475785
Conc: 11.43 ng/ml

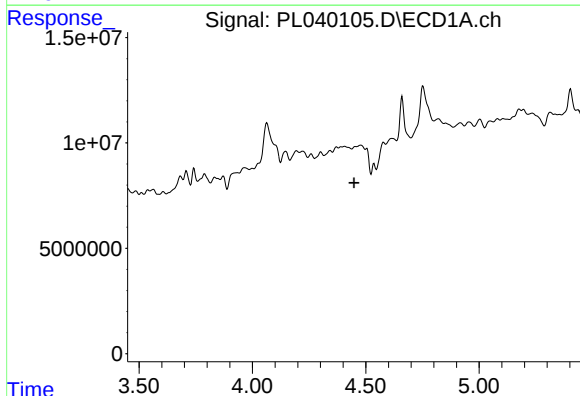


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.449 min
Response: 0
Conc: N.D.

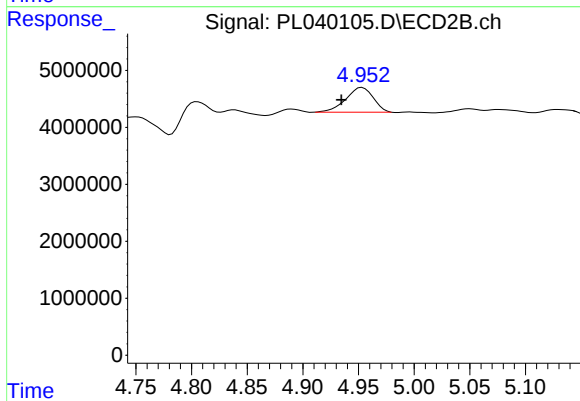

#7 delta-BHC


R.T.: 4.953 min
Delta R.T.: 0.019 min
Response: 7447672
Conc: 1.87 ng/ml

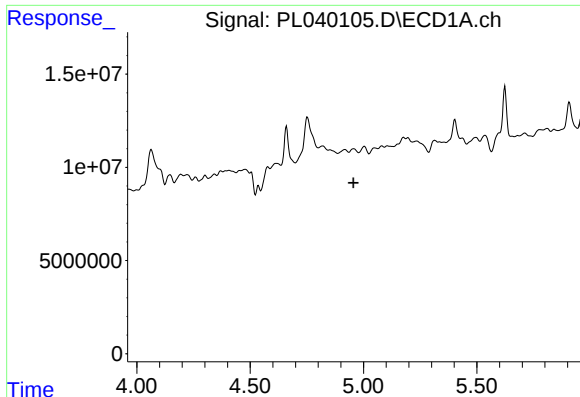

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.956 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

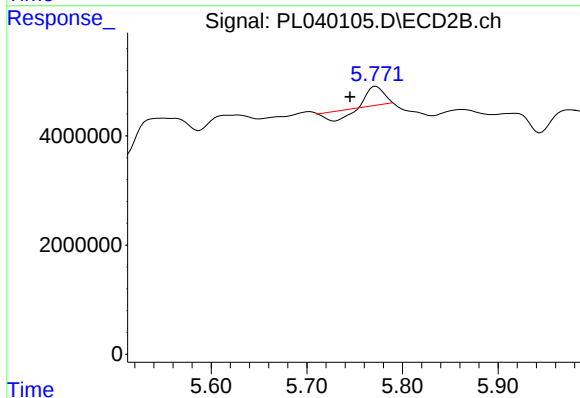


#8 Heptachlor epoxide

R.T.: 5.773 min
Delta R.T.: 0.027 min
Response: 2004348
Conc: 0.51 ng/ml

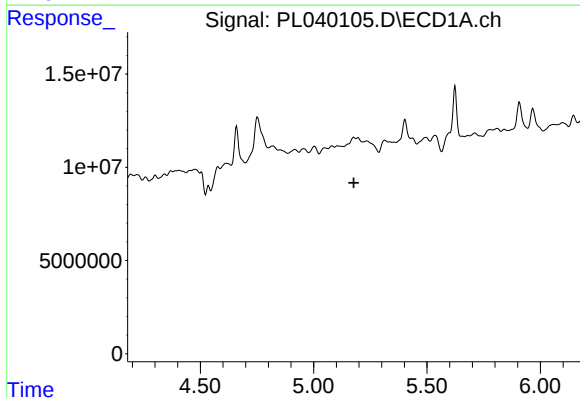


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.178 min
Response: 0
Conc: N.D.

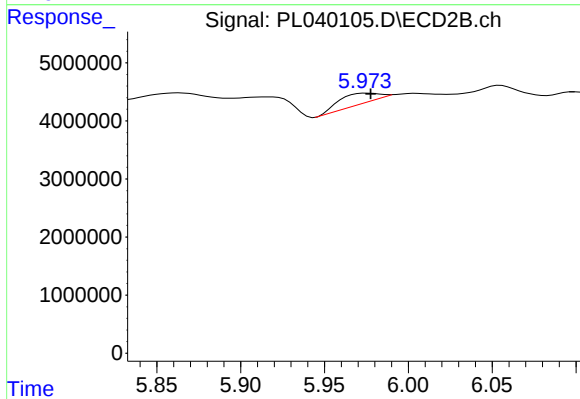

#10 gamma-Chlordane


R.T.: 5.976 min
Delta R.T.: -0.002 min
Response: 2853375
Conc: 0.75 ng/ml

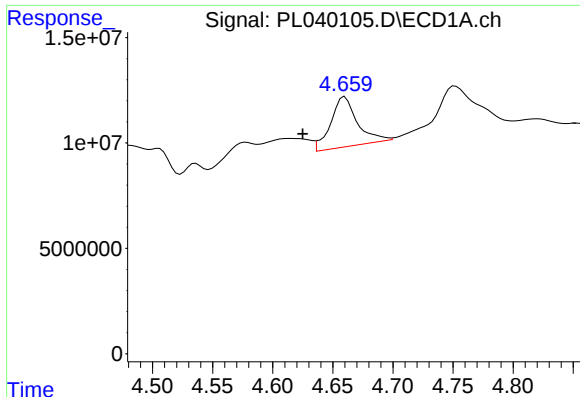

#24 Chlordane-2


R.T.: 4.660 min
Delta R.T.: 0.035 min
Response: 36733286
Conc: 97.53 ng/ml

Instrument :
ECD_L
ClientSampleId :

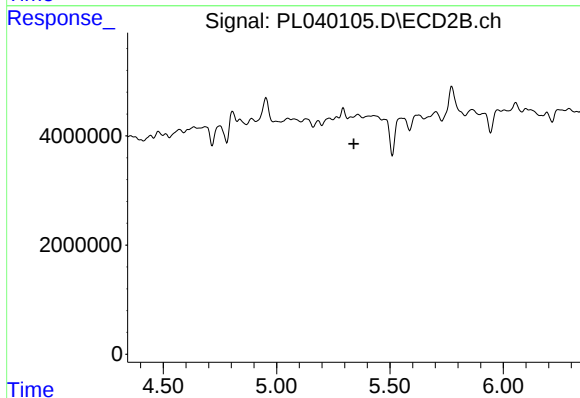


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.341 min
Response: 0
Conc: N.D.

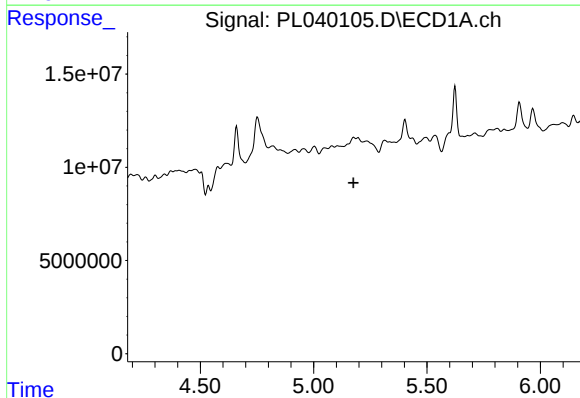


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.176 min
Response: 0
Conc: N.D.

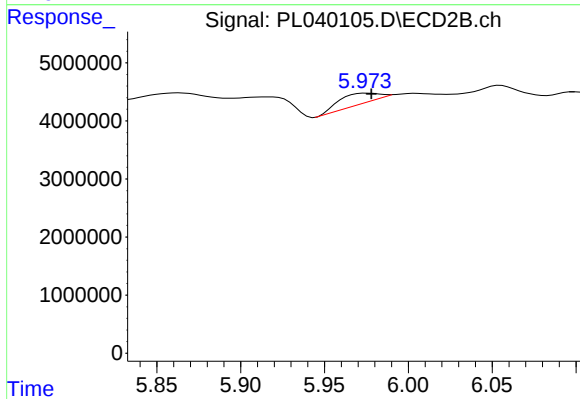

#25 Chlordane-3


R.T.: 5.976 min
Delta R.T.: -0.002 min
Response: 2853375
Conc: 5.57 ng/ml

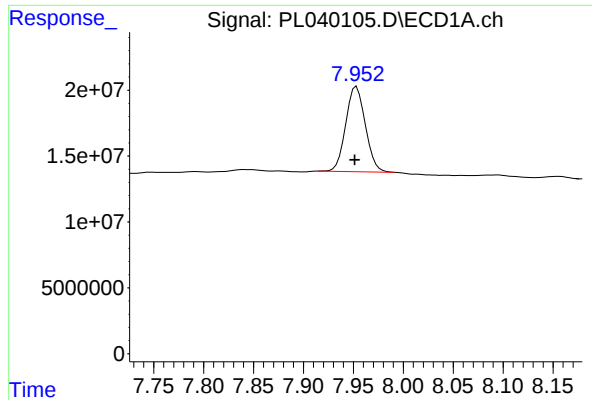

#28 Decachlorobiphenyl

R.T.: 7.953 min
Delta R.T.: 0.002 min
Response: 88204784
Conc: 10.59 ng/ml

Instrument :
ECD_L
ClientSampleId :

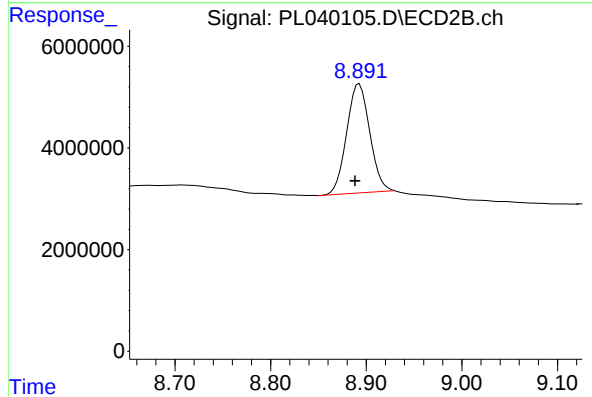

#28 Decachlorobiphenyl

R.T.: 8.893 min
Delta R.T.: 0.005 min
Response: 36167913
Conc: 13.32 ng/ml