

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091818\
 Data File : PL040109.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Sep 2018 19:25
 Operator : AJ\SJ
 Sample : J4941-01DL 5X
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 19 01:11:33 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 14 23:10:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	0.000	3.903	0	6147897	N.D.	1.927 #
28)	SA Decachlor...	0.000	8.892	0	7513473	N.D.	2.766 #
Target Compounds							
10)	B gamma-Chl...	5.184	5.951	20994756	7184429	1.884	1.898
11)	B alpha-Chl...	5.184f	0.000	20994756	0	1.965	N.D. #
12)	B 4,4'-DDE	5.403	6.209	155.9E6	55796016	14.711	14.669
13)	MA Dieldrin	5.552	6.305f	80491293	19331698	7.258	5.080 #
16)	A 4,4'-DDD	5.914	6.690	345.9E6	121.1E6	39.902	41.881
17)	MA 4,4'-DDT	6.147	6.989	424.9E6	146.9E6	46.943	49.103
25)	Chlordane-3	5.184	5.951	20994756	7184429	17.109	14.034
26)	Chlordane-4	5.184	0.000	20994756	0	19.152	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091818\
Data File : PL040109.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Sep 2018 19:25
Operator : AJ\SJ
Sample : J4941-01DL 5X
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 19 01:11:33 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
Quant Title : GC Extractables
QLast Update : Fri Sep 14 23:10:39 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

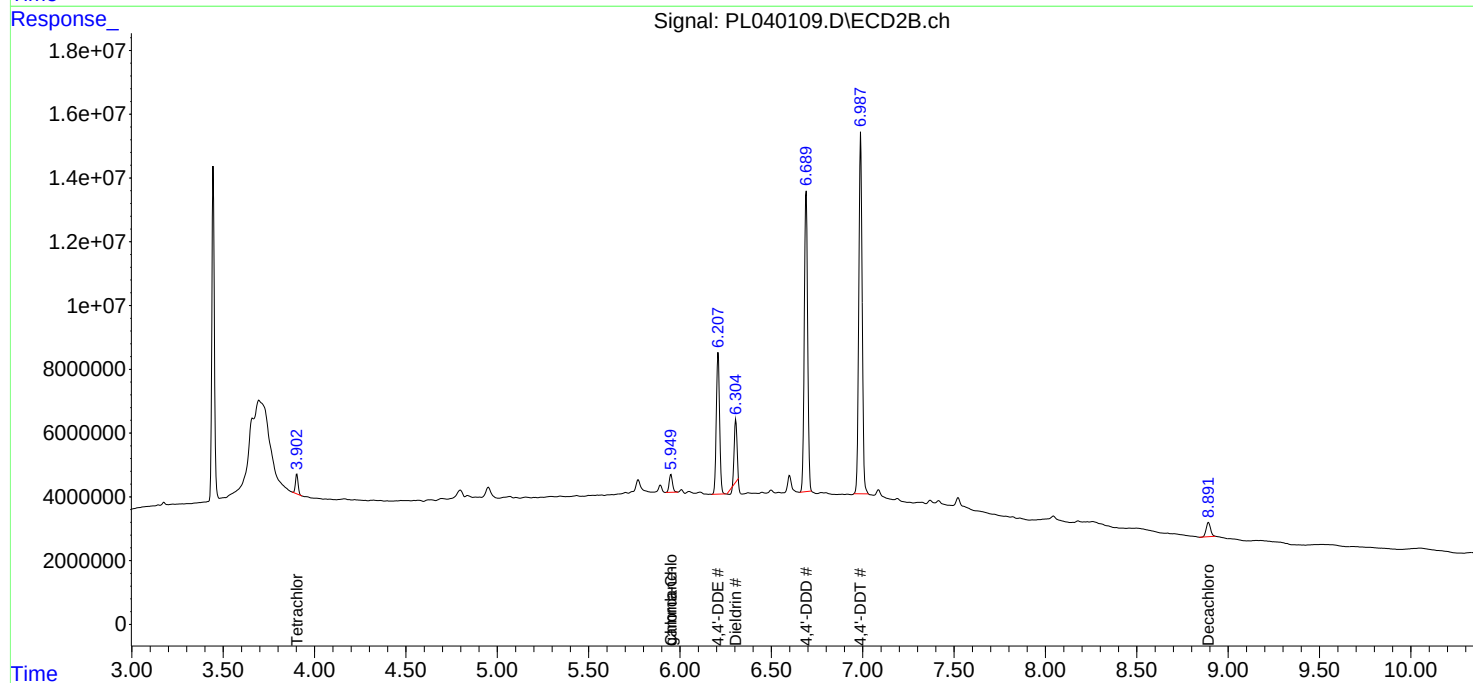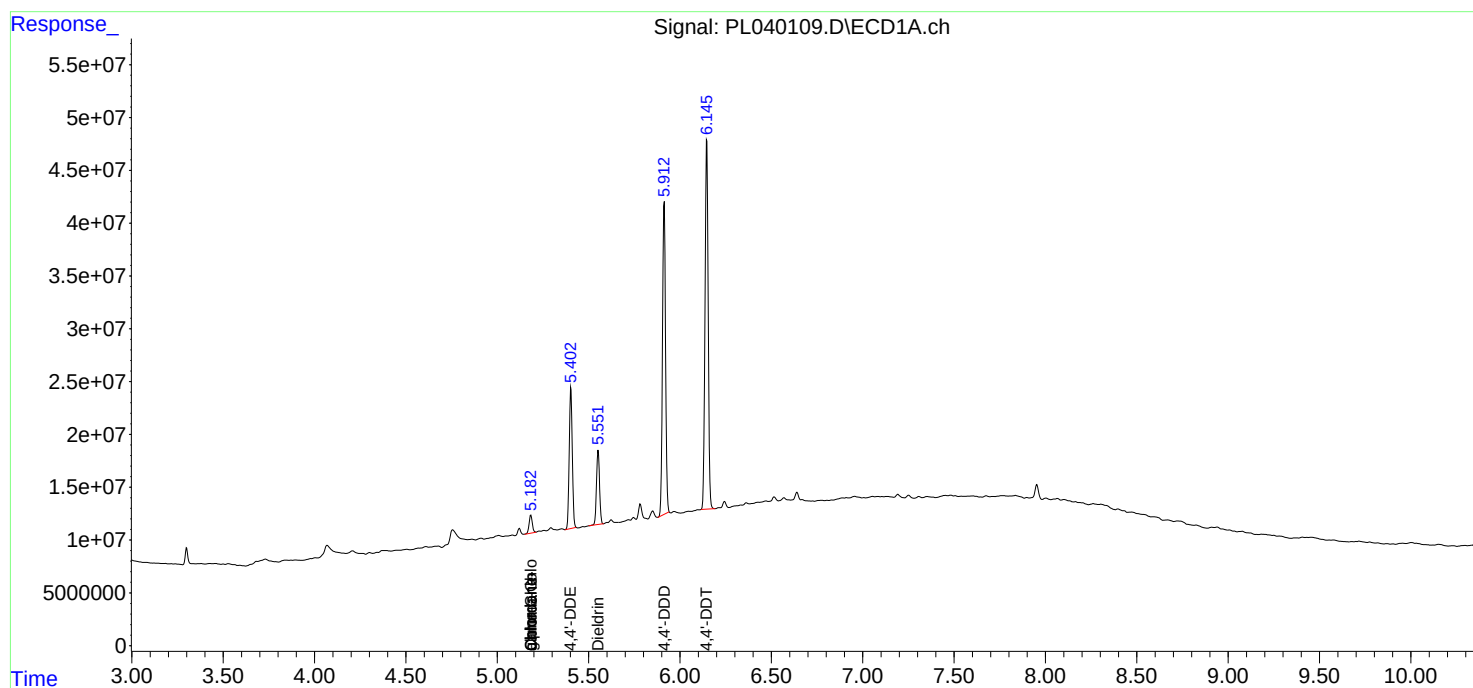


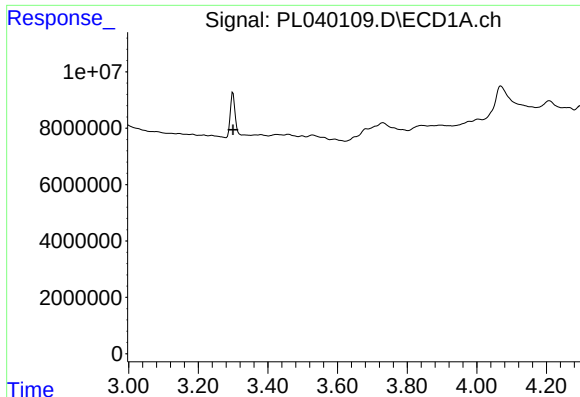

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.300 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

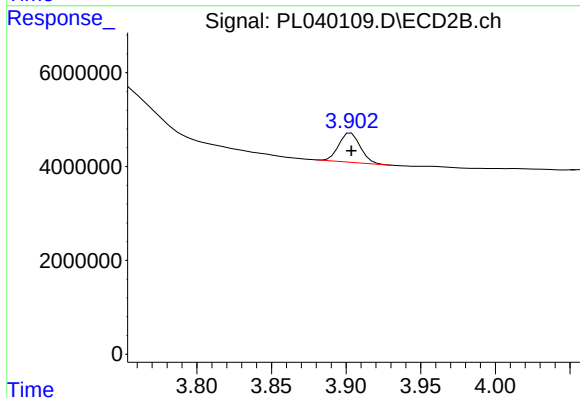


#1 Tetrachloro-m-xylene

R.T.: 3.903 min
Delta R.T.: 0.000 min
Response: 6147897
Conc: 1.93 ng/ml

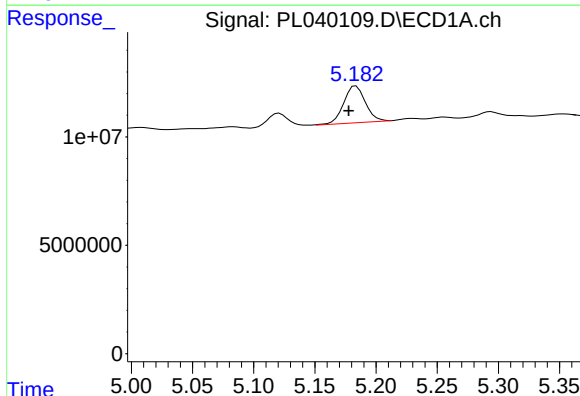


#10 gamma-Chlordane

R.T.: 5.184 min
Delta R.T.: 0.006 min
Response: 20994756
Conc: 1.88 ng/ml

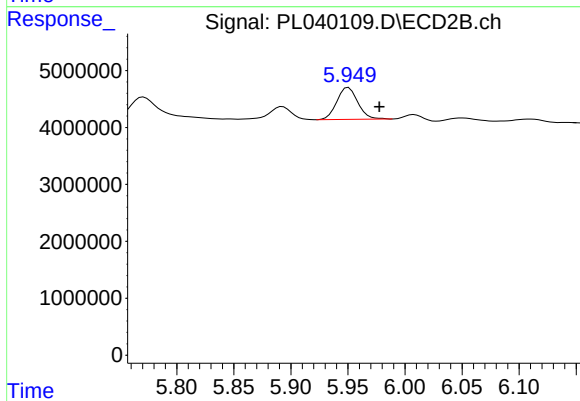

#10 gamma-Chlordane


R.T.: 5.951 min
Delta R.T.: -0.027 min
Response: 7184429
Conc: 1.90 ng/ml

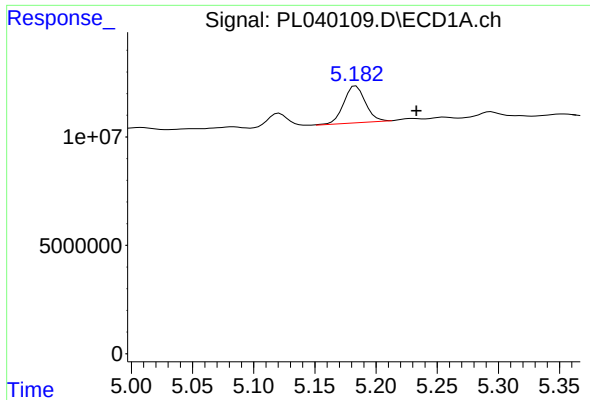

#11 alpha-Chlordane


R.T.: 5.184 min
Delta R.T.: -0.049 min
Response: 20994756
Conc: 1.97 ng/ml

Instrument :
ECD_L
ClientSampleId :

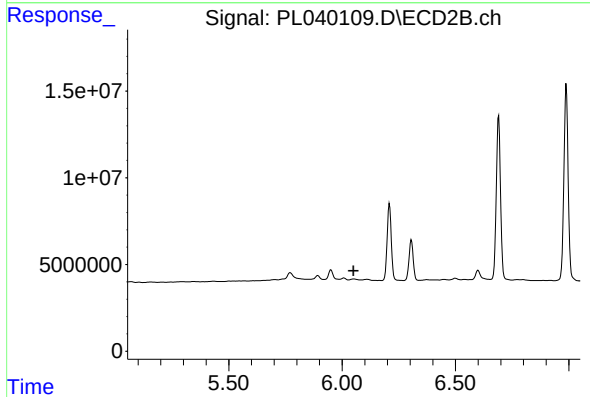


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.050 min
Response: 0
Conc: N.D.

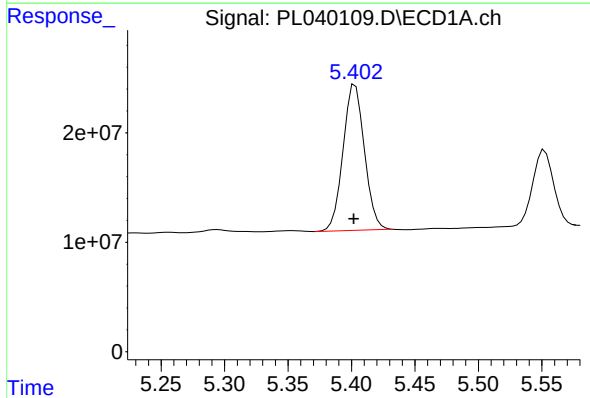


#12 4,4'-DDE

R.T.: 5.403 min
Delta R.T.: 0.001 min
Response: 155920801
Conc: 14.71 ng/ml

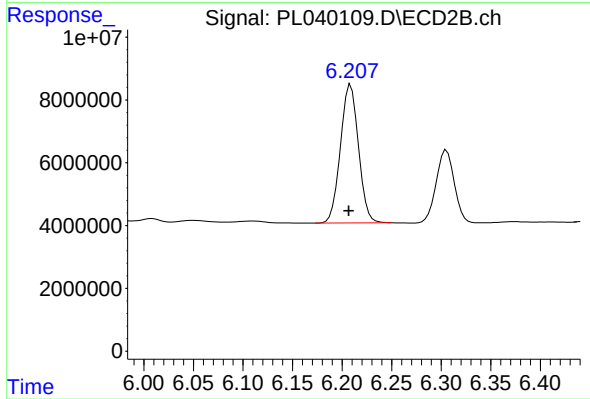

#12 4,4'-DDE


R.T.: 6.209 min
Delta R.T.: 0.002 min
Response: 55796016
Conc: 14.67 ng/ml

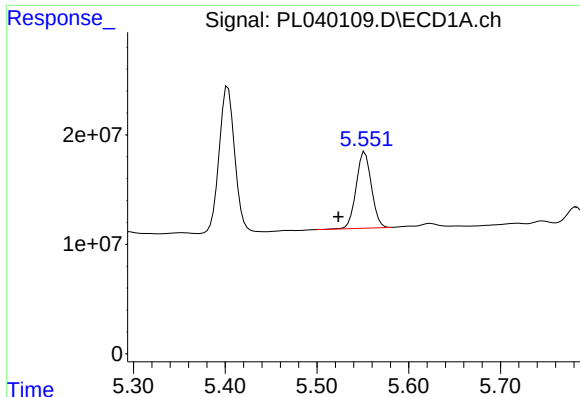

#13 Dieldrin


R.T.: 5.552 min
Delta R.T.: 0.029 min
Response: 80491293
Conc: 7.26 ng/ml

Instrument :
ECD_L
ClientSampleId :

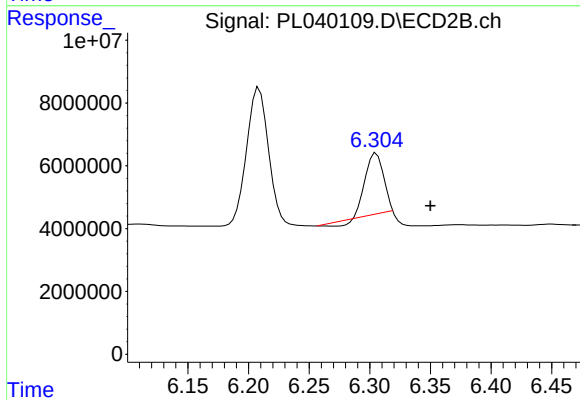


#13 Dieldrin

R.T.: 6.305 min
Delta R.T.: -0.045 min
Response: 19331698
Conc: 5.08 ng/ml

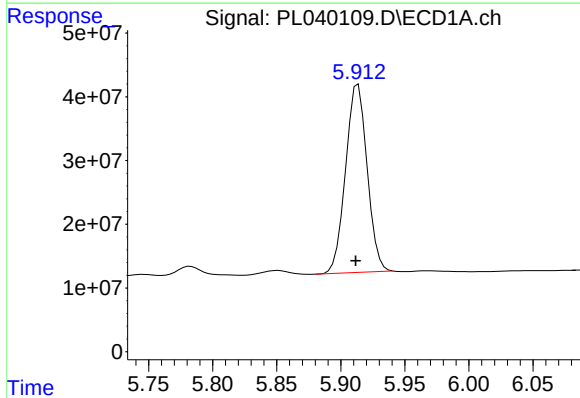


#16 4,4'-DDD

R.T.: 5.914 min
Delta R.T.: 0.002 min
Response: 345947623
Conc: 39.90 ng/ml

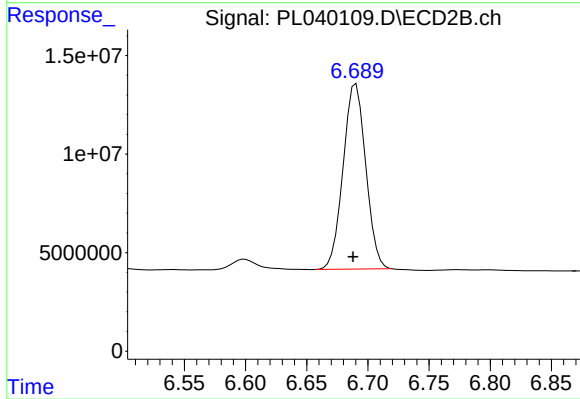

#16 4,4'-DDD


R.T.: 6.690 min
Delta R.T.: 0.002 min
Response: 121075481
Conc: 41.88 ng/ml

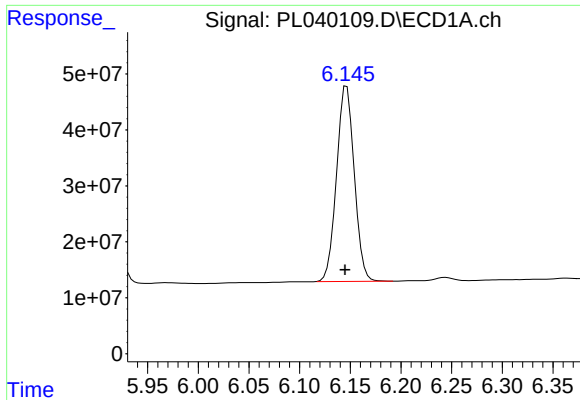

#17 4,4'-DDT


R.T.: 6.147 min
Delta R.T.: 0.002 min
Response: 424896624
Conc: 46.94 ng/ml

Instrument :
ECD_L
ClientSampleId :

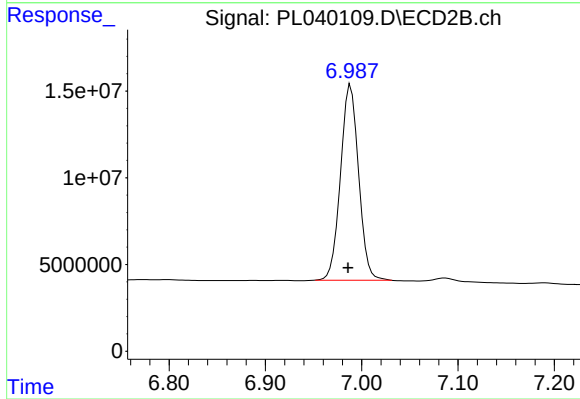


#17 4,4'-DDT

R.T.: 6.989 min
Delta R.T.: 0.003 min
Response: 146902054
Conc: 49.10 ng/ml

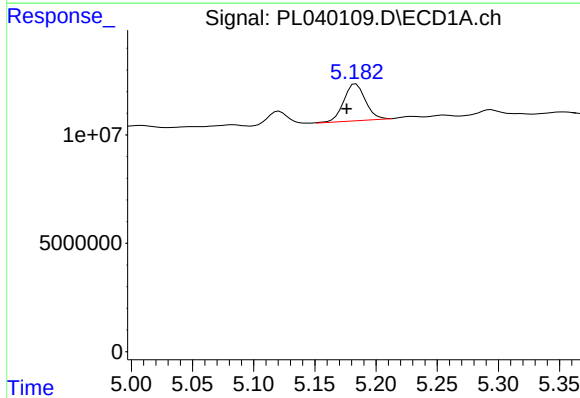


#25 Chlordane-3

R.T.: 5.184 min
Delta R.T.: 0.007 min
Response: 20994756
Conc: 17.11 ng/ml

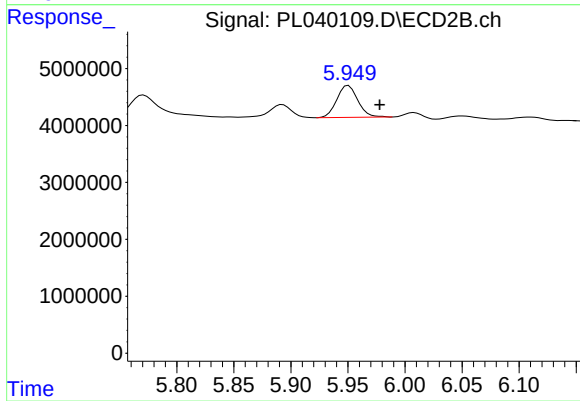

#25 Chlordane-3


R.T.: 5.951 min
Delta R.T.: -0.027 min
Response: 7184429
Conc: 14.03 ng/ml

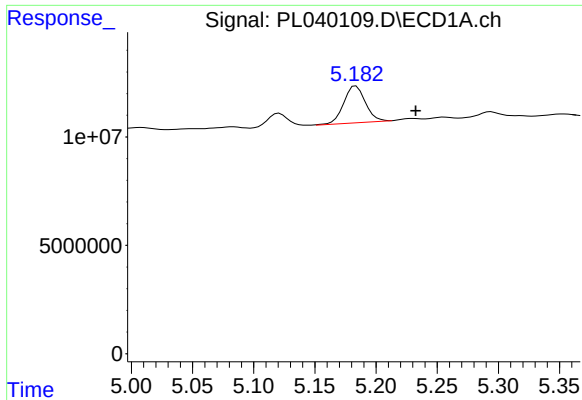

#26 Chlordane-4


R.T.: 5.184 min
Delta R.T.: -0.049 min
Response: 20994756
Conc: 19.15 ng/ml

Instrument :
ECD_L
ClientSampleId :

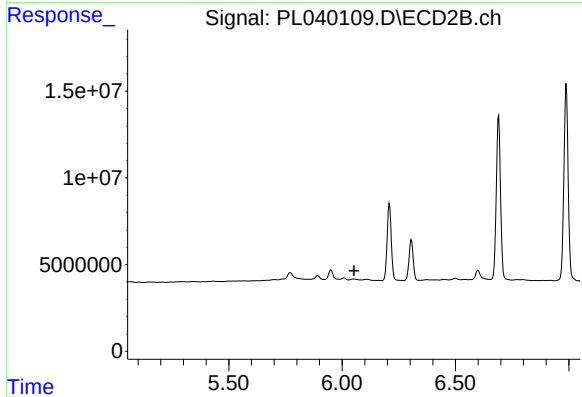


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.053 min
Response: 0
Conc: N.D.

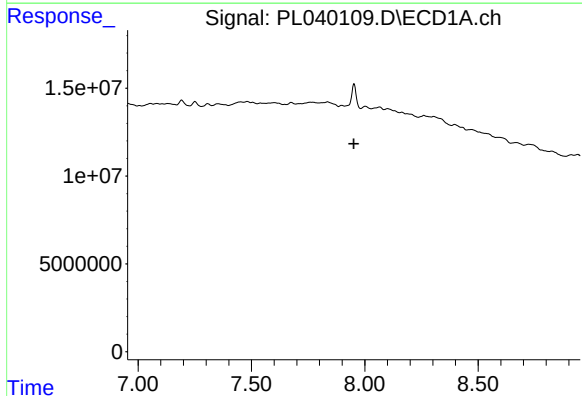

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.951 min
Response: 0
Conc: N.D.

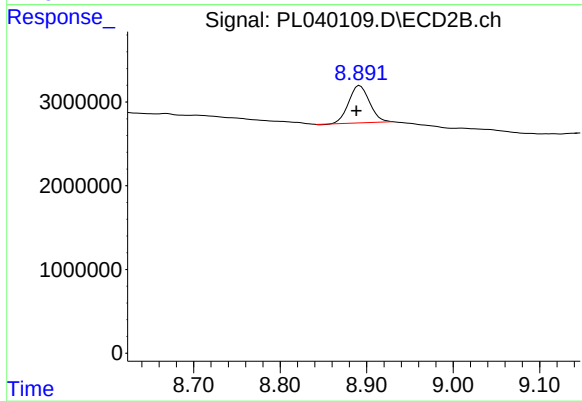

#28 Decachlorobiphenyl

R.T.: 8.892 min
Delta R.T.: 0.004 min
Response: 7513473
Conc: 2.77 ng/ml