

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091819\
 Data File : PL052596.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Sep 2019 20:17
 Operator : SG\AJ
 Sample : K4942-05
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 19 01:54:34 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091719.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 17 11:25:25 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.550	4.046	125.1E6	37773357	16.041	17.336
28)	SA Decachlor...	8.350	9.119	117.7E6	39667562	13.464	16.565
Target Compounds							
6)	B beta-BHC	0.000	4.913f	0	594510	N.D.	0.446 #
7)	B delta-BHC	0.000	5.085f	0	535555	N.D.	0.187 #
8)	B Heptachlo...	0.000	5.912	0	1398981	N.D.	0.533 #
12)	B 4,4'-DDE	0.000	6.384	0	670211	N.D.	0.275 #
15)	B Endosulfa...	0.000	6.953	0	1010664	N.D.	0.453 #
16)	A 4,4'-DDD	0.000	6.878	0	2141118	N.D.	1.163 #
17)	MA 4,4'-DDT	0.000	7.145f	0	1889432	N.D.	1.033 #
23)	Chlordane-1	0.000	5.045	0	28859	N.D.	0.372 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091819\
Data File : PL052596.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Sep 2019 20:17
Operator : SG\AJ
Sample : K4942-05
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 19 01:54:34 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091719.M
Quant Title : GC Extractables
QLast Update : Tue Sep 17 11:25:25 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

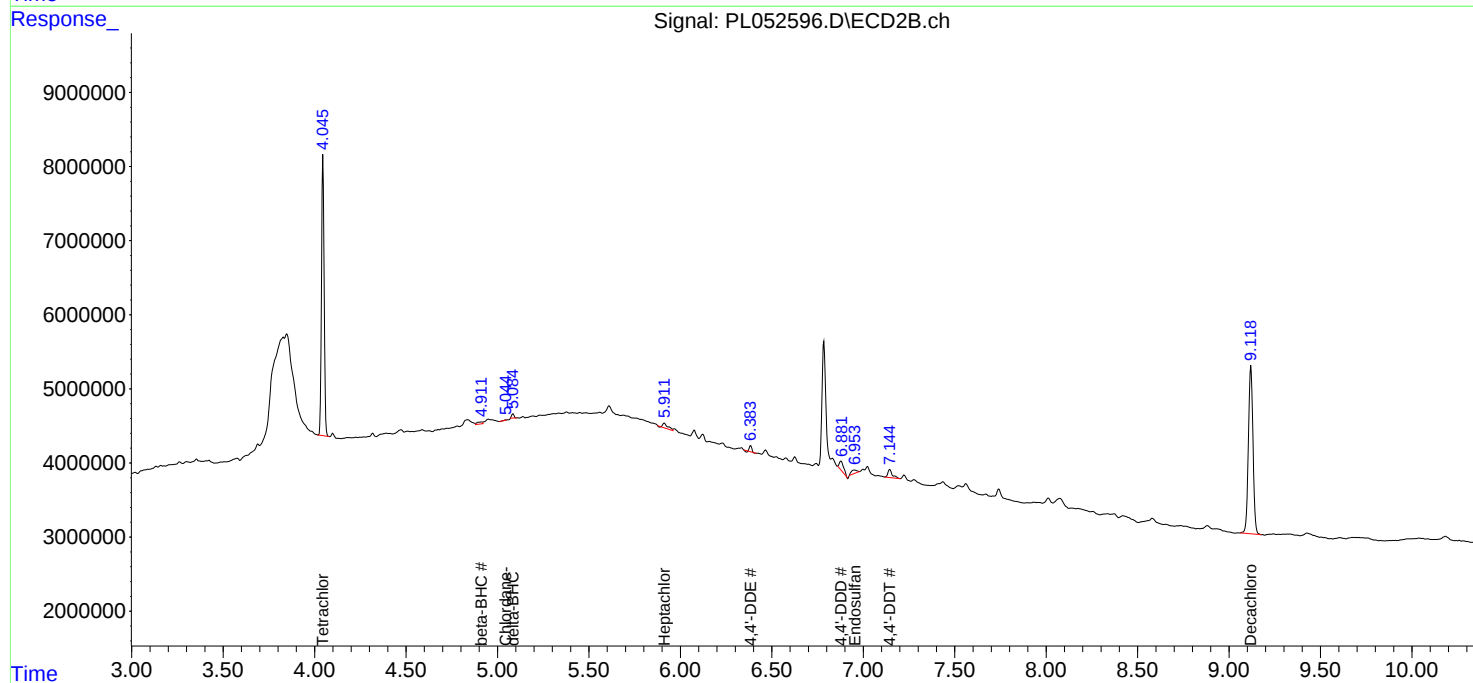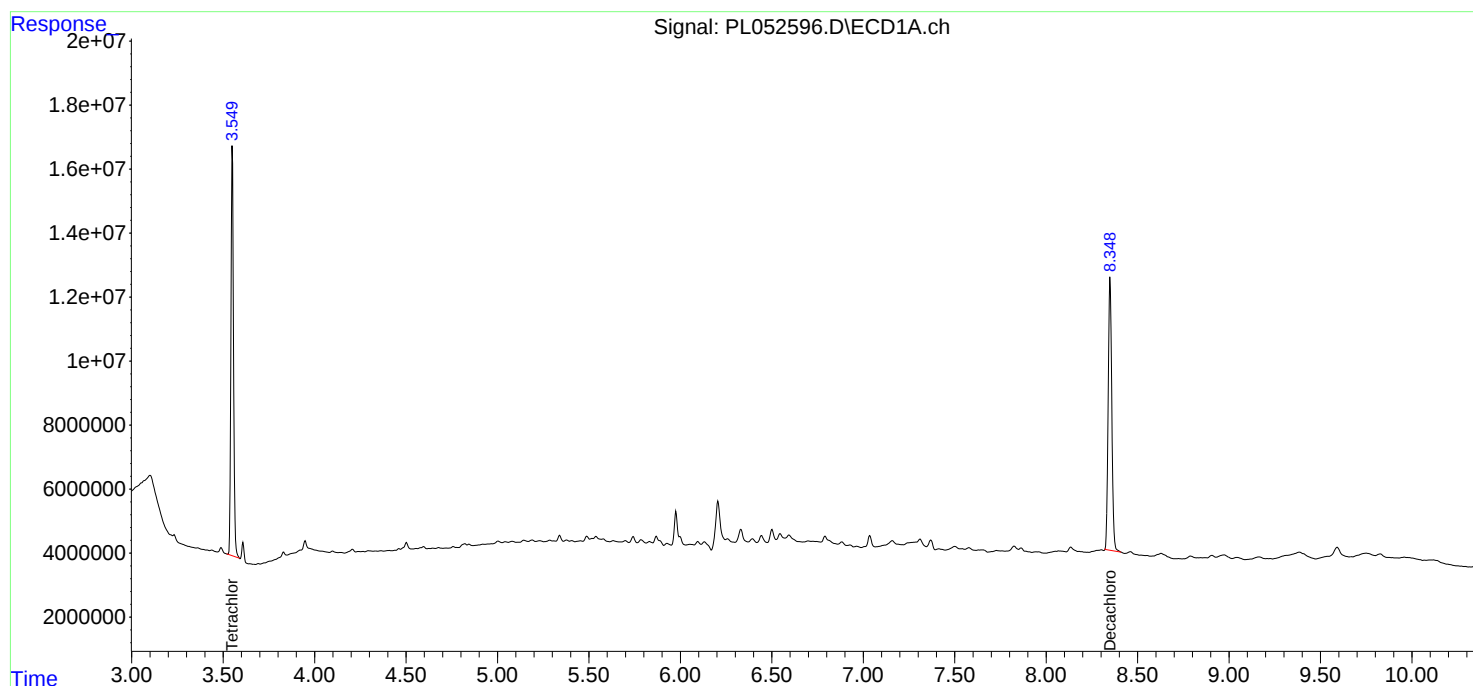


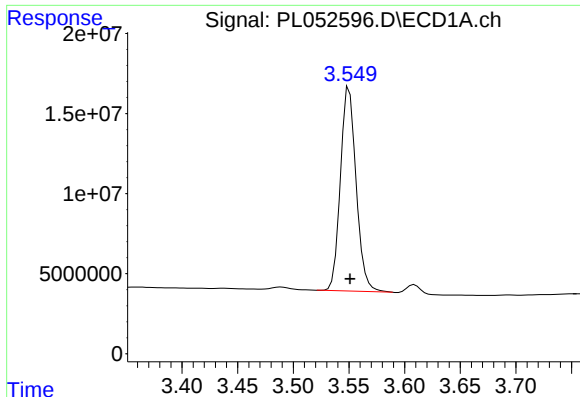

#1 Tetrachloro-m-xylene


R.T.: 3.550 min
Delta R.T.: 0.000 min
Response: 125086084
Conc: 16.04 ng/ml

Instrument :
ECD_L
ClientSampleId :

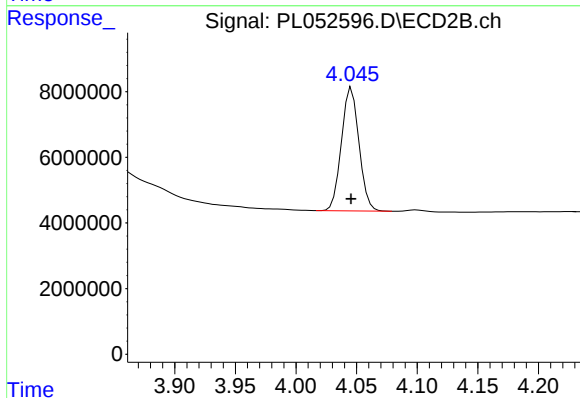


#1 Tetrachloro-m-xylene

R.T.: 4.046 min
Delta R.T.: 0.000 min
Response: 37773357
Conc: 17.34 ng/ml

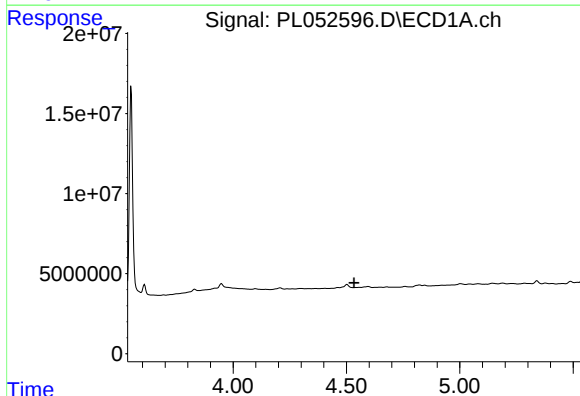


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.534 min
Response: 0
Conc: N.D.

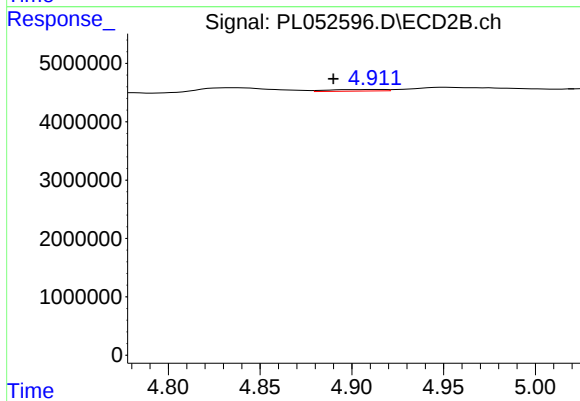

#6 beta-BHC


R.T.: 4.913 min
Delta R.T.: 0.023 min
Response: 594510
Conc: 0.45 ng/ml

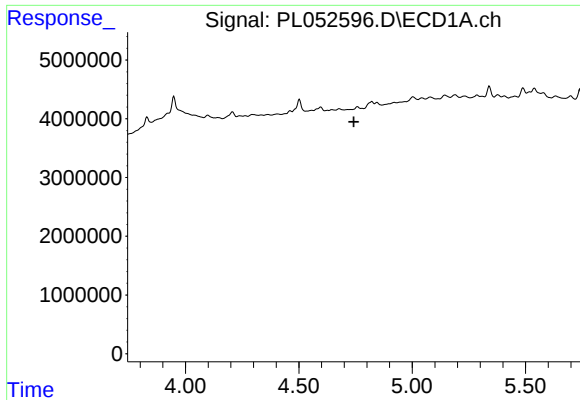

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.743 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

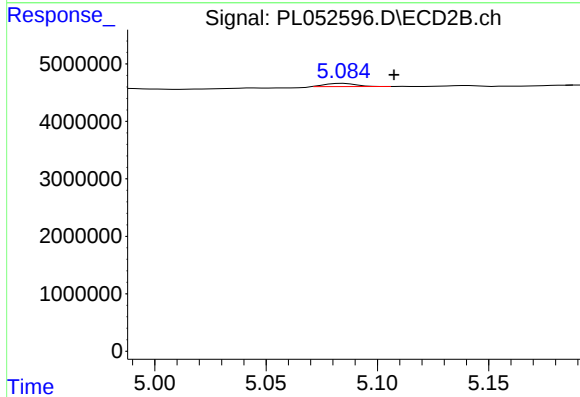


#7 delta-BHC

R.T.: 5.085 min
Delta R.T.: -0.023 min
Response: 535555
Conc: 0.19 ng/ml

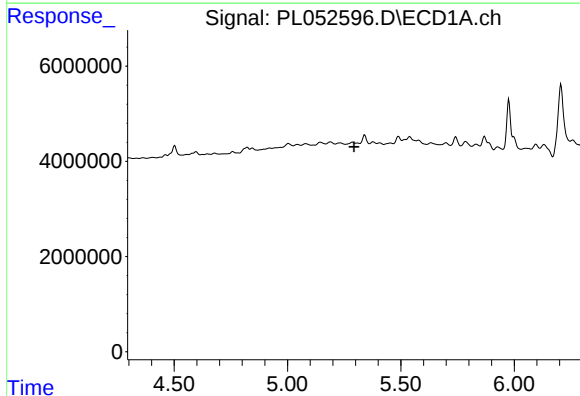


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.293 min
Response: 0
Conc: N.D.

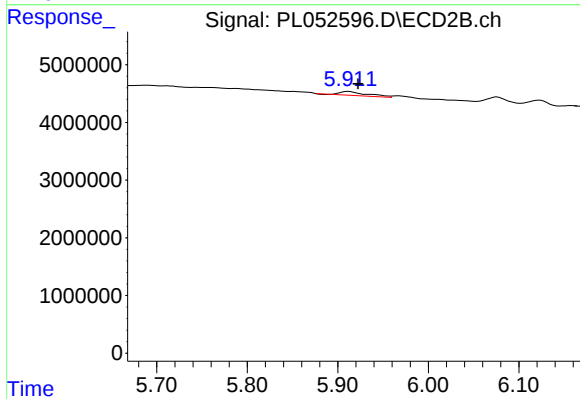

#8 Heptachlor epoxide


R.T.: 5.912 min
Delta R.T.: -0.010 min
Response: 1398981
Conc: 0.53 ng/ml

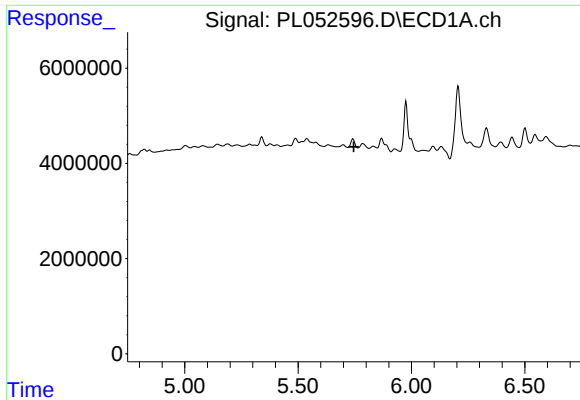

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 5.746 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

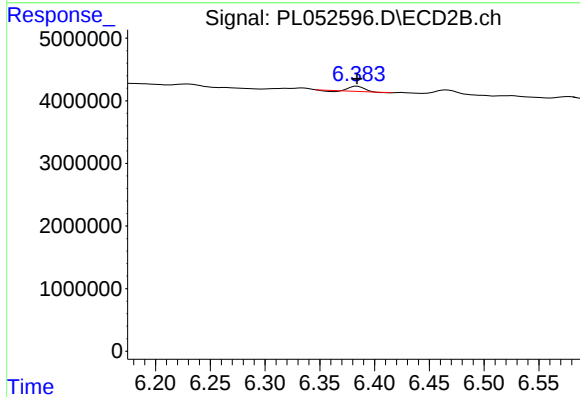


#12 4,4'-DDE

R.T.: 6.384 min
Delta R.T.: 0.000 min
Response: 670211
Conc: 0.27 ng/ml

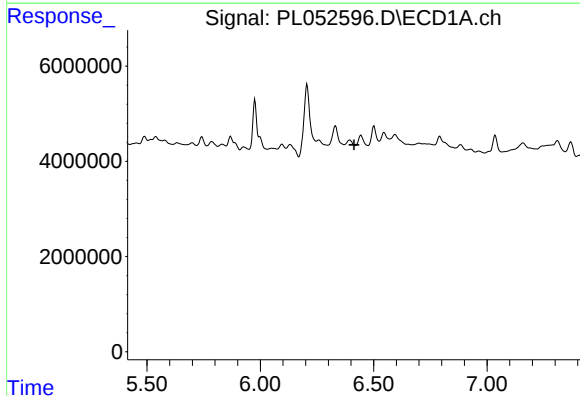


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.414 min
Response: 0
Conc: N.D.

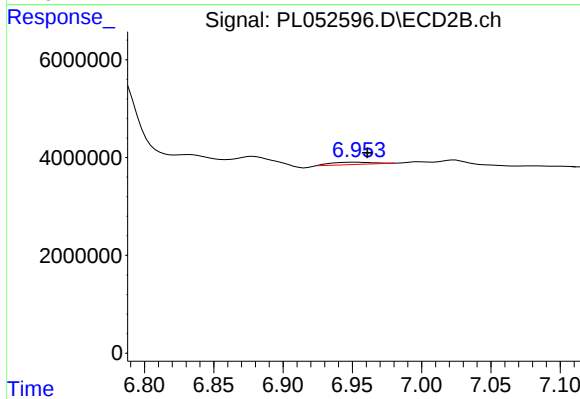

#15 Endosulfan II


R.T.: 6.953 min
Delta R.T.: -0.007 min
Response: 1010664
Conc: 0.45 ng/ml

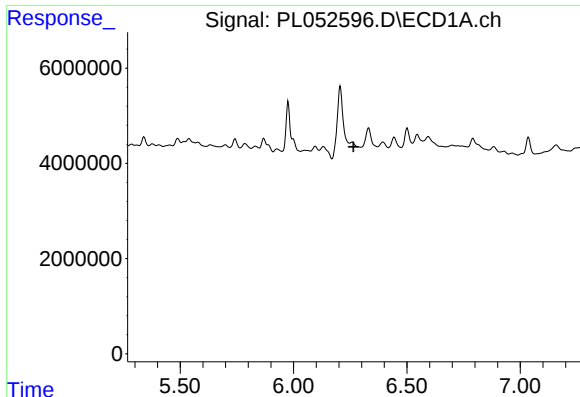

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.265 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

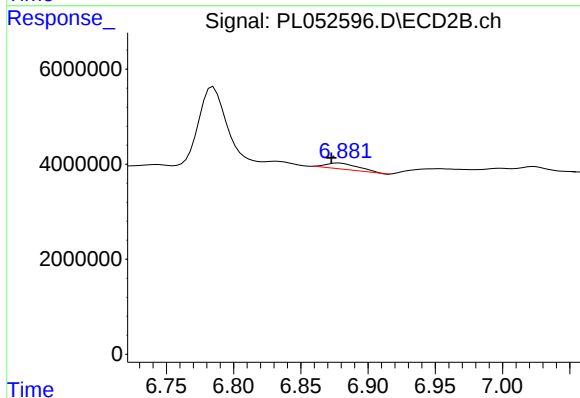


#16 4,4'-DDD

R.T.: 6.878 min
Delta R.T.: 0.006 min
Response: 2141118
Conc: 1.16 ng/ml

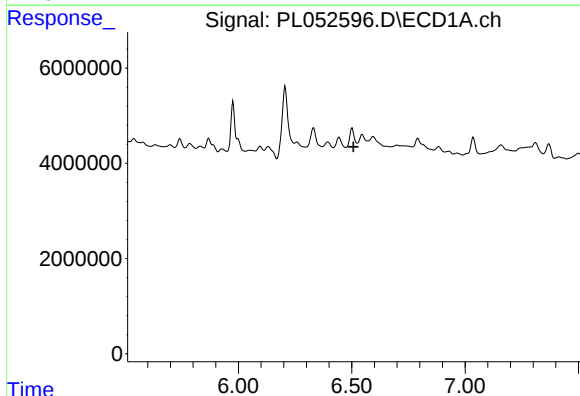


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 6.508 min
Response: 0
Conc: N.D.

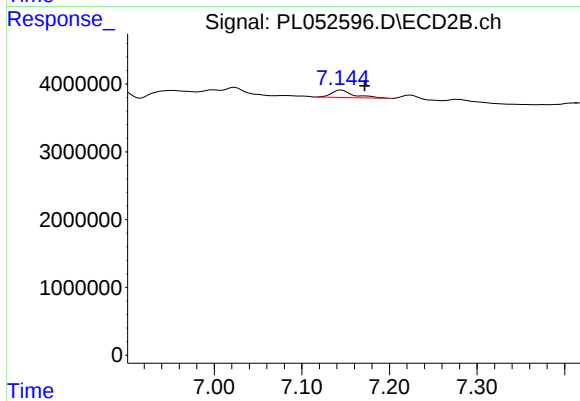

#17 4,4'-DDT


R.T.: 7.145 min
Delta R.T.: -0.027 min
Response: 1889432
Conc: 1.03 ng/ml

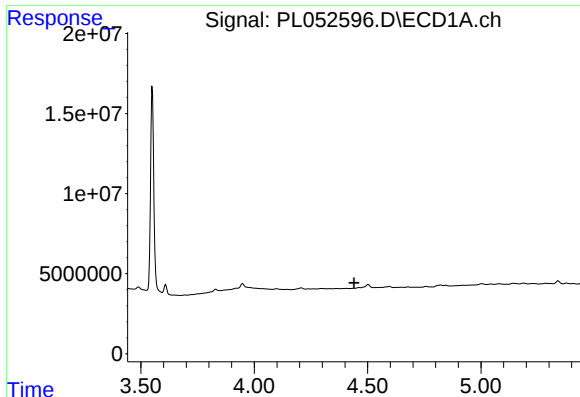

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.440 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

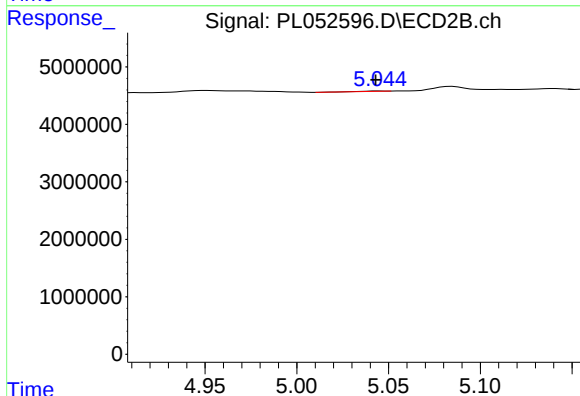


#23 Chlordane-1

R.T.: 5.045 min
Delta R.T.: 0.002 min
Response: 28859
Conc: 0.37 ng/ml

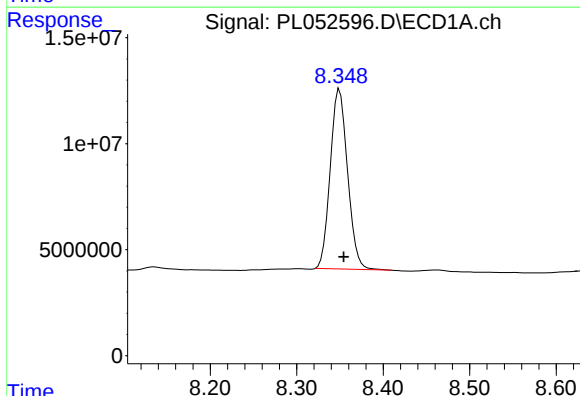

#28 Decachlorobiphenyl

R.T.: 8.350 min
Delta R.T.: -0.005 min
Response: 117734037
Conc: 13.46 ng/ml

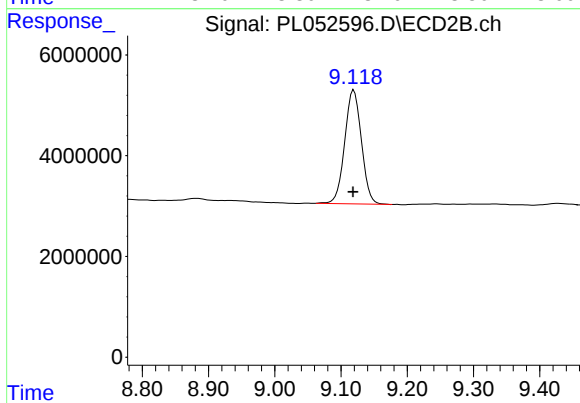

#28 Decachlorobiphenyl

R.T.: 9.119 min
Delta R.T.: 0.000 min
Response: 39667562
Conc: 16.57 ng/ml