

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091819\
 Data File : PL052598.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Sep 2019 20:45
 Operator : SG\AJ
 Sample : K4942-09
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-5

Manual Integrations
 APPROVED

Ankita
 9/19/2019 2:11:26 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 19 01:54:53 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091719.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 17 11:25:25 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.550	4.046	98942125	30074486	12.689	13.802
28) SA Decachlor...	8.350	9.117	105.3E6	39764841	12.043	16.606m#
Target Compounds						
10) B gamma-Chl...	5.519	6.157	5446288	1355639	0.513m	0.533
11) B alpha-Chl...	5.578	6.230	7781845	3422835	0.753m	1.370 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091819\
Data File : PL052598.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Sep 2019 20:45
Operator : SG\AJ
Sample : K4942-09
Misc :
ALS Vial : 39 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP-5


Manual Integrations
APPROVED

Ankita
9/19/2019 2:11:26 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 19 01:54:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091719.M
Quant Title : GC Extractables
QLast Update : Tue Sep 17 11:25:25 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

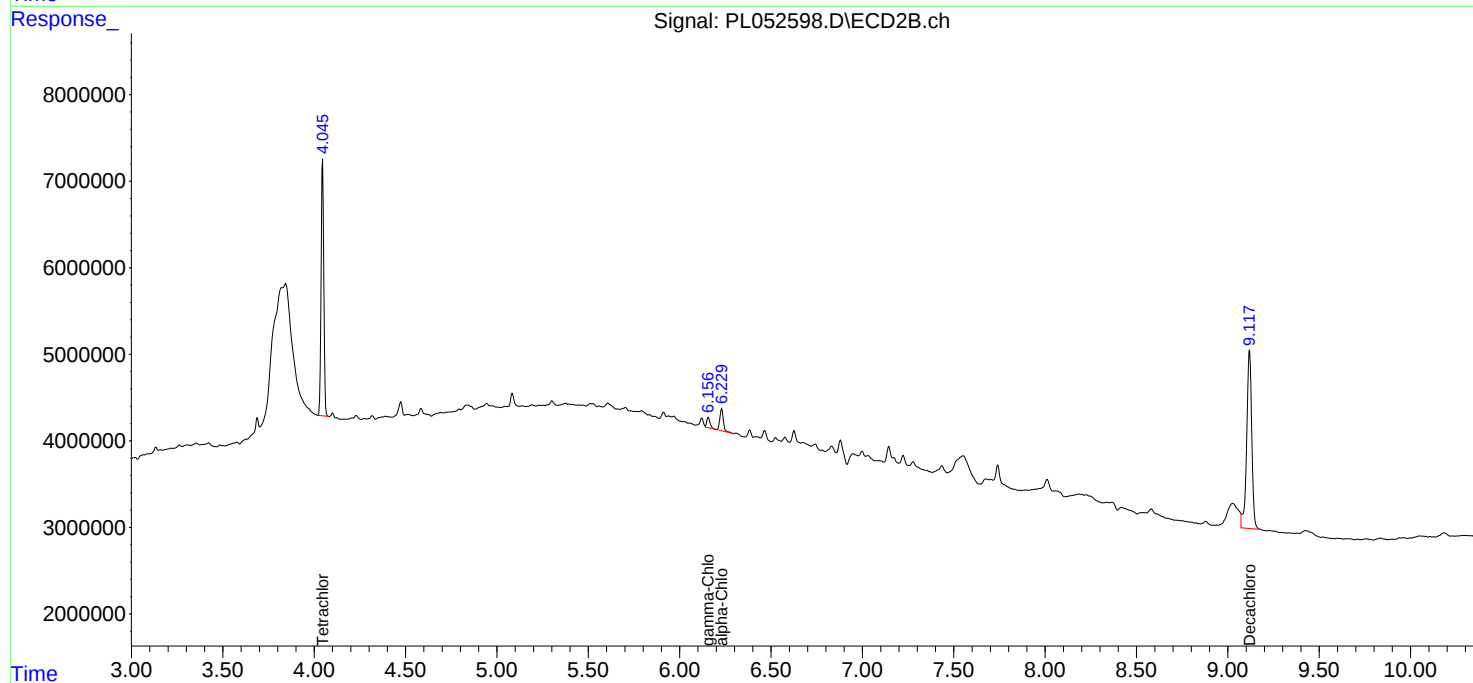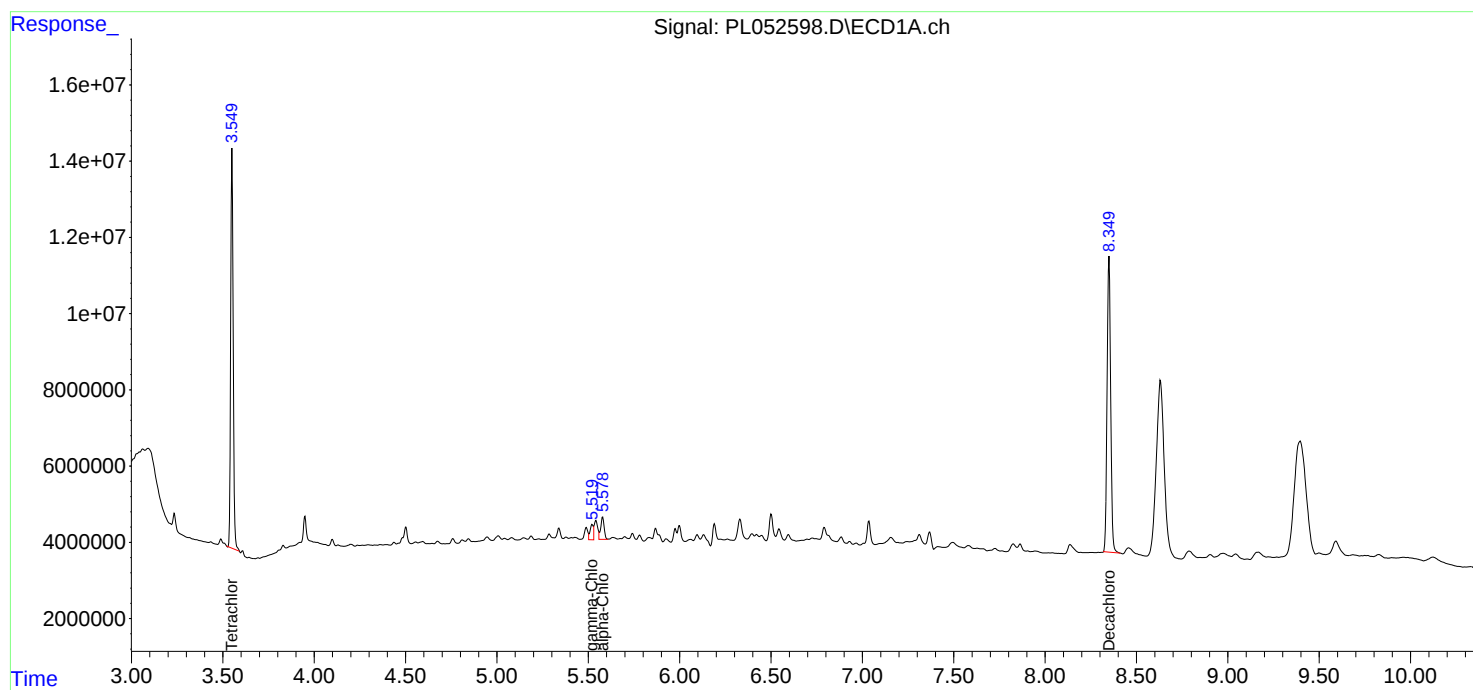

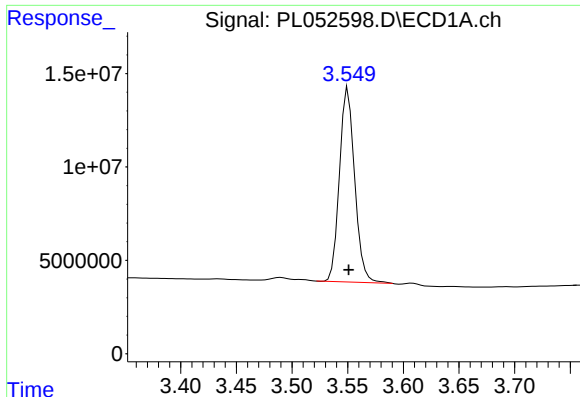


#1 Tetrachloro-m-xylene

R.T.: 3.550 min
Delta R.T.: 0.000 min
Response: 98942125
Conc: 12.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-5


Manual Integrations
APPROVED

Ankita
9/19/2019 2:11:26 PM

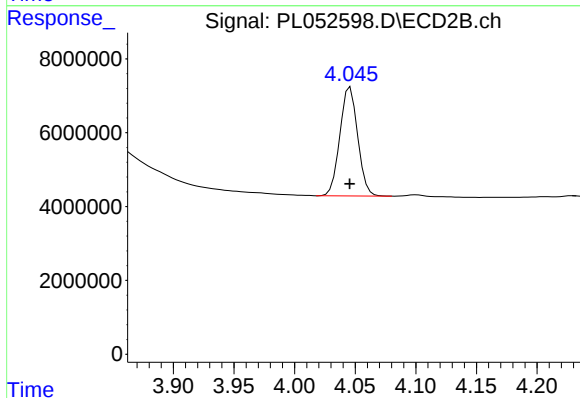


#1 Tetrachloro-m-xylene

R.T.: 4.046 min
Delta R.T.: 0.000 min
Response: 30074486
Conc: 13.80 ng/ml

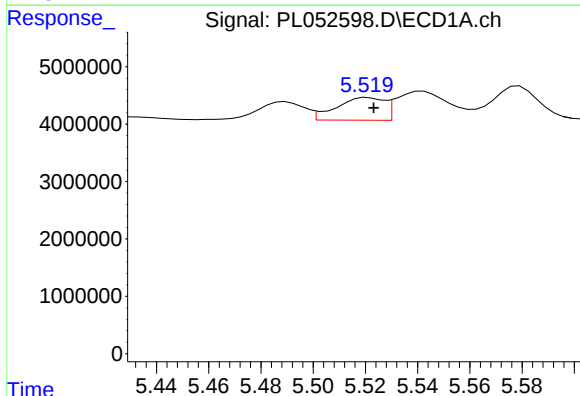


#10 gamma-Chlordane

R.T.: 5.519 min
Delta R.T.: -0.004 min
Response: 5446288
Conc: 0.51 ng/ml m

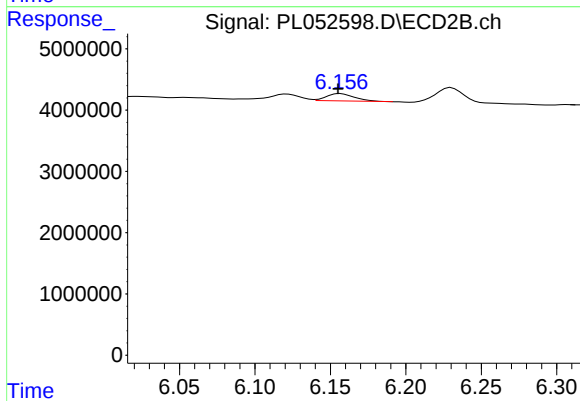

#10 gamma-Chlordane

R.T.: 6.157 min
Delta R.T.: 0.002 min
Response: 1355639
Conc: 0.53 ng/ml

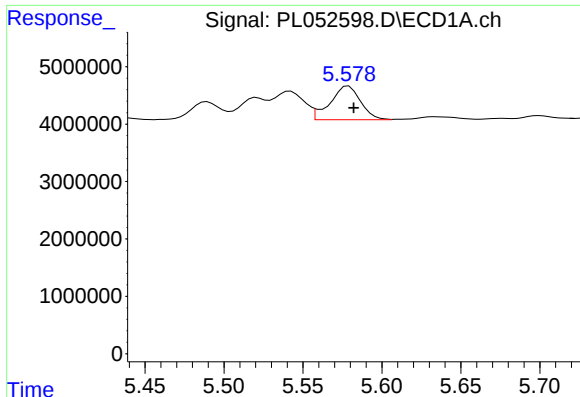


#11 alpha-Chlordane

R.T.: 5.578 min
Delta R.T.: -0.005 min
Response: 7781845
Conc: 0.75 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TP-5


Manual Integrations
APPROVED

Ankita
9/19/2019 2:11:26 PM

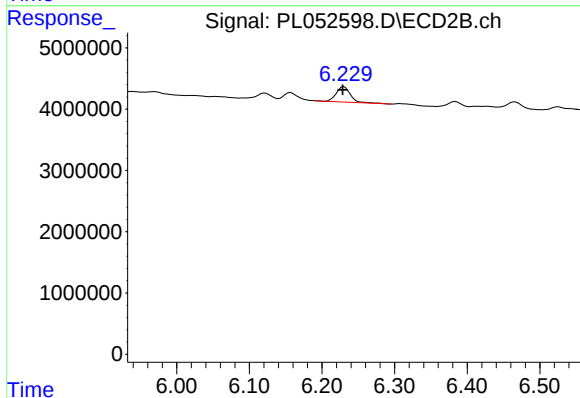


#11 alpha-Chlordane

R.T.: 6.230 min
Delta R.T.: 0.001 min
Response: 3422835
Conc: 1.37 ng/ml

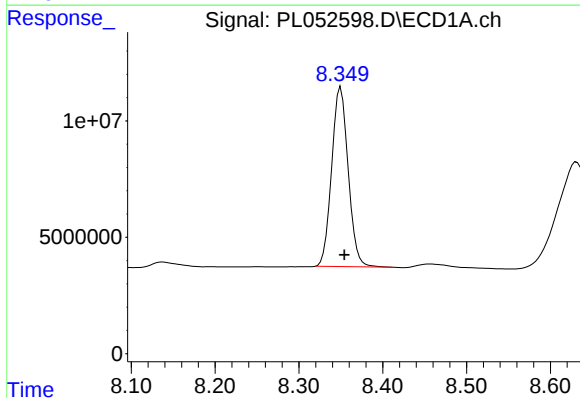

#28 Decachlorobiphenyl

R.T.: 8.350 min
Delta R.T.: -0.004 min
Response: 105311381
Conc: 12.04 ng/ml

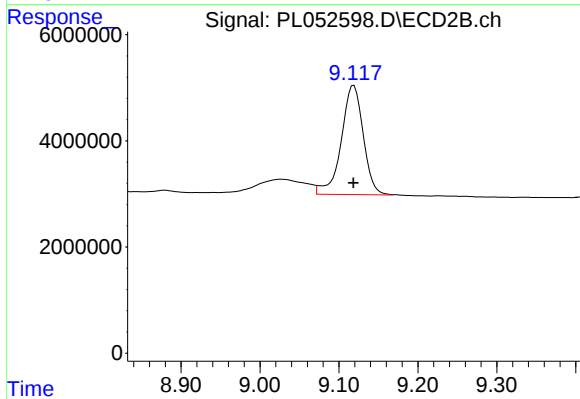

#28 Decachlorobiphenyl

R.T.: 9.117 min
Delta R.T.: -0.001 min
Response: 39764841
Conc: 16.61 ng/ml m