

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091820\
 Data File : PL061571.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Sep 2020 08:55
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 18 15:14:43 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 09 01:27:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.460	4.008	38047422	68705928	22.060	22.336
28)	SA Decachlor...	8.213	9.097	31961709	44732585	19.158	18.918
Target Compounds							
19)	B Endosulfa...	0.000	7.270	0	8139127	N.D.	2.975 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091820\
Data File : PL061571.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Sep 2020 08:55
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 18 15:14:43 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
Quant Title : GC Extractables
QLast Update : Wed Sep 09 01:27:38 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

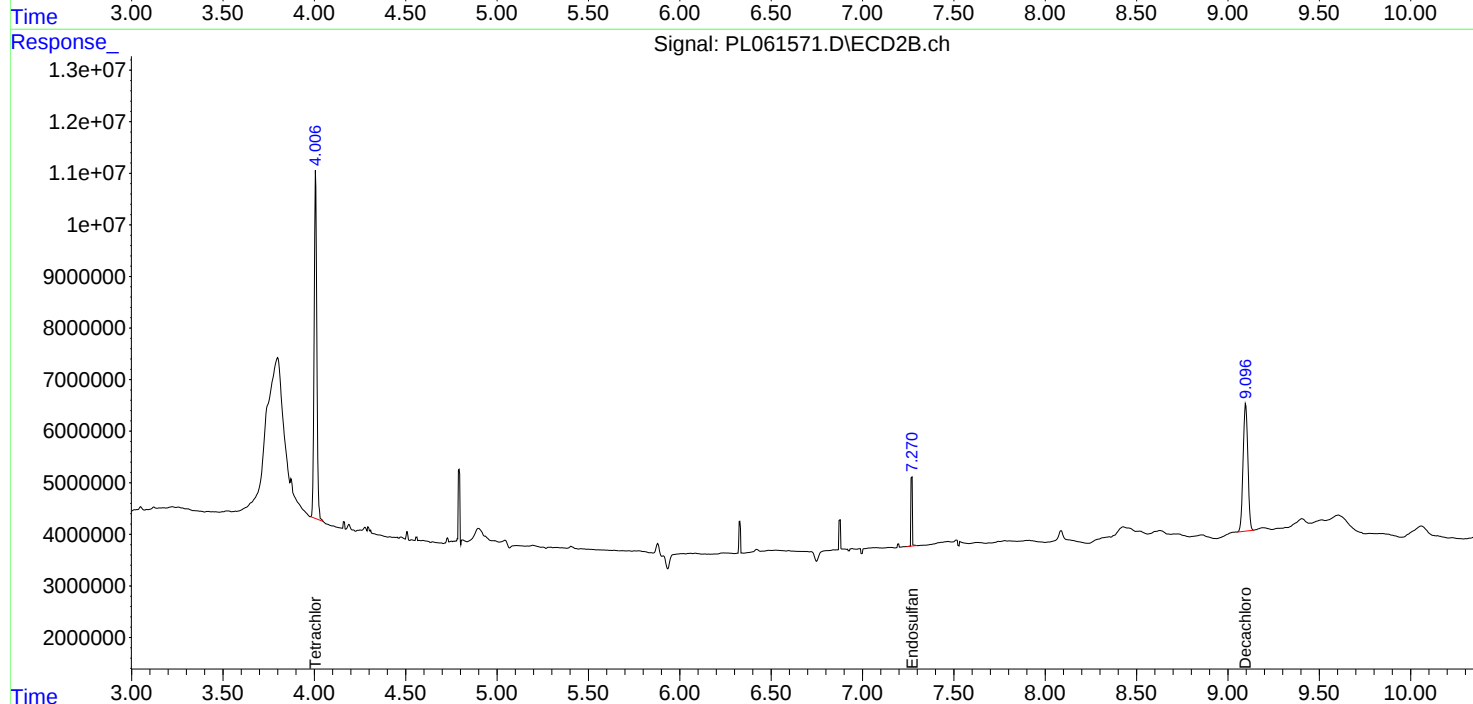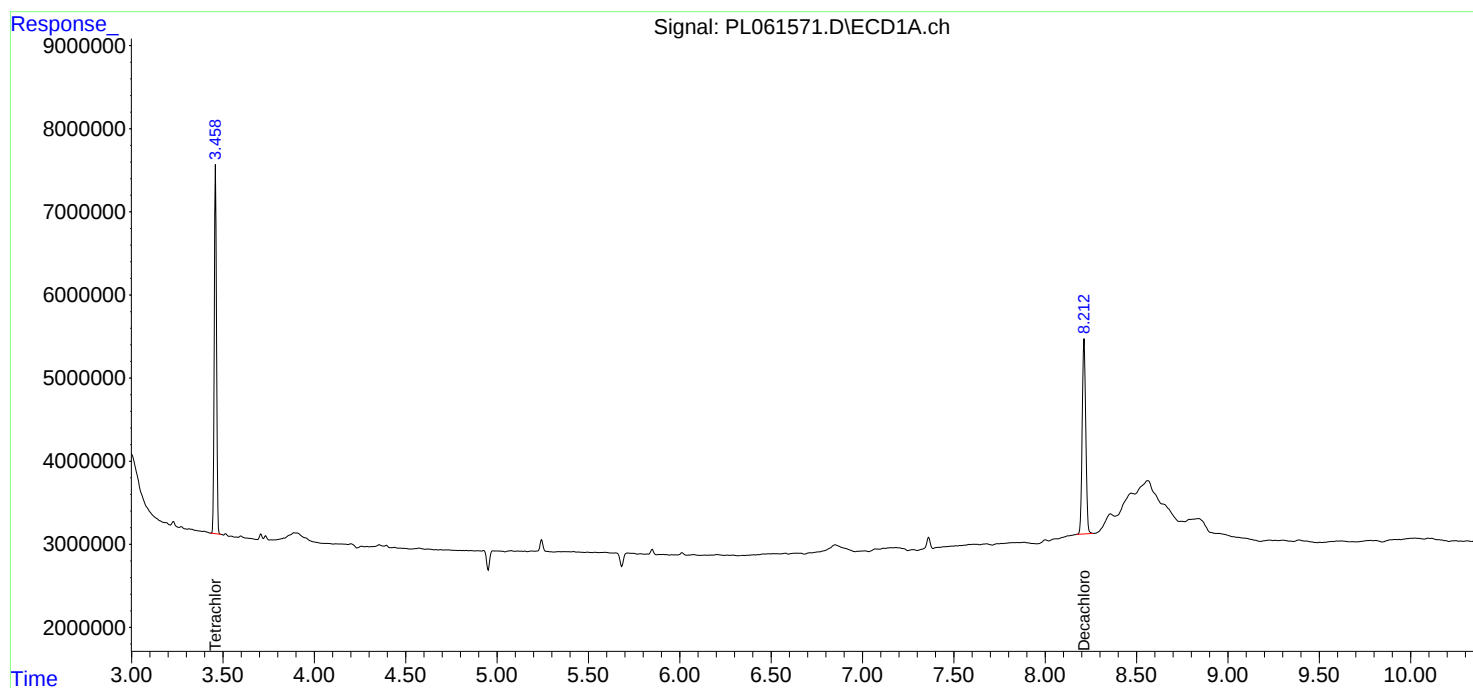


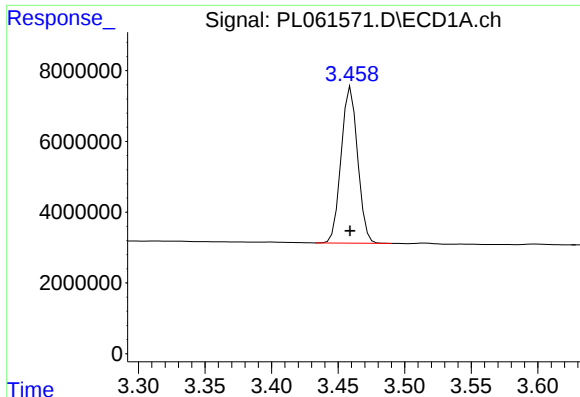

#1 Tetrachloro-m-xylene


R.T.: 3.460 min
Delta R.T.: 0.000 min
Response: 38047422
Conc: 22.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

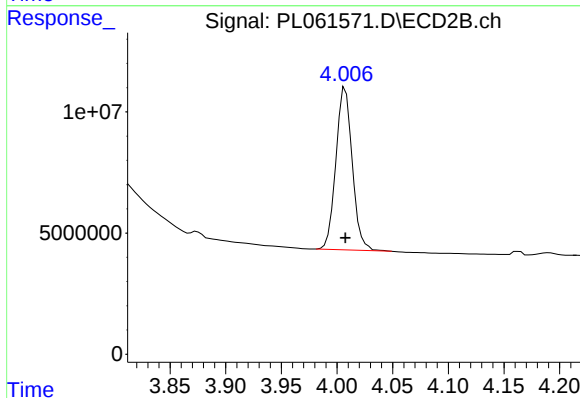


#1 Tetrachloro-m-xylene

R.T.: 4.008 min
Delta R.T.: 0.000 min
Response: 68705928
Conc: 22.34 ng/ml

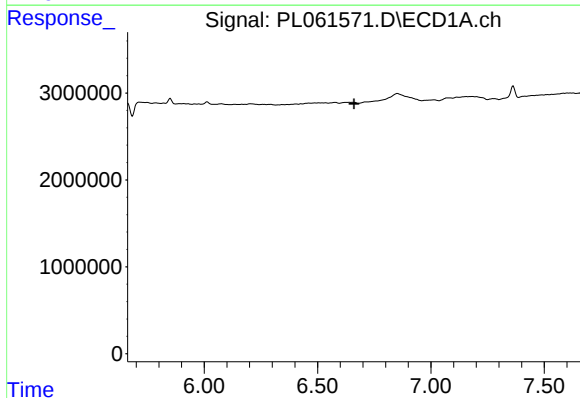


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 6.662 min
Response: 0
Conc: N.D.

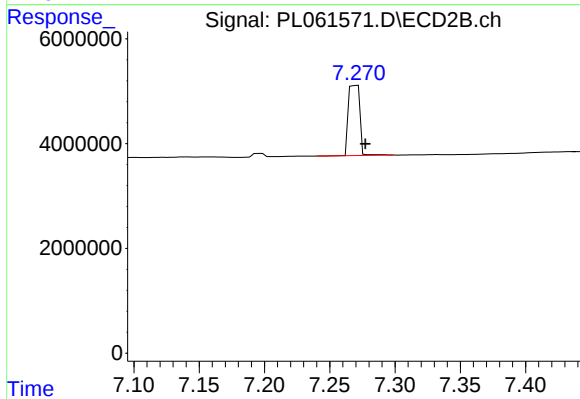

#19 Endosulfan Sulfate


R.T.: 7.270 min
Delta R.T.: -0.008 min
Response: 8139127
Conc: 2.98 ng/ml

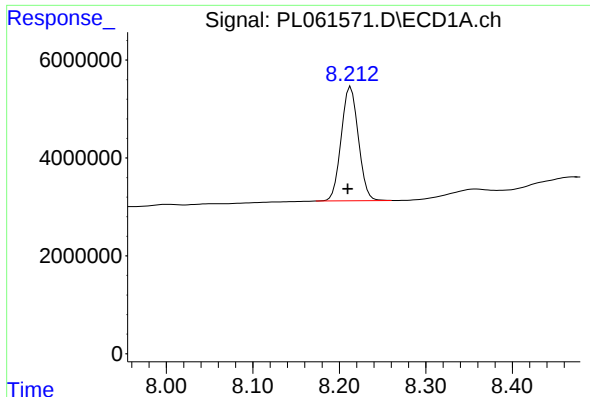

#28 Decachlorobiphenyl

R.T.: 8.213 min
Delta R.T.: 0.004 min
Response: 31961709
Conc: 19.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

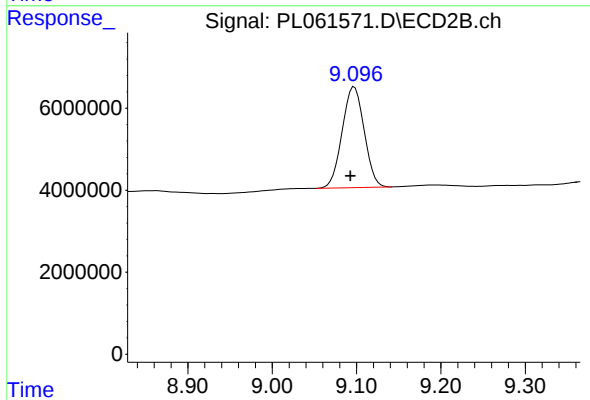

#28 Decachlorobiphenyl

R.T.: 9.097 min
Delta R.T.: 0.005 min
Response: 44732585
Conc: 18.92 ng/ml