

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091820\
 Data File : PL061575.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Sep 2020 09:53
 Operator : DD\AJ
 Sample : L4038-07
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 18 15:15:43 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 09 01:27:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.462	4.009	28609568	47700503	16.588	15.507
28)	SA Decachlor...	8.214	9.099	24006864	34242074	14.390	14.481
Target Compounds							
5)	MB Aldrin	0.000	5.470f	0	13010568	N.D.	3.443 #
6)	B beta-BHC	0.000	4.878f	0	2873084	N.D.	1.645 #
9)	A Endosulfan I	5.527f	6.242	9264839	1875686	5.385	0.585 #
10)	B gamma-Chl...	0.000	6.130	0	5086100	N.D.	1.475 #
11)	B alpha-Chl...	0.000	6.175f	0	9750570	N.D.	2.802 #
24)	Chlordane-2	0.000	5.470	0	13010568	N.D.	106.524 #
25)	Chlordane-3	0.000	6.130	0	5086100	N.D.	11.774 #
26)	Chlordane-4	0.000	6.175f	0	9750570	N.D.	18.627 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091820\
Data File : PL061575.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Sep 2020 09:53
Operator : DD\AJ
Sample : L4038-07
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 18 15:15:43 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
Quant Title : GC Extractables
QLast Update : Wed Sep 09 01:27:38 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

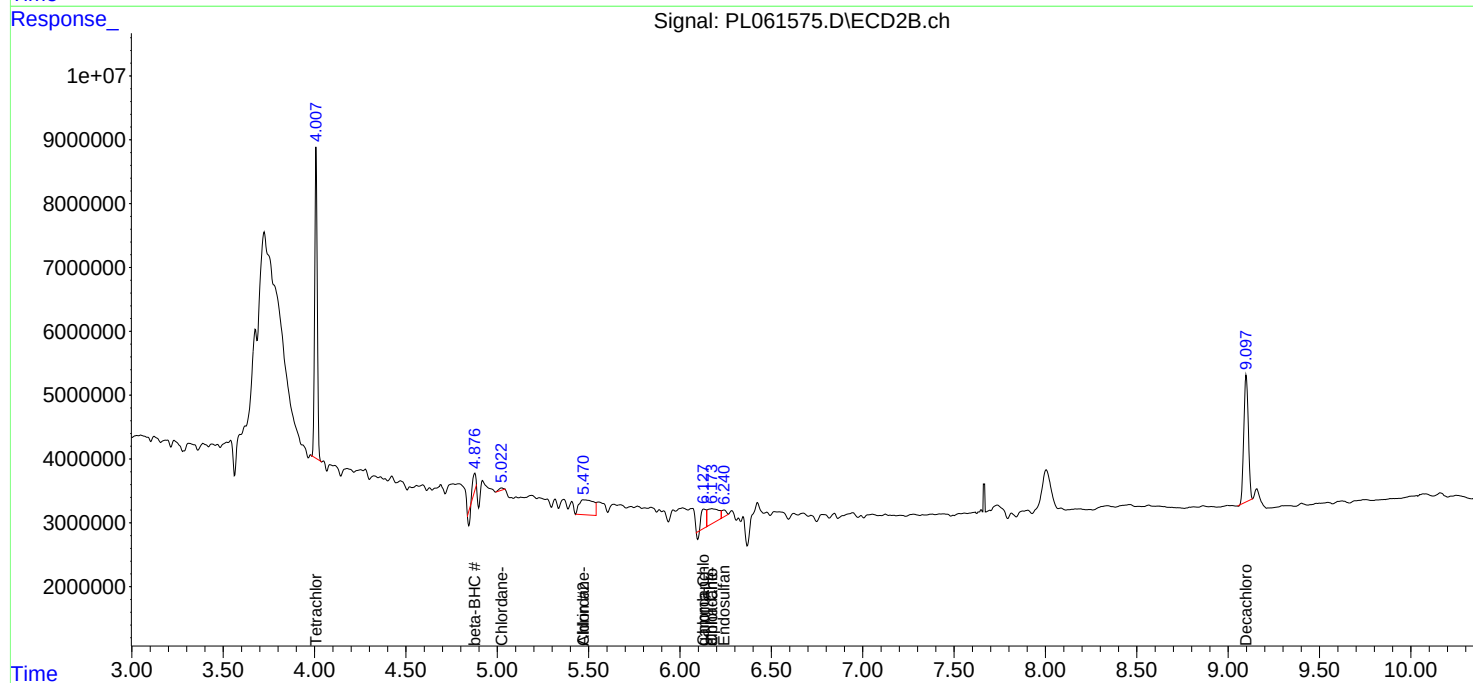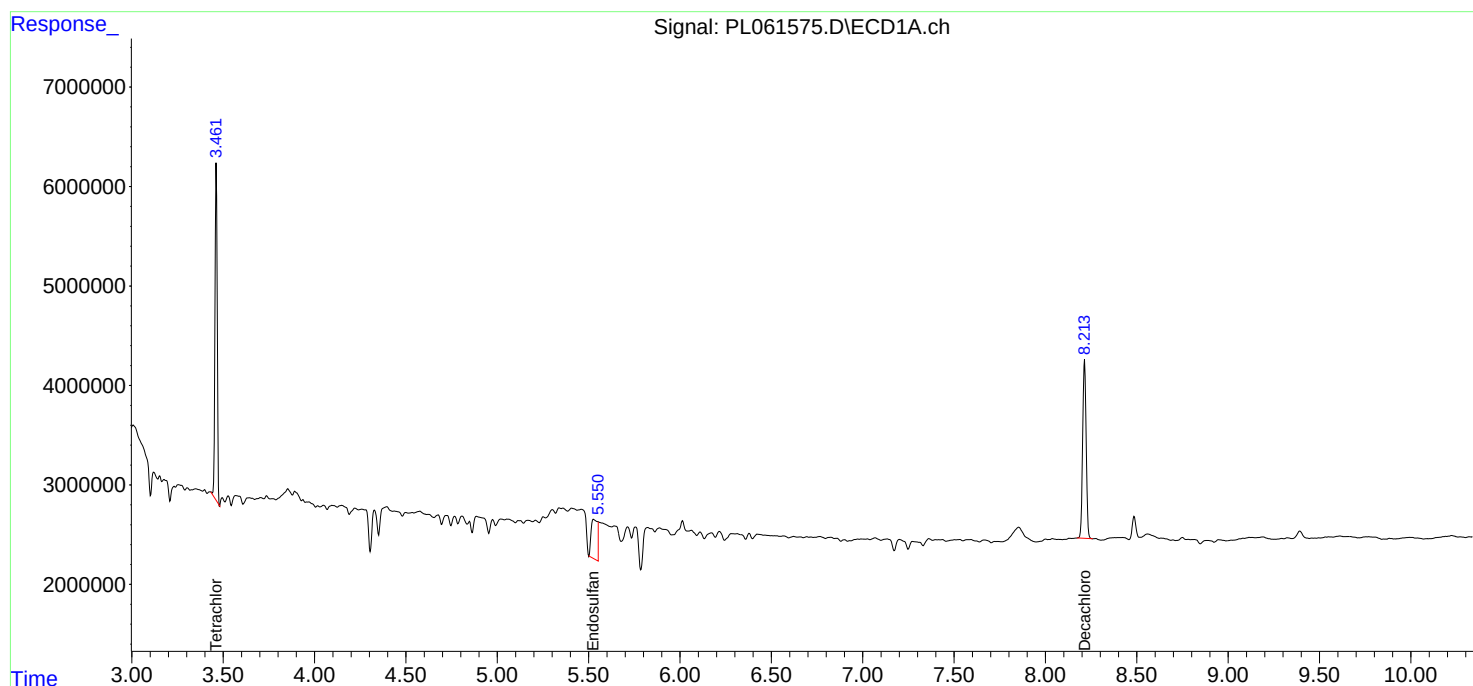


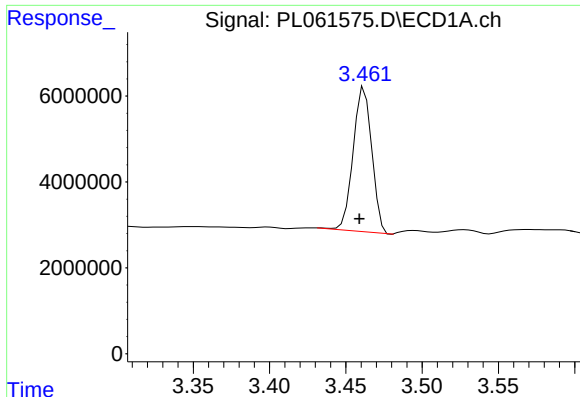

#1 Tetrachloro-m-xylene


R.T.: 3.462 min
Delta R.T.: 0.003 min
Response: 28609568
Conc: 16.59 ng/ml

Instrument :
ECD_L
ClientSampleId :

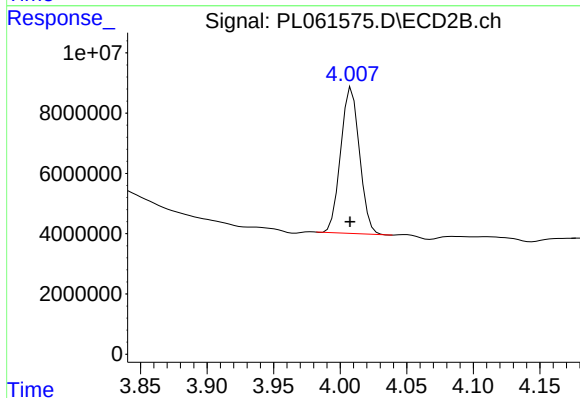


#1 Tetrachloro-m-xylene

R.T.: 4.009 min
Delta R.T.: 0.001 min
Response: 47700503
Conc: 15.51 ng/ml

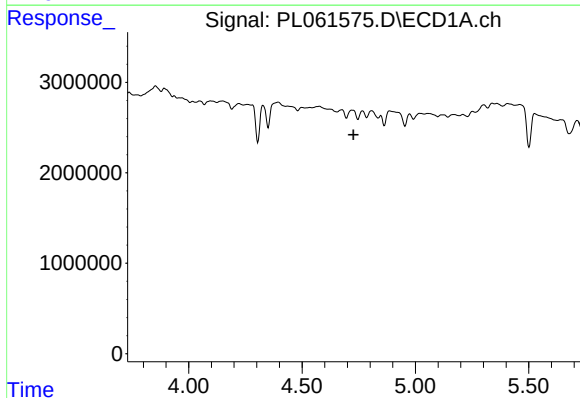


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.727 min
Response: 0
Conc: N.D.

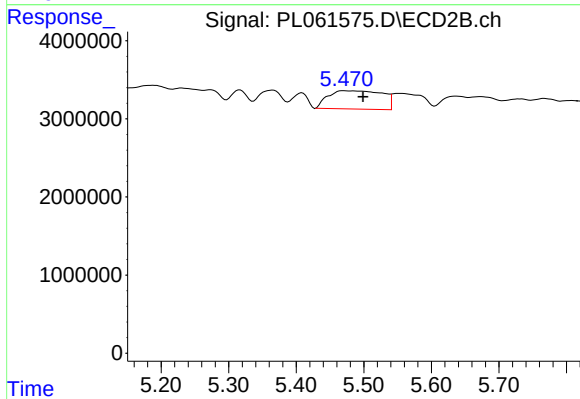

#5 Aldrin


R.T.: 5.470 min
Delta R.T.: -0.028 min
Response: 13010568
Conc: 3.44 ng/ml

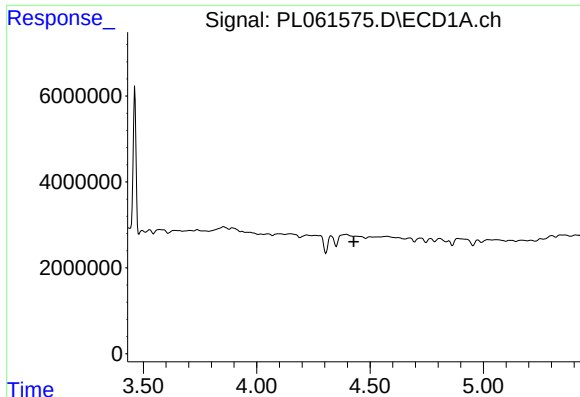

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.429 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

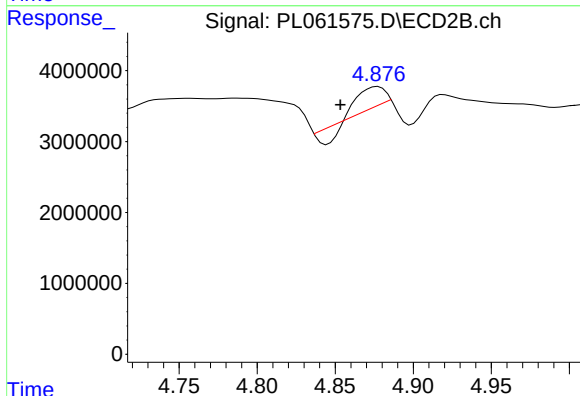


#6 beta-BHC

R.T.: 4.878 min
Delta R.T.: 0.024 min
Response: 2873084
Conc: 1.65 ng/ml

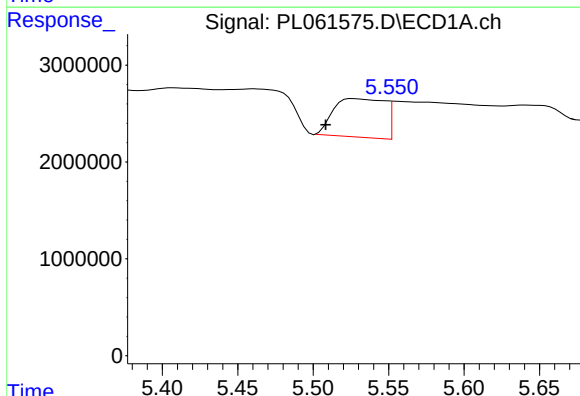


#9 Endosulfan I

R.T.: 5.527 min
Delta R.T.: 0.018 min
Response: 9264839
Conc: 5.39 ng/ml

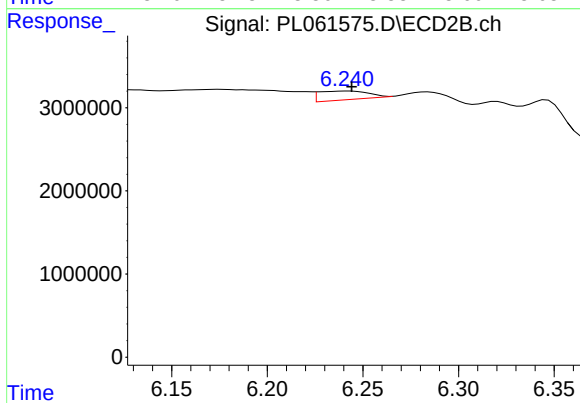

#9 Endosulfan I


R.T.: 6.242 min
Delta R.T.: -0.002 min
Response: 1875686
Conc: 0.58 ng/ml

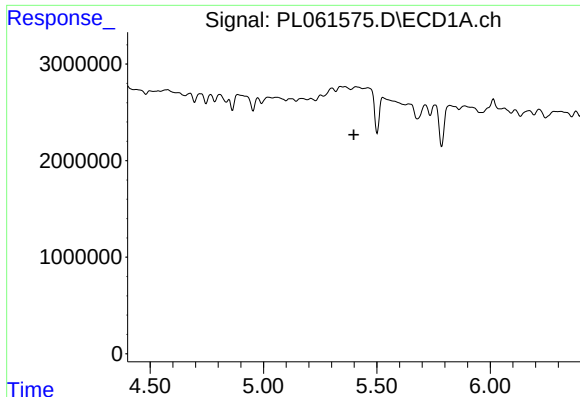

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.398 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

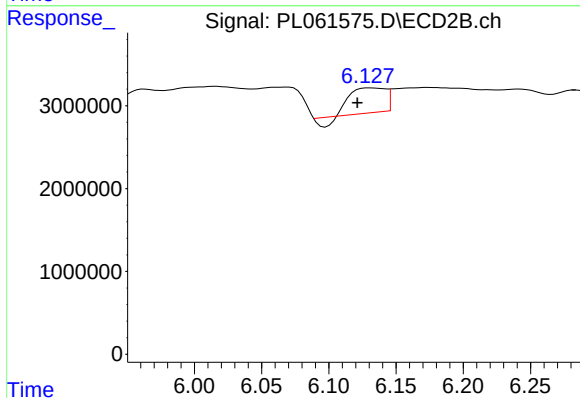


#10 gamma-Chlordane

R.T.: 6.130 min
Delta R.T.: 0.009 min
Response: 5086100
Conc: 1.48 ng/ml

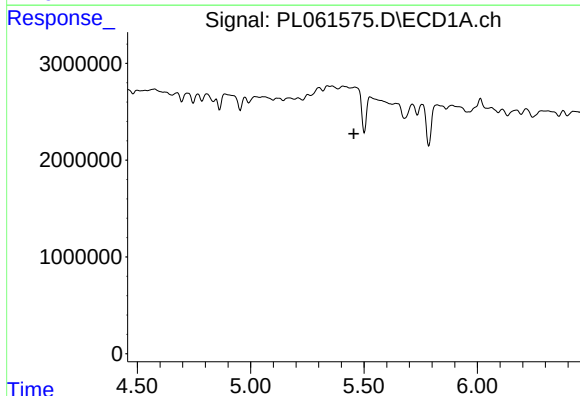


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.456 min
Response: 0
Conc: N.D.

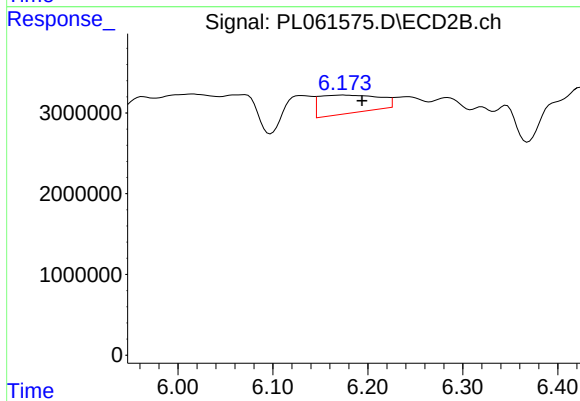

#11 alpha-Chlordane


R.T.: 6.175 min
Delta R.T.: -0.019 min
Response: 9750570
Conc: 2.80 ng/ml

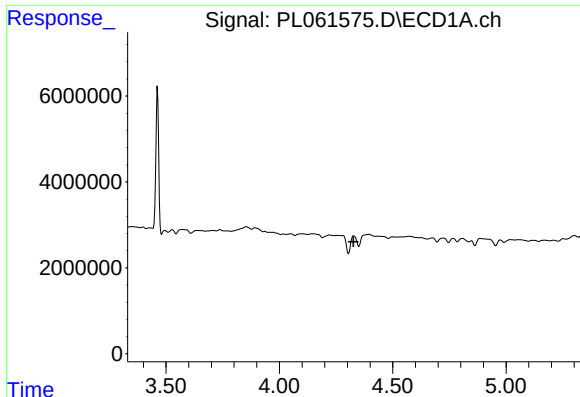

#23 Chlordane-1


R.T.: 4.328 min
Delta R.T.: 0.000 min
Response: -424624
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

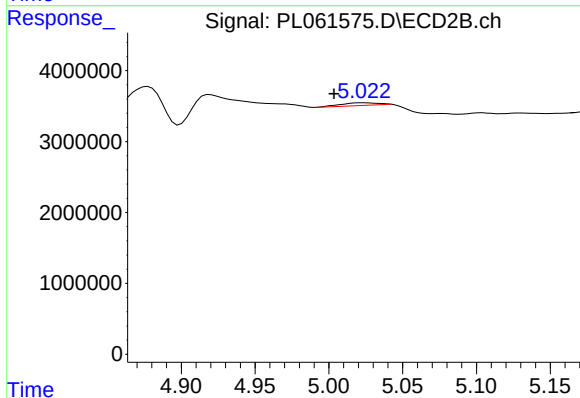


#23 Chlordane-1

R.T.: 5.024 min
Delta R.T.: 0.020 min
Response: 709841
Conc: 6.53 ng/ml

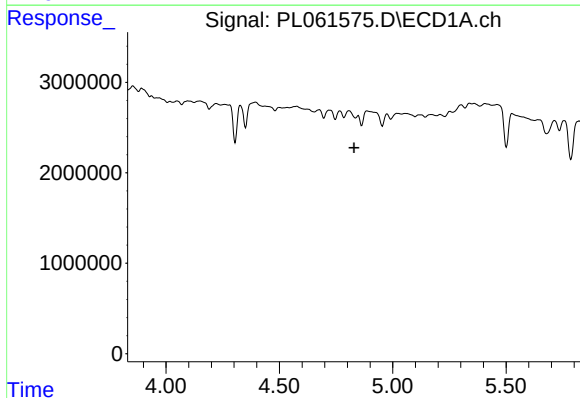


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 4.829 min
Response: 0
Conc: N.D.

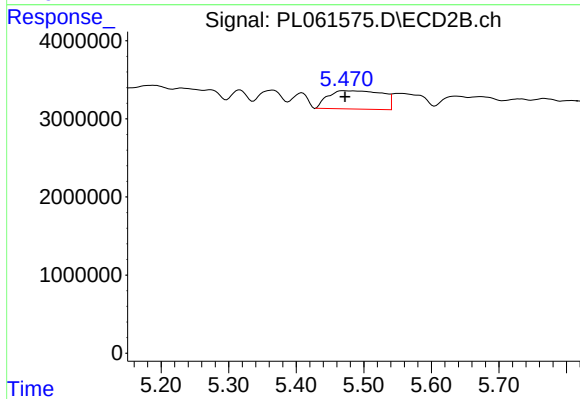

#24 Chlordane-2


R.T.: 5.470 min
Delta R.T.: -0.002 min
Response: 13010568
Conc: 106.52 ng/ml

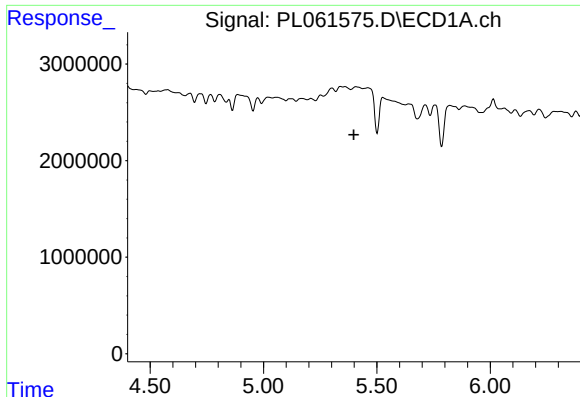

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.398 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

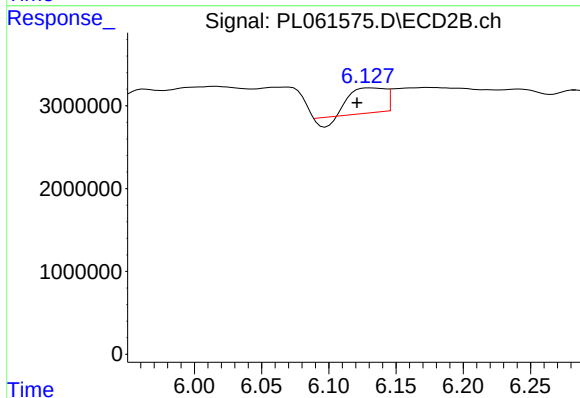


#25 Chlordane-3

R.T.: 6.130 min
Delta R.T.: 0.009 min
Response: 5086100
Conc: 11.77 ng/ml

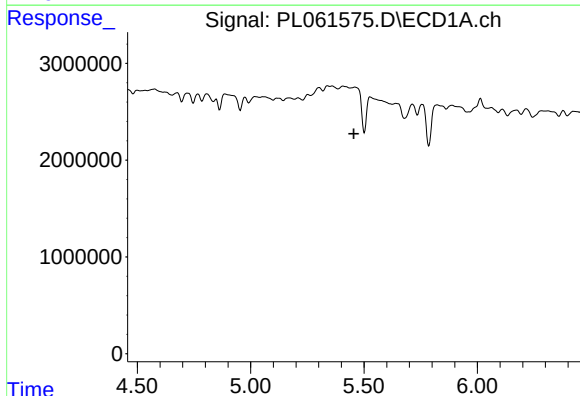


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.456 min
Response: 0
Conc: N.D.

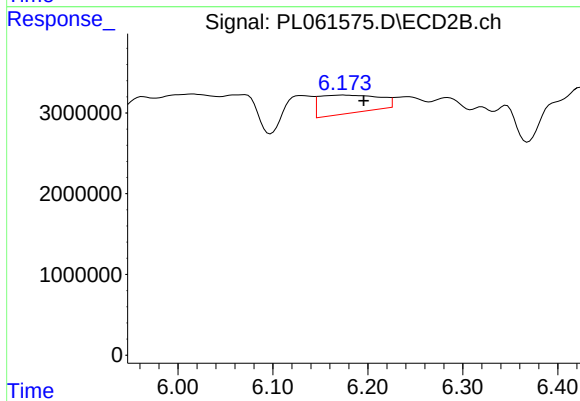

#26 Chlordane-4


R.T.: 6.175 min
Delta R.T.: -0.021 min
Response: 9750570
Conc: 18.63 ng/ml

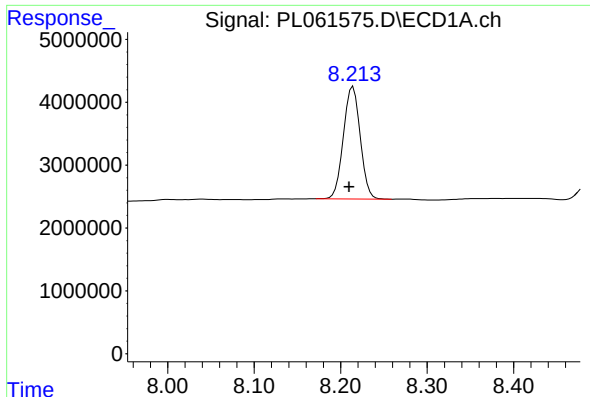

#28 Decachlorobiphenyl

R.T.: 8.214 min
Delta R.T.: 0.005 min
Response: 24006864
Conc: 14.39 ng/ml

Instrument :
ECD_L
ClientSampleId :

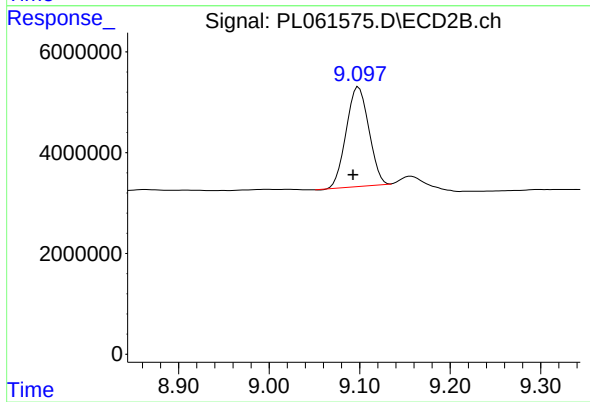

#28 Decachlorobiphenyl

R.T.: 9.099 min
Delta R.T.: 0.006 min
Response: 34242074
Conc: 14.48 ng/ml