

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091820\
 Data File : PL061596.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Sep 2020 16:28
 Operator : DD\AJ
 Sample : L4074-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 KTS-IB-0102-0-6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 18 17:43:33 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 09 01:27:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.459	4.007	21899218	36301043	12.697	11.802
28)	SA Decachlor...	8.210	9.095	18788193	27105905	11.262	11.463
Target Compounds							
13)	MA Dieldrin	0.000	6.494	0	3961857	N.D.	1.208 #
16)	A 4,4'-DDD	0.000	6.850	0	9353344	N.D.	3.642 #
17)	MA 4,4'-DDT	6.372	7.117f	3125773	6908228	2.276	2.760
19)	B Endosulfa...	6.660	0.000	4375643	0	2.659	N.D. #
20)	A Methoxychlor	6.906f	0.000	7017399	0	8.197	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091820\
Data File : PL061596.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Sep 2020 16:28
Operator : DD\AJ
Sample : L4074-01
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
KTS-IB-0102-0-6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 18 17:43:33 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
Quant Title : GC Extractables
QLast Update : Wed Sep 09 01:27:38 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

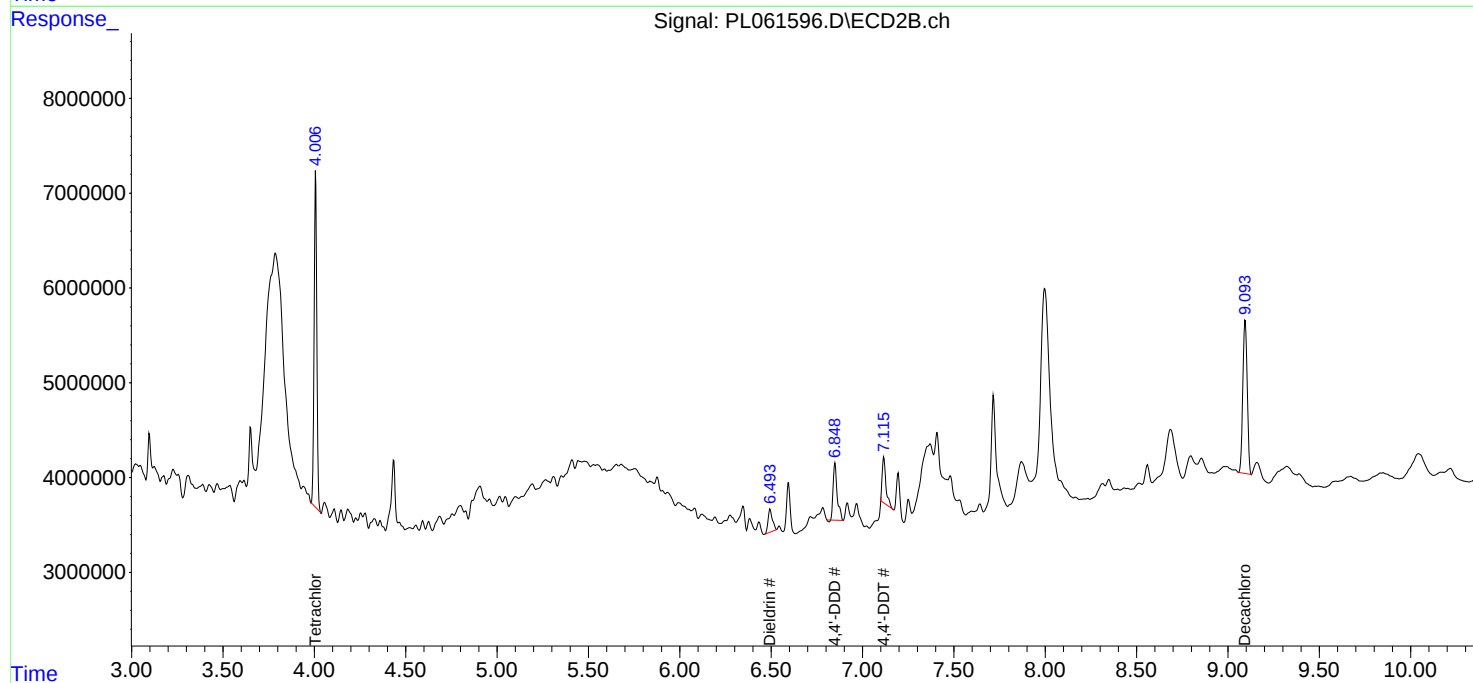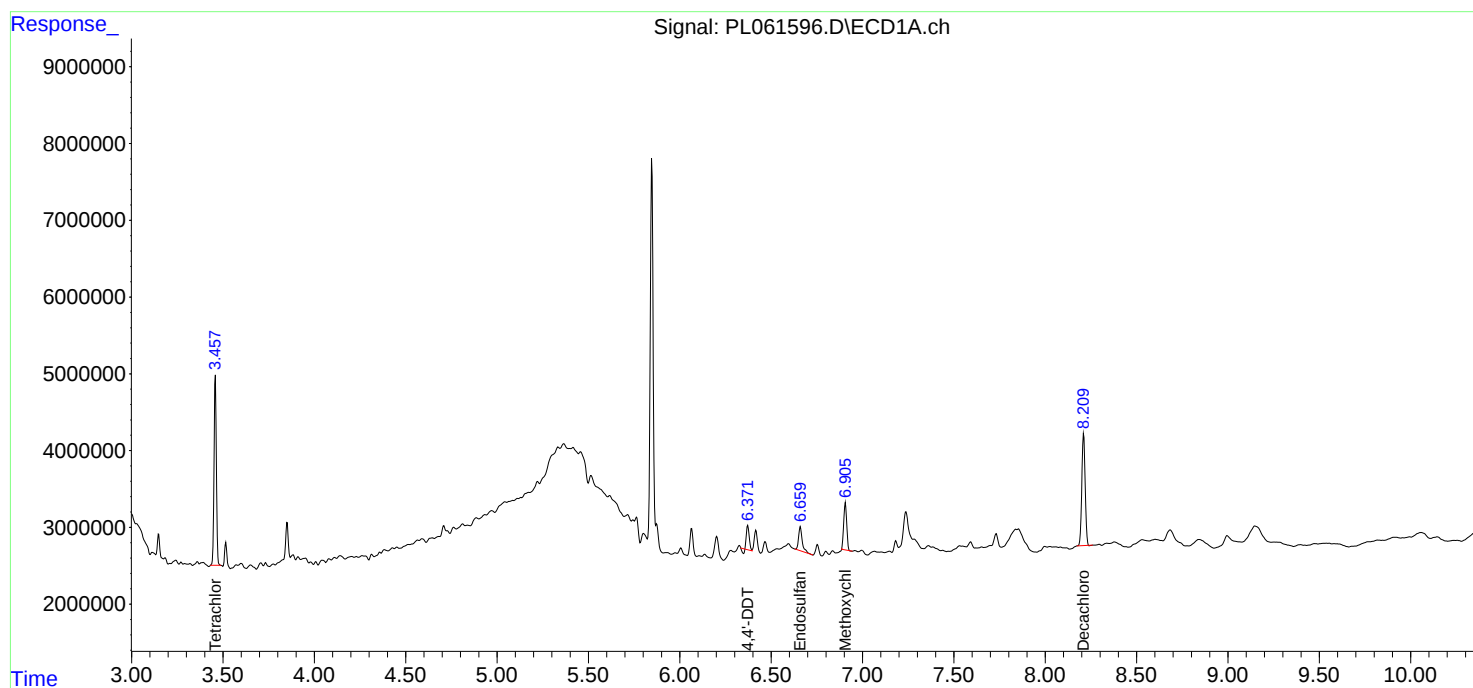


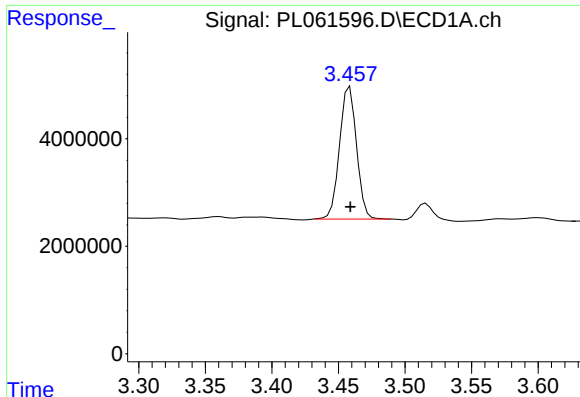

#1 Tetrachloro-m-xylene


R.T.: 3.459 min
Delta R.T.: 0.000 min
Response: 21899218
Conc: 12.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
KTS-IB-0102-0-6

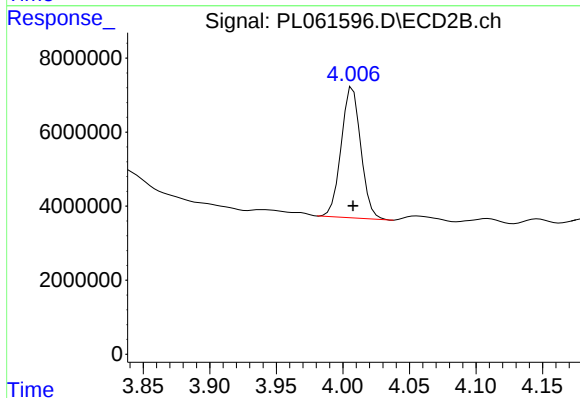


#1 Tetrachloro-m-xylene

R.T.: 4.007 min
Delta R.T.: 0.000 min
Response: 36301043
Conc: 11.80 ng/ml

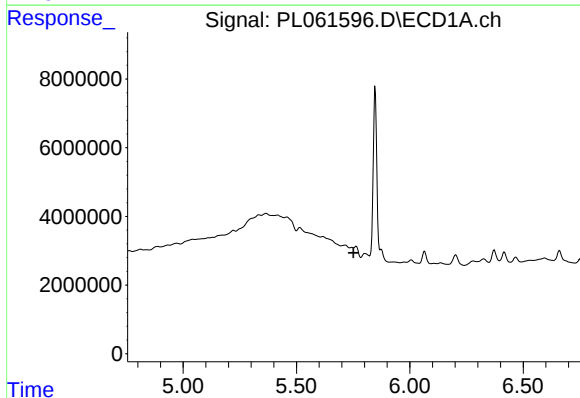


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 5.752 min
Response: 0
Conc: N.D.

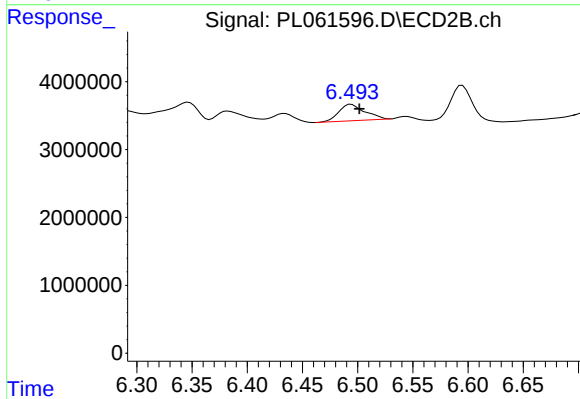

#13 Dieldrin


R.T.: 6.494 min
Delta R.T.: -0.007 min
Response: 3961857
Conc: 1.21 ng/ml

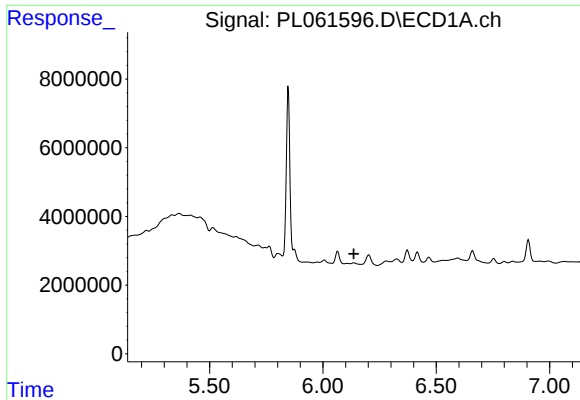

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.136 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
KTS-IB-0102-0-6

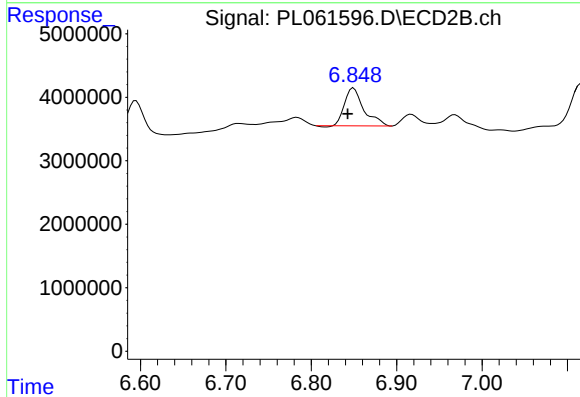


#16 4,4'-DDD

R.T.: 6.850 min
Delta R.T.: 0.007 min
Response: 9353344
Conc: 3.64 ng/ml

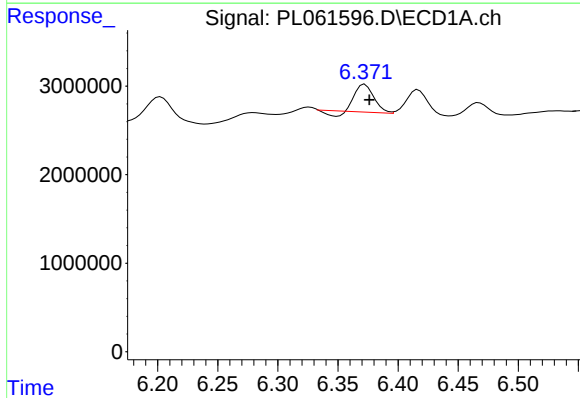


#17 4,4'-DDT

R.T.: 6.372 min
Delta R.T.: -0.004 min
Response: 3125773
Conc: 2.28 ng/ml

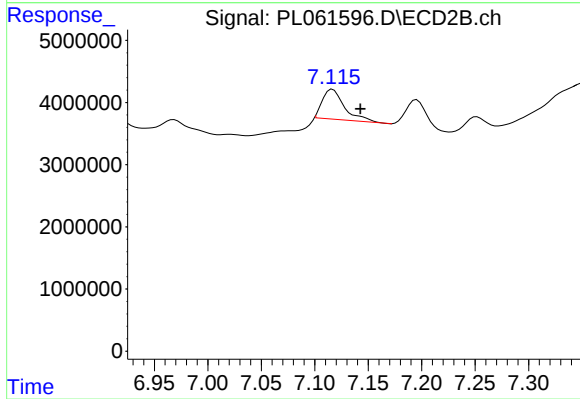

#17 4,4'-DDT


R.T.: 7.117 min
Delta R.T.: -0.026 min
Response: 6908228
Conc: 2.76 ng/ml

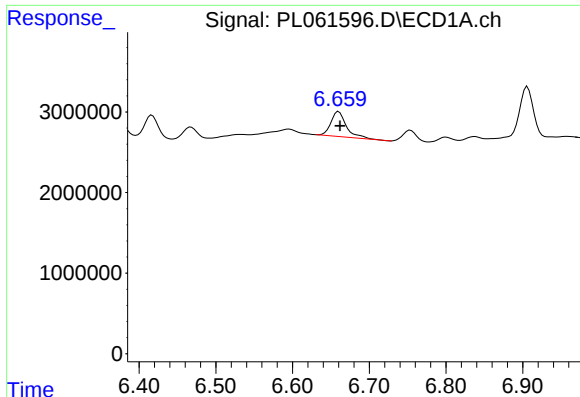

#19 Endosulfan Sulfate


R.T.: 6.660 min
Delta R.T.: -0.002 min
Response: 4375643
Conc: 2.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
KTS-IB-0102-0-6

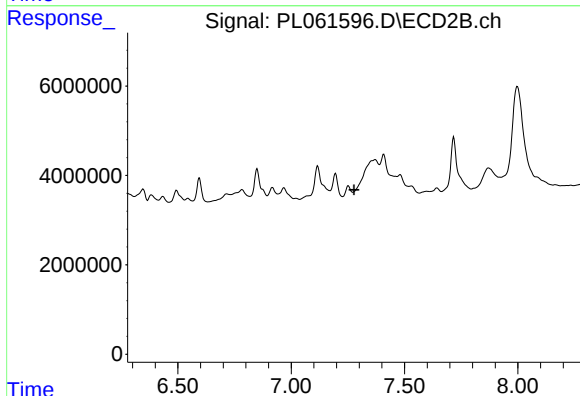


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.277 min
Response: 0
Conc: N.D.

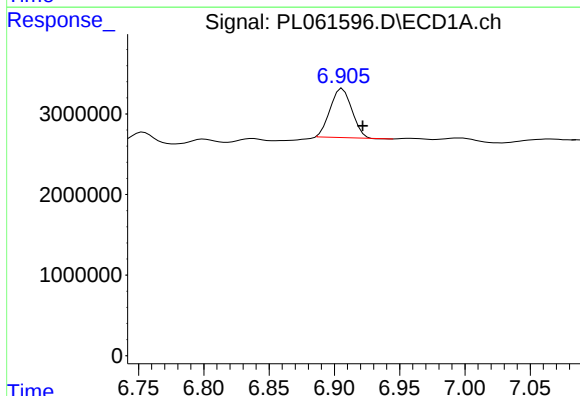


#20 Methoxychlor

R.T.: 6.906 min
Delta R.T.: -0.016 min
Response: 7017399
Conc: 8.20 ng/ml

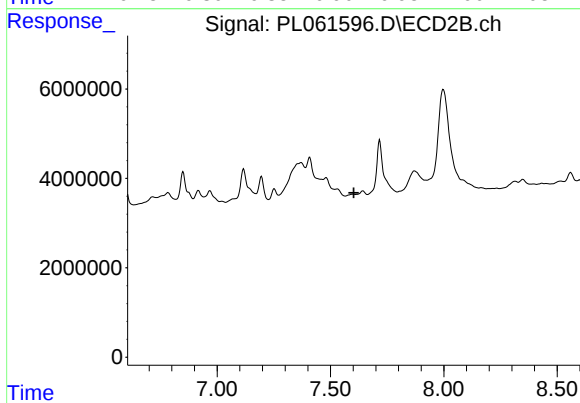

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.603 min
Response: 0
Conc: N.D.

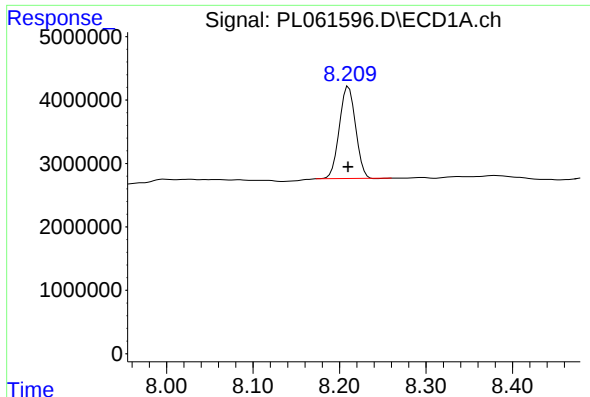

#28 Decachlorobiphenyl

R.T.: 8.210 min
Delta R.T.: 0.000 min
Response: 18788193
Conc: 11.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
KTS-IB-0102-0-6

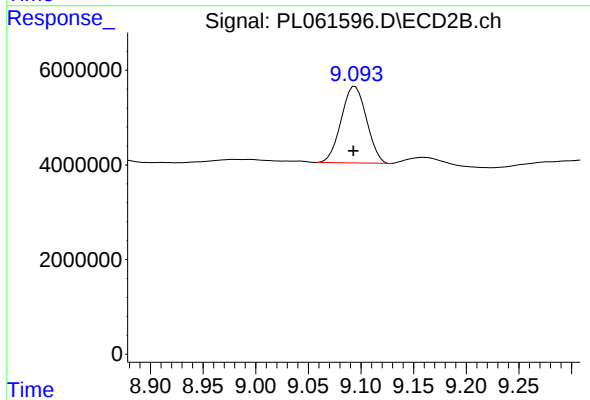

#28 Decachlorobiphenyl

R.T.: 9.095 min
Delta R.T.: 0.002 min
Response: 27105905
Conc: 11.46 ng/ml