

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091820\
 Data File : PL061576.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Sep 2020 10:07
 Operator : DD\AJ
 Sample : L4038-09
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PAV-B36-091620-10-15

Manual Integrations
 APPROVED

Ankita
 9/21/2020 12:26:33 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 18 15:15:56 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 09 01:27:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.458	4.007	27492339	34861899	15.940	11.334m#
28)	SA Decachlor...	8.212	9.095	21531059	34505680	12.906	14.593m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091820\
Data File : PL061576.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Sep 2020 10:07
Operator : DD\AJ
Sample : L4038-09
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PAV-B36-091620-10-15


Manual Integrations
APPROVED

Ankita
9/21/2020 12:26:33 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 18 15:15:56 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
Quant Title : GC Extractables
QLast Update : Wed Sep 09 01:27:38 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

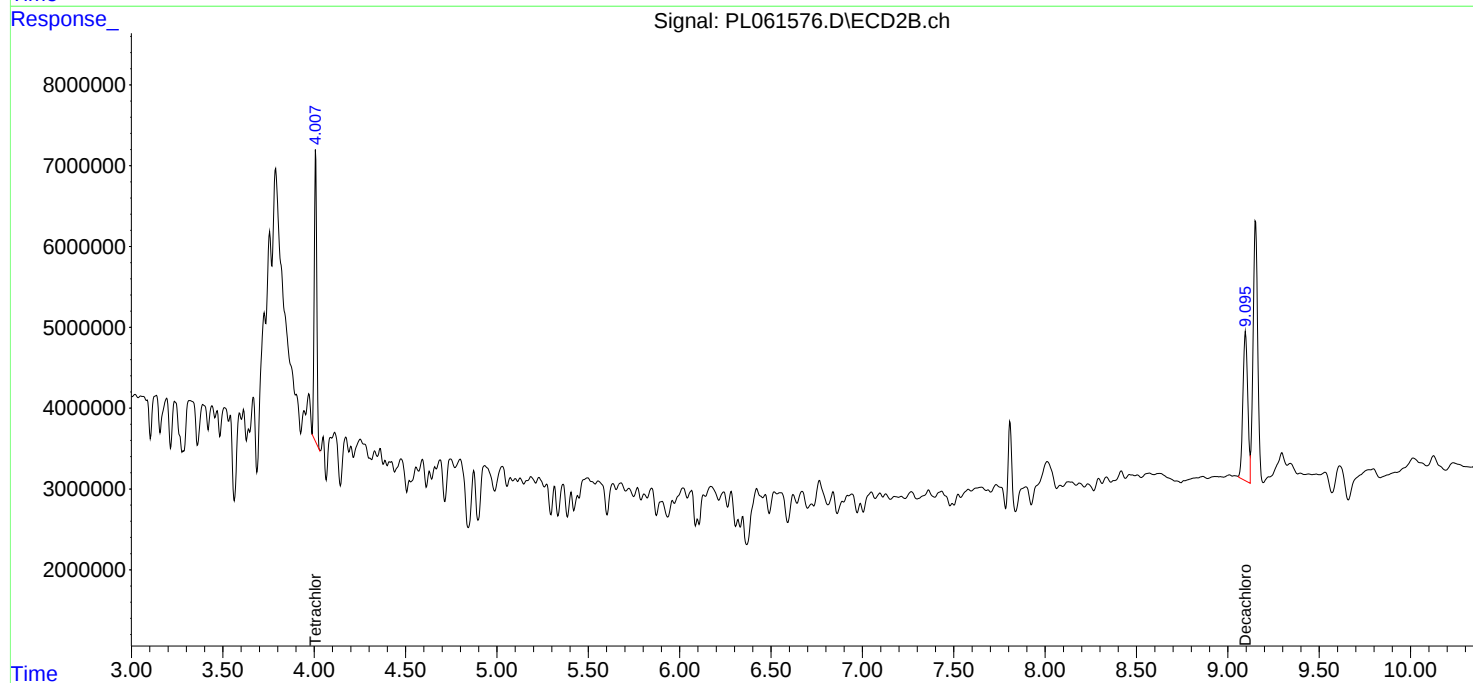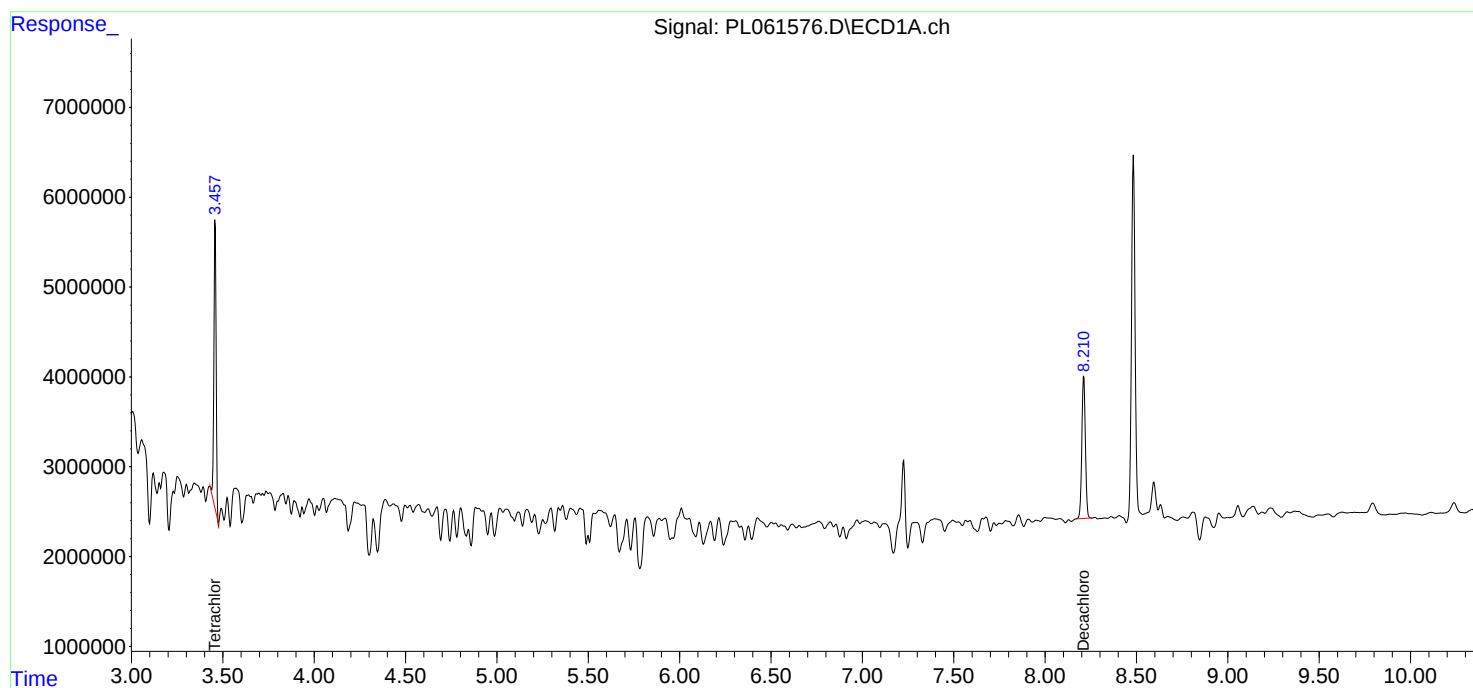

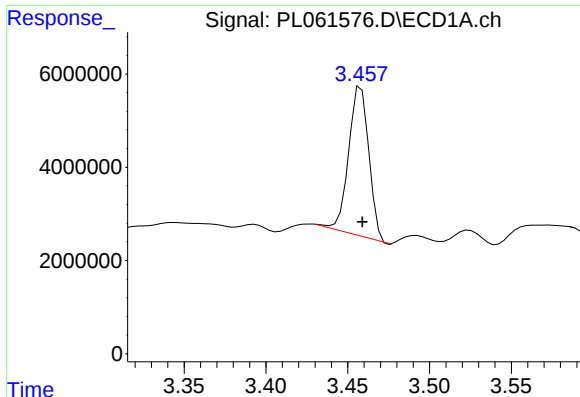


#1 Tetrachloro-m-xylene

R.T.: 3.458 min
Delta R.T.: 0.000 min
Response: 27492339
Conc: 15.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
PAV-B36-091620-10-15


Manual Integrations
APPROVED

Ankita
9/21/2020 12:26:33 PM

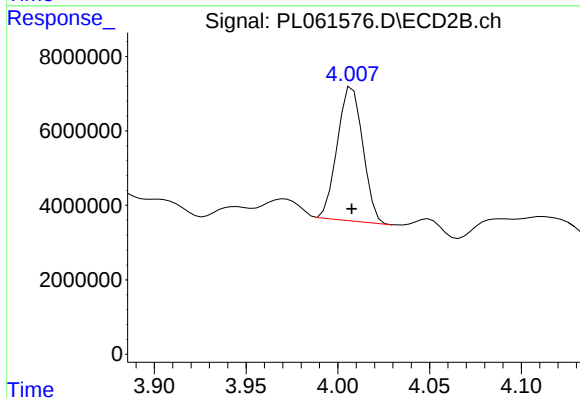


#1 Tetrachloro-m-xylene

R.T.: 4.007 min
Delta R.T.: 0.000 min
Response: 34861899
Conc: 11.33 ng/ml m

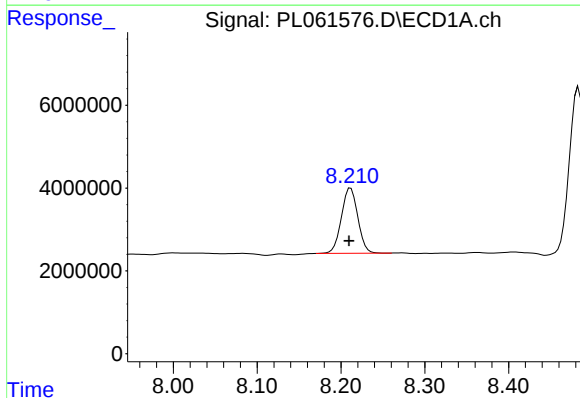

#28 Decachlorobiphenyl

R.T.: 8.212 min
Delta R.T.: 0.002 min
Response: 21531059
Conc: 12.91 ng/ml

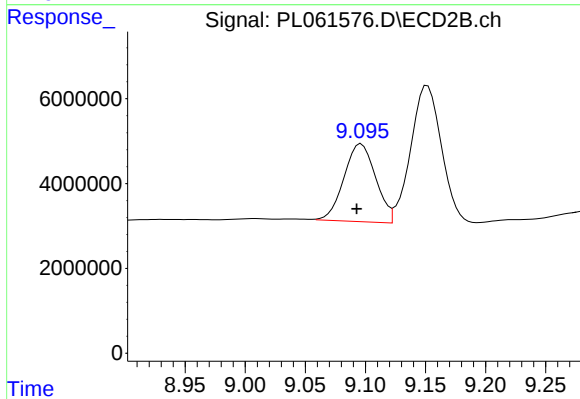

#28 Decachlorobiphenyl

R.T.: 9.095 min
Delta R.T.: 0.002 min
Response: 34505680
Conc: 14.59 ng/ml m