

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL091825\  
 Data File : PL097240.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 17 Sep 2025 16:00  
 Operator : AR\AJ  
 Sample : HEXANE  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 ECD\_L  
 ClientSampleId :  
 HEXANE

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Sep 18 02:00:03 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL082025.M  
 Quant Title : GC Extractables  
 QLast Update : Thu Aug 21 06:34:01 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

#### System Monitoring Compounds

##### Target Compounds

|        |              |        |       |          |          |        |        |   |
|--------|--------------|--------|-------|----------|----------|--------|--------|---|
| 8) B   | Heptachlo... | 5.645  | 0.000 | 57128016 | 0        | 11.102 | N.D.   | # |
| 13) MA | Dieldrin     | 0.000  | 5.418 | 0        | 18423283 | N.D.   | 2.811  | # |
| 14) MA | Endrin       | 0.000  | 5.711 | 0        | 37511030 | N.D.   | 6.350  | # |
| 15) B  | Endosulfa... | 6.774f | 0.000 | 3985402  | 0        | 0.905  | N.D.   | # |
| 24)    | Chlordane-2  | 0.000  | 4.403 | 0        | 3419670  | N.D.   | 14.610 | # |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL091825\  
Data File : PL097240.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 17 Sep 2025 16:00  
Operator : AR\AJ  
Sample : HEXANE  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
ECD\_L  
ClientSampleId :  
HEXANE

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 18 02:00:03 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL082025.M  
Quant Title : GC Extractables  
QLast Update : Thu Aug 21 06:34:01 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

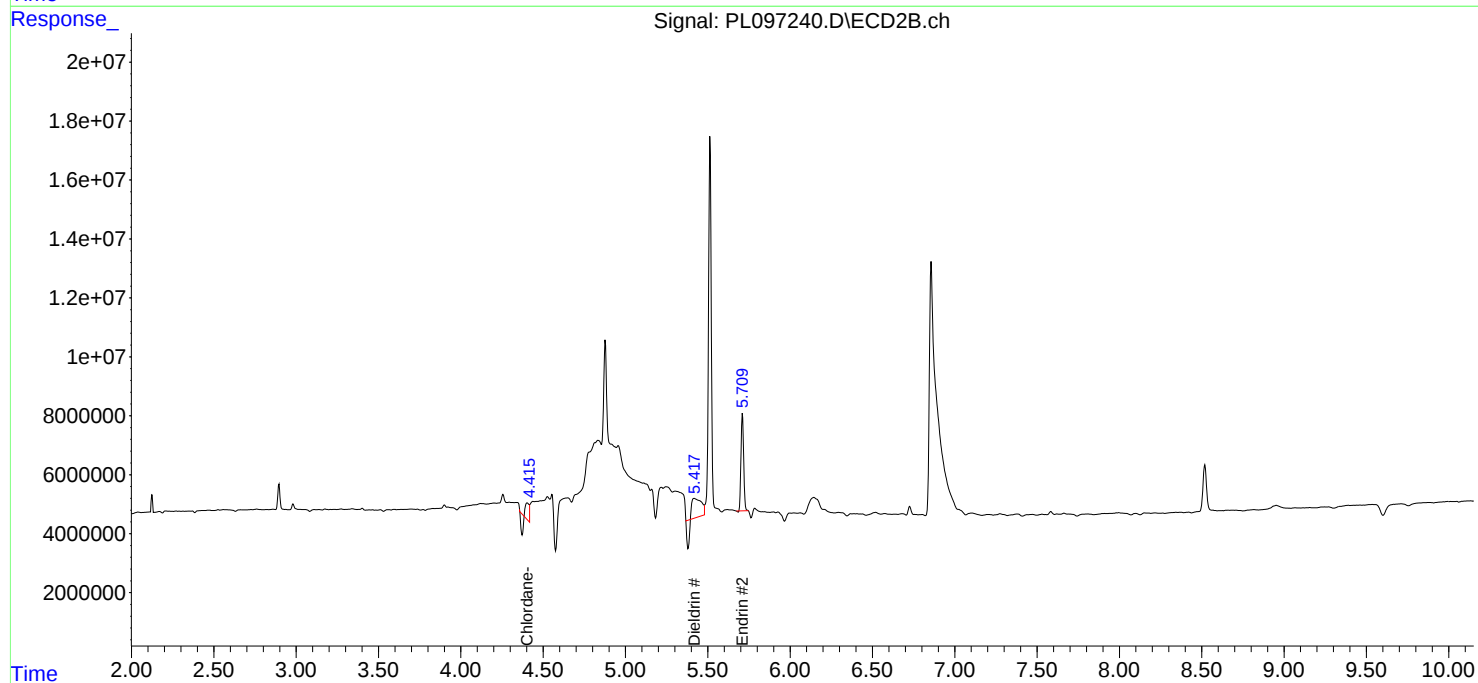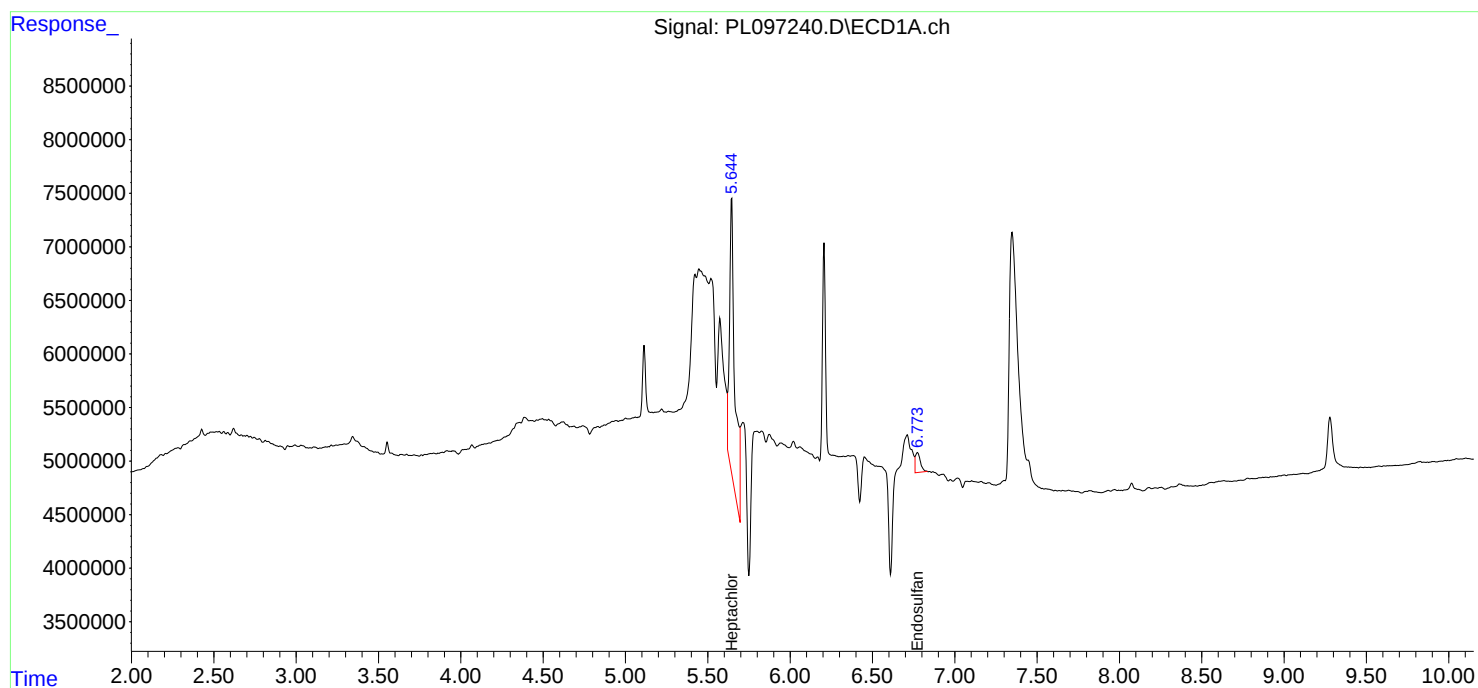


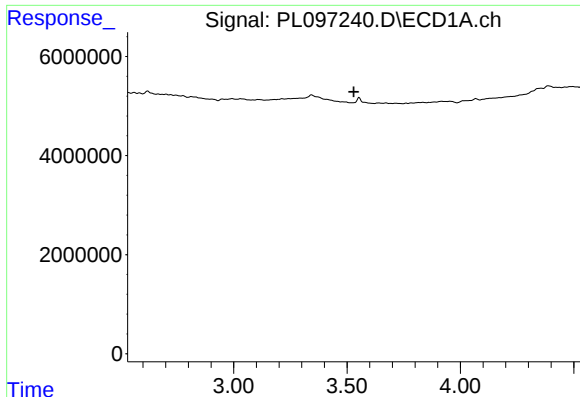

#1 Tetrachloro-m-xylene


R.T.: 0.000 min  
Exp R.T.: 3.530 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_L  
ClientSampleId :  
HEXANE

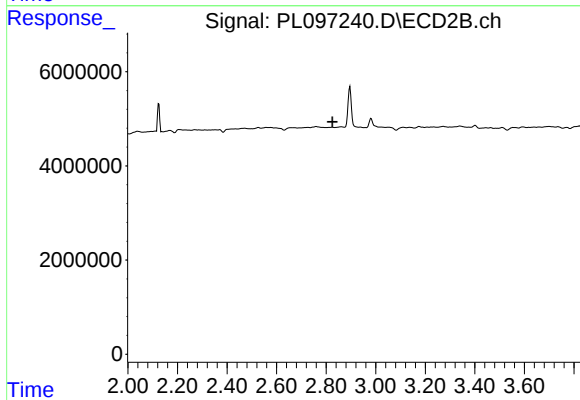


#1 Tetrachloro-m-xylene

R.T.: 0.000 min  
Exp R.T.: 2.825 min  
Response: 0  
Conc: N.D.

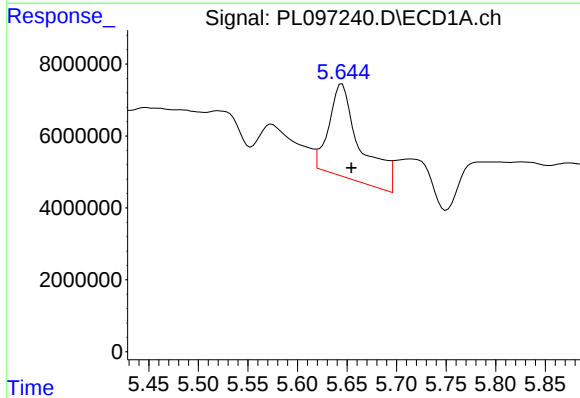


#8 Heptachlor epoxide

R.T.: 5.645 min  
Delta R.T.: -0.009 min  
Response: 57128016  
Conc: 11.10 ng/ml

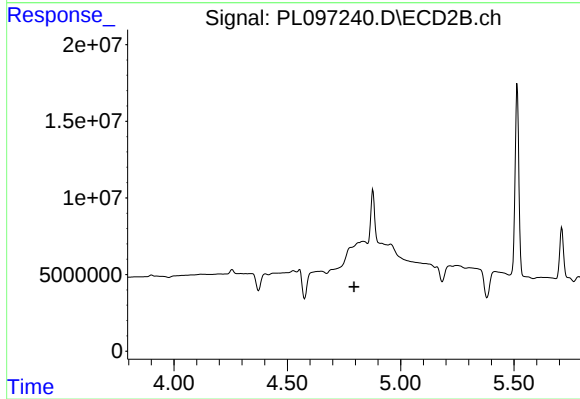

#8 Heptachlor epoxide


R.T.: 0.000 min  
Exp R.T.: 4.795 min  
Response: 0  
Conc: N.D.

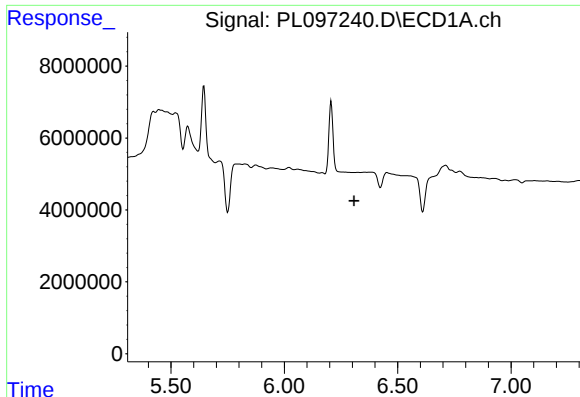

#13 Dieldrin


R.T.: 0.000 min  
Exp R.T.: 6.308 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_L  
ClientSampleId :  
HEXANE

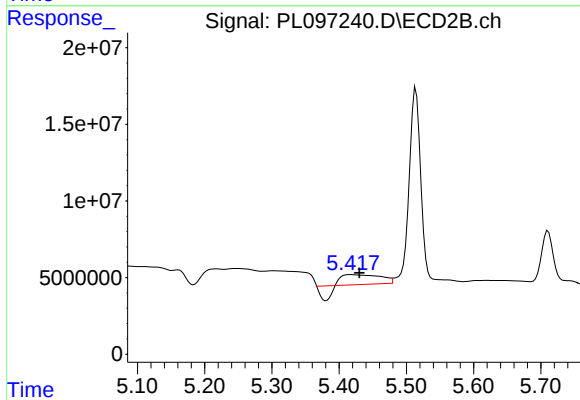


#13 Dieldrin

R.T.: 5.418 min  
Delta R.T.: -0.012 min  
Response: 18423283  
Conc: 2.81 ng/ml

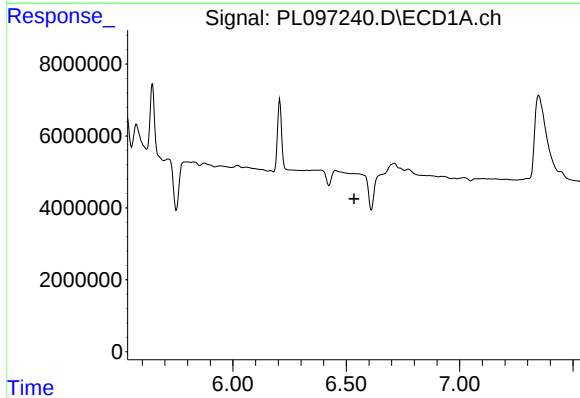


#14 Endrin

R.T.: 0.000 min  
Exp R.T.: 6.534 min  
Response: 0  
Conc: N.D.

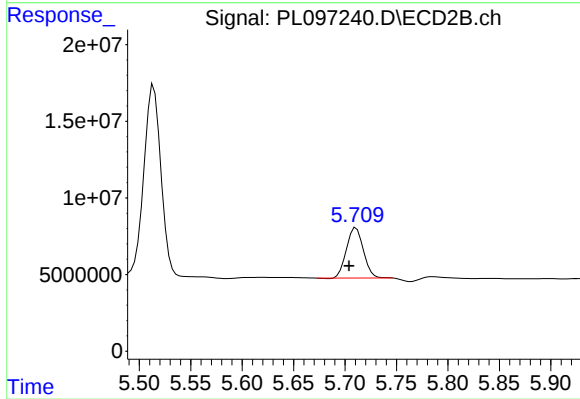

#14 Endrin


R.T.: 5.711 min  
Delta R.T.: 0.007 min  
Response: 37511030  
Conc: 6.35 ng/ml

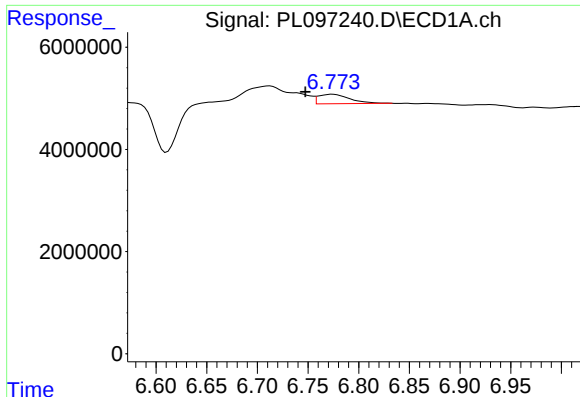

#15 Endosulfan II


R.T.: 6.774 min  
Delta R.T.: 0.026 min  
Response: 3985402  
Conc: 0.90 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :  
HEXANE

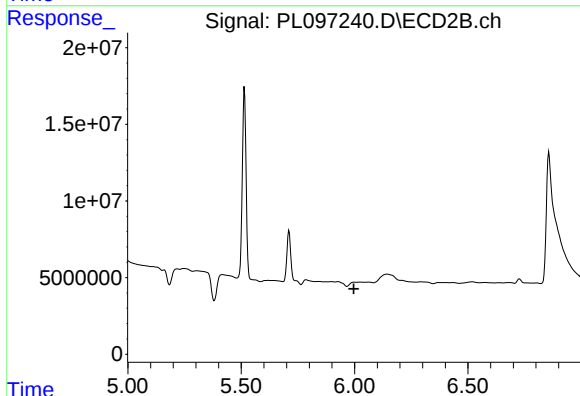


#15 Endosulfan II

R.T.: 0.000 min  
Exp R.T. : 5.996 min  
Response: 0  
Conc: N.D.

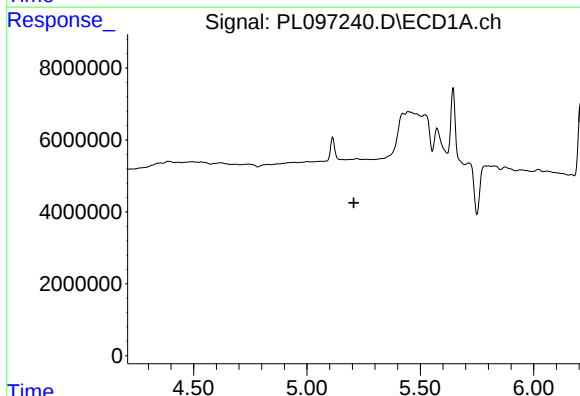


#24 Chlordane-2

R.T.: 0.000 min  
Exp R.T. : 5.206 min  
Response: 0  
Conc: N.D.

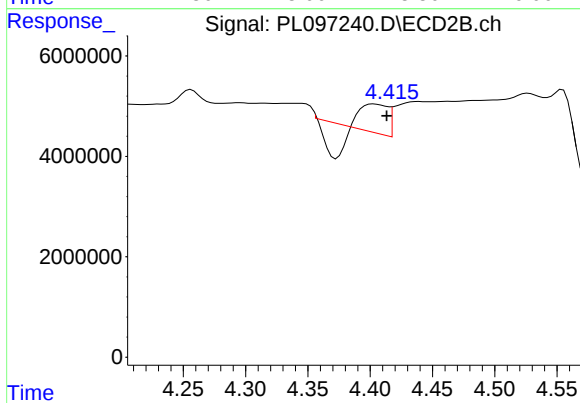

#24 Chlordane-2


R.T.: 4.403 min  
Delta R.T.: -0.010 min  
Response: 3419670  
Conc: 14.61 ng/ml

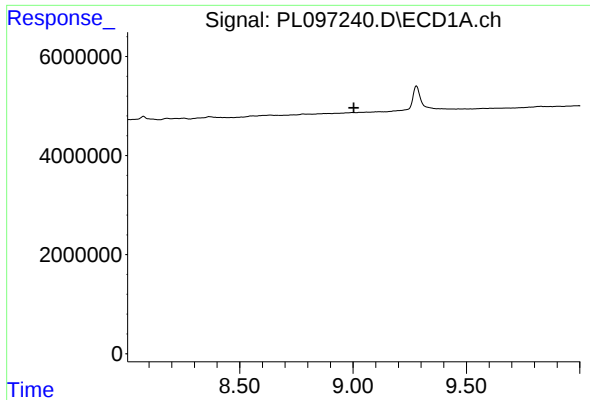

#28 Decachlorobiphenyl

R.T.: 0.000 min  
Exp R.T. : 9.004 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_L  
ClientSampleId :  
HEXANE

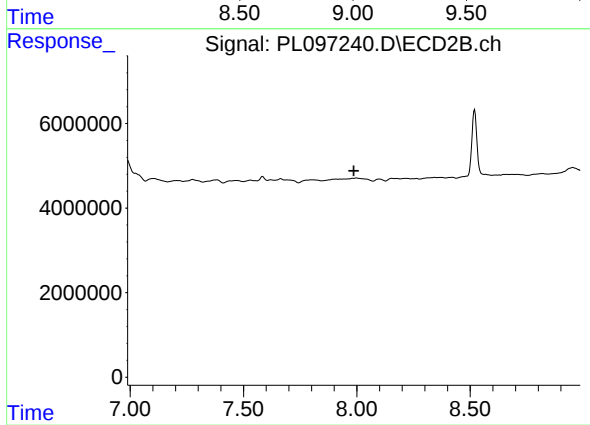

#28 Decachlorobiphenyl

R.T.: 0.000 min  
Exp R.T. : 7.987 min  
Response: 0  
Conc: N.D.