

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091825\
 Data File : PL097246.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Sep 2025 17:36
 Operator : AR\AJ
 Sample : Q3115-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TR-05-09162025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 18 02:00:47 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082025.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 21 06:34:01 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.528	2.824	41569954	57362891	10.540	10.177
28)	SA Decachlor...	9.000	7.983	44794352	60918132	15.130	12.702
Target Compounds							
10)	B gamma-Chl...	5.906	0.000	4525542	0	0.983	N.D. #
11)	B alpha-Chl...	5.989	0.000	7138404	0	1.517	N.D. #
23)	Chlordane-1	0.000	3.827	0	10040159	N.D.	51.295 #
25)	Chlordane-3	5.906	0.000	4525542	0	7.196	N.D. #
26)	Chlordane-4	5.989	0.000	7138404	0	8.777	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091825\
Data File : PL097246.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Sep 2025 17:36
Operator : AR\AJ
Sample : Q3115-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TR-05-09162025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 18 02:00:47 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082025.M
Quant Title : GC Extractables
QLast Update : Thu Aug 21 06:34:01 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

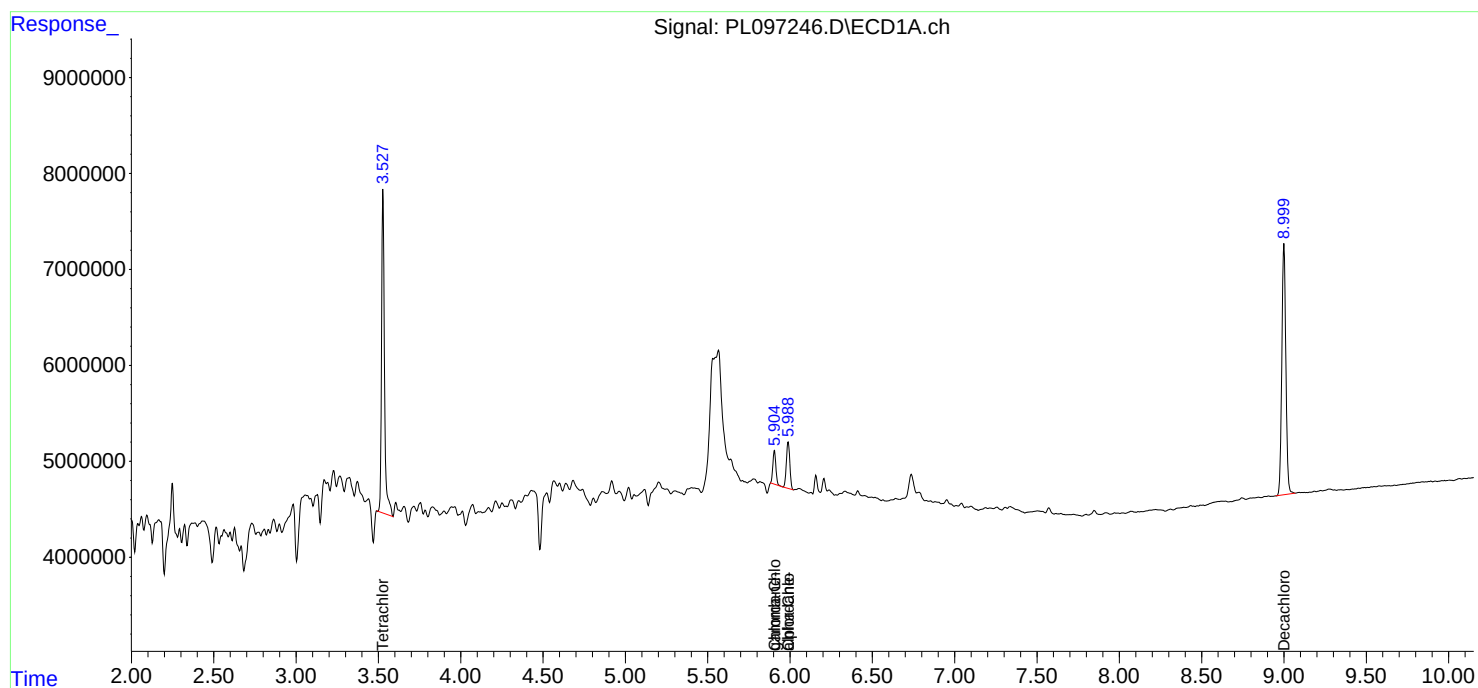


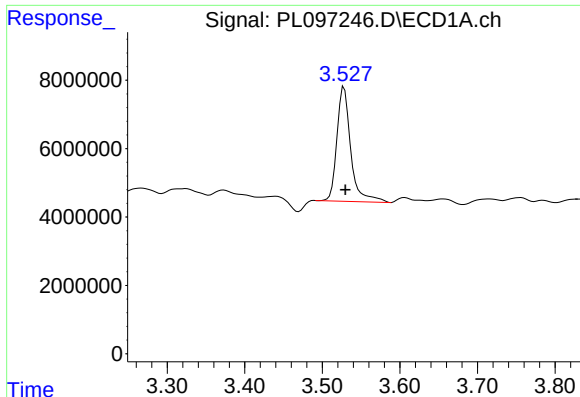

#1 Tetrachloro-m-xylene


R.T.: 3.528 min
Delta R.T.: -0.002 min
Response: 41569954
Conc: 10.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-05-09162025

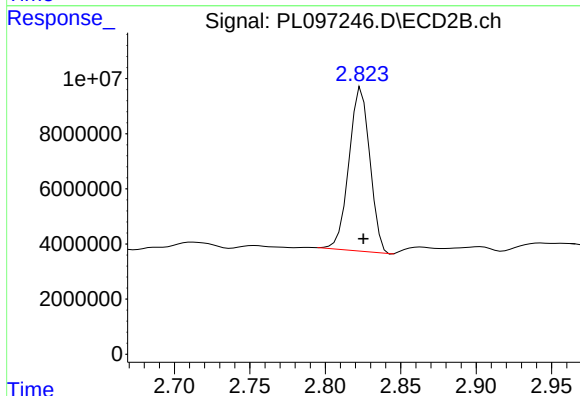


#1 Tetrachloro-m-xylene

R.T.: 2.824 min
Delta R.T.: -0.001 min
Response: 57362891
Conc: 10.18 ng/ml

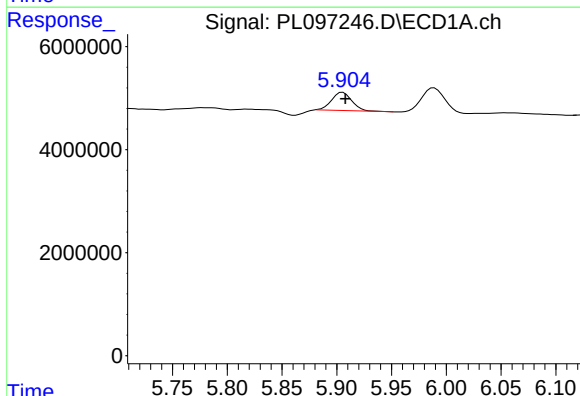


#10 gamma-Chlordane

R.T.: 5.906 min
Delta R.T.: -0.002 min
Response: 4525542
Conc: 0.98 ng/ml

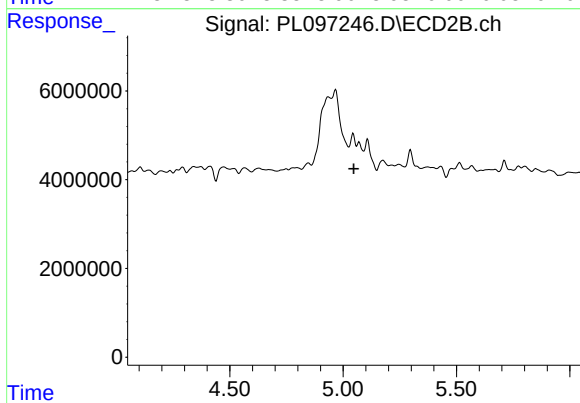

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.047 min
Response: 0
Conc: N.D.

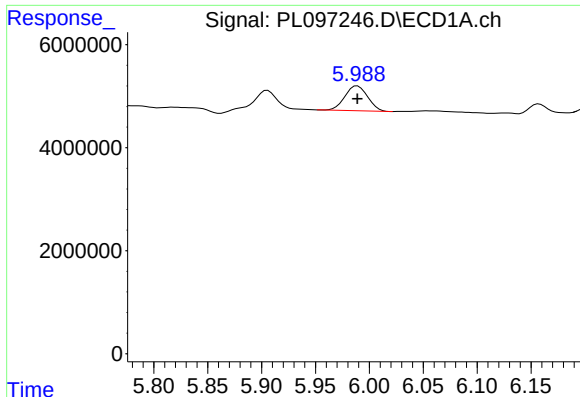

#11 alpha-Chlordane


R.T.: 5.989 min
Delta R.T.: 0.000 min
Response: 7138404
Conc: 1.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-05-09162025

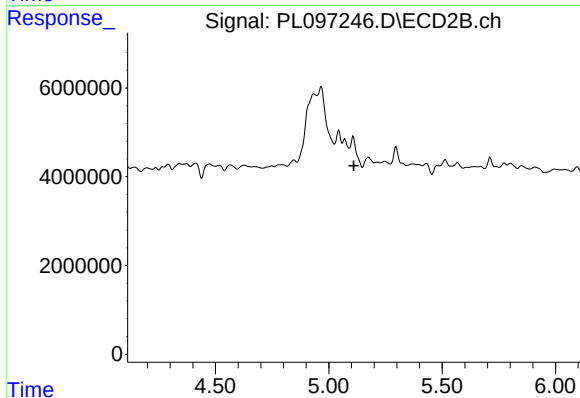


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.111 min
Response: 0
Conc: N.D.

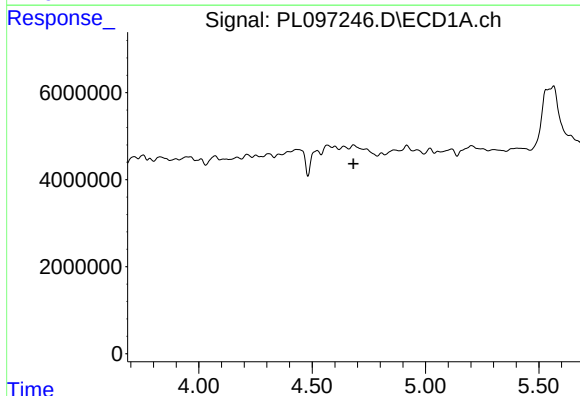


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.683 min
Response: 0
Conc: N.D.

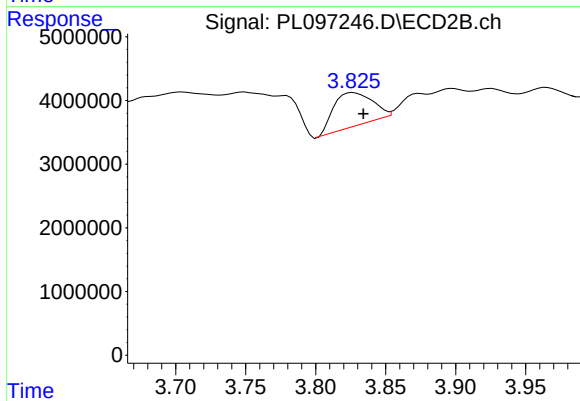

#23 Chlordane-1


R.T.: 3.827 min
Delta R.T.: -0.007 min
Response: 10040159
Conc: 51.29 ng/ml

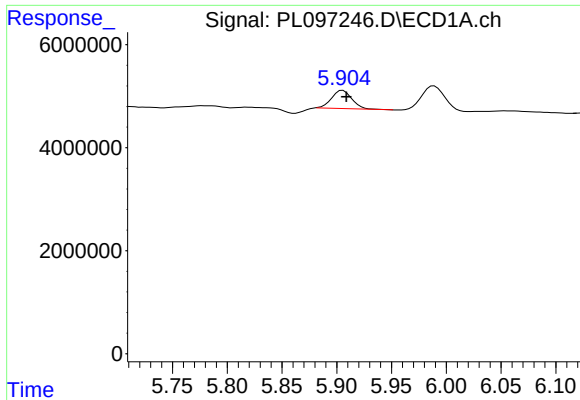

#25 Chlordane-3


R.T.: 5.906 min
Delta R.T.: -0.003 min
Response: 4525542
Conc: 7.20 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-05-09162025

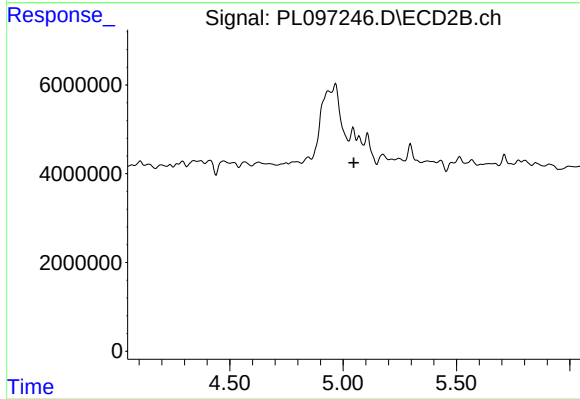


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.046 min
Response: 0
Conc: N.D.

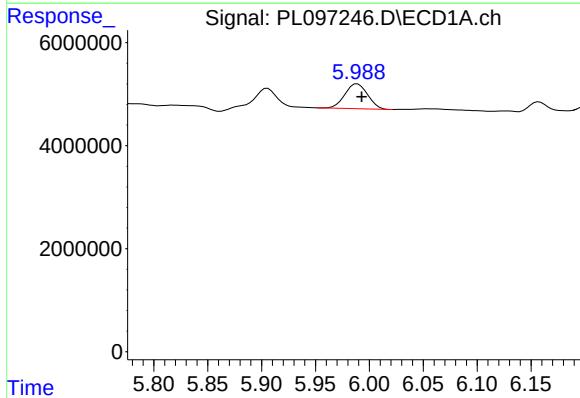


#26 Chlordane-4

R.T.: 5.989 min
Delta R.T.: -0.004 min
Response: 7138404
Conc: 8.78 ng/ml

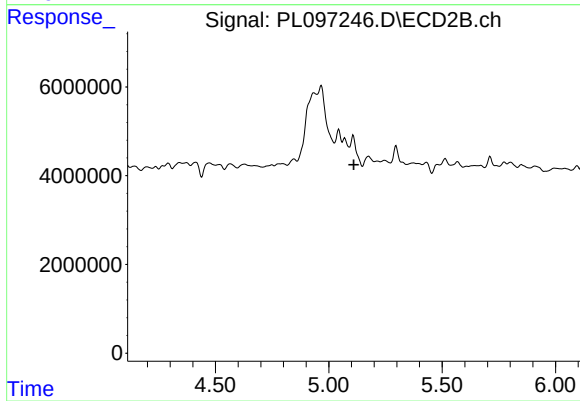

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 5.110 min
Response: 0
Conc: N.D.

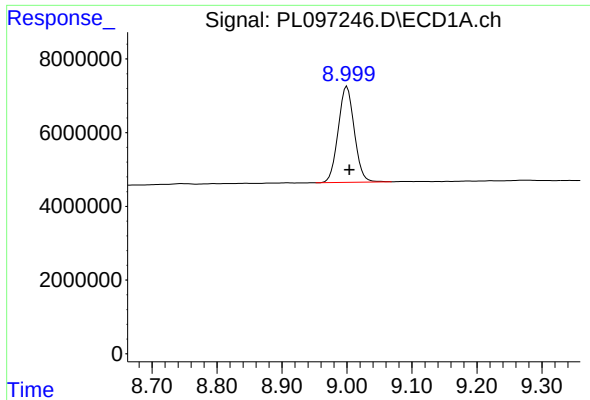

#28 Decachlorobiphenyl

R.T.: 9.000 min
Delta R.T.: -0.004 min
Response: 44794352
Conc: 15.13 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-05-09162025

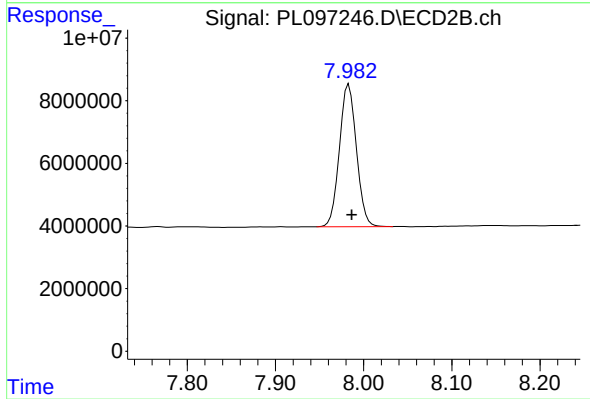

#28 Decachlorobiphenyl

R.T.: 7.983 min
Delta R.T.: -0.003 min
Response: 60918132
Conc: 12.70 ng/ml