

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091918\
 Data File : PL040131.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Sep 2018 20:01
 Operator : AJ\SJ
 Sample : PB113025TB
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 20 01:18:00 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 14 23:10:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.299	3.903	139.7E6	57975608	18.019	18.170
28)	SA Decachlor...	7.953	8.891	160.4E6	58916640	19.247	21.692
Target Compounds							
19)	B Endosulfa...	6.448	0.000	46008015	0	5.020	N.D. #
20)	A Methoxychlor	6.628f	0.000	68793562	0	14.842	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091918\
Data File : PL040131.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Sep 2018 20:01
Operator : AJ\SJ
Sample : PB113025TB
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 20 01:18:00 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
Quant Title : GC Extractables
QLast Update : Fri Sep 14 23:10:39 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

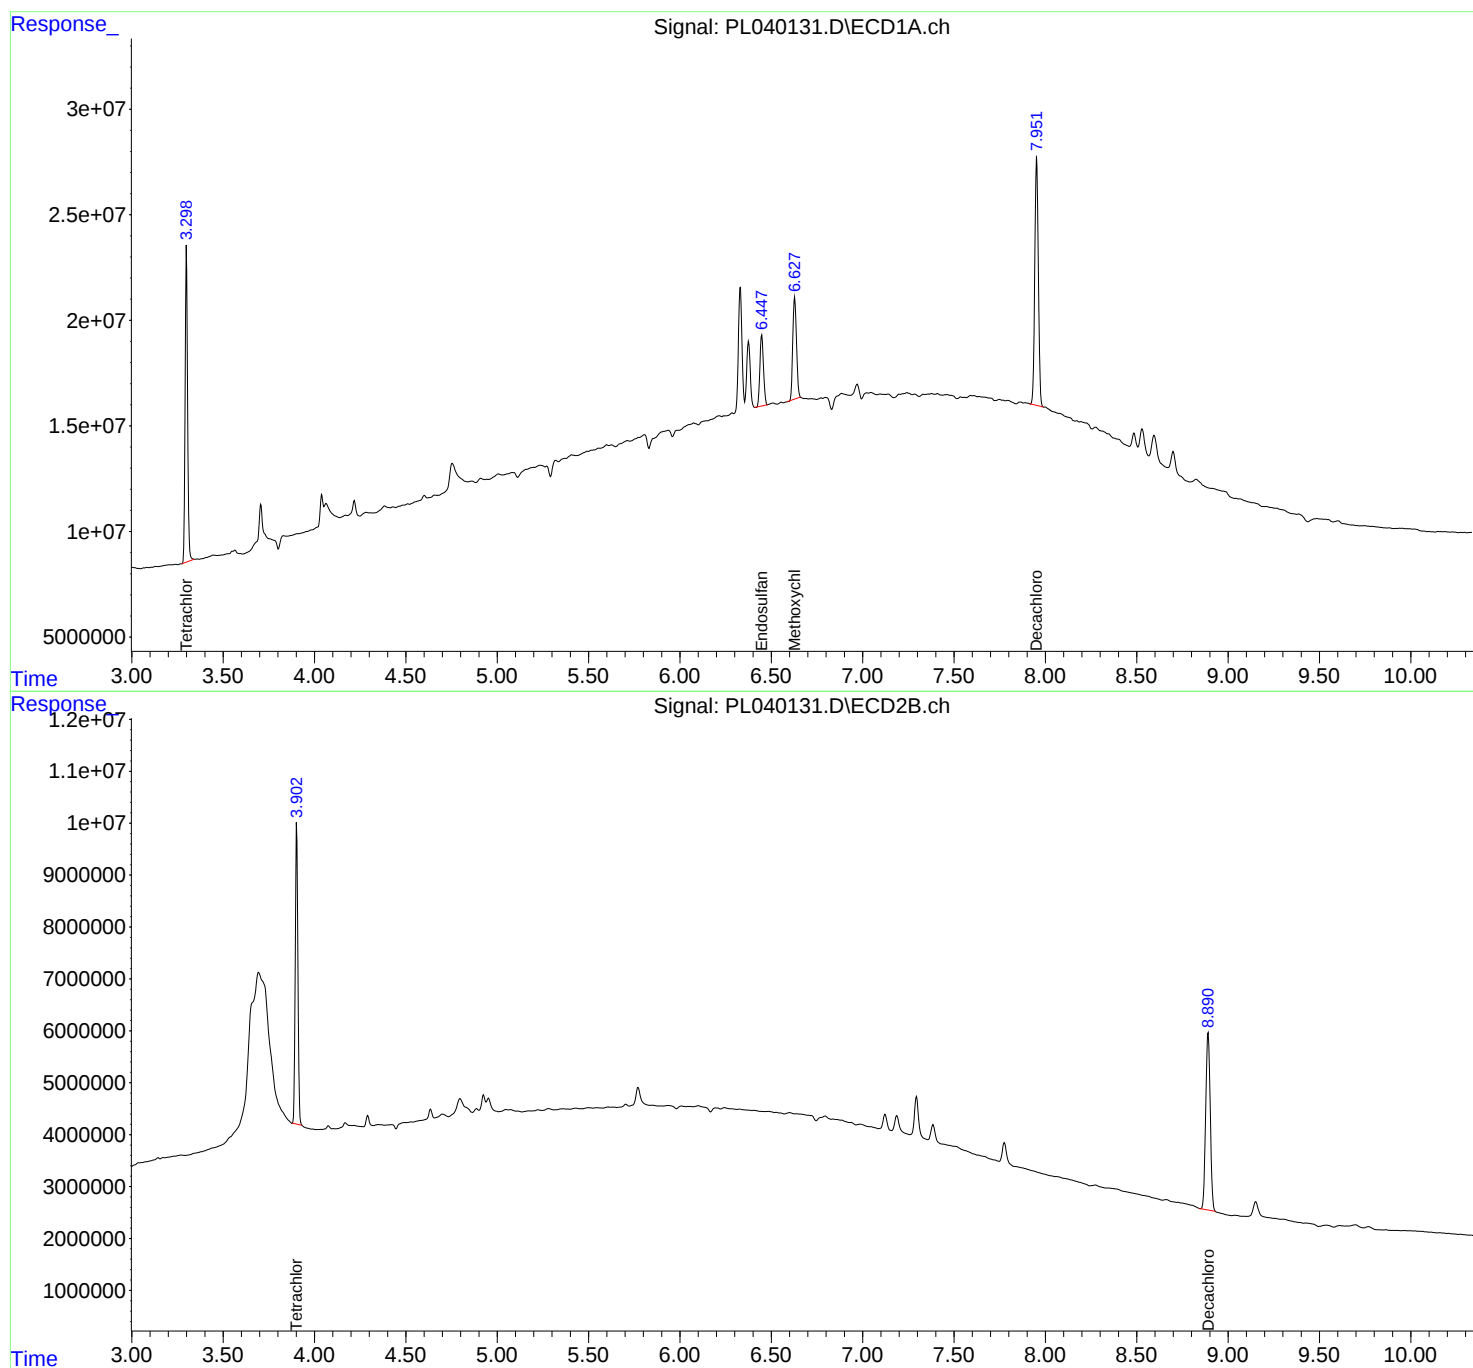


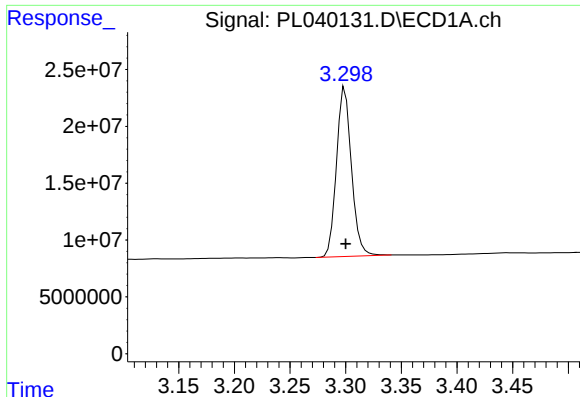

#1 Tetrachloro-m-xylene


R.T.: 3.299 min
Delta R.T.: 0.000 min
Response: 139736818
Conc: 18.02 ng/ml

Instrument :
ECD_L
ClientSampleId :

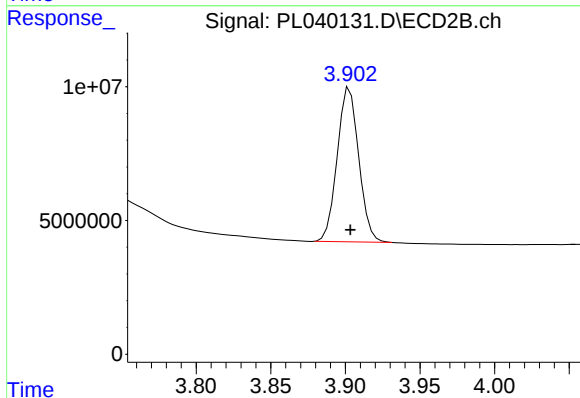


#1 Tetrachloro-m-xylene

R.T.: 3.903 min
Delta R.T.: 0.000 min
Response: 57975608
Conc: 18.17 ng/ml

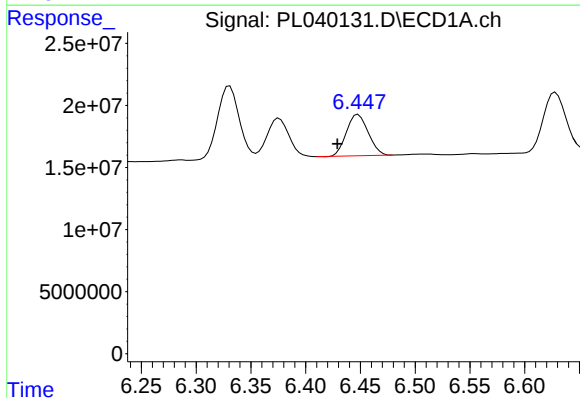


#19 Endosulfan Sulfate

R.T.: 6.448 min
Delta R.T.: 0.019 min
Response: 46008015
Conc: 5.02 ng/ml

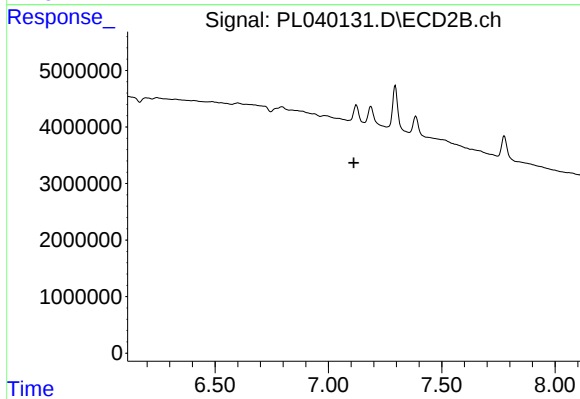

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 7.112 min
Response: 0
Conc: N.D.

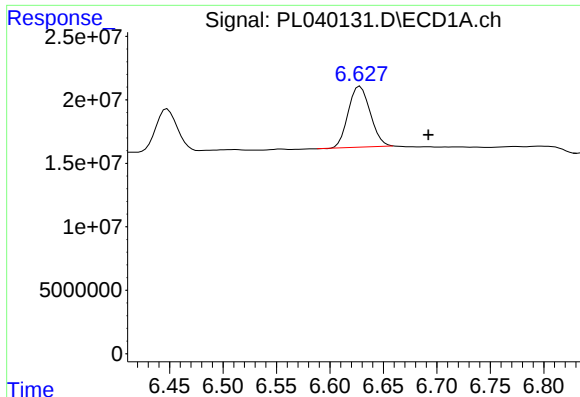

#20 Methoxychlor


R.T.: 6.628 min
Delta R.T.: -0.064 min
Response: 68793562
Conc: 14.84 ng/ml

Instrument :
ECD_L
ClientSampleId :

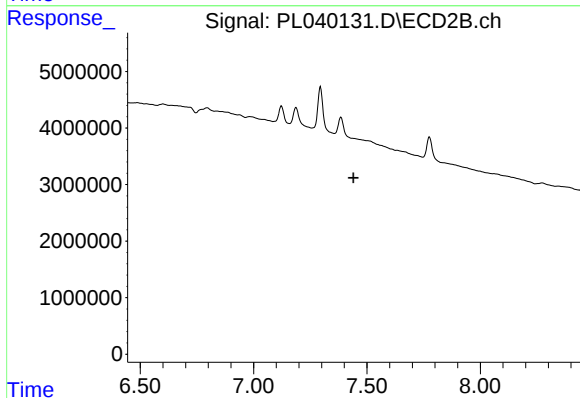


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.441 min
Response: 0
Conc: N.D.

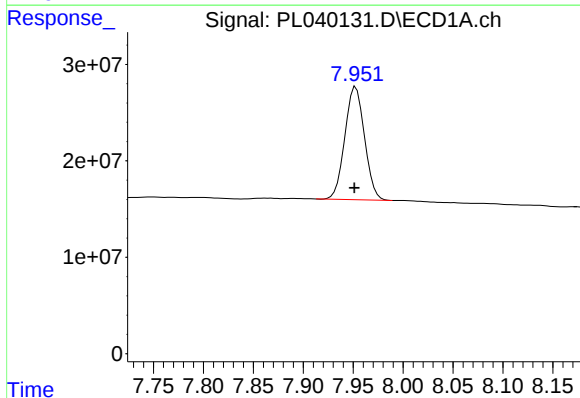

#28 Decachlorobiphenyl

R.T.: 7.953 min
Delta R.T.: 0.001 min
Response: 160374705
Conc: 19.25 ng/ml

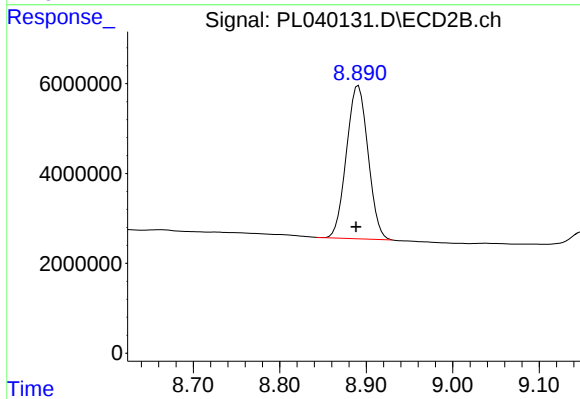

#28 Decachlorobiphenyl

R.T.: 8.891 min
Delta R.T.: 0.003 min
Response: 58916640
Conc: 21.69 ng/ml