

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091918\
 Data File : PL040141.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Sep 2018 22:36
 Operator : AJ\SJ
 Sample : J4975-04
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 20 01:19:46 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 14 23:10:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.299	3.903	138.9E6	55937895	17.910	17.531
28)	SA Decachlor...	7.951	8.890	146.7E6	54204305	17.605	19.957
Target Compounds							
8)	B Heptachlo...	0.000	5.771	0	5350049	N.D.	1.353 #
20)	A Methoxychlor	6.627f	0.000	22344506	0	4.821	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091918\
Data File : PL040141.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Sep 2018 22:36
Operator : AJ\SJ
Sample : J4975-04
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 20 01:19:46 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
Quant Title : GC Extractables
QLast Update : Fri Sep 14 23:10:39 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

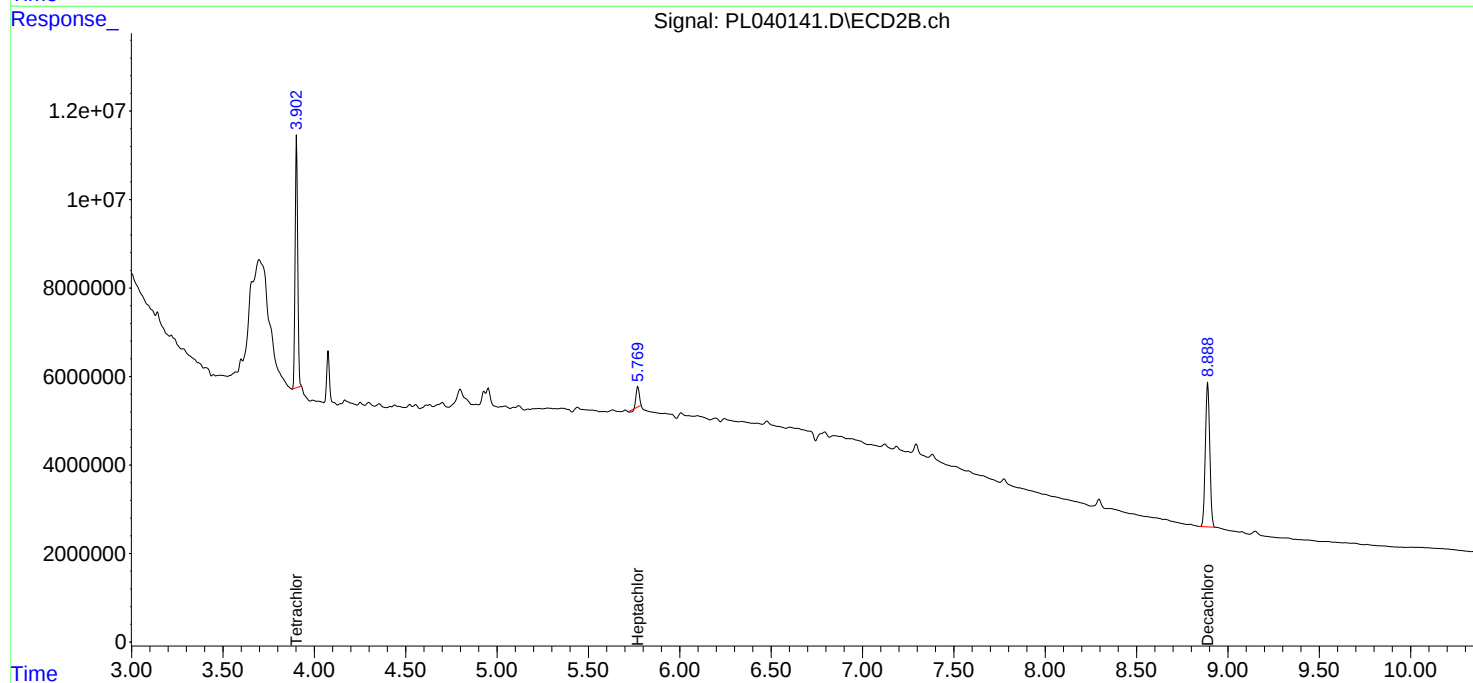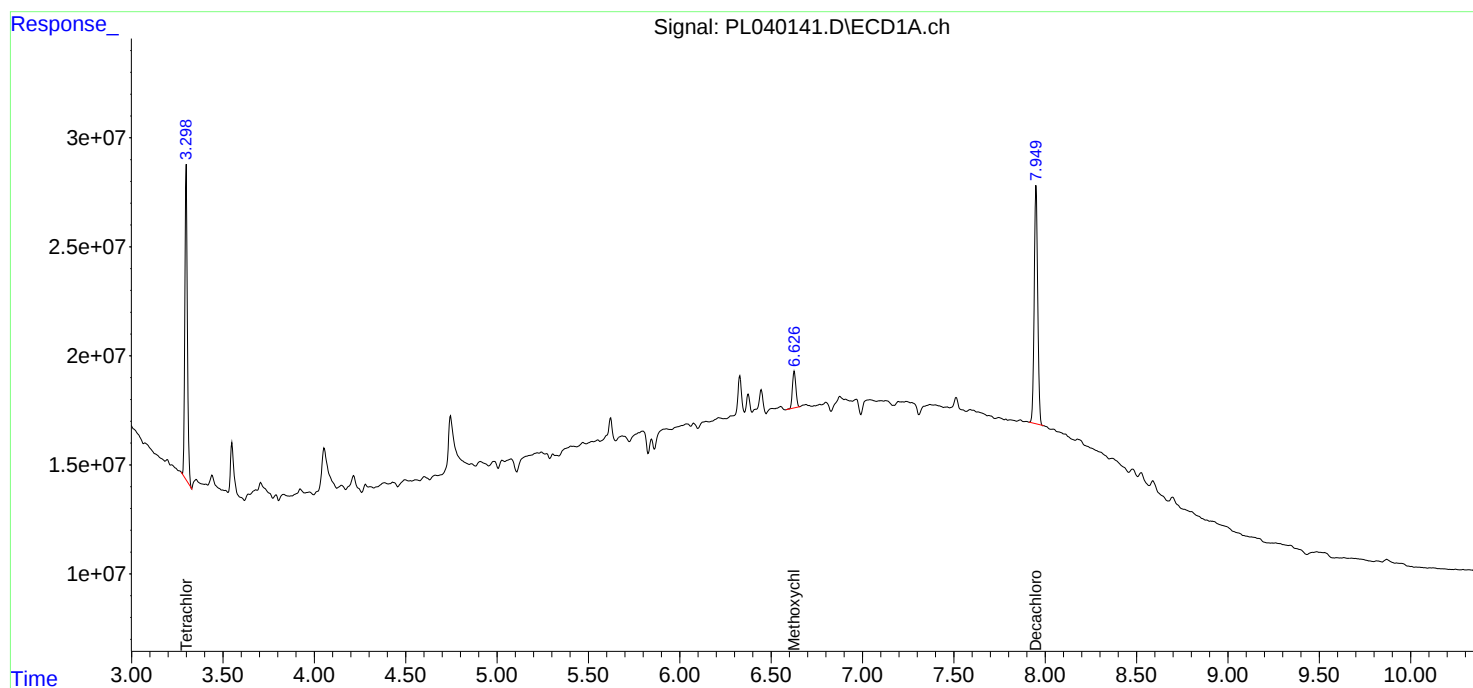


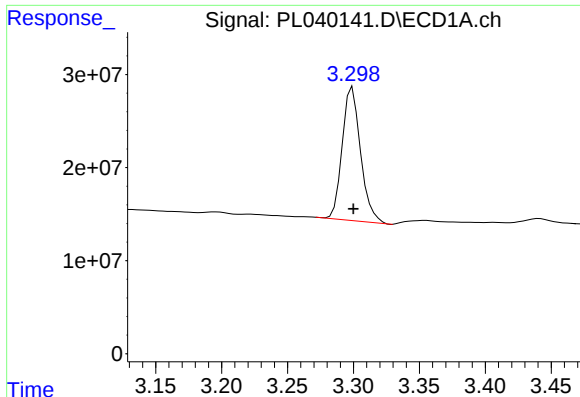

#1 Tetrachloro-m-xylene


R.T.: 3.299 min
Delta R.T.: 0.000 min
Response: 138890713
Conc: 17.91 ng/ml

Instrument :
ECD_L
ClientSampleId :

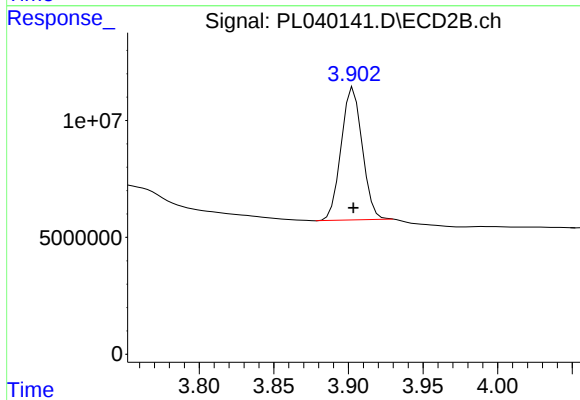


#1 Tetrachloro-m-xylene

R.T.: 3.903 min
Delta R.T.: 0.000 min
Response: 55937895
Conc: 17.53 ng/ml

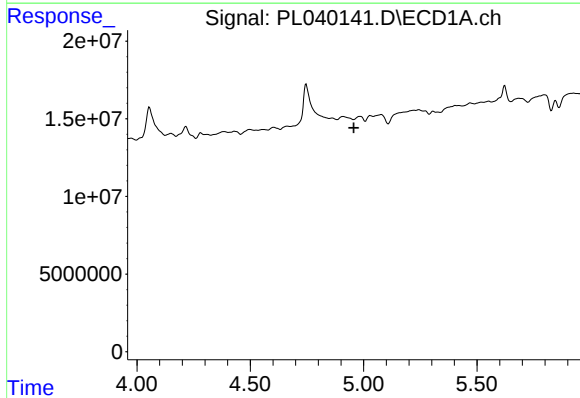


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.956 min
Response: 0
Conc: N.D.

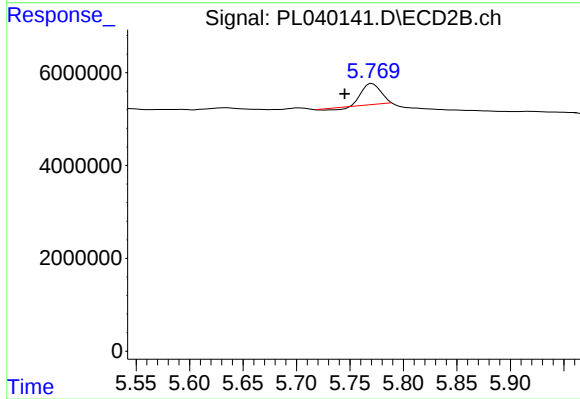

#8 Heptachlor epoxide


R.T.: 5.771 min
Delta R.T.: 0.026 min
Response: 5350049
Conc: 1.35 ng/ml

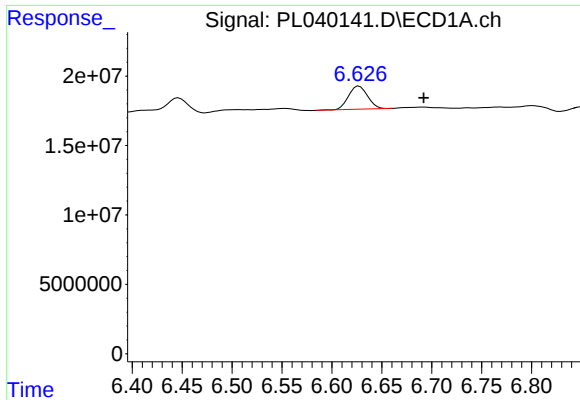

#20 Methoxychlor


R.T.: 6.627 min
Delta R.T.: -0.065 min
Response: 22344506
Conc: 4.82 ng/ml

Instrument :
ECD_L
ClientSampleId :

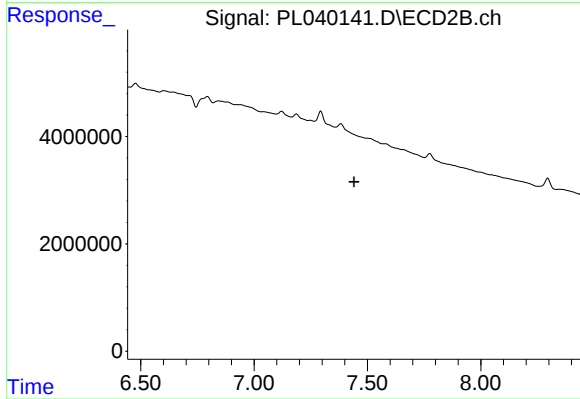


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.441 min
Response: 0
Conc: N.D.

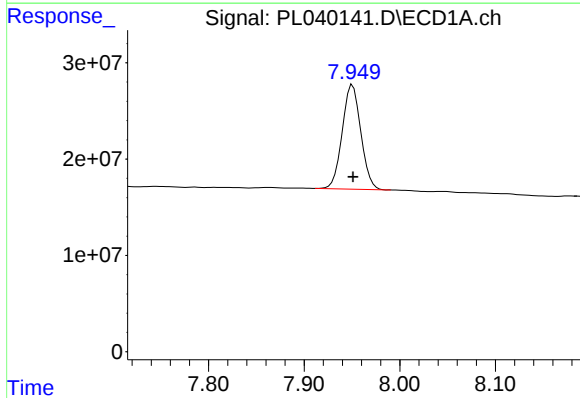

#28 Decachlorobiphenyl

R.T.: 7.951 min
Delta R.T.: 0.000 min
Response: 146696894
Conc: 17.61 ng/ml

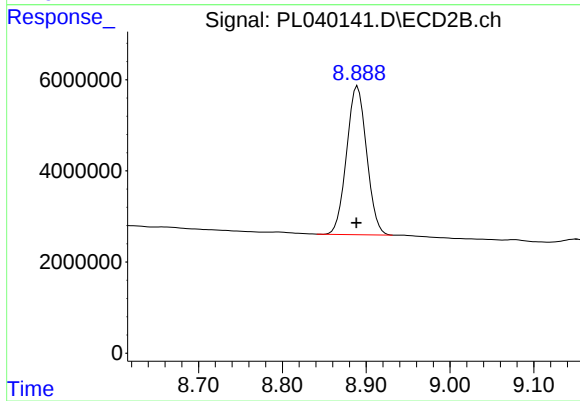

#28 Decachlorobiphenyl

R.T.: 8.890 min
Delta R.T.: 0.002 min
Response: 54204305
Conc: 19.96 ng/ml