

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091919\
 Data File : PL052611.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Sep 2019 08:51
 Operator : SG\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 20 00:51:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091719.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 17 11:25:25 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

8) B	Heptachlo...	0.000	5.918	0	32953477	N.D.	12.566 #
9) A	Endosulfan I	5.666f	0.000	8736756	0	0.896	N.D. #
10) B	gamma-Chl...	0.000	6.127f	0	3007991	N.D.	1.182 #
14) MA	Endrin	0.000	6.751	0	11238977	N.D.	5.807 #
17) MA	4,4'-DDT	0.000	7.178	0	2721303	N.D.	1.488 #
18) B	Endrin al...	0.000	7.108f	0	1524425	N.D.	0.822 #
24)	Chlordane-2	4.959	0.000	33203973	0	109.175	N.D. #
25)	Chlordane-3	0.000	6.127f	0	3007991	N.D.	9.831 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091919\
Data File : PL052611.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Sep 2019 08:51
Operator : SG\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 20 00:51:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091719.M
Quant Title : GC Extractables
QLast Update : Tue Sep 17 11:25:25 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

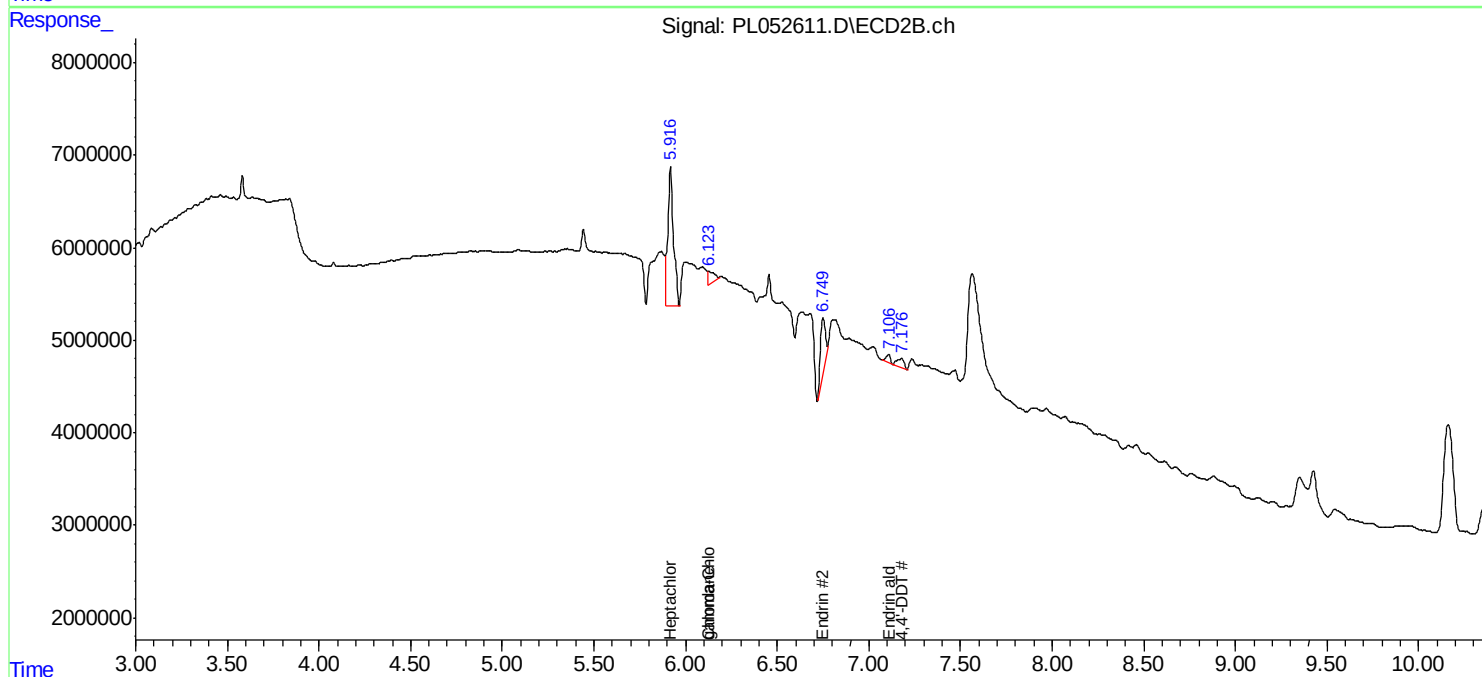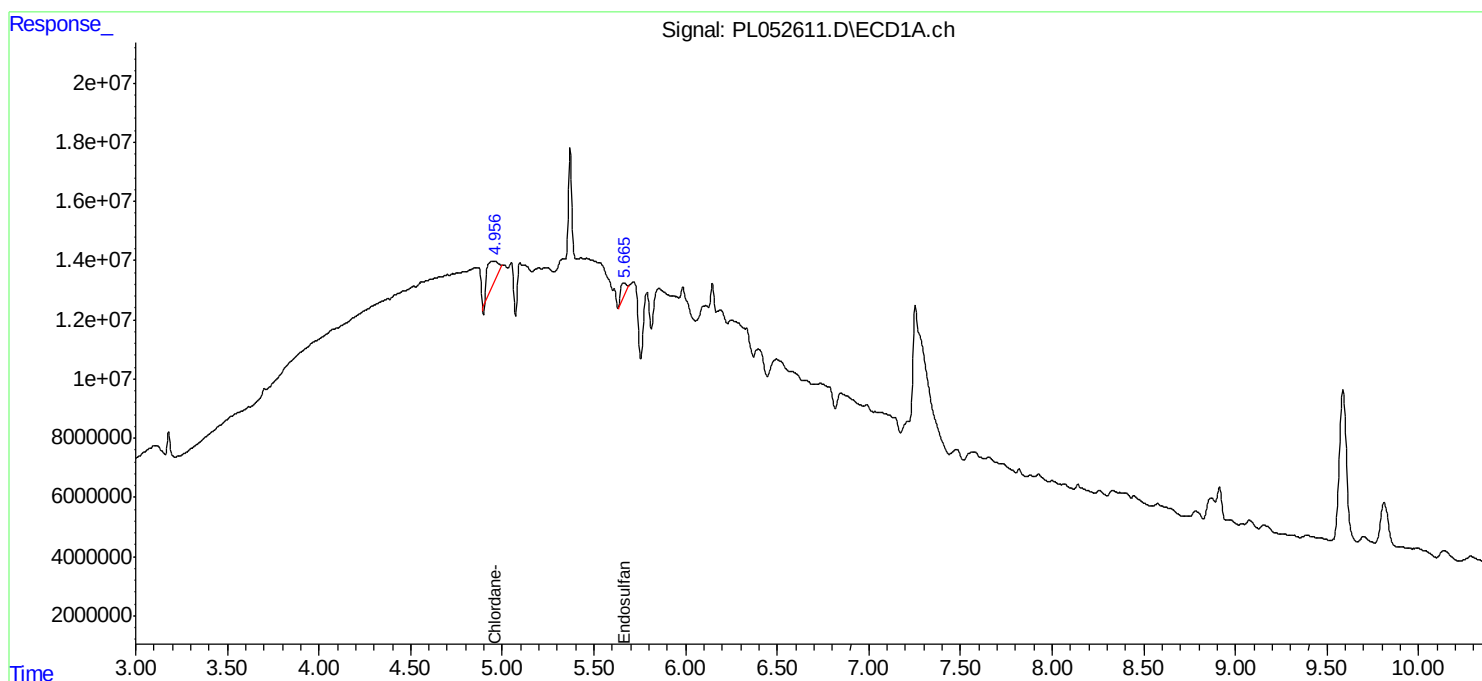


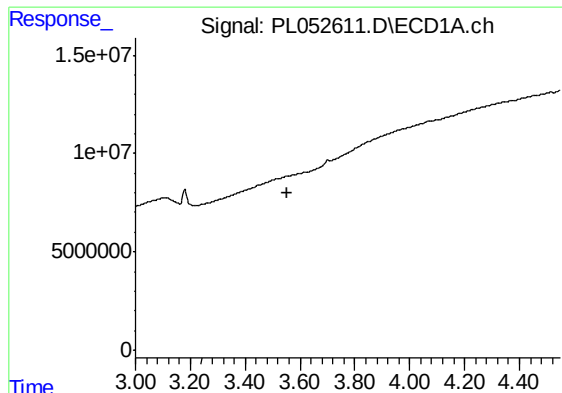

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.551 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

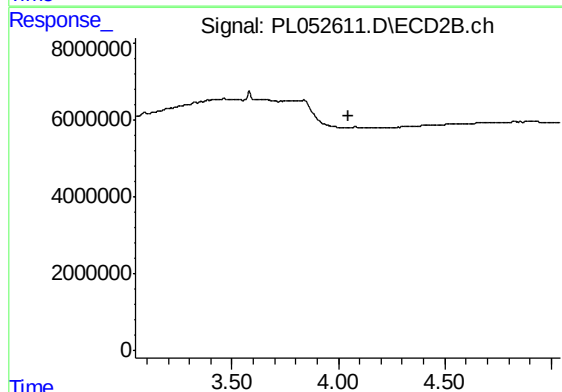


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.045 min
Response: 0
Conc: N.D.

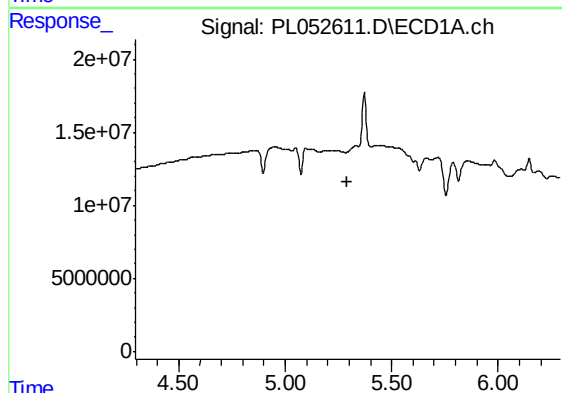


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.293 min
Response: 0
Conc: N.D.

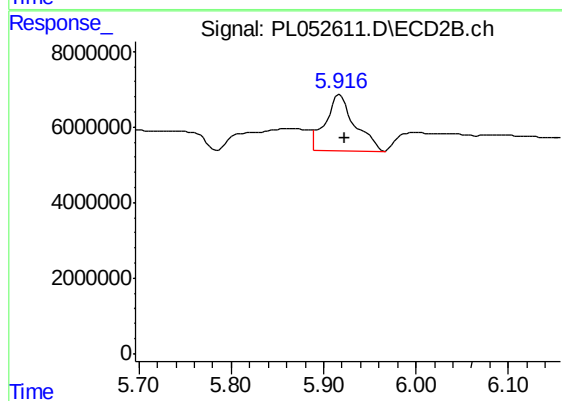

#8 Heptachlor epoxide


R.T.: 5.918 min
Delta R.T.: -0.005 min
Response: 32953477
Conc: 12.57 ng/ml

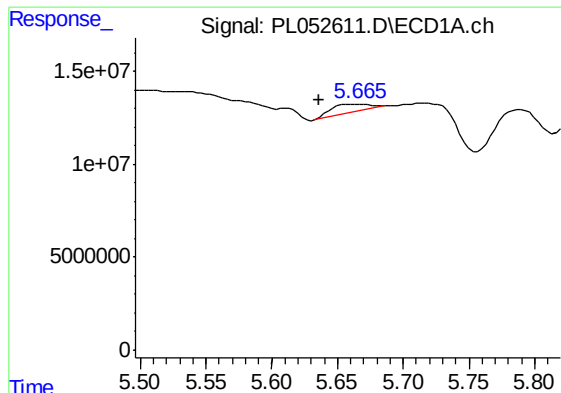

#9 Endosulfan I


R.T.: 5.666 min
Delta R.T.: 0.029 min
Response: 8736756
Conc: 0.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

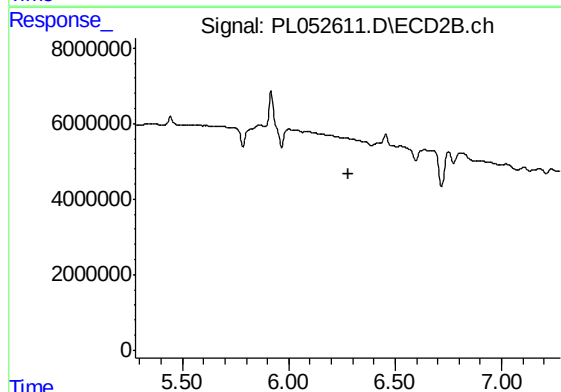


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.279 min
Response: 0
Conc: N.D.

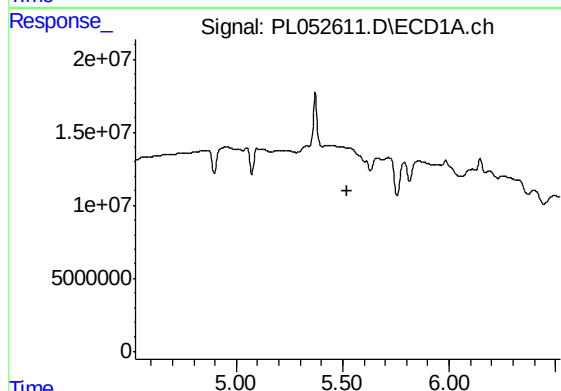


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.523 min
Response: 0
Conc: N.D.

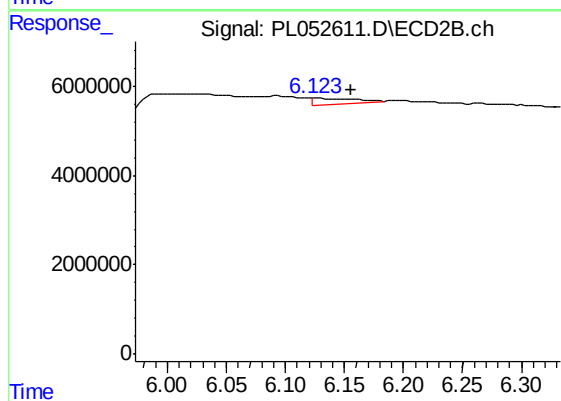

#10 gamma-Chlordane


R.T.: 6.127 min
Delta R.T.: -0.028 min
Response: 3007991
Conc: 1.18 ng/ml

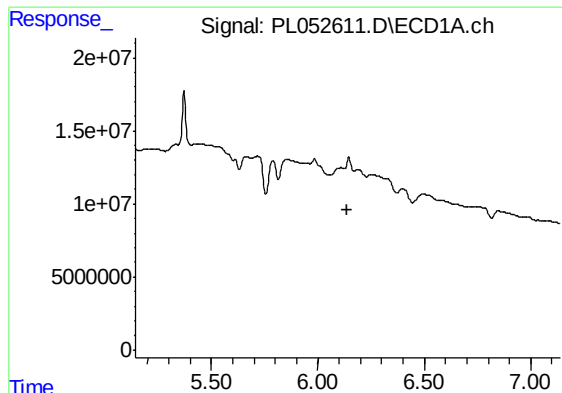

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.140 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

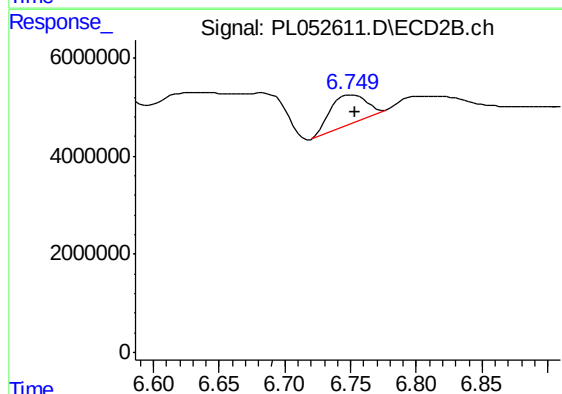


#14 Endrin

R.T.: 6.751 min
Delta R.T.: -0.002 min
Response: 11238977
Conc: 5.81 ng/ml

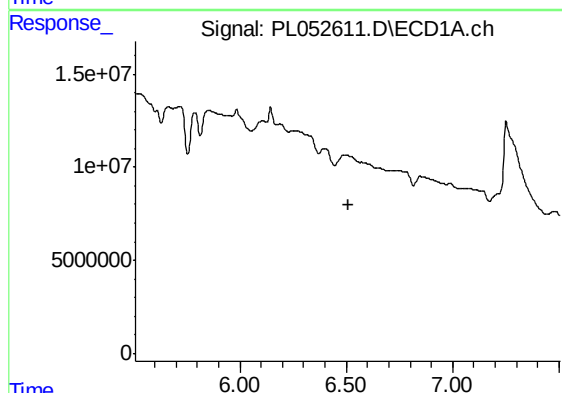


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 6.508 min
Response: 0
Conc: N.D.

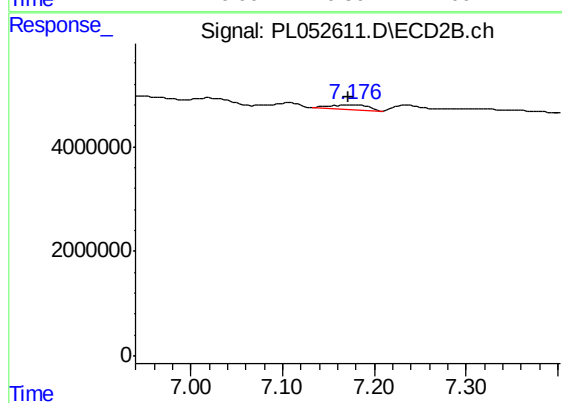

#17 4,4'-DDT


R.T.: 7.178 min
Delta R.T.: 0.006 min
Response: 2721303
Conc: 1.49 ng/ml

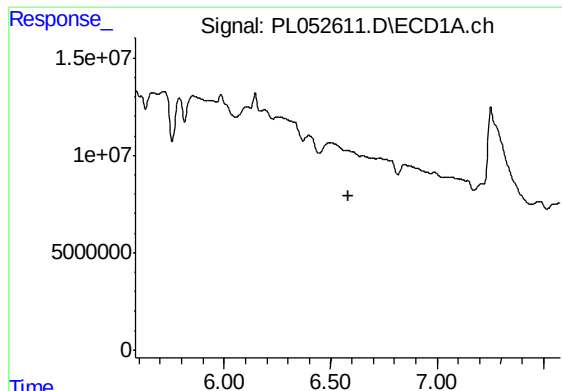

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 6.583 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

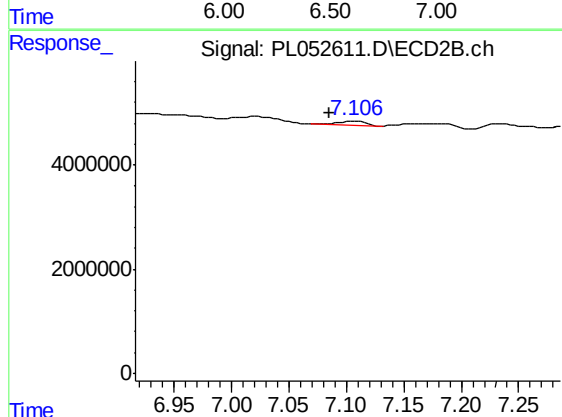


#18 Endrin aldehyde

R.T.: 7.108 min
Delta R.T.: 0.023 min
Response: 1524425
Conc: 0.82 ng/ml

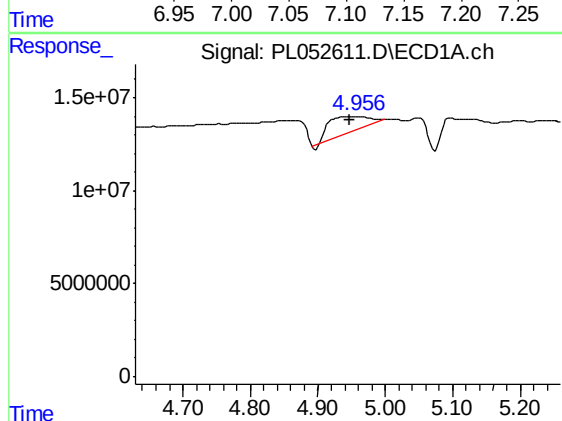


#24 Chlordane-2

R.T.: 4.959 min
Delta R.T.: 0.011 min
Response: 33203973
Conc: 109.18 ng/ml

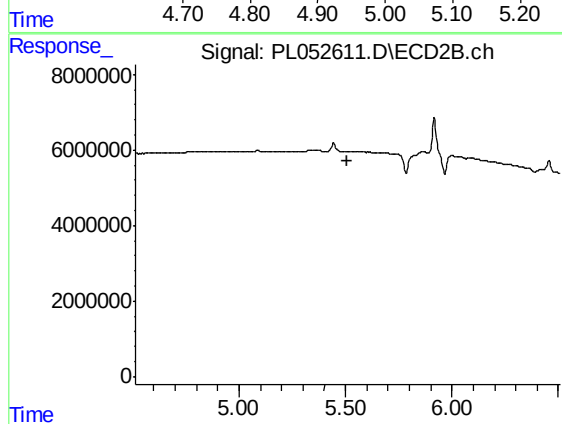

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.510 min
Response: 0
Conc: N.D.

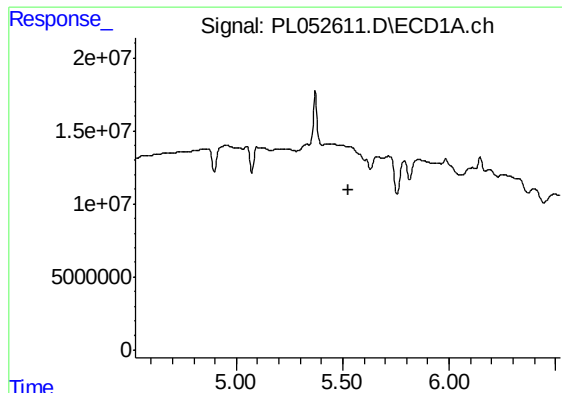

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 5.525 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

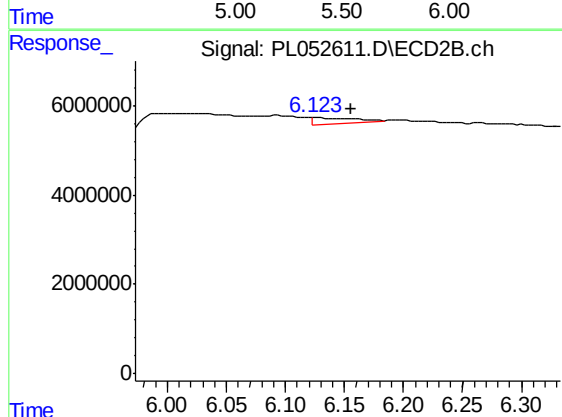


#25 Chlordane-3

R.T.: 6.127 min
Delta R.T.: -0.028 min
Response: 3007991
Conc: 9.83 ng/ml

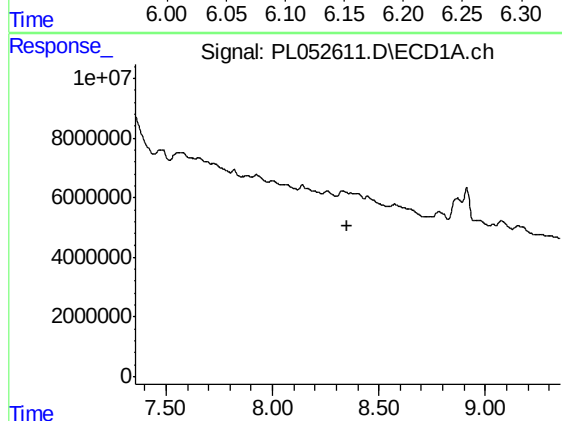

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.354 min
Response: 0
Conc: N.D.

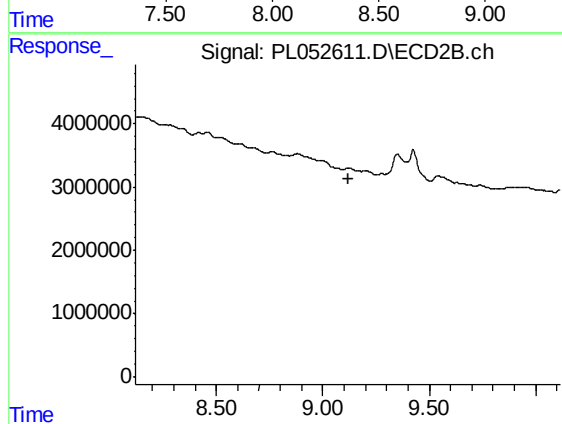

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.118 min
Response: 0
Conc: N.D.