

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091919\
 Data File : PL052639.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Sep 2019 17:49
 Operator : SG\AJ
 Sample : K4969-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FK-PS-01-059

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 20 01:01:14 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091719.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 17 11:25:25 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.550	4.046	88505611	27442939	11.350	12.595
28)	SA Decachlor...	8.349	9.119	76905912	25938656	8.795	10.832
Target Compounds							
4)	MA Heptachlor	0.000	5.253f	0	440292	N.D.	0.150 #
7)	B delta-BHC	0.000	5.085f	0	995943	N.D.	0.348 #
10)	B gamma-Chl...	5.543f	6.156	16987759	3071443	1.600	1.207
11)	B alpha-Chl...	0.000	6.231	0	7599066	N.D.	3.042 #
12)	B 4,4'-DDE	0.000	6.383	0	1012850	N.D.	0.415 #
23)	Chlordane-1	0.000	5.042	0	837058	N.D.	10.780 #
25)	Chlordane-3	5.543f	6.156	16987759	3071443	17.559	10.038 #
26)	Chlordane-4	0.000	6.231	0	7599066	N.D.	19.758 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091919\
Data File : PL052639.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Sep 2019 17:49
Operator : SG\AJ
Sample : K4969-01
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
FK-PS-01-059

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 20 01:01:14 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091719.M
Quant Title : GC Extractables
QLast Update : Tue Sep 17 11:25:25 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

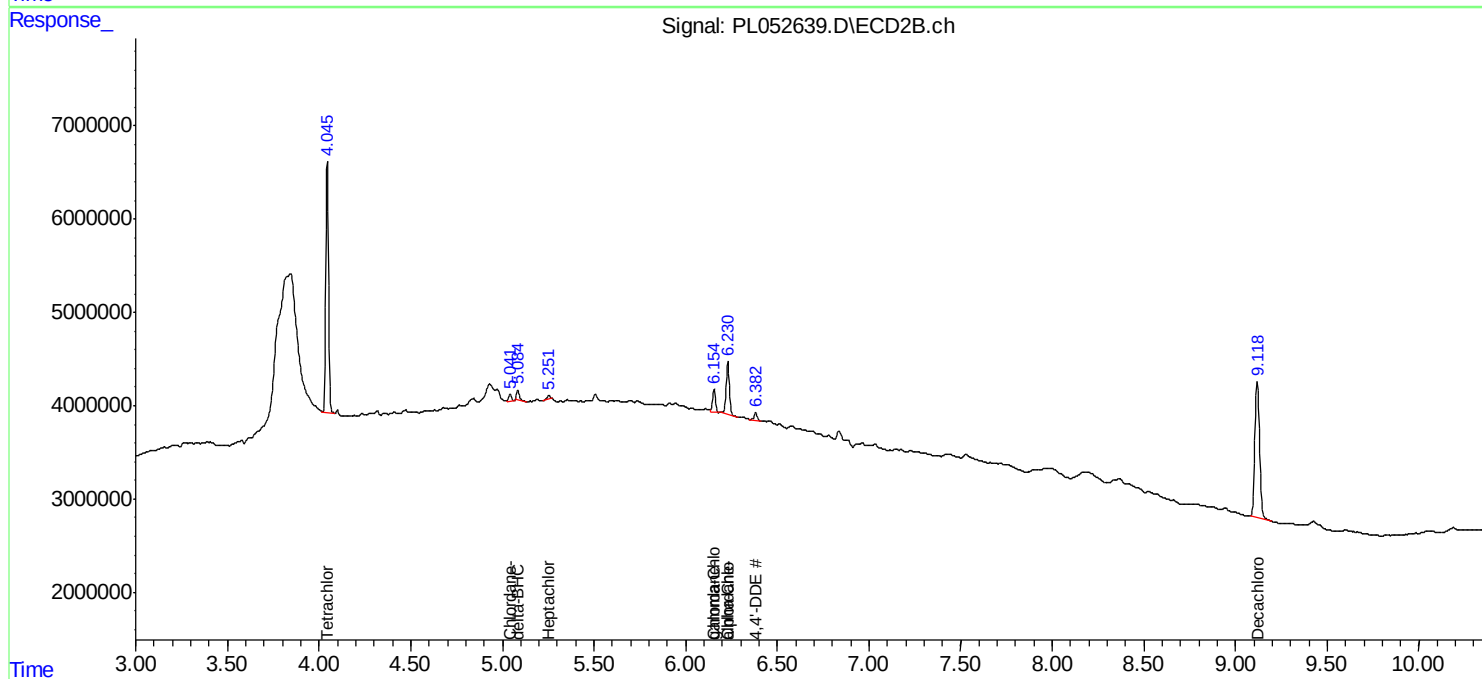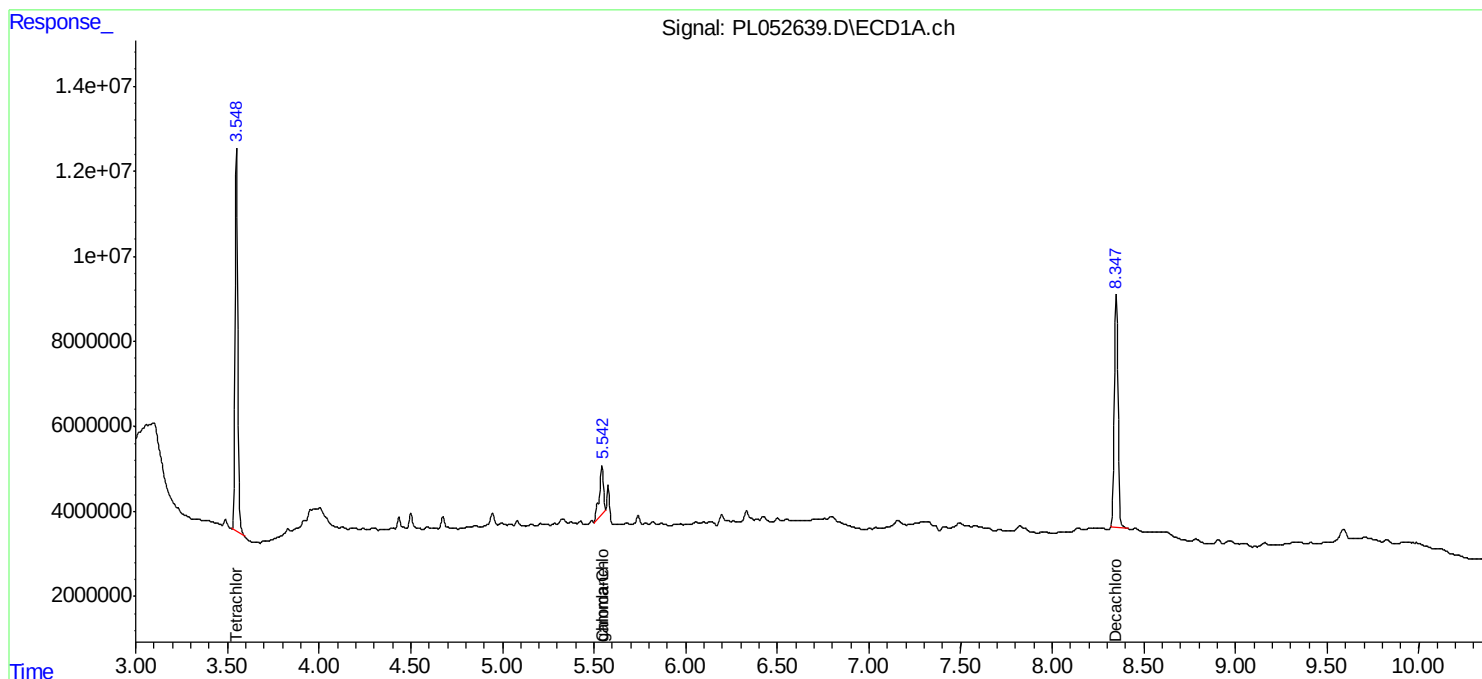


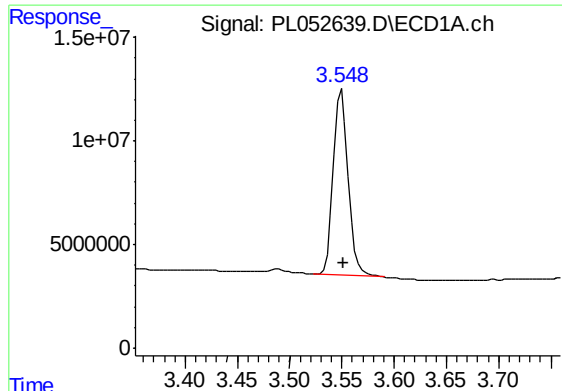

#1 Tetrachloro-m-xylene


R.T.: 3.550 min
Delta R.T.: -0.001 min
Response: 88505611
Conc: 11.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-PS-01-059

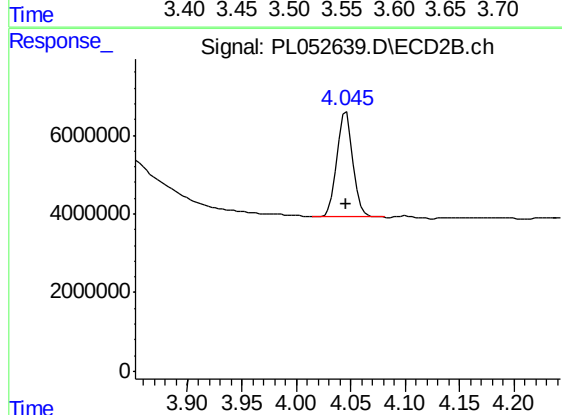


#1 Tetrachloro-m-xylene

R.T.: 4.046 min
Delta R.T.: 0.000 min
Response: 27442939
Conc: 12.59 ng/ml

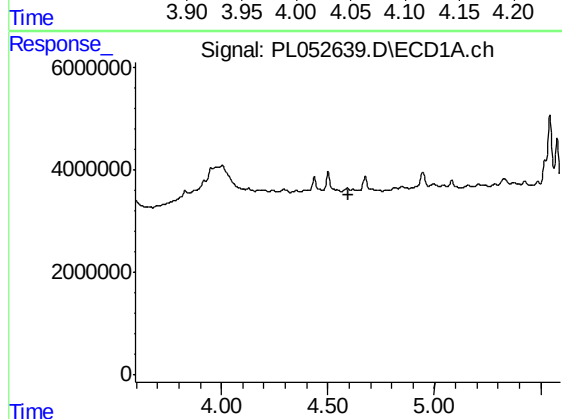


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.594 min
Response: 0
Conc: N.D.

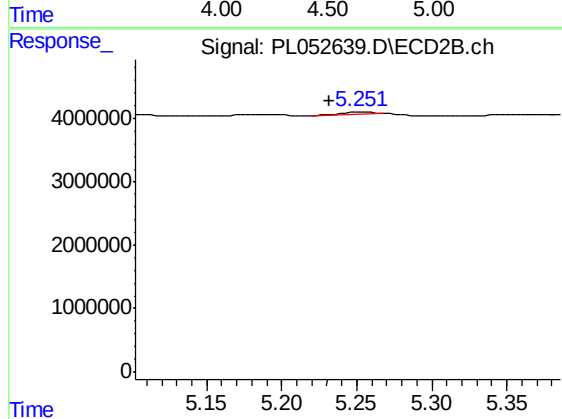

#4 Heptachlor


R.T.: 5.253 min
Delta R.T.: 0.021 min
Response: 440292
Conc: 0.15 ng/ml

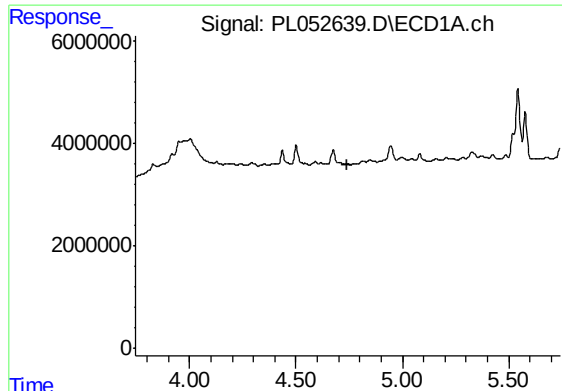

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.743 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
FK-PS-01-059

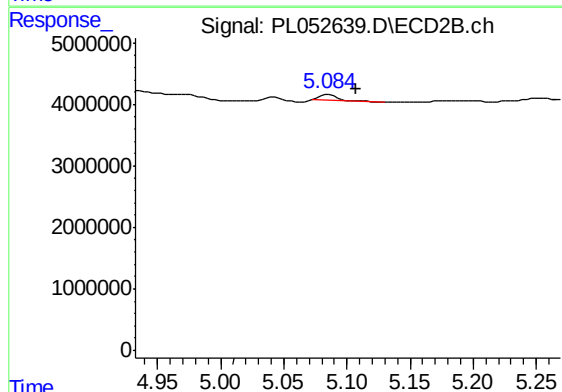


#7 delta-BHC

R.T.: 5.085 min
Delta R.T.: -0.022 min
Response: 995943
Conc: 0.35 ng/ml

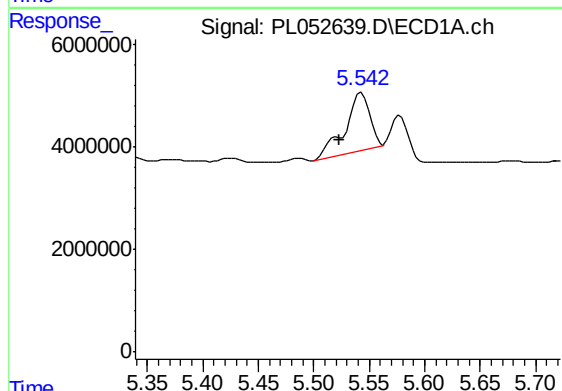


#10 gamma-Chlordane

R.T.: 5.543 min
Delta R.T.: 0.020 min
Response: 16987759
Conc: 1.60 ng/ml

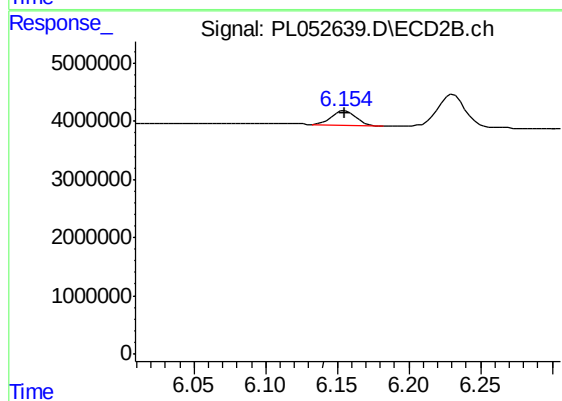

#10 gamma-Chlordane


R.T.: 6.156 min
Delta R.T.: 0.000 min
Response: 3071443
Conc: 1.21 ng/ml

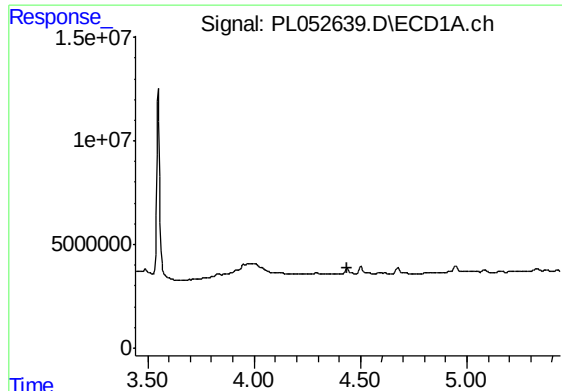

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.440 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
FK-PS-01-059

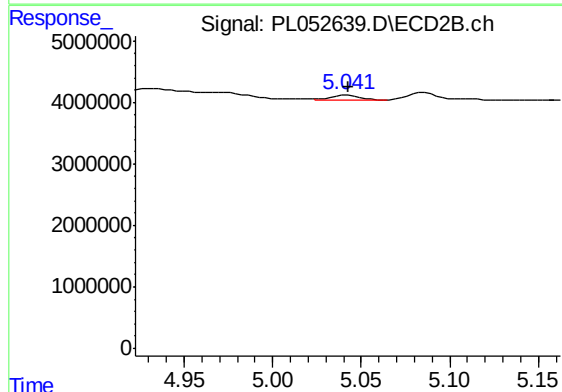


#23 Chlordane-1

R.T.: 5.042 min
Delta R.T.: 0.000 min
Response: 837058
Conc: 10.78 ng/ml

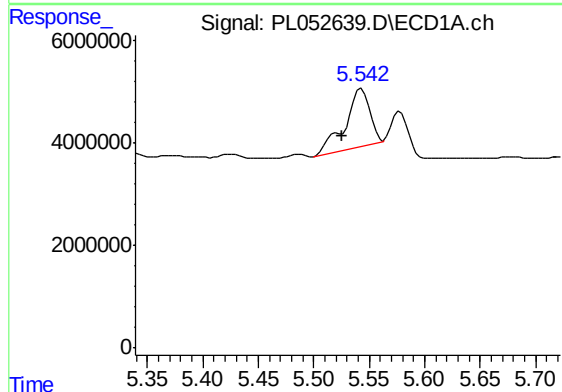


#25 Chlordane-3

R.T.: 5.543 min
Delta R.T.: 0.018 min
Response: 16987759
Conc: 17.56 ng/ml

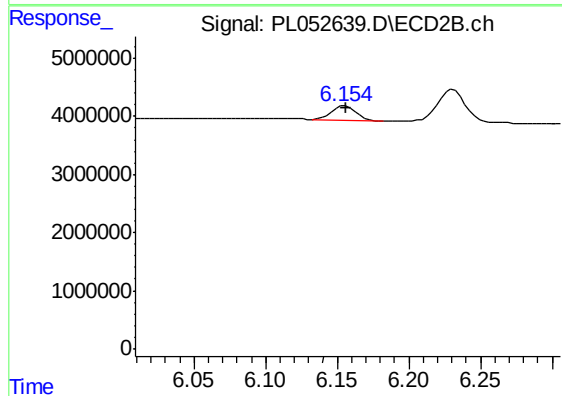

#25 Chlordane-3


R.T.: 6.156 min
Delta R.T.: 0.000 min
Response: 3071443
Conc: 10.04 ng/ml

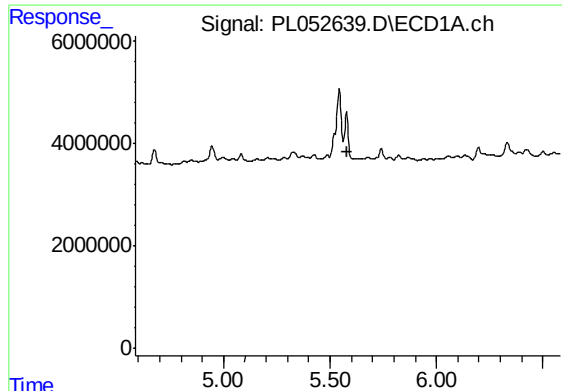

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.583 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
FK-PS-01-059

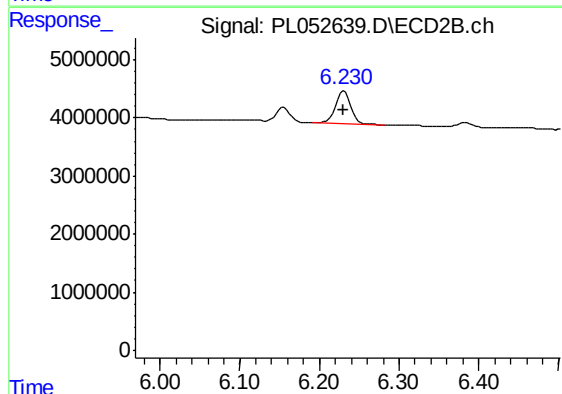


#26 Chlordane-4

R.T.: 6.231 min
Delta R.T.: 0.000 min
Response: 7599066
Conc: 19.76 ng/ml

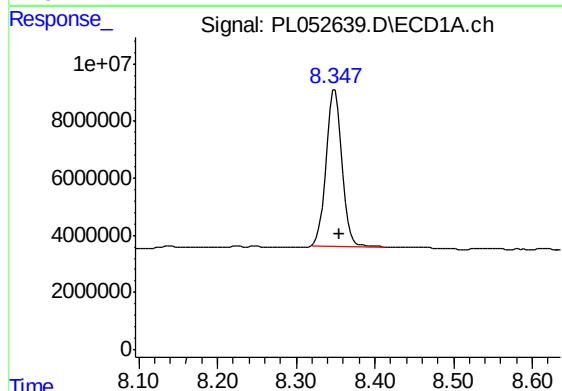

#28 Decachlorobiphenyl

R.T.: 8.349 min
Delta R.T.: -0.006 min
Response: 76905912
Conc: 8.79 ng/ml

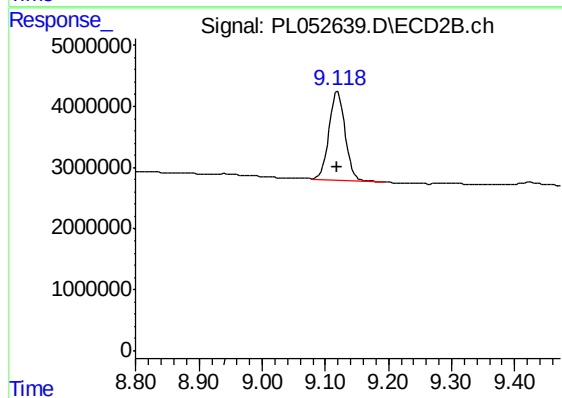

#28 Decachlorobiphenyl

R.T.: 9.119 min
Delta R.T.: 0.000 min
Response: 25938656
Conc: 10.83 ng/ml